
# Remote Photoplethysmography for Heart Rate and Blood Oxygenation Measurement: A Review

Pireh Pirzada, Adriana Wilde, and David Harris-Birtill

***Abstract*—Usually measured through obtrusive contact-based methods, heart rate (HR) and peripheral oxygen saturation ($SpO_2$) are critical physiological signs used by clinicians during emergency interventions. Remote photoplethysmography (rPPG) allows for unobtrusive sensing of these vital signs for health monitoring in various settings. We present a review of rPPG-related research conducted including related processes and techniques, such as regions of interest (ROI) selection, extracting the raw signal, preprocessing data, applying noise reduction algorithms, fast Fourier transforms (FFTs), and filtering and extracting these vital signs. Furthermore, we present a detailed, critical evaluation of available rPPG systems. Limitations and future directions have also been identified to further advance this field.**

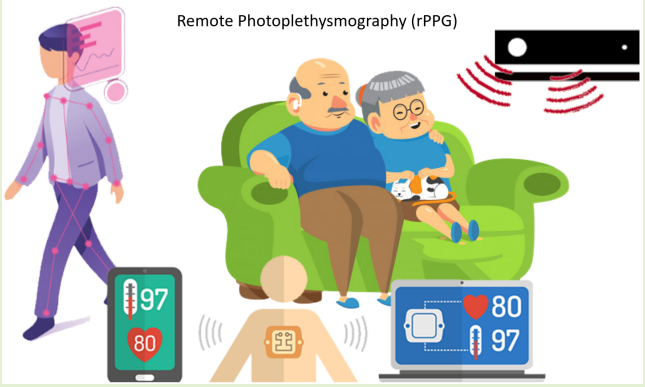


***Index Terms*— Blood oxygenation, health monitoring, heart rate (HR), remote photoplethysmography (rPPG), signal processing.**

## I. Introduction

HEART rate (HR) and blood oxygen saturation ($SpO_2$) are the physiological signs used as critical indicators for human health, as they are clinical alerts of a significant change [1]. The first of these signs, HR, is a critical measure of cardiac activity [2], used for the assessment of emergent ill health. At rest, normal values lie between 60 and 100 beats/min (BPM) [3]. Lower values ("bradycardia") might indicate hypovolemic shock [4] and higher ones ("tachycardia") [3], high intracranial pressure [5].

The second sign, $SpO_2$, is a broad measure of blood oxygen saturation, the percentage of hemoglobin (Hb) in the blood carrying oxygen. When a person breathes, oxygen enters the lungs, transfers across the alveolar membrane and into the bloodstream [6], allowing oxygen transfer to all body cells [7]. Once the oxygen has been off-loaded, the Hb becomes deoxygenated Hb, "deoxy-Hb" [7], returning to the heart which then sends it on to the lungs to acquire more oxygen, and so the process continues [2]. Abnormal changes in $SpO_2$ can affect organs and is often associated with disease [7], such as pneumonia [8], asthma [9], chronic obstructive pulmonary disease (COPD) [10], [11], hypoxia [12], drug overdose [12], respiratory [13], or heart diseases [14]. $SpO_2$ values below 94% are abnormal for most people, although some individuals with stable chronic conditions may have readings of 88%–94% [15]. Monitoring changes in $SpO_2$ can help identifying complications including respiratory failure [13]. Here, we introduce the measurement of HR and $SpO_2$, explaining the methods used for these measurements, including contact-based pulse oximetry, and their limitations, which motivate the use of remote photoplethysmography (rPPG), as an innovative approach to overcome them.

### A. Measuring HR and $SpO_2$

Measurement of these vitals impacts clinical decisions [16]. For HR, electrocardiograms (ECGs) are used to characterize the cardiac rhythm in detail but require keeping electrodes in place, typically with gel patches or chest straps [17], often requiring shaving body hair and adherent tape, which may irritate the skin or cause allergic reactions [18], [19] especially in

Manuscript received 24 April 2024; accepted 16 May 2024. Date of publication 7 June 2024; date of current version 1 August 2024. The work of Pireh Pirzada was supported in part by St Leonard's Scholarship by the University of St Andrews. The work of Adriana Wilde was supported in part by the Centre for Health Technologies at the University of Southampton. The associate editor coordinating the review of this article and approving it for publication was Prof. Huang Chen Lee. *(Corresponding author: Pireh Pirzada.)*

Pireh Pirzada is with the Department of Digital Technologies, University of Winchester, SO22 4NR Winchester, U.K. (e-mail: pireh.pirzada@winchester.ac.uk).

Adriana Wilde is with the School of Electronics and Computer Science, University of Southampton, SO17 1BJ Southampton, U.K.

David Harris-Birtill is with the School of Computer Science, University of St Andrews, KY16 9AJ St Andrews, U.K.

This article has supplementary downloadable material available at https://doi.org/10.1109/JSEN.2024.3405414, provided by the authors.

Digital Object Identifier 10.1109/JSEN.2024.3405414

1558-1748 © 2024 IEEE. Personal use is permitted, but republication/redistribution requires IEEE permission.
See https://www.ieee.org/publications/rights/index.html for more information.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

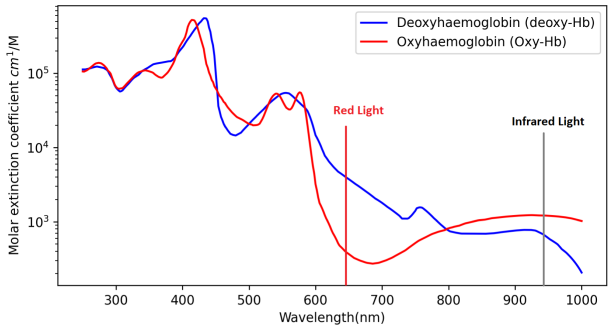



Fig. 1. Optical extinction spectra of oxy-Hb and deoxy-Hb within the blood. Figure generated using data by Pirzada et al. [29] and Prahl [31].

long-term monitoring [19]. For $SpO_2$, invasive procedures like arterial blood gas (ABG) sampling can be used. Here, blood is drawn from an artery [20], which is painful and adds a risk of infection [15], [20]. Regular sampling is time-consuming [21] and adds a risk of blood loss in neonatal care [22]. These vitals can also be monitored with contact-based pulse oximetry [23], [24], [25], discussed next.

### B. Contact-Based Pulse Oximetry

Pulse oximetry is based on the photoplethysmography (PPG) principles introduced by Hertzman and Spealman [26]. Blood flow is measured through changes in light dispersion [25], [27]. Pulse oximetry has a red and infrared (IR) light-emitting diode (LED) placed on one side of the probe and a photodetector on the other side. Pulse oximetry uses two wavelengths of light through the finger to a photodetector, where light is absorbed by the finger and the rest reaches the photodetector. The light absorption is governed by Beer's law [28], i.e., proportionately to the concentration of the light-absorbing material (e.g., Hb and deoxy-Hb), hence, the higher their concentration, the more light is absorbed. As light-absorbing materials, Hb and deoxy-Hb differ: Hb absorbs more IR light whereas deoxy-Hb absorbs more red light as shown in Fig. 1 [29]. Pulse oximeter LEDs emit light at 660-nm (red) and 940-nm (IR) wavelengths [30].

Pulse oximeters are the cheapest and most common way to measure HR and $SpO_2$ [32]. They are comparatively less intrusive in clinical settings [25], as they can be clipped on a fingertip, an earlobe [33], wrapped on a baby's foot, on a wrist band [34], or even stuck to the forehead [35]. Portable pulse oximeters have now become adopted worldwide for self-evaluating health vitals at home [36] and played an important role during the COVID-19 pandemic [37]. They are also used for sports [38], [39], and devices may have Bluetooth connectivity with smartphones, allowing data recording over time [40], [41], [42]. Commercial wearable devices (e.g., Apple Watch 6) use PPG [43], but their accuracy decreases in the active state compared with resting state [44]. These solutions require each patient to have such a device which can be costly, burdensome and time-consuming to set up for each patient, for example, in a triage setting for clinicians to monitor multiple patients simultaneously. In addition, contact-based devices encounter challenges, as mentioned below, when used with patients who have physical or cognitive impairments.

Although effective, pulse oximetry presents some accuracy problems as a monitoring tool [15], [20]. A pulse oximeter must be physically placed on a finger, which is hard for some patients with incapacities or cognitive challenges [45], [46], [47], during surgery [46], sensitive skin [18], burned skin [46], and in those with severe illness [18] as well as infants [48], [49] and young children [22]. It may be cumbersome to wear for long periods of time [50], restricting movement if wire-based pulse oximeter devices are used [35] and providing a constant physical reminder that their health is being monitored [18], [51]. It also increases risk of cross-infection [52].

Accuracy of pulse oximeters has been reported to be low for $SpO_2$ values under 83% [7] and is affected by nail varnish, skin tone, access movement, intravascular dyes and having abnormal levels of Hb and carboxyhaemoglobin [7], [45]. Research shows that for participants with dark skin the error rate is higher [53], [54]. One study found a substantial bias in pulse oximeter devices used with people with darker skin tone had a higher error rate ($5.1\% \pm 9.2\%$) in comparison with the white skin tone ($1.9\% \pm 10.2\%$) for $SpO_2$ [55], [56]. Another study reported an increased error rate of $3.56\% \pm 2.45\%$ among darker skin tone participants compared with white skin tone participants with an error rate of $0.37\% \pm 3.20\%$ $SpO_2$ [57] , an issue that has more recently been researched [58], [59], [60]. Also, in a research study with anemic participants during hypoxemia, it was observed that the error rate for the anemic participants was 15% compared with 6.4% among nonanemic participants [55], [61]. Surveyed literature disagrees on the effect of nail varnish, as some studies report a reduction of $SpO_2$ values [62], [63] (especially for black, blue, and green varnish [62]), whereas others found no effect [64], [65]. Next, we explore the novelty and process of rPPG working to help overcome PPG limitations.

### C. Remote Photoplethysmography (rPPG)

The novelty in rPPG technology is its noninvasive nature to monitor physiological signs with no skin contact, as shown in Fig. 2, addressing the limitations discussed in Section I-B. As a noncontact technique, rPPG avoids the need for physical touch required by conventional PPG devices or smartwatches. This feature is advantageous for participants with cognitive or physical impairments, as discussed in Section I-B. It is also a safer, noninvasive alternative to the ABG method for measuring $SpO_2$ levels (with risks listed in Section I-A), and other vitals at a distance, with applications ranging from healthcare to fitness [46]. This approach measures changes in the blood flow and is based on subtle changes on the skin, where the pulse flashes lighter and darker over time. This phenomenon is not visible to the naked eye; however, it can be detected by measuring the reflectance of light over a period of time from skin pixel intensity extracted from regions of interest (ROIs) using a camera-based system [46]. rPPG systems measure the HR by analyzing the skin pixel intensity of the heartbeats over time; the skin flashes darker and lighter as more and less blood flows through the region. $SpO_2$ is measured through the differences in optical absorption across the visible and near-infrared wavelength regions between Hb

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

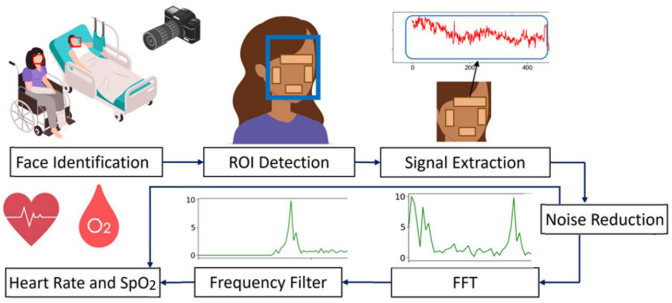



Fig. 2. rPPG process flow shown in the image from identifying the faces of people to obtaining their HR and blood oxygenation levels remotely (vector images by Freekpik and graph images generated by the authors.)

and deoxy-Hb [28], [66]. Various techniques from diverse research systems have been critically evaluated, summarized, and presented in this survey.

## II. Research Motivation

As seen, contact-based pulse oximeters pose challenges for many, which are mitigated with rPPG, a safer and more accessible solution to monitor multiple patients at a time. Despite its rapid growth, rPPG research still predominantly focuses on monitoring HR, with few studies simultaneously tracking both HR and $SpO_2$. To advance these systems their performance needs to be evaluated in various settings, including labs, clinics, and homes. Up to date, there is currently no comprehensive review conducted on the rPPG process for both HR and $SpO_2$ with an in-depth analysis of the limitations of rPPG systems, as reviews focus solely on HR measurement [67], [68], [69], [70], [71], with deep learning [72]. Most omit a comprehensive analysis of $SpO_2$ estimation methods [67], [67], [69], [73]. This review addresses these gaps.

## III. rPPG Process

Here, we discuss the processes followed in rPPG systems. Surveyed articles used a variety of equipment and set-ups to obtain vital signs data from participants, such as thermal cameras [74], [75], [76], [77], charge-coupled device (CCD) cameras [78], [79], other web cameras or those built-in laptops [80], [81], [82], [83], [84], [85], [86], [87], [88], iPads [89], MS Kinect V2 [66], [90], [91], Kinect Azure [92], GoPro cameras on drones [93], [94], and smartphones [95], [96], [97], [98], [99], [100], [101], [102], [103], [104], [105] have been used to obtain a person's vital signs. Tables IV and V (in Supplementary material) [29] list studies conducted with various equipments and the vital signs under observation. The most common steps in rPPG systems are detailed below.

### A. Face and ROI Detection

This involves identifying the person's face from the frame, typically stationing participants in front of a camera in a static position to acquire face images. The participants are often required to be in a specific or fixed location with no or minimal movement. In the case of minimal movement, ROIs are selected manually [106], [107], [108], whereas to cater to head movement or rotation of the head to some degree, various algorithms are used, among which Viola and Jones [109], [110], [111], [112] is common. One main reason for using this library is its availability. Neural network-based classifiers have been used to detect ROIs [113], [114], [115], a statistical model to match a face to an image frame [116] and tracking algorithms of features points for head movement in image frames [117], [118]. One way of addressing the movement problem and identifying the correct ROI is to detect the face and ROI for each frame. However, the Viola–Jones bounding box is not very accurate and can report false positives and negatives [117] along with additional computational power in the case of real-time applications [117]. Kanade–Lucas–Tomasi (KLT) was used by various researchers to track feature points from a face to update ROI location [113], [119], [120], [121], [122]. Research has also used Openface [123], [124] and hyperbolic embedding graph structure [125], multitask cascaded convolutional networks (MTCNNs) [126] to obtain ROIs. Various parts of the body have been used as ROI to obtain vitals [127], [128], [129], [130], such as the entire face, forehead, and palm. Others have also segmented face into several patches to obtain better signals [66], [131], [132].

### B. Signal Extraction and Preprocessing

Here, the raw signal from the ROI image data over a given period is extracted. Raw signals from a color image include RGB channels and values obtained from each channel of the image frame are averaged over all pixels at a time period. Researchers have also used IR channel to obtain these values in addition to color [66], [133]. For example, red channel pixels averaged for ROI image data for a time period of 60 s $[s_R(t), s_G(t), s_B(t)]$ with $s$ the signal obtained over time $t$ for RGB channels. This process is called spatial pooling, and it helps average the noise contained in each pixel [18], [46], [134], [135], [136], [137].

### C. Reducing Noise, Applying FFT, and Filtering

After the raw signal is obtained, the signal (S) containing data from all channels $[S = s_r, s_g, s_b]$ is passed through a signal separation process, e.g., independent component analysis (ICA) or principal component analysis (PCA). This is applied as the signal can contain noise due to skin tone, light source, or movement. Signal separation processes extract a clearer signal from the raw signal input [18], [46], [134], [135], [138]. FFT is applied to raw signals to convert them into the frequency domain. The signal is enhanced by removing unwanted frequencies, increasing signal-to-noise ratio (SNR) [139], [140]. Bandpass filters are often used to remove low and high frequencies, e.g., 0.65 and 3.5 Hz [18], [46], [134], [135], [141], [142], [143].

### D. Extracting Vitals and Reliability Checks

Vital sign data are extracted from the signal [18], [46], [134], [135], [144], [145], [146], [147], [148], [149]. A peak is identified from the signal to obtain HR data. HR is calculated by multiplying the frequency value on that peak by 60 to convert it into BPM, and for respiratory rate (RR), it is multiplied by the ratio of the number of peaks over a time

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

TABLE I
INCLUSION AND EXCLUSION CRITERIA FOR rPPG LITERATURE REVIEW

| Inclusion Criteria | Exclusion Criteria |
|---|---|
| **Focus**: On HR, $SpO_2$ and methods or techniques for measuring these signs. | On blood pressure and general health and activity monitoring. On security, perception, management, face detection and/or advantages of remote health monitoring. On economic, post-operative health monitoring involving carers. |
| Remote sensing with **camera-based** tech. | Contact-based monitoring, e.g., wearable (including pulse oximetry), wireless sensors or radars. |
| **Protocol**: Human participants able to consent, in a conscious state within a lab, clinic or home setting. | Experiments on animals or people who cannot consent for themselves. Measuring driver state or accident monitoring. Not reporting a complete experiment protocol, a complete system evaluation, or not peer reviewed. |
| **Language:** English. | Published in other languages. |

period. Researchers used various methods to obtain $SpO_2$ from the pulse signal, which is mentioned in Section V-B. Only two surveyed papers [66], [150] used SNR ratio and previous estimates within a window to perform consistency checks to ensure history-based reliability of vital signs data.

## IV. METHODOLOGY

For this survey, we applied a metaanalytic approach to systematically evaluate the performance of noncontact HR and $SpO_2$ measurement systems on reviewed literature. We used PubMed, MedlinePlus, ACM, IEEE Xplore, and Springer databases with the keywords: *remote*, *noncontact*, *HR monitoring*, *blood oxygenation level*, and *rPPG*. The date range for the review was January 1990–October 2022, from which 16 389 records were identified. This was refined to 2416 after screening and then reduced to 187 (after removing 394 duplicate records, and applying the criteria in Table I). A second round was made based using the same criteria, to include research published in October 2022–September 2023. In this round, 57 papers were added. A final round of review, added 132 publications from September 2023 to February 2024.

## V. LITERATURE REVIEW FINDINGS: PREVIOUS WORK

This section provides details of surveyed research on rPPG systems, performance, conditions, and limitations. Most of the surveyed publications focus only on HR [151], a few focus on $SpO_2$ and much fewer focus on both. The system performance metrics [root mean square error (RMSE), r-correlation, and standard deviation error ($\sigma$)] of the previous work are listed in Table III (in Supplementary material) for HR and Table II (in Supplementary material) for $SpO_2$ [29]. These noncontact-based rPPG systems have been validated by comparing their performance against clinical or commercial counterparts (i.e., contact-based ground-truth devices). Research conditions and participant information are in Tables IV and V (in Supplementary material) [29].

### A. Remote HR Measurement

We delve here into surveyed research measuring HR with rPPG, and their approaches for face identification, ROIs, signal extraction, participant movement, and other environmental characteristics, all under the lens of their effectiveness and potential for deployment in real environments.

*1) Face Identification:* Thermal cameras can be used for rPPG data capture [74], [75]. Information about cardiac pulse, blood flow, and breathing rate can be extracted and the face movement tracked, with blood vessel registration used as ROI. After extracting the thermal signal and removing noise, a Fourier transform is applied to obtain a pulse signal. The performance of one of such systems [74] is 88%, but RMSE, r-correlation or mean absolute error (MAE) were not reported. In addition, the data gathering took place in a controlled illumination and participants' movement was restricted (still state). The system might not perform well in a real-life scenario as illumination may vary and participants are not restricted from movement. Furthermore, this thermal equipment can be prohibitively expensive [76], [117]. Similarly, Gatto [76] used a thermal camera, with the forehead as ROI, to measure and analyze the signal data to generate HR. During data acquisition, if the participant changed the head position in any direction, the system failed to capture data from the defined ROI. Box et al. [152] used the autoregressive moving average (ARMA) model to obtain HR from the signal. The main drawback is that the participant's movement in real life can fail the system since it only tracks the forehead. In the case of a headscarf or longer hair, it is also highly likely to produce a reading that is not accurate. Along with that, a person's body temperature (BT) and environmental temperature could impact the signal extracted from a thermal video. The expensive thermal equipment would also make it unfeasible to deploy on a low budget [117], [153].

Remote HR measurement has also been achieved with CCD cameras. Researchers used 30 mean seconds of image data captured from the camera and analyzed the change in brightness on participants' face regions from the cheeks. After analyzing the signal data obtained from participants, HR peak was identified [78]. CCD camera and dual-wavelength LED lighting have also been used to measure HR but required a dark room and participants to have closed eyes, which may be impractical and uncomfortable [154]. In addition, it is more vulnerable to ambient light and motion artifacts. Another study used a CCD camera to measure HR remotely. It focused on participants' movement and noise from light using chrominance rPPG to remove specular reflection variation. They used a combination of red and green channels to extract signals from defined ROI [79]. A study introduced a dual-bridging network to align domains and synthesize target noise, coupled with adversarial noise generation and hard noise pattern mining, aiming to boost rPPG model robustness [155]. Once again, these studies were conducted in a controlled setting or used public datasets with specific lighting. Deploying this system in a real-life scenario could impact the results (inaccurate readings) due to various types of illumination present in realistic environments. CCD camera used in this research is also expensive and bulky [78], [117].

Studies obtained HR used a laptop camera to acquire face color images consisting of RGB channels. ICA, FFT, and a frequency filter were applied to the channel data (RGB) to obtain the pulse signal. The second component (green channel)

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

was found to typically produce the strongest pulse signal in this research study [80], [156], [157], [158], [158]. This was further refined through signal preprocessing such as detrending and smoothing the signal data. The system was updated to select the highest peak after applying FFT and filter, which was further smoothed by moving average filter [81]. However, the study was conducted within a laboratory setting (in a controlled environment) with a limited number of participants ($n = 12$). In addition to that, restricted movement within a controlled environment does not replicate realistic environments. The face tracker used in the study detected multiple or no faces which the system handled by using the previous face captured; however, this method can fail in a real-life setting as it may not capture the real vital reading over time (using the previous face for a certain time) resulting in inaccurate HR readings.

*2) Regions of Interest (ROIs):* Several researchers used various ROIs from face images obtained from participants to measure HR remotely. Face ROIs included full face, forehead, lips, eyes or nose, and cheeks, which varied in pixel size. These ROIs may contain regions which cannot provide information related to HR, for example, eyes, teeth, and beards, which can impact the overall performance of results. In the case, where only the mouth area is focused to obtain HR, it can impact the error rate when a person is talking or laughing as teeth do not provide a pulse signal to obtain HR. To address this problem, researchers [113] introduced neural networks for skin classification [159] to determine skin color from the face image. This ROI (skin pixel) was labeled and tracked using a mean-shift tracker, which iteratively shifts points of data to the average of points of data nearby [122]. The HR was obtained after applying FFT and used a data adjustment scheme which resulted in obtaining HR in a short time. This work was further extended using multiple video data, which reduced the error rate [160], though with no variety in light sources nor freedom of movement of participants expected in realistic settings.

*3) Signal Extraction:* Researchers most commonly used PCA [108], [133], [161], [162], [163], [164], ICA [113], [165], [166], [167], [168], [169], [170], [171], [172], [173], [174], FastICA [52], [113], [119], [166], [168], [169], [175], [176], [177], [178], [179], [180], [181], [182], RobustICA [183], joint approximation diagonalization of eigenmatrices (JADE) [184], and also Laplacian eigenmap (LE) algorithms [185] for extracting source signals from RGB channels to obtain HR. Wei et al. [185] used LE to extract signal sources from the face data obtained from participants. LE is also a dimensionality reduction technique but is nonlinear to find the internal structure of the data. The research revealed better results in comparison with other dimensionality reduction techniques. Where one study suggested bypassing PCA or ICA to enhance processing speed, though this approach might not sufficiently reduce signal noise, potentially compromising effectiveness in real-world scenarios [186].

Eulerian video magnification (EVM) has been used to measure changes in the face region of the participants. The data were obtained in the form of a video that was spatially decomposed into various frequency bands to which temporal filtering was applied and finally amplified by a factor. This was implemented on data where participants were in a still state [187]. Other studies followed a similar approach to estimate HR and RR from video data as well [188], [189], [190], [191], [192], [193]. This method is not feasible for HR measurements in realistic settings, where a person could be in motion. In addition to that, this method may not work well when there is high noise present in the signal. Ciftci and Yin [194] presented a method to generate facial videos with varied HR by synthesizing effects on skin color, aiming to enrich HR estimation research with sufficient annotated videos. However, ensuring the realistic synthesis of HR effects across all facial regions and skin types in synthetic videos remains a challenge [194]. Kossack et al. [195] evaluated the tissue perfusion using locally resolved rPPG signals from RGB data to enable the detection of whether a tissue is adequately supplied with blood across different scales. However, challenges include analyzing rPPG signals under changing lighting conditions, occlusions, and movements, affecting accuracy [195]. Other studies have also proposed methods for measuring [154], [196] and mapping rhythmical phenomena in tissue perfusion [197]. Some studies also used dual-wavelength measuring HR [198], [198], [199]. Research conducted also used machine learning techniques such as deep learning, convolutional neural network (CNN), and unsupervised and more to measure remote HR [106], [134], [200], [201], [202], [203], [204], [205], [206], [207], [208], [209], [210], [211], [212], [213], [214], [215], [216], [217], [218], [219], [220], [221]. However, these studies need to ensure the real-world applicability of these models so it can be generalized across diverse environmental conditions and demographics for effective training. This can be a considerable challenge to extending these technologies to broad, practical applications.

*4) Participant Movement:* Monkaresi et al. [222] allowed more movement among participants, but they used a machine learning approach to select the pulse component among all channels (RGB components) instead of choosing a single pulse component to identify peaks [80]. This approach includes applying power spectrum analysis, $k$-nearest neighbor (KNN), and linear regression to each component extracted after applying ICA to obtain features and classify them. KNN outperformed linear regression for selecting pulse signal components to obtain HR. However, generalizing the model among the participants can bear different results or not perform well when new participants are introduced to the system on which it has not been trained yet and may therefore fail in a real-life scenario. Furthermore, the study was conducted in a controlled environment with specific light conditions.

To cater to challenges associated with different illumination and participant movement, Li et al. [177] used a technique based on normalized least mean square (NLMS) adaptive filtering and face tracking using the Viola–Jones face detector [223] to overcome these challenges. NLMS is an extension of the least mean square (LMS) adaptive filter, which is used to simulate the selected filter. NLMS was used on raw signals to improve the data impacted by different light variations. To identify and locate face landmarks discriminative response map fitting (DRMF), the method was used in the initial image frame. KLT [224], [225] algorithm

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

was then used to continue tracking the ROI. Researchers used the MAHNOB-HCI [226], [227], [228], [229], [230], [231], [232], [233], [234], [235], [236], [237], [238], [239] dataset for research studies to test their techniques. The results from their research exceeded the accuracy of previous studies. However, the database contains data obtained in a controlled environment with only slight movement in a laboratory setting. ROI tracking also fails when participants move at an extensive angle and participants' facial expressions create noise which then shows high variations in the obtained signal. Researchers have used datasets collected from lab setups to test and validate their methods, such as ARPOS [240], PURE [235], [238], [239], [241], [242], [243], [244], [245], [246], [247], [248], [249], [250], COHFACE [238], [239], [249], [251], MMSE-HR [238], [247], [250], [252], BH-rPPG [253], IIPHCI [249], [254], MPSC-rPPG [255], DOHA [256], OBF [237], [246], [250], [257], VIPL-HR [236], [258], [259], [260], [261], DEAP [262], [263], and UBFC-RPPG [235], [238], [239], [242], [243], [244], [245], [246], [247], [250], [264].

Bousefsaf et al. [265] used a method to select the most suitable ROI pixels, segmenting the face region into various subregions on the basis of lightness dispersal. The most suitable subregions were then chosen and grouped by assessing their SNR [265]. Another study focused on improving signal quality by reducing noise obtained from participants' face data by applying the block-based spatial–temporal on the face data. The spatial–temporal quality dissemination of the face ROI was then calculated depending on SNR. Adaptive ROIs were obtained by computing mean shift clustering and adaptive thresholding SNR maps, which then increased the accuracy of estimating HR [266], [267]. However, the system validation is limited to only control laboratory-based environments and needs to be stress tested for realistic environments. Laurie et al. [268] introduced an exposure control algorithm for optimizing the SNR by adjusting the camera's exposure time to maximize it without distortion. However, the algorithm is sensitive to subject movement and has a longer execution time compared with standard controls. It requires participants to be relatively still to maintain accuracy, as movement can lead to color channel saturation. Its longer execution time may limit its use in real-time or emergency situations [268]. A study used Kinect V2 and tracked skeletons to obtain HR and RR by monitoring the chest region movement with and without a blanket over a participant. This was to monitor cardiopulmonary irregularities such as bradycardia to process unclear ROI under well-lit and dark light conditions with different sleeping positions. In case abnormalities were detected, an alarm would be triggered to notify the career [90]. However, the system may fail if a participant is sleeping on their stomach. Another constraint is the reliability of movement features to obtain the vital, which can create inaccurate observations for different types of motions, such as walking, talking, or microfacial gestures. These voluntary movements can impact the reliability of the vital data obtained. A robot with a video camera incorporated has also been used to obtain HR. The aim was to design a robot for older adults to do some exercise and measure their vital [241]; however, the accuracy drops with movement. Another research used a robot with color and IR to measure HR [269]. However, these systems are not inexpensive which can be difficult to deploy on budget, especially for those within the middle to lower income households around the world. Others capture rPPG from fingers [270], [271] which may be impractical when deployed in a real-life setting.

Most studies restricted participants from any movement [272], such as a person moving their head or walking around in the room, and even the motion of facial features such as while talking. In a real-life situation, these movements would be expected, which can increase noise when calculating vital signs. Research focusing on the head motion of participants has been addressed by the authors [107], [119], [273], [274], [275], [276], [277], [278], [279], [280], [281], [282], [283], [284], [285], [286], [287], [288], [289], [290], [291], [292], [293], [294], [295], [296], [297], [298], and [299]. Where one of the researchers suggested tracking velocities of feature points on the face using Viola–Jones face detector and then tracking ROI by using KLT [107]. While other researchers focused on a single ROI, specifically the forehead [300], [301], [302], this was as microexpressions below the eye line are prone to more motion compared with the forehead [301]. Researchers have also addressed this movement-based HR monitoring by using face quality assessment (FQA) to discard low-quality image frames, limiting the noise in the final obtained values. FQA uses four parameters, including resolution, luminance, sharpness, and face trajectory, to determine if the image requires to be removed. To track face feature points, the good feature tracking (GFT) method was used on the image obtained. Landmarks from the face were obtained using the supervised descent method (SDM) combined with GFT to obtain face feature points and track movement and hence provided improved signal quality to obtain HR [303]. However, these motions were restricted and conducted in a controlled manner within a laboratory setting. The systems deployed by the researchers had specific hardware requirements (e.g., large random access memory (RAM) and graphics processing unit (GPU) were needed) for these techniques, including controlled guidance to participants which is not feasible in real-life environments. Furthermore, people from lower to middle income backgrounds cannot take advantage of the system requiring expensive hardware [304], [305].

*5) Other Environmental Concerns:* In addition to the above, a single ROI such as the forehead can fail where a participant is not fully facing the camera. Furthermore, various research methods focusing on measuring HR need to be validated within realistic environments to check how different factors such as illumination, facial hair (such as beard), makeup, and frames per second (FPS) impact signal data used to obtain vital sign data [306], [307], [308], [309]. To increase SNR, some researchers use a monochromatic camera with a green range filter. This study also used weighted averages on the various face ROI. A deformable face fitting algorithm and KLT tracking [224], [310] algorithm tracked and extracted face features [49]. However, the RMSE obtained from this research is very high as shown in Table III (in Supplementary material), making it an inadequate method for real-life systems. Another study, by Zheng et al. [311], used EVM,

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

quality assessment (QA) of signal, and adaptive chirp model decomposition (ACMD) to obtain HR. They validated the system in different illuminations and with some head motion. Researchers anonymised facial-rPPG videos to protect identity during vital sign measurement [312], [313], [314], [314]. However, its applicability may vary in different real-world conditions due to factors such as lighting, movement, and camera quality.

Hasan et al. [315] introduced RhythmEdge which focused on model compression for use on devices with limited resources to obtain HR. It applies a multitask learning framework to handle sensor differences, enhancing versatility. However, it faces challenges with camera variability, lighting, subject movement, and device limitations, which may affect measurement accuracy and consistency [315]. Different researchers also looked into ambient, natural, and varying illumination [124], [316], [317]; however, once again, the setup was within a controlled setting where participants were at a distance of 0.6 m from the camera. The participant diversity information was not revealed in this article. In addition to that, only the forehead is selected as ROI which would fail if the participant is not facing the camera.

Wang et al. [318] proposed a new continuous-spectrum IR illuminator using phosphor LED technology, addressing limitations of previous light sources. It offers improved color homogeneity and energy efficiency for multiwavelength near infrared PPG (NIR-PPG) setups, useful in dark environments and nonobtrusive monitoring applications [318]. This article acknowledges limitations in the prototyping phase, including difficulties in achieving consistent color homogeneity and adapting the illuminator to various spatial constraints and power needs. While effective in dark settings and with body motion, further validation is needed across diverse real-world conditions [318].

To address environmental challenges, particularly those posed by uneven lighting and color variations, Song et al. [319] employed a combination of ensemble empirical mode decomposition (EEMD) and multiset canonical correlation analysis (MCCA) to specifically address spatially uneven illuminations. Decomposing the green signal and extracting the pulse enhances the robustness against uneven lighting. Ahmadi et al. [320] used amplitude-selective filtering (ASF) and color-distortion filtering (CDF) to counteract the effects of spatial variations in skin color and lighting. Whereas Lu et al. [321] introduced neural structure modeling (NEST), aimed at enhancing the generalization of rPPG models across different unseen environments. NEST tackles the domain shift challenge in rPPG tasks through three main strategies: optimizing feature space coverage, aligning multidomain features at an instance level, and enriching discriminative features. Only one study [66] was found that was conducted in participants' homes, involving different camera-to-subject distances, and shared its open dataset. However, it reported a higher error rate, particularly among individuals with darker skin tones and those in an active state [66]. van Esch et al. [322] used RGB cameras in a hospital environment, applying machine learning to detect cardiac arrhythmia, including atrial fibrillation and flutter, without limiting patient movement. Although it is a significant advancement in noninvasive cardiac monitoring, the study highlights a persistent challenge: the difficulty in accurately differentiating arrhythmia due to their similar signal characteristics, especially when patients move. This issue underscores the need for refinement of the detection models.

### B. Remote $SpO_2$ Measurement

Relatively few studies used methods to obtain $SpO_2$. One method, canceling aliased frequency components induced by light flickering (based on autoregressive modeling and pole cancellation), improved its effectiveness under fluorescent illumination [323]. The research was conducted on patients undergoing kidney dialysis (at rest, with minimal movement) [323]. However, movement and illumination change increased noise, in turn impacting system accuracy. The research also does not provide RMSE, r-correlation, or $\sigma$ for $SpO_2$. While using a webcam, another research measured $SpO_2$ and HR by using an algorithm for noise removal based on dual-tree complex wavelet transform (DTCWT) to fix motion artifacts and artificial illumination [32]. RGB channels have been used to obtain $SpO_2$ by assessing the pulse signal at two wavelengths of 660 and 940 nm [324], comparing red and blue wavelength bands and using a 50-cm range [32], [324], [325].

A study used wavelet transform denoising to address lighting and movement artifacts. It was validated for healthy individuals and pediatric intensive care unit (PICU) patients, noting the impact of Hb levels on estimation accuracy. Despite showing strong correlations with oximeter readings, the method faced challenges in accurately estimating values for anemic patients and requires further validation across varied clinical conditions [32]. Kim et al. [326] measured $SpO_2$ using RGB camera and YCgCr color space, enabling estimation in ambient light without direct contact. It leveraged absorption differences of Hb for $SpO_2$ analysis. However, movement, lighting, and makeup on signal quality, and its validation is limited to $SpO_2$ levels of 85%–100%, indicating a need for broader testing [326]. Another research used RGB webcams, focusing on enhancing noise resistance and accuracy through BSS and energy coefficient analysis. However, it has only been validated on a small and homogeneous group of participants. In addition, as with most research, this needs to be validated in a real-life setting to further evaluate the system [327]. Stogiannopoulos et al. [328] used IR and EVM to highlight skin pixel intensity variations for nighttime monitoring to obtain $SpO_2$. It evaluates machine learning regression techniques like the generalized additive model (GAM) and extra trees regressor, alongside deep learning approaches including 3-D CNN and video vision transformer (ViViT), on amplified PPG signals from facial videos demonstrating an acceptable range of accuracy. However, validation primarily under controlled conditions and the method's adaptability to varying equipment and environmental settings may be a challenge when replicating to real-world scenarios [328].

Researchers also measured $SpO_2$ using ambient light and two cameras equipped with narrow-band filters at wavelengths of 660 and 520 nm. The need for precise alignment and adjustment due to the use of two separate cameras and

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

potential challenges in filtering out motion artifacts and other interferences in ambient light conditions is a challenge. The method also depends on the ambient light's intensity and spectrum, which might limit its applicability in varying environmental conditions [329]. Verkruysse et al. [330] used digital RGB cameras and Monte Carlo simulation for light transport analysis. This was validated in controlled conditions for an $SpO_2$ range of 83%–100%. The study acknowledges limitations, including its validation in a controlled environment, a small sample size, and challenges in adapting to uncontrolled conditions like variable lighting and movement [330].

Another approach [66] to measuring $SpO_2$ uses the extinction spectra of oxy-Hb and deoxy-Hb, via a ratiometric measurement technique, dividing the recorded pixel intensity between two distinct spectral ranges, red (600–700 nm) and IR (800–900 nm) to obtain this vital data. The reported error rate was consistent over all participants of diverse skin tones in resting and active states of ±2%, but this was not yet clinically validated. To obtain $SpO_2$, Al-Naji et al. [331] used EEMD and ICA. However, the system's use of visible light cameras may face issues like unclear ROI from movement and skin tone challenges. In addition, further real-world validation is needed to confirm its practicality [331]. Other researchers used a complementary metal–oxide–semiconductor (CMOS) camera and dual-wavelength LED illumination at optimized wavelengths (611 and 880 nm), showing strong accuracy and consistency across a clinically relevant $SpO_2$ range. Despite its innovation, limitations include hardware dependency, sensitivity to environmental conditions, and a validation range of 83%–100% $SpO_2$, suggesting a need for further clinical and real-world validation [332]. Xi et al. [333] employed singular spectrum analysis (SSA) for signal decomposition and a spectral masking algorithm to measure $SpO_2$. Once again, it has been tested in controlled settings and requires validation for motion and skin tone [333]. Researchers also used a deep learning approach for measuring $SpO_2$ by employing a spatial–temporal map (STMap) for data encoding. However, challenges such as the need for broader clinical trials and data standardization were highlighted [261]. One approach uses hand palms to measure $SpO_2$ by applying spatial averaging, obtaining RGB time series, and applying a CNN [95], [334]. However, using palms or fingers under a camera is impractical in real-life due to the need to keep hands still. In addition, hands are a less exposed part of the body compared to the face, which would make it difficult to deploy it in real-life scenarios [95], [270], [334].

A variety of equipment has been used for rPPG, including CCD cameras, smartphones, laptops' webcams, drones with cameras, and Kinect. Each device has its characteristics such as resolution, dimensions, processing power, and data type collected and cost. Low- and high-resolution digital cameras, and smartphone cameras capture RGB channels have been used in most studies to obtain vital values; whereas thermal cameras allow capturing the thermal data of a participant. However, smartphones need to be held continuously, which can be impractical for long periods. Also, the cost of thermal [76], [117] and CCD equipment [78] may be prohibitive for certain deployments (as discussed in Section V-A).

## VI. Limitations of Existing rPPG Systems

In what follows, limitations of reviewed rPPG systems are summarized, with areas for further research and improvement.

### A. Equipment Limitations

Thermal and CCD cameras used in these studies can be prohibitively expensive [76], [117], [153], [304], [305], [335]. A problem with using a thermal camera is that it can generate temperature from the body and also the environment, which can impact the data acquired from a participant, such as thermal noise [117]. Furthermore, ambient sensing of oxygen saturation through multispectral imaging has been explored but using specialist scientific equipment which can be expensive to measure $SpO_2$ [336], [337], [338], [339], [340]. These studies have primarily been conducted in laboratory settings, utilizing specialized hardware with ample RAM and GPU resources. However, this laboratory-based approach may not readily translate to real-world environments. In clinical or home settings, individuals may be positioned at varying distances from the equipment, making it essential for the system to deliver accurate readings under diverse circumstances. All of the research studies (except one [66] conducted among participants' homes) used specific hardware to acquire data with camera FPS set at 15, 30, or 60 as shown in Table V (in Supplementary material) [29]. This ensured a constant FPS for each RGB channel. The system (code) and equipment (computer and camera) were set up by the researcher in all studies and had enough processing power, RAM, graphics card, and storage space to collect this data. However, people in a real-life scenario may not have access to expensive scientific equipment where the RAM, graphics card, and GPU may impact the FPS and in turn, impact the number of samples in a signal obtained for each channel and if the system does not cater to this, it may impact error rate of the system. FPS impacts signal quality that is used to obtain vital data obtained data from realistic scenarios [66]. Bit depth, with 8 bits per channel (multichannel), is prevalent; however, a higher bit depth could yield a cleaner signal. Developed rPPG systems report using various resolutions and equipment, as shown in Tables IV and V (in Supplementary material). The quantum efficiency needed for this improvement remains uncertain and needs further research. In addition, the precise impact of parameters such as resolution and bit depth on accuracy is not well understood, indicating further research.

### B. Controlled Environments

rPPG studies have predominantly been conducted within controlled environments where only one study evaluated their system in participants' homes. While it is important to initially test and validate these systems in controlled environments, it is equally crucial to evaluate their performance in real-world scenarios, particularly within clinical settings. Clinical environments encompass a wide range of HR and respiratory conditions, involving diverse participants. Real-world validation against clinical standards is vital for ensuring the effectiveness and reliability of such systems. Researchers need to ensure they share evaluation measures when discussing the results of their research systems to progress in the field.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

Currently, there is no commercially available (and clinically validated) rPPG systems able to monitor these vital signs. It is crucial for such systems to be validated in real-life environments including laboratories, homes, and clinics to stress these systems. Furthermore, the effectiveness of these systems for monitoring health in clinical settings has yet to be fully validated. It is crucial that rPPG systems demonstrate the ability to promptly identify patients at the highest risk of health deterioration, highlighting the significant advantages of utilizing such remote technology in healthcare.

### C. ROI Selection and Occlusion

Using a single ROI can prove ineffective in measuring vital signs. This limitation becomes evident when the chosen ROI is obscured from the camera's view, for instance, when a person wears a headscarf or has long hair that conceals the forehead, or when the individual is positioned at an oblique angle to the camera. Therefore, it is crucial to test systems comprehensively across diverse settings to validate their performance and evaluate their error rate.

Tracking people can also be occluded by objects, other people, or both from the camera's view to send data to the system which is common for front-viewing cameras used by the systems [341]. Due to occlusion, a user's skeleton cannot be identified; however, there are several methods to address this issue, including hand over face occlusion [342], API tracking of multiple people's positions in environments where occlusion occurs [341], [343], [344], location-aware wearable haptics [345], sound localization [346], using API, a toolkit to track and multiple cameras within an environment to track multiple peoples and joints using depth data [341], and using shadow and skeletal fusion data to track people within an environment [347]. Occlusion in rPPG systems needs to be further studied.

### D. Participant Diversity and Experiment Conditions

Most of the surveyed research in [29, Tables IV and V] have a small number of participants and a small variation in skin tone. For $SpO_2$ specifically, all studies included fewer than 15 participants (except one [66] as shown in [29, Table II]. Similarly, for HR measurement, most studies had a small number of participants [348], [349], [350], [351], [352], [353], [354]. Only three studies stood out with a larger number of participants [66], [79], [311]. Among these, two studies involved 40 participants each [66], [311]. However, only one of these studies collected vital sign data within realistic home environments, encompassing both HR and $SpO_2$ measurements [66]. The third study [79], which included 117 participants, focused on measuring HR only and was conducted in a controlled environment resembling a studio setup with limited movement and using expensive equipment [79]. The remaining studies surveyed in Table IV (in Supplementary material) had much fewer participants and strict experiment conditions. Furthermore, most of the surveyed studies in Table V (in Supplementary material) did not measure oxygenation levels at a distance [29].

The surveyed literature considered only one participant at a time (with exceptions, with up to six participants [46], [66]). Measuring multiple participants simultaneously is required, especially in shared environments. All the research studies mentioned above had participants closer to the camera (up to 0.5 m from the camera). Very few studies measured HR up to 4 m [66], [90], up to 60 m [355], and up to 100 m [356]. For participants whose HR was measured at up to 100 m, light reflectance was lower. Reduced ROI at long distances also impacted accuracy as shown by large MAEs with greater imager-to-subject distances [356]. Most studies do not disclose participant characteristics and typically focus on a specific demographic [320] limiting the generalizability of the findings, including women, older adults, or individuals with cardiovascular conditions. A wider range of demographics and skin tones need to be included in research studies.

Realistic environments are varied (e.g., homes and triage rooms in clinics and hospitals) and various factors, such as facial expressions, rotation, distance from the camera, illumination, facial hair, and skin tone can impact the system's obtained data. Parameters related to makeup and beard were only reported in two publications, albeit with a small number of participants [66], [357] and one study also does not analyze or segment results based on these parameters [357]. These experiments ought to be conducted with diversity in mind (both environmental and experimental).

### E. Datasets

Most of the surveyed studies did not share data or code. Publicly available datasets were collected under laboratory conditions with restricted parameters such as light, movement, and fixed camera distances. There is a lack of publicly available data collected from a real-life environment, so the system evaluation measures can be tested on those to evaluate their system [46], [66]. Only one dataset includes data from home environments, yet this did not include participants with black skin tone [66]. Studies conducted restrict participants from microfacial gestures or physical movement during vital data acquisition. In addition, if the error rate is not evaluated for realistic environments with natural movement or for example during undergoing treatment, it can result in failure to accurately measure vitals due to the presence of noise. Therefore, it is essential to measure vital sign data in real-life environments [46], [66]. Face tracking will also impact ROI selection when movement takes place, depending upon the lighting, and exposure length of the camera, it could potentially create blurry frames, and it is important to analyze data with noise to ensure the system will be able to perform as required in a real-life environment [46]. It would be more beneficial if video streams of color, IR, and depth videos would be made available open source so researchers can analyze the realistic data including various movements, illumination, environments, skin tone, and other factors with their respective timestamps to analyze their algorithms.

## VII. Bias in rPPG Systems

The use of camera-based technology to capture facial data poses some challenges in rPPG systems, in particular, due to the diversity of skin tone in humans [69]. rPPG systems must be highly accurate for clinical use. Therefore,

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

the rigorous validation and extensive testing across a diverse range of participants are imperative. Many publicly available databases primarily emphasize individuals with lighter skin tones. Neglecting diversity can pose a significant disadvantage when deploying rPPG systems; making it beneficial only for a specific group of people. One study [49] reported a higher error rate in such cases. Another study [66], reported a lower error rate and introduced effective techniques across a range of skin tones. A critical observation from this review is the limited consideration given to participants who wear makeup (e.g., lipstick or concealer), or those with facial hair. These factors can significantly influence the accuracy of data readings in rPPG systems. Only two research studies were found that stated participants wearing makeup [66], [358]. Both studies found makeup in color and IR impacted the accuracy of the rPPG systems and suggested further rigorous testing. However, only two studies [66], [358] reported participants wearing lipstick or foundation. Consequently, it becomes important to rigorously validate these systems, accounting for bias, and further evaluating their performance across a wide demographic.

## VIII. Summary

This article offers an in-depth review of rPPG-related research that can measure HR and/or $SpO_2$. Processes, techniques, participant characteristics, equipment, and experiment conditions used in the surveyed research were discussed, as well as the performance, evaluation measures and limitations of these studies. The majority of the studies focused on measuring HR, a few on $SpO_2$ and very few on both. Previous research needs to consider various factors when designing an rPPG system including varying camera-to-subject distances, fluctuating frames per second, computational resource requirements, diverse environments, illumination conditions, and participant diversity. Furthermore, it is crucial to validate systems under conditions involving natural movements during vital sign measurements to improve accuracy. This issue is critical when considering real-world deployment and clinical use.

In conclusion, the field of rPPG has made significant progress in recent years. We have highlighted various aspects of these methods for measuring HR and $SpO_2$, identifying several important findings and research challenges. Addressing these challenges is crucial for advancing this field, as rPPG has great potential for clinical and nonclinical applications. This article serves as a valuable resource for researchers seeking to further improve the accuracy and reliability of these systems in real-world scenarios as this continuously evolving field grows.

## References


[1] C. Brüser, C. H. Antink, T. Wartzek, M. Walter, and S. Leonhardt, "Ambient and unobtrusive cardiorespiratory monitoring techniques," *IEEE Rev. Biomed. Eng.*, vol. 8, pp. 30–43, 2015, doi: 10.1109/RBME.2015.2414661.

[2] T. Chakrabarti, S. Saha, S. Roy, and I. Chel, "Phonocardiogram signal analysis–practices, trends and challenges: A critical review," in *Proc. Int. Conf. Workshop Comput. Commun. (IEMCON)*, Oct. 2015, pp. 1–4, doi: 10.1109/IEMCON.2015.7344426.

[3] D. H. Spodick, P. Raju, R. L. Bishop, and R. D. Rifkin, "Operational definition of normal sinus heart rate," *Amer. J. Cardiol.*, vol. 69, no. 14, pp. 1245–1246, May 1992, doi: 10.1016/0002-9149(92)90947-w.

[4] R. A. S. Taghavi, *Hypovolemic Shock*. National Center for Biotechnology Information, 2022.

[5] A. A. Venessa, L. Pinto, and P. Tadi, *Increased Intracranial Pressure*. National Center for Biotechnology Information, 2021. [Online]. Available: https://europepmc.org/article/NBK/nbk482119#impact

[6] A. S. Popel, "Theory of oxygen transport to tissue," *Crit. Rev. Biomed. Eng.*, vol. 17, no. 3, p. 257, 1989. [Online]. Available: https://pubmed.ncbi.nlm.nih.gov/2673661/

[7] B. B. Hafen and S. Sharma, *Oxygen Saturation*. Treasure Island, FL, USA: StatPearls, 2022. [Online]. Available: http://europepmc.org/books/NBK525974

[8] S. R. Majumdar, D. T. Eurich, J.-M. Gamble, A. Senthilselvan, and T. J. Marrie, "Oxygen saturations less than 92% are associated with major adverse events in outpatients with pneumonia: A population-based cohort study," *Clin. Infectious Diseases*, vol. 52, no. 3, pp. 325–331, Feb. 2011, doi: 10.1093/cid/ciq076.

[9] A. Plüddemann, M. Thompson, C. Heneghan, and C. Price, "Pulse oximetry in primary care: Primary care diagnostic technology update," *Brit. J. Gen. Pract.*, vol. 61, no. 586, pp. 358–359, May 2011, doi: 10.3399/bjgp11x572553.

[10] V. Kim, J. O. Benditt, R. A. Wise, and A. Sharafkhaneh, "Oxygen therapy in chronic obstructive pulmonary disease," *Proc. Amer. Thoracic Soc.*, vol. 5, no. 4, pp. 513–518, May 2008, doi: 10.1513/pats.200708-124et.

[11] J. Buekers et al., "Wearable finger pulse oximetry for continuous oxygen saturation measurements during daily home routines of patients with chronic obstructive pulmonary disease (COPD) over one week: Observational study," *JMIR mHealth uHealth*, vol. 7, no. 6, Jun. 2019, Art. no. e12866, doi: 10.2196/12866.

[12] E. A. Kiyatkin, "Respiratory depression and brain hypoxia induced by opioid drugs: Morphine, oxycodone, heroin, and fentanyl," *Neuropharmacology*, vol. 151, pp. 219–226, Jun. 2019, doi: 10.1016/j.neuropharm.2019.02.008.

[13] B. B. E. Shebl, *Respiratory Failure*. National Center for Biotechnology Information, 2021.

[14] B. Govindaswami, P. Jegatheesan, and D. Song, "Oxygen saturation screening for critical congenital heart disease," *NeoReviews*, vol. 13, no. 12, pp. e724–e731, Dec. 2012, doi: 10.1542/neo.13-12-e724.

[15] E. A. Suprayitno, M. R. Marlianto, and M. I. Mauliana, "Measurement device for detecting oxygen saturation in blood, heart rate, and temperature of human body," *J. Phys., Conf. Ser.*, vol. 1402, no. 3, Dec. 2019, Art. no. 033110.

[16] P. S. Ross, F. Hammes, M. Dignum, A. Magic-Knezev, B. Hambsch, and L. C. Rietveld, "A comparative study of three different assimilable organic carbon (AOC) methods: Results of a round-robin test," *Water Supply*, vol. 13, no. 4, pp. 1024–1033, Aug. 2013, doi: 10.2166/ws.2013.079.

[17] M. Ghamari, "A review on wearable photoplethysmography sensors and their potential future applications in health care," *Int. J. Biosensors Bioelectron.*, vol. 4, no. 4, p. 195, 2018.

[18] P. V. Rouast, M. T. P. Adam, R. Chiong, D. Cornforth, and E. Lux, "Remote heart rate measurement using low-cost RGB face video: A technical literature review," *Frontiers Comput. Sci.*, vol. 12, no. 5, pp. 858–872, Oct. 2018.

[19] E. Nemati, M. Deen, and T. Mondal, "A wireless wearable ECG sensor for long-term applications," *IEEE Commun. Mag.*, vol. 50, no. 1, pp. 36–43, Jan. 2012, doi: 10.1109/MCOM.2012.6122530.

[20] N. Rauniyar, S. Pujari, and P. Shrestha, "Study of oxygen saturation by pulse oximetry and arterial blood gas in ICU patients: A descriptive cross-sectional study," *J. Nepal Med. Assoc.*, vol. 58, no. 230, p. 789, Oct. 2020.

[21] N. Joglekar, J. Chandran, R. Veljanovski, A. Stojcevski, A. Zayegh, and M. Dorairaj, "A review of blood gas sensors and a proposed portable solution," in *Proc. Int. Symp. Integr. Circuits*, Sep. 2007, pp. 244–247.

[22] Y. Mendelson, "Pulse oximetry: Theory and applications for noninvasive monitoring," *Clin. Chem.*, vol. 38, no. 9, pp. 1601–1607, Sep. 1992.

[23] F. Chiappini and L. Fuso, "Usefulness of pulse oximetry in respiratory diseases," *Recenti Progressi Medicina*, vol. 88, no. 12, pp. 574–578, 1997. [Online]. Available: https://pubmed.ncbi.nlm.nih.gov/9522598/

[24] A. Kamal, J. Harness, G. Irving, and A. Mearns, "Skin photoplethysmography—A review," *Comput. Methods Programs Biomed.*, vol. 28, no. 4, pp. 257–269, 1989.


Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[25] J. Allen, "Photoplethysmography and its application in clinical physiological measurement," *Physiological Meas.*, vol. 28, no. 3, pp. R1–R39, Mar. 2007.

[26] A. Hertzman and C. Spealman, "Observations on the finger volume pulse recorded photoelectrically," *Amer. J. Physiol.*, vol. 119, no. 2, pp. 334–335, May 1937.

[27] H. Lee, H. Ko, and J. Lee, "Reflectance pulse oximetry: Practical issues and limitations," *ICT Exp.*, vol. 2, no. 4, pp. 195–198, Dec. 2016.

[28] J. G. Webster, *Design of Pulse Oximeters*. Boca Raton, FL, USA: CRC Press, 1997.

[29] P. Pirzada, A. Wilde, G. H. Doherty, and D. Harris-Birtill, "Remote photoplethysmography (rPPG): A state-of-the-art review," *MedRxiv*, p. 20, Jan. 2023, doi: 10.1101/2023.10.12.23296882.

[30] A. Jubran, "Pulse oximetry," *Crit. Care*, vol. 3, pp. 1–7, May 1999, Art. no. R11.

[31] S. Prahl. *Tabulated Molar Extinction Coefficient for Hemoglobin*. Accessed: Jun. 7, 2024. [Online]. Available: https://omlc.org/spectra/hemoglobin/summary.html

[32] U. Bal, "Non-contact estimation of heart rate and oxygen saturation using ambient light," *Biomed. Opt. Exp.*, vol. 6, no. 1, pp. 86–97, 2015, doi: 10.1364/boe.6.000086.

[33] N. Mackenzie, "Comparison of a pulse oximeter with an ear oximeter and an in-vitro oximeter," *J. Clin. Monitor.*, vol. 1, no. 3, pp. 156–160, Jul. 1985.

[34] G. Pang and C. Ma, "A neo-reflective wrist pulse oximeter," *IEEE Access*, vol. 2, pp. 1562–1567, 2014.

[35] A. Azhari et al., "A patch-type wireless forehead pulse oximeter for $SpO_2$ measurement," in *Proc. IEEE Biomed. Circuits Syst. Conf. (BioCAS)*, Oct. 2017, pp. 1–4.

[36] Z. Yuan et al., "A novel reflection pulse oximeter for home health care applications," in *Proc. 5th Int. Conf. Intell. Syst. Design Eng. Appl.*, Jun. 2014, pp. 64–68.

[37] A. M. Luks and E. R. Swenson, "Pulse oximetry for monitoring patients with COVID-19 at home. Potential pitfalls and practical guidance," *Ann. Amer. Thoracic Soc.*, vol. 17, no. 9, pp. 1040–1046, 2020.

[38] L. Martins, O. Gaidos, and I. dos Santos, "Pulse oximeter for cyclists in smartphone," in *Proc. 10th Int. Symp. Med. Inf. Process. Anal.*, vol. 9287, 2015, p. 92870.

[39] M. W. Wukitsch, M. T. Petterson, D. R. Tobler, and J. A. Pologe, "Pulse oximetry: Analysis of theory, technology, and practice," *J. Clin. Monitor.*, vol. 4, no. 4, pp. 290–301, Oct. 1988.

[40] A. H. Işik and I. Güler, "Pulse oximeter based mobile biotelemetry application," *Stud. Health Technol. Inf.*, vol. 181, pp. 197–201, Sep. 2012.

[41] M. Pflugradt, I. Fritzsch, S. Mann, T. Tigges, and R. Orglmeister, "A novel pulseoximeter for Bluetooth synchronized measurements in a body sensor network," in *Proc. 6th Eur. Embedded Design Educ. Res. Conf. (EDERC)*, Sep. 2014, pp. 21–25.

[42] Y. Dai and J. Luo, "Design of noninvasive pulse oximeter based on Bluetooth 4.0 BLE," in *Proc. 7th Int. Symp. Comput. Intell. Design*, vol. 1, Dec. 2014, pp. 100–103.

[43] L. Z. Pipek, R. F. V. Nascimento, M. M. P. Acencio, and L. R. Teixeira, "Comparison of $SpO_2$ and heart rate values on apple watch and conventional commercial oximeters devices in patients with lung disease," *Sci. Rep.*, vol. 11, no. 1, pp. 1–7, Sep. 2021.

[44] A. Khushhal et al., "Validity and reliability of the apple watch for measuring heart rate during exercise," *Sports Med. Int. Open*, vol. 1, no. 6, pp. E206–E211, Oct. 2017.

[45] G. Mardirossian and R. E. Schneider, "Limitations of pulse oximetry," *Anesthesia Prog.*, vol. 39, no. 6, p. 194, 1992.

[46] F.-T.-Z. Khanam, A. Al-Naji, and J. Chahl, "Remote monitoring of vital signs in diverse non-clinical and clinical scenarios using computer vision systems: A review," *Appl. Sci.*, vol. 9, no. 20, p. 4474, 2019.

[47] X. Chen, J. Cheng, R. Song, Y. Liu, R. Ward, and Z. J. Wang, "Video-based heart rate measurement: Recent advances and future prospects," *IEEE Trans. Instrum. Meas.*, vol. 68, no. 10, pp. 3600–3615, Oct. 2019, doi: 10.1109/TIM.2018.2879706.

[48] S. Phansalkar et al., "A review of human factors principles for the design and implementation of medication safety alerts in clinical information systems," *J. Amer. Med. Inform. Assoc.*, vol. 17, no. 5, pp. 493–501, Sep. 2010.

[49] M. Kumar, A. Veeraraghavan, and A. Sabharwal, "DistancePPG: Robust non-contact vital signs monitoring using a camera," *Biomed. Opt. Exp.*, vol. 6, no. 5, pp. 1565–1588, Apr. 2015.

[50] K. M. van der Kooij and M. Naber, "An open-source remote heart rate imaging method with practical apparatus and algorithms," *Behav. Res. Methods*, vol. 51, no. 5, pp. 2106–2119, 2019.

[51] M. J. Moron, E. Casilari, R. Luque, and J. A. Gazquez, "A wireless monitoring system for pulse-oximetry sensors," in *Proc. Syst. Commun. (ICW, ICHSN, ICMCS, SENET)*, Aug. 2005, pp. 79–84.

[52] L. A. M. Aarts et al., "Non-contact heart rate monitoring utilizing camera photoplethysmography in the neonatal intensive care unit—A pilot study," *Early Human Develop.*, vol. 89, no. 12, pp. 943–948, Dec. 2013.

[53] K. E. J. Philip, R. Tidswell, and C. McFadyen, "Racial bias in pulse oximetry: More statistical detail may help tackle the problem," *BMJ*, vol. 372, p. n298, Feb. 2021.

[54] M. S. Arefin, A. P. Dumont, and C. A. Patil, "Monte Carlo based simulations of racial bias in pulse oximetry," *Proc. SPIE*, vol. 11951, Mar. 2022, Art. no. 1195103.

[55] L. J. Mengelkoch, D. Martin, and J. Lawler, "A review of the principles of pulse oximetry and accuracy of pulse oximeter estimates during exercise," *Phys. Therapy*, vol. 74, no. 1, pp. 40–49, Jan. 1994.

[56] C. Cahan, M. J. Decker, P. L. Hoekje, and K. P. Strohl, "Agreement between noninvasive oximetric values for oxygen saturation," *Chest*, vol. 97, no. 4, pp. 814–819, Apr. 1990.

[57] P. E. Bickler, J. R. Feiner, and J. W. Severinghaus, "Effects of skin pigmentation on pulse oximeter accuracy at low saturation," *Anesthesiology*, vol. 102, no. 4, pp. 715–719, Apr. 2005.

[58] C. J. Crooks et al., "Pulse oximeter measurements vary across ethnic groups: An observational study in patients with COVID-19," *Eur. Respiratory J.*, vol. 59, no. 4, Apr. 2022, Art. no. 2103246.

[59] G. W. Burnett et al., "Self-reported race/ethnicity and intraoperative occult hypoxemia: A retrospective cohort study," *Anesthesiology*, vol. 136, no. 5, pp. 688–696, May 2022.

[60] M. W. Sjoding, R. P. Dickson, T. J. Iwashyna, S. E. Gay, and T. S. Valley, "Racial bias in pulse oximetry measurement," *New England J. Med.*, vol. 383, no. 25, pp. 2477–2478, Dec. 2020.

[61] A. Jubran, "Pulse oximetry," in *Applied Physiology in Intensive Care Medicine*, vol. 30. Springer-Verlag, 2004, pp. 2017–2020, doi: 10.1007/s00134-004-2399-x.

[62] M. M. Chan, M. M. Chan, and E. D. Chan, "What is the effect of fingernail polish on pulse oximetry?" *Chest*, vol. 123, no. 6, pp. 2163–2164, Jun. 2003, doi: 10.1378/chest.123.6.2163.

[63] D. A. Raipure, "Effect of nail paint on pulse oximetry values & clinical importance," *J. Med. Sci. Clin. Res.*, vol. 7, no. 9, pp. 261–265, Sep. 2019.

[64] T. M. Brand, M. E. Brand, and G. D. Jay, "Enamel nail polish does not interfere with pulse oximetry among normoxic volunteers," *J. Clin. Monitor. Comput.*, vol. 17, no. 2, pp. 93–96, 2002.

[65] O. Jakpor, "Do artificial nails and nail polish interfere with the accurate measurement of oxygen saturation by pulse oximetry?" *Young Scientists J.*, vol. 4, no. 9, p. 33, 2011.

[66] P. Pirzada, D. Morrison, G. Doherty, D. Dhasmana, and D. Harris-Birtill, "Automated remote pulse oximetry system (ARPOS)," *Sensors*, vol. 22, no. 13, p. 4974, Jun. 2022.

[67] H. Xiao, T. Liu, Y. Sun, Y. Li, S. Zhao, and A. Avolio, "Remote photoplethysmography for heart rate measurement: A review," *Biomed. Signal Process. Control*, vol. 88, Feb. 2024, Art. no. 105608, doi: 10.1016/j.bspc.2023.105608.

[68] D. McDuff, "Camera measurement of physiological vital signs," *ACM Comput. Surv.*, vol. 55, no. 9, pp. 1–40, Sep. 2023, doi: 10.1145/3558518.

[69] S. Premkumar and D. J. Hemanth, "Intelligent remote photoplethysmography-based methods for heart rate estimation from face videos: A survey," *Informatics*, vol. 9, no. 3, p. 57, Aug. 2022, doi: 10.3390/informatics9030057.

[70] J. K. Lu, M. Sijm, G. E. Janssens, J. Goh, and A. B. Maier, "Remote monitoring technologies for measuring cardiovascular functions in community-dwelling adults: A systematic review," *GeroScience*, vol. 45, no. 5, pp. 2939–2950, 2023.

[71] R. Karthick, M. S. Dawood, and P. Meenalochini, "Analysis of vital signs using remote photoplethysmography (RPPG)," *J. Ambient Intell. Humanized Comput.*, vol. 14, no. 12, pp. 16729–16736, Dec. 2023.

[72] A. Gupta, A. G. Ravelo-García, and F. M. Dias, "Availability and performance of face based non-contact methods for heart rate and oxygen saturation estimations: A systematic review," *Comput. Methods Programs Biomed.*, vol. 219, Jun. 2022, Art. no. 106771, doi: 10.1016/j.cmpb.2022.106771.


Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[73] R. J. Lee, S. Sivakumar, and K. H. Lim, "Review on remote heart rate measurements using photoplethysmography," *Multimedia Tools Appl.*, vol. 83, no. 15, pp. 44699–44728, Oct. 2023, doi: 10.1007/s11042-023-16794-9.

[74] I. Pavlidis, "Continuous physiological monitoring," in *Proc. 25th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Sep. 2003, pp. 1084–1087.

[75] M. Garbey, N. Sun, A. Merla, and I. Pavlidis, "Contact-free measurement of cardiac pulse based on the analysis of thermal imagery," *IEEE Trans. Biomed. Eng.*, vol. 54, no. 8, pp. 1418–1426, Aug. 2007.

[76] R. G. Gatto, *Estimation of Instantaneous Heart Rate Using Video Infrared Thermography and ARMA Models*. Chicago, IL, USA: Univ. of Illinois Press, 2009.

[77] D.-Y. Chen, H.-S. Zou, and A.-T. Hsieh, "Thermal image based remote heart rate measurement on dynamic subjects using deep learning," in *Proc. IEEE Int. Conf. Consum. Electron.-Taiwan (ICCE-Taiwan)*, Sep. 2020, pp. 1–2.

[78] C. Takano and Y. Ohta, "Heart rate measurement based on a time-lapse image," *Med. Eng. Phys.*, vol. 29, no. 8, pp. 853–857, Oct. 2007.

[79] G. de Haan and V. Jeanne, "Robust pulse rate from chrominance-based rPPG," *IEEE Trans. Biomed. Eng.*, vol. 60, no. 10, pp. 2878–2886, Oct. 2013.

[80] M.-Z. Poh, D. J. McDuff, and R. W. Picard, "Non-contact, automated cardiac pulse measurements using video imaging and blind source separation," *Opt. Exp.*, vol. 18, no. 10, pp. 10762–10774, 2010.

[81] M.-Z. Poh, D. J. McDuff, and R. W. Picard, "Advancements in noncontact, multiparameter physiological measurements using a webcam," *IEEE Trans. Biomed. Eng.*, vol. 58, no. 1, pp. 7–11, Jan. 2010.

[82] M. Oviyaa, P. Renvitha, and R. Swathika, "Real time tracking of heart rate from facial video using webcam," in *Proc. 2nd Int. Conf. Inventive Res. Comput. Appl. (ICIRCA)*, Jul. 2020, pp. 1–7.

[83] M. Kopeliovich, M. Petrushan, and D. Shaposhnikov, "Approximation-based transformation of color signal for heart rate estimation with a webcam," *Pattern Recognit. Image Anal.*, vol. 28, no. 4, pp. 646–651, Oct. 2018.

[84] Y. Muratov, M. Nikiforov, O. Melnik, and A. Loskutov, "Heart rate measurements with a web camera based on the facial image moving in the frame," in *Proc. 10th Medit. Conf. Embedded Comput. (MECO)*, Jun. 2021, pp. 1–5.

[85] H. Lee, H. Ko, H. Chung, Y. Nam, S. Hong, and J. Lee, "Real-time realizable mobile imaging photoplethysmography," *Sci. Rep.*, vol. 12, no. 1, p. 7141, May 2022.

[86] D. Wang, X. Yang, X. Liu, J. Jing, and S. Fang, "Detail-preserving pulse wave extraction from facial videos using consumer-level camera," *Biomed. Opt. Exp.*, vol. 11, no. 4, pp. 1876–1891, Mar. 2020.

[87] M. Das, T. Choudhary, M. K. Bhuyan, and L. N. Sharma, "Non-contact heart rate measurement from facial video data using a 2D-VMD scheme," *IEEE Sensors J.*, vol. 22, no. 11, pp. 11153–11161, Jun. 2022.

[88] R. Qian, T. Jin, H. Li, and Y. Dai, "WT-based data-length-variation technique for fast heart rate detection," in *Proc. Prog. Electromagn. Res. Symp. (PIERS-Toyama)*, Aug. 2018, pp. 399–404.

[89] C. Pham et al., "Video plethysmography for contactless blood pressure and heart rate measurement in perioperative care," *J. Clin. Monitor. Comput.*, vol. 38, no. 1, pp. 121–130, Feb. 2024.

[90] A. Al-Naji and J. Chahl, "Detection of cardiopulmonary activity and related abnormal events using Microsoft Kinect sensor," *Sensors*, vol. 18, no. 3, p. 920, Mar. 2018.

[91] L. Zhou, M. Yin, X. Xu, X. Yuan, and X. Liu, "Non-contact detection of human heart rate with Kinect," *Cluster Comput.*, vol. 22, pp. 8199–8206, Jul. 2019.

[92] A. Shokouhmand, S. Eckstrom, B. Gholami, and N. Tavassolian, "Camera-augmented non-contact vital sign monitoring in real time," *IEEE Sensors J.*, vol. 22, no. 12, pp. 11965–11978, Jun. 2022.

[93] A. Al-Naji, A. G. Perera, and J. Chahl, "Remote monitoring of cardiorespiratory signals from a hovering unmanned aerial vehicle," *Biomed. Eng. OnLine*, vol. 16, no. 1, pp. 1–20, Dec. 2017.

[94] L. Mösch et al., "For heart rate assessments from drone footage in disaster scenarios," *Bioengineering*, vol. 10, no. 3, p. 336, Mar. 2023.

[95] J. Mathew, X. Tian, M. Wu, and C.-W. Wong, "Remote blood oxygen estimation from videos using neural networks," 2021, *arXiv:2107.05087*.

[96] N. Molinaro, E. Schena, S. Silvestri, and C. Massaroni, "Multi-ROI spectral approach for the continuous remote cardio-respiratory monitoring from mobile device built-in cameras," *Sensors*, vol. 22, no. 7, p. 2539, Mar. 2022.

[97] N. Q. Al-Naggar, H. M. Al-Hammadi, A. M. Al-Fusail, and Z. A. Al-Shaebi, "Design of a remote real-time monitoring system for multiple physiological parameters based on smartphone," *J. Healthcare Eng.*, vol. 2019, pp. 1–13, Nov. 2019.

[98] T. Burton, G. Saiko, M. Cao, and A. Douplik, "Remote photoplethysmography with consumer smartphone reveals temporal differences between glabrous and nonglabrous skin: Pilot in vivo study," *J. Biophotonics*, vol. 16, no. 1, Jan. 2023, Art. no. e202200187.

[99] S. Sanyal and K. K. Nundy, "Algorithms for monitoring heart rate and respiratory rate from the video of a user's face," *IEEE J. Transl. Eng. Health Med.*, vol. 6, 2018, Art. no. 2700111.

[100] T. Coppetti et al., "Accuracy of smartphone apps for heart rate measurement," *Eur. J. Preventive Cardiol.*, vol. 24, no. 12, pp. 1287–1293, Aug. 2017.

[101] Y. Nam, Y. Kong, B. Reyes, N. Reljin, and K. H. Chon, "Monitoring of heart and breathing rates using dual cameras on a smartphone," *PLoS ONE*, vol. 11, no. 3, Mar. 2016, Art. no. e0151013.

[102] S.-Y. Lin and M.-R. Tsai, "Non-contact heart rate monitoring with mobile phone camera," in *Proc. IEEE Int. Conf. Consum. Electron.-Taiwan (ICCE-TW)*, May 2019, pp. 1–2.

[103] M. Ben Ayed, S. A. Alshaya, and A. Alshammari, "Enhanced heart rate estimation based on face features," in *Proc. 18th Int. Multi-Conf. Syst., Signals Devices (SSD)*, Mar. 2021, pp. 840–844.

[104] Z. Sun, Q. He, Y. Li, W. Wang, and R. K. Wang, "Robust non-contact peripheral oxygenation saturation measurement using smartphone-enabled imaging photoplethysmography," *Biomed. Opt. Exp.*, vol. 12, no. 3, p. 1746, 2021, doi: 10.1364/boe.419268.

[105] R.-Y. Huang and L.-R. Dung, "Measurement of heart rate variability using off-the-shelf smart phones," *Biomed. Eng. OnLine*, vol. 15, no. 1, pp. 1–16, Jan. 2016.

[106] W. Verkruysse, L. O. Svaasand, and J. S. Nelson, "Remote plethysmographic imaging using ambient light," *Opt. Exp.*, vol. 16, no. 26, pp. 21434–21445, Dec. 2008.

[107] G. Balakrishnan, F. Durand, and J. Guttag, "Detecting pulse from head motions in video," in *Proc. IEEE Conf. Comput. Vis. Pattern Recognit.*, Jun. 2013, pp. 3430–3437.

[108] M. Lewandowska, J. Ruminski, T. Kocejko, and J. Nowak, "Measuring pulse rate with a webcam—A non-contact method for evaluating cardiac activity," in *Proc. Federated Conf. Comput. Sci. Inf. Syst. (FedCSIS)*, Sep. 2011, pp. 405–410.

[109] P. Viola and M. Jones, "Rapid object detection using a boosted cascade of simple features," in *Proc. IEEE Comput. Soc. Conf. Comput. Vis. Pattern Recognit.* Kauai, HI, USA: IEEE, Dec. 2001.

[110] N. A. Akbar, A. Muneer, S. M. Taib, and S. M. Fati, "Measuring accuracy towards facial video heart-rate estimation using Haar–Cascade and CNN method," in *Proc. Int. Conf. Decis. Aid Sci. Appl. (DASA)*, Mar. 2022, pp. 1607–1611.

[111] G. H. Martinez-Delgado, A. J. Correa-Balan, J. A. May-Chan, C. E. Parra-Elizondo, L. A. Guzman-Rangel, and A. Martinez-Torteya, "Measuring heart rate variability using facial video," *Sensors*, vol. 22, no. 13, p. 4690, Jun. 2022, doi: 10.3390/s22134690.

[112] M. Islam, T. Biswas, A. Saad, C. A. Haque, and M. S. U. Yusuf, "A non-invasive heart rate estimation approach from photoplethysmography," in *Proc. Int. Joint Conf. Comput. Intell.*, 2018, doi: 10.1007/978-981-13-7564-4_33.

[113] K. Z. Lee, P. C. Hung, and L. W. Tsai, "Contact-free heart rate measurement using a camera," in *Proc. 9th Conf. Comput. Robot Vis. (CRV)*, May 2012, pp. 147–152.

[114] Y. Fujita, M. Hiromoto, and T. Sato, "Fast and robust heart rate estimation from videos through dynamic region selection," in *Proc. 40th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2018, pp. 3024–3027.

[115] K. Zheng et al., "Heart rate prediction from facial video with masks using eye location and corrected by convolutional neural networks," *Biomed. Signal Process. Control*, vol. 75, May 2022, Art. no. 103609.

[116] T. F. Cootes, G. J. Edwards, and C. J. Taylor, "Active appearance models," in *Proc. Eur. Conf. Comput. Vis.* Springer, 1998, pp. 484–498.

[117] M. Waqar, "Contact-free heart rate measurement from human face videos and its biometric recognition application," Ph.D. dissertation, Dept. Comput. Sci., Aberystwyth Univ., 2019.

[118] R. Van Luijtelaar, W. Wang, S. Stuijk, and G. de Haan, "Automatic roi detection for camera-based pulse-rate measurement," in *Proc. Asian Conf. Comput. Vis.* Springer, 2014, pp. 360–374.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[119] L. Feng, L.-M. Po, X. Xu, Y. Li, and R. Ma, "Motion-resistant remote imaging photoplethysmography based on the optical properties of skin," *IEEE Trans. Circuits Syst. Video Technol.*, vol. 25, no. 5, pp. 879–891, May 2015.

[120] L. Feng, L.-M. Po, X. Xu, and Y. Li, "Motion artifacts suppression for remote imaging photoplethysmography," in *Proc. 19th Int. Conf. Digit. Signal Process.*, Aug. 2014, pp. 18–23.

[121] B. Lucas and T. Kanade, "An iterative image registration technique with an application to stereo vision," in *Proc. IJCAI*, Apr. 1981.

[122] D. Comaniciu, V. Ramesh, and P. Meer, "Kernel-based object tracking," *IEEE Trans. Pattern Anal. Mach. Intell.*, vol. 25, no. 5, pp. 564–577, May 2003.

[123] A. Zadeh, Y. C. Lim, T. Baltrusaitis, and L.-P. Morency, "Convolutional experts constrained local model for 3D facial landmark detection," in *Proc. IEEE Int. Conf. Comput. Vis. Workshops*, 2017, pp. 2519–2528.

[124] B. Lokendra and G. Puneet, "AND-rPPG: A novel denoising-rPPG network for improving remote heart rate estimation," *Comput. Biol. Med.*, vol. 141, Feb. 2022, Art. no. 105146.

[125] H. Shao, L. Luo, S. Chen, C. Hu, and J. Yang, "Hyperbolic embedding steered spatiotemporal graph convolutional network for video-based remote heart rate estimation," *Eng. Appl. Artif. Intell.*, vol. 124, Sep. 2023, Art. no. 106642.

[126] Y. Deshpande, S. Thapa, A. Sarkar, and A. L. Abbott, "Camera-based recovery of cardiovascular signals from unconstrained face videos using an attention network," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2023, pp. 5975–5984, doi: 10.1109/CVPRW59228.2023.00636.

[127] D.-Y. Kim, K. Lee, and C.-B. Sohn, "Assessment of ROI selection for facial video-based rPPG," *Sensors*, vol. 21, no. 23, p. 7923, Nov. 2021.

[128] S. Kwon, J. Kim, D. Lee, and K. Park, "ROI analysis for remote photoplethysmography on facial video," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2015, pp. 4938–4941.

[129] A. R. Arppana, N. K. Reshmma, G. Raghu, N. Mathew, H. R. Nair, and R. P. Aneesh, "Real time heart beat monitoring using computer vision," in *Proc. 7th Int. Conf. Bio Signals, Images, Instrum. (ICBSII)*, Mar. 2021, pp. 1–6.

[130] C. Wang, Y. Jiang, Z. Cai, and L. Lin, "Non-contact measurement of heart rate based on facial video," in *Proc. Photon. Electromagn. Res. Symp. (PIERS-Fall)*, Dec. 2019, pp. 2269–2275.

[131] Y. Maki, Y. Monno, K. Yoshizaki, M. Tanaka, and M. Okutomi, "Inter-beat interval estimation from facial video based on reliability of BVP signals," in *Proc. 41st Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2019, pp. 6525–6528, doi: 10.1109/EMBC.2019.8857081.

[132] S. Kado, Y. Monno, K. Moriwaki, K. Yoshizaki, M. Tanaka, and M. Okutomi, "Remote heart rate measurement from RGB-NIR video based on spatial and spectral face patch selection," in *Proc. 40th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2018, pp. 5676–5680, doi: 10.1109/EMBC.2018.8513464.

[133] W. Wang and A. C. den Brinker, "Modified RGB cameras for infrared remote-PPG," *IEEE Trans. Biomed. Eng.*, vol. 67, no. 10, pp. 2893–2904, Oct. 2020.

[134] A. Ni, A. Azarang, and N. Kehtarnavaz, "A review of deep learning-based contactless heart rate measurement methods," *Sensors*, vol. 21, no. 11, p. 3719, May 2021, doi: 10.3390/s21113719.

[135] M. A. Hassan et al., "Heart rate estimation using facial video: A review," *Biomed. Signal Process. Control*, vol. 38, pp. 346–360, Sep. 2017.

[136] W. Wang, A. C. den Brinker, and G. de Haan, "Full video pulse extraction," *Biomed. Opt. Exp.*, vol. 9, no. 8, pp. 3898–3914, Aug. 2018.

[137] R. Mitsuhashi et al., "Noncontact pulse wave detection by two-band infrared video-based measurement on face without visible lighting," *Artif. Life Robot.*, vol. 23, no. 3, pp. 345–352, Sep. 2018, doi: 10.1007/s10015-018-0430-5.

[138] J. Cheng et al., "Remote heart rate measurement from near-infrared videos based on joint blind source separation with delay-coordinate transformation," *IEEE Trans. Instrum. Meas.*, vol. 70, pp. 1–13, 2021.

[139] H. Ernst, H. Malberg, and M. Schmidt, "More reliable remote heart rate measurement by signal quality indexes," in *Proc. Comput. Cardiol. Conf.*, Sep. 2020, pp. 1–4.

[140] H. Gao, X. Wu, J. Geng, and Y. Lv, "Remote heart rate estimation by signal quality attention network," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2022, pp. 2121–2128.

[141] H. Liu, Y. Wang, and L. Wang, "A review of non-contact, low-cost physiological information measurement based on photoplethysmographic imaging," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2012, pp. 2088–2091.

[142] G. Cennini, J. Arguel, K. Akşit, and A. van Leest, "Heart rate monitoring via remote photoplethysmography with motion artifacts reduction," *Opt. Exp.*, vol. 18, no. 5, pp. 4867–4875, Mar. 2010.

[143] W. Wang, A. C. den Brinker, S. Stuijk, and G. de Haan, "Amplitude-selective filtering for remote-PPG," *Biomed. Opt. Exp.*, vol. 8, no. 3, pp. 1965–1980, Mar. 2017.

[144] C. Pham et al., "Effectiveness of consumer-grade contactless vital signs monitors: A systematic review and meta-analysis," *J. Clin. Monitor. Comput.*, vol. 36, no. 1, pp. 41–54, Feb. 2022.

[145] O. Havakuk et al., "Validation of a novel contact-free heart and respiratory rate monitor," *J. Med. Eng. Technol.*, vol. 45, no. 5, pp. 344–350, Jul. 2021.

[146] V. Saran, R. Kumar, G. Kumar, K. Chokalingam, M. Rawooth, and G. Parchani, "Validation of dozee, a ballistocardiography-based device, for contactless and continuous heart rate and respiratory rate measurement," in *Proc. 44th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2022, pp. 1939–1943.

[147] H. Lee, A. Cho, and M. Whang, "Fusion method to estimate heart rate from facial videos based on RPPG and RBCG," *Sensors*, vol. 21, no. 20, p. 6764, Oct. 2021.

[148] P. Li et al., "Video-based pulse rate variability measurement using periodic variance maximization and adaptive two-window peak detection," *Sensors*, vol. 20, no. 10, p. 2752, May 2020.

[149] K. S. Alam et al., "Remote heart rate and heart rate variability detection and monitoring from face video with minimum resources," in *Proc. IEEE 44th Annu. Comput., Softw., Appl. Conf. (COMPSAC)*, Jul. 2020, pp. 1385–1390.

[150] H. Demirezen and C. E. Erdem, "Heart rate estimation from facial videos using nonlinear mode decomposition and improved consistency check," *Signal, Image Video Process.*, vol. 15, no. 7, pp. 1415–1423, Oct. 2021.

[151] M. J. Bautista, M. Kowal, D. G. W. Cave, C. Downey, and D. G. Jayne, "Clinical applications of contactless photoplethysmography for monitoring in adults: A systematic review and meta-analysis," *J. Clin. Transl. Sci.*, vol. 7, no. 1, 1017, doi: 10.1017/cts.2023.547.

[152] G. E. Box, G. M. Jenkins, G. C. Reinsel, and G. M. Ljung, *Time Series Analysis: Forecasting and Control*. Hoboken, NJ, USA: Wiley, 2015.

[153] A. K. Abbas, K. Heimann, K. Jergus, T. Orlikowsky, and S. Leonhardt, "Neonatal non-contact respiratory monitoring based on real-time infrared thermography," *Biomed. Eng. OnLine*, vol. 10, no. 1, p. 93, 2011.

[154] J. Zheng, S. Hu, A. S. Echiadis, V. Azorin-Peris, P. Shi, and V. Chouliaras, "A remote approach to measure blood perfusion from the human face," *Proc. SPIE*, vol. 7169, pp. 221–227, Feb. 2009.

[155] J. Du, S.-Q. Liu, B. Zhang, and P. C. Yuen, "Dual-bridging with adversarial noise generation for domain adaptive rPPG estimation," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. (CVPR)*, Jun. 2023, pp. 10355–10364, doi: 10.1109/cvpr52729.2023.00998.

[156] S. Guler, O. Ozturk, A. Golparvar, H. Dogan, and M. K. Yapici, "Effects of illuminance intensity on the green channel of remote photoplethysmography (rPPG) signals," *Phys. Eng. Sci. Med.*, vol. 45, no. 4, pp. 1317–1323, Aug. 2022.

[157] A. Hammer et al., "Camera-based assessment of cutaneous perfusion strength in a clinical setting," *Physiol. Meas.*, vol. 43, no. 2, Feb. 2022, Art. no. 025007.

[158] R. Sinhal, K. R. Singh, and K. O. Gupta, "Color intensity: A study of RPPG algorithm for heart rate estimation," in *Proc. Int. Conf. Comput. Perform. Eval. (ComPE)*, Dec. 2021, pp. 580–584, doi: 10.1109/ComPE53109.2021.9752363.

[159] K. K. Bhoyar and O. Kakde, "Skin color detection model using neural networks and its performance evaluation," *J. Comput. Sci.*, vol. 6, no. 9, pp. 963–968, Sep. 2010.

[160] P.-C. Hung, K.-Z. Lee, and L.-W. Tsai, "Contact-free heart rate measurement using multiple video data," *AIP Conf. Proc.*, vol. 1559, no. 1, pp. 57–66, Oct. 2013.

[161] L. Scalise, N. Bernacchia, I. Ercoli, and P. Marchionni, "Heart rate measurement in neonatal patients using a webcamera," in *IEEE Int. Symp. Med. Meas. Appl. Proc.*, May 2012, pp. 1–4.

[162] A. Panigrahi and H. Sharma, "Non-contact HR extraction from different color spaces using RGB camera," in *Proc. Nat. Conf. Commun. (NCC)*, May 2022, pp. 332–337.


Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[163] P. V. Rouast, M. Adam, V. Dorner, and E. Lux, "Remote photoplethysmography: Evaluation of contactless heart rate measurement in an information systems setting," in *Proc. Appl. Informat. Technol. Innov. Conf.*, 2016, pp. 1–17.

[164] K. Gupta, R. Sinhal, and S. S. Badhiye, "Remote photoplethysmography-based human vital sign prediction using cyclical algorithm," *J. Biophotonics*, vol. 17, no. 1, Jan. 2024, Art. no. e202300286.

[165] D. McDuff, S. Gontarek, and R. Picard, "Remote measurement of cognitive stress via heart rate variability," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Aug. 2014, pp. 2957–2960.

[166] C. Lueangwattana, T. Kondo, and H. Haneishi, "A comparative study of video signals for non-contact heart rate measurement," in *Proc. 12th Int. Conf. Electr. Eng./Electron., Comput., Telecommun. Inf. Technol. (ECTI-CON)*, Jun. 2015, pp. 1–5.

[167] K. Mannapperuma, B. D. Holton, P. J. Lesniewski, and J. C. Thomas, "Performance limits of ICA-based heart rate identification techniques in imaging photoplethysmography," *Physiol. Meas.*, vol. 36, no. 1, pp. 67–83, Jan. 2015.

[168] E. Christinaki et al., "Comparison of blind source separation algorithms for optical heart rate monitoring," in *Proc. 4th Int. Conf. Wireless Mobile Commun. Healthcare-Transforming Healthcare Through Innov. Mobile Wireless Technol. (MOBIHEALTH)*, Nov. 2014, pp. 339–342.

[169] W. J. Jiang, S. C. Gao, P. Wittek, and L. Zhao, "Real-time quantifying heart beat rate from facial video recording on a smart phone using Kalman filters," in *Proc. IEEE 16th Int. Conf. e-Health Netw., Appl. Services (Healthcom)*, Oct. 2014, pp. 393–396.

[170] L. Qi, H. Yu, L. Xu, R. S. Mpanda, and S. E. Greenwald, "Robust heart-rate estimation from facial videos using Project_ICA," *Physiol. Meas.*, vol. 40, no. 8, Sep. 2019, Art. no. 085007.

[171] R. Macwan, Y. Benezeth, and A. Mansouri, "Remote photoplethysmography with constrained ICA using periodicity and chrominance constraints," *Biomed. Eng. OnLine*, vol. 17, no. 1, p. 22, Feb. 2018.

[172] J.-Y. Hsu, T.-Y. Jiang, and P. C.-P. Chao, "A fast FPGA hardware accelerator for remote heart rate detection based on RGB vision," *IEEE Trans. Biomed. Circuits Syst.*, vol. 18, no. 3, pp. 592–607, Jun. 2024.

[173] A. Al-Naji, J. Chahl, and S.-H. Lee, "Cardiopulmonary signal acquisition from different regions using video imaging analysis," *Comput. Methods Biomechanics Biomed. Eng., Imag. Visualizat.*, vol. 7, no. 2, pp. 117–131, Mar. 2019, doi: 10.1080/21681163.2018.1441075.

[174] R. M. Fouad, O. A. Omer, and M. H. Aly, "Optimizing remote photoplethysmography using adaptive skin segmentation for real-time heart rate monitoring," *IEEE Access*, vol. 7, pp. 76513–76528, 2019, doi: 10.1109/ACCESS.2019.2922304.

[175] L. K. Mestha, S. Kyal, B. Xu, L. E. Lewis, and V. Kumar, "Towards continuous monitoring of pulse rate in neonatal intensive care unit with a webcam," in *Proc. 36th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2014, pp. 3817–3820.

[176] Y.-P. Yu, B.-H. Kwan, C.-L. Lim, S.-L. Wong, and P. Raveendran, "Video-based heart rate measurement using short-time Fourier transform," in *Proc. Int. Symp. Intell. Signal Process. Commun. Syst.*, Nov. 2013, pp. 704–707.

[177] X. Li, J. Chen, G. Zhao, and M. Pietikäinen, "Remote heart rate measurement from face videos under realistic situations," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. (CVPR)*, Jun. 2014, pp. 4264–4271.

[178] A. Lam and Y. Kuno, "Robust heart rate measurement from video using select random patches," in *Proc. IEEE/CVF Int. Conf. Comput. Vis. (ICCV)*, Dec. 2015, pp. 3640–3648.

[179] A. V. Moço, S. Stuijk, and G. de Haan, "Ballistocardiographic artifacts in PPG imaging," *IEEE Trans. Biomed. Eng.*, vol. 63, no. 9, pp. 1804–1811, Sep. 2016.

[180] J. R. Estepp, E. B. Blackford, and C. M. Meier, "Recovering pulse rate during motion artifact with a multi-imager array for non-contact imaging photoplethysmography," in *Proc. IEEE Conf. Syst., Man, Cybern. (SMC)*, 2014, pp. 1462–1469.

[181] G. de Haan and A. V. Leest, "Improved motion robustness of remote-PPG by using the blood volume pulse signature," *Physiol. Meas.*, vol. 35, no. 9, p. 1913, 2014.

[182] S. M. Karmuse, A. L. Kakhandki, and M. Anandhalli, "A robust rPPG approach for continuous heart rate measurement based on face," *J. Inst. Eng. India, Ser. B*, p. 12, Oct. 2022, doi: 10.1007/s40031-022-00817-4.

[183] T. Pursche, J. Krajewski, and R. Moeller, "Video-based heart rate measurement from human faces," in *Proc. IEEE Int. Conf. Consum. Electron. (ICCE)*, Jan. 2012, pp. 544–545.

[184] S. Kwon, H. Kim, and K. S. Park, "Validation of heart rate extraction using video imaging on a built-in camera system of a smartphone," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, 2012, pp. 2174–2177.

[185] L. Wei, Y. Tian, Y. Wang, T. Ebrahimi, and T. Huang, "Automatic webcam-based human heart rate measurements using Laplacian Eigenmap," in *Proc. Asian Conf. Comput. Vis.* Springer, 2012, pp. 281–292.

[186] D. Djeldjli, C. Maaoui, and F. B. Reguig, "Robust heart activity measurement using webcam," in *Proc. Int. Conf. Control, Autom. Diagnosis (ICCAD)*, Jul. 2019, pp. 1–6, doi: 10.1109/iccad46983.2019.9037962.

[187] H.-Y. Wu, M. Rubinstein, E. Shih, J. Guttag, F. Durand, and W. Freeman, "Eulerian video magnification for revealing subtle changes in the world," *ACM Trans. Graph.*, vol. 31, no. 4, pp. 1–8, Aug. 2012.

[188] B. Wallace, L. Y. Kassab, A. Law, R. Goubran, and F. Knoefel, "Contactless remote assessment of heart rate and respiration rate using video magnification," *IEEE Instrum. Meas. Mag.*, vol. 25, no. 1, pp. 20–27, Feb. 2022.

[189] J. Zhang, K. Zhang, X. Yang, and C. Wen, "Heart rate measurement based on video acceleration magnification," in *Proc. Chin. Control Decis. Conf. (CCDC)*, Aug. 2020, pp. 1179–1182.

[190] A. de Fátima Galvão Rosa and R. C. Betini, "Noncontact $SpO_2$ measurement using Eulerian video magnification," *IEEE Trans. Instrum. Meas.*, vol. 69, no. 5, pp. 2120–2130, May 2020, doi: 10.1109/TIM.2019.2920183.

[191] K. H. Suh and E. C. Lee, "Contactless physiological signals extraction based on skin color magnification," *J. Electron. Imag.*, vol. 26, no. 6, p. 1, Nov. 2017, doi: 10.1117/1.jei.26.6.063003.

[192] J. Comas Martínez, A. Ruiz, and F. M. Sukno, "Deep pulse-signal magnification for remote heart rate estimation in compressed videos," *SSRN J.*, p. 13, Feb. 2024. [Online]. Available: https://arxiv.org/pdf/2405.02652

[193] M. Alnaggar, A. I. Siam, M. Handosa, T. Medhat, and M. Z. Rashad, "Video-based real-time monitoring for heart rate and respiration rate," *Expert Syst. Appl.*, vol. 225, Sep. 2023, Art. no. 120135.

[194] U. A. Ciftci and L. Yin, "Heart rate based face synthesis for pulse estimation," in *Advances in Visual Computing*, 2019, pp. 540–551, doi: 10.1007/978-3-030-33720-9_42.

[195] B. Kossack, E. Wisotzky, P. Eisert, S. P. Schraven, B. Globke, and A. Hilsmann, "Perfusion assessment via local remote photoplethysmography (rPPG)," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, New Orleans, LA, USA, 2022, pp. 2191–2200, doi: 10.1109/CVPRW56347.2022.00238.

[196] M. Paul, A. F. Mota, C. H. Antink, V. Blazek, and S. Leonhardt, "Modeling photoplethysmographic signals in camera-based perfusion measurements: Optoelectronic skin phantom," *Biomed. Opt. Exp.*, vol. 10, no. 9, pp. 4353–4368, 2019.

[197] M. Huelsbusch and V. Blazek, "Contactless mapping of rhythmical phenomena in tissue perfusion using PPGI," *Proc. SPIE*, vol. 4683, pp. 110–117, Apr. 2002.

[198] J. Zheng, S. Hu, V. Azorin-Peris, A. Echiadis, V. Chouliaras, and R. Summers, "Remote simultaneous dual wavelength imaging photoplethysmography: A further step towards 3-D mapping of skin blood microcirculation," *Proc. SPIE*, vol. 6850, Feb. 2008, Art. no. 68500S, doi: 10.1117/12.761705.

[199] K. Humphreys, T. Ward, and C. Markham, "Noncontact simultaneous dual wavelength photoplethysmography: A further step toward noncontact pulse oximetry," *Rev. Sci. Instrum.*, vol. 78, no. 4, Apr. 2007, doi: 10.1063/1.2724789.

[200] C.-H. Cheng, K.-L. Wong, J.-W. Chin, T.-T. Chan, and R. H. Y. So, "Deep learning methods for remote heart rate measurement: A review and future research agenda," *Sensors*, vol. 21, no. 18, p. 6296, Sep. 2021, doi: 10.3390/s21186296.

[201] B. Li, W. Jiang, J. Peng, and X. Li, "Deep learning-based remote-photoplethysmography measurement from short-time facial video," *Physiol. eas.*, vol. 43, no. 11, Nov. 2022, Art. no. 115003.

[202] Y. Sun et al., "Contactless facial video recording with deep learning models for the detection of atrial fibrillation," *Sci. Rep.*, vol. 12, no. 1, p. 281, Jan. 2022.

[203] E. Quanyu, "Pulse signal analysis based on deep learning network," *BioMed Res. Int.*, vol. 2022, Sep. 2022, Art. no. 6256126.

[204] L. C. Lampier, C. T. Valadão, L. A. Silva, D. Delisle-Rodríguez, E. M. D. O. Caldeira, and T. F. Bastos-Filho, "A deep learning approach to estimate pulse rate by remote photoplethysmography," *Physiol. Meas.*, vol. 43, no. 7, Jul. 2022, Art. no. 075012.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[205] A. Al-Naji, K. Gibson, and J. Chahl, "Remote sensing of physiological signs using a machine vision system," *J. Med. Eng. Technol.*, vol. 41, no. 5, pp. 396–405, Jul. 2017.

[206] O. Perepelkina, M. Artemyev, M. Churikova, and M. Grinenko, "HeartTrack: Convolutional neural network for remote video-based heart rate monitoring," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2020, pp. 1163–1171.

[207] W. Chen and D. J. McDuff, "DeepPhys: Vdeo-based physiological measurement using convolutional attention networks," in *Proc. Eur. Conf. Comput. Vis. (ECCV)*, 2018, pp. 356–373, doi: 10.1007/978-3-030-01216-8_22.

[208] X. Zhang, Z. Xia, J. Dai, L. Liu, J. Peng, and X. Feng, "MSDN: A multistage deep network for heart-rate estimation from facial videos," *IEEE Trans. Instrum. Meas.*, vol. 72, pp. 1–15, 2023, doi: 10.1109/TIM.2023.3329095.

[209] Y. Ouzar, D. Djeldjli, F. Bousefsaf, and C. Maaoui, "X-iPPGNet: A novel one stage deep learning architecture based on depth-wise separable convolutions for video-based pulse rate estimation," *Comput. Biol. Med.*, vol. 154, Mar. 2023, Art. no. 106592, doi: 10.1016/j.compbiomed.2023.106592.

[210] A. Helwan, D. Azar, and M. K. S. Ma'aitah, "Conventional and deep learning methods in heart rate estimation from RGB face videos," *Physiological Meas.*, vol. 45, no. 2, Feb. 2024, Art. no. 02TR01.

[211] L. Kong, K. Xie, K. Niu, J. He, and W. Zhang, "Remote photoplethysmography and motion tracking convolutional neural network with bidirectional long short-term memory: Non-invasive fatigue detection method based on multi-modal fusion," *Sensors*, vol. 24, no. 2, p. 455, Jan. 2024, doi: 10.3390/s24020455.

[212] B. Li, P. Zhang, J. Peng, and H. Fu, "Non-contact PPG signal and heart rate estimation with multi-hierarchical convolutional network," *Pattern Recognit.*, vol. 139, Jul. 2023, Art. no. 109421, doi: 10.1016/j.patcog.2023.109421.

[213] J. S. Lee, G. Hwang, M. Ryu, and S. J. Lee, "LSTC-rPPG: Long short-term convolutional network for remote photoplethysmography," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2023, pp. 6015–6023, doi: 10.1109/cvprw59228.2023.00640.

[214] Q. Zhan, W. Wang, and G. de Haan, "Analysis of CNN-based remote-PPG to understand limitations and sensitivities," *Biomed. Opt. Exp.*, vol. 11, no. 3, pp. 1268–1283, 2020.

[215] S. Chaichulee et al., "Multi-task convolutional neural network for patient detection and skin segmentation in continuous non-contact vital sign monitoring," in *Proc. 12th IEEE Int. Conf. Autom. Face Gesture Recognit. (FG)*, May 2017, pp. 266–272, doi: 10.1109/FG.2017.41.

[216] R.-X. Wang, H.-M. Sun, R.-R. Hao, A. Pan, and R.-S. Jia, "TransPhys: Tansformer-based unsupervised contrastive learning for remote heart rate measurement," *Biomed. Signal Process. Control*, vol. 86, Sep. 2023, Art. no. 105058, doi: 10.1016/j.bspc.2023.105058.

[217] Z. Guo et al., "Remote heart rate estimation via convolutional neural networks with transformers," *J. Franklin Inst.*, vol. 360, no. 17, pp. 13149–13165, Nov. 2023, doi: 10.1016/j.jfranklin.2023.10.013.

[218] C. Á. Casado and M. B. López, "Face2PPG: An unsupervised pipeline for blood volume pulse extraction from faces," *IEEE J. Biomed. Health Informat.*, vol. 27, no. 11, pp. 5530–5541, Nov. 2023, doi: 10.1109/JBHI.2023.3307942.

[219] N. Zhang, H.-M. Sun, J.-R. Ma, and R.-S. Jia, "A self-supervised learning network for remote heart rate measurement," *Measurement*, vol. 228, Mar. 2024, Art. no. 114379.

[220] X. Liu, Y. Zhang, Z. Yu, H. Lu, H. Yue, and J. Yang, "RPPG-MAE: Self-supervised pre-training with masked autoencoders for remote physiological measurement," 2023, *arXiv:2306.02301*.

[221] X. Liu et al., "rPPG-Toolbox: Deep remote ppg toolbox," in *Proc. Adv. Neural Inf. Process. Syst.*, vol. 36, 2024.

[222] H. Monkaresi, R. A. Calvo, and H. Yan, "A machine learning approach to improve contactless heart rate monitoring using a webcam," *IEEE J. Biomed. Health Informat.*, vol. 18, no. 4, pp. 1153–1160, Jul. 2014.

[223] P. Viola and M. J. Jones, "Robust real-time face detection," *Int. J. Comput. Vis.*, vol. 57, no. 2, pp. 137–154, May 2004.

[224] S. Baker and I. Matthews, "Lucas–Kanade 20 years on: A unifying framework," *Int. J. Comput. Vis.*, vol. 56, no. 3, pp. 221–255, 2004.

[225] H. Wang, D. Gao, G. Chen, Y. Jing, and M. Wang, "KLT algorithm for non-contact heart rate detection based on image photoplethysmography," in *Proc. 5th Int. Conf. Artif. Intell. Big Data (ICAIBD)*, May 2022, pp. 465–469.

[226] M. Soleymani, J. Lichtenauer, T. Pun, and M. Pantic, "A multimodal database for affect recognition and implicit tagging," *IEEE Trans. Affect. Comput.*, vol. 3, no. 1, pp. 42–55, Jan. 2012.

[227] M. Finžgar and P. Podržaj, "A wavelet-based decomposition method for a robust extraction of pulse rate from video recordings," *PeerJ*, vol. 6, p. e5859, Nov. 2018.

[228] X. Niu, H. Han, S. Shan, and X. Chen, "Continuous heart rate measurement from face: A robust rPPG approach with distribution learning," in *Proc. IEEE Int. Joint Conf. Biometrics (IJCB)*, Oct. 2017, pp. 642–650, doi: 10.1109/BTAS.2017.8272752.

[229] R. Song, S. Zhang, C. Li, Y. Zhang, J. Cheng, and X. Chen, "Heart rate estimation from facial videos using a spatiotemporal representation with convolutional neural networks," *IEEE Trans. Instrum. Meas.*, vol. 69, no. 10, pp. 7411–7421, Oct. 2020.

[230] K. B. Jaiswal and T. Meenpal, "Heart rate estimation network from facial videos using spatiotemporal feature image," *Comput. Biol. Med.*, vol. 151, Dec. 2022, Art. no. 106307.

[231] C. Wang, T. Pun, and G. Chanel, "A comparative survey of methods for remote heart rate detection from frontal face videos," *Frontiers Bioeng. Biotechnol.*, vol. 6, May 2018, doi: 10.3389/fbioe.2018.00033.

[232] E. Lee, E. Chen, and C.-Y. Lee, "Meta-rPPG: Remote heart rate estimation using a transductive meta-learner," in *Proc. 16th Eur. Conf. Comput. Vis.*, Glasgow, U.K. Springer, 2020, pp. 392–409.

[233] S. Petridis, B. Martinez, and M. Pantic, "The MAHNOB laughter database," *Image Vis. Comput.*, vol. 31, no. 2, pp. 186–202, Feb. 2013. [Online]. Available: https://www.sciencedirect.com/science/article/pii/S0262885612001461

[234] J. Lichtenauer, J. Shen, M. Valstar, and M. Pantic, "Cost-effective solution to synchronised audio-visual data capture using multiple sensors," *Image Vis. Comput.*, vol. 29, no. 10, pp. 666–680, Sep. 2011.

[235] R. Song, H. Chen, J. Cheng, C. Li, Y. Liu, and X. Chen, "PulseGAN: Learning to generate realistic pulse waveforms in remote photoplethysmography," *IEEE J. Biomed. Health Informat.*, vol. 25, no. 5, pp. 1373–1384, May 2021, doi: 10.1109/JBHI.2021.3051176.

[236] Z. Yu, X. Li, X. Niu, J. Shi, and G. Zhao, "AutoHR: A strong end-to-end baseline for remote heart rate measurement with neural searching," *IEEE Signal Process. Lett.*, vol. 27, pp. 1245–1249, 2020.

[237] Z. Yu, W. Peng, X. Li, X. Hong, and G. Zhao, "Remote heart rate measurement from highly compressed facial videos: An end-to-end deep learning solution with video enhancement," in *Proc. IEEE/CVF Int. Conf. Comput. Vis. (ICCV)*, Oct. 2019, pp. 151–160.

[238] S.-Q. Liu and P. C. Yuen, "Robust remote photoplethysmography estimation with environmental noise disentanglement," *IEEE Trans. Image Process.*, vol. 33, pp. 27–41, 2024, doi: 10.1109/TIP.2023.3330108.

[239] G. Boccignone, D. Conte, V. Cuculo, A. D'Amelio, G. Grossi, and R. Lanzarotti, "An open framework for remote-PPG methods and their assessment," *IEEE Access*, vol. 8, pp. 216083–216103, 2020, doi: 10.1109/ACCESS.2020.3040936.

[240] P. Pirzada, May 2022, "Dataset for automated remote pulse oximetry system (ARPOS)," *Zenodo*, doi: 10.5281/zenodo.6522389.

[241] R. Stricker, S. Müller, and H.-M. Gross, "Non-contact video-based pulse rate measurement on a mobile service robot," in *Proc. 23rd IEEE Int. Symp. Robot Human Interact. Commun.*, Aug. 2014, pp. 1056–1062.

[242] W. Qian, D. Guo, K. Li, X. Tian, and M. Wang, "Dual-path tokenlearner for remote photoplethysmography-based physiological measurement with facial videos," 2023, *arXiv:2308.07771*.

[243] X. Liu, W. Wei, H. Kuang, and X. Ma, "Heart rate measurement based on 3D central difference convolution with attention mechanism," *Sensors*, vol. 22, no. 2, p. 688, Jan. 2022, doi: 10.3390/s22020688.

[244] J. Speth, N. Vance, P. Flynn, and A. Czajka, "Non-contrastive unsupervised learning of physiological signals from video," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. (CVPR)*, Jun. 2023, pp. 14464–14474, doi: 10.1109/CVPR52729.2023.01390.

[245] J. Comas, A. Ruiz, and F. Sukno, "Efficient remote photoplethysmography with temporal derivative modules and time-shift invariant loss," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2022, pp. 2181–2190, doi: 10.1109/CVPRW56347.2022.00237.

[246] Z. Sun and X. Li, "Contrast-Phys+: Unsupervised and weakly-supervised video-based remote physiological measurement via spatiotemporal contrast," *IEEE Trans. Pattern Anal. Mach. Intell.*, 2024, doi: 10.1109/TPAMI.2024.3367910.

[247] M. Hu, D. Guo, M. Jiang, F. Qian, X. Wang, and F. Ren, "RPPG-based heart rate estimation using spatial–temporal attention network," *IEEE Trans. Cogn. Develop. Syst.*, vol. 14, no. 4, pp. 1630–1641, Dec. 2022, doi: 10.1109/TCDS.2021.3131197.


Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[248] X. Fan et al., "Remote photoplethysmography based on reflected light angle estimation," *Physiol. Meas.*, vol. 45, no. 3, Mar. 2024, Art. no. 035005.
[249] H. Gao, C. Zhang, S. Pei, and X. Wu, "IDTL-rPPG: Remote heart rate estimation using instance-based deep transfer learning," *Biomed. Signal Process. Control*, vol. 95, Sep. 2024, Art. no. 106416.
[250] Z. Sun and X. Li, "Contrast-phys: Unsupervised video-based remote physiological measurement via spatiotemporal contrast," in *Proc. Eur. Conf. Comput. Vis. (ECCV)*, 2022, doi: 10.1007/978-3-031-19775-8_29.
[251] G. Heusch, A. Anjos, and S. Marcel, "A reproducible study on remote heart rate measurement," 2017, *arXiv:1709.00962*.
[252] Z. Zhang et al., "Multimodal spontaneous emotion corpus for human behavior analysis," in *Proc. IEEE Conf. Comput. Vis. Pattern Recognit. (CVPR)*, Jun. 2016, pp. 3438–3446.
[253] Z. Yang, H. Wang, and F. Lu, "Assessment of deep learning-based heart rate estimation using remote photoplethysmography under different illuminations," *IEEE Trans. Hum.-Mach. Syst.*, vol. 52, no. 6, pp. 1236–1246, Dec. 2022.
[254] J. Geng, C. Zhang, H. Gao, Y. Lv, and X. Wu, "Motion resistant facial video based heart rate estimation method using head-mounted camera," in *Proc. IEEE Int. Conferences Internet Things (iThings), IEEE Green Comput. Commun. (GreenCom), IEEE Cyber, Phys. Social Comput. (CPSCom), IEEE Smart Data (SmartData), IEEE Congr. Cybermatics (Cybermatics)*, Dec. 2021, pp. 229–237.
[255] Z. Hasan, S. R. Ramamurthy, and N. Roy, 2021, "MPSC-rPPG dataset," *IEEE DataPort*, doi: 10.21227/ddgz-tx88.
[256] W. Sun et al., "Resolve domain conflicts for generalizable remote physiological measurement," in *Proc. 31st ACM Int. Conf. Multimedia*, Oct. 2023, doi: 10.1145/3581783.3612265.
[257] X. Li et al., "The OBF database: A large face video database for remote physiological signal measurement and atrial fibrillation detection," in *Proc. 13th IEEE Int. Conf. Autom. Face Gesture Recognit. (FG)*, May 2018, pp. 242–249.
[258] Y. Dong, G. Yang, and Y. Yin, "DRNet: Decomposition and reconstruction network for remote physiological measurement," 2022, *arXiv:2206.05687*.
[259] C. Wu, Z. Yuan, S. Wan, L. Wang, and W. Zhang, "Anti-jamming heart rate estimation using a spatial–temporal fusion network," *Comput. Vis. Image Understand.*, vol. 216, Feb. 2022, Art. no. 103327, doi: 10.1016/j.cviu.2021.103327.
[260] X. Zhang et al., "Self-similarity prior distillation for unsupervised remote physiological measurement," 2023, *arXiv:2311.05100*.
[261] C.-H. Cheng et al., "Contactless blood oxygen saturation estimation from facial videos using deep learning," *Bioengineering*, vol. 11, no. 3, p. 251, Mar. 2024.
[262] S. Koelstra et al., "DEAP: A database for emotion analysis using physiological signals," *IEEE Trans. Affective Comput.*, vol. 3, no. 1, pp. 18–31, Jan. 2012.
[263] A. M. Unakafov, "Pulse rate estimation using imaging photoplethysmography: Generic framework and comparison of methods on a publicly available dataset," *Biomed. Phys. Eng. Exp.*, vol. 4, no. 4, Apr. 2018, Art. no. 045001, doi: 10.1088/2057-1976/aabd09.
[264] S. Bobbia, R. Macwan, Y. Benezeth, A. Mansouri, and J. Dubois, "Unsupervised skin tissue segmentation for remote photoplethysmography," *Pattern Recognit. Lett.*, vol. 124, pp. 82–90, Jun. 2019.
[265] F. Bousefsaf, C. Maaoui, and A. Pruski, "Automatic selection of webcam photoplethysmographic pixels based on lightness criteria," *J. Med. Biol. Eng.*, vol. 37, no. 3, pp. 374–385, Jun. 2017.
[266] L.-M. Po, L. Feng, Y. Li, X. Xu, T. C.-H. Cheung, and K.-W. Cheung, "Block-based adaptive ROI for remote photoplethysmography," *Multimedia Tools Appl.*, vol. 77, no. 6, pp. 6503–6529, Mar. 2018.
[267] A. Woyczyk, V. Fleischhauer, and S. Zaunseder, "Adaptive Gaussian mixture model driven level set segmentation for remote pulse rate detection," *IEEE J. Biomed. Health Informat.*, vol. 25, no. 5, pp. 1361–1372, May 2021.
[268] J. Laurie, N. Higgins, T. Peynot, and J. Roberts, "Dedicated exposure control for remote photoplethysmography," *IEEE Access*, vol. 8, pp. 116642–116652, 2020.
[269] H.-W. Huang et al., "Mobile robotic platform for contactless vital sign monitoring," *Cyborg Bionic Syst.*, vol. 2022, Jan. 2022.
[270] J. Herranz Olazábal, F. Wieringa, E. Hermeling, and C. Van Hoof, "Camera-derived photoplethysmography (rPPG) and speckle plethysmography (rSPG): Comparing reflective and transmissive mode at various integration times using LEDs and lasers," *Sensors*, vol. 22, no. 16, p. 6059, Aug. 2022, doi: 10.3390/s22166059.
[271] J. Herranz Olazabal, F. Wieringa, E. Hermeling, and C. Van Hoof, "Comparing remote speckle plethysmography and finger-clip photoplethysmography with non-invasive finger arterial pressure pulse waves, regarding morphology and arrival time," *Bioengineering*, vol. 10, no. 1, p. 101, Jan. 2023, doi: 10.3390/bioengineering10010101.
[272] A. Trumpp, P. L. Bauer, S. Rasche, H. Malberg, and S. Zaunseder, "The value of polarization in camera-based photoplethysmography," *Biomed. Opt. Exp.*, vol. 8, no. 6, pp. 2822–2834, 2017.
[273] R. Irani, K. Nasrollahi, and T. B. Moeslund, "Improved pulse detection from head motions using DCT," in *Proc. Int. Conf. Comput. Vis. Theory Appl.*, vol. 3, 2014, pp. 118–124.
[274] J.-P. Lomaliza and H. Park, "Detecting pulse from head motions using smartphone camera," in *Proc. Int. Conf. Adv. Eng. Theory Appl.* Springer, 2016, pp. 243–251.
[275] G. Balakrishnan, "Analyzing pulse from head motions in video," Ph.D. issertation, Massachusetts Inst. Technol., Cambridge, MA, USA, 2014.
[276] H. Lee, A. Cho, S. Lee, and M. Whang, "Vision-based measurement of heart rate from ballistocardiographic head movements using unsupervised clustering," *Sensors*, vol. 19, no. 15, p. 3263, Jul. 2019.
[277] A. Al-Naji and J. Chahl, "Contactless cardiac activity detection based on head motion magnification," *Int. J. Image Graph.*, vol. 17, no. 1, Jan. 2017, Art. no. 1750001.
[278] X. Liu, X. Yang, Z. Meng, Y. Wang, J. Zhang, and A. Wong, "MANet: A motion-driven attention network for detecting the pulse from a facial video with drastic motions," in *Proc. IEEE/CVF Int. Conf. Comput. Vis. Workshops (ICCVW)*, Oct. 2021, pp. 2385–2390.
[279] M. van Gastel, S. Stuijk, and G. de Haan, "Motion robust remote-PPG in infrared," *IEEE Trans. Biomed. Eng.*, vol. 62, no. 5, pp. 1425–1433, May 2015.
[280] W. Wang, S. Stuijk, and G. de Haan, "Exploiting spatial redundancy of image sensor for motion robust rPPG," *IEEE Trans. Biomed. Eng.*, vol. 62, no. 2, pp. 415–425, Feb. 2015.
[281] Y. Yang, C. Liu, H. Yu, D. Shao, F. Tsow, and N. Tao, "Motion robust remote photoplethysmography in CIELab color space," *J. Biomed. Opt.*, vol. 21, no. 11, Nov. 2016, Art. no. 117001.
[282] B.-F. Wu, B.-J. Wu, S.-E. Cheng, Y. Sun, and M.-L. Chung, "Motion-robust atrial fibrillation detection based on remote-photoplethysmography," *IEEE J. Biomed. Health Informat.*, May 2022.
[283] H. Wang, X. Yang, X. Liu, and D. Wang, "Heart rate estimation from facial videos with motion interference using T-SNE-based signal separation," *Biomed. Opt. Exp.*, vol. 13, no. 9, p. 4494, Sep. 2022.
[284] Y. Liu et al., "Motion-robust multimodal heart rate estimation using BCG fused remote-PPG with deep facial ROI tracker and pose constrained Kalman filter," *IEEE Trans. Instrum. Meas.*, vol. 70, pp. 1–15, 2021.
[285] D. Cho, J. Kim, K. J. Lee, and S. Kim, "Reduction of motion artifacts from remote photoplethysmography using adaptive noise cancellation and modified HSI model," *IEEE Access*, vol. 9, pp. 122655–122667, 2021.
[286] M. A. Hassan, A. S. Malik, N. Saad, D. Fofi, and F. Meriaudeau, "Effect of motion artifact on digital camera based heart rate measurement," in *Proc. 39th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2017, pp. 2851–2854.
[287] S. K. A. Prakash and C. S. Tucker, "Bounded Kalman filter method for motion-robust, non-contact heart rate estimation," *Biomed. Opt. Exp.*, vol. 9, no. 2, pp. 873–897, Feb. 2018.
[288] Y. Sun, "Motion-compensated noncontact imaging photoplethysmography to monitor cardiorespiratory status during exercise," *J. Biomed. Opt.*, vol. 16, no. 7, Jul. 2011, Art. no. 077010.
[289] H. Rahman, M. U. Ahmed, and S. Begum, "Non-contact physiological parameters extraction using facial video considering illumination, motion, movement and vibration," *IEEE Trans. Biomed. Eng.*, vol. 67, no. 1, pp. 88–98, Jan. 2020.
[290] N. S. Suriani, N. A. Jumain, A. A. Ali, and N. H. Mohd, "Facial video based heart rate estimation for physical exercise," in *Proc. IEEE Symp. Ind. Electron. Appl. (ISIEA)*, Jul. 2021, pp. 1–5.
[291] Y. Napolean, A. Marwade, N. Tomen, P. Alkemade, T. Eijsvogels, and J. C. van Gemert, "Heart rate estimation in intense exercise videos," in *Proc. IEEE Int. Conf. Image Process. (ICIP)*, Oct. 2022, pp. 3933–3937.
[292] M. Hu, F. Qian, X. Wang, L. He, D. Guo, and F. Ren, "Robust heart rate estimation with spatial–temporal attention network from facial videos," *IEEE Trans. Cogn. Develop. Syst.*, vol. 14, no. 2, pp. 639–647, Jun. 2022.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[293] D. Botina-Monsalve et al., "Long short-term memory deep-filter in remote photoplethysmography," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2020, pp. 1242–1249.

[294] O.-Y. Batubayaer, Y.-J. Zhao, L.-Q. Kong, L.-Q. Dong, M. Liu, and M. Hui, "Adaptive non-contact robust heart rate detection method under head rotation motion," *Acta Phys. Sinica*, vol. 71, no. 5, 2022, Art. no. 058704, doi: 10.7498/aps.71.20211634.

[295] X. Niu, S. Shan, H. Han, and X. Chen, "RhythmNet: End-to-end heart rate estimation from face via spatial–temporal representation," *IEEE Trans. Image Process.*, vol. 29, pp. 2409–2423, 2020, doi: 10.1109/TIP.2019.2947204.

[296] M. A. Hassan, A. S. Malik, D. Fofi, N. M. Saad, Y. S. Ali, and F. Meriaudeau, "Video-based heartbeat rate measuring method using ballistocardiography," *IEEE Sensors J.*, vol. 17, no. 14, pp. 4544–4557, Jul. 2017, doi: 10.1109/JSEN.2017.2708133.

[297] S. Kado, Y. Monno, K. Yoshizaki, M. Tanaka, and M. Okutomi, "Spatial–spectral–temporal fusion for remote heart rate estimation," *IEEE Sensors J.*, vol. 20, no. 19, pp. 11688–11697, Oct. 2020, doi: 10.1109/JSEN.2020.2997785.

[298] R. Zhong, Y. Zhou, and C. Gou, "EST-TSANet: Video-based remote heart rate measurement using temporal shift attention network and ESTmap," *IEEE Trans. Instrum. Meas.*, vol. 73, pp. 1–14, 2024, doi: 10.1109/TIM.2023.3331414.

[299] Q. Zhang, X. Lin, Y. Zhang, Q. Liu, and F. Cai, "Non-contact high precision pulse-rate monitoring system for moving subjects in different motion states," *Med. Biol. Eng. Comput.*, vol. 61, no. 10, pp. 2769–2783, Oct. 2023, doi: 10.1007/s11517-023-02884-1.

[300] R. P. Dresher and Y. Mendelson, "Reflectance forehead pulse oximetry: Effects of contact pressure during walking," in *Proc. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2006.

[301] L. Shan and M. Yu, "Video-based heart rate measurement using head motion tracking and ICA," in *Proc. 6th Int. Congr. Image Signal Process. (CISP)*, vol. 1, Dec. 2013, pp. 160–164.

[302] M. A. Adelabu, A. L. Imoize, and K. E. Adesoji, "Enhancement of a camera-based continuous heart rate measurement algorithm," *Social Netw. Comput. Sci.*, vol. 3, no. 4, p. 284, Jul. 2022.

[303] M. A. Haque, R. Irani, K. Nasrollahi, and T. B. Moeslund, "Heartbeat rate measurement from facial video," *IEEE Intell. Syst.*, vol. 31, no. 3, pp. 40–48, May 2016.

[304] E. Kviesis-Kipge and U. Rubins, "Remote photoplethysmography device with adaptive illumination for skin microcirculation assessment," *Proc. SPIE*, vol. 11585, Oct. 2020, Art. no. 1158505.

[305] W. Wang, A. C. den Brinker, S. Stuijk, and G. de Haan, "Robust heart rate from fitness videos," *Physiol. Meas.*, vol. 38, no. 6, pp. 1023–1044, Jun. 2017.

[306] P. Gupta, B. Bhowmick, and A. Pal, "MOMBAT: Heart rate monitoring from face video using pulse modeling and Bayesian tracking," *Comput. Biol. Med.*, vol. 121, Jun. 2020, Art. no. 103813.

[307] S. H. Fouladi, I. Balasingham, T. A. Ramstad, and K. Kansanen, "Accurate heart rate estimation from camera recording via MUSIC algorithm," in *Proc. 37th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Aug. 2015, pp. 7454–7457.

[308] W. Wang, L. Vosters, and A. C. den Brinker, "Modified camera setups for day-and-night pulse-rate monitoring," in *Proc. 43rd Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Nov. 2021, pp. 1744–1748.

[309] X. Yang, Z. Zhang, Y. Huang, Y. Zheng, and Y. Shen, "Using a graph-based image segmentation algorithm for remote vital sign estimation and monitoring," *Sci. Rep.*, vol. 12, no. 1, p. 15197, Sep. 2022.

[310] Lekshmy. H. Nair and P. R. Aparna, "Non-contact heart-rate measurement using KLT-algorithm," in *Proc. 2nd Int. Conf. Electron., Commun. Aerosp. Technol. (ICECA)*, Mar. 2018, pp. 1944–1947.

[311] X. Zheng, C. Zhang, H. Chen, Y. Zhang, and X. Yang, "Remote measurement of heart rate from facial video in different scenarios," *Measurement*, vol. 188, Jan. 2022, Art. no. 110243.

[312] M. Chen, X. Liao, and M. Wu, "PulseEdit: Editing physiological signals in facial videos for privacy protection," *IEEE Trans. Inf. Forensics Security*, vol. 17, pp. 457–471, 2022.

[313] M. Chen, A. Jayaweera, C.-W. Wong, and M. Wu, "Identity-privacy protection for facial-rPPG based smart health research," *Authorea Preprints*, Jul. 2023.

[314] Z. Sun and X. Li, "Privacy-phys: Facial video-based physiological modification for privacy protection," *IEEE Signal Process. Lett.*, vol. 29, pp. 1507–1511, 2022, doi: 10.1109/LSP.2022.3185964.

[315] Z. Hasan, E. Dey, S. R. Ramamurthy, N. Roy, and A. Misra, "RhythmEdge: Enabling contactless heart rate estimation on the edge," in *Proc. IEEE Int. Conf. Smart Comput. (SMARTCOMP)*, Jun. 2022, pp. 92–99.

[316] R.-N. Yin et al., "Heart rate estimation based on face video under unstable illumination," *Int. J. Speech Technol.*, vol. 51, no. 8, pp. 5388–5404, Aug. 2021.

[317] Y. C. Lin and Y. H. Lin, "A study of color illumination effect on the SNR of rPPG signals," in *Proc. 39th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2017, pp. 4301–4304.

[318] W. Wang, L. Vosters, and A. C. den Brinker, "Continuous-spectrum infrared illuminator for camera-PPG in darkness," *Sensors*, vol. 20, no. 11, p. 3044, May 2020.

[319] R. Song, J. Li, M. Wang, J. Cheng, C. Li, and X. Chen, "Remote photoplethysmography with an EEMD-MCCA method robust against spatially uneven illuminations," *IEEE Sensors J.*, vol. 21, no. 12, pp. 13484–13494, Jun. 2021.

[320] N. Ahmadi et al., "Development and evaluation of a contactless heart rate measurement device based on rPPG," in *Proc. 29th IEEE Int. Conf. Electron., Circuits Syst. (ICECS)*, Oct. 2022, pp. 1–4.

[321] H. Lu, Z. Yu, X. Niu, and Y. Chen, "Neuron structure modeling for generalizable remote physiological measurement," in *Proc. IEEE/CVF Conf. Comput. Vis. Pattern Recognit. (CVPR)*, Jun. 2023, pp. 18589–18599, doi: 10.1109/CVPR52729.2023.01783.

[322] R. J. van Esch et al., "Video health monitoring for cardiac arrhythmia detection in a real hospital scenario," in *Medical Imaging 2023: Imaging Informatics for Healthcare, Research, and Applications*, vol. 12469. Bellingham, WA, USA: SPIE, 2023, pp. 65–70, doi: 10.1117/12.2653550.

[323] L. Tarassenko, M. Villarroel, A. Guazzi, J. Jorge, D. A. Clifton, and C. Pugh, "Non-contact video-based vital sign monitoring using ambient light and auto-regressive models," *Physiol. Meas.*, vol. 35, no. 5, pp. 807–831, May 2014, doi: 10.1088/0967-3334/35/5/807.

[324] G. Casalino, G. Castellano, and G. Zaza, "A mHealth solution for contact-less self-monitoring of blood oxygen saturation," in *Proc. IEEE Symp. Comput. Commun. (ISCC)*, Jul. 2020, pp. 1–7, doi: 10.1109/ISCC50000.2020.9219718.

[325] G. Casalino, G. Castellano, and G. Zaza, "Evaluating the robustness of a contact-less mHealth solution for personal and remote monitoring of blood oxygen saturation," *J. Ambient Intell. Humanized Comput.*, vol. 14, no. 7, pp. 8871–8880, Jul. 2023, doi: 10.1007/s12652-021-03635-6.

[326] N. H. Kim, S.-G. Yu, S.-E. Kim, and E. C. Lee, "Non-contact oxygen saturation measurement using YCgCr color space with an RGB camera," *Sensors*, vol. 21, no. 18, p. 6120, Sep. 2021, doi: 10.3390/s21186120.

[327] B. Wei, X. Wu, C. Zhang, and Z. Lv, "Analysis and improvement of non-contact $SpO_2$ extraction using an RGB webcam," *Biomed. Opt. Exp.*, vol. 12, no. 8, pp. 5227–5245, 2021, doi: 10.1364/boe.423508.

[328] T. Stogiannopoulos, G.-A. Cheimariotis, and N. Mitianoudis, "A study of machine learning regression techniques for non-contact $SpO_2$ estimation from infrared motion-magnified facial video," *Information*, vol. 14, no. 6, p. 301, May 2023, doi: 10.3390/info14060301.

[329] L. Kong et al., "Non-contact detection of oxygen saturation based on visible light imaging device using ambient light," *Opt. Exp.*, vol. 21, no. 15, p. 17464, 2013, doi: 10.1364/oe.21.017464.

[330] W. Verkruysse, M. Bartula, E. Bresch, M. Rocque, M. Meftah, and I. Kirenko, "Calibration of contactless pulse oximetry," *Anesthesia Analgesia*, vol. 124, no. 1, pp. 136–145, Jan. 2017, doi: 10.1213/ane.0000000000001381.

[331] A. Al-Naji, G. A. Khalid, J. F. Mahdi, and J. Chahl, "Non-contact $SpO_2$ prediction system based on a digital camera," *Appl. Sci.*, vol. 11, no. 9, p. 4255, May 2021, doi: 10.3390/app11094255.

[332] D. Shao et al., "Noncontact monitoring of blood oxygen saturation using camera and dual-wavelength imaging system," *IEEE Trans. Biomed. Eng.*, vol. 63, no. 6, pp. 1091–1098, Jun. 2016, doi: 10.1109/TBME.2015.2481896.

[333] L. Xi, X. Wu, W. Chen, J. Wang, and C. Zhao, "Weighted combination and singular spectrum analysis based remote photoplethysmography pulse extraction in low-light environments," *Med. Eng. Phys.*, vol. 105, Jul. 2022, Art. no. 103822, doi: 10.1016/j.medengphy.2022.103822.

[334] Y. Kurzweil-Segev et al., "Remote monitoring of phasic heart rate changes from the palm," *IEEE Trans. Terahertz Sci. Technol.*, vol. 4, no. 5, pp. 618–623, Sep. 2014.

[335] V. Selvaraju et al., "Continuous monitoring of vital signs using cameras: A systematic review," *Sensors*, vol. 22, no. 11, p. 4097, May 2022.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.

[336] M. Attas, M. Hewko, J. Payette, T. Posthumus, M. Sowa, and H. Mantsch, "Visualization of cutaneous hemoglobin oxygenation and skin hydration using near-infrared spectroscopic imaging," *Skin Res. Technol.*, vol. 7, no. 4, pp. 238–245, Nov. 2001.

[337] K. J. Zuzak, M. D. Schaeberle, E. N. Lewis, and I. W. Levin, "Visible reflectance hyperspectral imaging: Characterization of a noninvasive, in vivo system for determining tissue perfusion," *Anal. Chem.*, vol. 74, no. 9, pp. 2021–2028, May 2002.

[338] K. J. Zuzak, R. P. Francis, E. F. Wehner, M. Litorja, J. A. Cadeddu, and E. H. Livingston, "Active DLP hyperspectral illumination: A noninvasive, in vivo, system characterization visualizing tissue oxygenation at near video rates," *Anal. Chem.*, vol. 83, no. 19, pp. 7424–7430, Oct. 2011.

[339] F. P. Wieringa, F. Mastik, R. H. Boks, A. Visscher, A. J. J. C. Bogers, and A. F. W. Van der Steen, "In vitro demonstration of an $SpO_2$-camera," in *Proc. Comput. Cardiol.*, Sep. 2007, doi: 10.1109/CIC.2007.4745594.

[340] F. P. Wieringa, F. Mastik, and A. F. W. V. D. Steen, "Contactless multiple wavelength photoplethysmographic imaging: A first step toward '$SpO_2$ camera' technology," *Ann. Biomed. Eng.*, vol. 33, no. 8, pp. 1034–1041, Aug. 2005, doi: 10.1007/s10439-005-5763-2.

[341] C.-J. Wu, A. Quigley, and D. Harris-Birtill, "Out of sight: A toolkit for tracking occluded human joint positions," *Pers. Ubiquitous Comput.*, vol. 21, no. 1, pp. 125–135, Feb. 2017.

[342] K. Zheng, J. Kong, L. Tian, B. Li, H. Li, and J. Zhou, "Hand-over-face occlusion and distance adaptive heart rate detection based on imaging photoplethysmography and pixel distance in online learning," *Biomed. Signal Process. Control*, vol. 85, Aug. 2023, Art. no. 104898, doi: 10.1016/j.bspc.2023.104898.

[343] D. Avola, L. Cinque, S. Levialdi, and G. Placidi, "Human body language analysis: A preliminary study based on Kinect skeleton tracking," in *Proc. Int. Conf. Image Anal. Process.* Springer, 2013.

[344] T. Ballendat, N. Marquardt, and S. Greenberg, "Proxemic interaction: Designing for a proximity and orientation-aware environment," in *Proc. ACM Int. Conf. Interact. Tabletops Surf.*, Nov. 2010, pp. 121–130.

[345] V. Frati and D. Prattichizzo, "Using Kinect for hand tracking and rendering in wearable haptics," in *Proc. IEEE World Haptics Conf.*, Jun. 2011, pp. 317–321, doi: 10.1109/WHC.2011.5945505.

[346] L. A. Seewald, L. Gonzaga, M. R. Veronez, V. P. Minotto, and C. R. Jung, "Combining SRP-PHAT and two Kinects for 3D sound source localization," *Expert Syst. Appl.*, vol. 41, no. 16, pp. 7106–7113, Nov. 2014.

[347] W. Gai et al., "Employing shadows for multi-person tracking based on a single RGB-D camera," *Sensors*, vol. 20, no. 4, p. 1056, Feb. 2020.

[348] A. R. Guazzi et al., "Non-contact measurement of oxygen saturation with an RGB camera," *Biomed. Opt. Exp.*, vol. 6, no. 9, pp. 3320–3338, 2015, doi: 10.1364/boe.6.003320.

[349] B. Xu, H. Madhu, R. Kulkarni, L. K. Mestha, S. Kyal, and G. Pennington, "Evaluating and improving the robustness of a video-based PR/RR monitoring system for a clinical environment," in *Proc. IEEE Healthcare Innov. Point-of-Care Technol. Conf. (HI-POCT)*, Nov. 2016, pp. 204–207, doi: 10.1109/HIC.2016.7797732.

[350] Y. Sun, C. Papin, V. Azorin-Peris, R. Kalawsky, S. Greenwald, and S. Hu, "Comparison of scientific CMOS camera and webcam for monitoring cardiac pulse after exercise," *Proc. SPIE*, vol. 8135, Sep. 2011, Art. no. 813506, doi: 10.1117/12.893362.

[351] O. Gupta, D. McDuff, and R. Raskar, "Real-time physiological measurement and visualization using a synchronized multi-camera system," in *Proc. IEEE Conf. Comput. Vis. Pattern Recognit. Workshops (CVPRW)*, Jun. 2016, pp. 312–319, doi: 10.1109/CVPRW.2016.46.

[352] Y. Sun, S. Hu, V. Azorin-Peris, R. Kalawsky, and S. Greenwald, "Non-contact imaging photoplethysmography to effectively access pulse rate variability," *J. Biomed. Opt.*, vol. 18, no. 6, Oct. 2012, Art. no. 061205, doi: 10.1117/1.jbo.18.6.061205.

[353] A. V. Moço, S. Stuijk, and G. de Haan, "Motion robust PPG-imaging through color channel mapping," *Biomed. Opt. Exp.*, vol. 7, no. 5, pp. 1737–1754, 2016, doi: 10.1364/BOE.7.001737.

[354] F. Haugg, M. Elgendi, and C. Menon, "GRGB rPPG: An efficient low-complexity remote photoplethysmography-based algorithm for heart rate estimation," *Bioengineering*, vol. 10, no. 2, p. 243, Feb. 2023, doi: 10.3390/bioengineering10020243.

[355] A. Al-Naji and J. Chahl, "Remote optical cardiopulmonary signal extraction with noise artifact removal, multiple subject detection & long-distance," *IEEE Access*, vol. 6, pp. 11573–11595, 2018, doi: 10.1109/ACCESS.2018.2811392.

[356] E. B. Blackford, J. Estepp, A. M. Piasecki, M. A. Bowers, and S. L. Klosterman, "Long-range non-contact imaging photoplethysmography: Cardiac pulse wave sensing at a distance," *Proc. SPIE*, vol. 9715, Mar. 2016, Art. no. 971512, doi: 10.1117/12.2208130.

[357] D. Nhan Tran, H. Lee, and C. Kim, "A robust real time system for remote heart rate measurement via camera," in *Proc. IEEE Int. Conf. Multimedia Expo (ICME)*, Jun. 2015, pp. 1–6.

[358] W. Wang and C. Shan, "Impact of makeup on remote-PPG monitoring," *Biomed. Phys. Eng. Exp.*, vol. 6, no. 3, Mar. 2020, Art. no. 035004.

Authorized licensed use limited to: BMS Institute of Technology. Downloaded on June 20,2026 at 17:46:46 UTC from IEEE Xplore. Restrictions apply.