
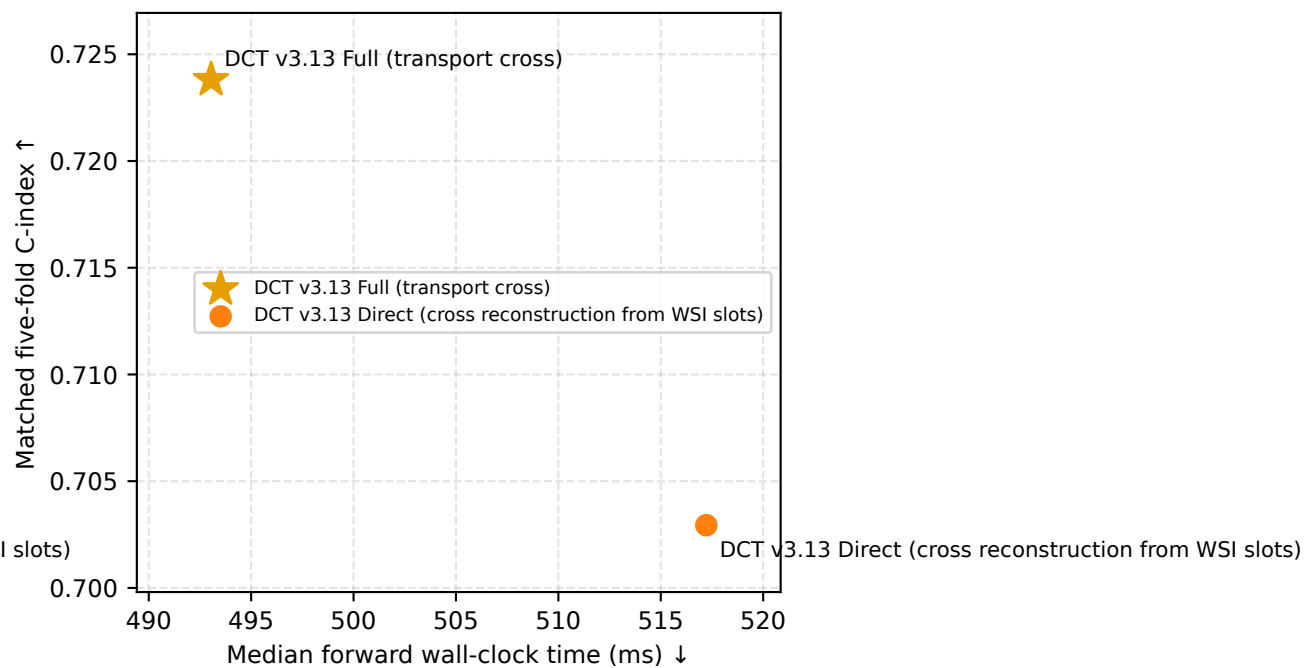


## DCT v3.13: performance / measured inference cost

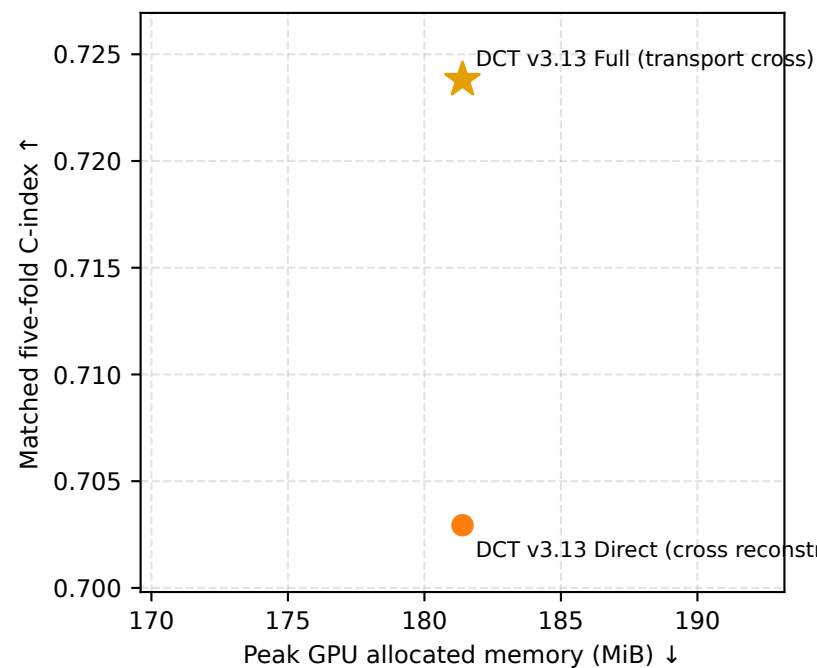

Same validation patients, UNI2-h WSI input, hardware, precision and timing settings; standard eval forward.