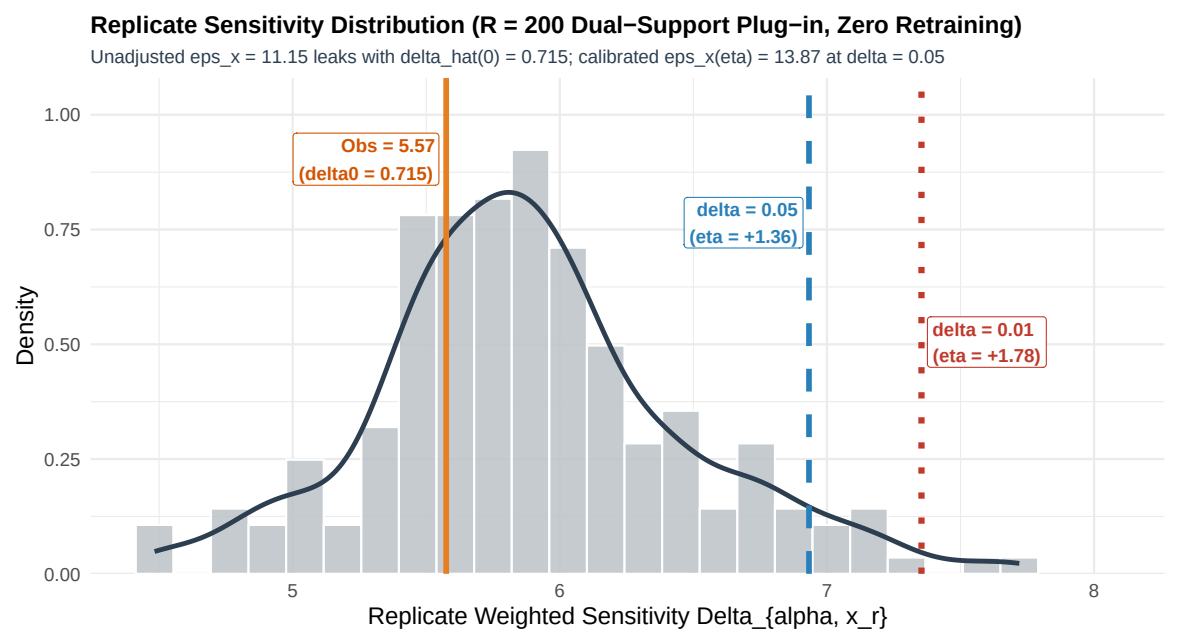
Replicate Sensitivity Distribution (R = 200 Dual−Support Plug−in, Zero Retraining)
Unadjusted eps_x = 11.15 leaks with delta_hat(0) = 0.715; calibrated eps_x(eta) = 13.87 at delta = 0.05
Obs = 5.57
(delta0 = 0.715)
delta = 0.05
(eta = +1.36)
delta = 0.01
(eta = +1.78)
Density
1.00
0.75
0.50
0.25
0.00
5
6
7
8
Replicate Weighted Sensitivity Delta_{alpha, x_r}