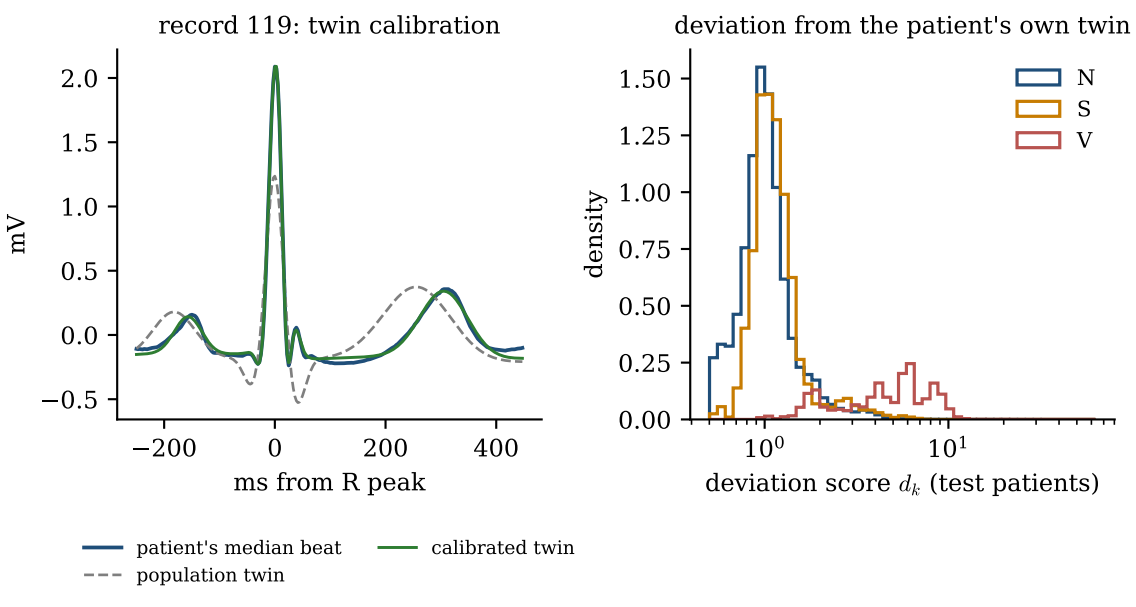
record 119: twin calibration
mV
2.0
1.5
1.0
0.5
0.0
−0.5
−200
0
200
400
ms from R peak
patient's median beat
calibrated twin
population twin
deviation from the patient's own twin
density
1.50
1.25
1.00
0.75
0.50
0.25
0.00
N
S
V
10^0
10^1
deviation score d_k (test patients)