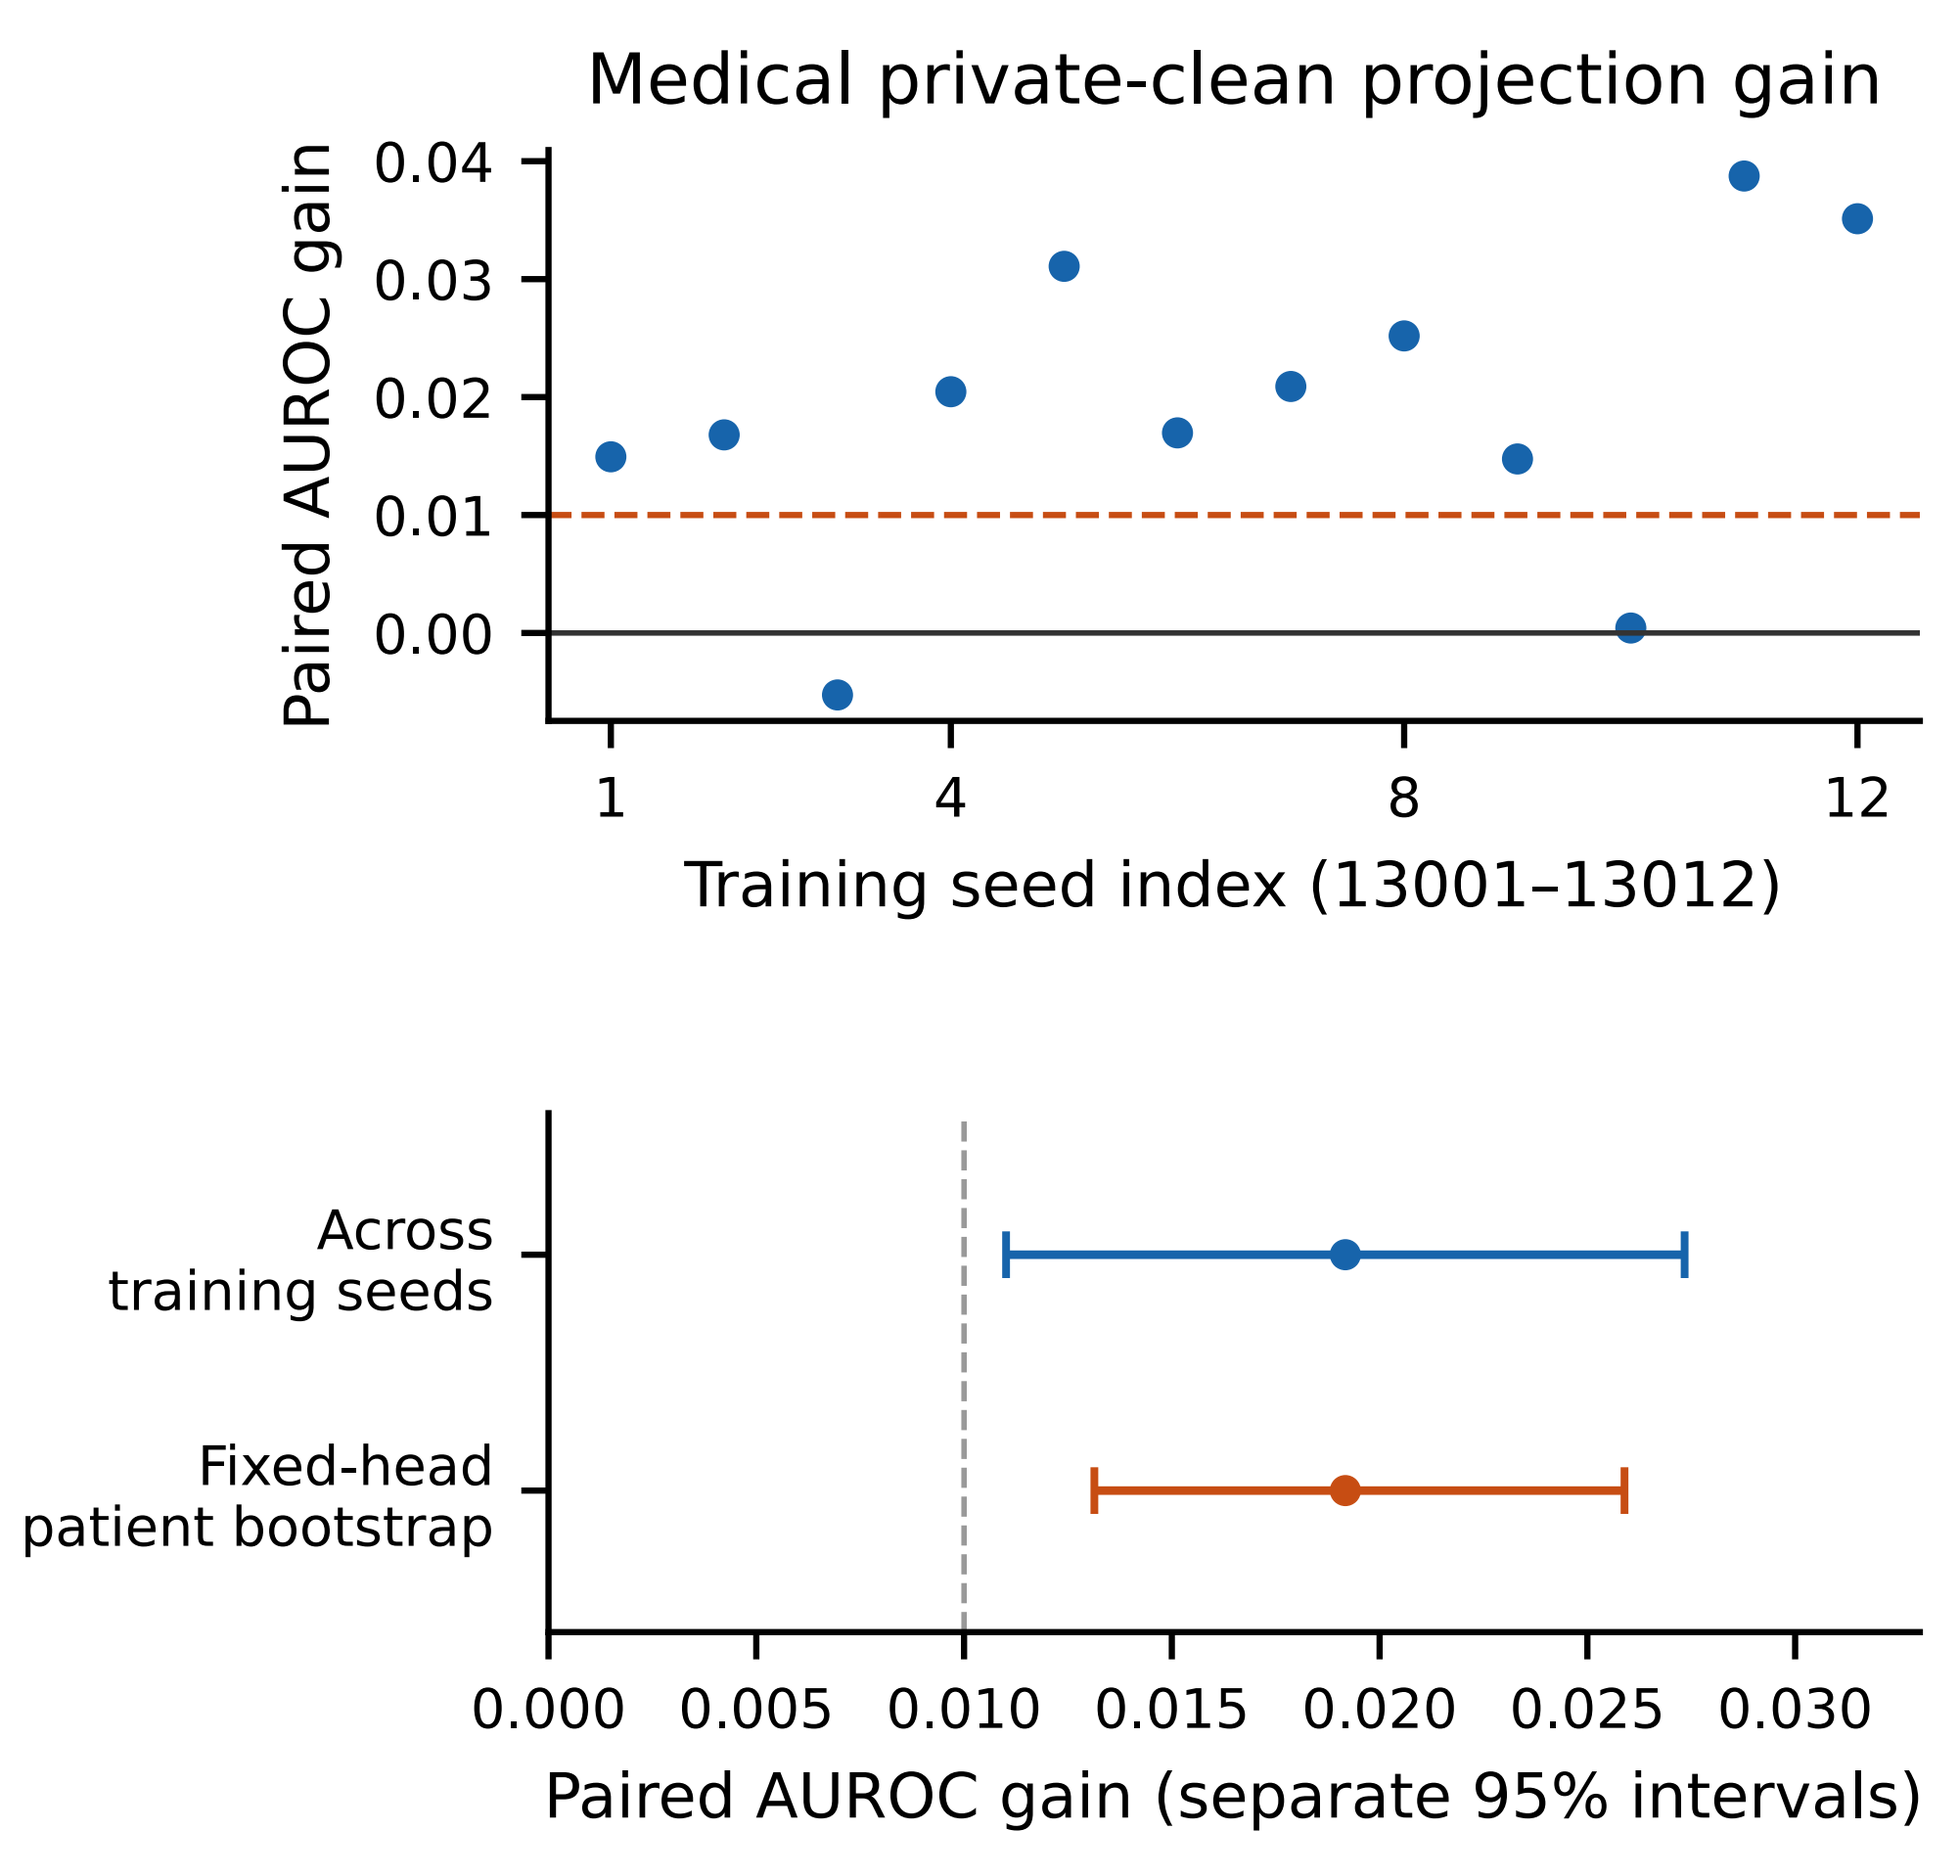
Medical private-clean projection gain
Paired AUROC gain
0.04
0.03
0.02
0.01
0.00
1
4
8
12
Training seed index (13001–13012)
Across
training seeds
Fixed-head
patient bootstrap
0.000
0.005
0.010
0.015
0.020
0.025
0.030
Paired AUROC gain (separate 95% intervals)