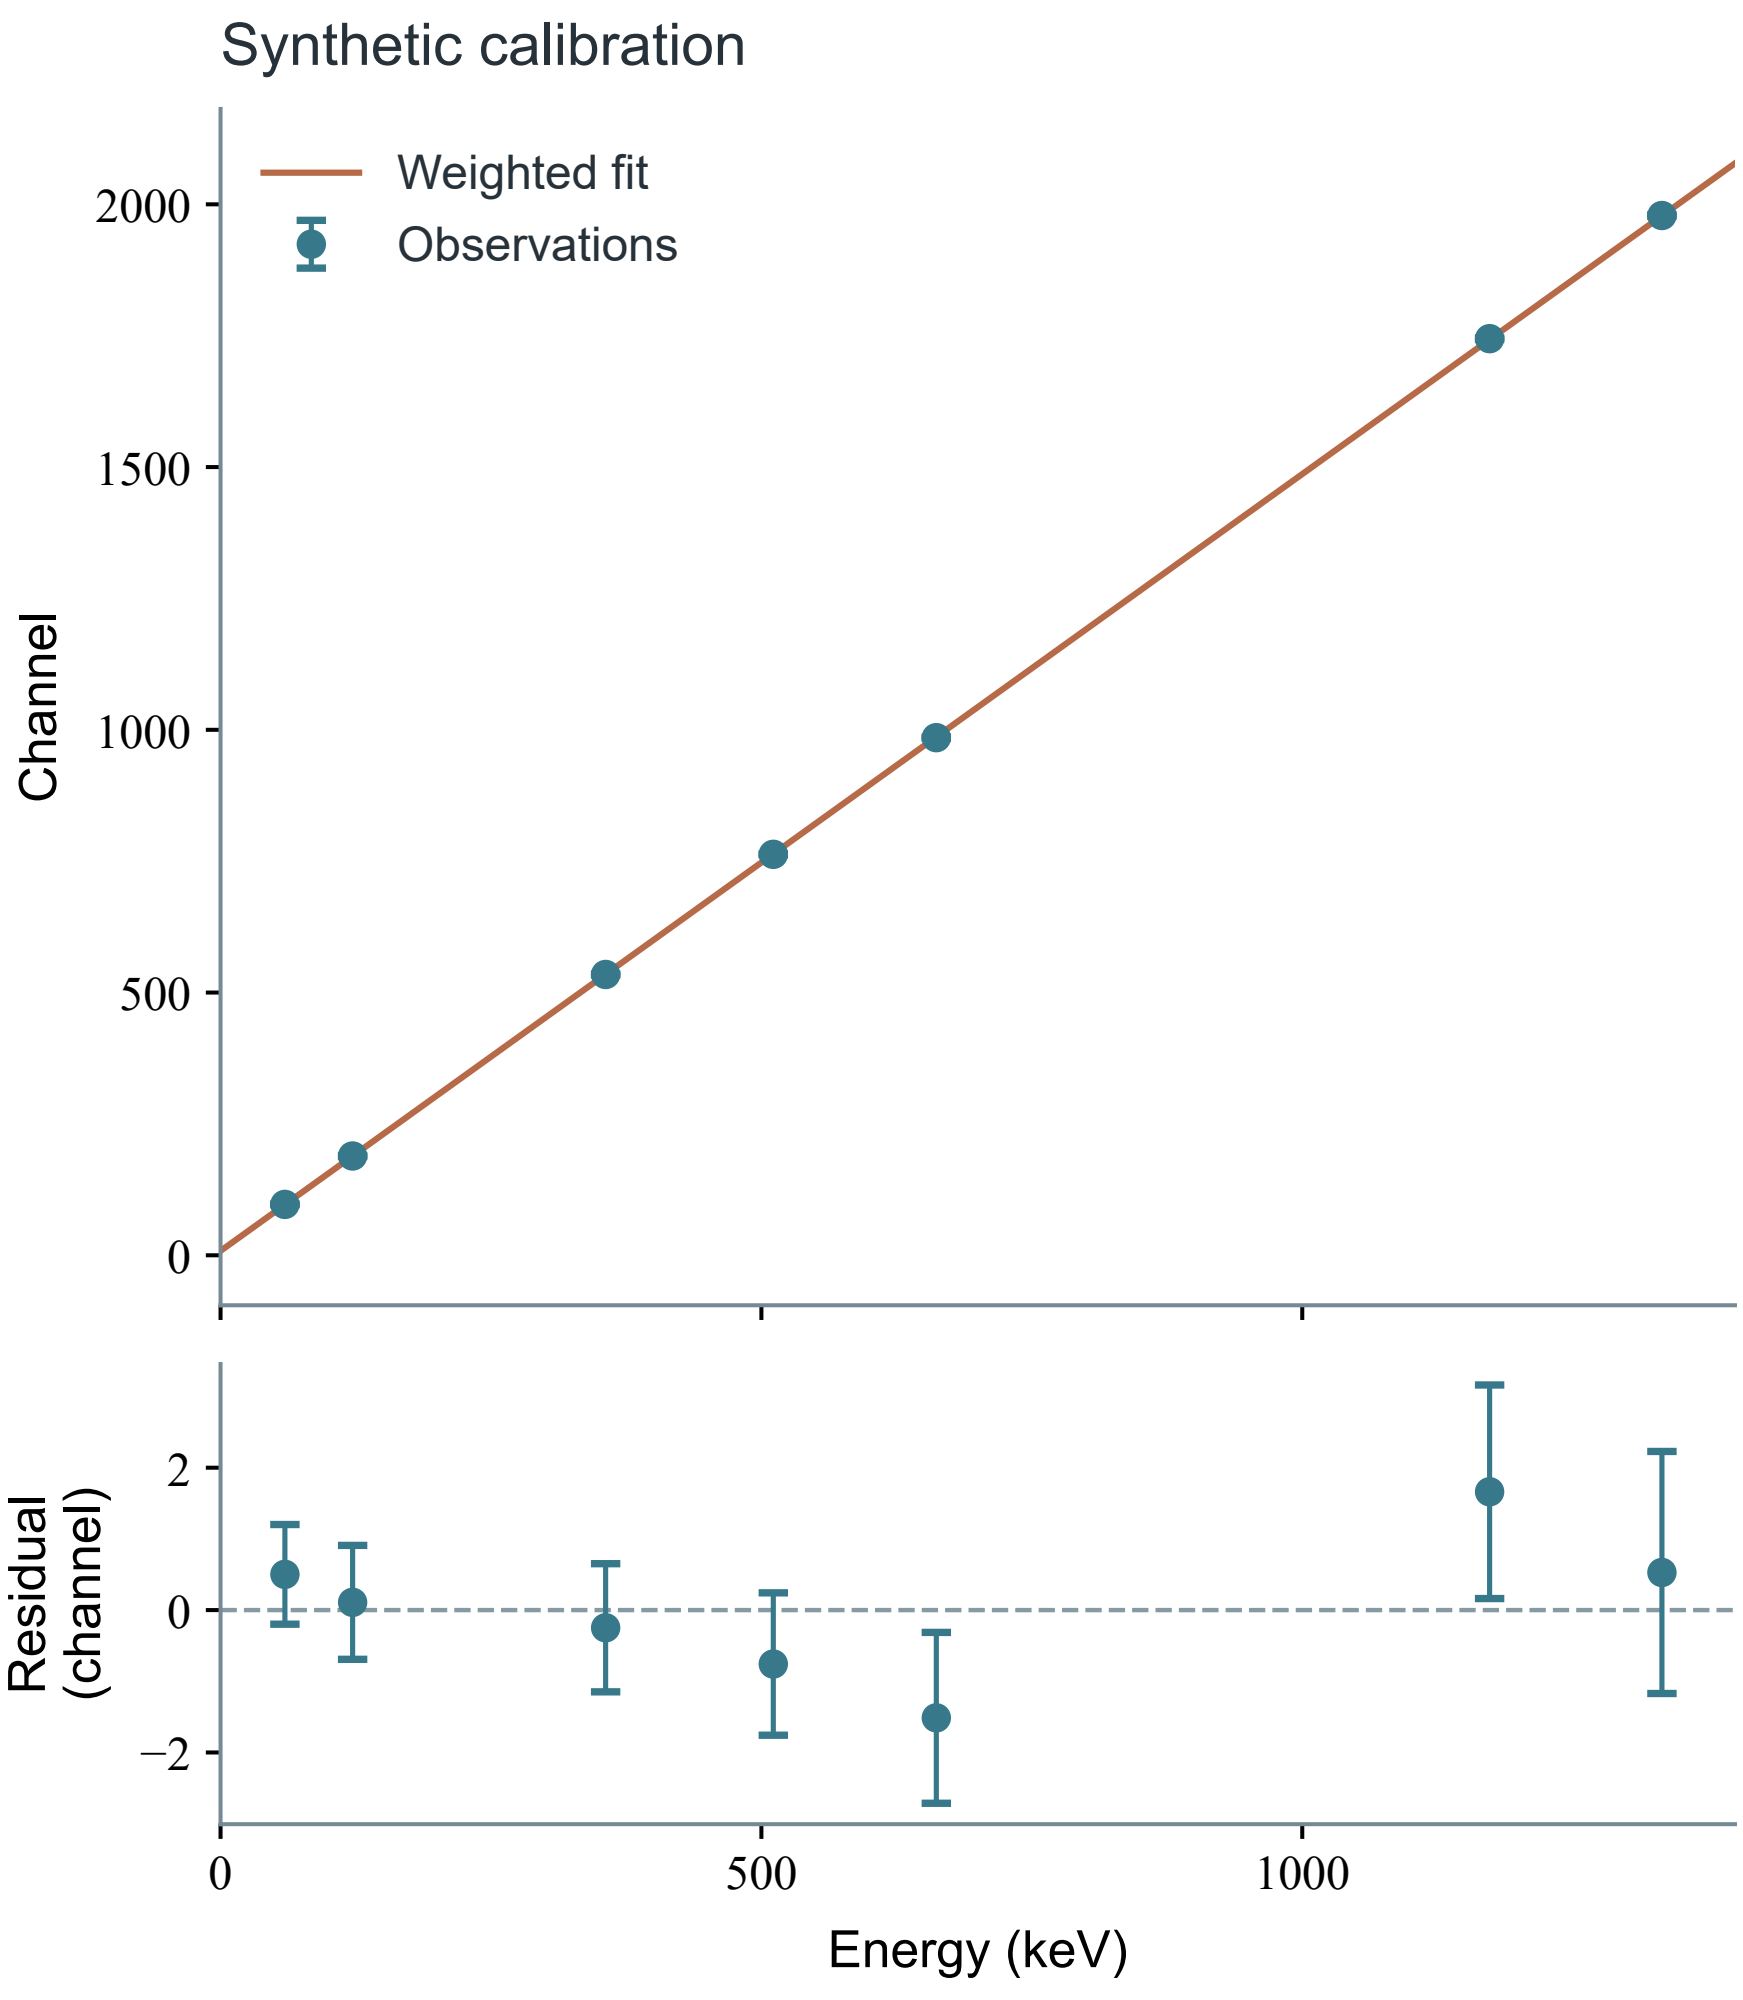
Synthetic calibration
Weighted fit
Observations
Channel
2000
1500
1000
500
0
Residual (channel)
2
0
−2
0
500
1000
Energy (keV)