



ECG 11924_NORM


Raw 12-lead ECG | ecg_id=11924 | label=NORM | amplitude=mV | time=s

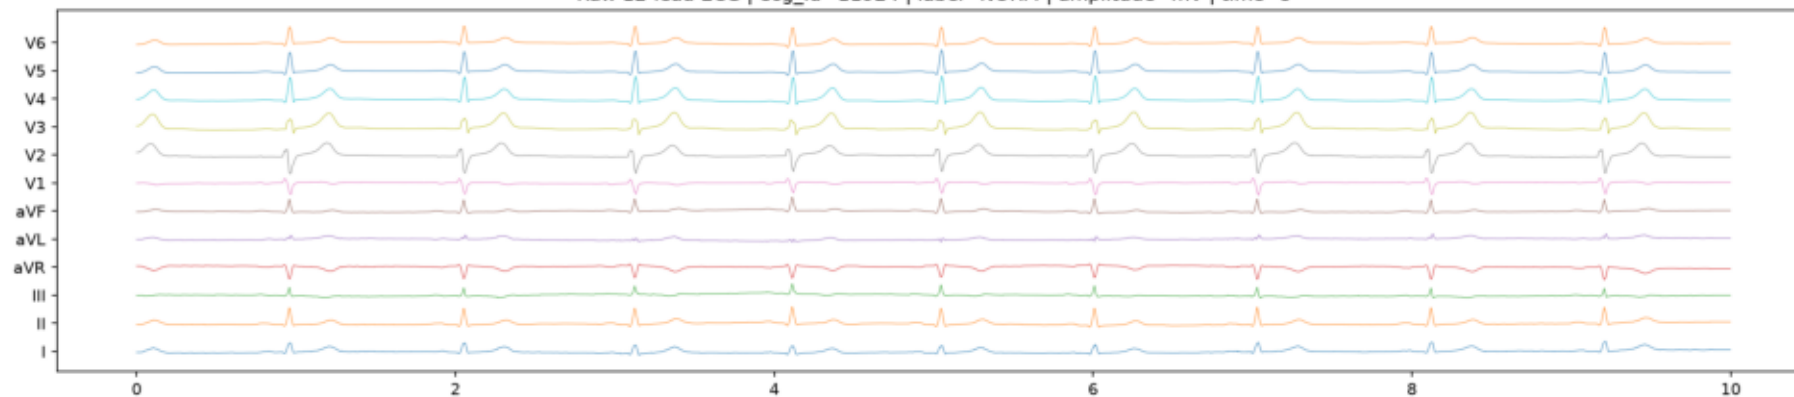


Detection bandpass composite and R candidates | peaks=16 | failure=rr_out_of_range

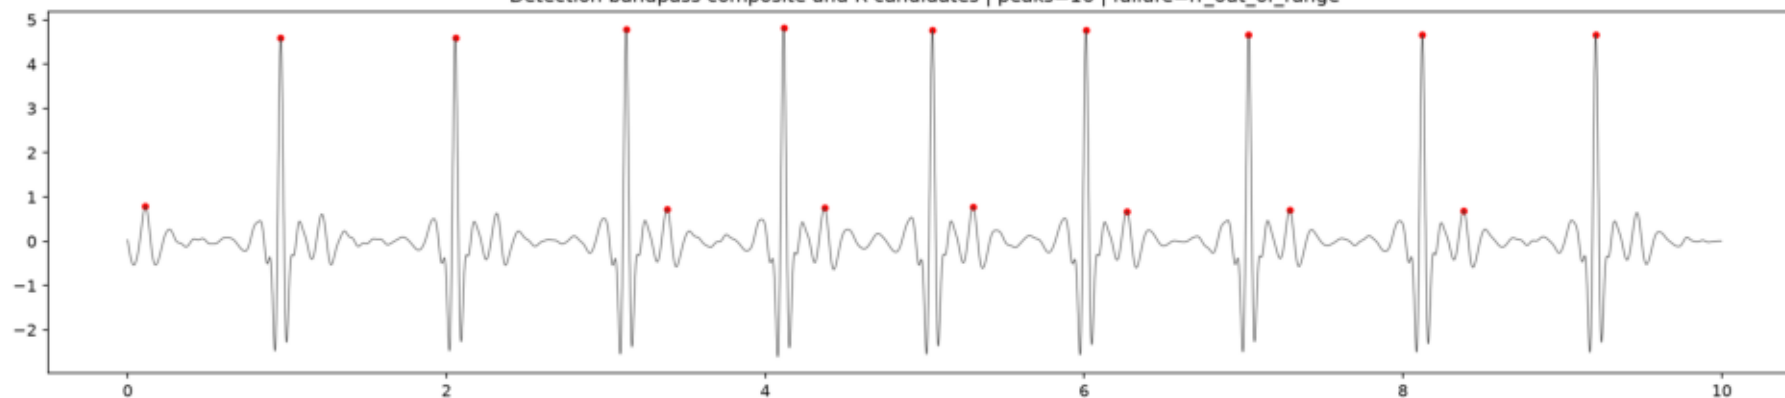

V5 segmentation boundaries | valid_beats=0 | units=mV,s

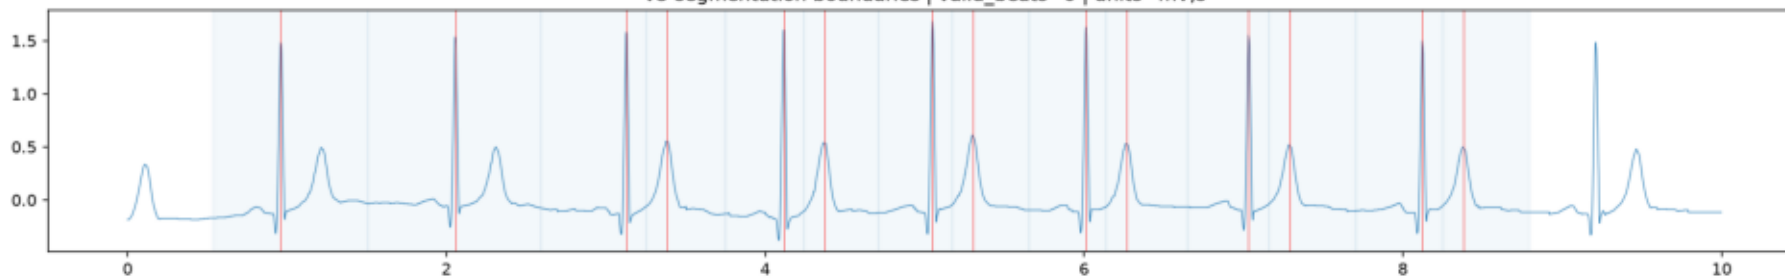


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

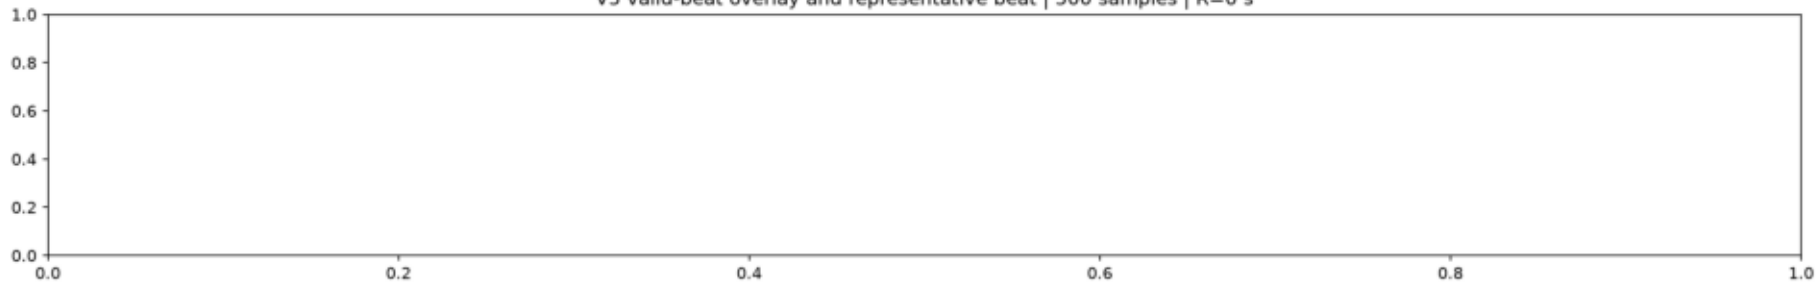


ECG 12118_NORM


Raw 12-lead ECG | ecg_id=12118 | label=NORM | amplitude=mV | time=s

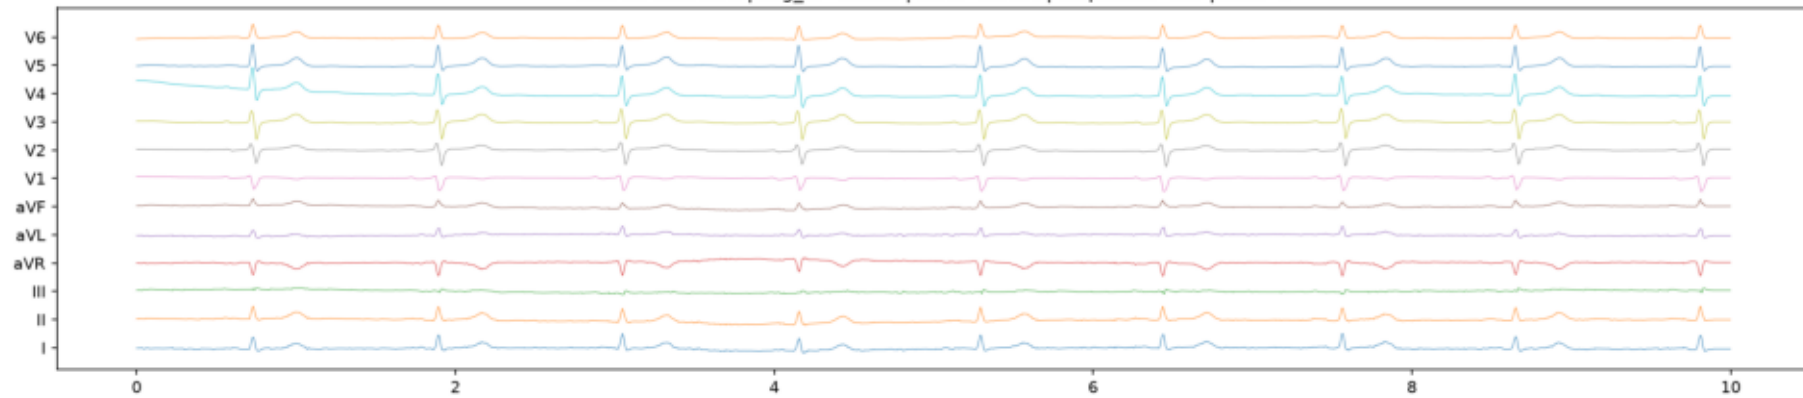


Detection bandpass composite and R candidates | peaks=17 | failure=rr_out_of_range

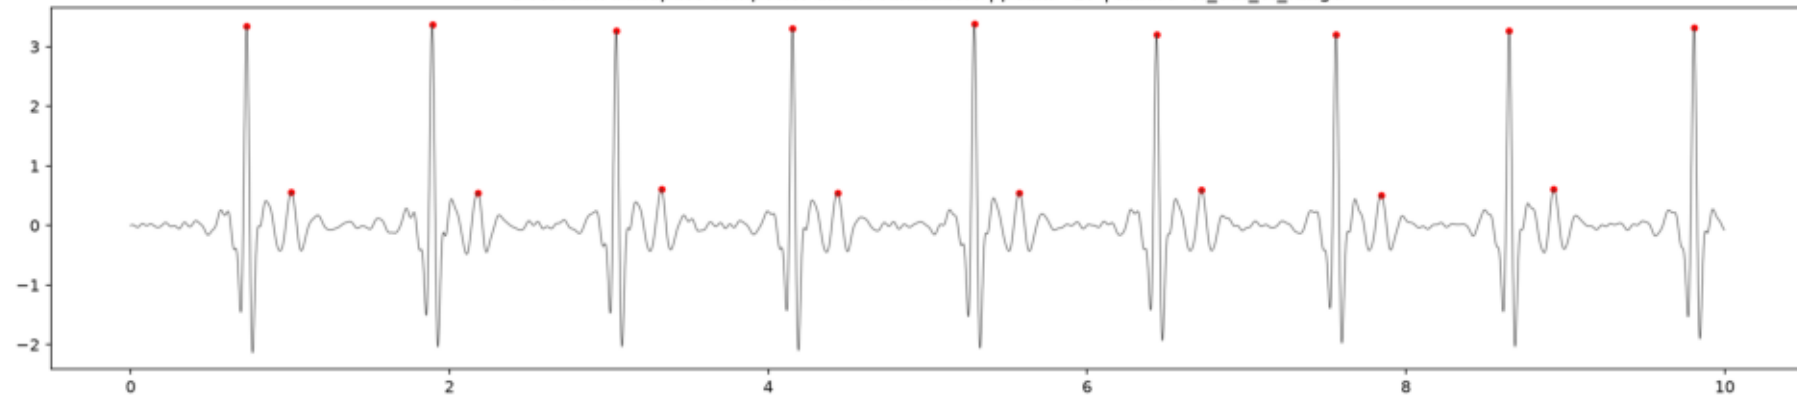

V5 segmentation boundaries | valid_beats=0 | units=mV,s

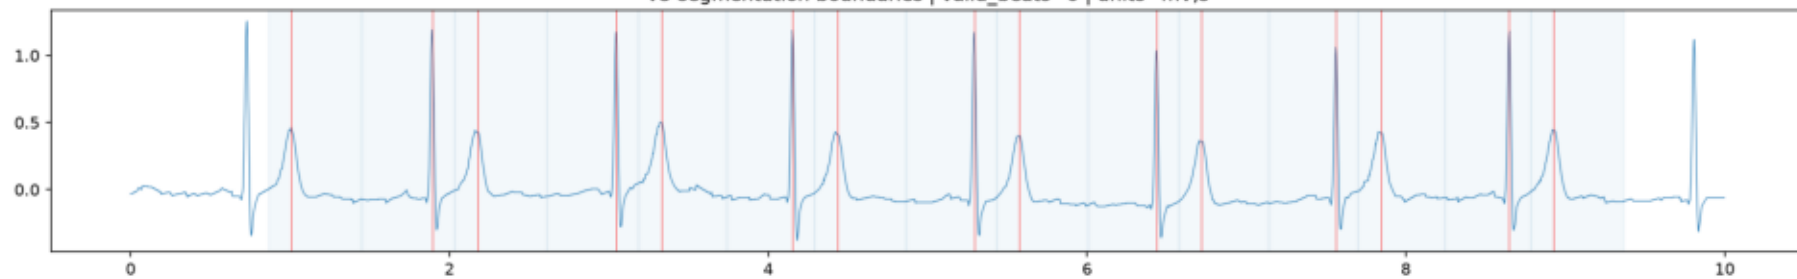


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

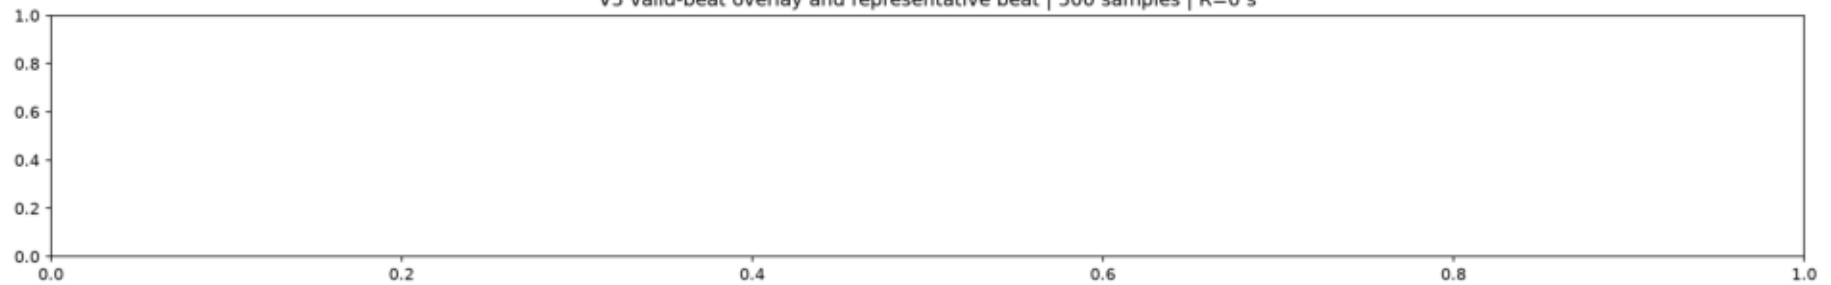


ECG 1385_LVH


Raw 12-lead ECG | ecg_id=1385 | label=LVH | amplitude=mV | time=s

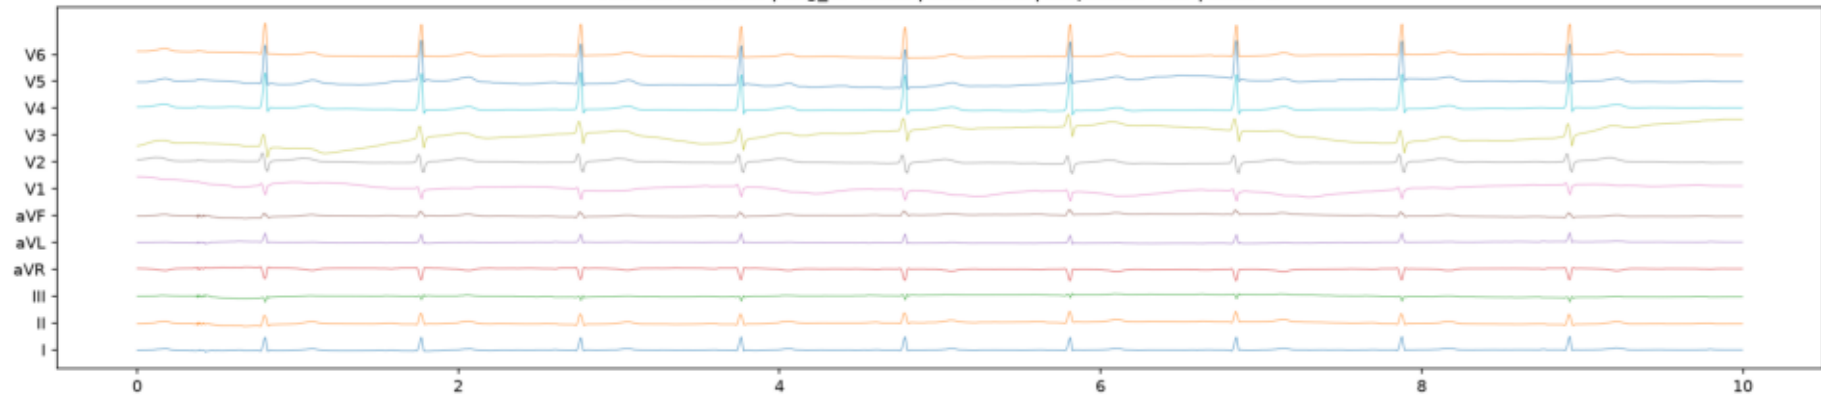


Detection bandpass composite and R candidates | peaks=9 | failure=nan

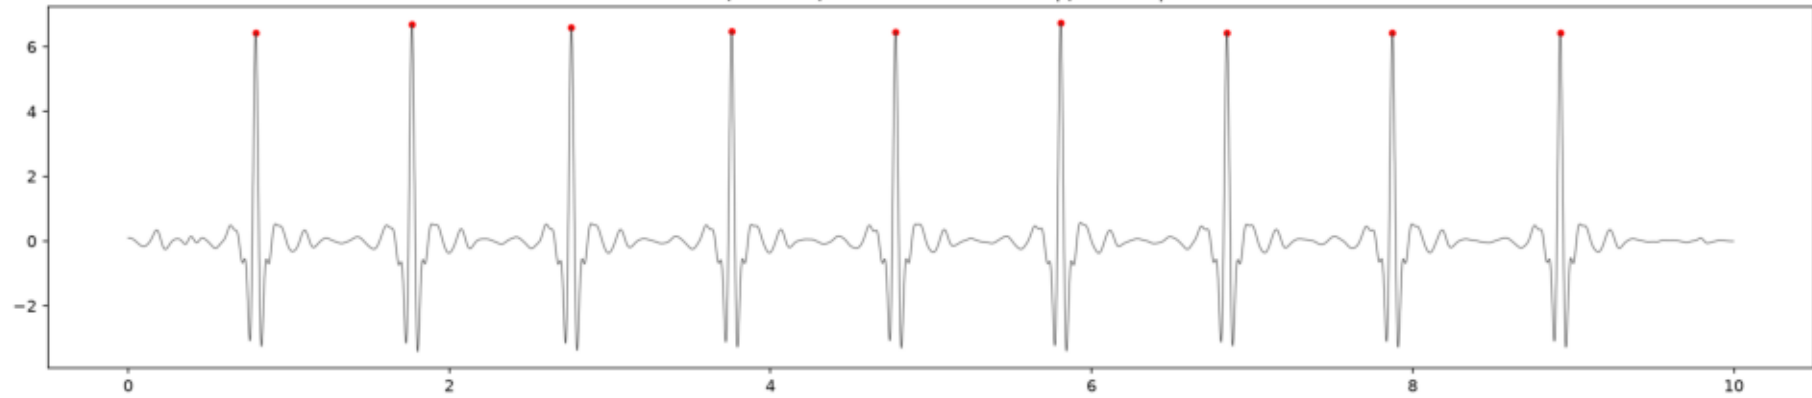

V5 segmentation boundaries | valid_beats=7 | units=mV,s

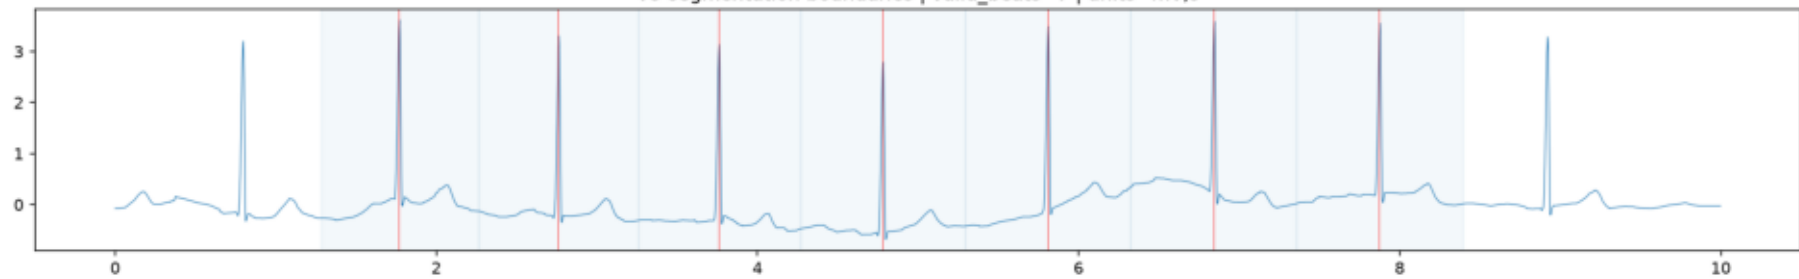


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

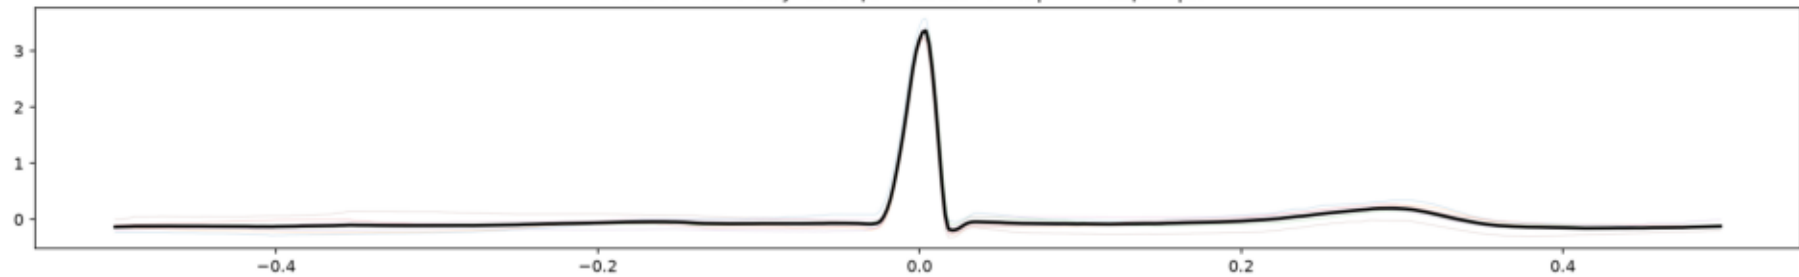


ECG 13919_LVH


Raw 12-lead ECG | ecg_id=13919 | label=LVH | amplitude=mV | time=s

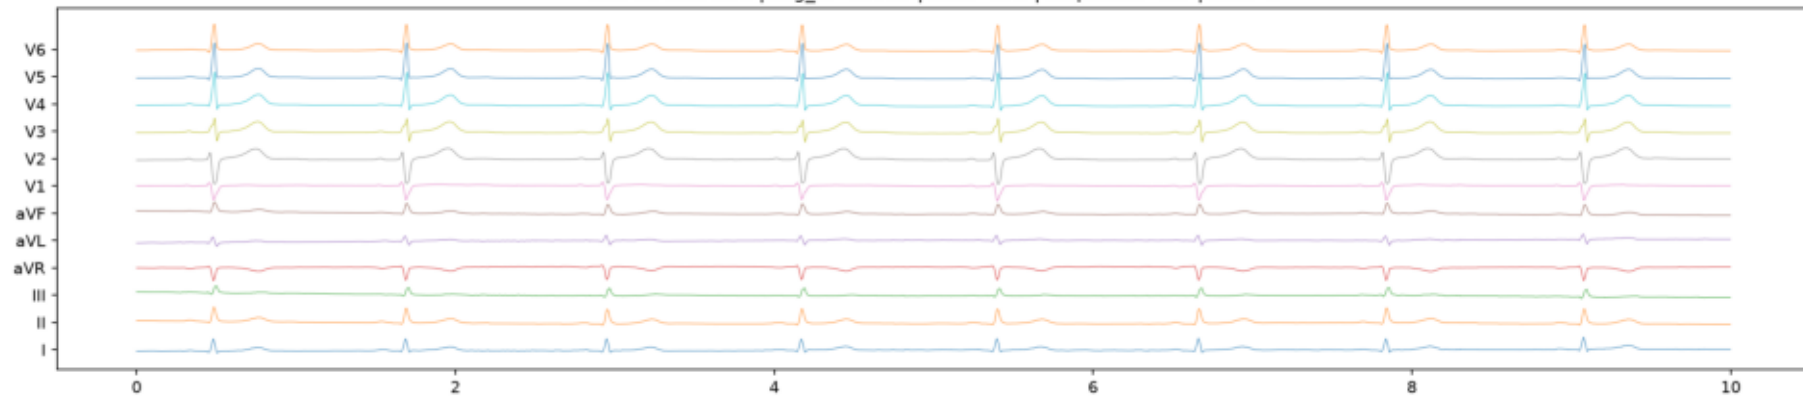


Detection bandpass composite and R candidates | peaks=16 | failure=rr_out_of_range

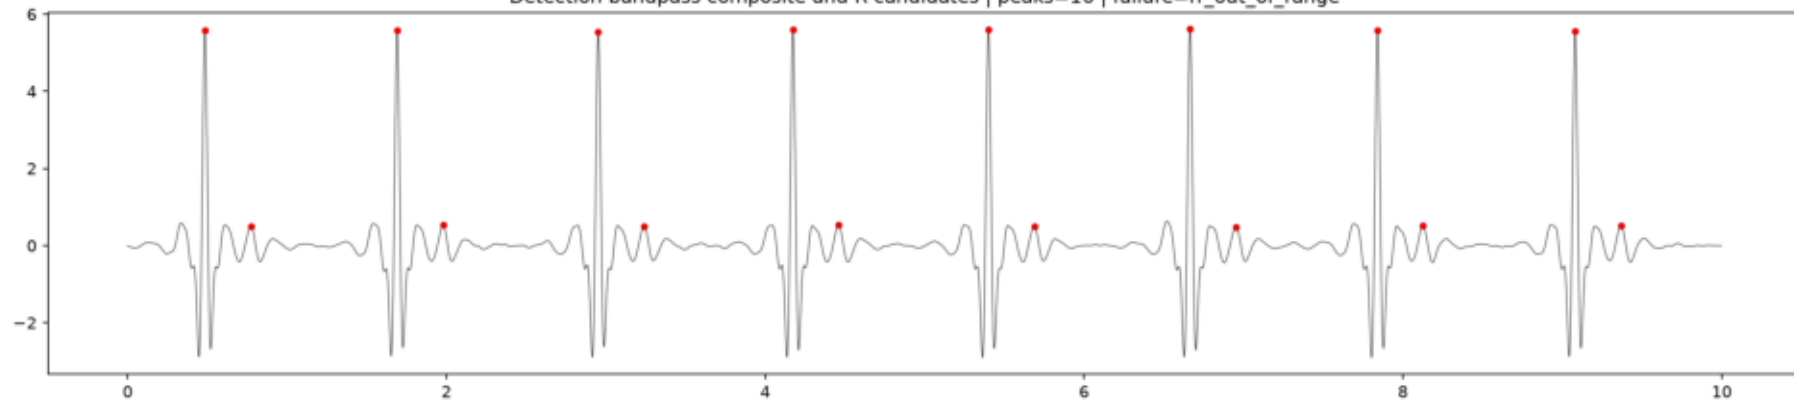

V5 segmentation boundaries | valid_beats=0 | units=mV,s

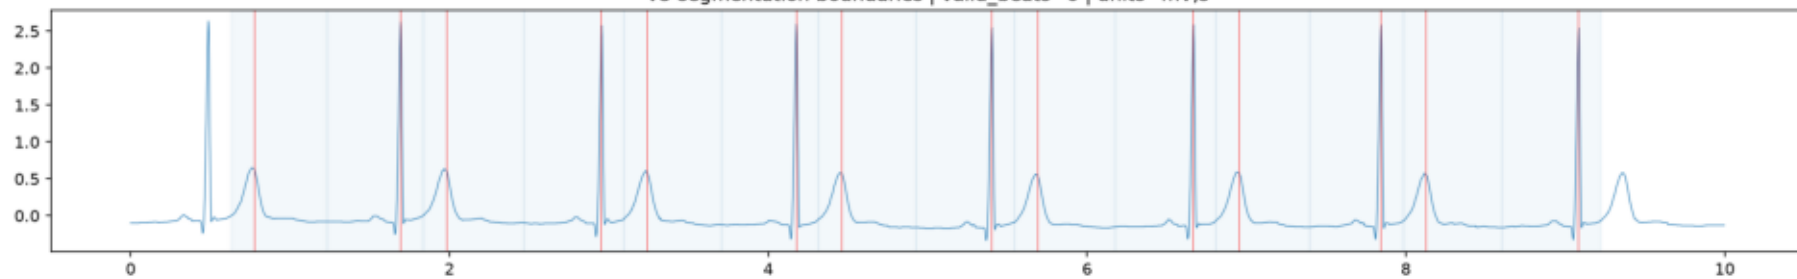


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

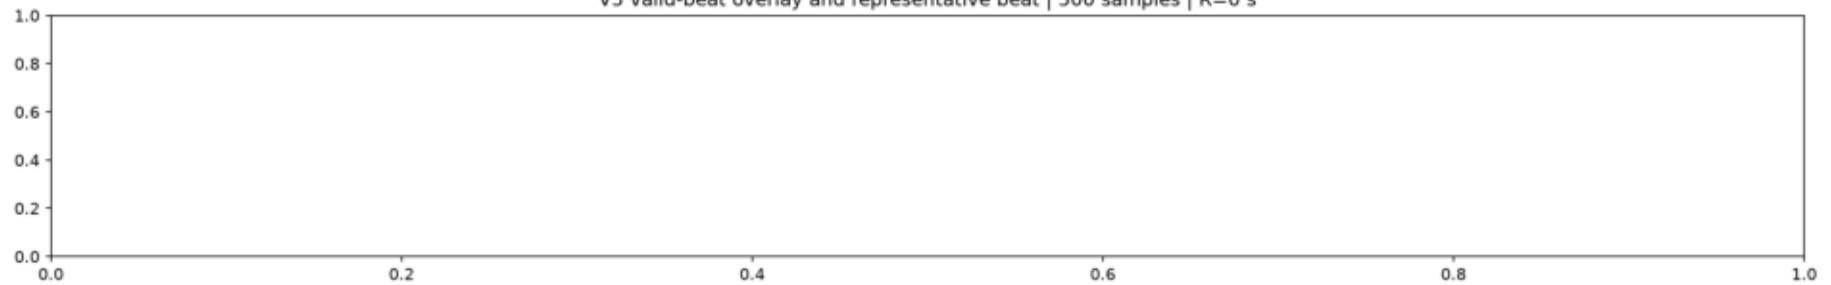


ECG 18147_LVH


Raw 12-lead ECG | ecg_id=18147 | label=LVH | amplitude=mV | time=s

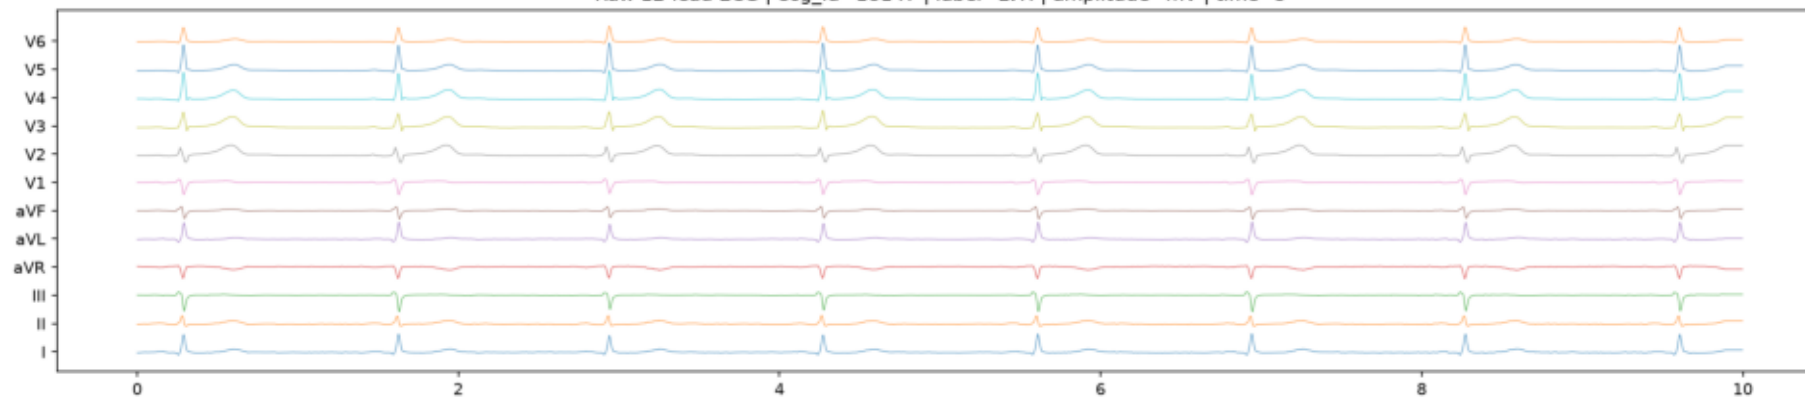


Detection bandpass composite and R candidates | peaks=8 | failure=nan

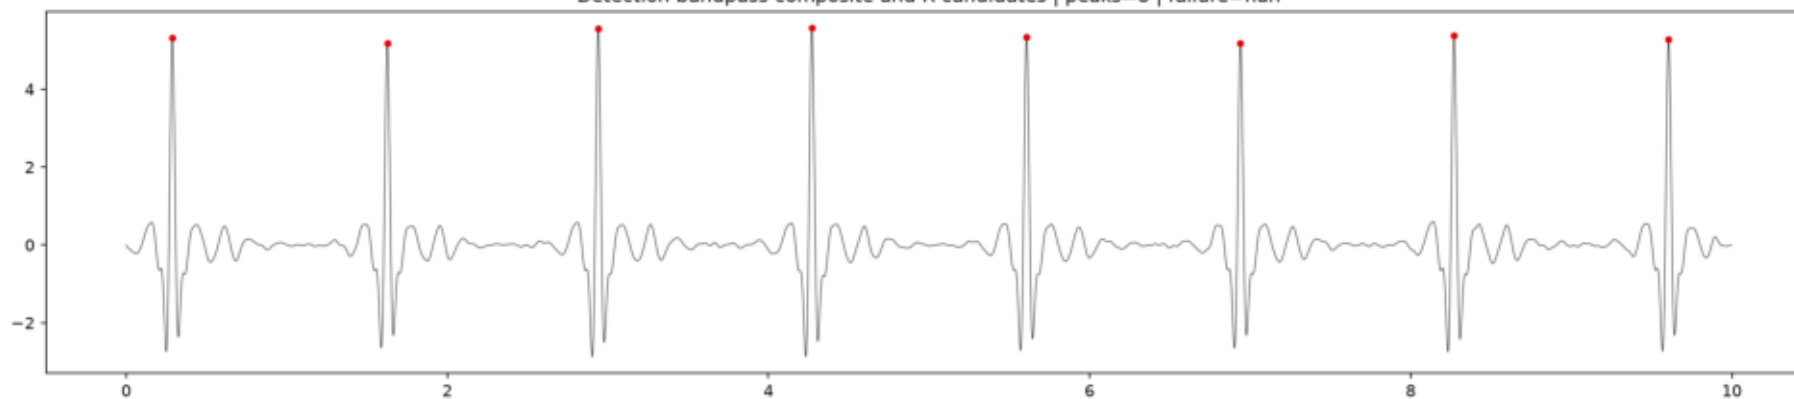

V5 segmentation boundaries | valid_beats=6 | units=mV,s

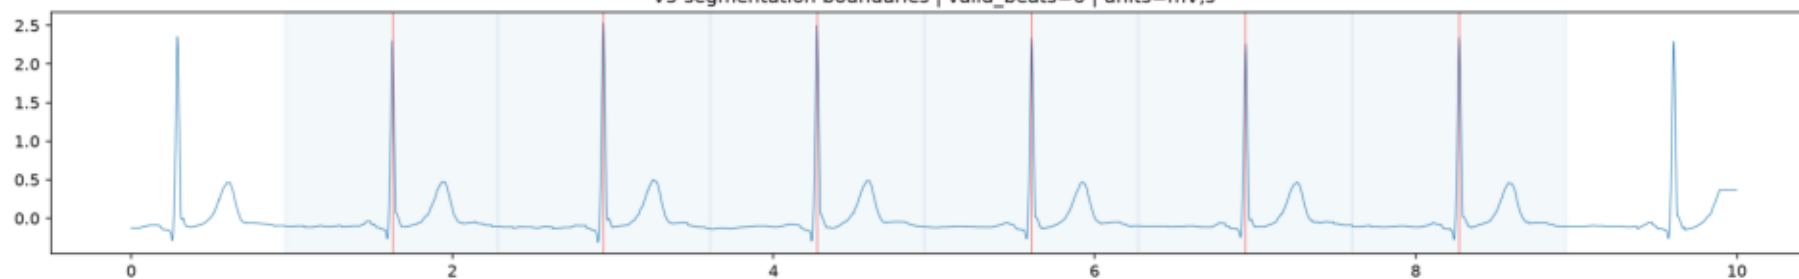


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

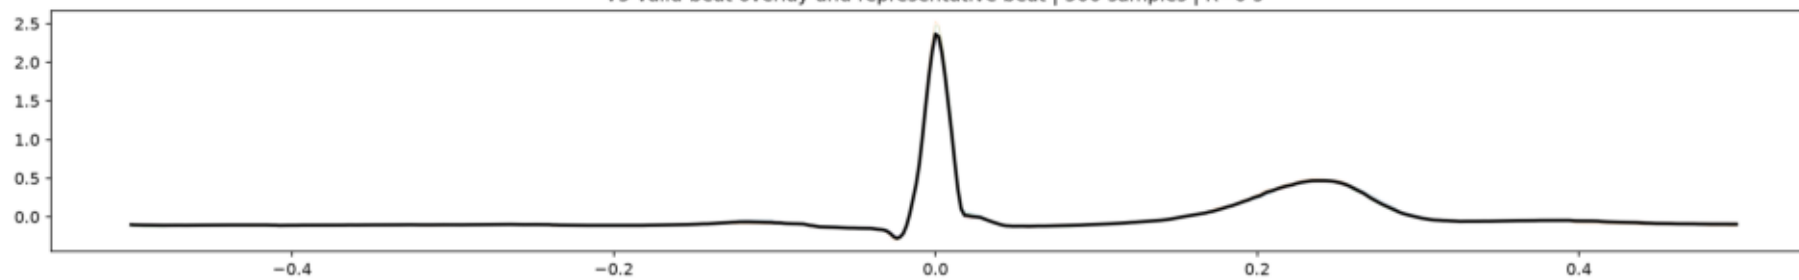


ECG 18572_NORM


Raw 12-lead ECG | ecg_id=18572 | label=NORM | amplitude=mV | time=s

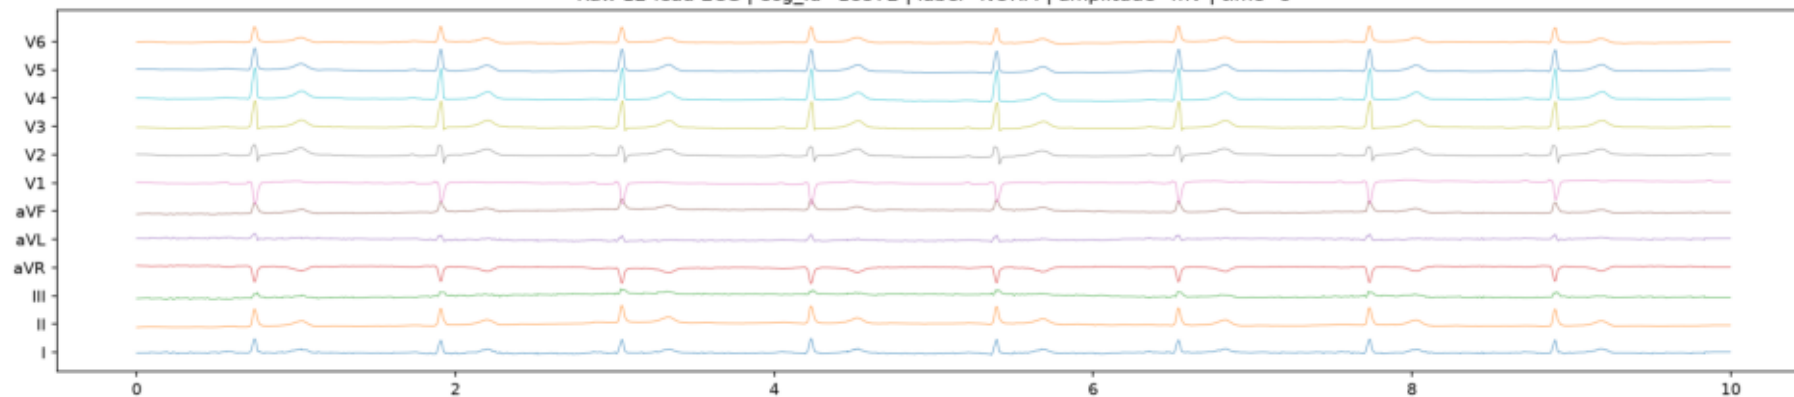


Detection bandpass composite and R candidates | peaks=16 | failure=rr_out_of_range

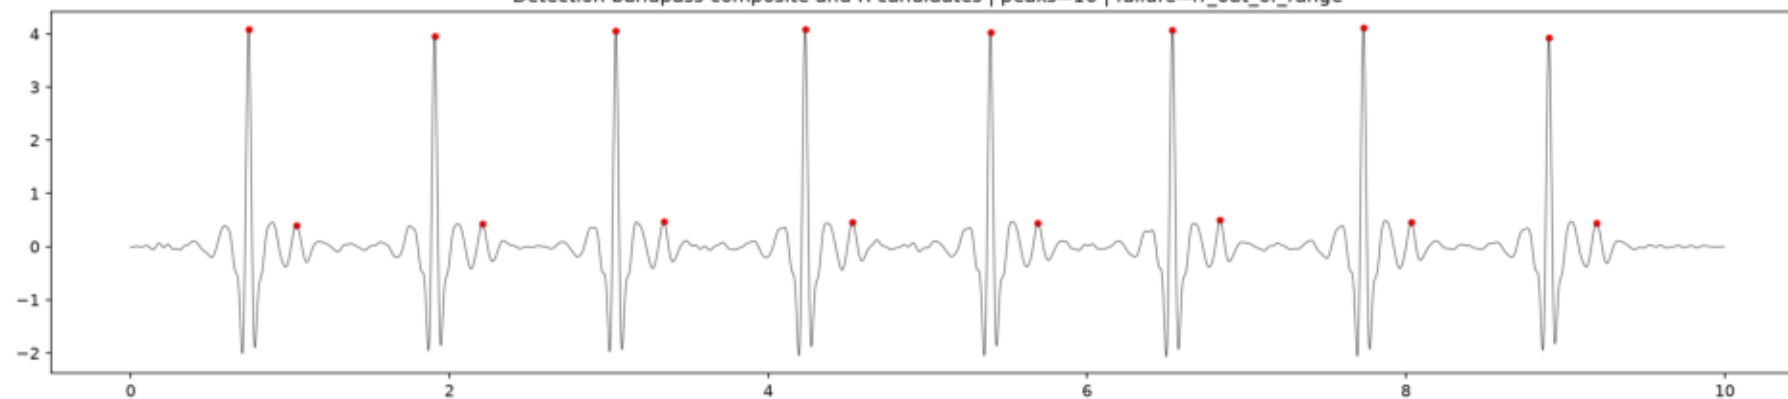

V5 segmentation boundaries | valid_beats=0 | units=mV,s

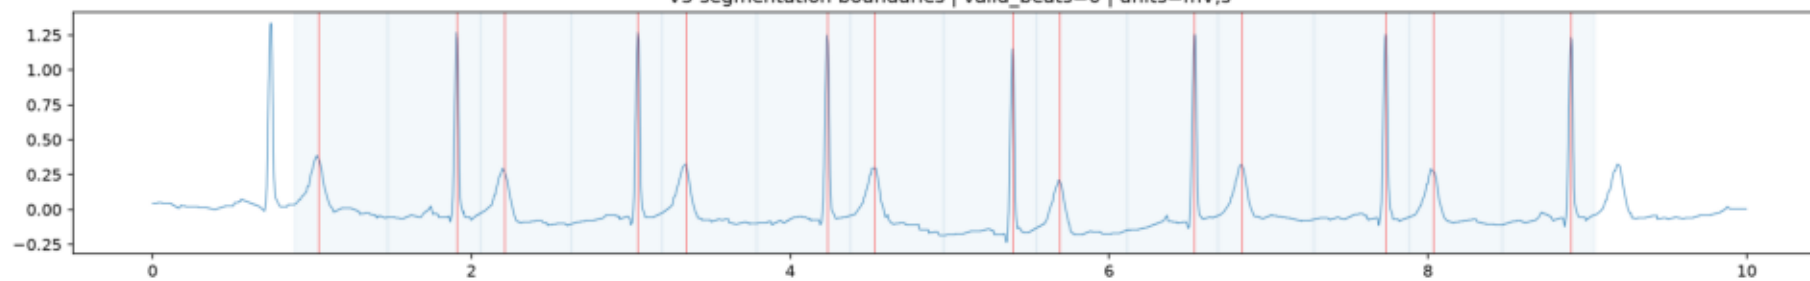


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

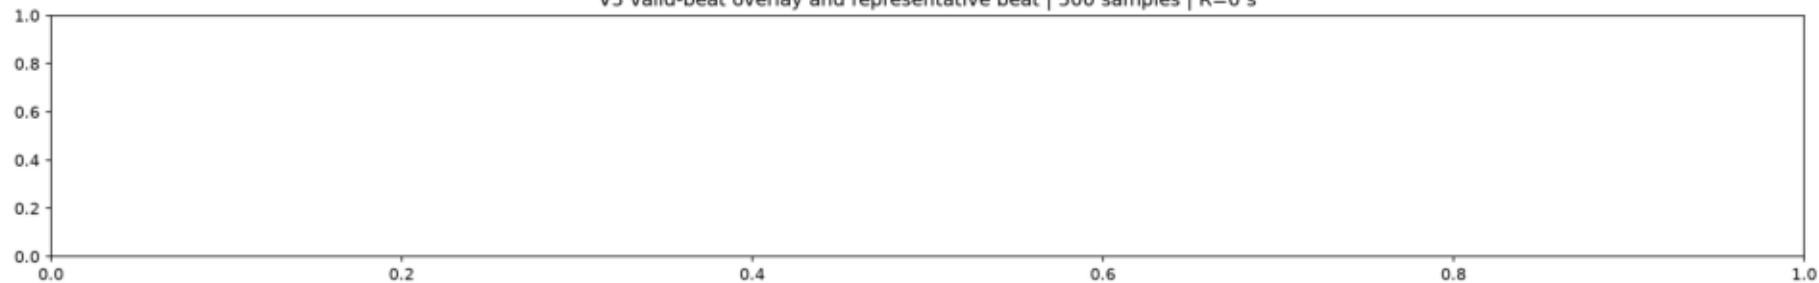


ECG 19122_NORM


Raw 12-lead ECG | ecg_id=19122 | label=NORM | amplitude=mV | time=s

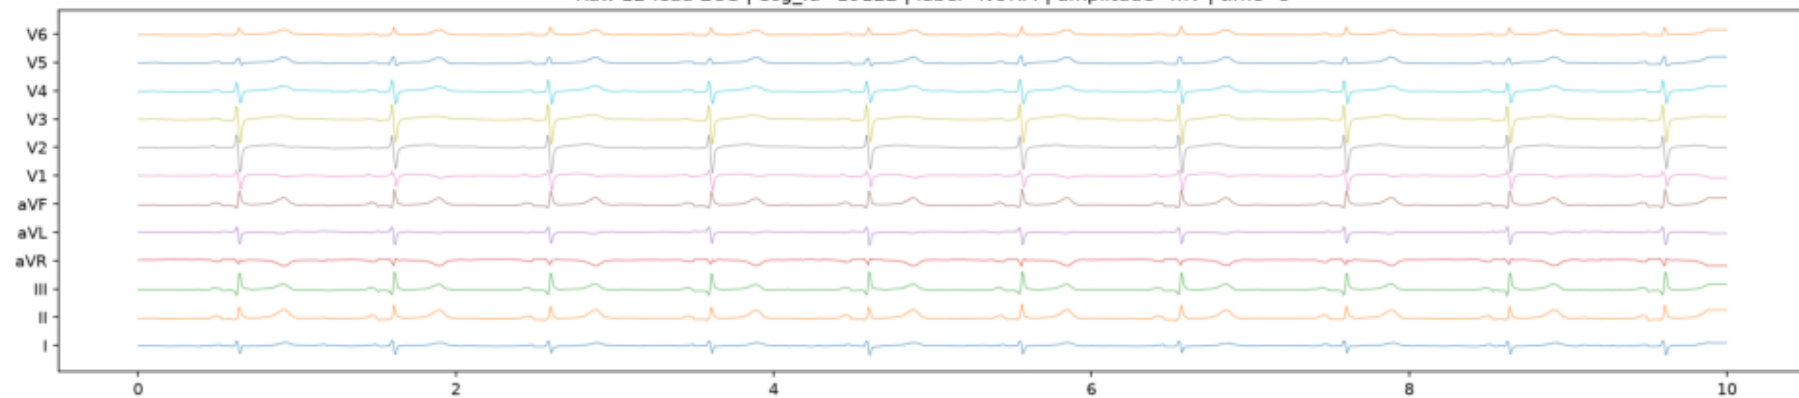


Detection bandpass composite and R candidates | peaks=19 | failure=rr_out_of_range

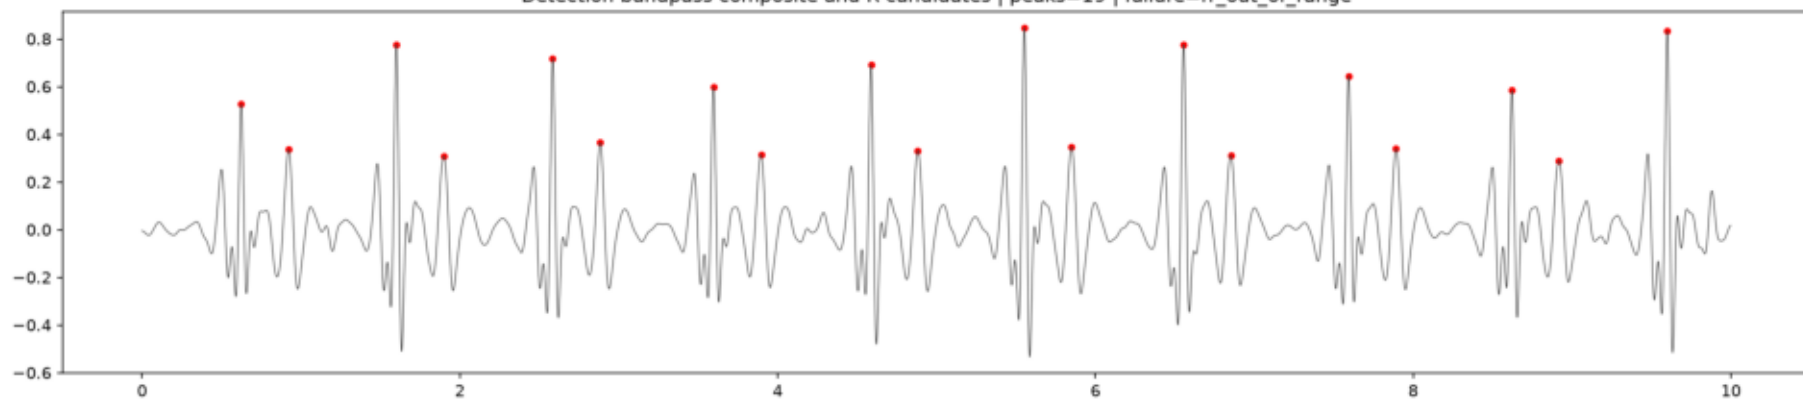

V5 segmentation boundaries | valid_beats=0 | units=mV,s

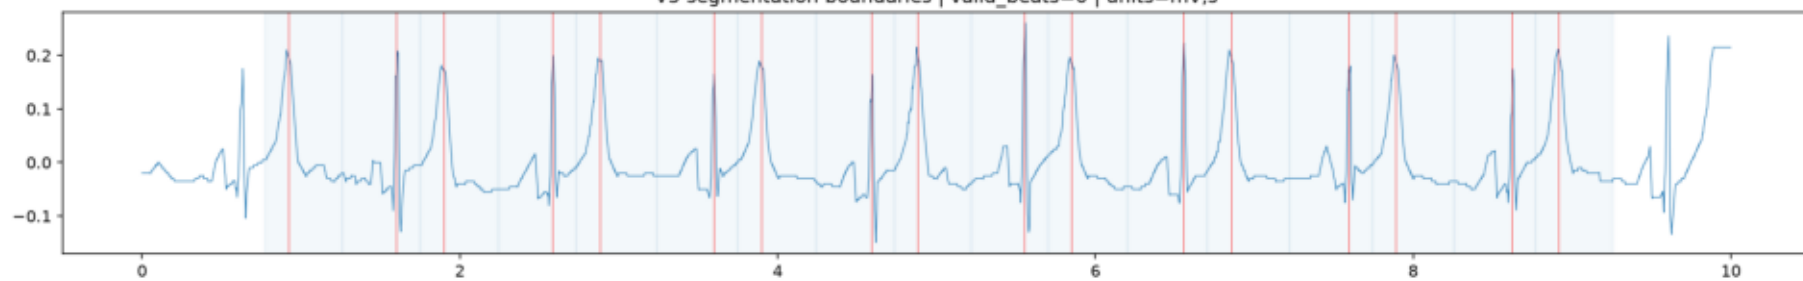


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

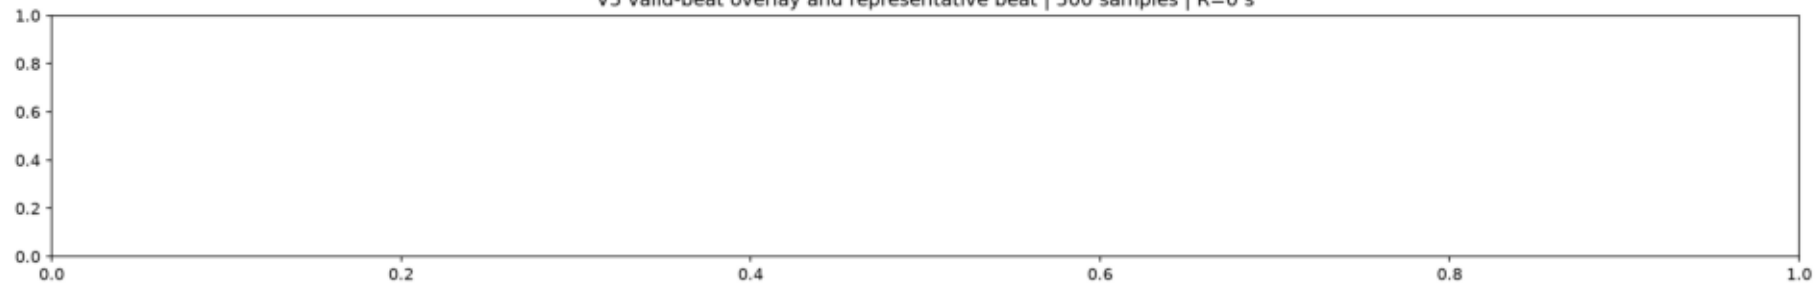


ECG 19635_LVH


Raw 12-lead ECG | ecg_id=19635 | label=LVH | amplitude=mV | time=s

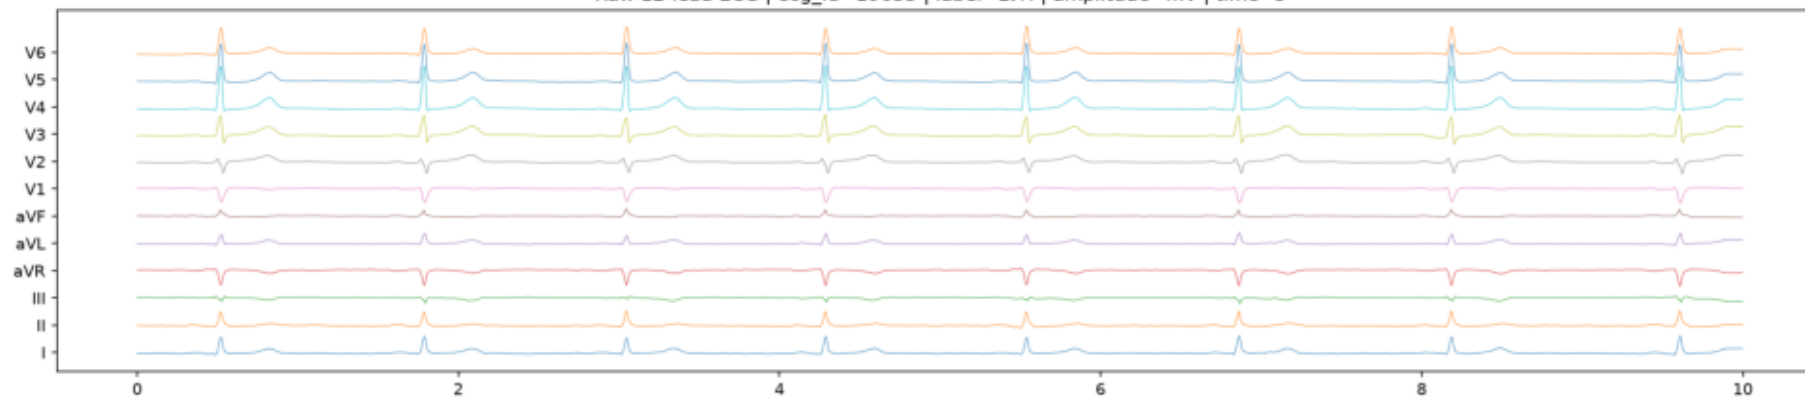


Detection bandpass composite and R candidates | peaks=8 | failure=nan

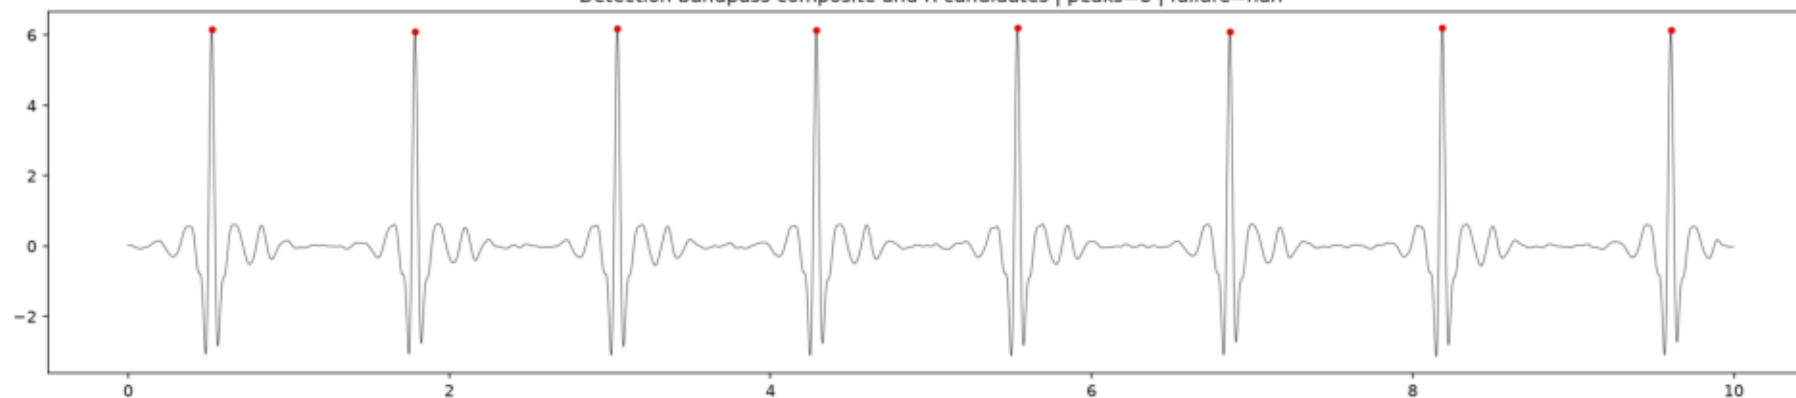

V5 segmentation boundaries | valid_beats=6 | units=mV,s

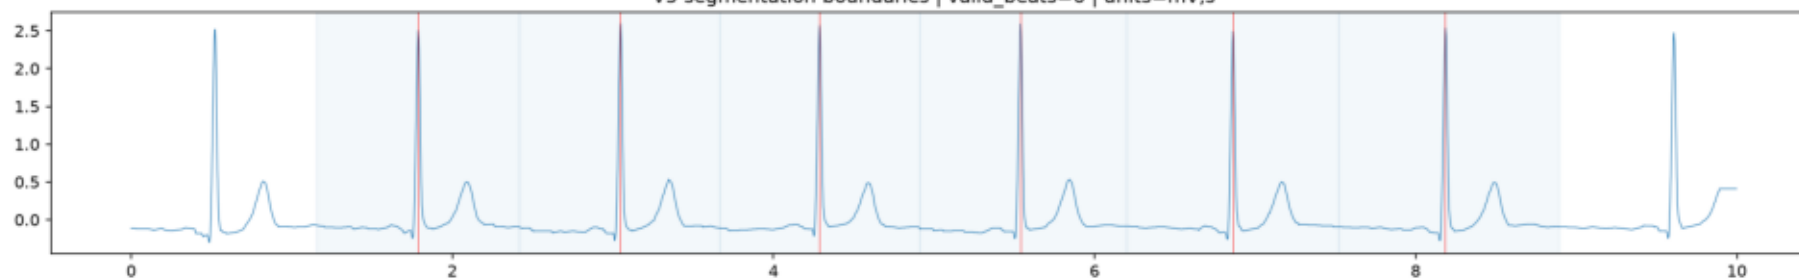


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

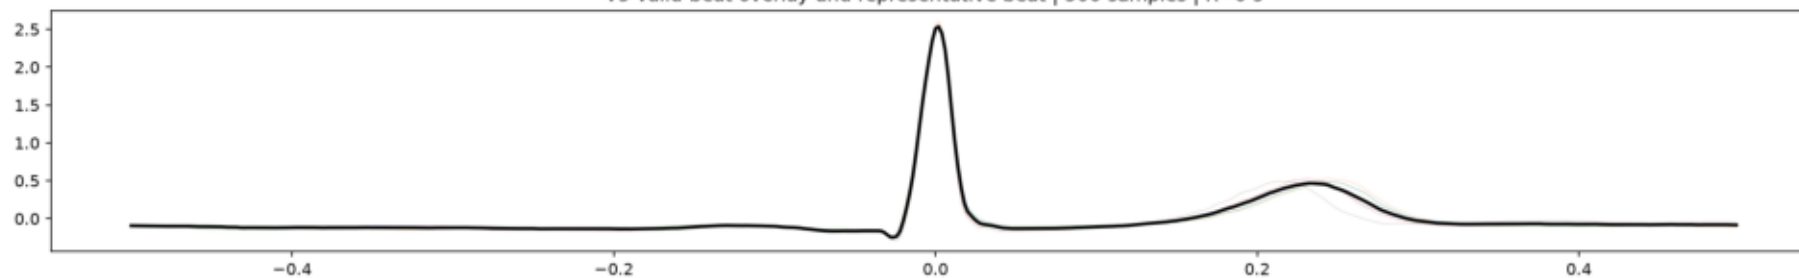


ECG 19708_NORM


Raw 12-lead ECG | ecg_id=19708 | label=NORM | amplitude=mV | time=s

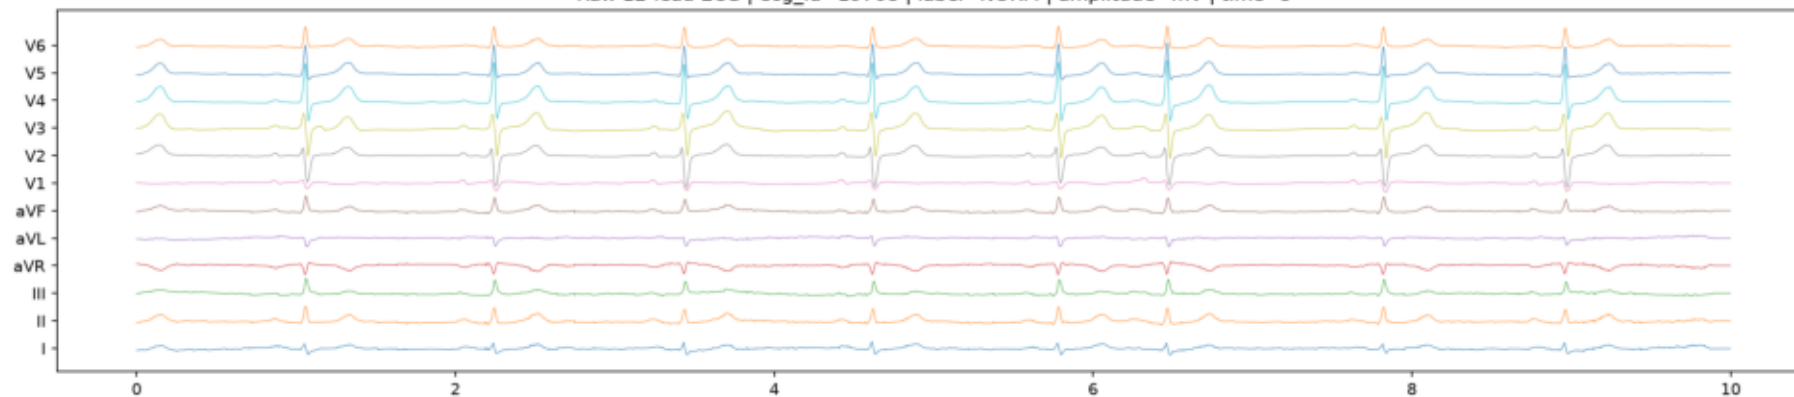


Detection bandpass composite and R candidates | peaks=17 | failure=rr_out_of_range

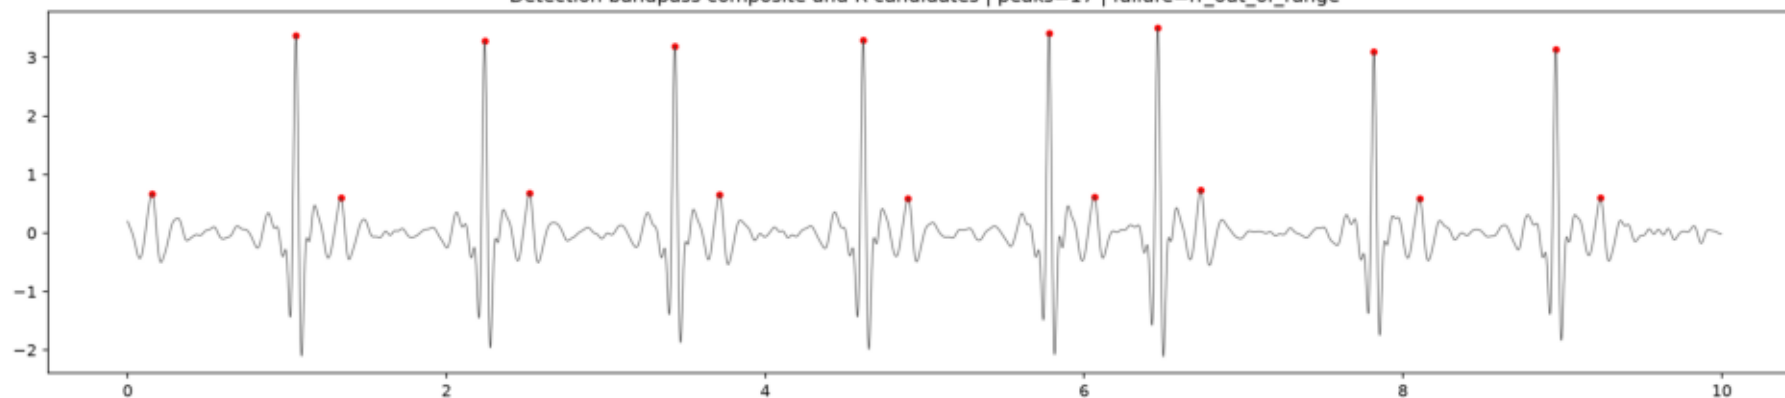

V5 segmentation boundaries | valid_beats=0 | units=mV,s

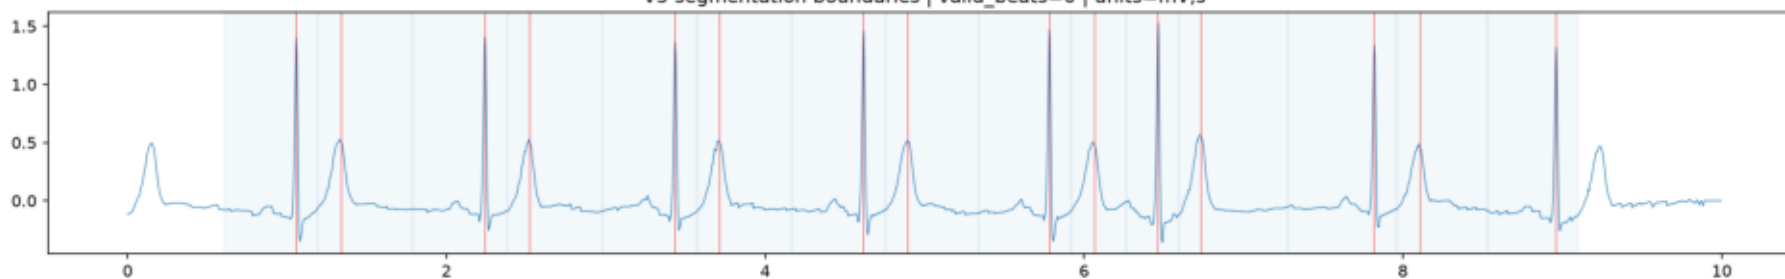


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

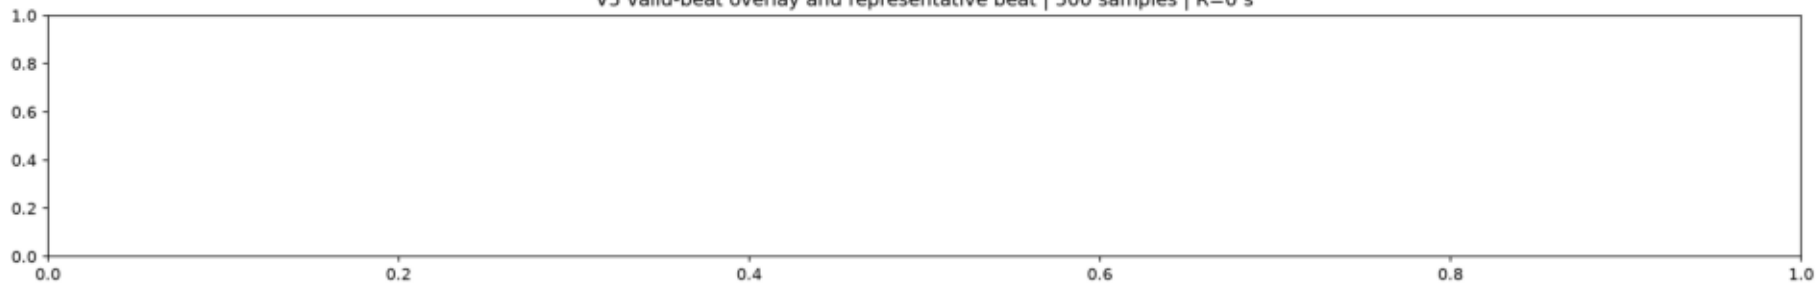


ECG 2762_LVH


Raw 12-lead ECG | ecg_id=2762 | label=LVH | amplitude=mV | time=s

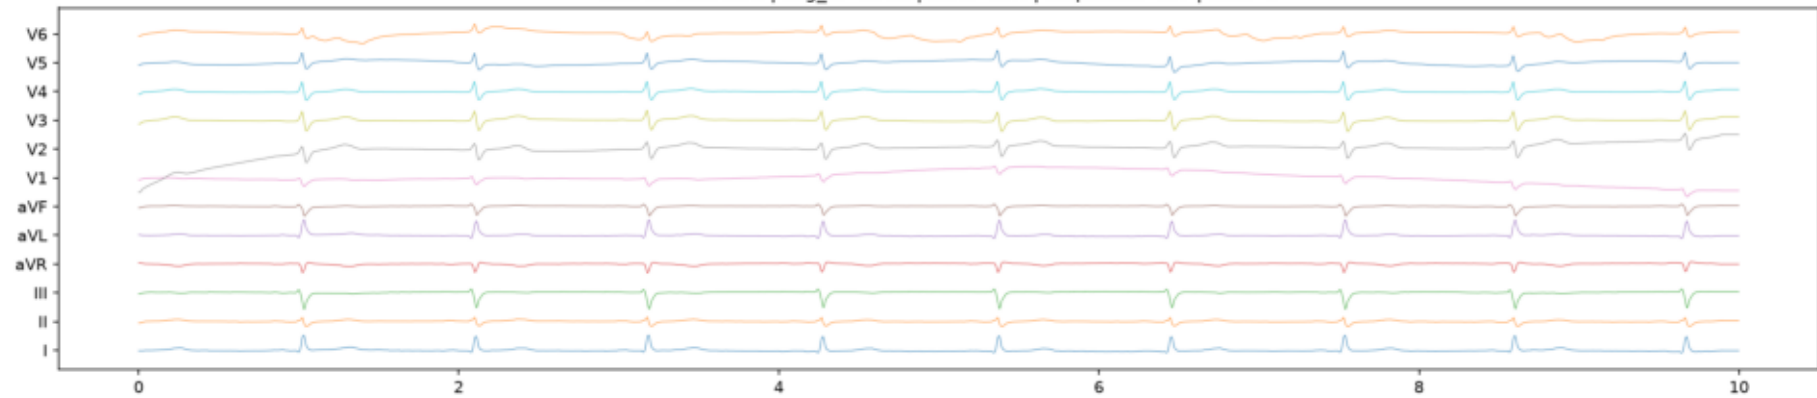


Detection bandpass composite and R candidates | peaks=11 | failure=nan

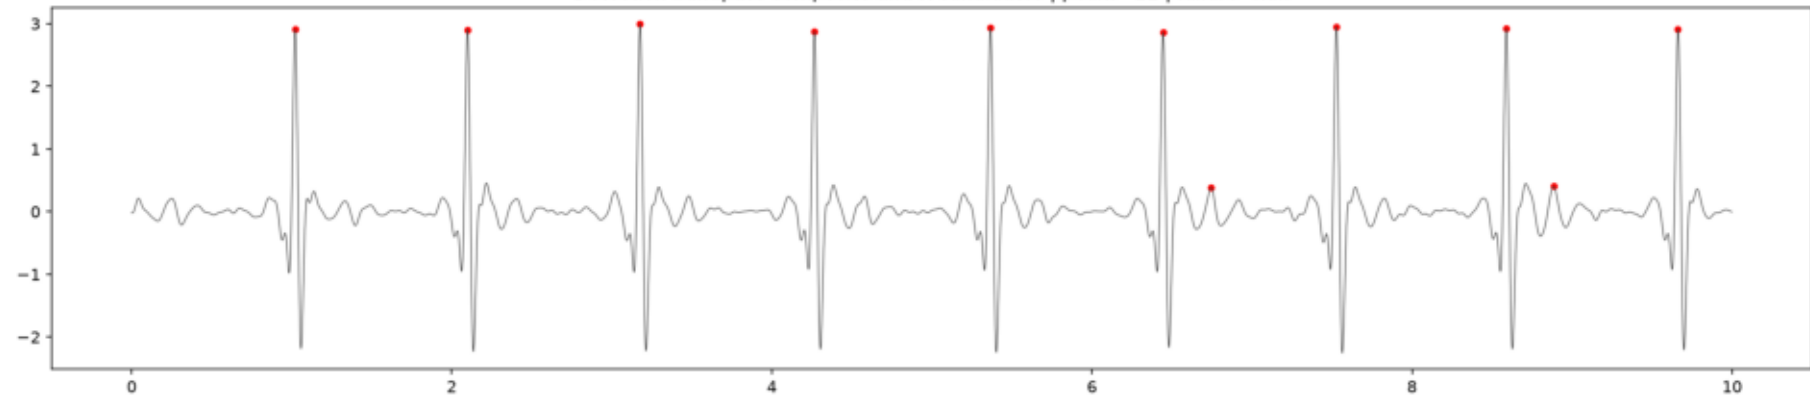

V5 segmentation boundaries | valid_beats=7 | units=mV,s

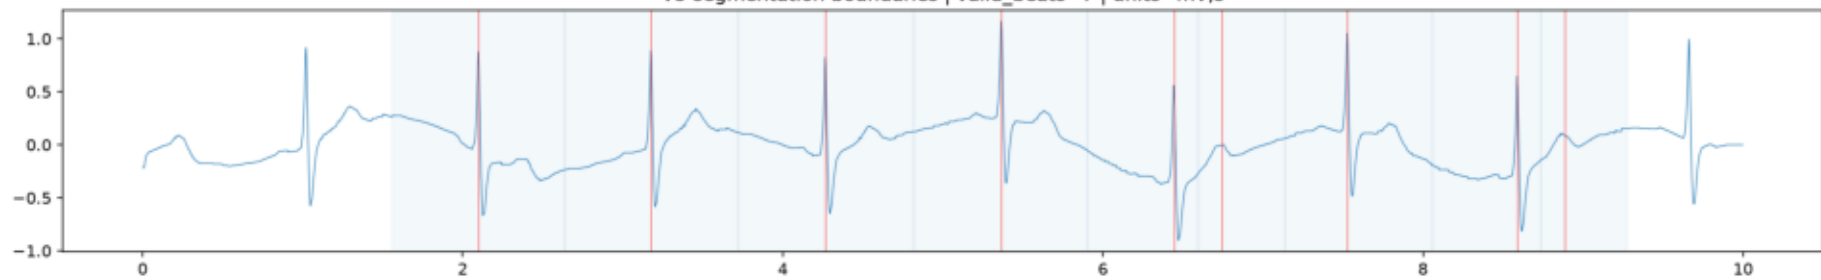


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

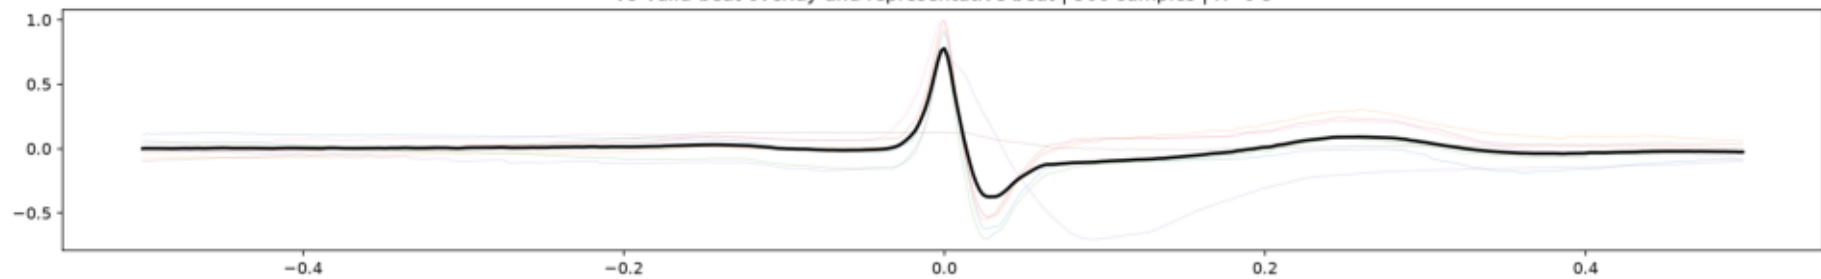


ECG 2858_LVH


Raw 12-lead ECG | ecg_id=2858 | label=LVH | amplitude=mV | time=s

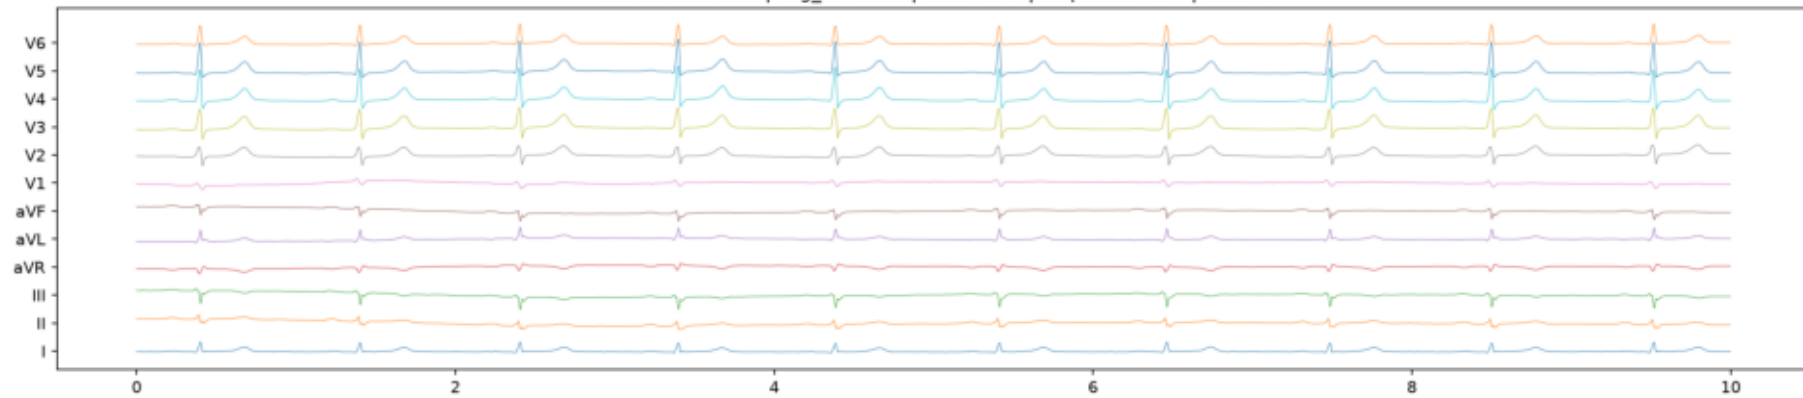


Detection bandpass composite and R candidates | peaks=20 | failure=rr_out_of_range

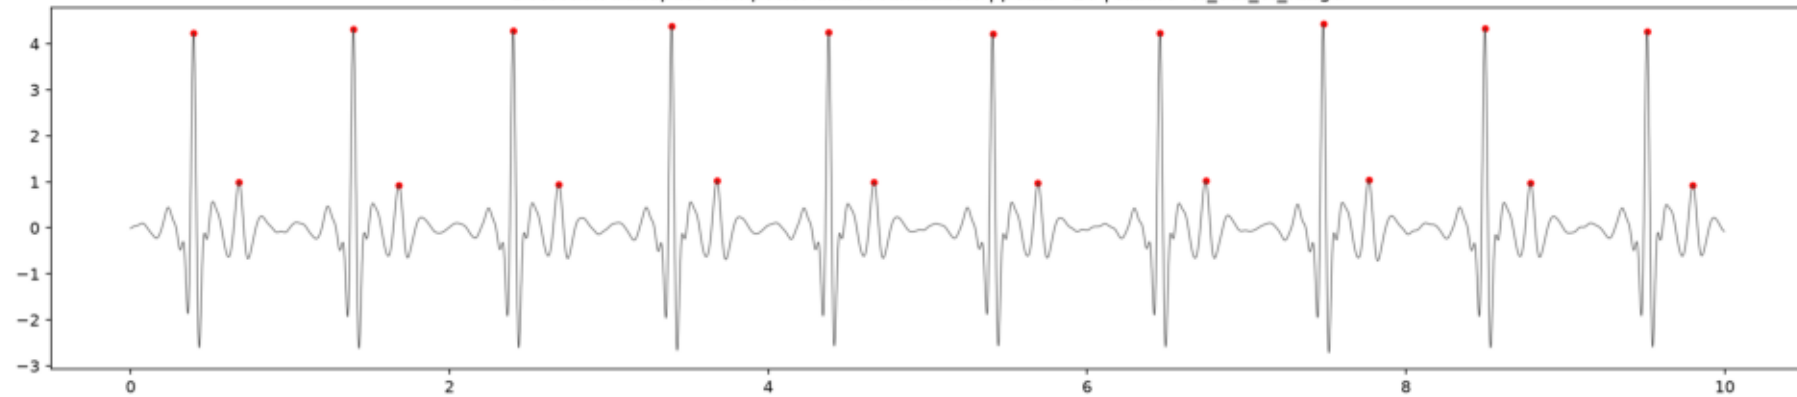

V5 segmentation boundaries | valid_beats=0 | units=mV,s

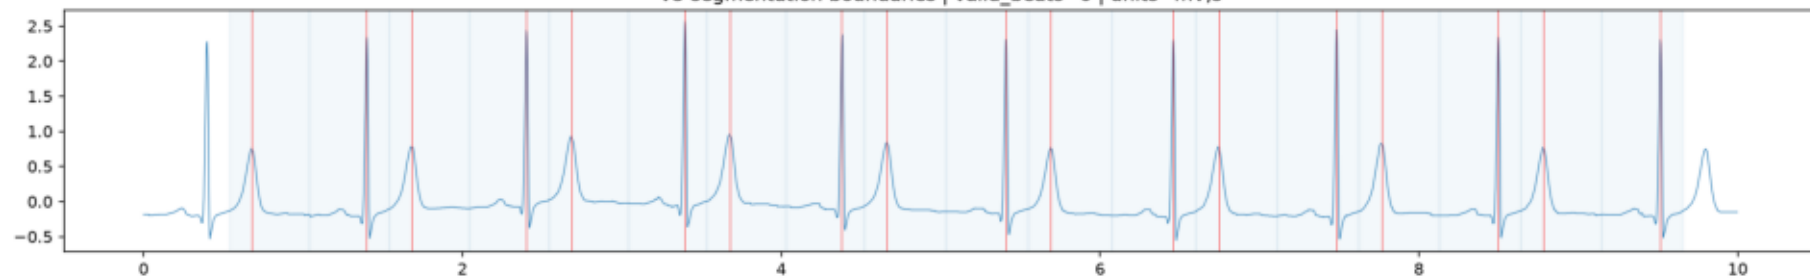


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

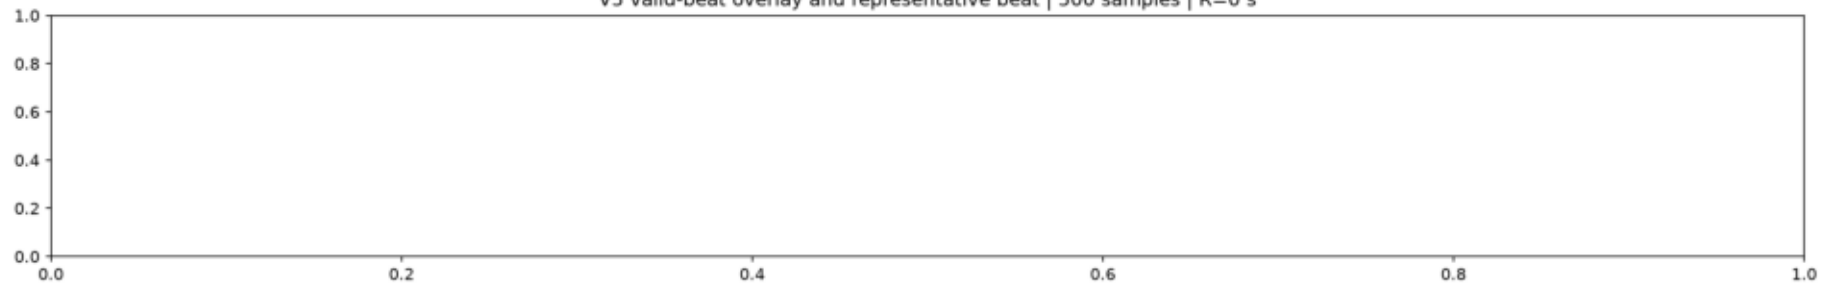


ECG 3316_LVH


Raw 12-lead ECG | ecg_id=3316 | label=LVH | amplitude=mV | time=s

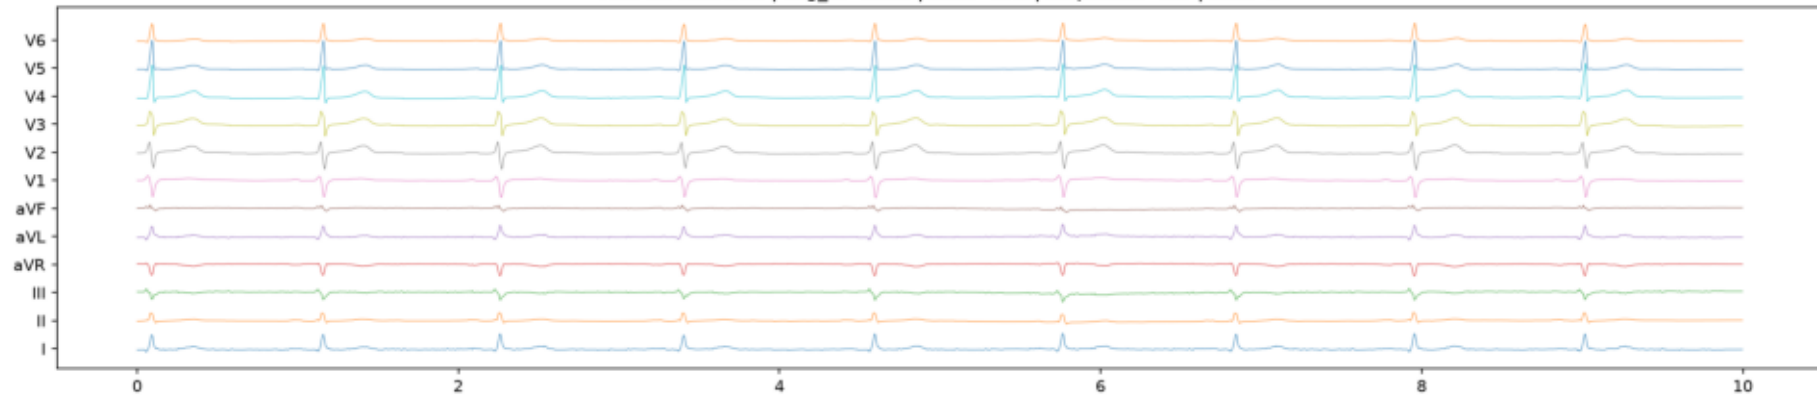


Detection bandpass composite and R candidates | peaks=9 | failure=nan

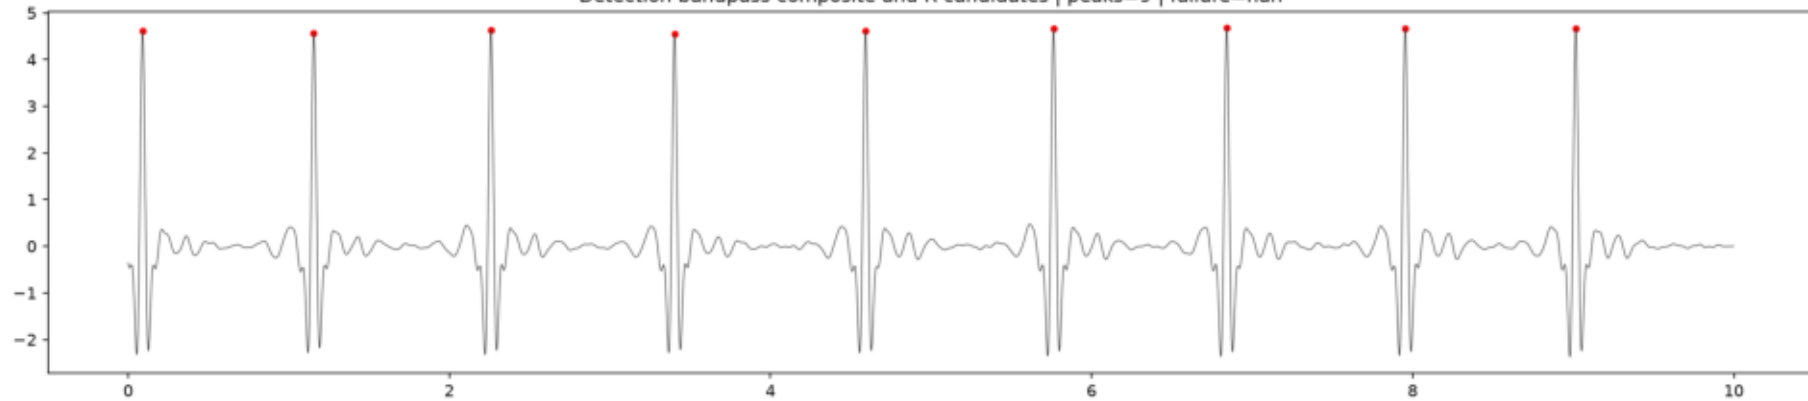

V5 segmentation boundaries | valid_beats=7 | units=mV,s

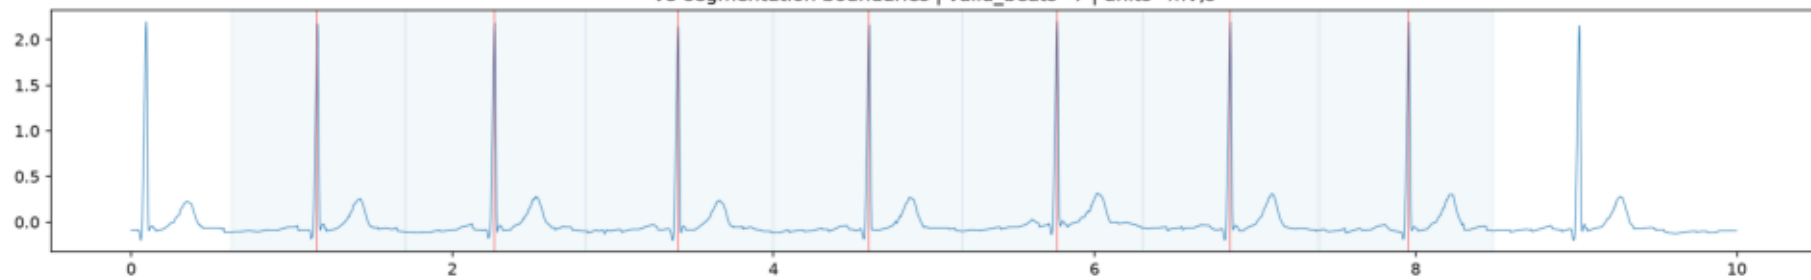


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

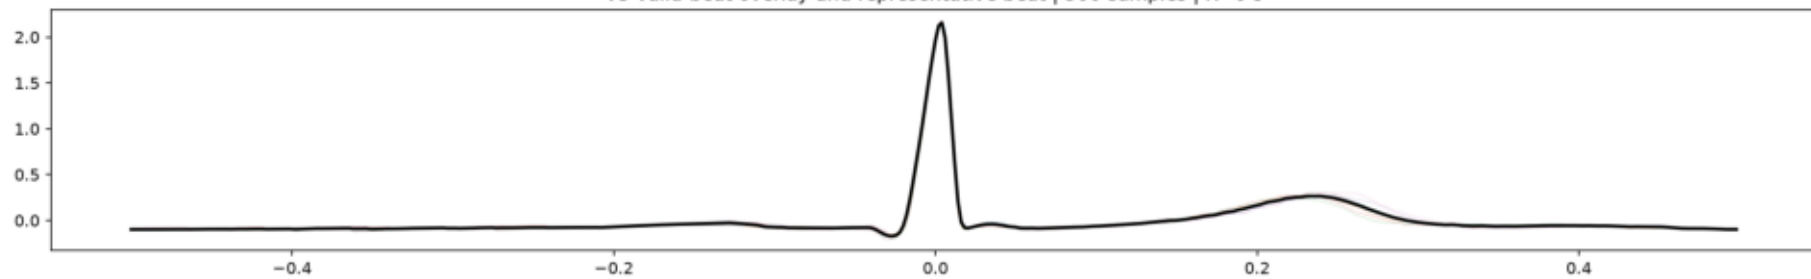


ECG 358_NORM


Raw 12-lead ECG | ecg_id=358 | label=NORM | amplitude=mV | time=s

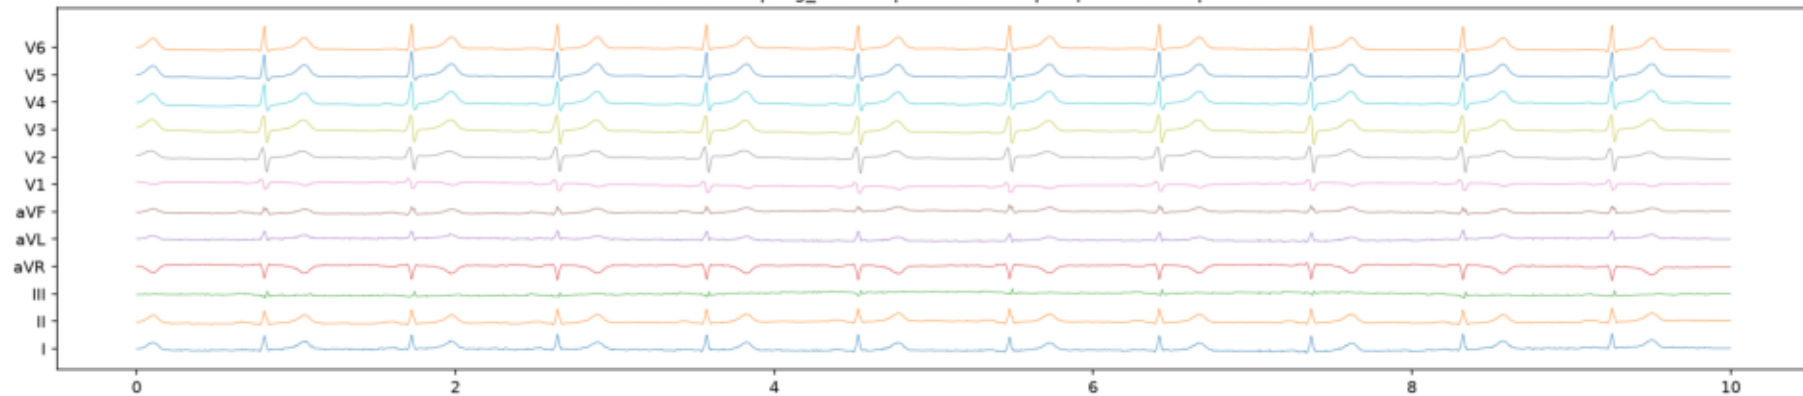


Detection bandpass composite and R candidates | peaks=21 | failure=rr_out_of_range

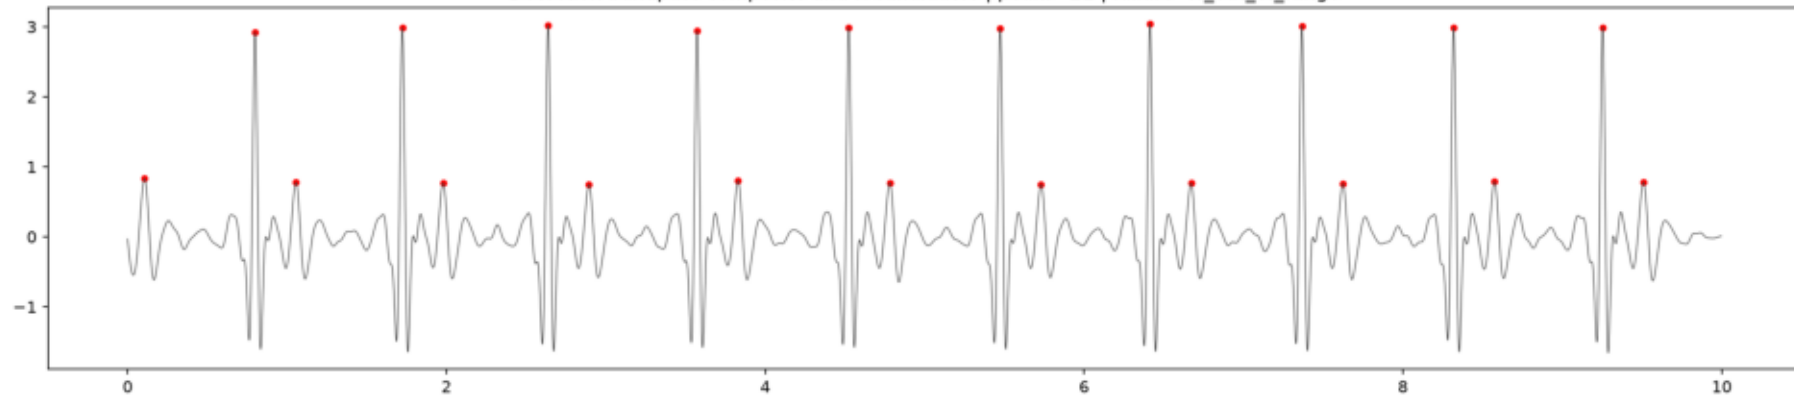

V5 segmentation boundaries | valid_beats=0 | units=mV,s

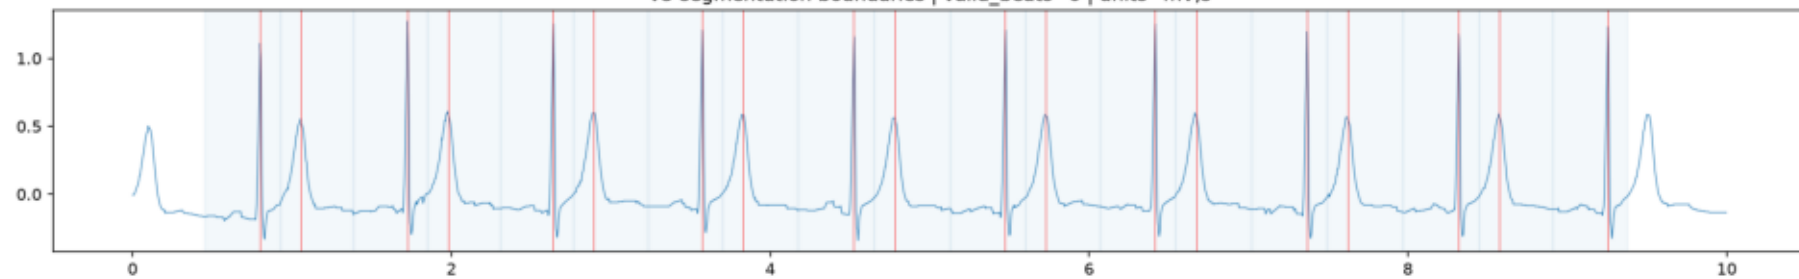


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

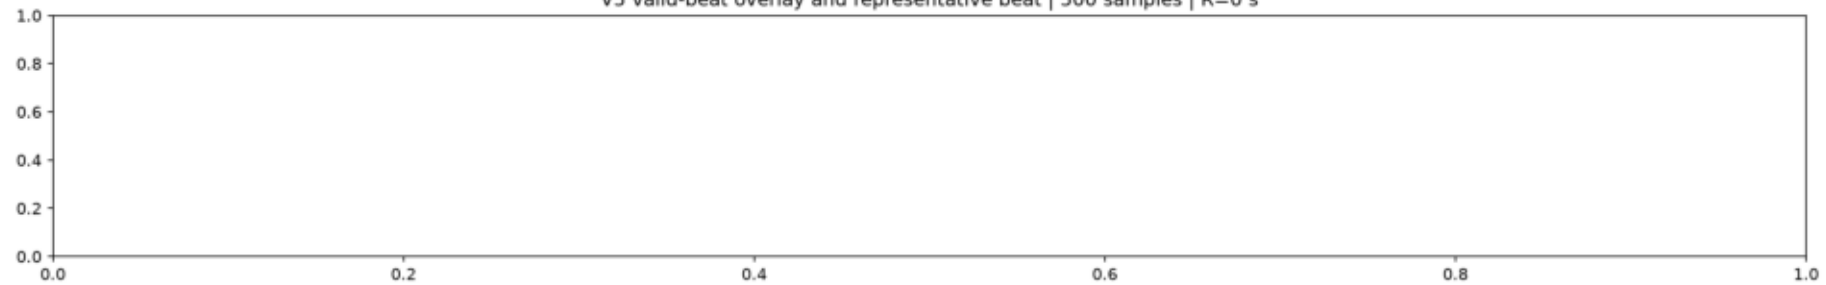


ECG 4210_NORM


Raw 12-lead ECG | ecg_id=4210 | label=NORM | amplitude=mV | time=s

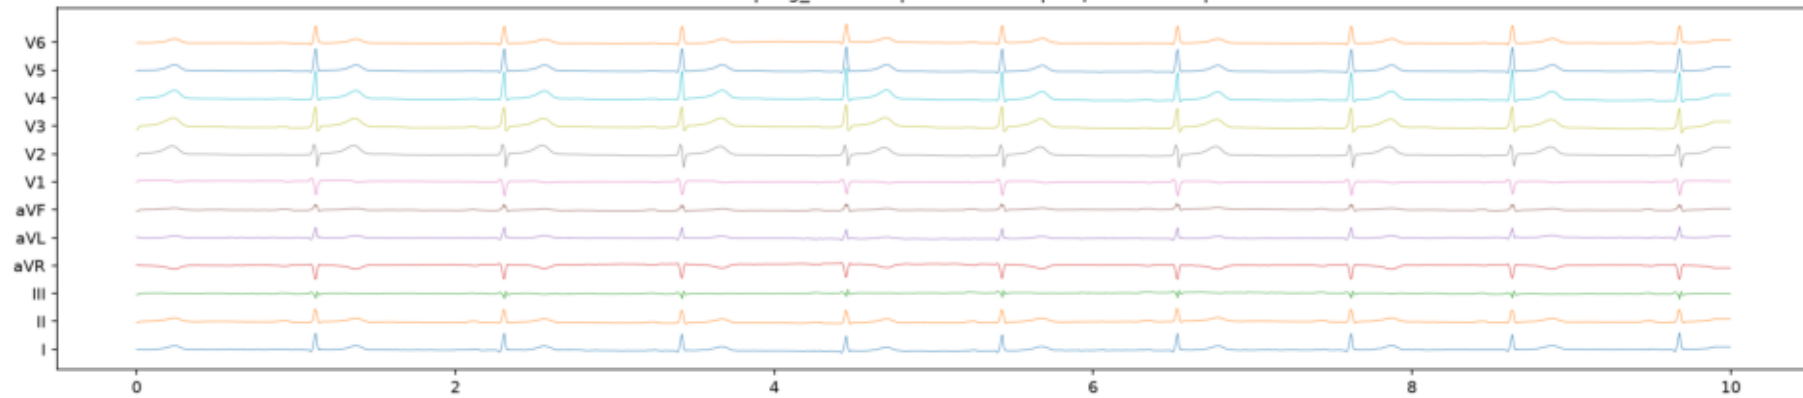


Detection bandpass composite and R candidates | peaks=17 | failure=rr_out_of_range

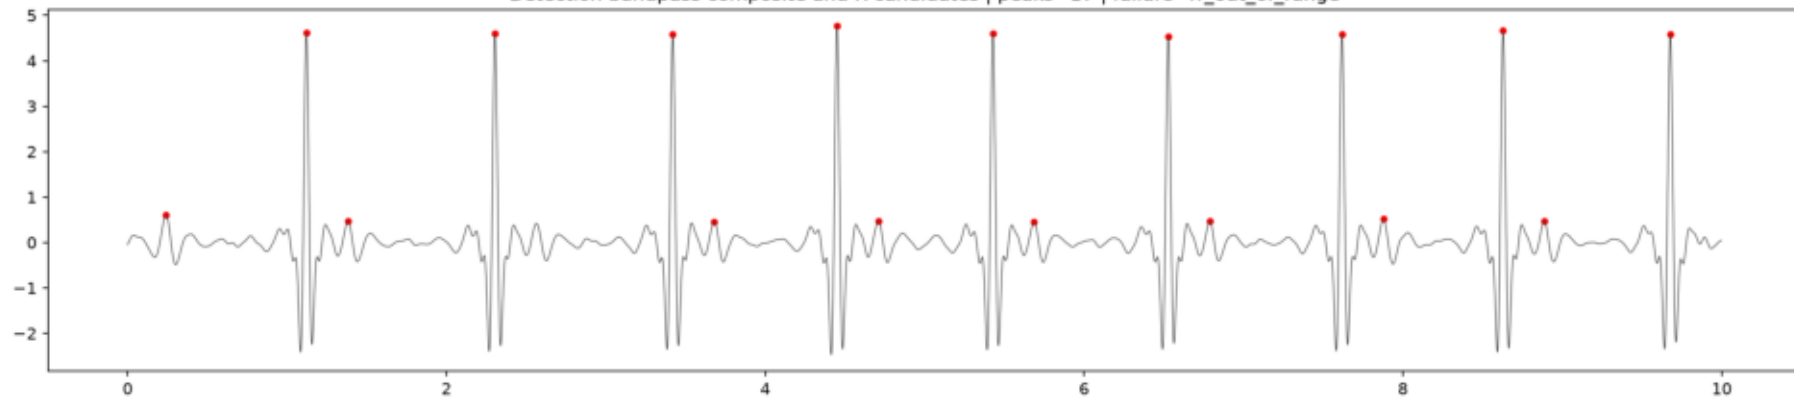

V5 segmentation boundaries | valid_beats=0 | units=mV,s

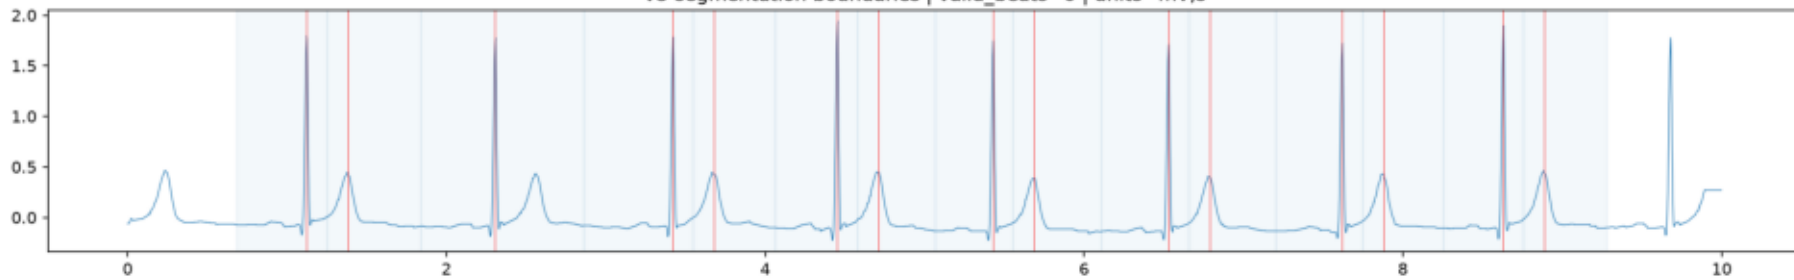


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

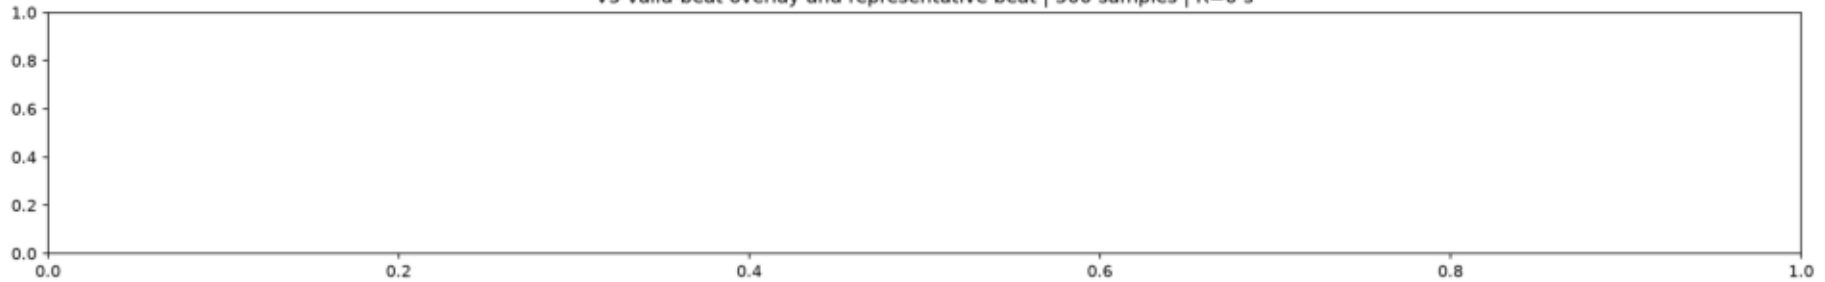


ECG 4374_NORM


Raw 12-lead ECG | ecg_id=4374 | label=NORM | amplitude=mV | time=s

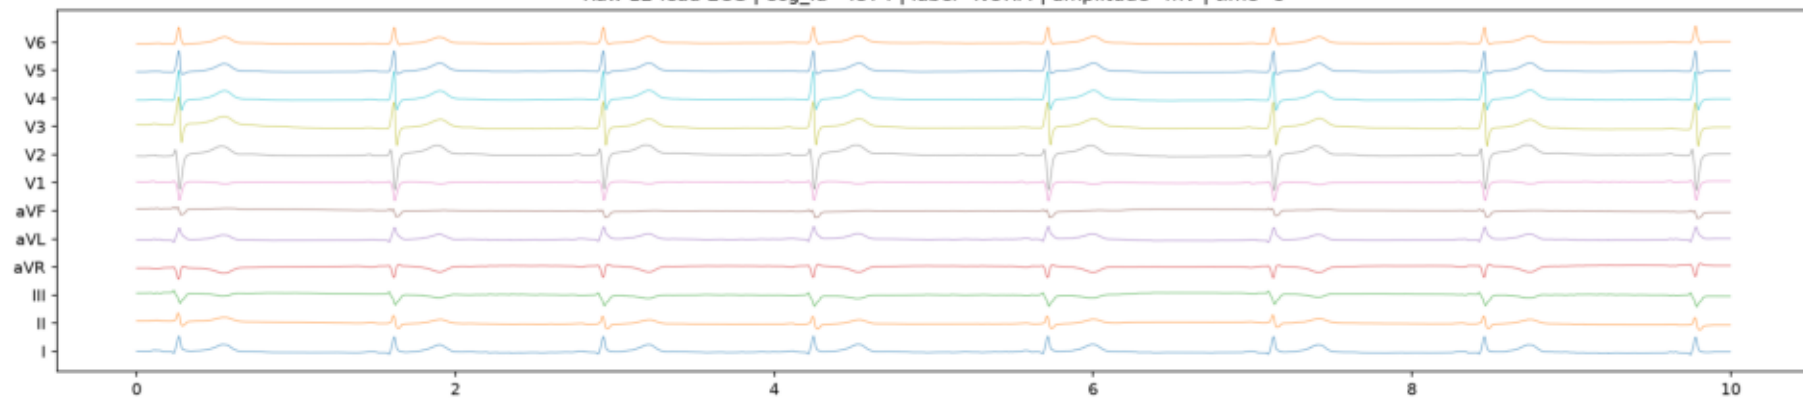


Detection bandpass composite and R candidates | peaks=15 | failure=rr_out_of_range

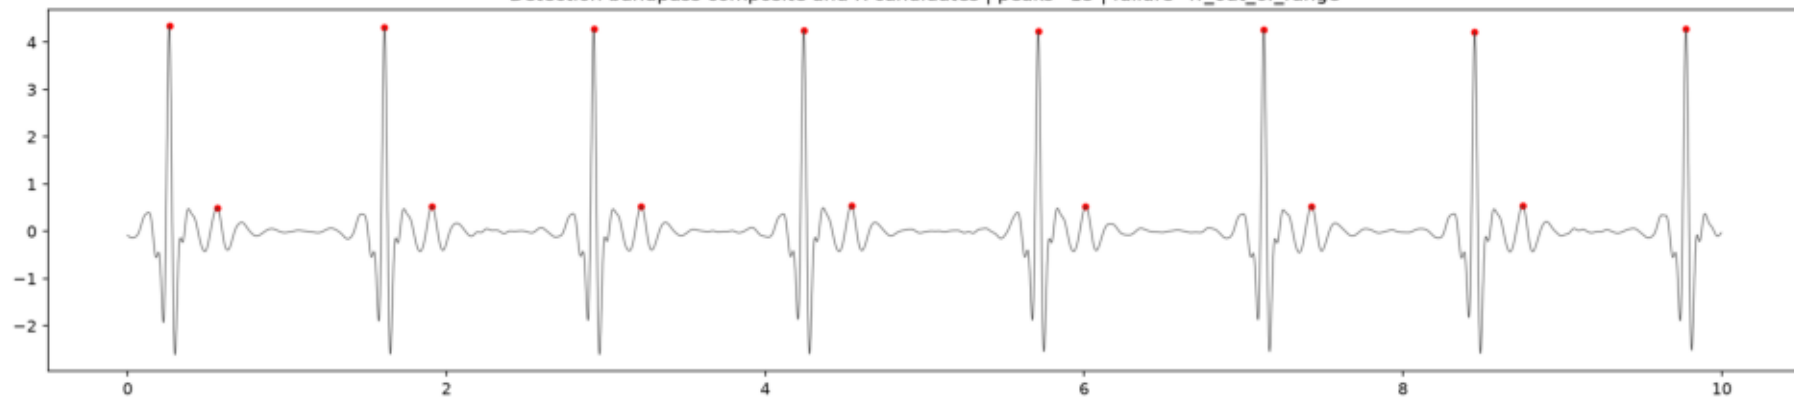

V5 segmentation boundaries | valid_beats=0 | units=mV,s

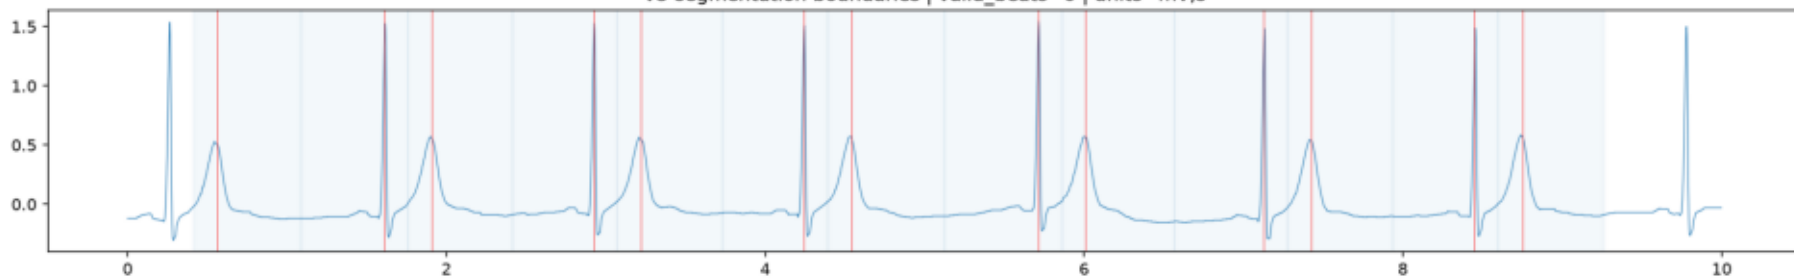


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

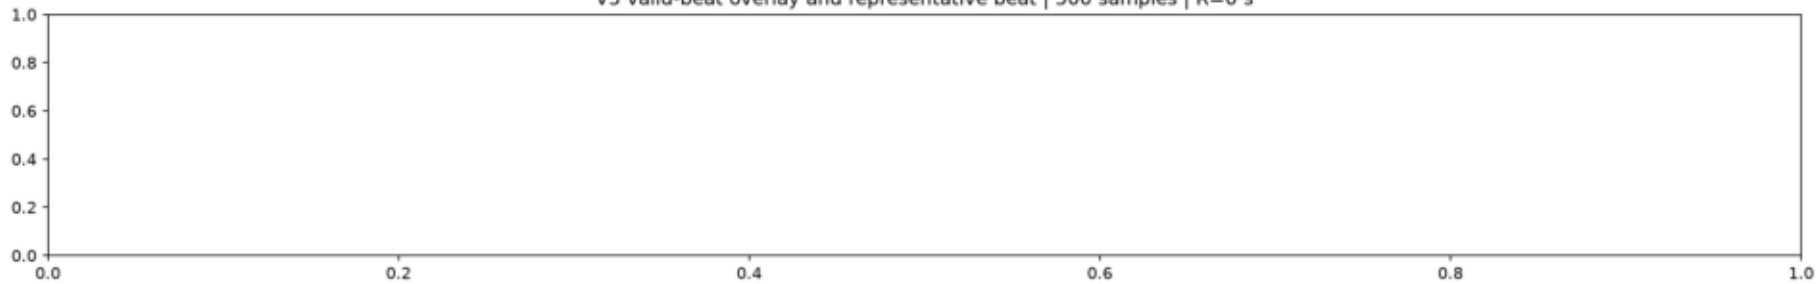


ECG 4802_NORM


Raw 12-lead ECG | ecg_id=4802 | label=NORM | amplitude=mV | time=s

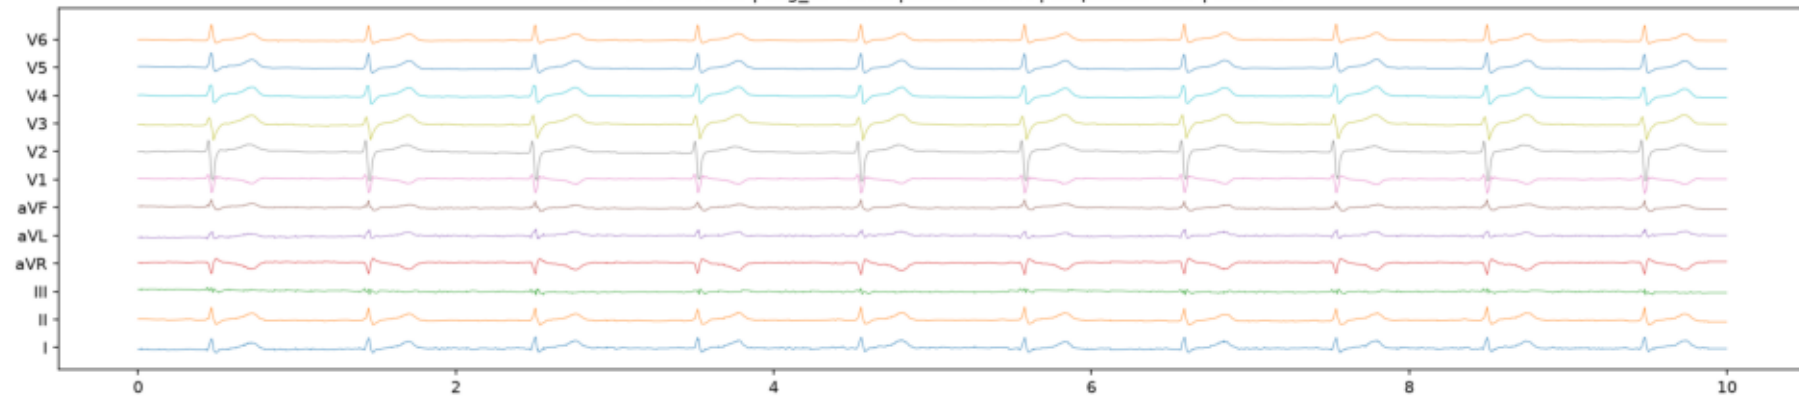


Detection bandpass composite and R candidates | peaks=18 | failure=rr_out_of_range

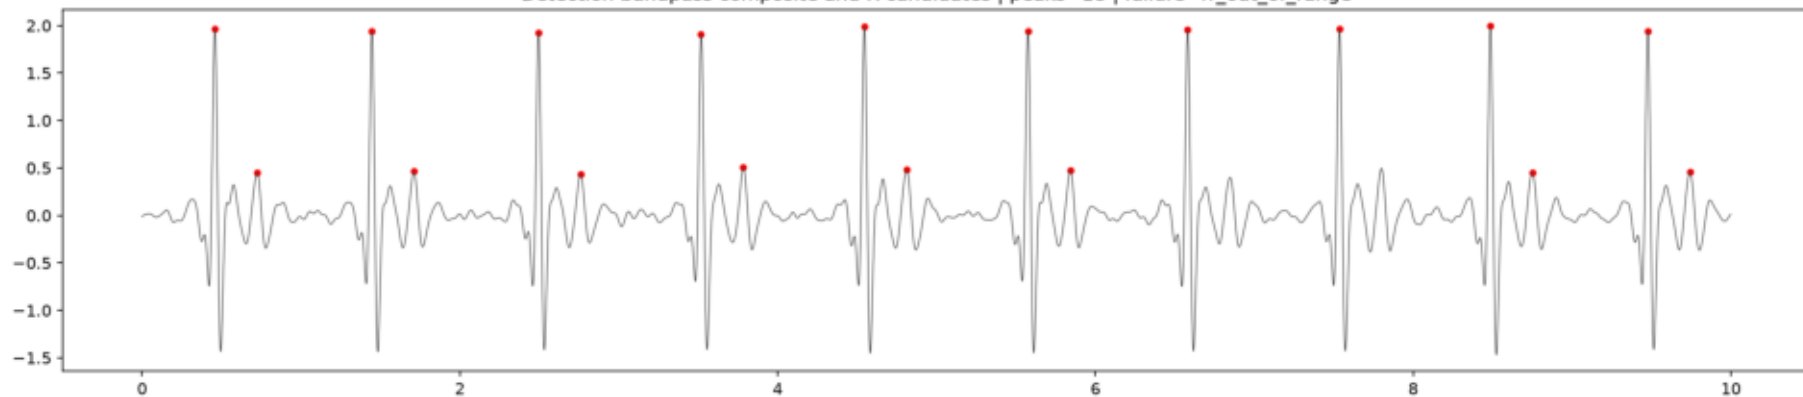

V5 segmentation boundaries | valid_beats=0 | units=mV,s

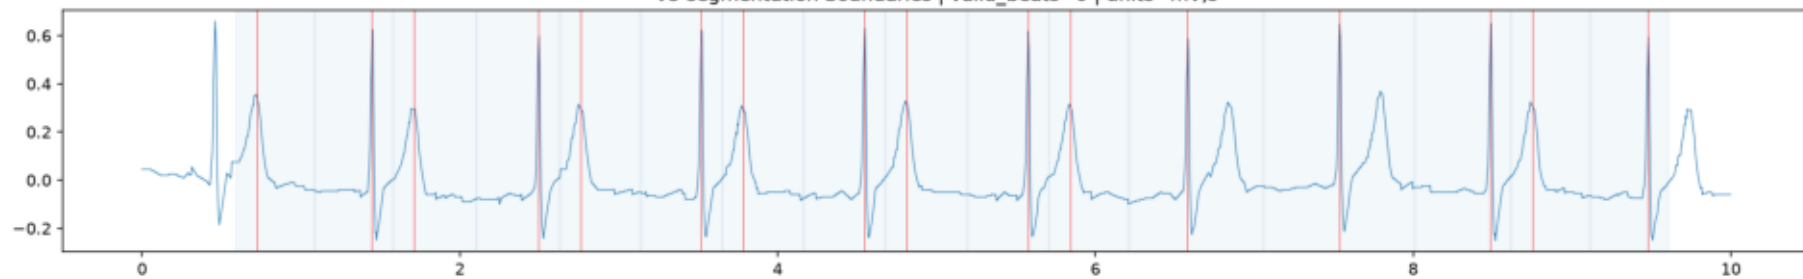


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

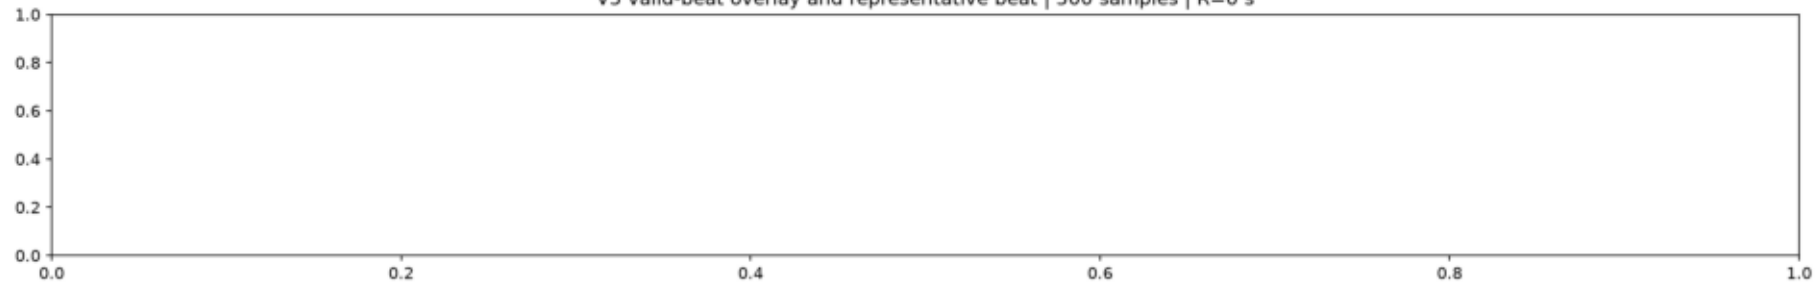


ECG 5783_NORM


Raw 12-lead ECG | ecg_id=5783 | label=NORM | amplitude=mV | time=s

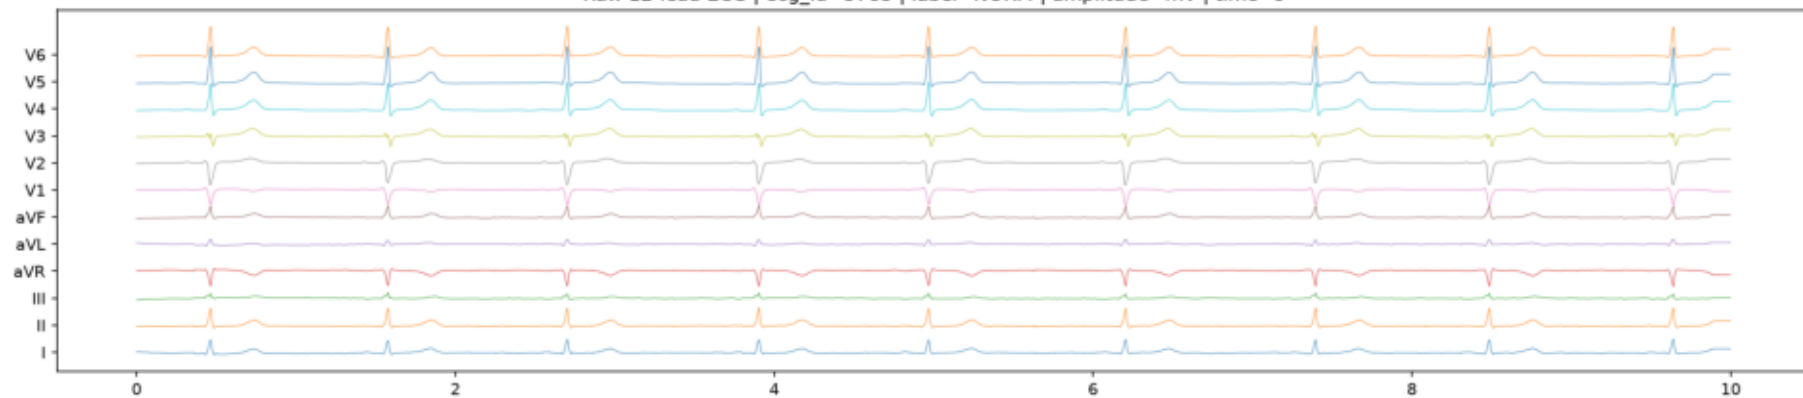


Detection bandpass composite and R candidates | peaks=17 | failure=rr_out_of_range

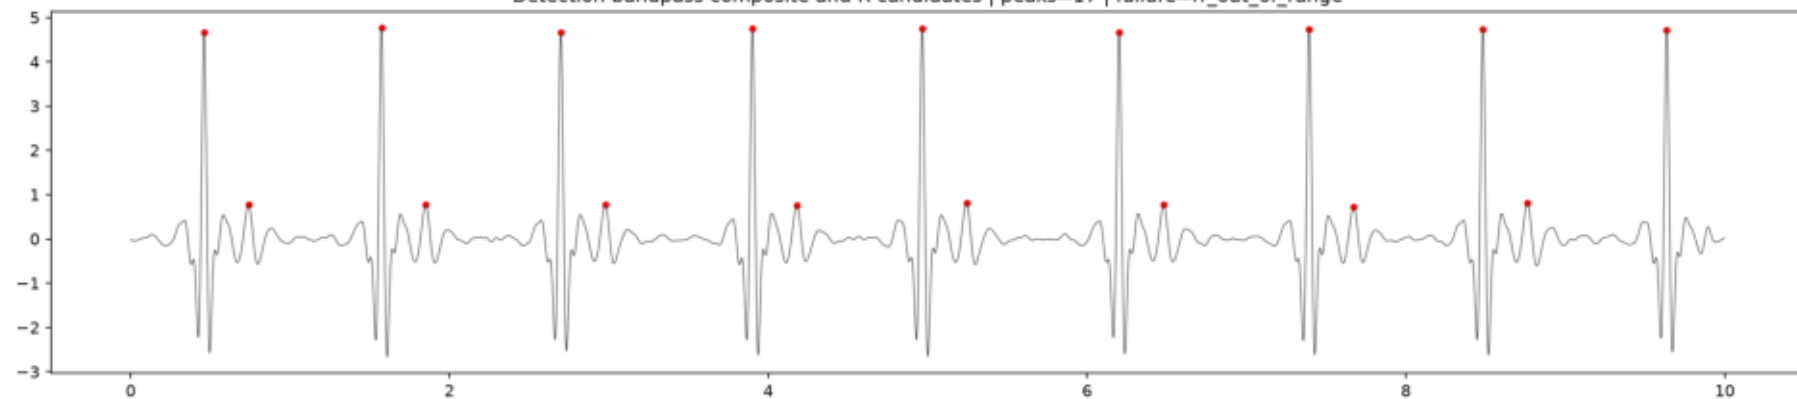

V5 segmentation boundaries | valid_beats=0 | units=mV,s

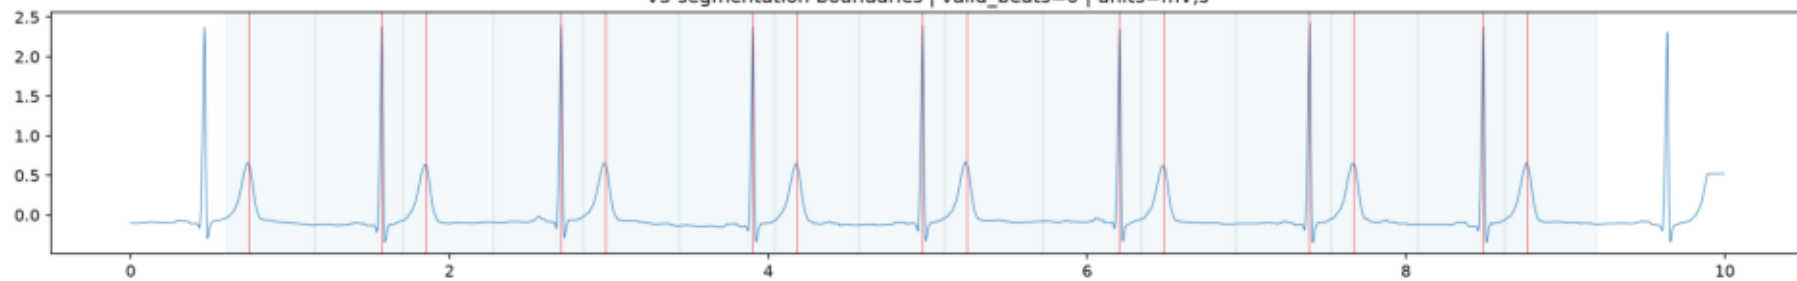


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

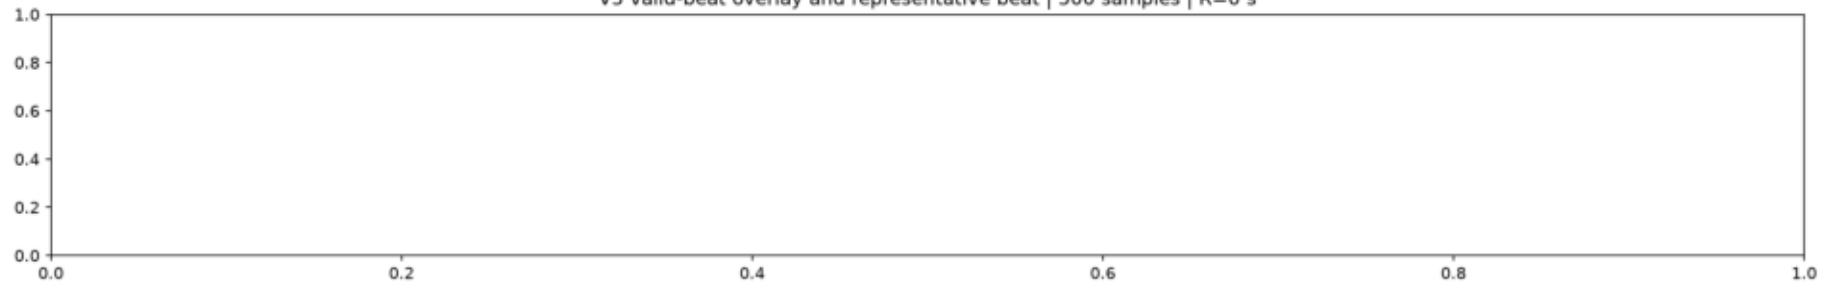


ECG 5962_NORM


Raw 12-lead ECG | ecg_id=5962 | label=NORM | amplitude=mV | time=s

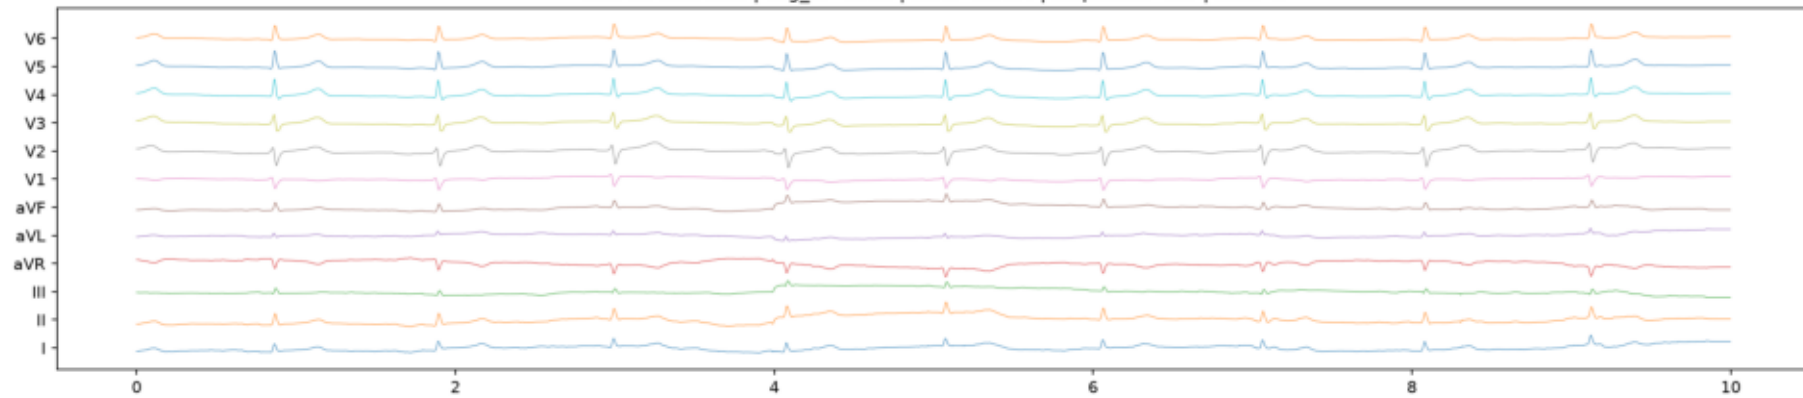


Detection bandpass composite and R candidates | peaks=16 | failure=rr_out_of_range

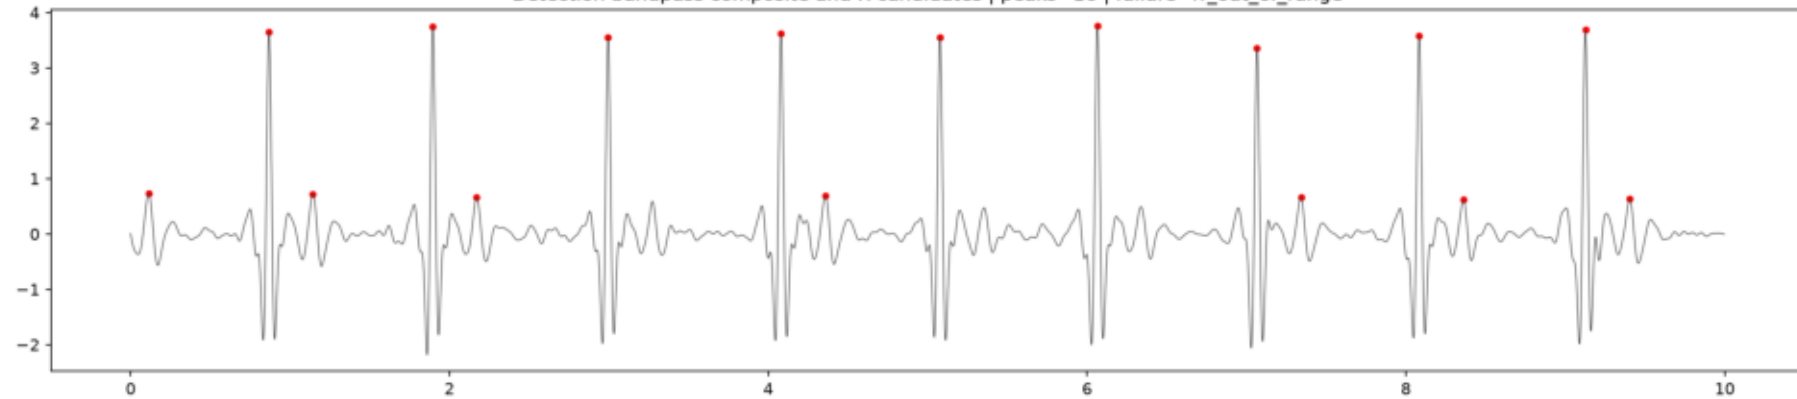

V5 segmentation boundaries | valid_beats=0 | units=mV,s

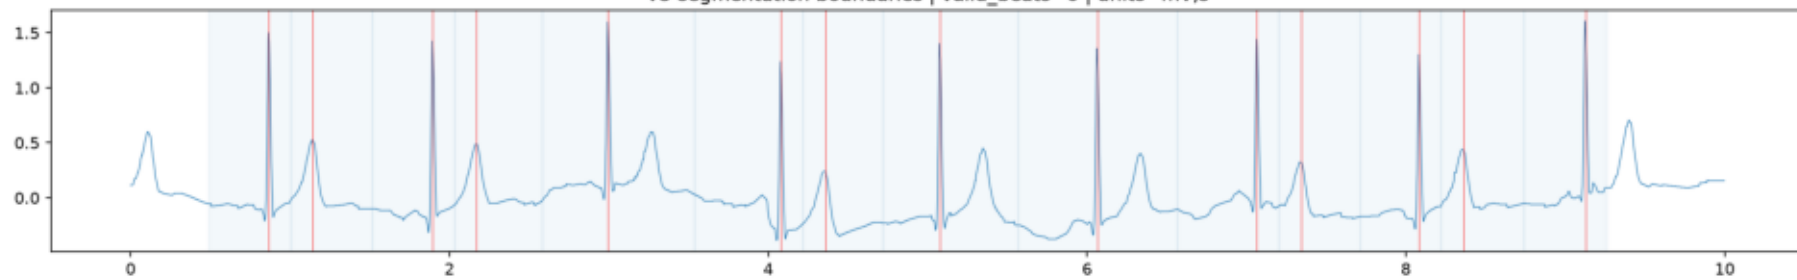


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

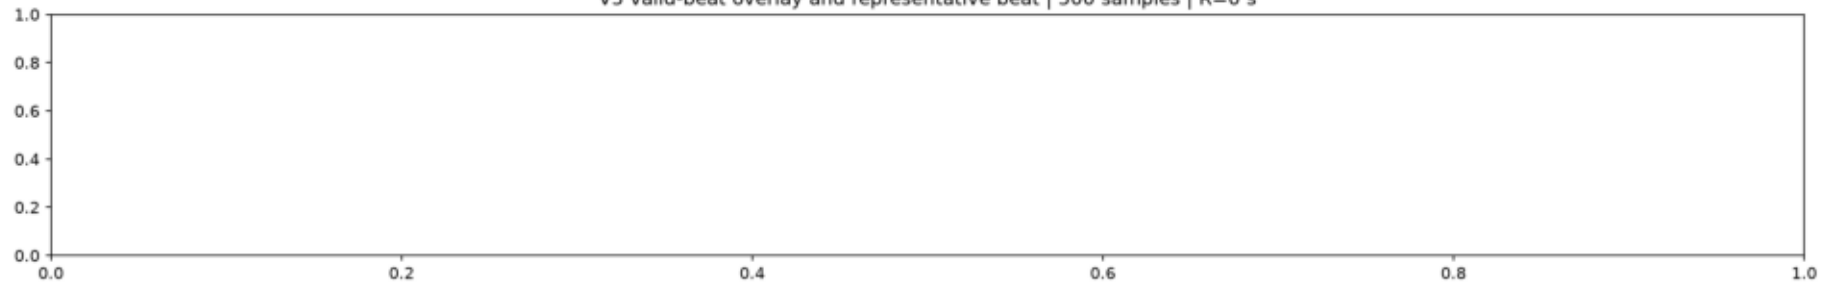


ECG 7198_LVH


Raw 12-lead ECG | ecg_id=7198 | label=LVH | amplitude=mV | time=s

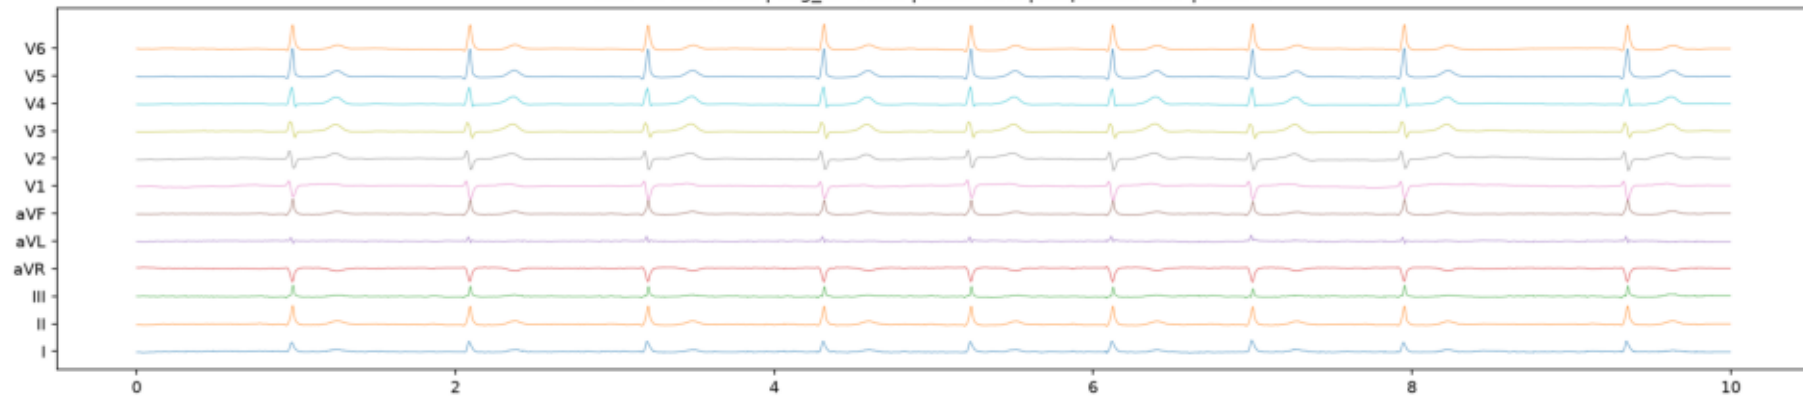


Detection bandpass composite and R candidates | peaks=16 | failure=rr_out_of_range

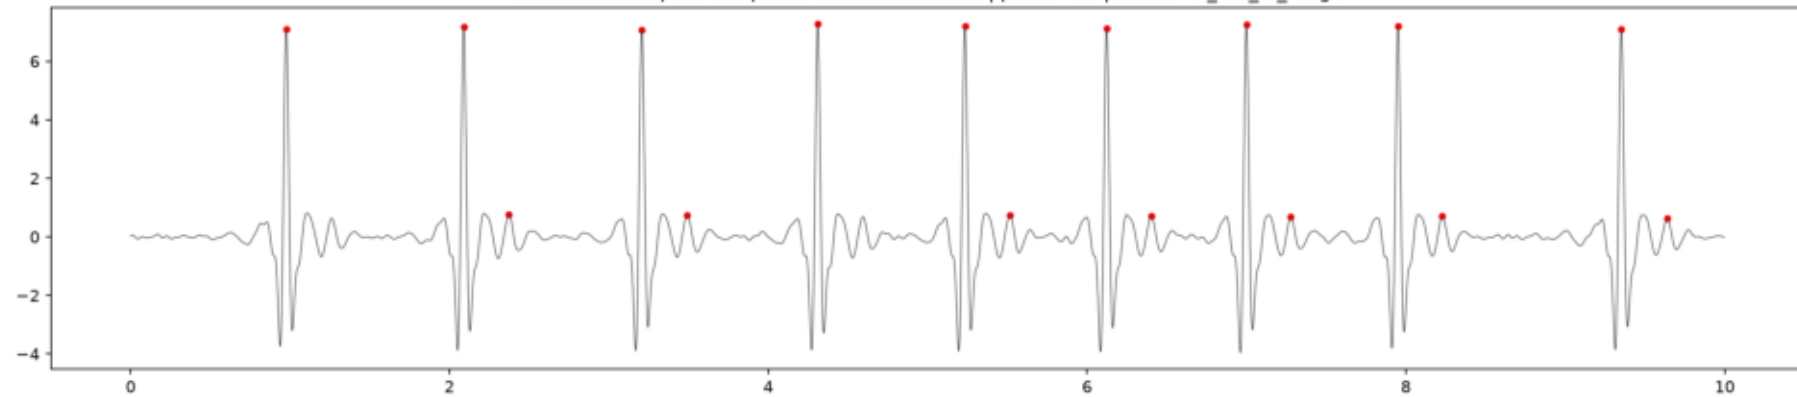

V5 segmentation boundaries | valid_beats=0 | units=mV,s

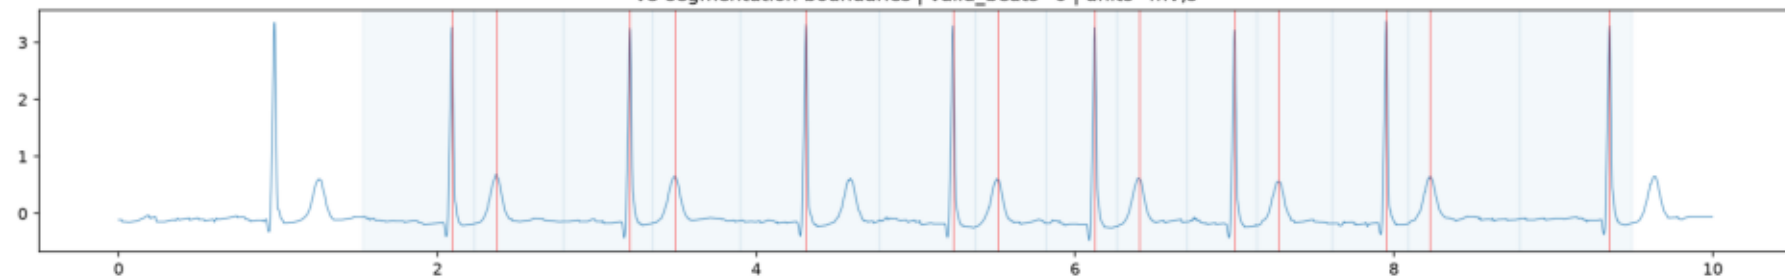


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

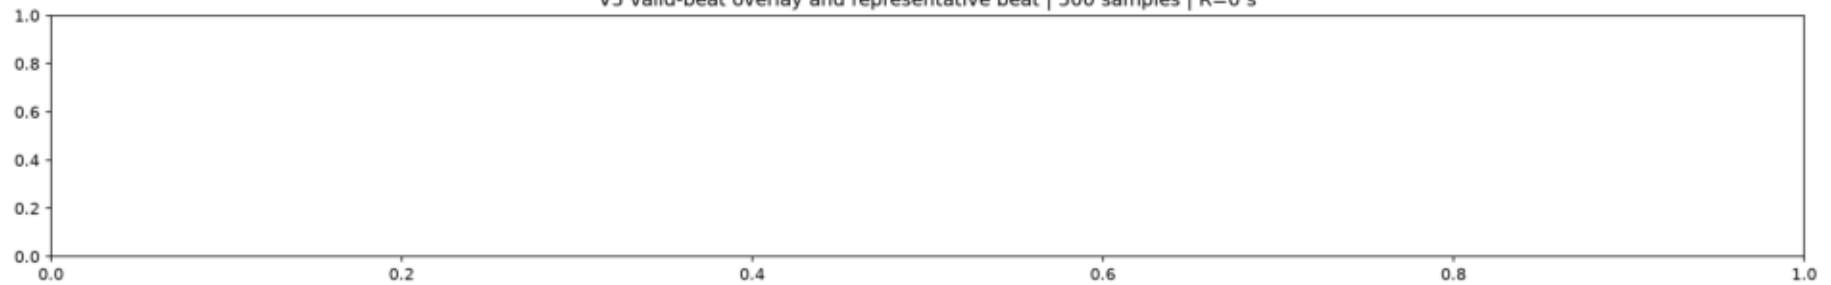


ECG 7503_LVH


Raw 12-lead ECG | ecg_id=7503 | label=LVH | amplitude=mV | time=s

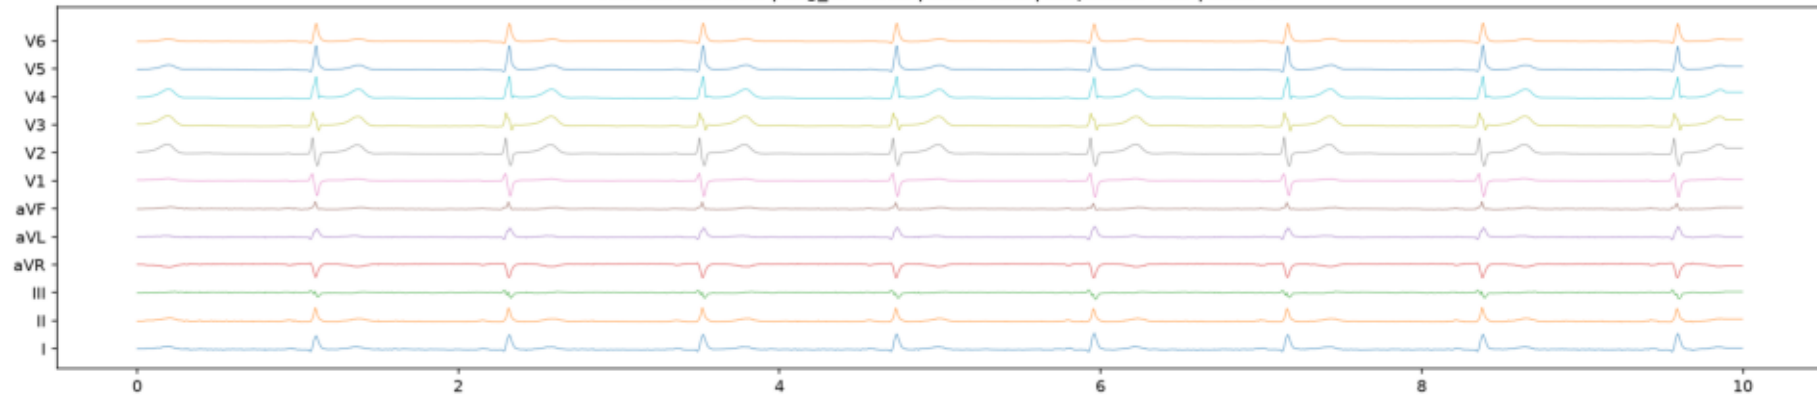


Detection bandpass composite and R candidates | peaks=8 | failure=nan

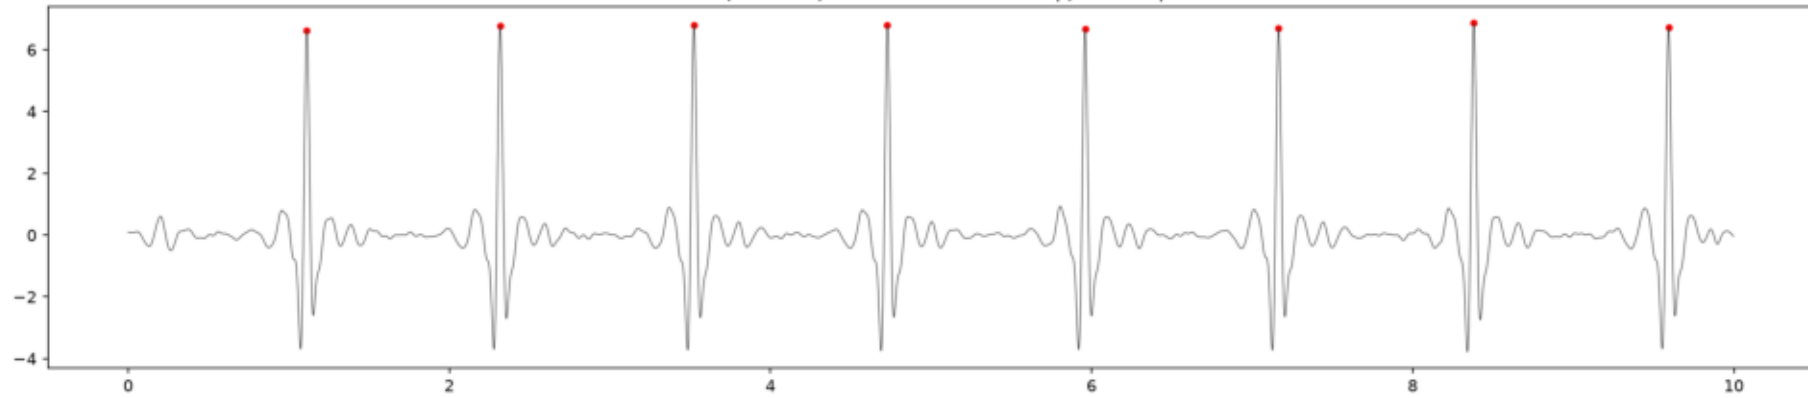

V5 segmentation boundaries | valid_beats=6 | units=mV,s

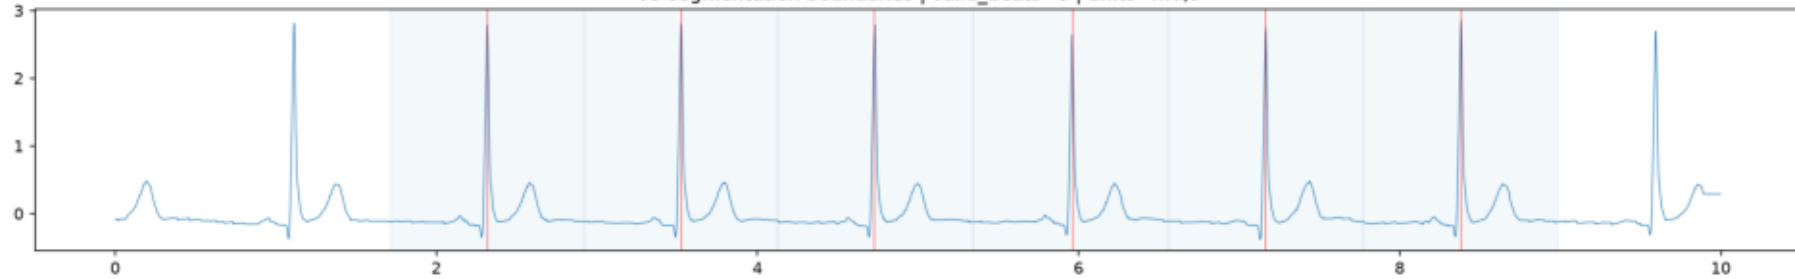


V5 valid-beat overlay and representative beat | 500 samples | R=0 s

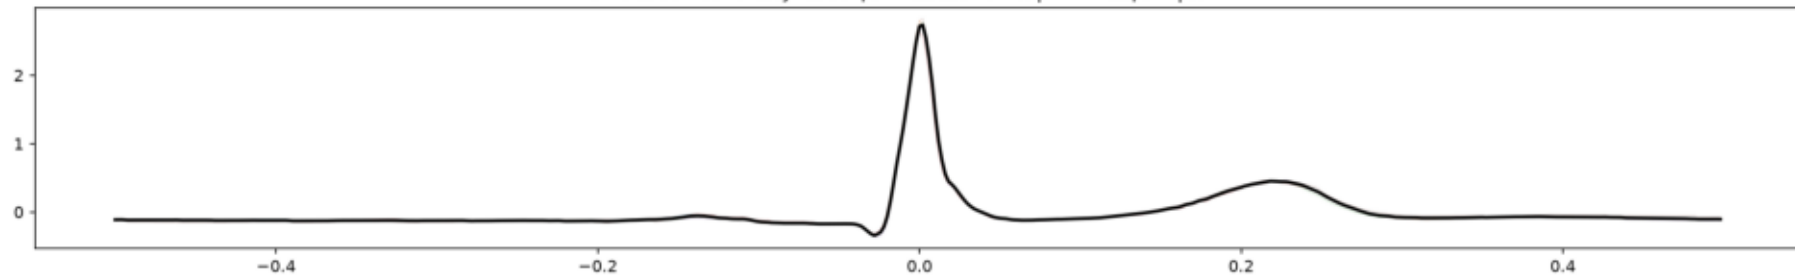


ECG 8315_LVH


Raw 12-lead ECG | ecg_id=8315 | label=LVH | amplitude=mV | time=s

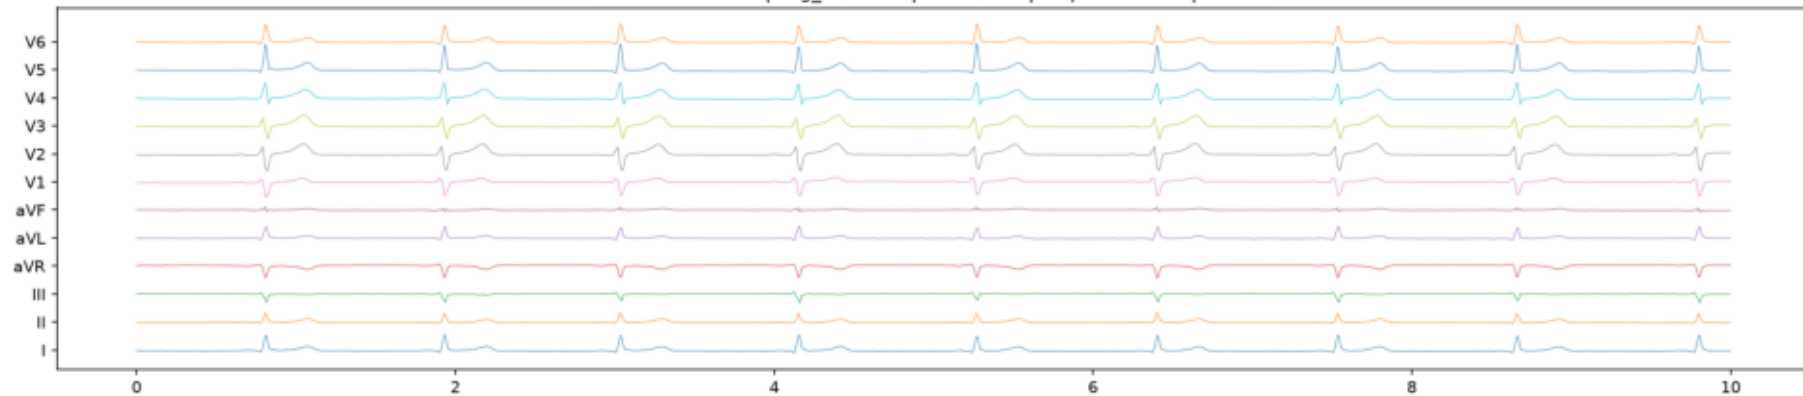

Detection bandpass composite and R candidates | peaks=17 | failure=rr_out_of_range

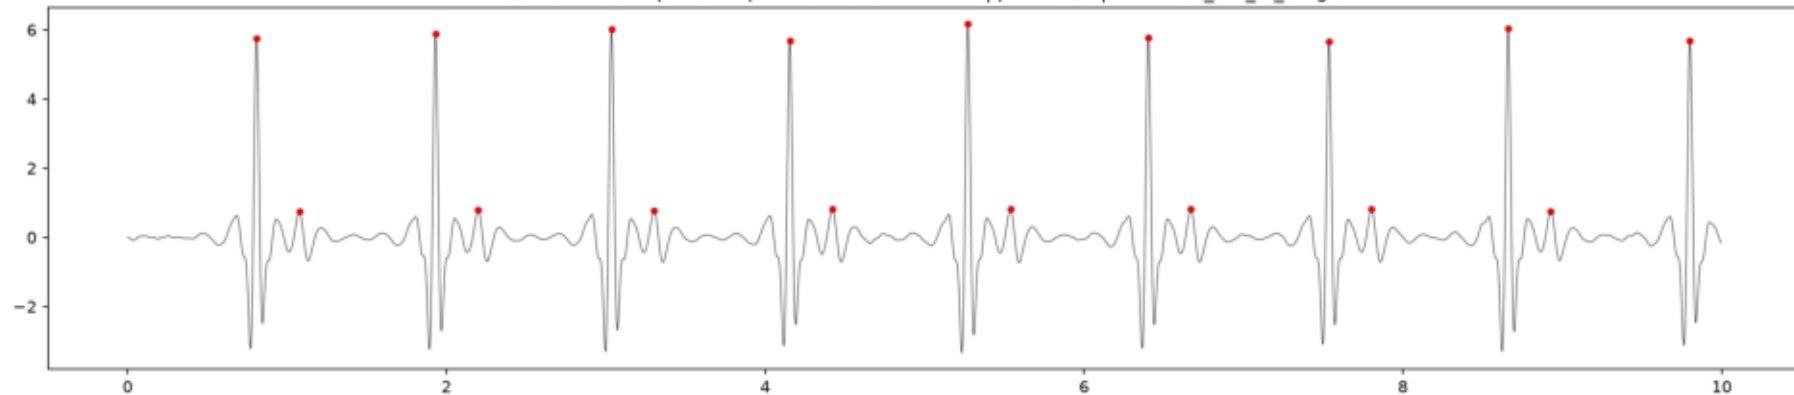

V5 segmentation boundaries | valid_beats=0 | units=mV,s

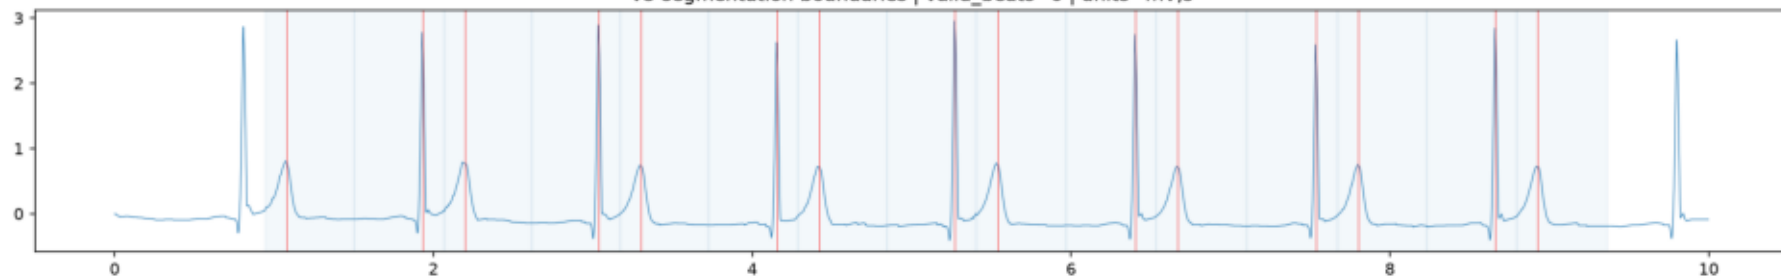

V5 valid-beat overlay and representative beat | 500 samples | R=0 s

