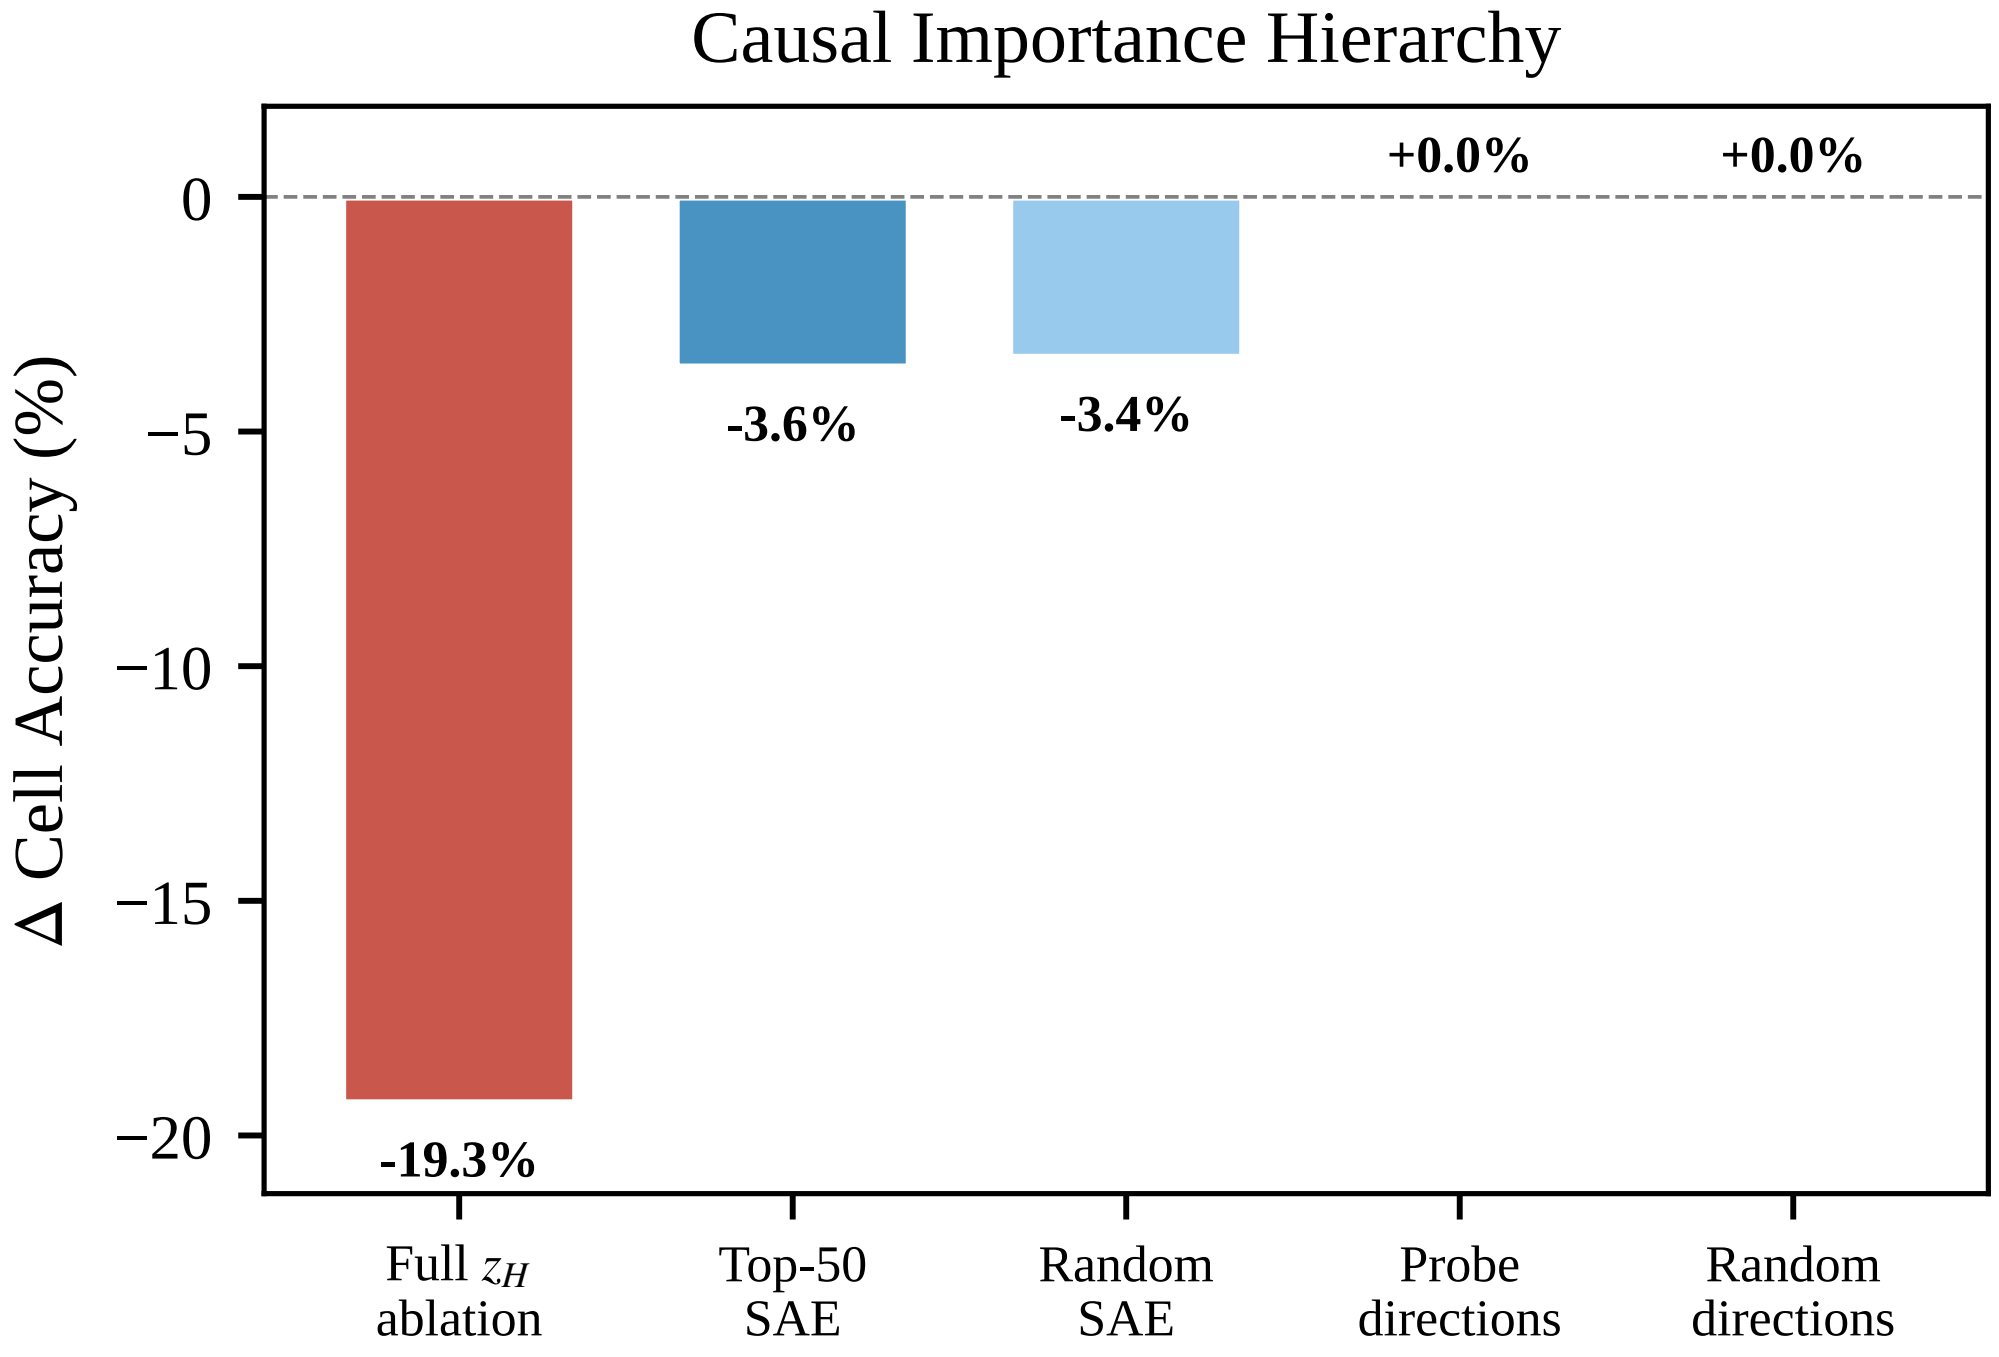
Causal Importance Hierarchy
Δ Cell Accuracy (%)
0
−5
−10
−15
−20
-19.3%
-3.6%
-3.4%
+0.0%
+0.0%
Full z_H ablation
Top-50 SAE
Random SAE
Probe directions
Random directions