
Filename: Briseno_05272025 - 2025-05-27 - 11.26.52.HSD5000

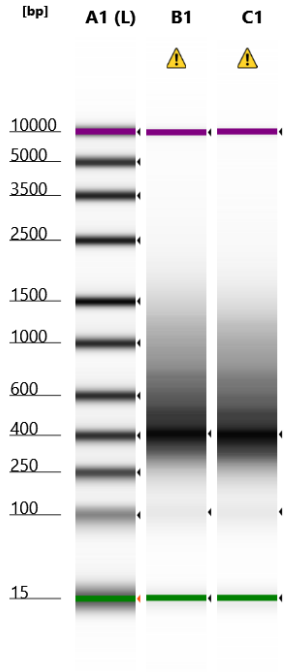

Default image (Contrast 50%), Image is Scaled to Highest Sample Peak

Sample Info

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
A1	2420	Ladder		Ladder
B1	12200	SL17	⚠	Sample concentration outside recommended range
C1	14300	SL18	⚠	Sample concentration outside recommended range

Compact Peak Table

Well	Sample Description	Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
A1	Ladder	15	362	-	37100	-		Lower Marker
A1	Ladder	100	261	-	4020	10.79		
A1	Ladder	250	283	-	1740	11.69		
A1	Ladder	400	289	-	1110	11.91		
A1	Ladder	600	282	-	723	11.63		
A1	Ladder	1000	272	-	418	11.22		
A1	Ladder	1500	283	-	290	11.68		
A1	Ladder	2500	252	-	155	10.40		
A1	Ladder	3500	256	-	112	10.56		
A1	Ladder	5000	245	-	75.4	10.12		
A1	Ladder	10000	180	180	27.7	-		Upper Marker
B1	SL17	15	281	-	28800	-		Lower Marker
B1	SL17	106	402	-	5840	3.30		
B1	SL17	407	11800	-	44600	96.70		
B1	SL17	10000	180	180	27.7	-		Upper Marker
C1	SL18	15	283	-	29000	-		Lower Marker
C1	SL18	106	450	-	6530	3.15		
C1	SL18	403	13800	-	52900	96.85		
C1	SL18	10000	180	180	27.7	-		Upper Marker

Compact Region Table


WellId	Sample Description	From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color

© Agilent Technologies, Inc. 2023


B1	SL17	200	3500	693	16200	47600	94.80		
C1	SL18	200	3500	648	17900	55400	94.39		

 © Agilent Technologies, Inc. 2023


A1: Ladder



B1: SL17




C1: SL18



© Agilent Technologies, Inc. 2023

Peak: A1: Ladder

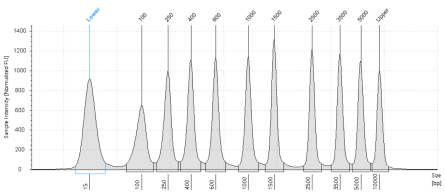


Location	A1
Concentration	2420
Description	Ladder
Observations	Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	362	-	37100	-		Lower Marker
100	261	-	4020	10.79		
250	283	-	1740	11.69		
400	289	-	1110	11.91		
600	282	-	723	11.63		
1000	272	-	418	11.22		
1500	283	-	290	11.68		
2500	252	-	155	10.40		
3500	256	-	112	10.56		
5000	245	-	75.4	10.12		

Peak: A1: Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
10000	180	180	27.7	-		Upper Marker


Peak: B1: SL17

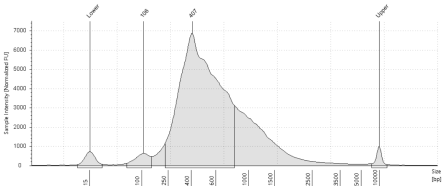

Location	B1
Concentration	12200
Description	SL17
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	281	-	28800	-		Lower Marker
106	402	-	5840	3.30		
407	11800	-	44600	96.70		
10000	180	180	27.7	-		Upper Marker

Region: B1: SL17

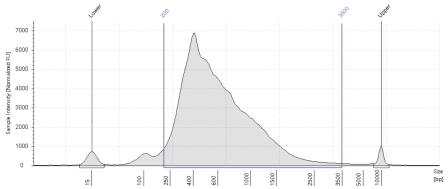


Location	B1
Concentration	12200
Description	SL17
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	693	16200	47600	94.80		

© Agilent Technologies, Inc. 2023


Peak: C1: SL18

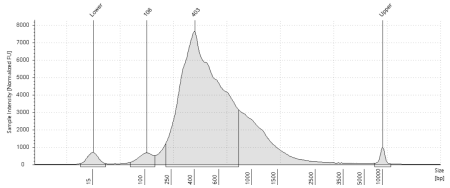

Location	C1
Concentration	14300
Description	SL18
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	283	-	29000	-		Lower Marker
106	450	-	6530	3.15		
403	13800	-	52900	96.85		
10000	180	180	27.7	-		Upper Marker

Region: C1: SL18

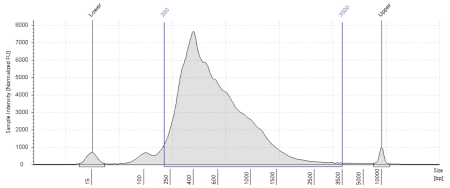

Location	C1
Concentration	14300
Description	SL18
Alert	⚠
Observations	Sample concentration outside recommended range


From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	648	17900	55400	94.39		

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Log Linear Piecewise
Alignment type: Between markers

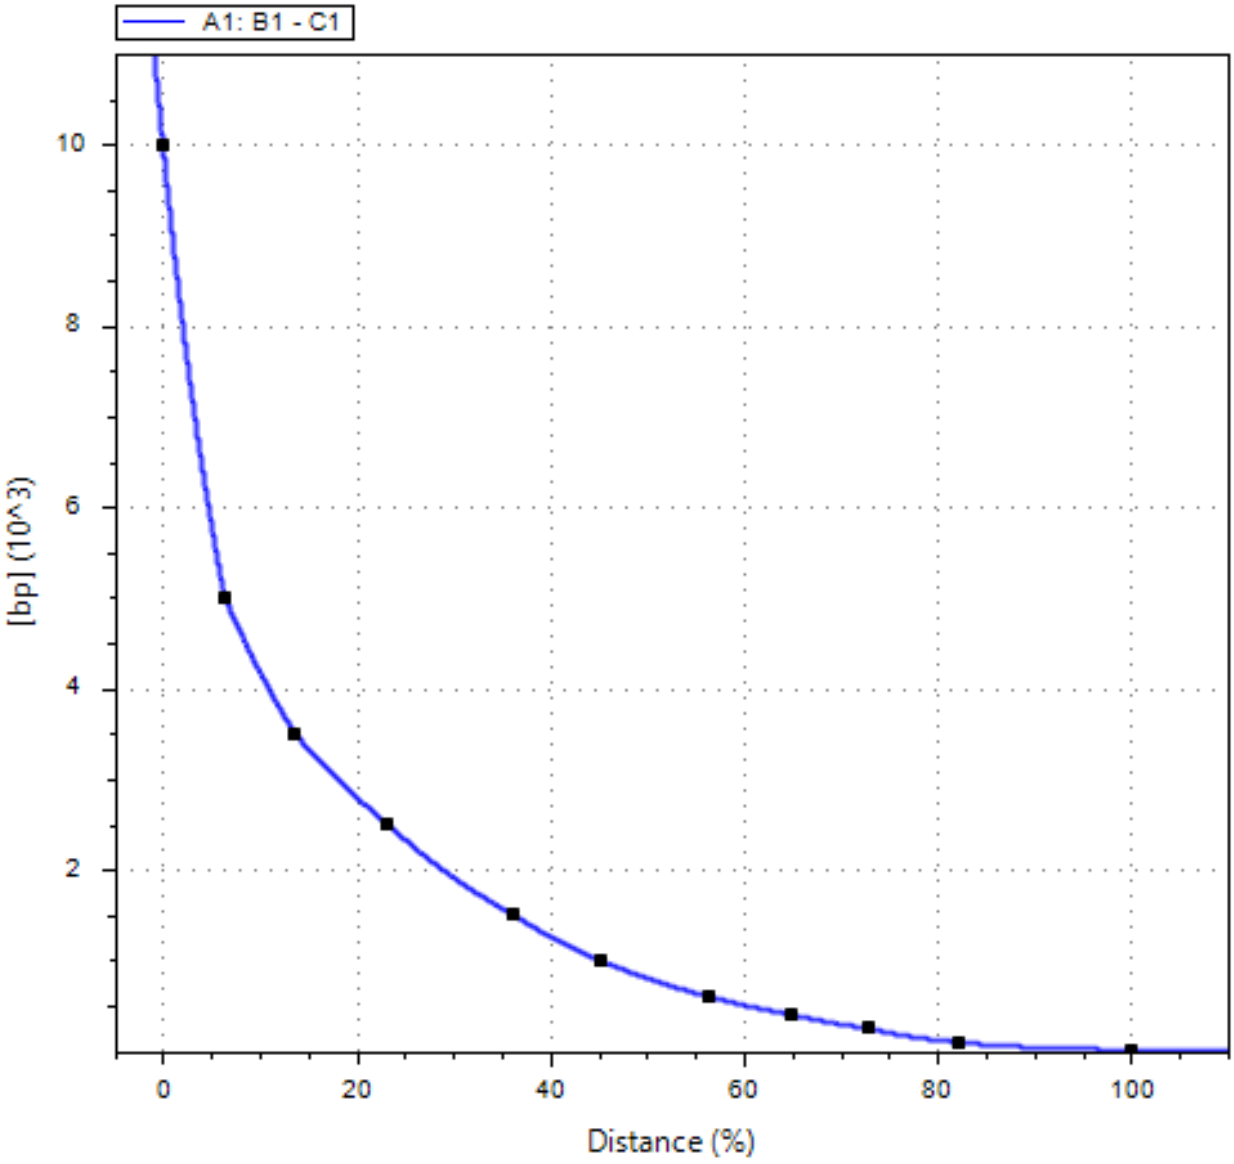

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

© Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2025-05-27\Briseno_05272025 - 2025-05-27 - 11.26.52.HSD5000
Assay	HSD5000
Run End Date	2025-05-27T11:34:50-04:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Zhou_Kanadia_23May25
ScreenTape Device ID	01-S032-241223-01-002290
Expiry Date	2025-06-10T23:59:59
ScreenTape Device History	First run 27 May 2025, 1 run(s) performed
Temperature [°C]	26.4
Electrophoresis Time [s]	213
Instrument Type	4200 TapeStation (G2991A)
Instrument Serial Number	DEDAA01484
Notes	
ScreenTape Device Run Date	2025-05-27T11:26:52-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

© Agilent Technologies, Inc. 2023