
Filename: Muller1stPCR_DBlibs_28May2025 - 2025-05-28 - 12.27.36.HSD1000

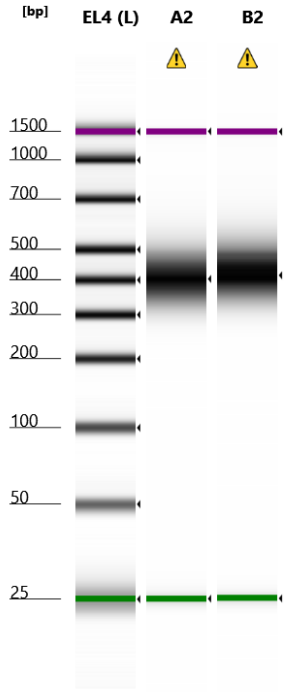

Default image (Contrast 50%), Image is Scaled to Highest Sample Peak

Sample Info


Well	Conc. [pg/µl]	Sample Description	Alert	Observations
EL4	2350	Electronic Ladder		Ladder
A2	8050	JB 17 (2ul)	⚠	Sample concentration outside recommended range
B2	10500	JB 18 (2ul)	⚠	Sample concentration outside recommended range

Compact Peak Table


Well	Sample Description	Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
EL4	Electronic Ladder	25	340	-	20900	-		Lower Marker
EL4	Electronic Ladder	50	265	-	8160	11.28		
EL4	Electronic Ladder	100	278	-	4270	11.82		
EL4	Electronic Ladder	200	290	-	2230	12.32		
EL4	Electronic Ladder	300	304	-	1560	12.95		
EL4	Electronic Ladder	400	306	-	1180	13.00		
EL4	Electronic Ladder	500	312	-	961	13.29		
EL4	Electronic Ladder	700	286	-	629	12.19		
EL4	Electronic Ladder	1000	309	-	476	13.15		
EL4	Electronic Ladder	1500	250	250	256	-		Upper Marker
A2	JB 17 (2ul)	25	356	-	21900	-		Lower Marker
A2	JB 17 (2ul)	402	8050	-	30800	100.00		
A2	JB 17 (2ul)	1500	250	250	256	-		Upper Marker
B2	JB 18 (2ul)	25	365	-	22500	-		Lower Marker
B2	JB 18 (2ul)	415	10500	-	38800	100.00		
B2	JB 18 (2ul)	1500	250	250	256	-		Upper Marker

© Agilent Technologies, Inc. 2023


EL4: Electronic Ladder



A2: JB 17 (2ul)




B2: JB 18 (2ul)



© Agilent Technologies, Inc. 2023


Peak: EL4: Electronic Ladder

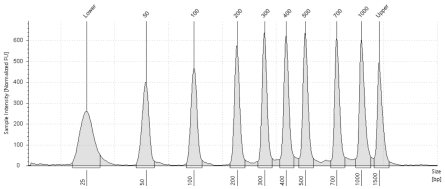

Location EL4
Concentration 2350
Description Electronic Ladder
Observations Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
25	340	-	20900	-		Lower Marker
50	265	-	8160	11.28		
100	278	-	4270	11.82		
200	290	-	2230	12.32		
300	304	-	1560	12.95		
400	306	-	1180	13.00		
500	312	-	961	13.29		
700	286	-	629	12.19		
1000	309	-	476	13.15		
1500	250	250	256	-		Upper Marker


Peak: A2: JB 17 (2ul)

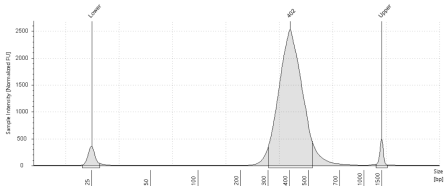

Location A2
Concentration 8050
Description JB 17 (2ul)
Alert ⚠
Observations Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
25	356	-	21900	-		Lower Marker
402	8050	-	30800	100.00		
1500	250	250	256	-		Upper Marker

Peak: B2: JB 18 (2ul)

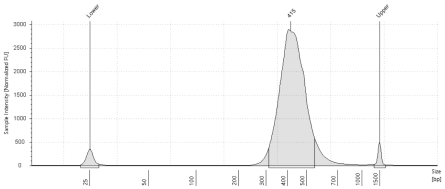

Location B2
Concentration 10500
Description JB 18 (2ul)
Alert ⚠
Observations Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
25	365	-	22500	-		Lower Marker
415	10500	-	38800	100.00		
1500	250	250	256	-		Upper Marker


© Agilent Technologies, Inc. 2023

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Piecewise Interpolation
Alignment type: Between markers

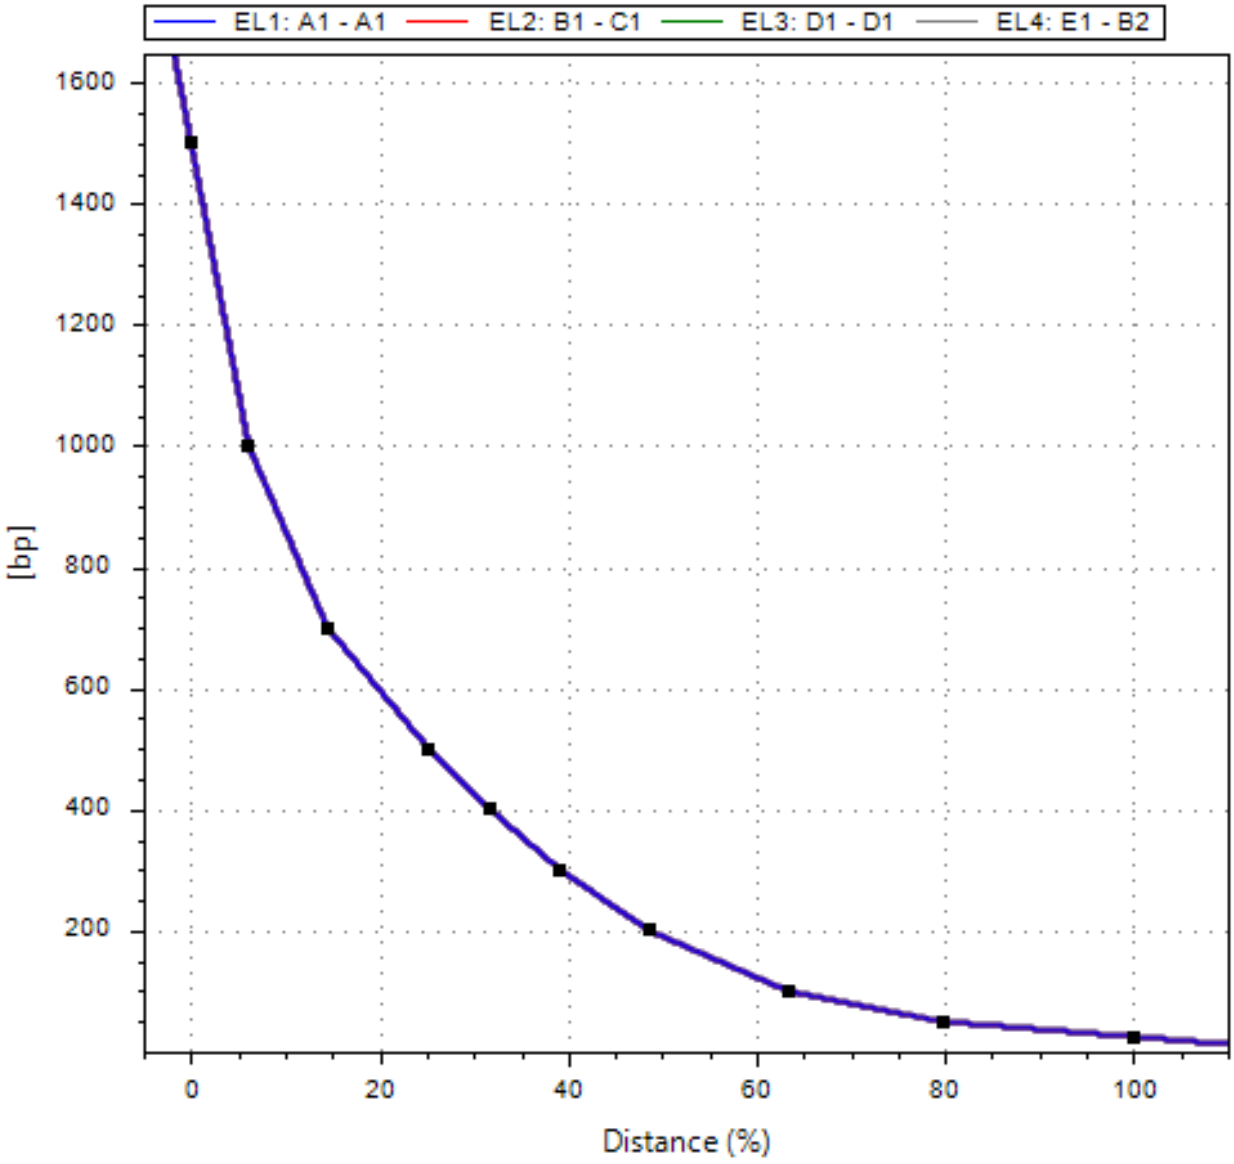

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

© Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2025-05-28\Muller1stPCR_DBlibs_28May2025 - 2025-05-28 - 12.27.36.HSD1000
Assay	D1000 High Sensitivity
Run End Date	2025-05-28T12:48:57-04:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Tapestation 4200B
ScreenTape Device ID	01-S030-250204-01-002371
Expiry Date	2025-05-27T23:59:59
ScreenTape Device History	First run 13 May 2025, 5 run(s) performed
Temperature [°C]	26.4
Electrophoresis Time [s]	145
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	1ul
ScreenTape Device Run Date	2025-05-28T12:27:36-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

ScreenTape Device 2

Username	Tapestation 4200B
ScreenTape Device ID	01-S030-250403-01-000518
Expiry Date	2025-05-28T23:59:59
ScreenTape Device History	First run 14 May 2025, 5 run(s) performed
Temperature [°C]	26.4
Electrophoresis Time [s]	145
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	1ul
ScreenTape Device Run Date	2025-05-28T12:27:36-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

ScreenTape Device 3

Username	Tapestation 4200B
ScreenTape Device ID	01-S030-250204-01-002374

© Agilent Technologies, Inc. 2023

Expiry Date	2025-05-15T23:59:59
ScreenTape Device History	First run 01 May 2025, 6 run(s) performed
Temperature [°C]	26.5
Electrophoresis Time [s]	145
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	1ul
ScreenTape Device Run Date	2025-05-28T12:27:36-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

ScreenTape Device 4

Username	Tapestation 4200B
ScreenTape Device ID	01-S030-250403-01-000517
Expiry Date	2025-06-11T23:59:59
ScreenTape Device History	First run 28 May 2025, 1 run(s) performed
Temperature [°C]	26.6
Electrophoresis Time [s]	145
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	1ul
ScreenTape Device Run Date	2025-05-28T12:27:36-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

© Agilent Technologies, Inc. 2023