
Filename: JB_cDNAQC_23Jul2025 - 2025-07-23 - 12.34.44.HSD5000

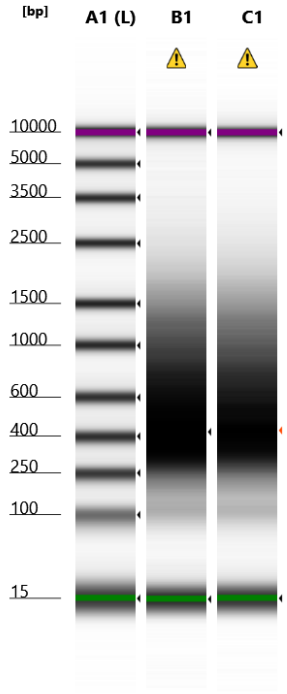

Default image (Contrast 100%)

Sample Info

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
A1	1470	Ladder		Ladder
B1	3900	19	⚠	Sample concentration outside recommended range
C1	3540	20	⚠	Sample concentration outside recommended range

Compact Peak Table

Well	Sample Description	Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
A1	Ladder	15	321	-	33000	-		Lower Marker
A1	Ladder	100	170	-	2610	11.54		
A1	Ladder	250	183	-	1120	12.41		
A1	Ladder	400	180	-	693	12.25		
A1	Ladder	600	172	-	441	11.69		
A1	Ladder	1000	168	-	258	11.41		
A1	Ladder	1500	161	-	165	10.96		
A1	Ladder	2500	149	-	91.5	10.10		
A1	Ladder	3500	146	-	64.1	9.91		
A1	Ladder	5000	143	-	44.1	9.74		
A1	Ladder	10000	180	180	27.7	-		Upper Marker
B1	19	15	306	-	31400	-		Lower Marker
B1	19	421	3900	-	14200	100.00		
B1	19	10000	180	180	27.7	-		Upper Marker
C1	20	15	325	-	33300	-		Lower Marker
C1	20	425	3540	-	12800	100.00		
C1	20	10000	180	180	27.7	-		Upper Marker


Compact Region Table

WellId	Sample Description	From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
B1	19	200	3500	685	3750	11400	93.28		
C1	20	200	3500	688	3380	10200	92.73		


© Agilent Technologies, Inc. 2023

 © Agilent Technologies, Inc. 2023


A1: Ladder



B1: 19




C1: 20



 © Agilent Technologies, Inc. 2023

A1: Ladder

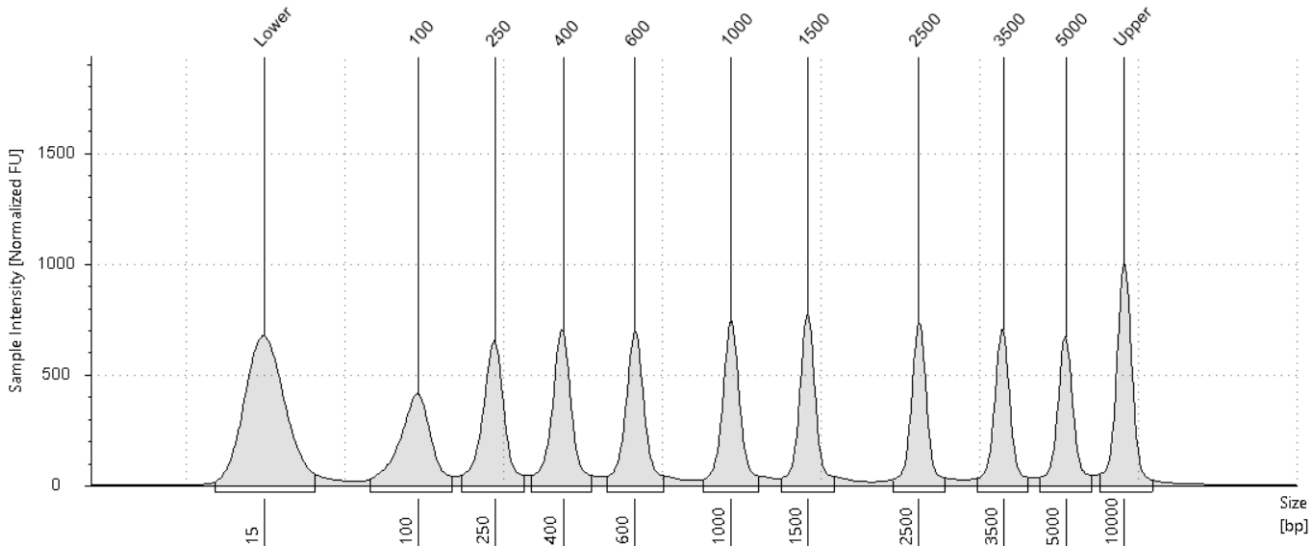

Sample Table


Well	Conc. [pg/µl]	Sample Description	Alert	Observations
A1	1470	Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
15	321	-	33000	-		Lower Marker
100	170	-	2610	11.54		
250	183	-	1120	12.41		
400	180	-	693	12.25		
600	172	-	441	11.69		
1000	168	-	258	11.41		
1500	161	-	165	10.96		
2500	149	-	91.5	10.10		
3500	146	-	64.1	9.91		
5000	143	-	44.1	9.74		
10000	180	180	27.7	-		Upper Marker

 © Agilent Technologies, Inc. 2023

B1: 19

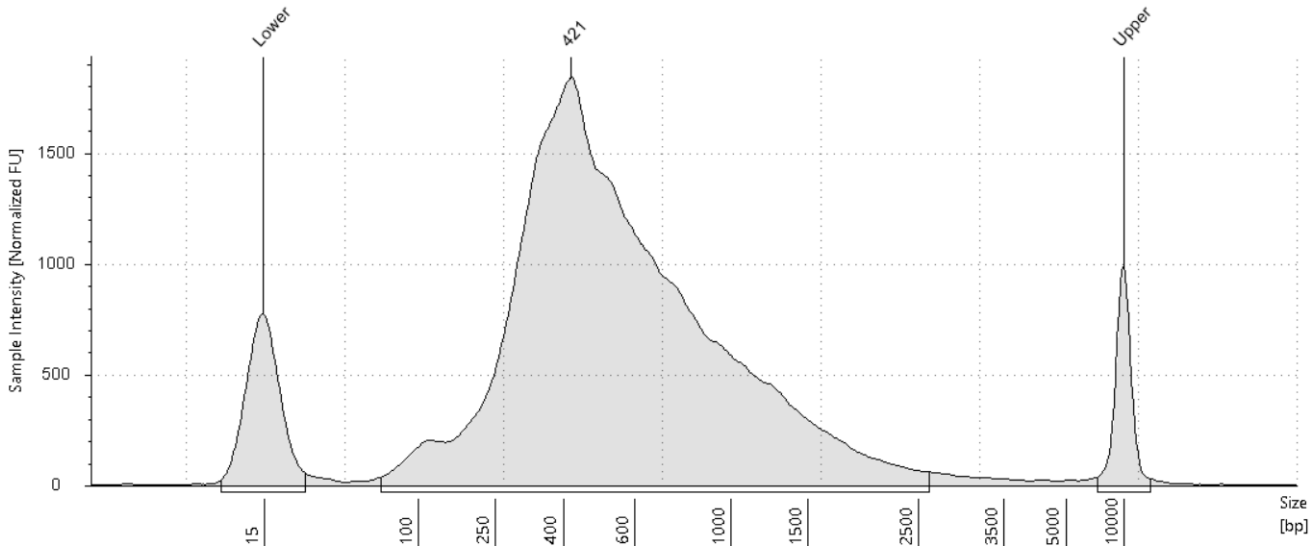


Sample Table

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
B1	3900	19	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
15	306	-	31400	-		Lower Marker
421	3900	-	14200	100.00		
10000	180	180	27.7	-		Upper Marker

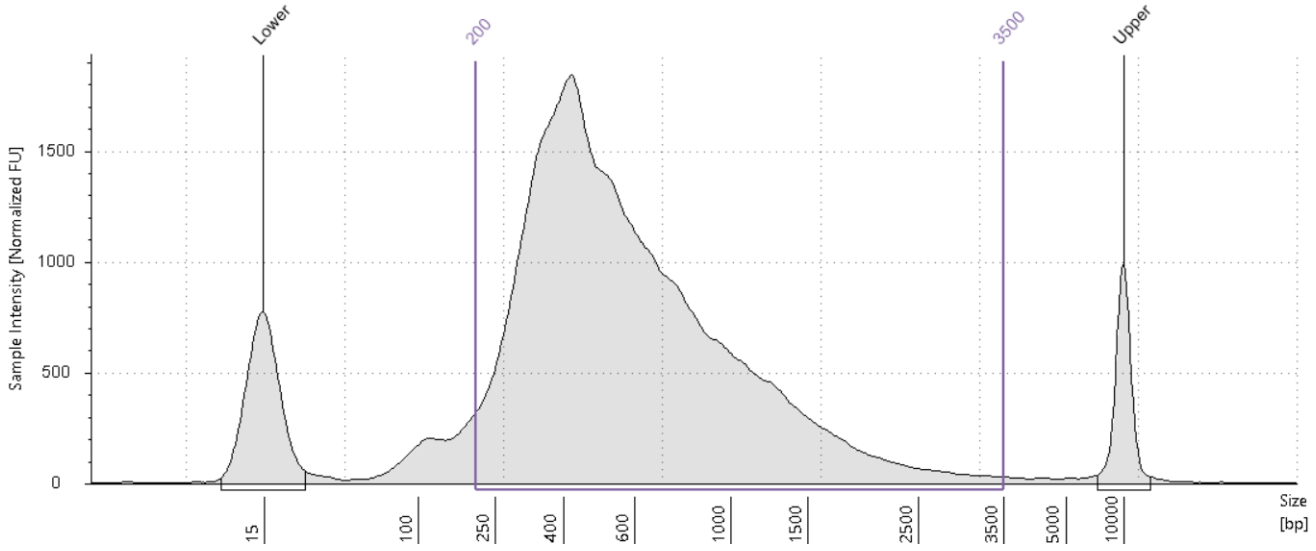


Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	685	3750	11400	93.28		

© Agilent Technologies, Inc. 2023

C1: 20

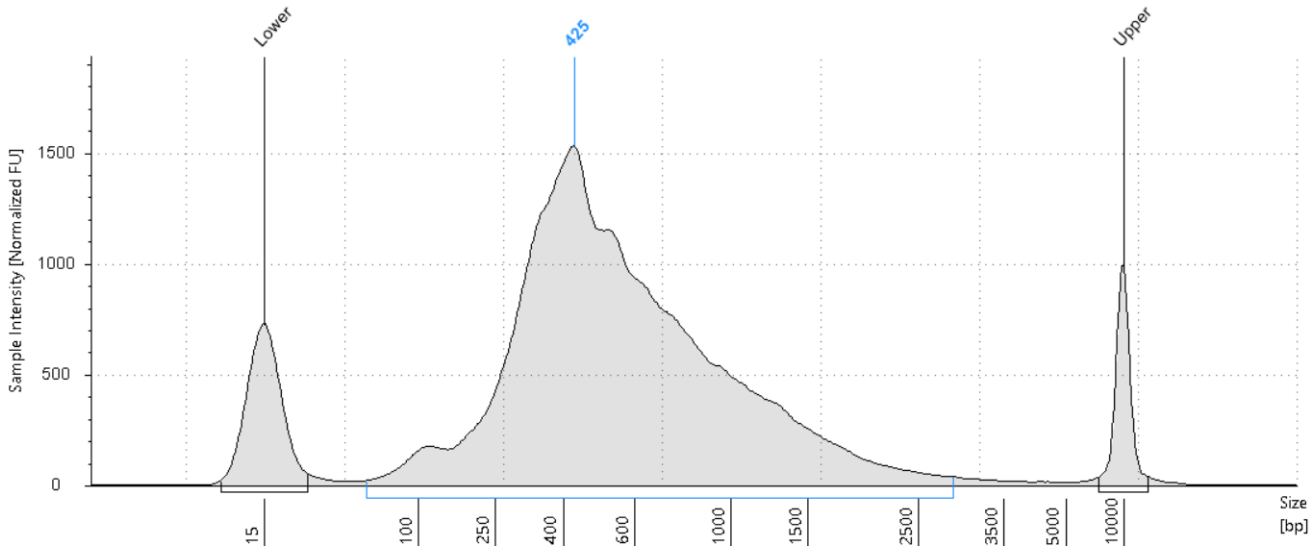


Sample Table

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
C1	3540	20	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
15	325	-	33300	-		Lower Marker
425	3540	-	12800	100.00		
10000	180	180	27.7	-		Upper Marker

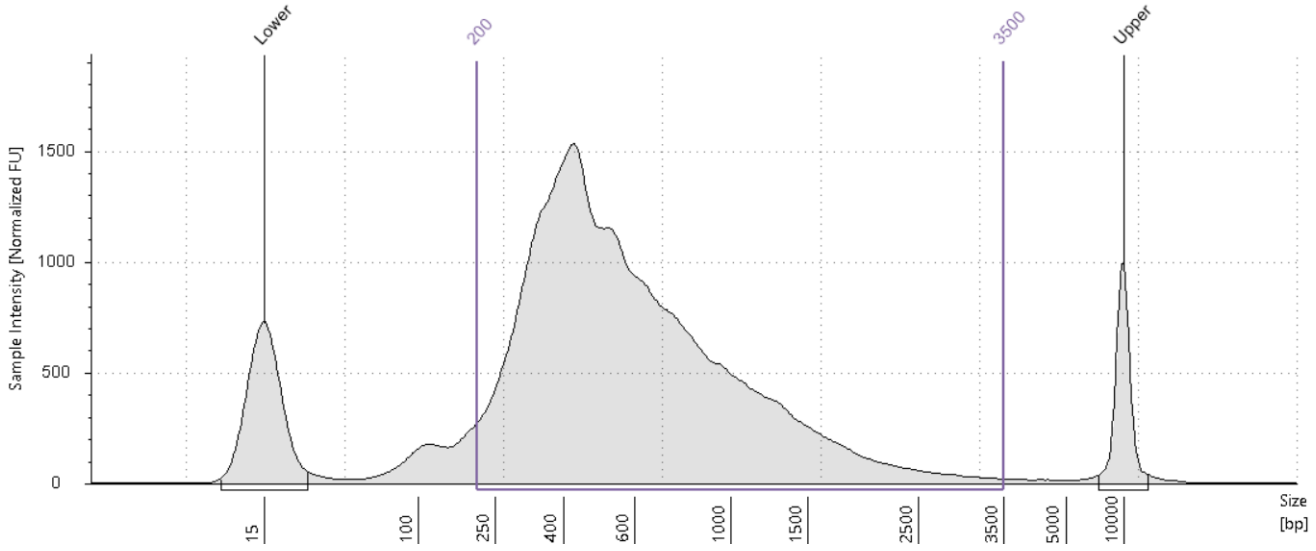

Region Table


From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	688	3380	10200	92.73		

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Log Linear Piecewise
Alignment type: Between markers

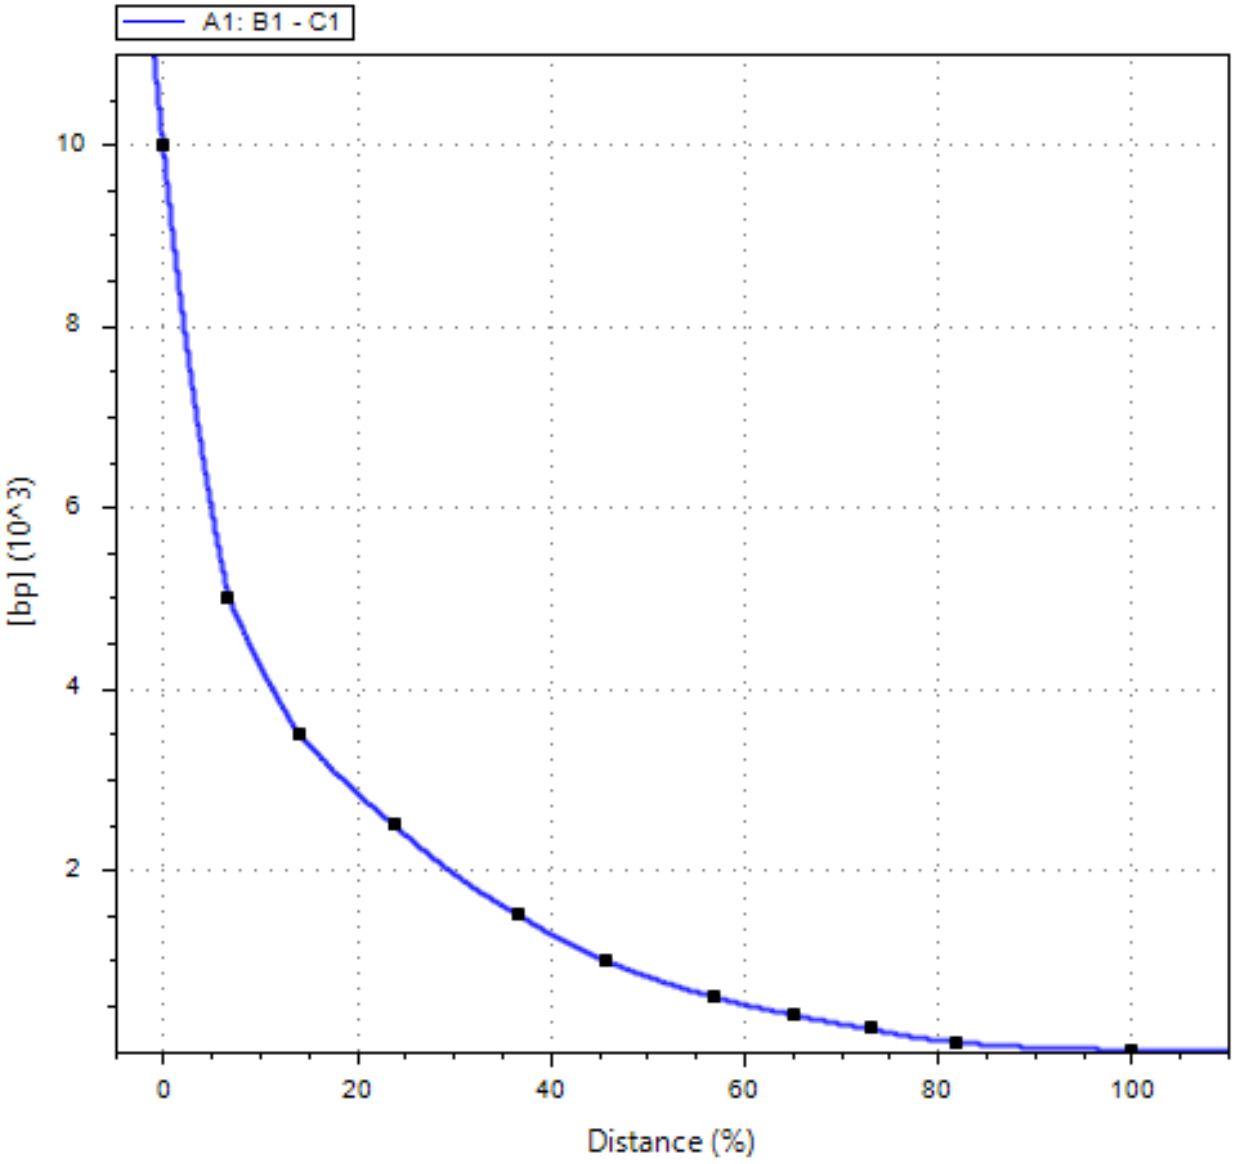

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

© Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2025-07-23\JB_cDNAQC_23Jul2025 - 2025-07-23 - 12.34.44.HSD5000
Assay	HSD5000
Run End Date	2025-07-23T12:42:30-04:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Tapestation 4200B
ScreenTape Device ID	01-S032-241223-01-001610
Expiry Date	2025-08-05T23:59:59
ScreenTape Device History	First run 22 Jul 2025, 2 run(s) performed
Temperature [°C]	26.8
Electrophoresis Time [s]	211
Instrument Type	4200 TapeStation (G2991A)
Instrument Serial Number	DEDAA01484
Notes	2ul
ScreenTape Device Run Date	2025-07-23T12:34:44-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

© Agilent Technologies, Inc. 2023