
Filename: JB_LibQC_30Jul2025 - 2025-07-30 - 11.12.42.D1000

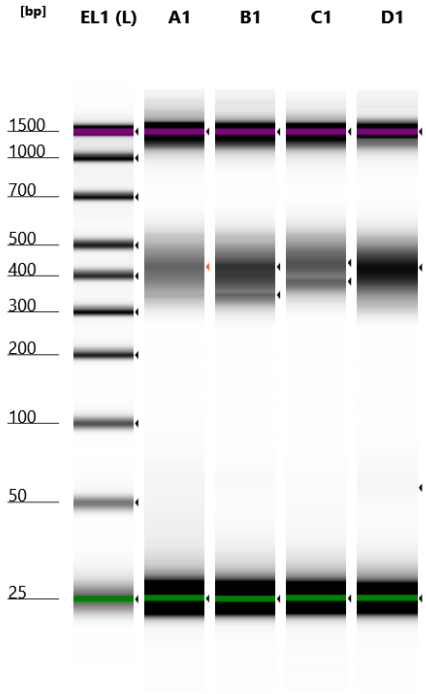

Default image (Contrast 50%), Image is Scaled to Highest Sample Peak

Sample Info

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
EL1	20.3	Electronic Ladder		Ladder
A1	1.51	1		
B1	2.11	2		
C1	1.81	19		
D1	3.04	20		

Compact Peak Table

Well	Sample Description	Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
EL1	Electronic Ladder	25	5.22	-	321	-		Lower Marker
EL1	Electronic Ladder	50	2.25	-	69.3	11.11		
EL1	Electronic Ladder	100	2.37	-	36.5	11.71		
EL1	Electronic Ladder	200	2.47	-	19.0	12.20		
EL1	Electronic Ladder	300	2.55	-	13.1	12.56		
EL1	Electronic Ladder	400	2.57	-	9.87	12.66		
EL1	Electronic Ladder	500	2.71	-	8.33	13.36		
EL1	Electronic Ladder	700	2.46	-	5.41	12.15		
EL1	Electronic Ladder	1000	2.89	-	4.44	14.25		
EL1	Electronic Ladder	1500	6.50	6.50	6.67	-		Upper Marker
A1	1	25	6.39	-	393	-		Lower Marker
A1	1	430	1.51	-	5.41	100.00		
A1	1	1500	6.50	6.50	6.67	-		Upper Marker
B1	2	25	6.21	-	382	-		Lower Marker
B1	2	348	0.426	-	1.88	20.21		
B1	2	430	1.68	-	6.00	79.79		
B1	2	1500	6.50	6.50	6.67	-		Upper Marker
C1	19	25	6.18	-	380	-		Lower Marker
C1	19	384	0.550	-	2.20	30.42		
C1	19	443	1.26	-	4.37	69.58		
C1	19	1500	6.50	6.50	6.67	-		Upper Marker
D1	20	25	6.37	-	392	-		Lower Marker
D1	20	59	0.0312	-	0.813	1.03		
D1	20	427	3.01	-	10.8	98.97		
D1	20	1500	6.50	6.50	6.67	-		Upper Marker


© Agilent Technologies, Inc. 2023

Compact Region Table


WellId	Sample Description	From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
A1	1	150	900	431	1.57	5.82	55.60		
B1	2	150	900	419	2.15	8.18	67.86		
C1	19	150	900	442	1.87	6.73	64.35		
D1	20	150	900	423	3.13	11.7	73.33		

© Agilent Technologies, Inc. 2023


EL1: Electronic Ladder




A1: 1




B1: 2



C1: 19




D1: 20



© Agilent Technologies, Inc. 2023

EL1: Electronic Ladder

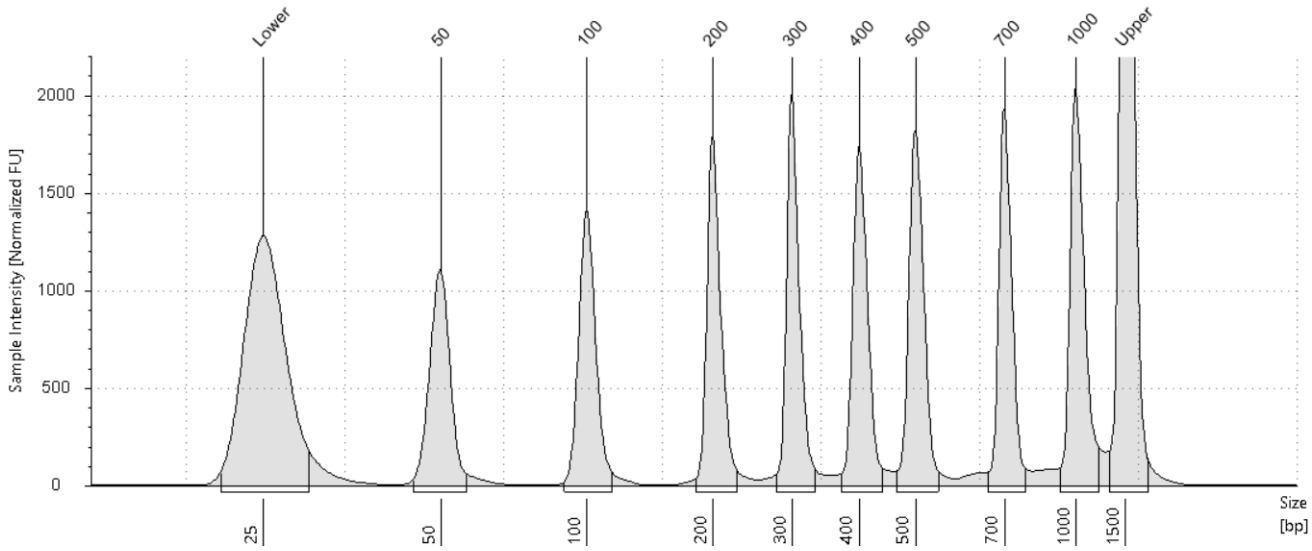

Sample Table


Well	Conc. [ng/µl]	Sample Description	Alert	Observations
EL1	20.3	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.22	-	321	-		Lower Marker
50	2.25	-	69.3	11.11		
100	2.37	-	36.5	11.71		
200	2.47	-	19.0	12.20		
300	2.55	-	13.1	12.56		
400	2.57	-	9.87	12.66		
500	2.71	-	8.33	13.36		
700	2.46	-	5.41	12.15		
1000	2.89	-	4.44	14.25		
1500	6.50	6.50	6.67	-		Upper Marker

© Agilent Technologies, Inc. 2023

A1: 1

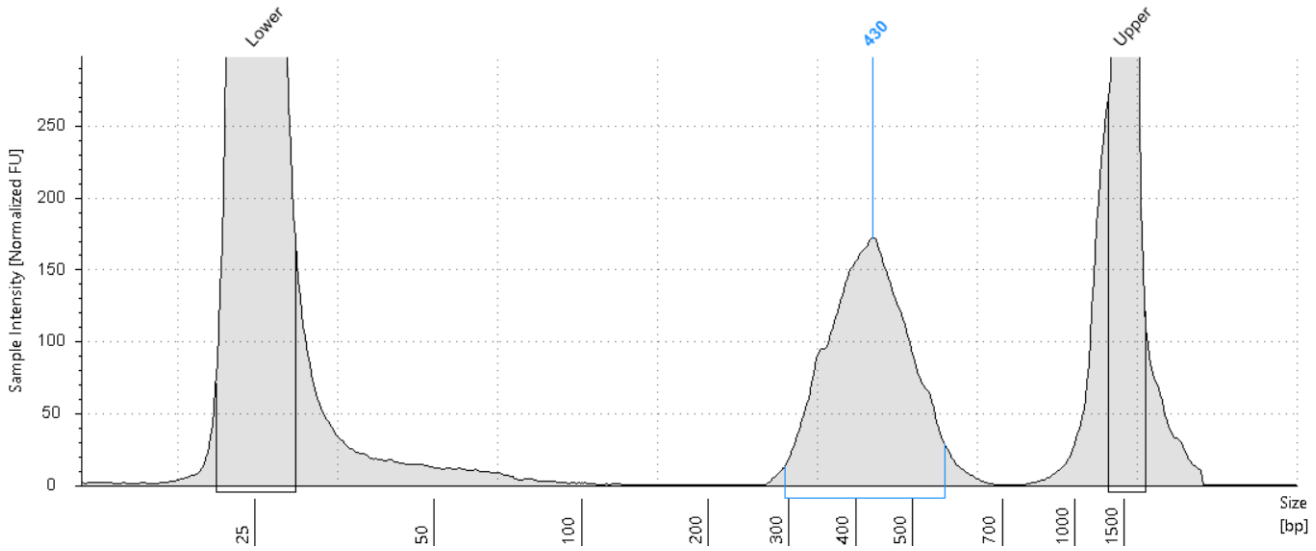


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	1.51	1		

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.39	-	393	-		Lower Marker
430	1.51	-	5.41	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

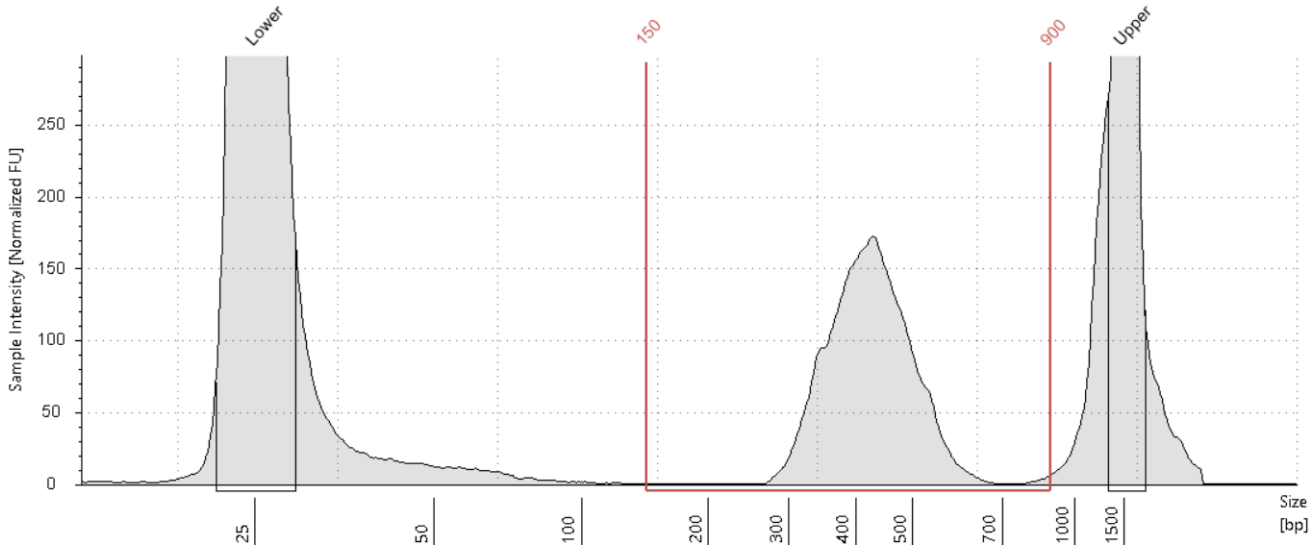


Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
150	900	431	1.57	5.82	55.60		

© Agilent Technologies, Inc. 2023

B1: 2

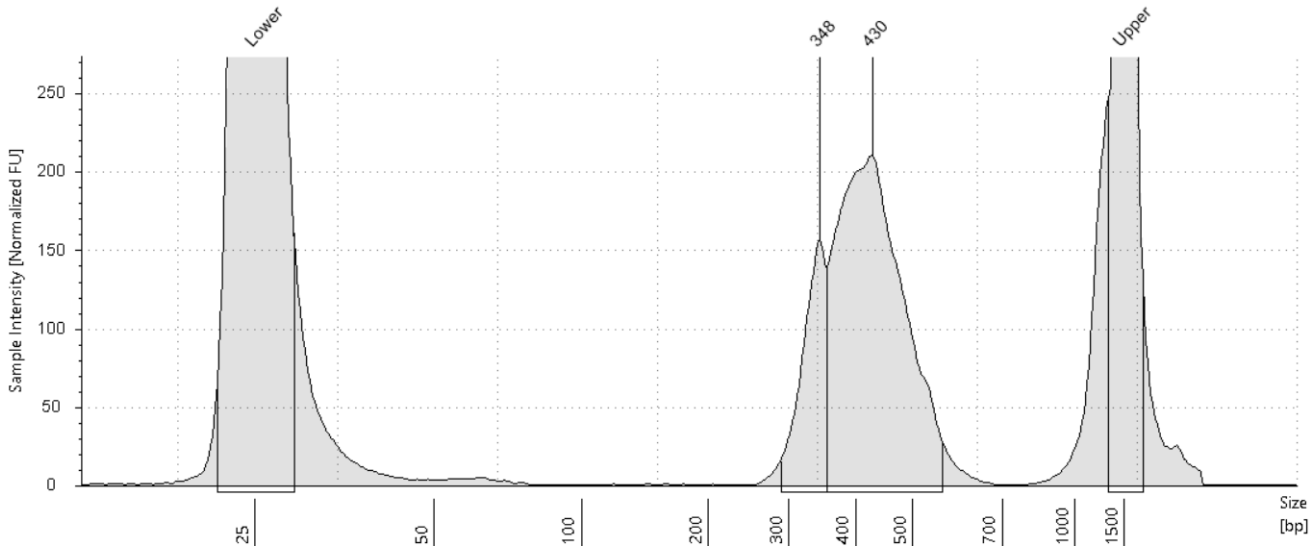


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
B1	2.11	2		

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.21	-	382	-		Lower Marker
348	0.426	-	1.88	20.21		
430	1.68	-	6.00	79.79		
1500	6.50	6.50	6.67	-		Upper Marker

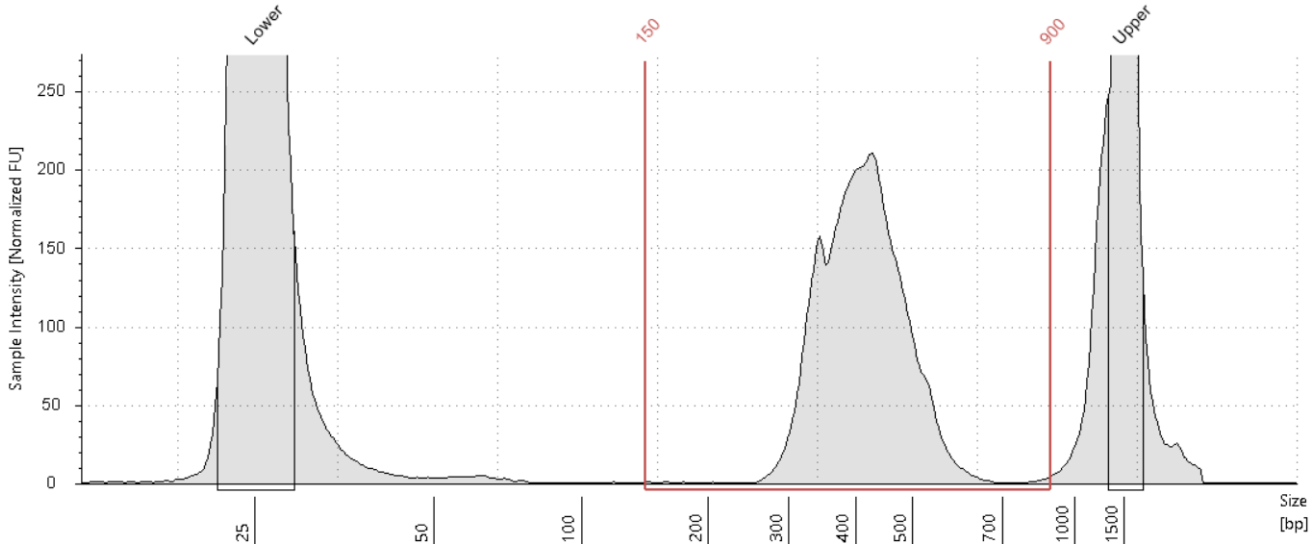


Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
150	900	419	2.15	8.18	67.86		

© Agilent Technologies, Inc. 2023

C1: 19

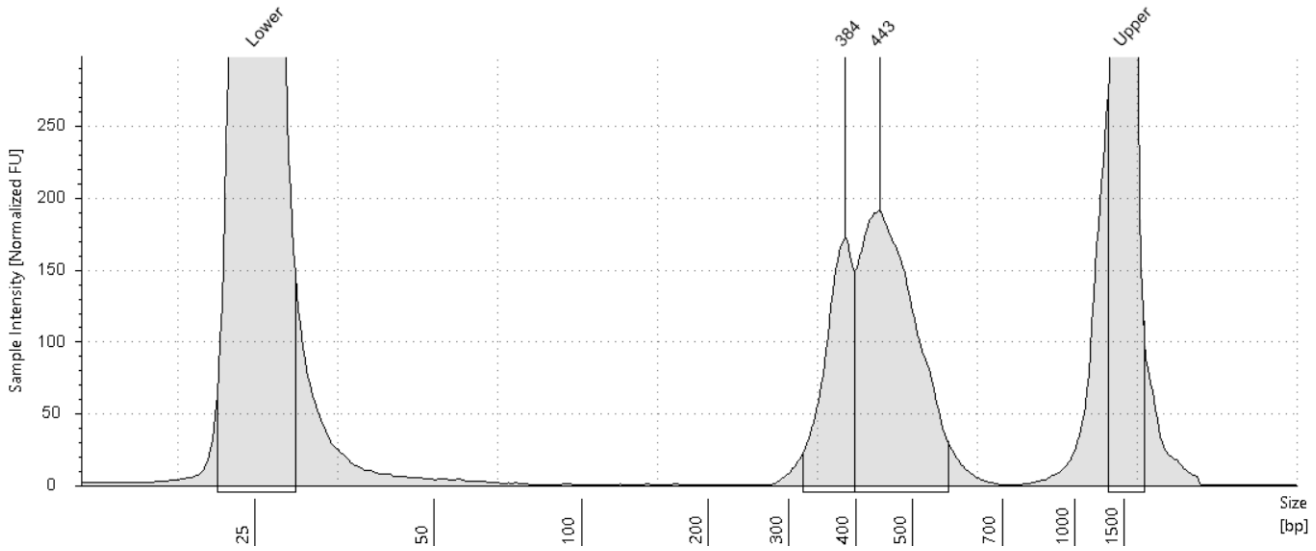


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	1.81	19		

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.18	-	380	-		Lower Marker
384	0.550	-	2.20	30.42		
443	1.26	-	4.37	69.58		
1500	6.50	6.50	6.67	-		Upper Marker

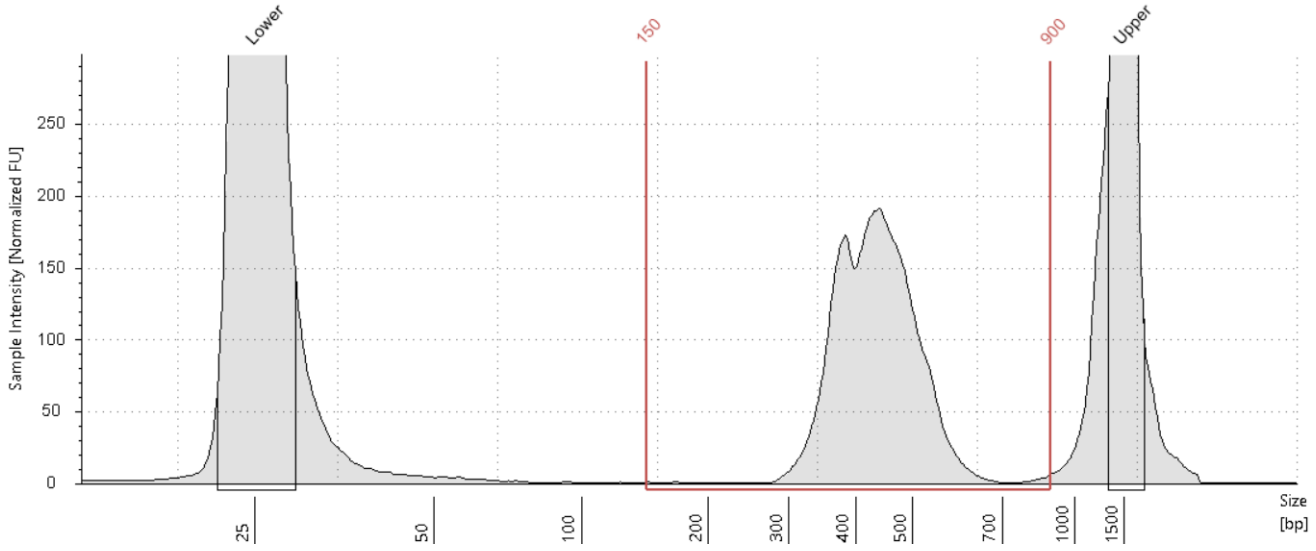


Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
150	900	442	1.87	6.73	64.35		

© Agilent Technologies, Inc. 2023

D1: 20

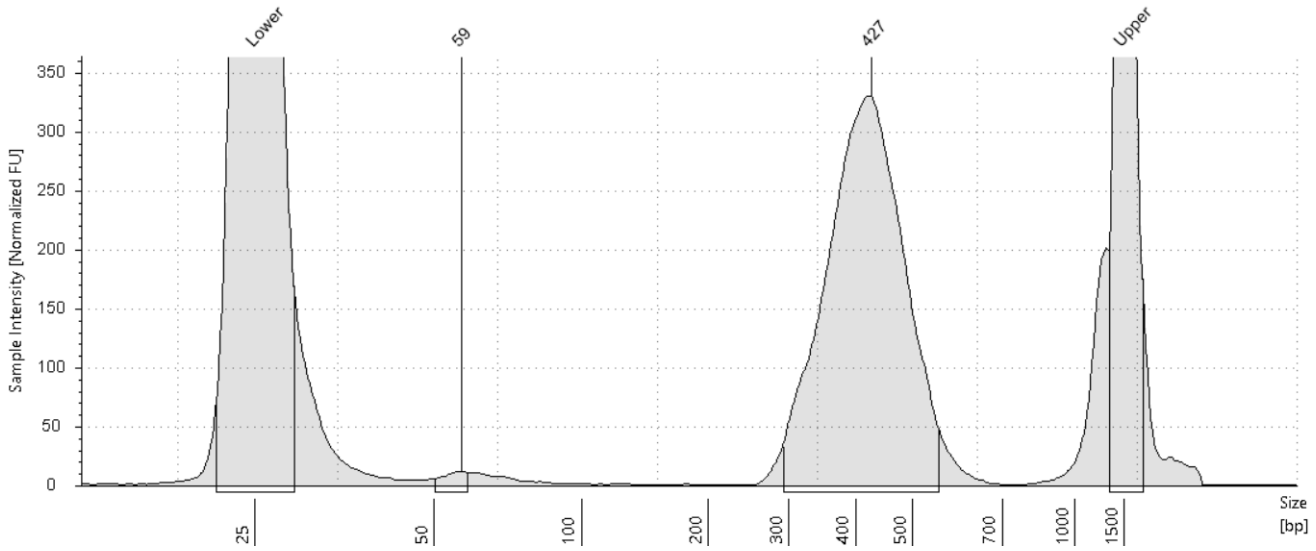


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D1	3.04	20		

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.37	-	392	-		Lower Marker
59	0.0312	-	0.813	1.03		
427	3.01	-	10.8	98.97		
1500	6.50	6.50	6.67	-		Upper Marker

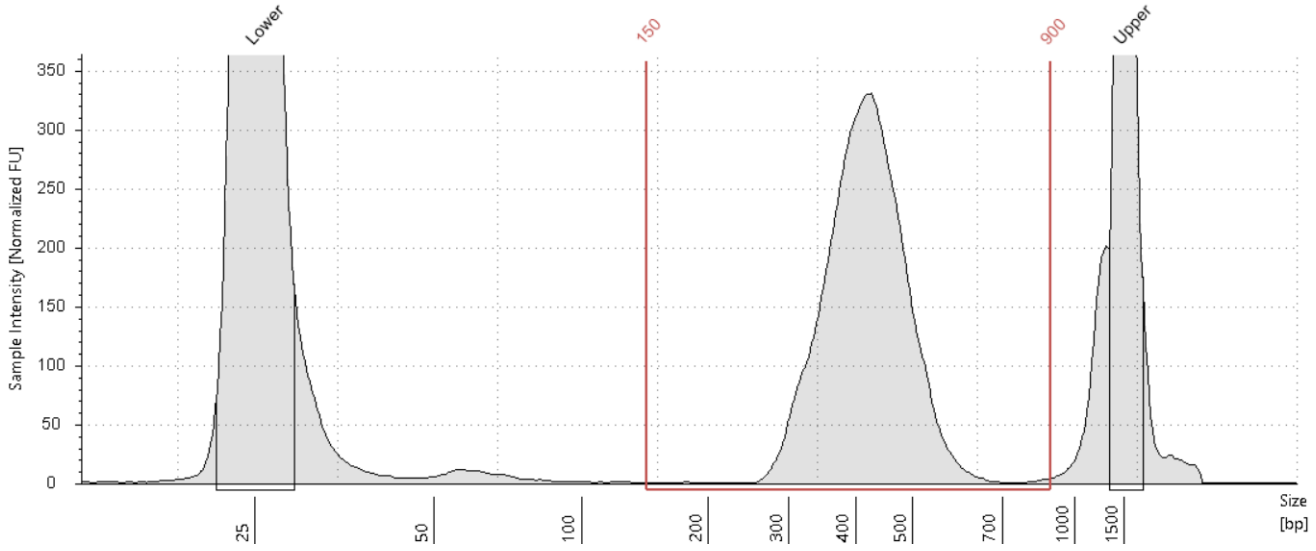

Region Table


From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
150	900	423	3.13	11.7	73.33		

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Piecewise Interpolation
Alignment type: Between markers

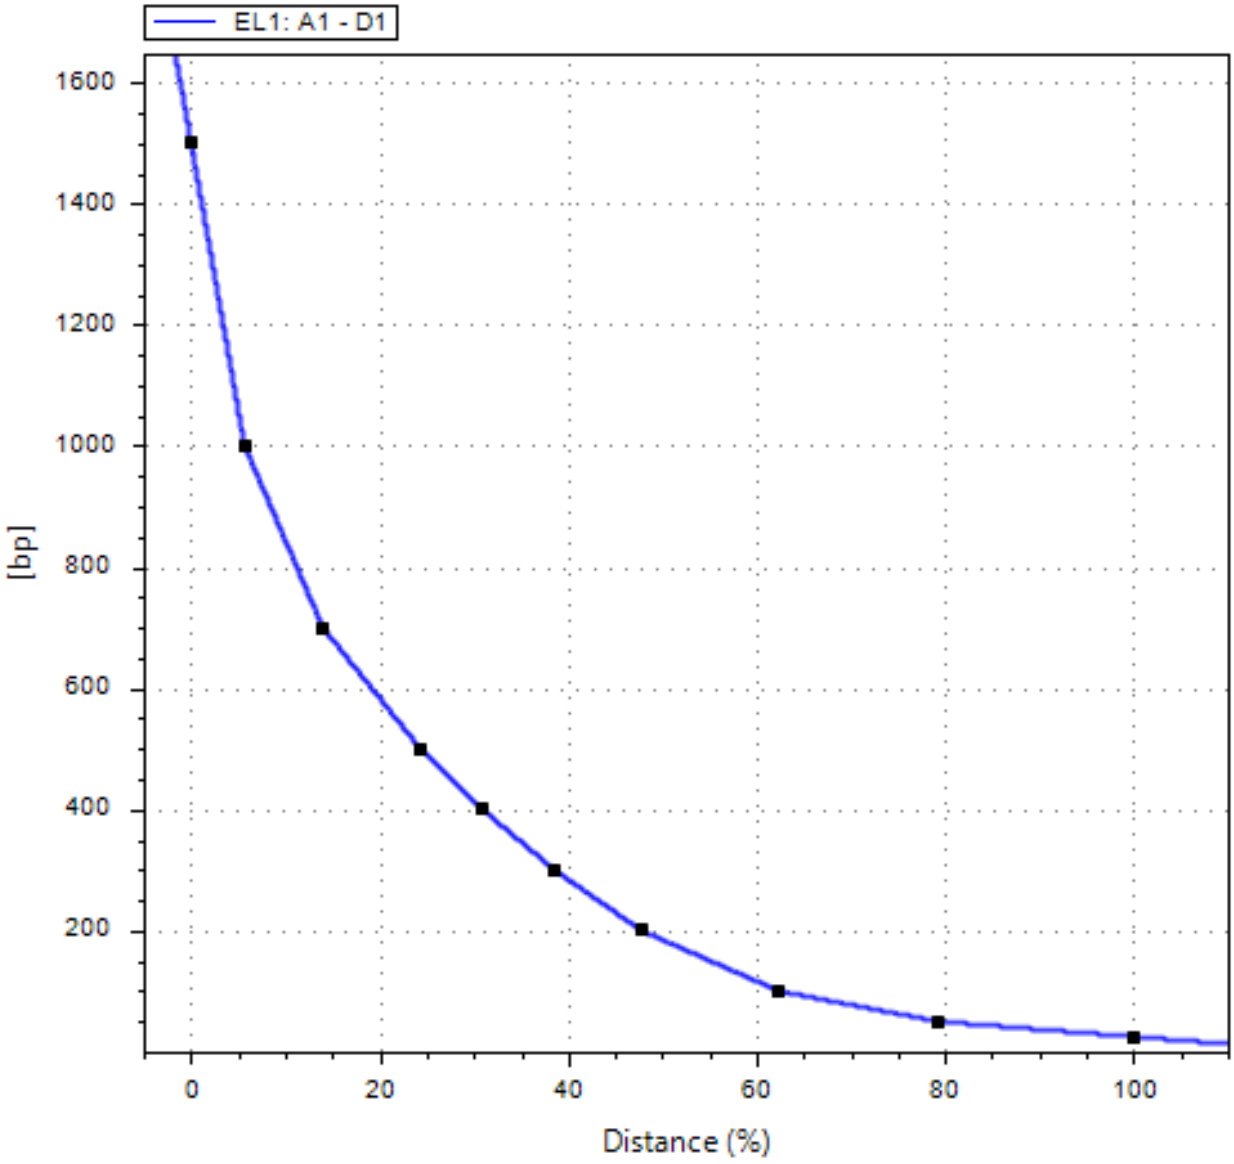

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

 © Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2025-07-30\JB_LibQC_30Jul2025 - 2025-07-30 - 11.12.42.D1000
Assay	D1000
Run End Date	2025-07-30T11:18:58-04:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Tapestation 4200B
ScreenTape Device ID	01-S029-250430-01-000101
Expiry Date	2025-08-11T23:59:59
ScreenTape Device History	First run 28 Jul 2025, 2 run(s) performed
Temperature [°C]	27
Electrophoresis Time [s]	140
Instrument Type	4200 TapeStation (G2991A)
Instrument Serial Number	DEDAA01484
Notes	1ul
ScreenTape Device Run Date	2025-07-30T11:12:42-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

 © Agilent Technologies, Inc. 2023