

Filename: Briseno_15May25 - 2025-05-15 - 09.37.28.HSD5000

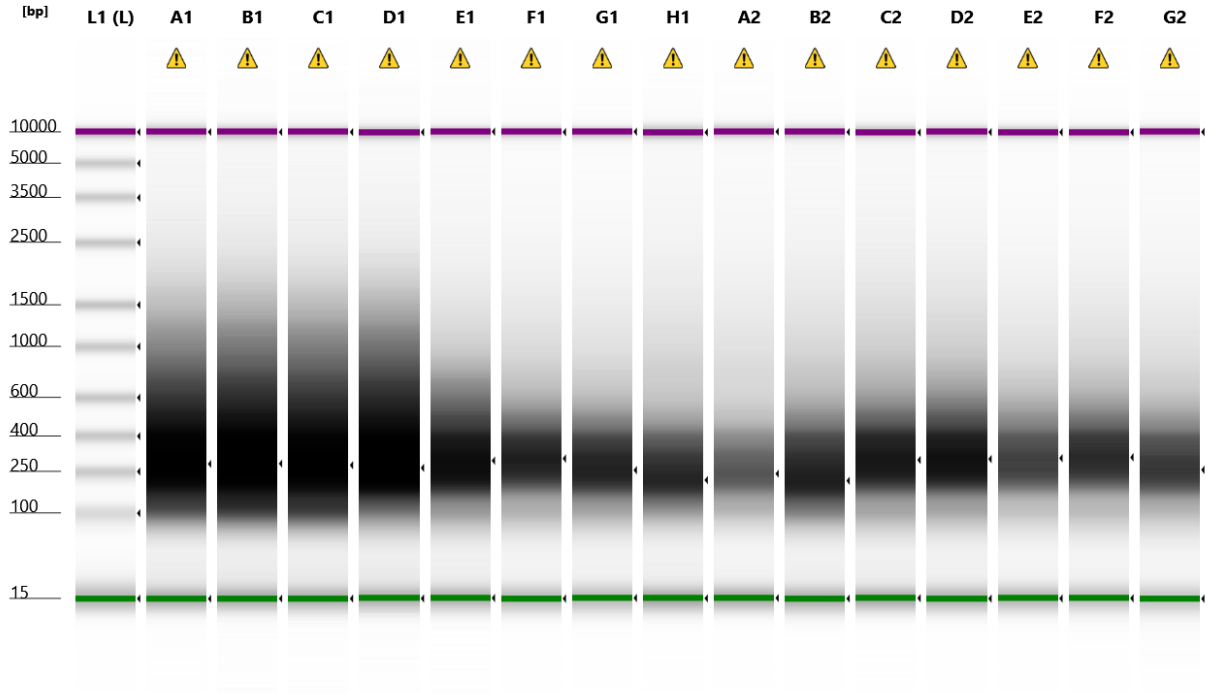

Default image (Contrast 100%)

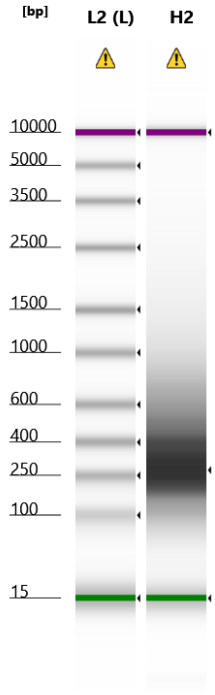

Default image (Contrast 100%)

Sample Info

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
L1	1440	Ladder		Ladder
A1	12800	SL1	⚠	Sample concentration outside recommended range

© Agilent Technologies, Inc. 2023

B1	14500	SL2	⚠	Sample concentration outside recommended range
C1	14200	SL3	⚠	Sample concentration outside recommended range
D1	13800	SL4	⚠	Sample concentration outside recommended range
E1	5960	SL5	⚠	Sample concentration outside recommended range
F1	6080	SL6	⚠	Sample concentration outside recommended range
G1	6350	SL7	⚠	Sample concentration outside recommended range
H1	4850	SL8	⚠	Sample concentration outside recommended range
A2	3250	SL9	⚠	Sample concentration outside recommended range
B2	6340	SL10	⚠	Sample concentration outside recommended range
C2	6690	SL11	⚠	Sample concentration outside recommended range
D2	7210	SL12	⚠	Sample concentration outside recommended range
E2	4410	SL13	⚠	Sample concentration outside recommended range
F2	5500	SL14	⚠	Sample concentration outside recommended range
G2	4920	SL15	⚠	Sample concentration outside recommended range
L2	2370	Ladder	⚠	Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
H2	5580	SL16	⚠	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

Compact Peak Table

Well	Sample Description	Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
L1	Ladder	15	397	-	40700	-		Lower Marker
L1	Ladder	100	167	-	2570	11.63		
L1	Ladder	250	176	-	1080	12.27		
L1	Ladder	400	171	-	659	11.93		
L1	Ladder	600	166	-	426	11.55		
L1	Ladder	1000	159	-	245	11.08		
L1	Ladder	1500	164	-	169	11.44		
L1	Ladder	2500	146	-	89.7	10.14		
L1	Ladder	3500	144	-	63.5	10.05		
L1	Ladder	5000	142	-	43.8	9.91		
L1	Ladder	10000	180	180	27.7	-		Upper Marker
A1	SL1	15	319	-	32700	-		Lower Marker
A1	SL1	277	12800	-	71200	100.00		
A1	SL1	10000	180	180	27.7	-		Upper Marker
B1	SL2	15	331	-	33900	-		Lower Marker
B1	SL2	278	14500	-	80500	100.00		
B1	SL2	10000	180	180	27.7	-		Upper Marker
C1	SL3	15	328	-	33600	-		Lower Marker
C1	SL3	272	14200	-	80200	100.00		
C1	SL3	10000	180	180	27.7	-		Upper Marker
D1	SL4	15	289	-	29600	-		Lower Marker
D1	SL4	262	13800	-	80700	100.00		
D1	SL4	10000	180	180	27.7	-		Upper Marker
E1	SL5	15	356	-	36500	-		Lower Marker
E1	SL5	287	5960	-	32000	100.00		
E1	SL5	10000	180	180	27.7	-		Upper Marker
F1	SL6	15	351	-	36000	-		Lower Marker
F1	SL6	297	6080	-	31500	100.00		
F1	SL6	10000	180	180	27.7	-		Upper Marker
G1	SL7	15	343	-	35200	-		Lower Marker
G1	SL7	253	6350	-	38600	100.00		
G1	SL7	10000	180	180	27.7	-		Upper Marker
H1	SL8	15	352	-	36100	-		Lower Marker
H1	SL8	207	4850	-	36100	100.00		

© Agilent Technologies, Inc. 2023


H1	SL8	10000	180	180	27.7	-		Upper Marker
A2	SL9	15	376	-	38600	-		Lower Marker
A2	SL9	236	3250	-	21200	100.00		
A2	SL9	10000	180	180	27.7	-		Upper Marker
B2	SL10	15	358	-	36700	-		Lower Marker
B2	SL10	204	6340	-	47700	100.00		
B2	SL10	10000	180	180	27.7	-		Upper Marker
C2	SL11	15	357	-	36600	-		Lower Marker
C2	SL11	291	6690	-	35400	100.00		
C2	SL11	10000	180	180	27.7	-		Upper Marker
D2	SL12	15	341	-	34900	-		Lower Marker
D2	SL12	295	7210	-	37600	100.00		
D2	SL12	10000	180	180	27.7	-		Upper Marker
E2	SL13	15	352	-	36100	-		Lower Marker
E2	SL13	298	4410	-	22800	100.00		
E2	SL13	10000	180	180	27.7	-		Upper Marker
F2	SL14	15	302	-	31000	-		Lower Marker
F2	SL14	302	5500	-	28100	100.00		
F2	SL14	10000	180	180	27.7	-		Upper Marker
G2	SL15	15	290	-	29700	-		Lower Marker
G2	SL15	256	4920	-	29600	100.00		
G2	SL15	10000	180	180	27.7	-		Upper Marker
L2	Ladder	15	470	-	48200	-		Lower Marker
L2	Ladder	100	282	-	4340	11.89		
L2	Ladder	250	304	-	1870	12.84		
L2	Ladder	400	306	-	1180	12.92		
L2	Ladder	600	285	-	732	12.03		
L2	Ladder	1000	269	-	413	11.33		
L2	Ladder	1500	265	-	272	11.17		
L2	Ladder	2500	226	-	139	9.52		
L2	Ladder	3500	220	-	96.8	9.29		
L2	Ladder	5000	213	-	65.6	8.99		
L2	Ladder	10000	180	180	27.7	-		Upper Marker
H2	SL16	15	315	-	32300	-		Lower Marker
H2	SL16	270	5580	-	31800	100.00		
H2	SL16	10000	180	180	27.7	-		Upper Marker

Compact Region Table


WellId	Sample Description	From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
A1	SL1	200	3500	578	14600	54700	81.13		
B1	SL2	200	3500	579	16300	61100	79.87		
C1	SL3	200	3500	575	15900	60200	79.69		
D1	SL4	200	3500	571	17300	65500	83.26		
E1	SL5	200	3500	515	9570	38900	79.25		
F1	SL6	200	3500	511	6720	27900	81.17		
G1	SL7	200	3500	495	6000	25800	75.41		
H1	SL8	200	3500	557	4590	19300	70.19		
A2	SL9	200	3500	583	3340	13600	72.63		
B2	SL10	200	3500	546	5940	24600	69.25		
C2	SL11	200	3500	548	7580	30500	80.88		
D2	SL12	200	3500	530	8190	33200	82.47		
E2	SL13	200	3500	527	4910	20000	80.05		
F2	SL14	200	3500	528	6290	25400	82.42		
G2	SL15	200	3500	519	5140	21600	76.74		
H2	SL16	200	3500	522	5900	23800	79.88		

© Agilent Technologies, Inc. 2023


L1: Ladder




A1: SL1




B1: SL2




C1: SL3




D1: SL4




E1: SL5




F1: SL6




G1: SL7




H1: SL8




A2: SL9




B2: SL10




C2: SL11




D2: SL12




E2: SL13




F2: SL14




G2: SL15



L2: Ladder




H2: SL16



© Agilent Technologies, Inc. 2023

Peak: L1: Ladder

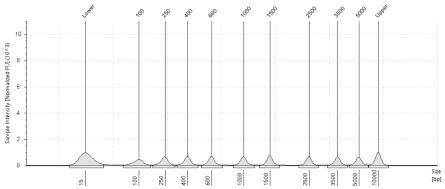


Location	L1
Concentration	1440
Description	Ladder
Observations	Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	397	-	40700	-		Lower Marker
100	167	-	2570	11.63		
250	176	-	1080	12.27		
400	171	-	659	11.93		
600	166	-	426	11.55		
1000	159	-	245	11.08		
1500	164	-	169	11.44		
2500	146	-	89.7	10.14		
3500	144	-	63.5	10.05		
5000	142	-	43.8	9.91		

Peak: L1: Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
10000	180	180	27.7	-		Upper Marker


Peak: A1: SL1

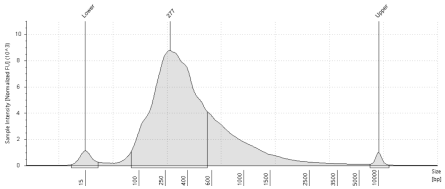

Location	A1
Concentration	12800
Description	SL1
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	319	-	32700	-		Lower Marker
277	12800	-	71200	100.00		
10000	180	180	27.7	-		Upper Marker

Region: A1: SL1

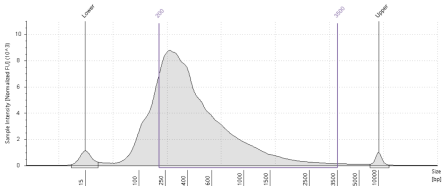


Location	A1
Concentration	12800
Description	SL1
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	578	14600	54700	81.13		

© Agilent Technologies, Inc. 2023


Peak: B1: SL2

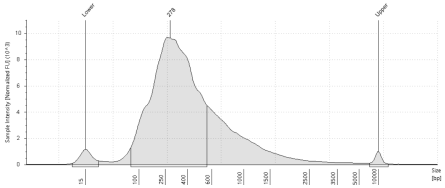

Location	B1
Concentration	14500
Description	SL2
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	331	-	33900	-		Lower Marker
278	14500	-	80500	100.00		
10000	180	180	27.7	-		Upper Marker


Region: B1: SL2

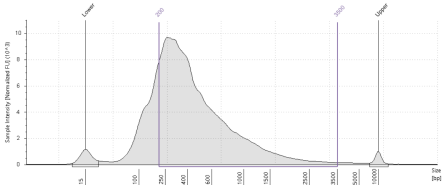

Location	B1
Concentration	14500
Description	SL2
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	579	16300	61100	79.87		


Peak: C1: SL3

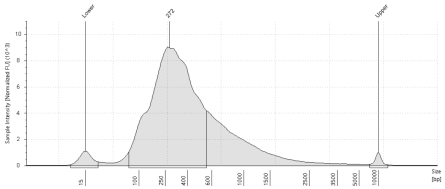

Location	C1
Concentration	14200
Description	SL3
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	328	-	33600	-		Lower Marker
272	14200	-	80200	100.00		
10000	180	180	27.7	-		Upper Marker

Region: C1: SL3

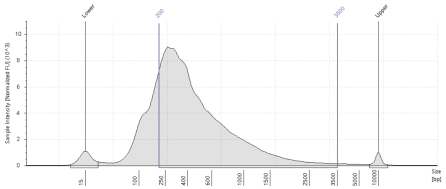


Location	C1
Concentration	14200
Description	SL3
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	575	15900	60200	79.69		

© Agilent Technologies, Inc. 2023


Peak: D1: SL4

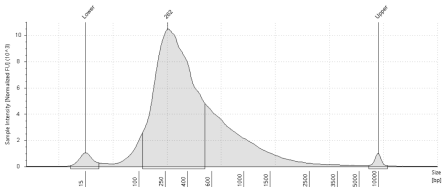

Location	D1
Concentration	13800
Description	SL4
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	289	-	29600	-		Lower Marker
262	13800	-	80700	100.00		
10000	180	180	27.7	-		Upper Marker


Region: D1: SL4

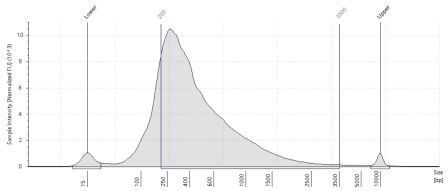

Location	D1
Concentration	13800
Description	SL4
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	571	17300	65500	83.26		


Peak: E1: SL5

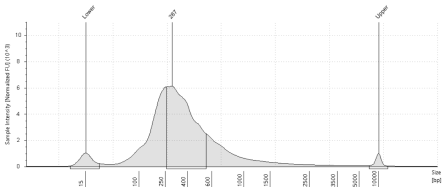

Location	E1
Concentration	5960
Description	SL5
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	356	-	36500	-		Lower Marker
287	5960	-	32000	100.00		
10000	180	180	27.7	-		Upper Marker

Region: E1: SL5

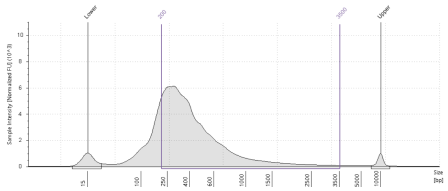


Location	E1
Concentration	5960
Description	SL5
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	515	9570	38900	79.25		

© Agilent Technologies, Inc. 2023


Peak: F1: SL6

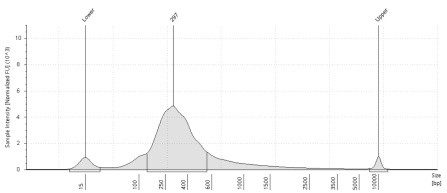

Location	F1
Concentration	6080
Description	SL6
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	351	-	36000	-		Lower Marker
297	6080	-	31500	100.00		
10000	180	180	27.7	-		Upper Marker


Region: F1: SL6

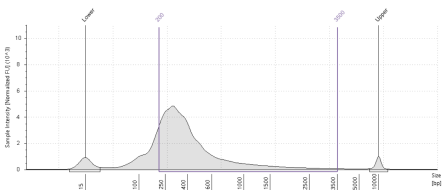

Location	F1
Concentration	6080
Description	SL6
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	511	6720	27900	81.17		


Peak: G1: SL7

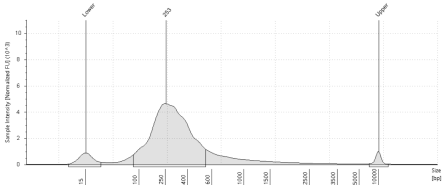

Location	G1
Concentration	6350
Description	SL7
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	343	-	35200	-		Lower Marker
253	6350	-	38600	100.00		
10000	180	180	27.7	-		Upper Marker

Region: G1: SL7

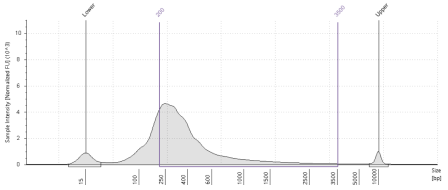


Location	G1
Concentration	6350
Description	SL7
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	495	6000	25800	75.41		

© Agilent Technologies, Inc. 2023


Peak: H1: SL8

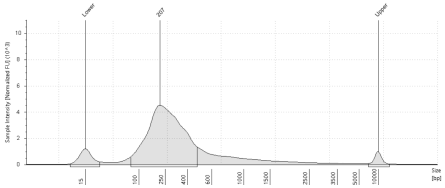

Location	H1
Concentration	4850
Description	SL8
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	352	-	36100	-		Lower Marker
207	4850	-	36100	100.00		
10000	180	180	27.7	-		Upper Marker


Region: H1: SL8

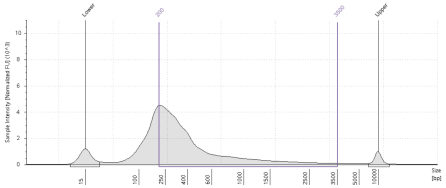

Location	H1
Concentration	4850
Description	SL8
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	557	4590	19300	70.19		


Peak: A2: SL9

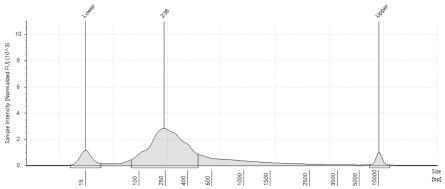

Location	A2
Concentration	3250
Description	SL9
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	376	-	38600	-		Lower Marker
236	3250	-	21200	100.00		
10000	180	180	27.7	-		Upper Marker

Region: A2: SL9

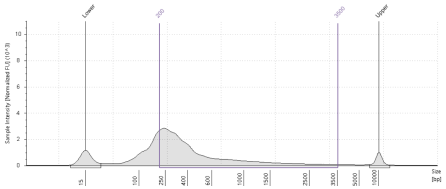


Location	A2
Concentration	3250
Description	SL9
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	583	3340	13600	72.63		

© Agilent Technologies, Inc. 2023


Peak: B2: SL10

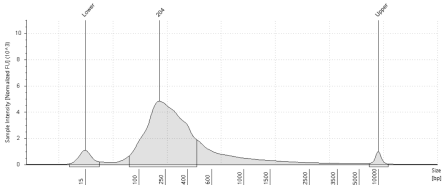

Location	B2
Concentration	6340
Description	SL10
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	358	-	36700	-		Lower Marker
204	6340	-	47700	100.00		
10000	180	180	27.7	-		Upper Marker


Region: B2: SL10

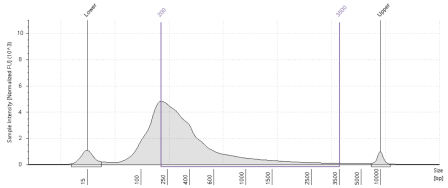

Location	B2
Concentration	6340
Description	SL10
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	546	5940	24600	69.25		


Peak: C2: SL11

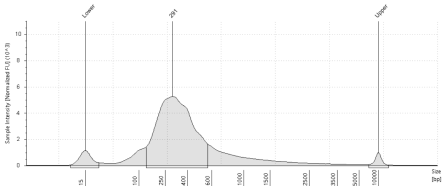

Location	C2
Concentration	6690
Description	SL11
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	357	-	36600	-		Lower Marker
291	6690	-	35400	100.00		
10000	180	180	27.7	-		Upper Marker

Region: C2: SL11

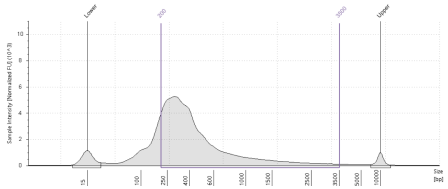


Location	C2
Concentration	6690
Description	SL11
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	548	7580	30500	80.88		

© Agilent Technologies, Inc. 2023


Peak: D2: SL12

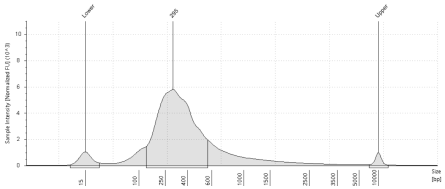

Location	D2
Concentration	7210
Description	SL12
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	341	-	34900	-		Lower Marker
295	7210	-	37600	100.00		
10000	180	180	27.7	-		Upper Marker


Region: D2: SL12

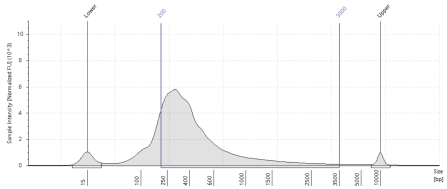

Location	D2
Concentration	7210
Description	SL12
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	530	8190	33200	82.47		


Peak: E2: SL13

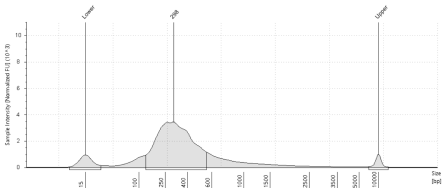

Location	E2
Concentration	4410
Description	SL13
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	352	-	36100	-		Lower Marker
298	4410	-	22800	100.00		
10000	180	180	27.7	-		Upper Marker

Region: E2: SL13

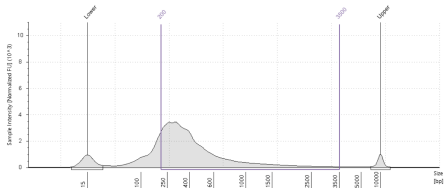


Location	E2
Concentration	4410
Description	SL13
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	527	4910	20000	80.05		

© Agilent Technologies, Inc. 2023


Peak: F2: SL14

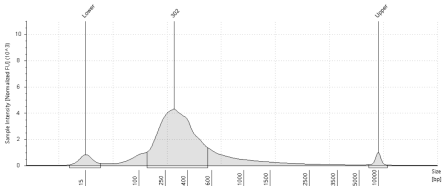

Location	F2
Concentration	5500
Description	SL14
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	302	-	31000	-		Lower Marker
302	5500	-	28100	100.00		
10000	180	180	27.7	-		Upper Marker


Region: F2: SL14

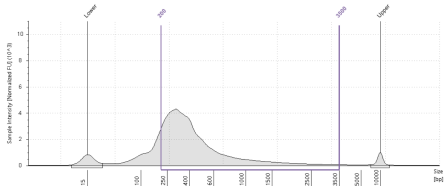

Location	F2
Concentration	5500
Description	SL14
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	528	6290	25400	82.42		


Peak: G2: SL15

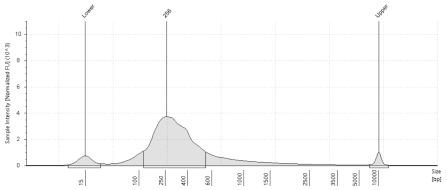

Location	G2
Concentration	4920
Description	SL15
Alert	⚠
Observations	Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	290	-	29700	-		Lower Marker
256	4920	-	29600	100.00		
10000	180	180	27.7	-		Upper Marker

Region: G2: SL15

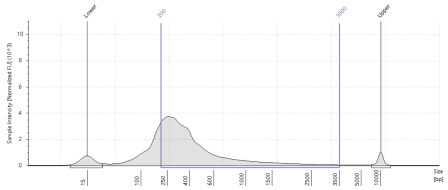


Location	G2
Concentration	4920
Description	SL15
Alert	⚠
Observations	Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	519	5140	21600	76.74		

© Agilent Technologies, Inc. 2023

Peak: L2: Ladder

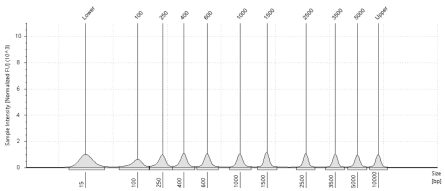


Location L2
Concentration 2370
Description Ladder
Alert ⚠
Observations Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	470	-	48200	-		Lower Marker
100	282	-	4340	11.89		
250	304	-	1870	12.84		
400	306	-	1180	12.92		
600	285	-	732	12.03		
1000	269	-	413	11.33		
1500	265	-	272	11.17		
2500	226	-	139	9.52		
3500	220	-	96.8	9.29		
5000	213	-	65.6	8.99		

Peak: L2: Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
10000	180	180	27.7	-		Upper Marker


Peak: H2: SL16

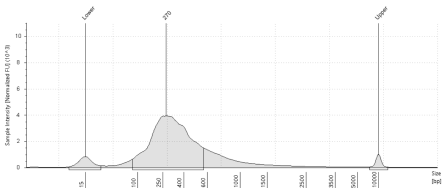

Location H2
Concentration 5580
Description SL16
Alert ⚠
Observations Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	315	-	32300	-		Lower Marker
270	5580	-	31800	100.00		
10000	180	180	27.7	-		Upper Marker

Region: H2: SL16

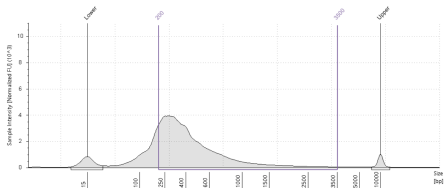

Location H2
Concentration 5580
Description SL16
Alert ⚠
Observations Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/µl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	3500	522	5900	23800	79.88		


© Agilent Technologies, Inc. 2023

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Log Linear Piecewise
Alignment type: Between markers

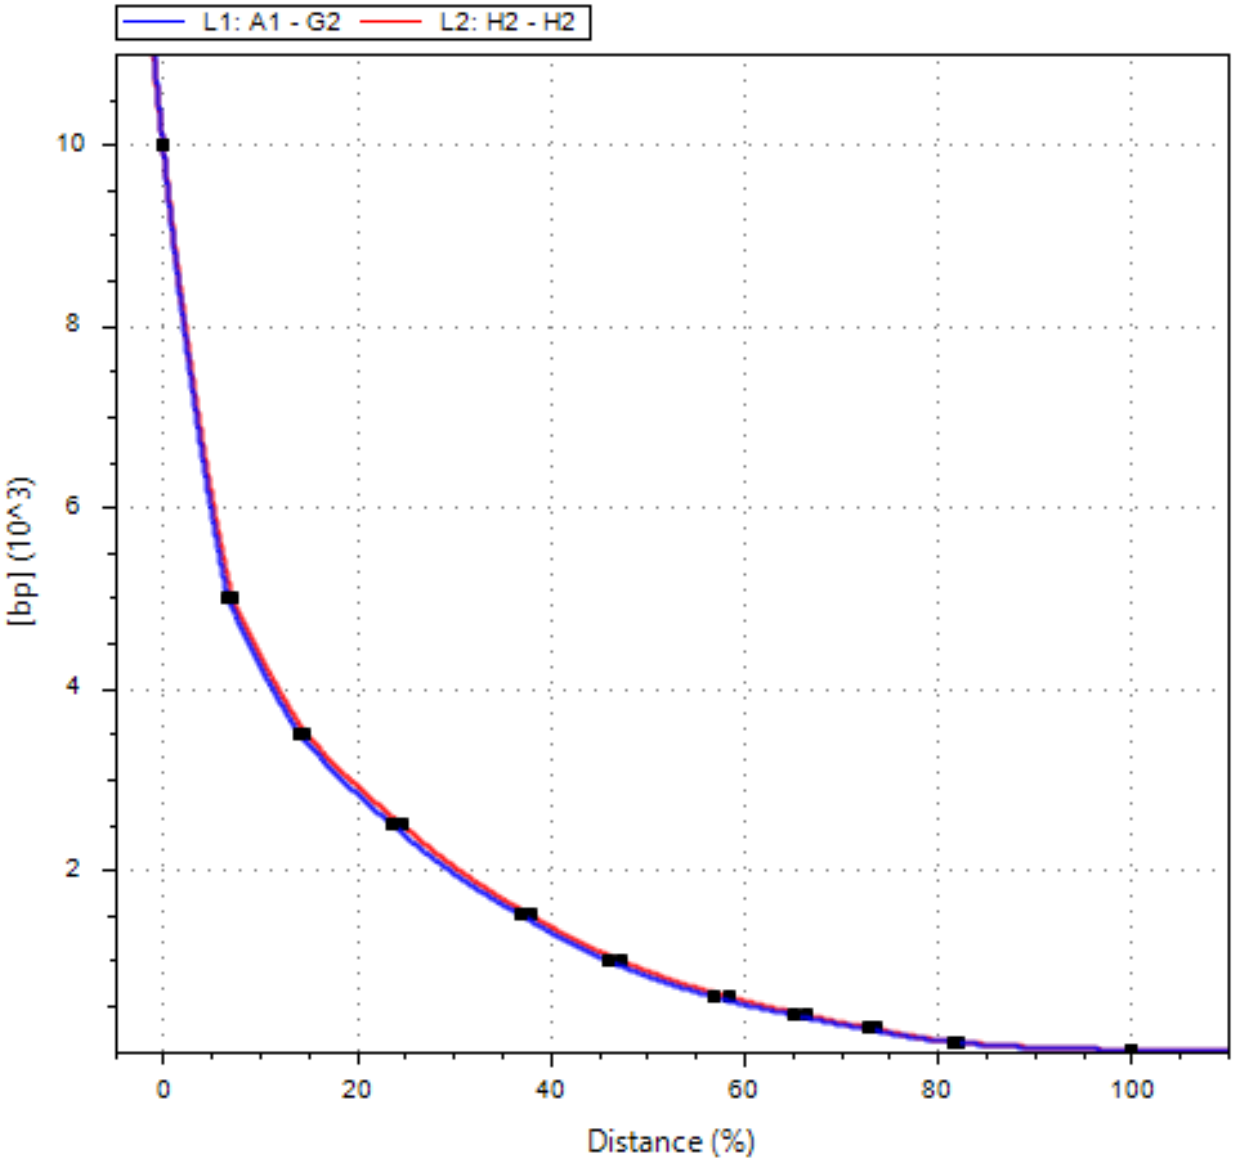

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

© Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2025-05-15\Briseno_15May25 - 2025-05-15 - 09.37.28.HSD5000
Assay	HSD5000
Run End Date	2025-05-15T10:04:20-04:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Tapestation 4200B
ScreenTape Device ID	01-S032-241223-01-002072
Expiry Date	2025-05-29T23:59:59
ScreenTape Device History	First run 15 May 2025, 1 run(s) performed
Temperature [°C]	21.6
Electrophoresis Time [s]	238
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	2ul
ScreenTape Device Run Date	2025-05-15T09:37:28-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

ScreenTape Device 2

Username	Tapestation 4200B
ScreenTape Device ID	01-S032-241223-01-002059
Expiry Date	2025-04-25T23:59:59
ScreenTape Device History	First run 11 Apr 2025, 4 run(s) performed
Temperature [°C]	21.6
Electrophoresis Time [s]	234
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	2ul
ScreenTape Device Run Date	2025-05-15T09:37:28-04:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

© Agilent Technologies, Inc. 2023