

Filename: Briseno_01302026 - 2026-01-30 - 10.46.14.HSD5000

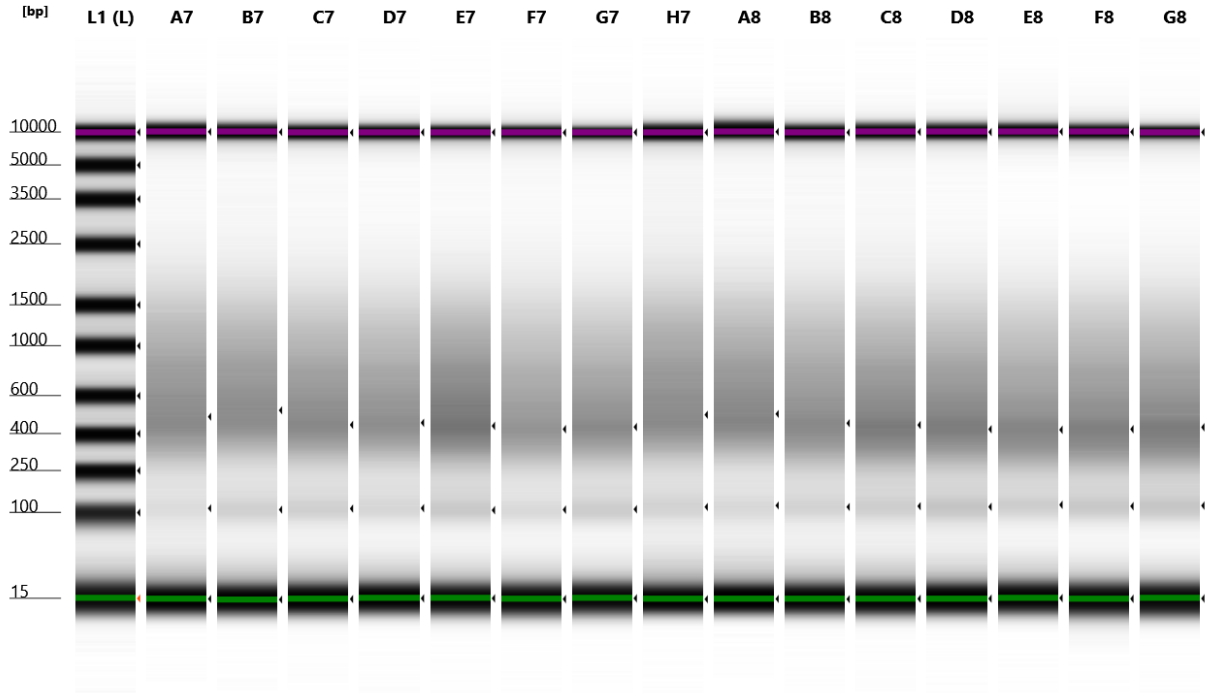

Default image (Contrast 100%)

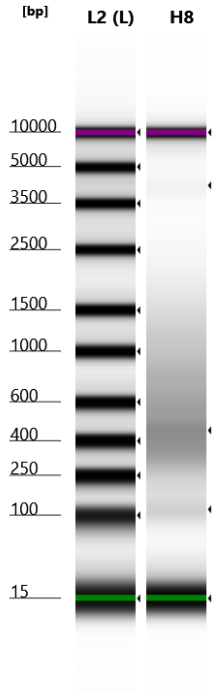

Default image (Contrast 100%)

Sample Info

Well	Conc. [pg/µl]	Sample Description	Alert	Observations
L1	1560	Ladder		Ladder
A7	123	1		
B7	150	2		

© Agilent Technologies, Inc. 2023

C7	154	3		
D7	154	4		
E7	226	5		
F7	166	6		
G7	203	7		
H7	130	8		
A8	66.0	9		
B8	175	10		
C8	208	11		
D8	197	12		
E8	204	13		
F8	221	14		
G8	246	15		
L2	1930	Ladder		Ladder
H8	246	16		

Compact Peak Table


Well	Sample Description	Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
L1	Ladder	15	248	-	25400	-		Lower Marker
L1	Ladder	100	160	-	2460	10.24		
L1	Ladder	250	177	-	1090	11.32		
L1	Ladder	400	180	-	693	11.52		
L1	Ladder	600	175	-	449	11.21		
L1	Ladder	1000	181	-	278	11.55		
L1	Ladder	1500	180	-	185	11.53		
L1	Ladder	2500	170	-	104	10.85		
L1	Ladder	3500	173	-	76.0	11.06		
L1	Ladder	5000	168	-	51.6	10.72		
L1	Ladder	10000	180	180	27.7	-		Upper Marker
A7	1	15	271	-	27800	-		Lower Marker
A7	1	111	7.11	-	98.9	5.78		
A7	1	480	116	-	371	94.22		
A7	1	10000	180	180	27.7	-		Upper Marker
B7	2	15	280	-	28700	-		Lower Marker
B7	2	109	29.1	-	411	19.42		
B7	2	517	121	-	359	80.58		
B7	2	10000	180	180	27.7	-		Upper Marker
C7	3	15	308	-	31600	-		Lower Marker
C7	3	110	29.2	-	407	18.95		
C7	3	442	125	-	435	81.05		
C7	3	10000	180	180	27.7	-		Upper Marker
D7	4	15	312	-	32000	-		Lower Marker
D7	4	110	18.1	-	253	11.75		
D7	4	450	136	-	465	88.25		
D7	4	10000	180	180	27.7	-		Upper Marker
E7	5	15	302	-	30900	-		Lower Marker
E7	5	105	38.3	-	560	16.98		
E7	5	435	187	-	663	83.02		
E7	5	10000	180	180	27.7	-		Upper Marker
F7	6	15	324	-	33300	-		Lower Marker
F7	6	108	25.0	-	357	15.12		
F7	6	422	141	-	512	84.88		
F7	6	10000	180	180	27.7	-		Upper Marker
G7	7	15	338	-	34600	-		Lower Marker
G7	7	107	39.8	-	569	19.55		
G7	7	430	164	-	586	80.45		
G7	7	10000	180	180	27.7	-		Upper Marker
H7	8	15	256	-	26300	-		Lower Marker
H7	8	115	17.4	-	234	13.42		
H7	8	493	113	-	351	86.58		
H7	8	10000	180	180	27.7	-		Upper Marker
A8	9	15	294	-	30100	-		Lower Marker
A8	9	118	14.6	-	192	22.17		
A8	9	495	51.3	-	160	77.83		
A8	9	10000	180	180	27.7	-		Upper Marker
B8	10	15	283	-	29000	-		Lower Marker
B8	10	115	25.9	-	347	14.80		
B8	10	450	149	-	509	85.20		
B8	10	10000	180	180	27.7	-		Upper Marker
C8	11	15	287	-	29400	-		Lower Marker
C8	11	116	29.7	-	396	14.27		

© Agilent Technologies, Inc. 2023

C8	11	439	179	-	626	85.73		
C8	11	10000	180	180	27.7	-		Upper Marker
D8	12	15	305	-	31300	-		Lower Marker
D8	12	114	37.9	-	513	19.26		
D8	12	420	159	-	583	80.74		
D8	12	10000	180	180	27.7	-		Upper Marker
E8	13	15	310	-	31800	-		Lower Marker
E8	13	118	31.2	-	408	15.28		
E8	13	415	173	-	640	84.72		
E8	13	10000	180	180	27.7	-		Upper Marker
F8	14	15	308	-	31600	-		Lower Marker
F8	14	116	38.2	-	509	17.29		
F8	14	420	183	-	669	82.71		
F8	14	10000	180	180	27.7	-		Upper Marker
G8	15	15	337	-	34600	-		Lower Marker
G8	15	117	43.1	-	569	17.49		
G8	15	429	203	-	730	82.51		
G8	15	10000	180	180	27.7	-		Upper Marker
L2	Ladder	15	314	-	32200	-		Lower Marker
L2	Ladder	100	225	-	3460	11.68		
L2	Ladder	250	245	-	1510	12.74		
L2	Ladder	400	244	-	937	12.65		
L2	Ladder	600	225	-	576	11.66		
L2	Ladder	1000	217	-	334	11.27		
L2	Ladder	1500	211	-	216	10.93		
L2	Ladder	2500	187	-	115	9.69		
L2	Ladder	3500	190	-	83.4	9.84		
L2	Ladder	5000	184	-	56.6	9.55		
L2	Ladder	10000	180	180	27.7	-		Upper Marker
H8	16	15	355	-	36400	-		Lower Marker
H8	16	115	37.6	-	505	15.27		
H8	16	446	204	-	702	82.63		
H8	16	4177	5.17	-	1.91	2.10		
H8	16	10000	180	180	27.7	-		Upper Marker

© Agilent Technologies, Inc. 2023

Peak: L1: Ladder

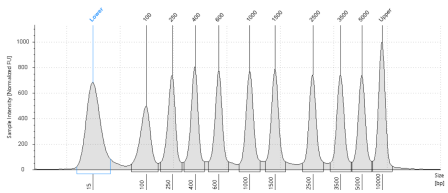


Location	L1
Concentration	1560
Description	Ladder
Observations	Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	248	-	25400	-		Lower Marker
100	160	-	2460	10.24		
250	177	-	1090	11.32		
400	180	-	693	11.52		
600	175	-	449	11.21		
1000	181	-	278	11.55		
1500	180	-	185	11.53		
2500	170	-	104	10.85		
3500	173	-	76.0	11.06		
5000	168	-	51.6	10.72		

Peak: L1: Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
10000	180	180	27.7	-		Upper Marker


Peak: A7: 1

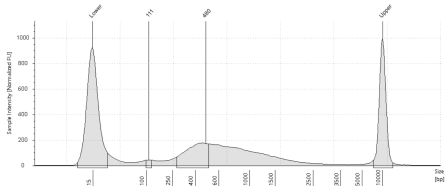

Location	A7
Concentration	123
Description	1
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	271	-	27800	-		Lower Marker
111	7.11	-	98.9	5.78		
480	116	-	371	94.22		
10000	180	180	27.7	-		Upper Marker

Peak: B7: 2

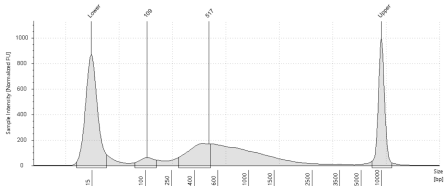


Location	B7
Concentration	150
Description	2
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	280	-	28700	-		Lower Marker
109	29.1	-	411	19.42		
517	121	-	359	80.58		
10000	180	180	27.7	-		Upper Marker

© Agilent Technologies, Inc. 2023


Peak: C7: 3

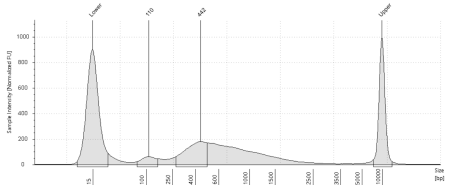

Location	C7
Concentration	154
Description	3
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	308	-	31600	-		Lower Marker
110	29.2	-	407	18.95		
442	125	-	435	81.05		
10000	180	180	27.7	-		Upper Marker


Peak: D7: 4

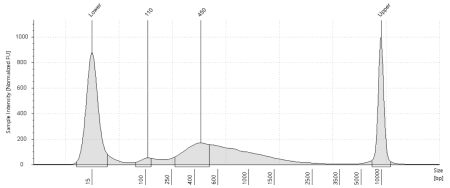

Location	D7
Concentration	154
Description	4
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	312	-	32000	-		Lower Marker
110	18.1	-	253	11.75		
450	136	-	465	88.25		
10000	180	180	27.7	-		Upper Marker


Peak: E7: 5

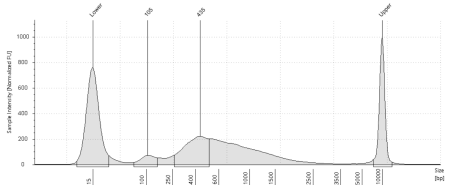

Location	E7
Concentration	226
Description	5
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	302	-	30900	-		Lower Marker
105	38.3	-	560	16.98		
435	187	-	663	83.02		
10000	180	180	27.7	-		Upper Marker

Peak: F7: 6

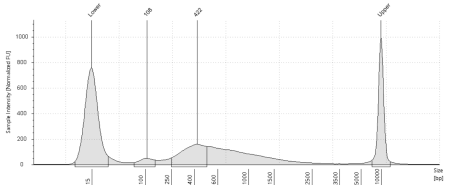


Location	F7
Concentration	166
Description	6
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	324	-	33300	-		Lower Marker
108	25.0	-	357	15.12		
422	141	-	512	84.88		
10000	180	180	27.7	-		Upper Marker

© Agilent Technologies, Inc. 2023


Peak: G7: 7

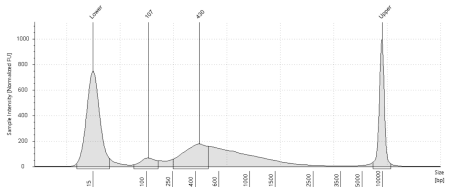

Location	G7
Concentration	203
Description	7
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	338	-	34600	-		Lower Marker
107	39.8	-	569	19.55		
430	164	-	586	80.45		
10000	180	180	27.7	-		Upper Marker


Peak: H7: 8

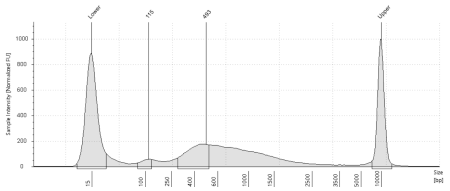

Location	H7
Concentration	130
Description	8
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	256	-	26300	-		Lower Marker
115	17.4	-	234	13.42		
493	113	-	351	86.58		
10000	180	180	27.7	-		Upper Marker


Peak: A8: 9

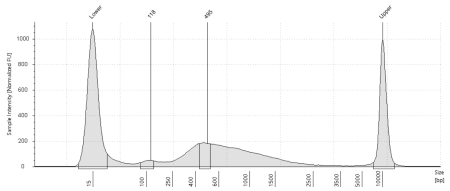

Location	A8
Concentration	66.0
Description	9
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	294	-	30100	-		Lower Marker
118	14.6	-	192	22.17		
495	51.3	-	160	77.83		
10000	180	180	27.7	-		Upper Marker

Peak: B8: 10

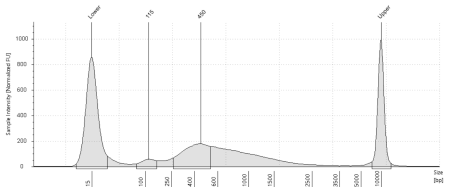


Location	B8
Concentration	175
Description	10
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	283	-	29000	-		Lower Marker
115	25.9	-	347	14.80		
450	149	-	509	85.20		
10000	180	180	27.7	-		Upper Marker

© Agilent Technologies, Inc. 2023


Peak: C8: 11

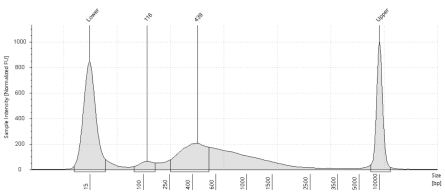

Location	C8
Concentration	208
Description	11
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	287	-	29400	-		Lower Marker
116	29.7	-	396	14.27		
439	179	-	626	85.73		
10000	180	180	27.7	-		Upper Marker


Peak: D8: 12

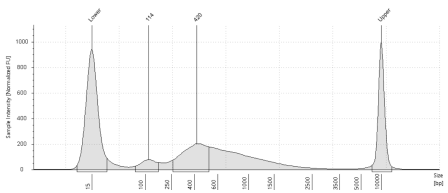

Location	D8
Concentration	197
Description	12
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	305	-	31300	-		Lower Marker
114	37.9	-	513	19.26		
420	159	-	583	80.74		
10000	180	180	27.7	-		Upper Marker


Peak: E8: 13

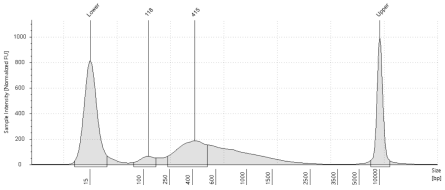

Location	E8
Concentration	204
Description	13
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	310	-	31800	-		Lower Marker
118	31.2	-	408	15.28		
415	173	-	640	84.72		
10000	180	180	27.7	-		Upper Marker

Peak: F8: 14

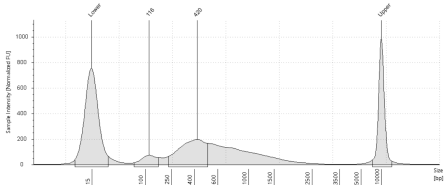


Location	F8
Concentration	221
Description	14
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	308	-	31600	-		Lower Marker
116	38.2	-	509	17.29		
420	183	-	669	82.71		
10000	180	180	27.7	-		Upper Marker

© Agilent Technologies, Inc. 2023


Peak: G8: 15

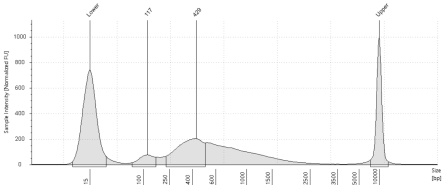

Location	G8
Concentration	246
Description	15
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	337	-	34600	-		Lower Marker
117	43.1	-	569	17.49		
429	203	-	730	82.51		
10000	180	180	27.7	-		Upper Marker

Peak: L2: Ladder

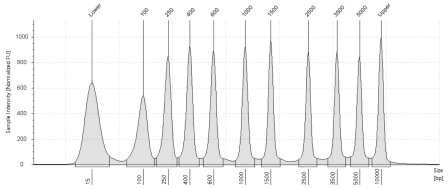


Location	L2
Concentration	1930
Description	Ladder
Observations	Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	314	-	32200	-		Lower Marker
100	225	-	3460	11.68		
250	245	-	1510	12.74		
400	244	-	937	12.65		
600	225	-	576	11.66		
1000	217	-	334	11.27		
1500	211	-	216	10.93		
2500	187	-	115	9.69		
3500	190	-	83.4	9.84		
5000	184	-	56.6	9.55		

Peak: L2: Ladder

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
10000	180	180	27.7	-		Upper Marker

Peak: H8: 16

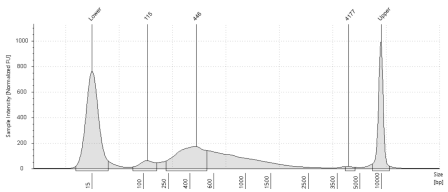

Location	H8
Concentration	246
Description	16
Observations	

Size [bp]	Calibrated Conc. [pg/µl]	Assigned Conc. [pg/µl]	PeakMolarity [pmol/l]	% Integrated Area	PeakComment	Observations
15	355	-	36400	-		Lower Marker
115	37.6	-	505	15.27		
446	204	-	702	82.63		
4177	5.17	-	1.91	2.10		
10000	180	180	27.7	-		Upper Marker


© Agilent Technologies, Inc. 2023

© Agilent Technologies, Inc. 2023

Calibration

Molecular Weight Settings

Fitting type: Log Linear Piecewise
Alignment type: Between markers

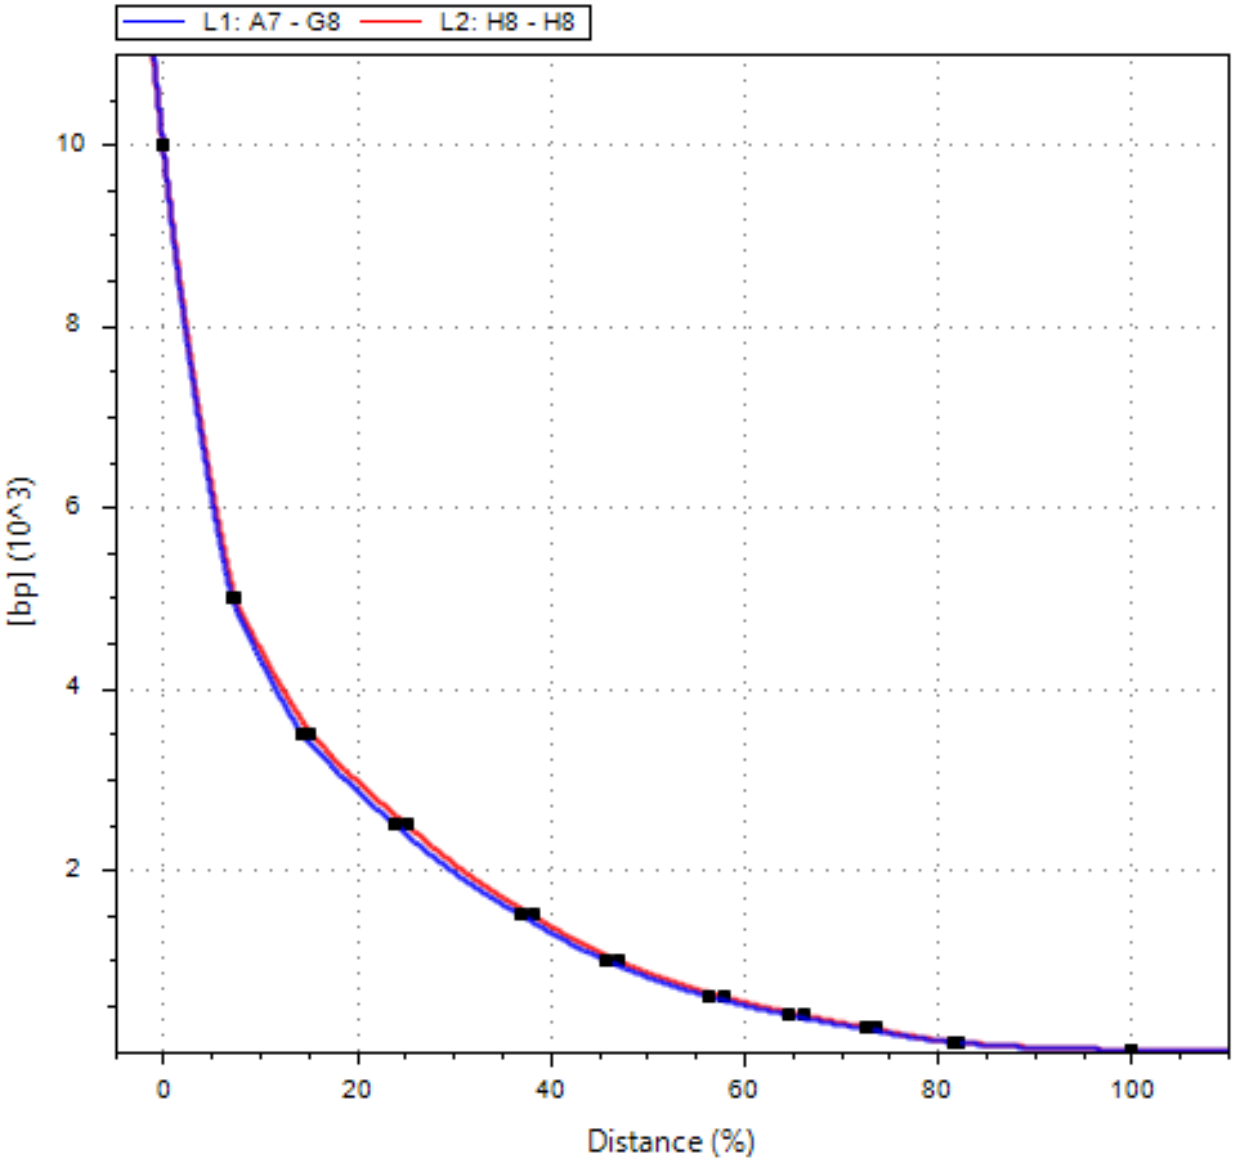

Concentration Settings

Calibration mode: Upper Marker
Normalise peaks from: Upper Marker
Fitting type: Linear Regression

© Agilent Technologies, Inc. 2023

Experiment Properties

Run Properties

Analysis Software Version	5.1.0.47235
Filename	C:\Users\Tapestation 4200B\Documents\Agilent\TapeStation Data\2026-01-30\Briseno_01302026 - 2026-01-30 - 10.46.14.HSD5000
Assay	HSD5000
Run End Date	2026-01-30T11:11:51-05:00
Last Saved Under Version	5.1.0.47235
Study	
Comments	

ScreenTape Device 1

Username	Tapestation 4200B
ScreenTape Device ID	01-S032-250625-01-001335
Expiry Date	2026-02-13T23:59:59
ScreenTape Device History	First run 30 Jan 2026, 1 run(s) performed
Temperature [°C]	25.9
Electrophoresis Time [s]	213
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	
ScreenTape Device Run Date	2026-01-30T10:46:14-05:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

ScreenTape Device 2

Username	Tapestation 4200B
ScreenTape Device ID	01-S032-250625-01-001322
Expiry Date	2026-02-02T23:59:59
ScreenTape Device History	First run 19 Jan 2026, 4 run(s) performed
Temperature [°C]	25.9
Electrophoresis Time [s]	211
Instrument Type	4200 TapeStation (G2991B)
Instrument Serial Number	DEDAC00892
Notes	
ScreenTape Device Run Date	2026-01-30T10:46:14-05:00
Reagent Lot #	
ScreenTape Lot #	

Controller Environment

Computer	DESKTOP-G53EHOQ
Instrument Controller Software Version	5.1.0.47235
First Run Analysis Version	5.1.0.47235
Operating System	Microsoft Windows 11 Pro

© Agilent Technologies, Inc. 2023