



EM-LS-TS ablation — cifar10h (resnet50)

(a) Calibration quality

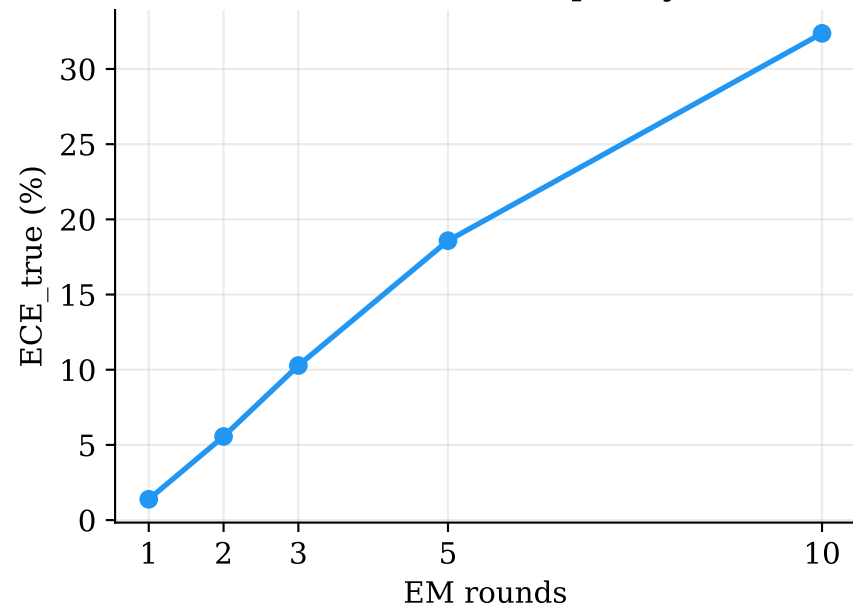

(b) Learned temperature

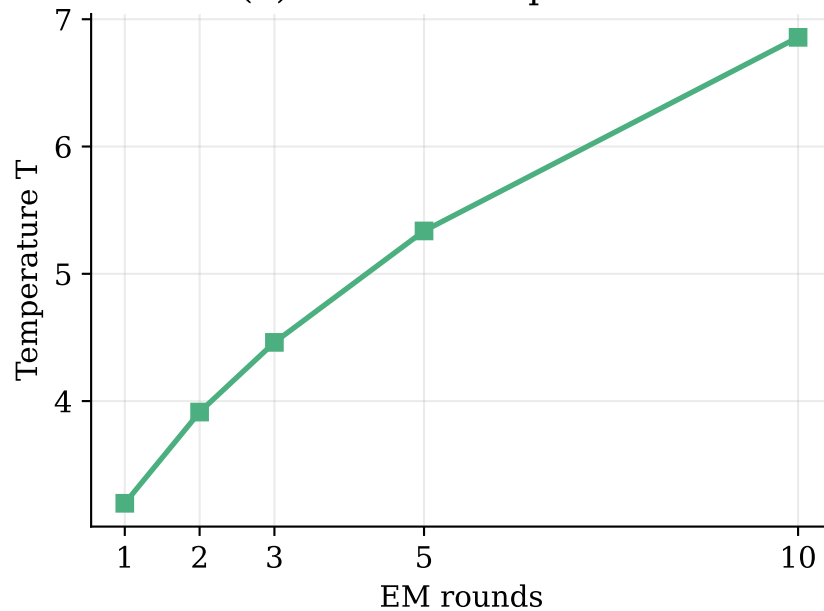

(c) Estimated ε

