Exploratory analysis of pediatric GCF FTIR measurements
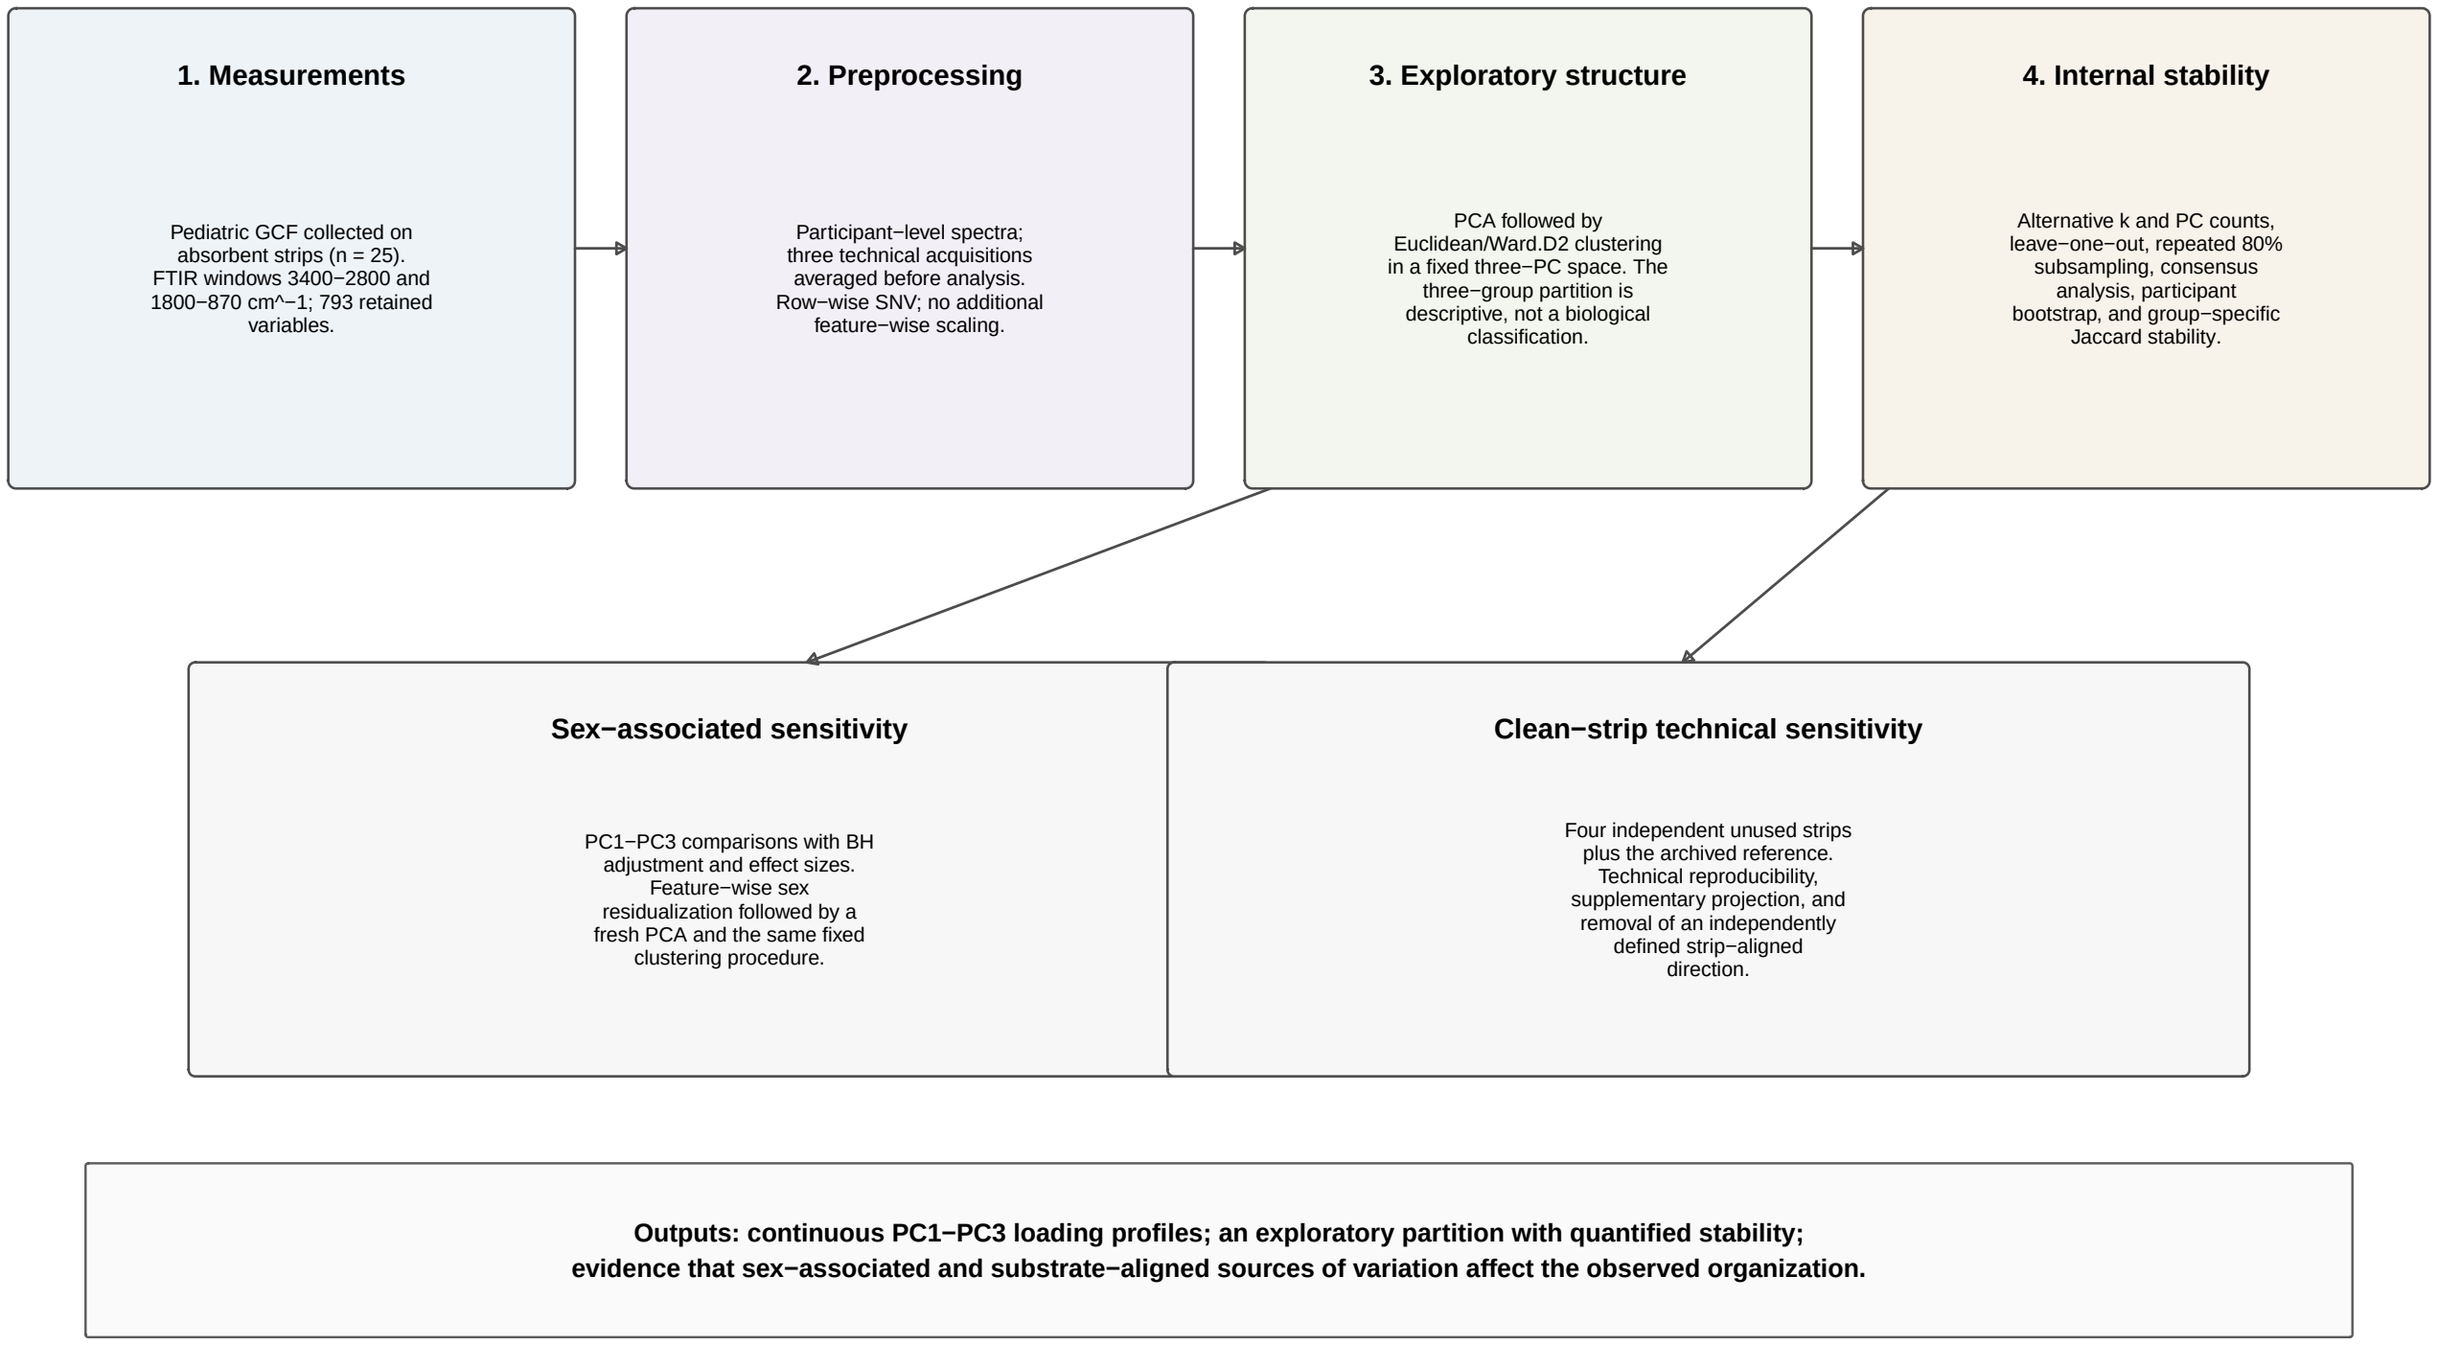
Pediatric−only workflow with explicit stability and technical−sensitivity assessment