
ATP-3.2 azimuth dial

Print at 100%. Place base plate on outline. Rotate the card, not the phantom.

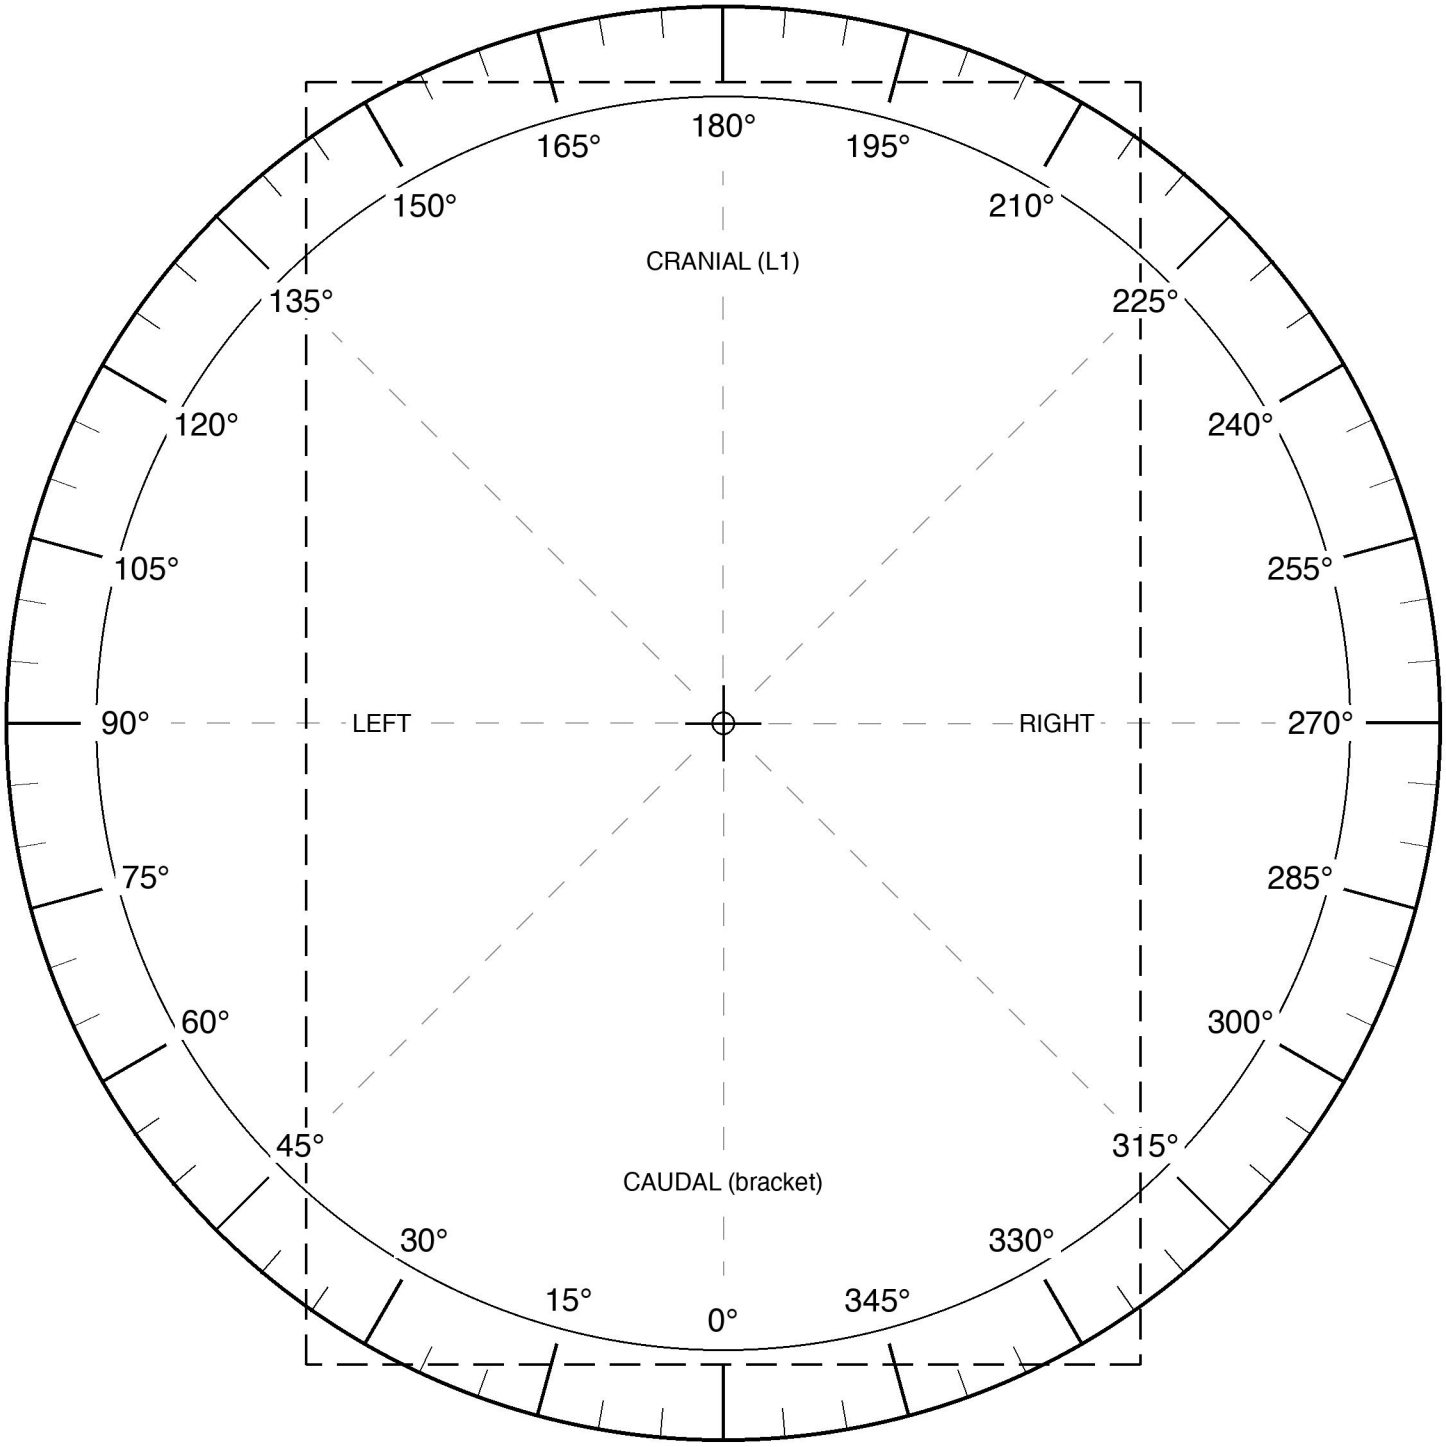

50 mm (measure to confirm print scale)

Azimuth = tick pointing at the camera. 0° caudal, 90° patient left (viewed from above).