D1_final dome markers: DICT_6X6_50, 25 mm black, 32 mm cut

Print on matte paper at 100% (no fit to page). Cut along the dotted outlines with a craft knife and steel ruler.

ID 10 TOP

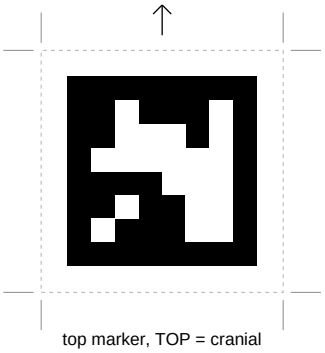

top marker, TOP = cranial

ID 11 TOP

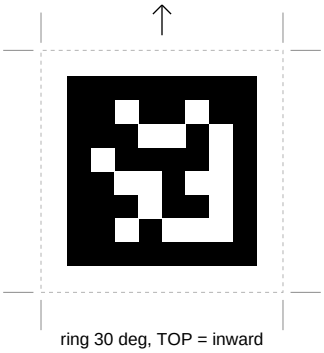

ring 30 deg, TOP = inward

ID 12 TOP

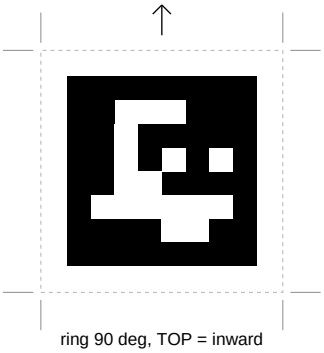

ring 90 deg, TOP = inward

ID 13 TOP

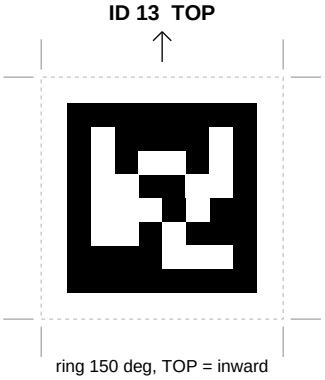

ring 150 deg, TOP = inward

ID 14 TOP

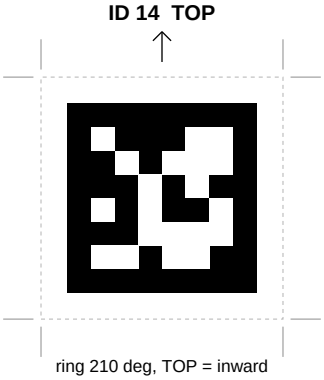

ring 210 deg, TOP = inward

ID 15 TOP

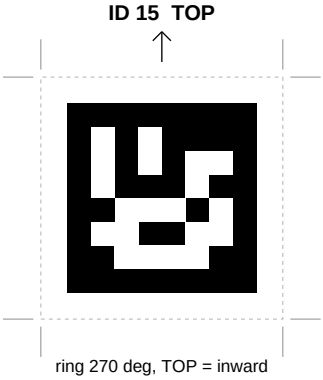

ring 270 deg, TOP = inward

ID 16 TOP

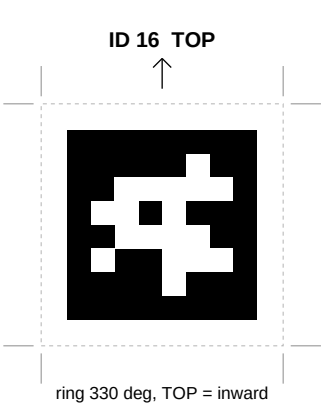

ring 330 deg, TOP = inward

ID 17 TOP

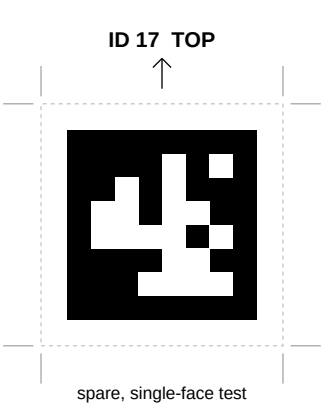

spare, single-face test

Key: top view, looking down

cranial up, patient left on the left

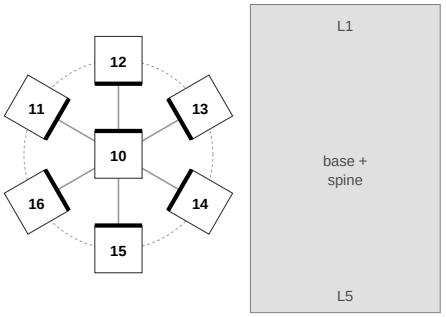

thick edge = marker TOP edge (inward on the ring, cranial on ID 10)

ID 10 sits raised in the centre; 17 is the spare

Scale check: this bar must measure 100.0 mm. If not, reprint at 100% / Actual size.