


# Validation F1 Score for MLP\_MNIST Ablation: MILO\_ablate\_adaptive

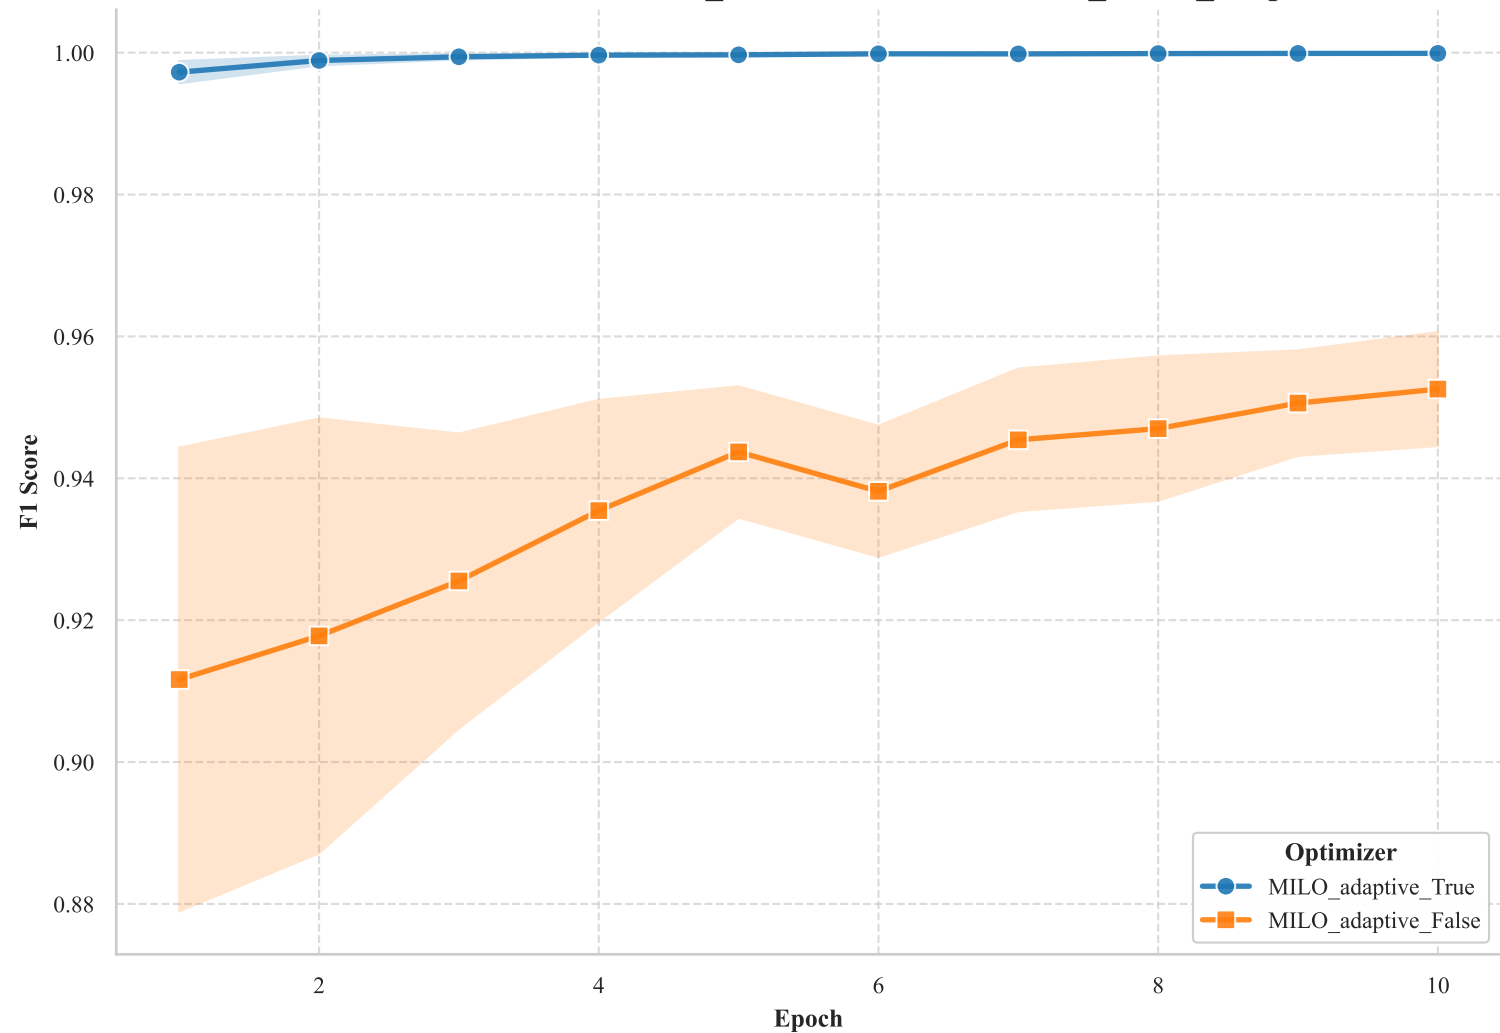

*Error bands represent standard error of the mean across runs. Markers indicate run end on walltime plots.*