


# Validation Accuracy for ResNet18\_CIFAR10 Ablation: MILO\_LW\_ablate\_normalize

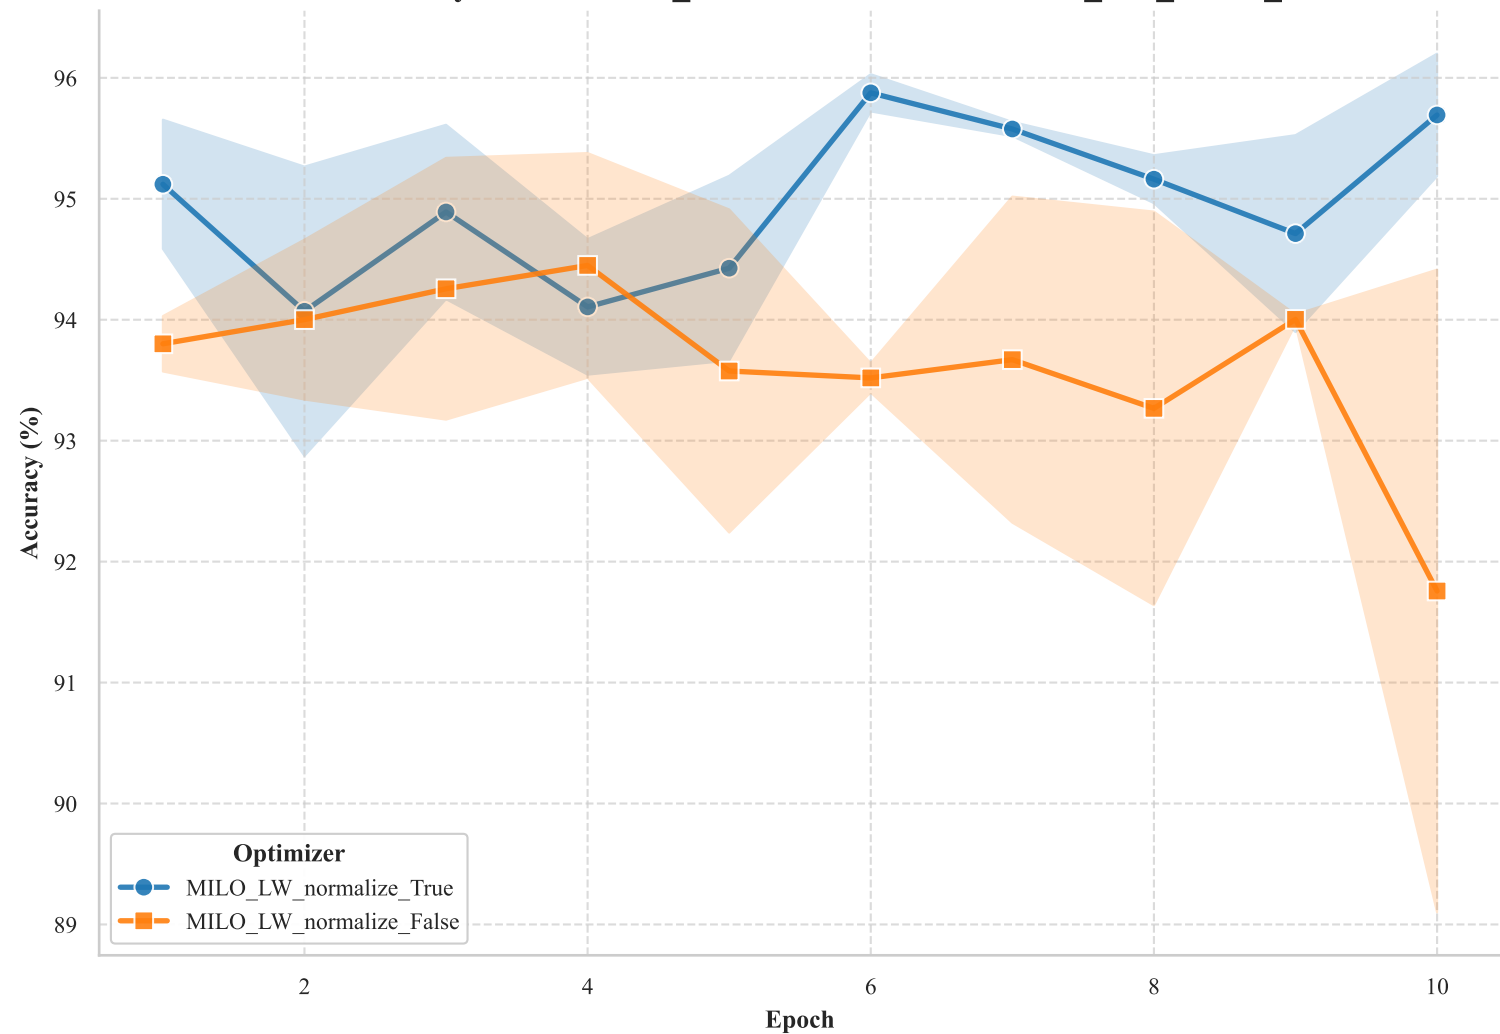

*Error bands represent standard error of the mean across runs. Markers indicate run end on walltime plots.*