


# Validation F1 Score for ResNet18\_CIFAR10 Ablation: MILO\_LW\_ablate\_scale\_aware

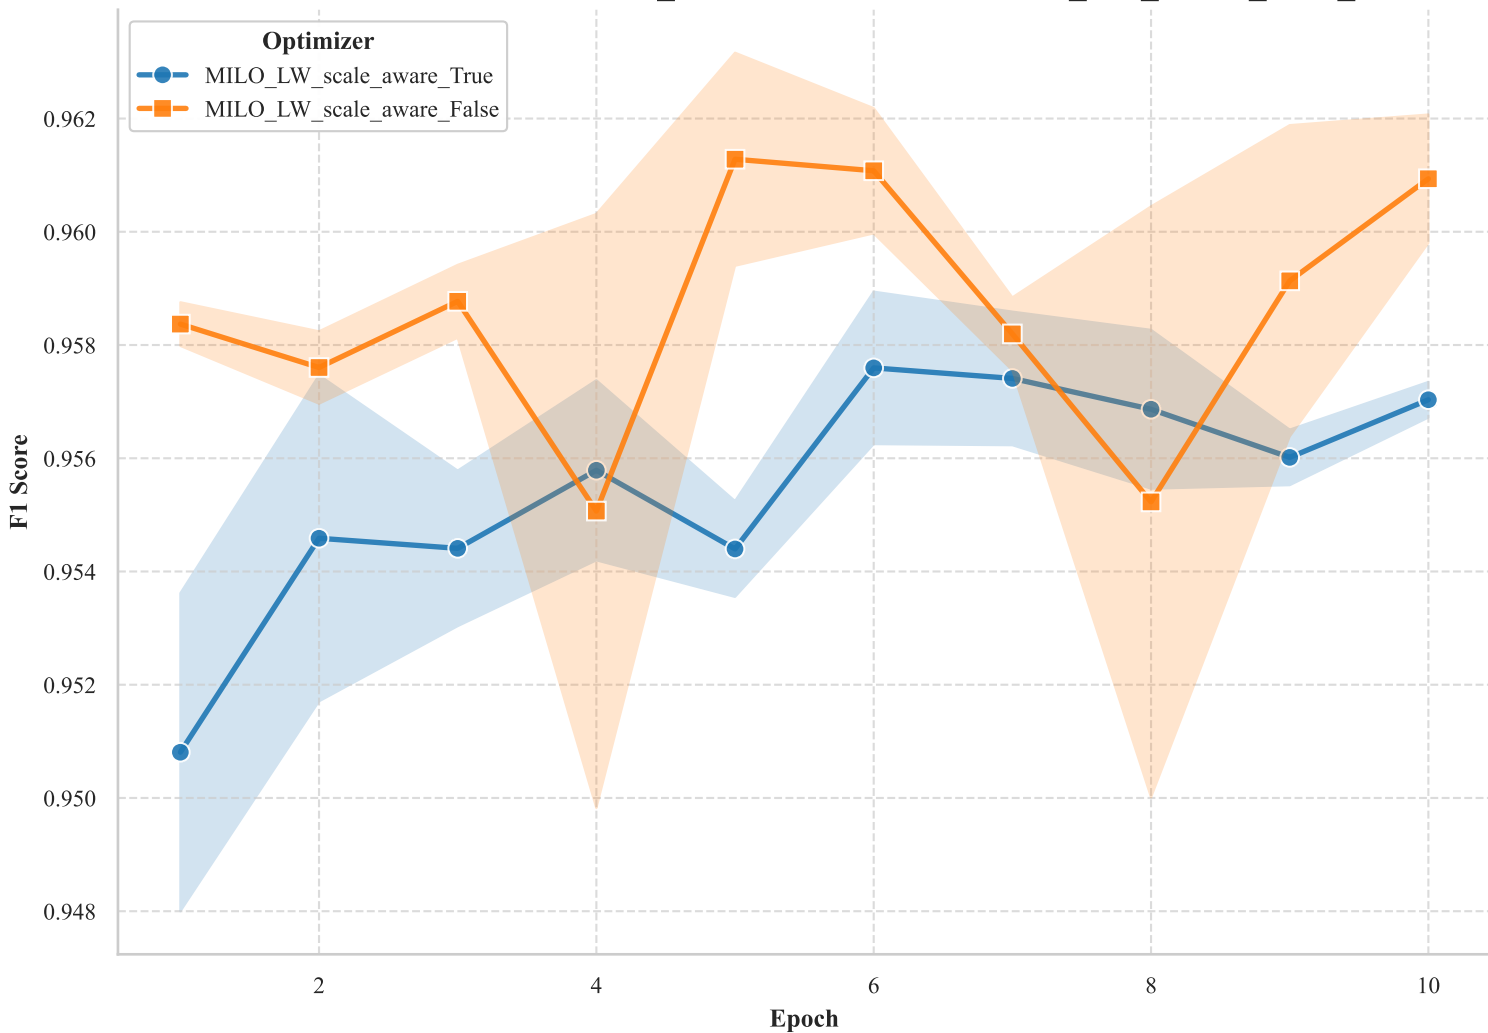

Error bands represent standard error of the mean across runs. Markers indicate run end on walltime plots.