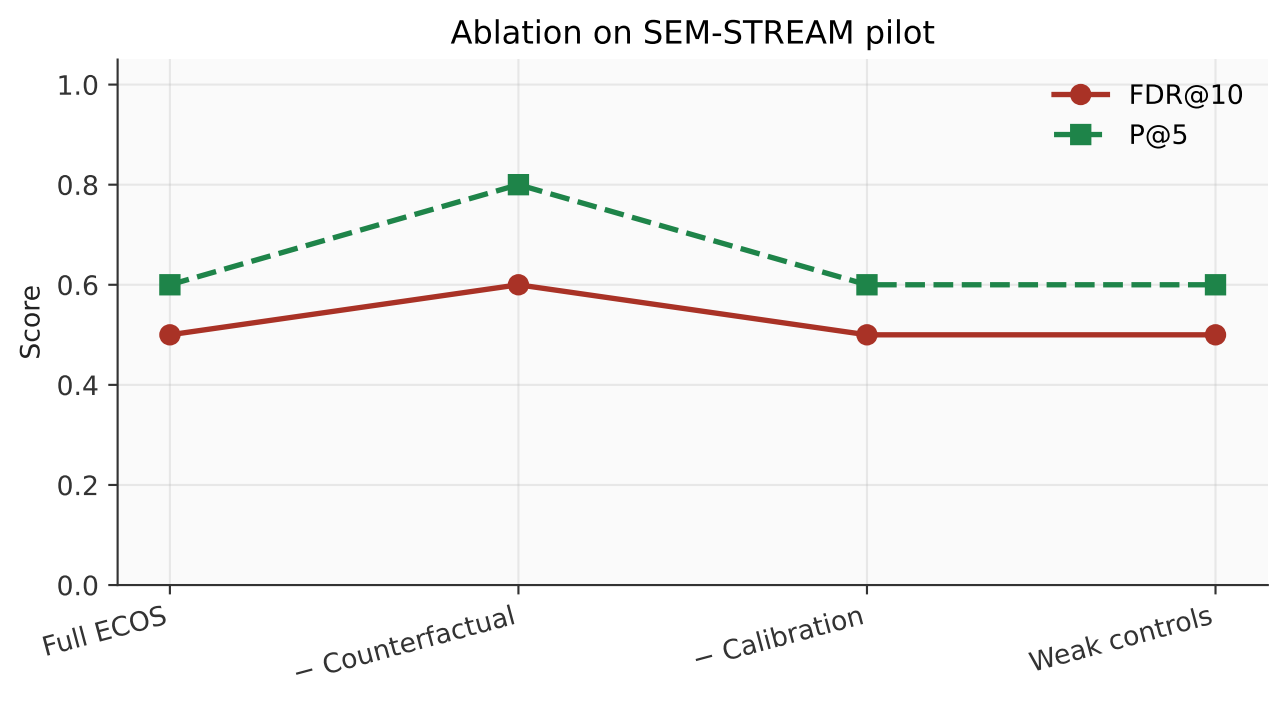
Ablation on SEM-STREAM pilot
FDR@10
P@5
Score
1.0
0.8
0.6
0.4
0.2
0.0
Full ECOS
− Counterfactual
− Calibration
Weak controls