

Single Field Analysis

Eye: Left

Name: SNASERIO091

DOB: 01-01-1969

ID: SNASERIO091

Central 24-2 Threshold Test

Fixation Monitor: Gaze/Blind Spot

Stimulus: III, White

Pupil Diameter: 7.2 mm

Date: 20-09-2018

Fixation Target: Central

Background: 31.5 ASB

Visual Acuity:

Time: 10:01 AM

Fixation Losses: 1/12

Strategy: SITA-Fast

RX: +0.50 DS -1.75 DC X 114




Age: 49

False POS Errors: 3 %

False NEG Errors: 6 %

Test Duration: 04:16

Fovea: 33 dB ::

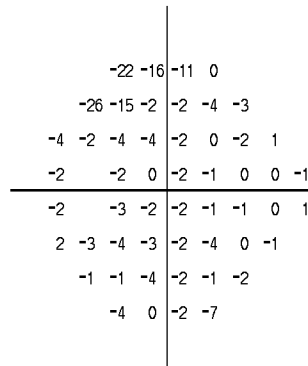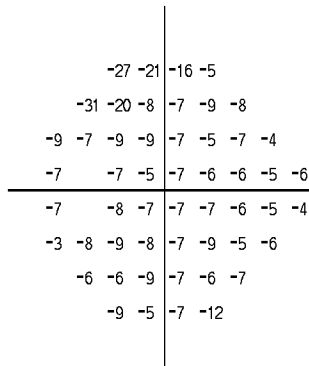
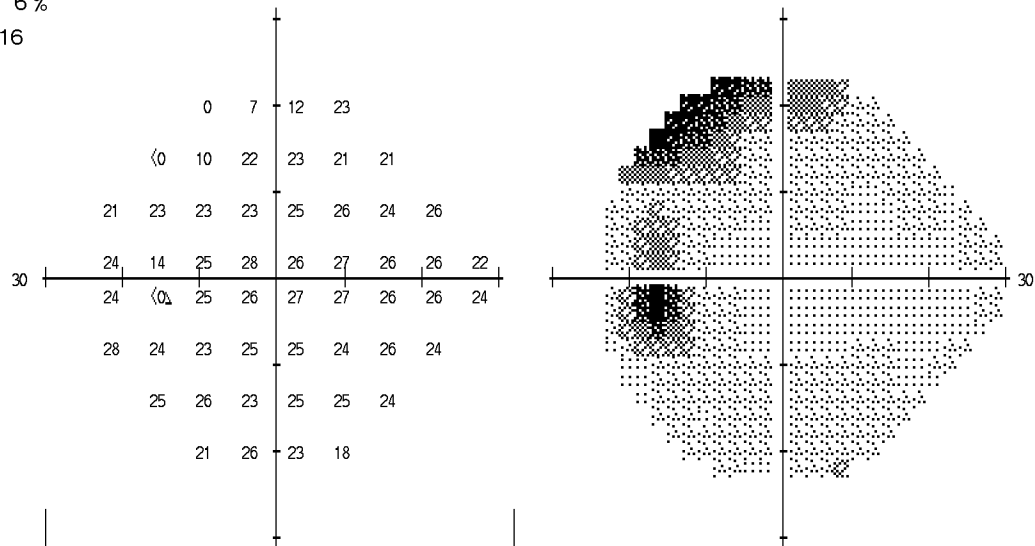


GHT
Outside normal limits

VFI 91%

MD -7.76 dB P < 0.5%

PSD 4.56 dB P < 0.5%

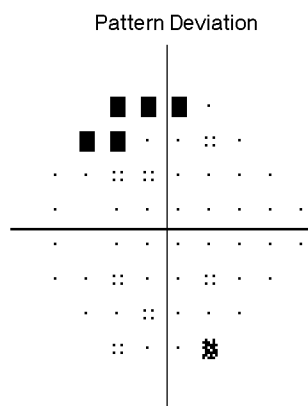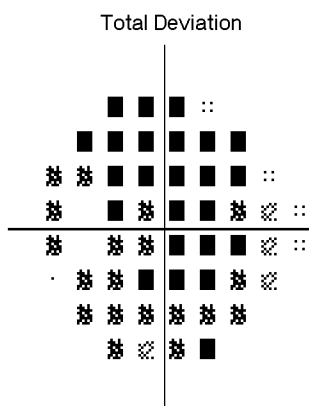

:: < 5%
 < 2%
 < 1%
 < 0.5%

