



**Patient: Smith, Eva**



Date of birth: 04.12.1972  
ID: ASDFGHJKL  
Gender: Male

**Session date: 31.03.2020 10:17**

Address: Address  
City: D-12169 City  
Mobile: +49157777777



## DPOAE

Frequencies for pass: 3/4; — SNR for pass: 6 dB; Averaging time: 4 s



## DPOAE

Frequencies for pass: 3/4; SNR for pass: 6 dB; — Min. OAE level: -5 dB SPL; Averaging time: 2 s







Patient: Smith, Eva

Session date: 31.03.2020 10:17



## DPOAE

Frequencies for pass: 3/4; SNR for pass: 6 dB; — Min. OAE level: -- dB SPL (-5 dB SPL); Averaging time: 4 s

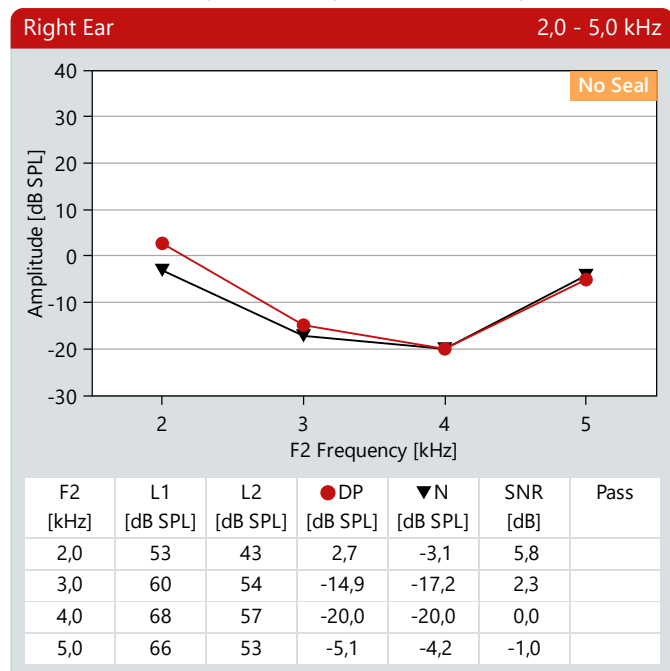

## DPOAE

\*Frequencies for pass: 2/4 (4/4); — SNR for pass: 4 dB (5 dB); Min. OAE level: -- dB SPL (-5 dB SPL); Averaging time: 1 s (2 s)

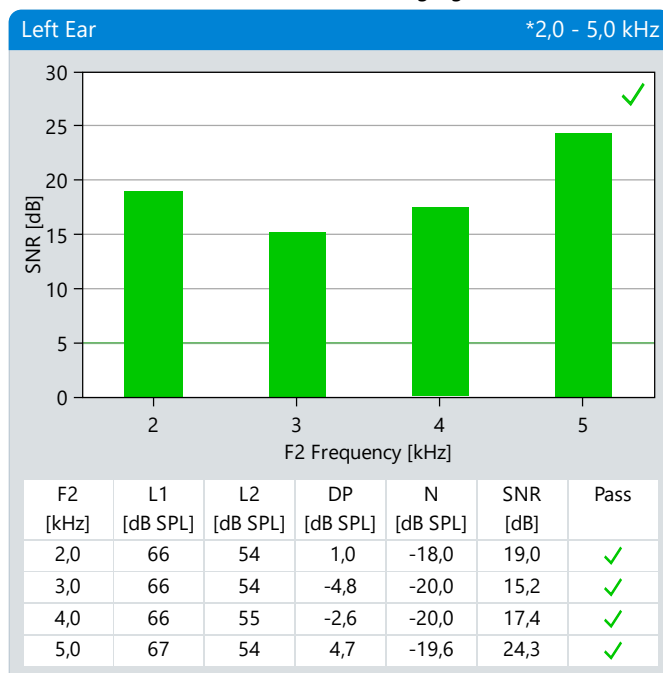





Patient: Smith, Eva

Session date: 31.03.2020 10:17



## DPOAE

SNR for pass: 6 dB; Averaging time: 4 s



## DPOAE

\*Frequencies for pass: 2/6; — SNR for pass: 3 dB; Min. OAE level: -5 dB SPL; Averaging time: 2 s

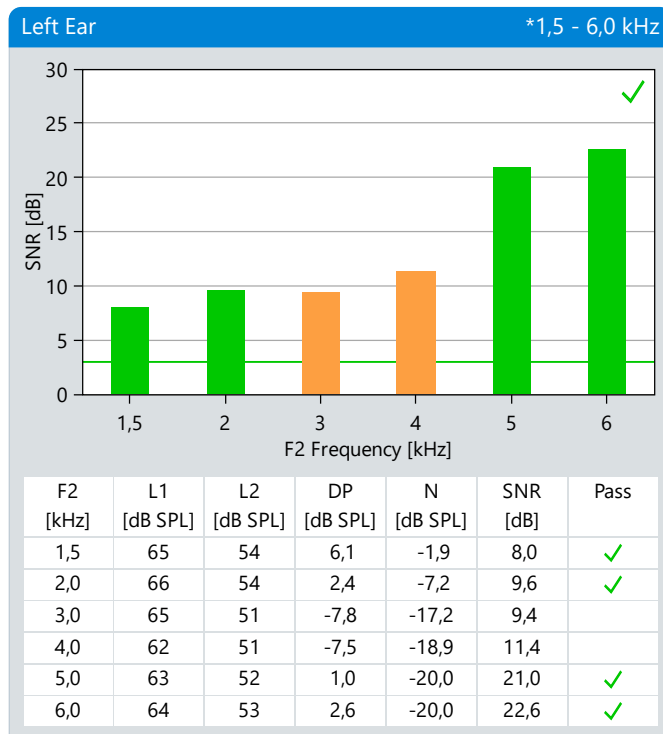



Patient: Smith, Eva


Session date: 31.03.2020 10:17

## DPOAE

SNR for pass: 6 dB; — Min. OAE level: -5 dB SPL; Averaging time: 4 s

### Right Ear


1,6 - 8,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | ● DP [dB SPL] | ▼ N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|---------------|--------------|----------|------|
| 1,6      | 65          | 56          | -0,5          | -12,9        | 12,4     |      |
| 2,0      | 64          | 54          | 1,1           | -4,8         | 5,9      |      |
| 2,5      | --          | --          | --            | -14,0        | --       |      |
| 3,2      | --          | --          | --            | -10,2        | --       |      |
| 3,6      | --          | --          | --            | -7,0         | --       |      |
| 4,0      | --          | --          | --            | -0,2         | --       |      |
| 4,5      | 70          | 59          | -8,4          | -9,2         | 0,8      |      |
| 5,0      | 69          | 59          | -17,2         | -10,9        | -6,3     |      |
| 5,6      | 69          | 65          | -13,4         | -20,0        | 6,6      |      |
| 6,3      | 72          | 66          | -10,2         | -14,7        | 4,5      |      |
| 7,1      | 73          | 69          | -12,0         | -16,3        | 4,4      |      |
| 8,0      | 76          | 70          | -10,1         | -12,9        | 2,8      |      |

### Left Ear

1,6 - 8,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | × DP [dB SPL] | ▼ N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|---------------|--------------|----------|------|
| 1,6      | 61          | 51          | -8,0          | -2,7         | -5,3     |      |
| 2,0      | 60          | 50          | 3,6           | 5,1          | -1,5     |      |
| 2,5      | 64          | 54          | -3,9          | -17,2        | 13,4     |      |
| 3,2      | 64          | 53          | 0,2           | -20,0        | 20,2     |      |
| 3,6      | 63          | 54          | -0,5          | -19,6        | 19,2     |      |
| 4,0      | 62          | 57          | -0,3          | -17,8        | 17,6     |      |
| 4,5      | 66          | 58          | 6,3           | -19,6        | 25,9     |      |
| 5,0      | 64          | 54          | 3,1           | -20,0        | 23,1     |      |
| 5,6      | 58          | 52          | -6,1          | -19,6        | 13,5     |      |
| 6,3      | 58          | 52          | -20,0         | -14,2        | -5,8     |      |
| 7,1      | 60          | 53          | -20,0         | -20,0        | 0,0      |      |
| 8,0      | 63          | 56          | -20,0         | -20,0        | 0,0      |      |



Patient: Smith, Eva


Session date: 31.03.2020 10:17

## DPOAE

\*Frequencies for pass: 12/12; — SNR for pass: 3 dB; Min. OAE level: -5 dB SPL; Averaging time: 2 s

### Right Ear


\*1,6 - 8,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | DP [dB SPL] | N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|-------------|------------|----------|------|
| 1,6      | 66          | 54          | -14,0       | -18,0      | 4,0      |      |
| 2,0      | 66          | 54          | -14,9       | -17,2      | 2,3      |      |
| 2,5      | 66          | 54          | -19,0       | -19,0      | 0,0      |      |
| 3,2      | 66          | 54          | -14,9       | -18,9      | 4,0      |      |
| 3,6      | 56          | 49          | -13,0       | -16,7      | 3,6      |      |
| 4,0      | 66          | 54          | -20,0       | -19,3      | -0,8     |      |
| 4,5      | 66          | 54          | -17,2       | -17,2      | 0,0      |      |
| 5,0      | 66          | 54          | -17,8       | -20,0      | 2,2      |      |
| 5,6      | 63          | 57          | -20,0       | -19,6      | -0,4     |      |
| 6,3      | 65          | 56          | -20,0       | -20,0      | 0,0      |      |
| 7,1      | 68          | 60          | -20,0       | -20,0      | 0,0      |      |
| 8,0      | 69          | 64          | -20,0       | -20,0      | 0,0      |      |

### Left Ear

\*1,6 - 8,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | DP [dB SPL] | N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|-------------|------------|----------|------|
| 1,6      | 66          | 54          | -2,0        | -14,7      | 12,7     | ✓    |
| 2,0      | 66          | 54          | 2,1         | 1,8        | 0,3      |      |
| 2,5      | 66          | 54          | -0,4        | -10,1      | 9,7      | ✓    |
| 3,2      | 66          | 54          | -5,5        | -14,7      | 9,2      |      |
| 3,6      | 66          | 54          | -1,8        | -20,0      | 18,2     | ✓    |
| 4,0      | 66          | 54          | -0,5        | -17,5      | 17,0     | ✓    |
| 4,5      | 66          | 54          | 6,0         | -19,3      | 25,3     | ✓    |
| 5,0      | 66          | 55          | 7,3         | -20,0      | 27,3     | ✓    |
| 5,6      | 53          | 50          | -1,2        | -20,0      | 18,8     | ✓    |
| 6,3      | 57          | 54          | 3,8         | -20,0      | 23,8     | ✓    |
| 7,1      | 63          | 58          | 2,1         | -20,0      | 22,1     | ✓    |
| 8,0      | 67          | 63          | 0,7         | -20,0      | 20,7     | ✓    |



Patient: Smith, Eva


Session date: 31.03.2020 10:17

## DPOAE

SNR for pass: 6 dB; — Min. OAE level: -5 dB SPL; Averaging time: 4 s

Right Ear


1,5 - 12,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | ● DP [dB SPL] | ▼ N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|---------------|--------------|----------|------|
| 1,5      |             |             |               |              |          |      |
| 2,0      |             |             |               |              |          |      |
| 3,0      |             |             |               |              |          |      |
| 4,0      |             |             |               |              |          |      |
| 5,0      |             |             |               |              |          |      |
| 6,0      |             |             |               |              |          |      |
| 7,0      |             |             |               |              |          |      |
| 8,0      |             |             |               |              |          |      |
| 9,0      |             |             |               |              |          |      |
| 10,0     |             |             |               |              |          |      |
| 11,0     |             |             |               |              |          |      |
| 12,0     |             |             |               |              |          |      |

Left Ear

1,5 - 12,0 kHz



| F2 [kHz] | L1 [dB SPL] | L2 [dB SPL] | × DP [dB SPL] | ▼ N [dB SPL] | SNR [dB] | Pass |
|----------|-------------|-------------|---------------|--------------|----------|------|
| 1,5      | 65          | 55          | -4,8          | -18,5        | 13,8     |      |
| 2,0      | 65          | 55          | 2,6           | -17,8        | 20,4     |      |
| 3,0      | 65          | 55          | -6,9          | -20,0        | 13,1     |      |
| 4,0      | 64          | 57          | 4,8           | -8,4         | 13,3     |      |
| 5,0      | 70          | 60          | 7,1           | -20,0        | 27,1     |      |
| 6,0      | 58          | 55          | -1,1          | -20,0        | 18,9     |      |
| 7,0      | 64          | 60          | -1,3          | -20,0        | 18,7     |      |
| 8,0      | 68          | 64          | -4,7          | -20,0        | 15,3     |      |
| 9,0      | 74          | 69          | -6,3          | -20,0        | 13,7     |      |
| 10,0     | 75          | 61          | 0,7           | -20,0        | 20,7     |      |
| 11,0     | 81          | 44          | -0,8          | -20,0        | 19,2     |      |
| 12,0     | 71          | 52          | -4,1          | -20,0        | 15,9     |      |





Patient: Smith, Eva

Session date: 31.03.2020 10:17



## DPOAE

\*Frequencies for pass: 3/12; SNR for pass: 3 dB; — Min. OAE level: -5 dB SPL; Averaging time: 2 s



## TEOAE

Frequencies for pass: 3/6; SNR for pass: 4 dB; Averaging time: 29 s







Patient: Smith, Eva

Session date: 31.03.2020 10:17



## TEOAE

Frequencies for pass: 3/6; SNR for pass: 4 dB; — Min. OAE level: -10 dB SPL (-5 dB SPL); Averaging time: 32 s



## TEOAE

Frequencies for pass: 3/6; — SNR for pass: 4 dB; Min. OAE level: -5 dB SPL (-10 dB SPL); Averaging time: 64 s









Patient: Smith, Eva

Session date: 31.03.2020 10:17



## TEOAE

\*Frequencies for pass: 1/6; — SNR for pass: 3 dB; Min. OAE level: -5 dB SPL; Averaging time: 9 s (16 s)



## TEOAE

SNR for pass: 4 dB; Averaging time: 64 s







Patient: Smith, Eva

Session date: 31.03.2020 10:17

## TEOAE

\*Frequencies for pass: 4/6 (2/6); SNR for pass: 4 dB (3 dB); — Min. OAE level: -5 dB SPL (-10 dB SPL); Averaging time: 16 s



Device: ERO•SCAN®

Serial number (probe): ME9999999 (ME2004677)

Calibration date:

Notes:

Examiner: mikk

Signature: \_\_\_\_\_