


Salem

Exploratory Parapsychology Instrument

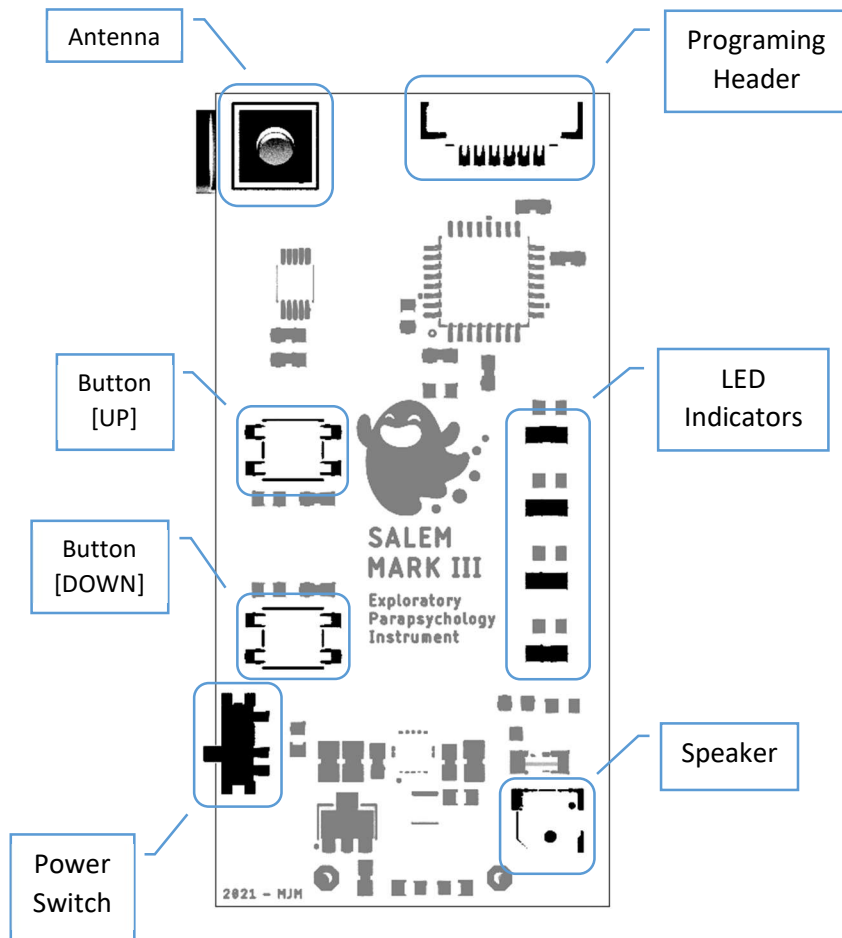

Quick Start

- 1.) Acclimate the device to the room's ambient temperature.
- 2.) Place the device on a smooth level surface and extend the antenna
- 3.) Power on the device and step out of the detection zone.
- 4.) Wait for the initialization sequence to complete (chirp).
- 5.) Adjust the sensitivity threshold as needed (up / down).