


FlowAccessV3

Date:2022-12-20 15:13:03

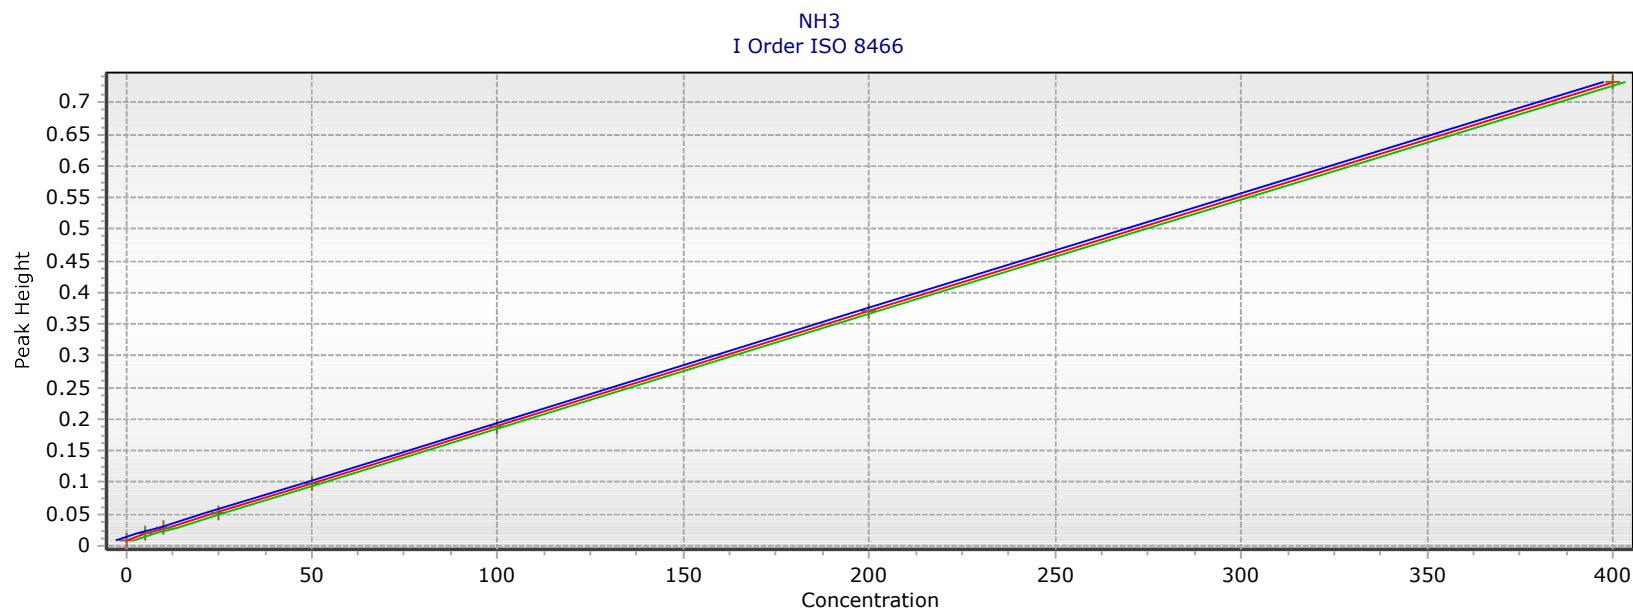

$a = 0.00878851141090$ $b = 0.00180859643220$ $RSD = 0.00169746901334$

$r = 0.99998045967593$ $R^2 = 0.99996091973368$ Detection Limit = 1.99544495943934 Determination Limit = 7

Run Name : x20221220xMAGMxresinrerun, Run Db Ref : SKALAR20221220A0

User Name : Administrator Operator Name : Administrator