


FlowAccessV3

Date:2022-12-20 15:15:40

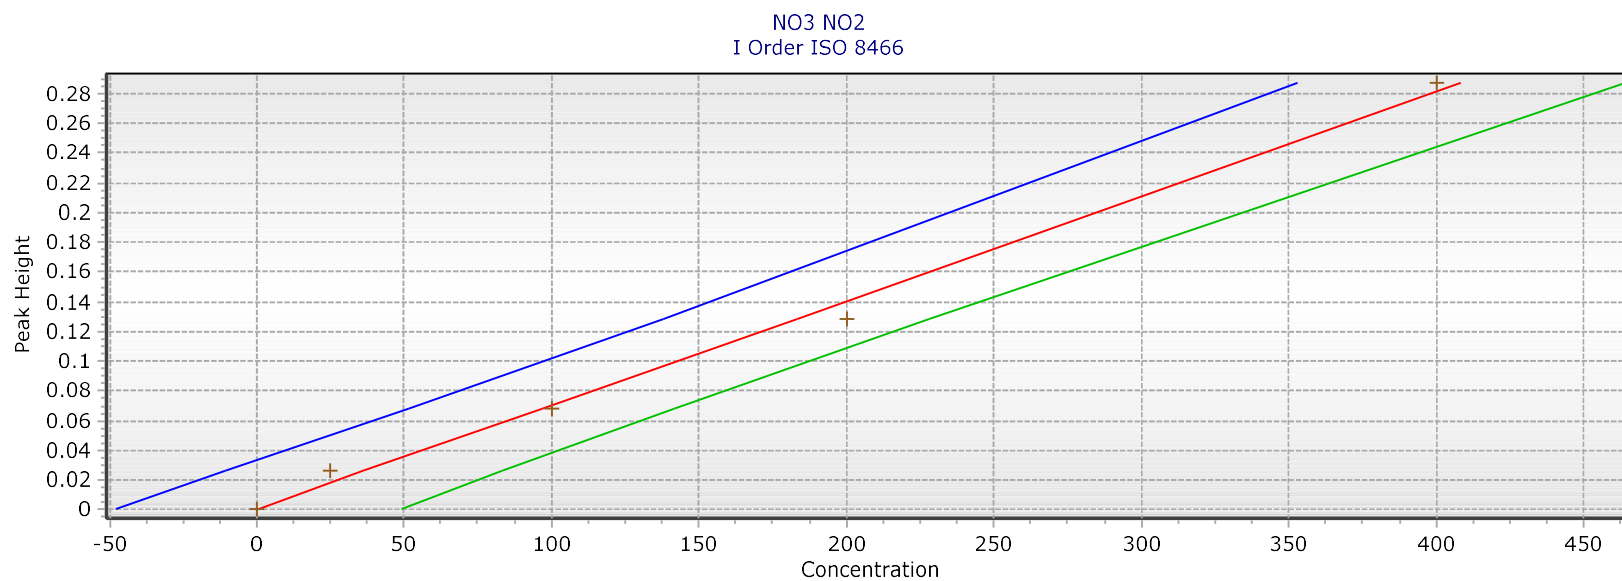

$a = 0.00027826647997$ $b = 0.00070271277036$ $RSD = 0.00903127119571$

$r = 0.99765979295917$ $R^2 = 0.99532506248733$ Detection Limit = 35.7778109131416 Determination Limit = 1

Run Name : x20221220xMAGMxresinrerun, Run Db Ref : SKALAR20221220A0

User Name : Administrator Operator Name : Administrator