


FlowAccessV3

Date:2024-12-05 16:21:21

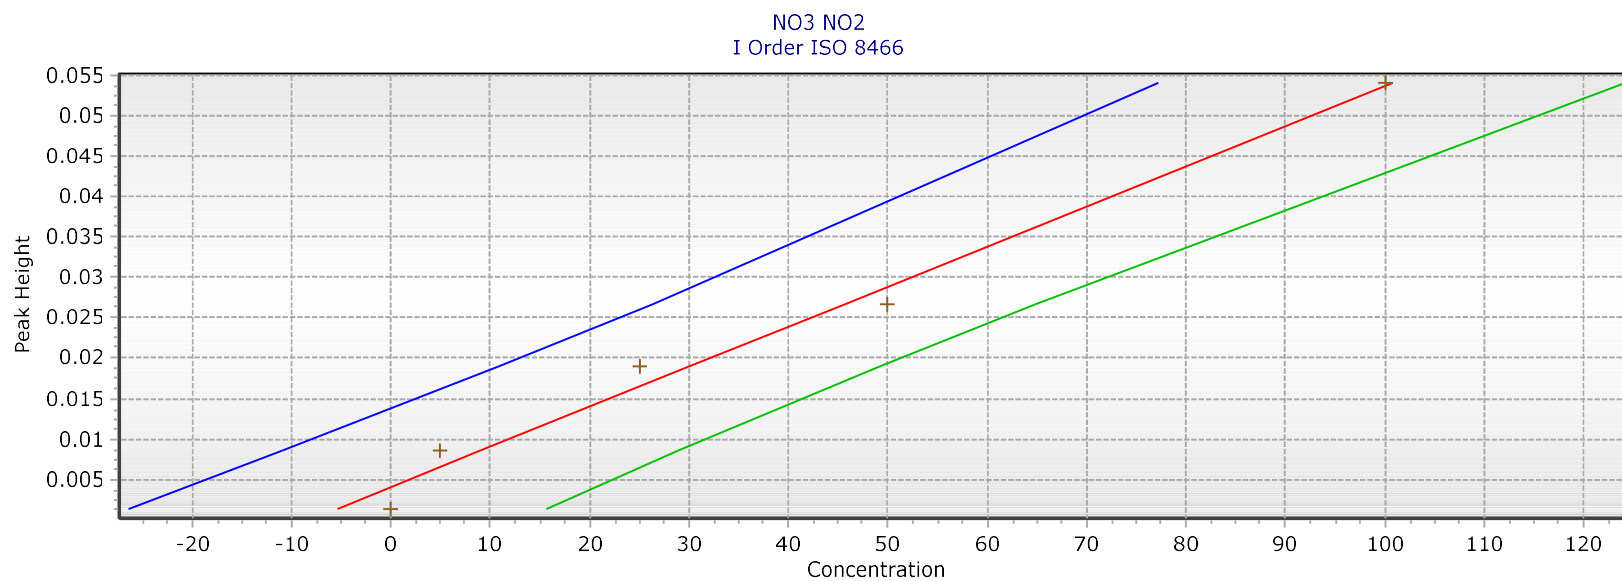

$a = 0.00402755922039$ $b = 0.00049594557721$ $RSD = 0.00271384398007$

$r = 0.99333335645422$ $R^2 = 0.98671115704461$ Detection Limit = 15.2061199950857 Determination Limit = 5

Run Name : x20241204xMAGMxKClctx202, Run Db Ref : SKALAR20241204A0

User Name : Administrator Operator Name : Administrator