


FlowAccessV3

Date:2024-12-05 16:25:34

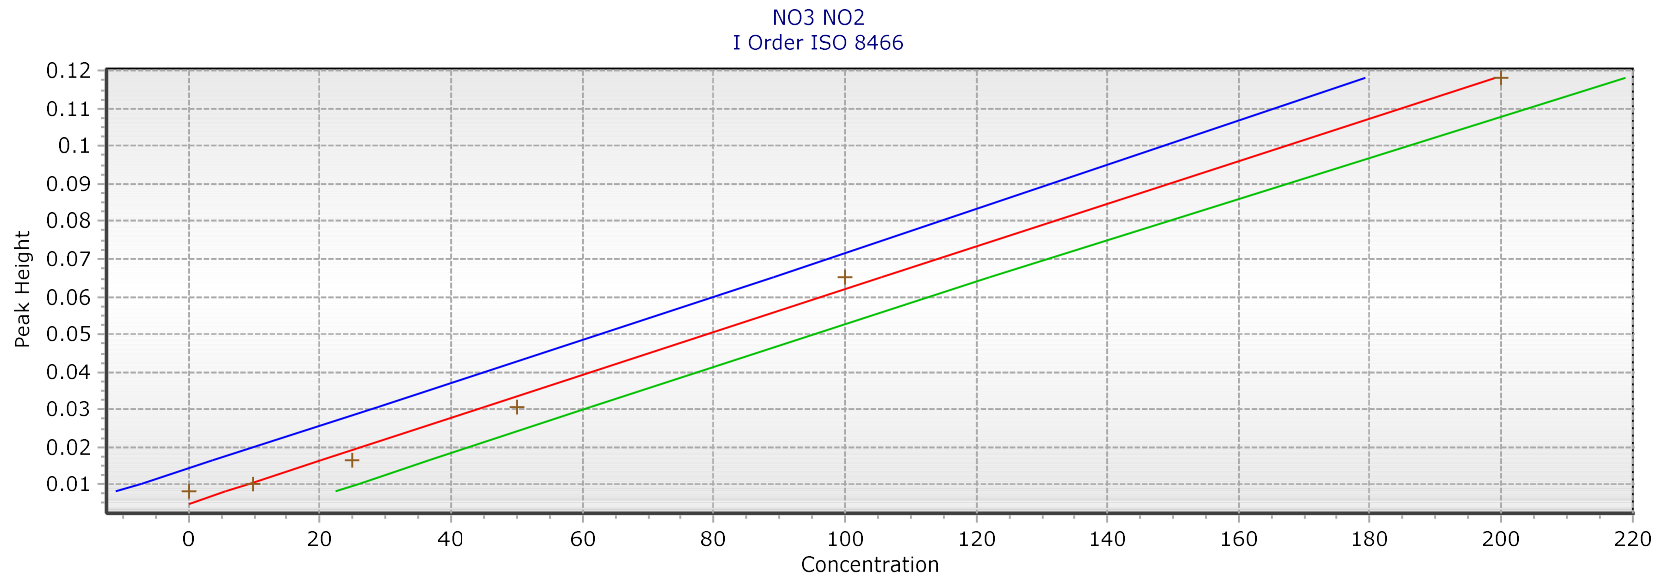

$a = 0.00485708286340$ $b = 0.00056889377356$ $RSD = 0.00303420758612$

$r = 0.99801116438808$ $R^2 = 0.99602628424325$ Detection Limit = 13.0189633364208 Determination Limit = 4

Run Name : z20241205xMAGMxKClresinex, Run Db Ref : SKALAR20241205A0

User Name : Administrator Operator Name : Administrator