



Figure 1: Radiologist interacting with traditional environment.

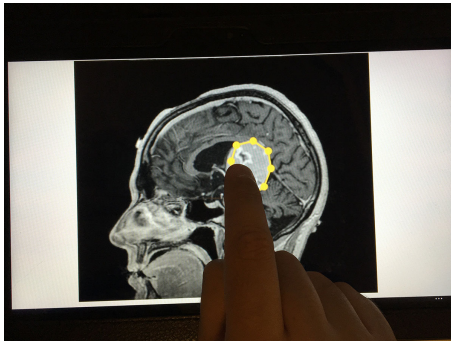


Figure 2: Touch environment interaction.

Towards Touch-Based Medical Image Diagnosis Annotation

Francisco Maria Calisto

Institute for Systems and Robotics (ISR/IST),
LARSyS, Instituto Superior Técnico,
Universidade de Lisboa
Lisbon, Portugal
francisco.calisto@tecnico.ulisboa.pt

Jacinto C. Nascimento

Institute for Systems and Robotics (ISR/IST),
LARSyS, Instituto Superior Técnico,
Universidade de Lisboa
Lisbon, Portugal
jacinto.nascimento@tecnico.ulisboa.pt

Alfredo Ferreira

INESC-ID, Instituto Superior Técnico,
Universidade de Lisboa
Lisbon, Portugal
alfredo.ferreira@tecnico.ulisboa.pt

Daniel Gonçalves

INESC-ID, Instituto Superior Técnico,
Universidade de Lisboa
Lisbon, Portugal
daniel.j.goncalves@tecnico.ulisboa.pt

ABSTRACT

A fundamental step in medical diagnosis for patient follow-up relies on the ability of radiologists to perform a trusty diagnostic from acquired images. Basically, the diagnosis strongly depends on the visual inspection over the shape of the lesions. As datasets increase in size, such visual evaluation becomes harder. For this reason, it is crucial to introduce easy-to-use interfaces that help the radiologists to perform a reliable visual inspection and allow the efficient delineation of the lesions. We will explore the radiologist's receptivity to the current touch environment solution. The advantages of touch are threefold: (i) the time performance is superior regarding the traditional use, (ii) it has more intuitive control and, (iii) for less time, the user interface delivers more information per action, concerning annotations. From our studies, we conclude that the radiologists still exhibit a resistance to change from traditional to touch based interfaces in current clinical setups.

ISS '17, October 17–20, 2017, Brighton, United Kingdom

© 2017 Copyright held by the owner/author(s).

This is the author's version of the work. It is posted here for your personal use. Not for redistribution. The definitive Version of Record was published in *Proceedings of ISS '17, October 17–20, 2017*, <https://doi.org/10.1145/3132272.3134111>.

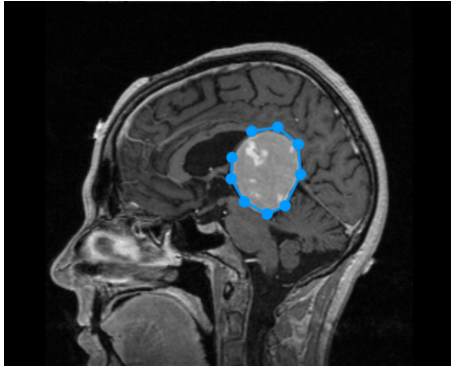


Figure 3: Hard difficulty DICOM annotated image.

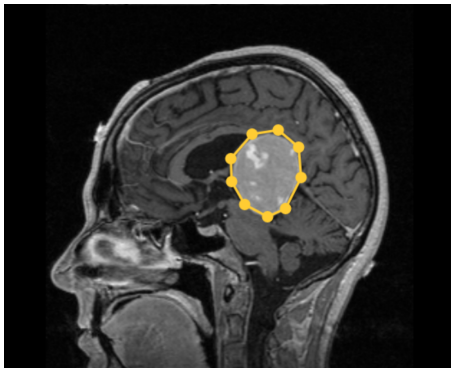


Figure 4: Hard difficulty DICOM annotated image.

CCS CONCEPTS

• **Human-centered computing** → **Touch screens**; *User studies*; *Usability testing*; Graphical user interfaces; Web-based interaction; Collaborative interaction; Gestural input;

KEYWORDS

Touch-Based, Medical Image Diagnosis, Medical Visualization, Interaction Design, Human-Computer Interaction

ACM Reference format:

Francisco Maria Calisto, Jacinto C. Nascimento, Alfredo Ferreira, and Daniel Gonçalves. 2017. Towards Touch-Based Medical Image Diagnosis Annotation. In *Proceedings of ISS '17, Brighton, United Kingdom, October 17–20, 2017*, 6 pages.

<https://doi.org/10.1145/3132272.3134111>

INTRODUCTION

Medical imaging diagnosis is a topic of great interest, that has been the subject of intensive research in the field of medicine, and more specifically in Radiology [3, 4, 7]. However, current tools do not fully support annotation collection. These annotations and their relationships are crucial for a proper diagnosis. Namely, to have the morphological time evolution of potential lesions that may be present in some human organs.

In this paper, we present a performance and experience analysis conducting a study of touch and traditional environments (Figures 1 and 2) that are aligned to the previous mentioned goals. Both environments are comfortable to interact with and fast enough to solve the annotation tasks. For each environment, the same simple image feature (e.g. delete/correct annotation) is considered.

The performance differences of traditional and touch input devices have been studied [10] in terms of speed and accuracy for a variety of clinical and medical interactive tasks. This includes features such as Regions of Interest (ROI) annotations and length measurements, among others. Although, user experience while inserting annotations is important when evaluating the input devices, there is still a lack of research examining how the experience compromises the interactive surfaces based on the input type. To tackle this issue, our main goals focus primarily on cognition and time-performance. The experience is also considered as a means to validate the sensation, affect and value of interaction.

Indeed, while user experience analysis and evaluation has been applied to clinical systems [2], time-measure and error scales are still missing. Moreover, a touch interactive surface application can improve medical and clinical competences, since it is able to reduce the running time figures to complete common tasks in the diagnosis loop.

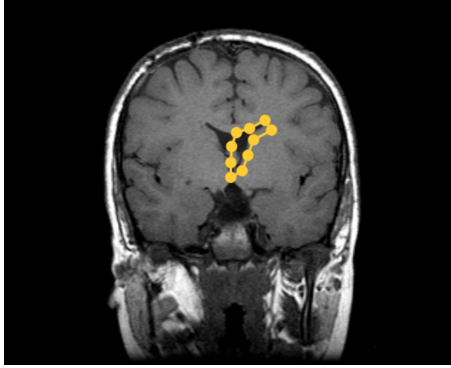


Figure 5: Hard difficulty DICOM annotated image.

Phase	Order 1	Order 2
1	Trn (M)	Trn (T)
2	Tst (M)	Tst (T)
3	Q (M)	Q (T)
4	Trn (T)	Trn (M)
5	Tst (T)	Tst (M)
6	Q (T)	Q (M)
7	QF	QF

Table 1: Study Ordering. Both Conditions (Tst (M) = Mouse Test, Tst (T) = Touch Test) took 5 minutes. Training (Trn) and Questionnaire (Q) took less than 1 minute. Participants complete a final questionnaire (QF = Final Questionnaire) that took less than 5 minutes.

¹Here, the ϵ is the diameter of the annotation point.

EVALUATION

Table 1 shows the order of the user (radiologist) tests. It can be seen that the “Order 1” column is the opposite regarding the “Order 2” column. In the “Order 1” column, the user trains on the mouse-based environment (Trn(M) in Table 1), then executes a set of pre-defined tests (Tst(M) in Table 1), followed by a questionnaire (Q(M)). The QF in the table, is related to a questionnaire that concerns issues such as the environment, functionality usability and seasickness issues among others. This procedure is then repeated for the touch environment. In the “order 2” column is similar, with the users training and performing their tasks in the touch setting first. Half of the users first perform the mouse and keyboard test, and the other half perform first the touch tests.

Task

Radiologists interact with this user interface by doing some annotations in certain regions of interest areas of the image. The images are chosen to be representative to the domain field and to understand the different levels of the difficulty in these images. In our work, the first task is to perform the annotations on the DICOM Image along with the brain lesion near of the cortex, as we can see on Figure 3 and Figure 4. The second image is almost similar of the first one (just a different frame) so the task is mainly the same. The last image we put radiologists doing some more difficult annotation as it is shown in Figure 5.

Measures

The following scales are considered: (i) Starting by the Positive and Negative Affect Scale [9] (PANAS), (ii) Intrinsic Motivation Inventory [6] (IMI) and (iii), Experience Needs Satisfaction [1] (ENS). When we achieve the end of the condition, radiologists are asked to provide information and rank each condition, providing any comments.

Performance. We measure accuracy by computing the Hit Rate Score (HRS). This measure is defined has the percentage of annotations that lie on three areas (Figure 6). These three areas are measured from the ground-truth (see black line in Figure 6). The first area, **Area A**, is the area delimited by the two **Green Lines**, having a width of 2ϵ , where ϵ is the perpendicular distance from a point in the ground truth (black line) to the **Green Line**¹. The second area, **Area B**, has also a width of 2ϵ . However, **Area B** embraces two regions, each region falling between the **Green Lines** (inner boundary) and **Red Lines** (outer boundary).

User Experience. To evaluate the user experience we embed, the IMI [6], PANAS [9] and ENS [1] measures in a 5-point Likert-scales, ranging from 1 (strongly disagree) to 5 (strongly agree).

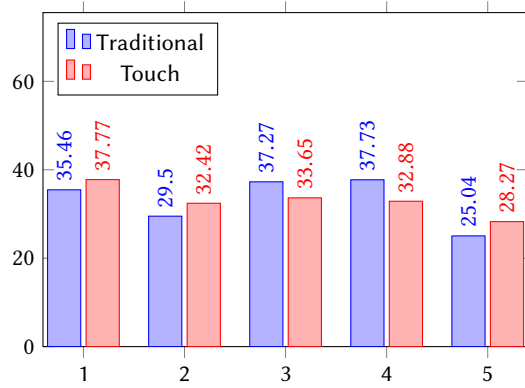


Table 2: Kruskal-Wallis.

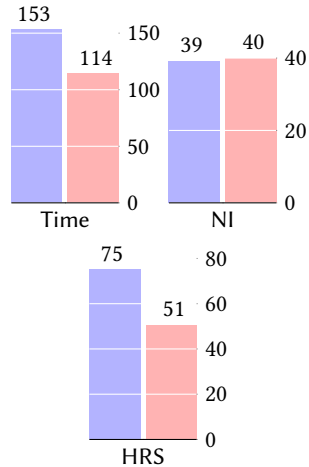


Table 3: Time Performance Mean; Number of Interactions (NI) Mean; Hit Rate Score (HRS) Mean.

²_{env}: environment (*env*) with both traditional (*tra*) and touch (*tou*) options;

χ^2_{env} : Chi-Square of the environment (*env*);

α_{env} : Alpha value of the environment (*env*);

RESULTS

Since the data collected does not meet the applicability pre-conditions required for ANOVA, i.e., does not follow a Gaussian distribution and also the number of samples is small, we resort to use the Kruskal-Wallis Analysis of Variance [8] to test the performance and experience that is useful for testing between-subjects effects for three or more conditions [5].

Figure 2 shows the overall results of the Kruskal-Wallis test. This result shows that all the mean differences for each of the radiologists is significant in the above 11 conditions (see Figures 3, 4 and 5)

A small number of radiologists is used in the tests. Three of the five radiologists (1, 2 and 5) have shown that touch environment is better classified then traditional environment. Although, we must consider and understand the other two radiologist (3 and 4) results. The Kruskal-Wallis test²revealed that radiologists have a significant main effect on touch environment ($\chi^2_{tou} = 1.711$, $\alpha_{tou} = 0.789$), against traditional environment ($\chi^2_{tra} = 4.587$, $\alpha_{tra} = 0.332$).

In the following sections (Figure 2 - Figure 5) we describe the results in terms of the first and second order statistics, using the mean (M_{env}) and standard deviation (σ_{env}), as well as the standard error of the mean³that is defined as:

$$sem_{env} = \sigma_{env} / \sqrt{N}$$

Performance

Figure 3 shows the mean time performance of the tasks as described in section Task.

Time. A significant main effect of the traditional input environment ($M_{tra}=153.4s$, $\sigma_{tra}=40.88$, $sem_{tra}(\bar{x}) = 18.28$) with radiologist maximum time spent of 210 seconds and radiologist minimum time spent of 109 seconds. For the touch input environment ($M_{tou}=114.20s$, $\sigma_{tou}=51.71$, $sem_{tou}(\bar{x}) = 23.12$) the radiologists take less time.



Number of Interactions (NI). The mean of the interactions on traditional ($M_{tra}=39.20$) is less than the touch environment ($M_{tou}=40$).

Hit Rate Score (HRS). It is shown that the HRS in traditional environment ($M_{tra}=75.2$, $\sigma_{tra}=22.72$, $sem_{tra}(\bar{x}) = 10.16$), has a higher value then touch environment ($M_{tou}=50.6$, $\sigma_{tou}=15.35$, $sem_{tou}(\bar{x}) = 6.86$).

User Experience

Responses to the final questionnaire suggest that both interactions are adequate for analyzing medical images. Moreover, no radiologist reported discomfort, dizziness or fatigue in neither environments.

Motivational. The motivational results are presented as *Competence*, *Autonomy*, *Relatedness* and *Immersion* (Figure 4) options.

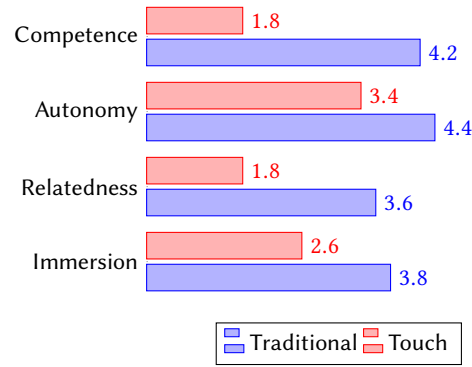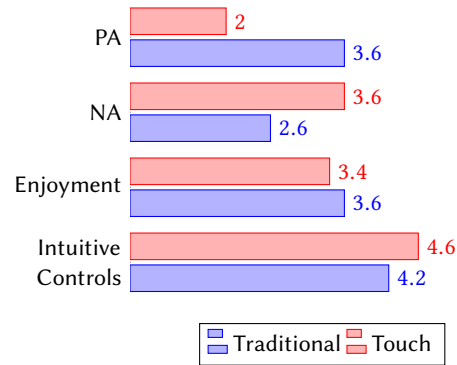**Table 4: Motivation Experience****Table 5: Overall Pleasure and Enjoyment of the Task**

Competence. The main outcome on traditional environment ($M_{tra}=4.2$, $\sigma_{tra}=0.83$, $sem_{tra}(\bar{x}) = 0.37$), has shown that radiologists feel more comfortable in traditional environment, as it can be expected. On the other hand, for touch environment ($M_{tou}=3.4$, $\sigma_{tou}=1.67$, $sem_{tou}(\bar{x}) = 0.74$), radiologists showed a rated above average, however, lower than traditional environment.

Autonomy. The traditional environment reflected ($M_{tra}=4.4$, $\sigma_{tra}=0.89$, $sem_{tra}(\bar{x}) = 0.4$) a high average level of autonomy with three radiologists choosing a $max(x_{tra}) = 5$. For the touch environment we also have values above average ($M_{tou}=3.4$, $\sigma_{tou}=1.14$, $sem_{tou}(\bar{x}) = 0.5$), we also have a $max(x_{tou}) = 5$ but just one radiologist scored this value.

Relatedness. Radiologists relatedness show us a touch environment below the average ($M_{tou}=1.8$, $\sigma_{tou}=0.44$, $sem_{tou}(\bar{x}) = 0.2$), where the $max(x_{tou}) = 2$ and the $min(x_{tou}) = 1$. On the other hand, the traditional environment the mean ($M_{tra}=3.6$) is above average of the touch environment.

Immersion. For motivational experience, the immersion values of traditional environment are ($M_{tra}=3.8$, $\sigma_{tra}=1.3$, $sem_{tra}(\bar{x}) = 0.58$). Here, we have a $max(x_{tra}) = 5$ and the $min(x_{tra}) = 2$, however two radiologists voted $x_{tra} = 5$ the mean value ($M_{tra}=3.8$) was not that high. The touch environment provided ($M_{tou}=2.6$, $\sigma_{tou}=1.51$, $sem_{tou}(\bar{x}) = 0.67$).

Pleasure and Enjoyment. We present the results of *Affect*, *Enjoyment* and *Intuitive Controls* (Figure 5).

Affect. The affecting computing has placed an emphasis on understanding the affective and cognitive-affective responses that radiologists have to their technological interactions. Traditional environment is perceived as more positive ($M_{tra}=3.6$, $\sigma_{tra}=0.54$, $sem_{tra}(\bar{x}) = 0.24$), whereas the marginal negative affect for traditional environment ($M_{tra}=2.6$, $\sigma_{tra}=0.54$, $sem_{tra}(\bar{x}) = 0.24$) showed a typical correlation. The touch environment is perceived as more negative ($M_{tou}=2$, $\sigma_{tou}=0.7$, $sem_{tou}(\bar{x}) = 0.31$) then positive ($M_{tou}=3.6$, $\sigma_{tou}=1.14$, $sem_{tou}(\bar{x}) = 0.5$).

Enjoyment. Intrinsic motivation is foundations of the enjoyment of interactive experiences, and can be attributed to volition and achievement inherent in the person. The traditional environment provides ($M_{tra}=3.6$, $\sigma_{tra}=1.14$, $sem_{tra}(\bar{x}) = 0.51$) which is almost the same as in the touch environment ($M_{tou}=3.4$, $\sigma_{tou}=1.67$, $sem_{tou}(\bar{x}) = 0.74$).

Intuitive Controls. Controls are intuitive when they do not interfere with one's sense of presence being easily mastered. For the intuitive controls the overall system was high rated by radiologists, however the behavior of traditional environment ($M_{tra}=4.2$, $\sigma_{tra}=0.44$, $sem_{tra}(\bar{x}) = 0.2$) was less 8% than touch environment ($M_{tou}=4.6$, $\sigma_{tou}=0.54$, $sem_{tou}(\bar{x}) = 0.24$).

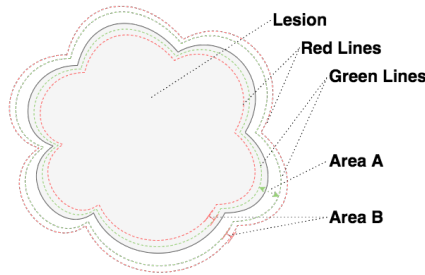


Figure 6: Annotation Classification Areas.

3N : the number of users (radiologists);

sem_{env} : standard error of the mean for the environment (env);

M_{env} : mean value of the environment env ;

σ_{env} : standard deviation of the environment env ;

ACKNOWLEDGMENTS

We would like to thank the Hospital Fernando Fonseca (HFF) for the collaboration. I would specially like to thank the Doctors Clara Aleluia, Gisela Andrade, Willian Schmitt and Ana Sofia Germano from the HFF for the generous support and medical expertise. My appreciation goes also to Bruno Cardoso and Bruno Dias for help and above all for the good companionship. Thanks to Professors Daniel Simões Lopes and Daniel Mendes for the support. Last but not least, thank to Joana Teixeira and Lúcia Freitas for the feedback. This work was partially supported by Fundação para a Ciência e a Tecnologia (FCT) and Instituto Superior Técnico (IST) through the FCT/UID/EEA/50009/2013 project, BL89/2017-IST-ID grant.

REFERENCES

- [1] Anja Broeck, Maarten Vansteenkiste, Hans Witte, Bart Soenens, and Willy Lens. 2010. Capturing autonomy, competence, and relatedness at work: Construction and initial validation of the Work-related Basic Need Satisfaction scale. *Journal of Occupational and Organizational Psychology* 83, 4 (2010), 981–1002.
- [2] Septimiu Crisan and Ioan Gavril Tarnovan. 2013. Optimization of a multi-touch sensing device for biomedical applications. In *Advanced Engineering Forum*, Vol. 8. Trans Tech Publ, 545–552.
- [3] Kunio Doi. 2005. Current status and future potential of computer-aided diagnosis in medical imaging. *The British journal of radiology* 78, suppl_1 (2005), s3–s19.
- [4] Kunio Doi. 2007. Computer-aided diagnosis in medical imaging: historical review, current status and future potential. *Computerized medical imaging and graphics* 31, 4 (2007), 198–211.
- [5] Daniel McFarlane. 2002. Comparison of four primary methods for coordinating the interruption of people in human-computer interaction. *Human-Computer Interaction* 17, 1 (2002), 63–139.
- [6] Richard M Ryan. 1982. Control and information in the intrapersonal sphere: An extension of cognitive evaluation theory. *Journal of personality and social psychology* 43, 3 (1982), 450.
- [7] Eric J Seibel. 2005. Medical imaging, diagnosis, and therapy using a scanning single optical fiber system. (Dec. 13 2005). US Patent 6,975,898.
- [8] Elvar Theodorsson-Norheim. 1986. Kruskal-Wallis test: BASIC computer program to perform nonparametric one-way analysis of variance and multiple comparisons on ranks of several independent samples. *Computer methods and programs in biomedicine* 23, 1 (1986), 57–62.
- [9] David Watson and Lee Anna Clark. 1999. The PANAS-X: Manual for the positive and negative affect schedule-expanded form. (1999).
- [10] Diane Watson, Mark Hancock, Regan L Mandryk, and Max Birk. 2013. Deconstructing the touch experience. In *Proceedings of the 2013 ACM international conference on Interactive tabletops and surfaces*. ACM, 199–208.