CATH PLAN · Case 4

70F, 66 kg · scheduled 11:30 · PCI to mid-RCA (inferior STEMI, day 2) · pathway: known intervention

Synthetic teaching content. Not clinical advice. Not a medical device. DRAFT for the chair to rule on.

Thresholds: PROPOSED values, not yet verified by the chair. Template logic (likelihood weights and bands, prep rules, Imaging triggers, Heart Team factors, stage assignment, Labs' eGFR cutoff) is also unreviewed.

4
flags from 4 agents

1.3
contrast ratio (Laskey 2007 discriminator 3.7, not a limit)

1 / 4
angio findings flagged (calcium, flow, bifurcation, multivessel)

0
devices out of stock

Contrast ratio = planned contrast (mL) ÷ eGFR; by Cockcroft-Gault creatinine clearance (61 mL/min, actual weight) it is 1.7, the basis the published cutoffs used. The published ratios use creatinine clearance, not eGFR (docs/EVIDENCE.md E1, E2): risk was flat below 2 and rose above 3 (Gurm 2011) and 3.7 was a discriminating cutoff (Laskey 2007). The plan shows both the eGFR ratio and, when age, sex, weight and creatinine are in the packet, a Cockcroft-Gault ratio, and applies the cutoffs to the higher. No guideline sets a limit; the chair confirms the basis.

Lesion map (Imaging)


Lesion	Vessel	Stenosis	TIMI	Calcium	Flag
L1	mid-RCA	95%	TIMI 1	calcium none	none

Triggers: TIMI flow below 3. · Cath report: indication inferior STEMI with persistent symptoms; access radial; hemodynamics not recorded

Rules that fired

- No template rule fired; read the agents' flags below. The rules are proposed, and no rule firing is not clearance.

Angiographic findings (synthetic)

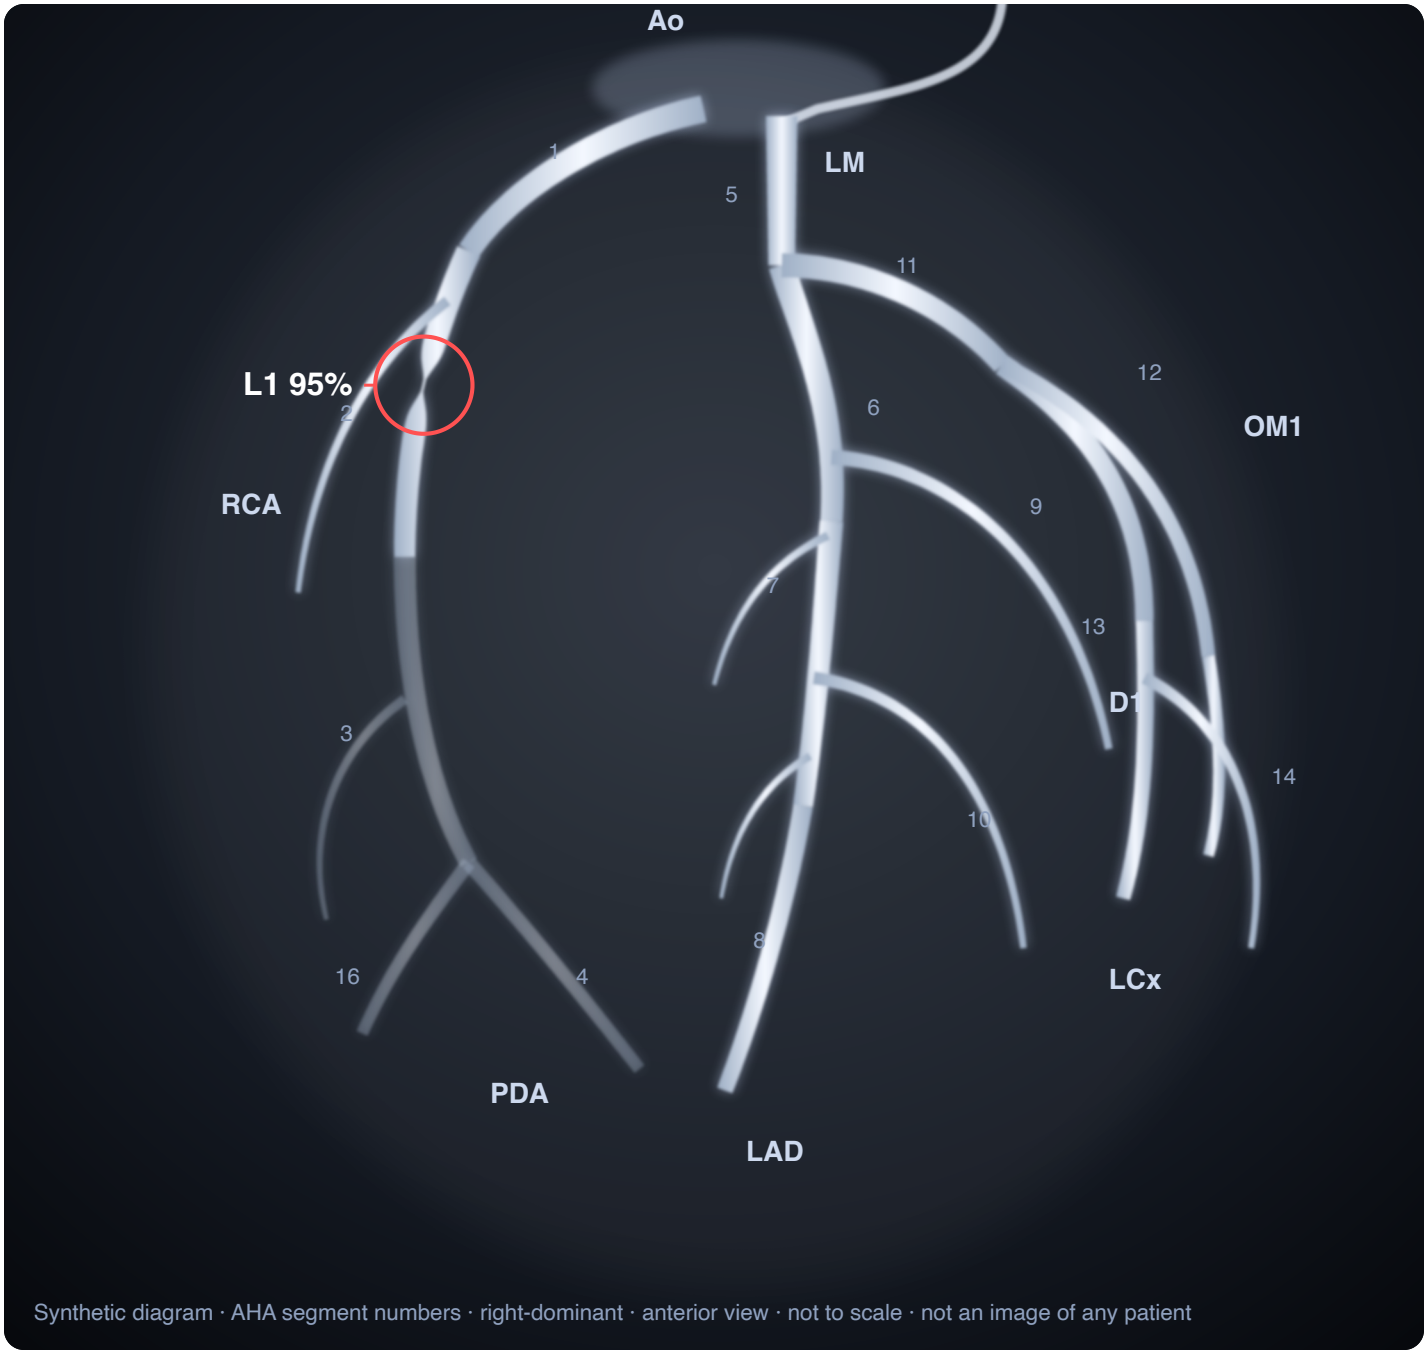

L1 · mid-RCA (AHA segment 2)
95% stenosis · TIMI 1 (poor filling: the distal vessel is drawn very faint) · calcium none · flag none

Drawn from the angio lines in the packet by tools/angio.py: right-dominant tree, anterior view, AHA segment numbers, lumen narrowed to the stated percentage, calcium shown as bright specks, distal filling dimmed when TIMI flow is below 3. Solid red ring = stenosis of 70% or more; dashed amber ring = under 70%, or a CCTA estimate not yet confirmed. A Medina 1,1,1 flag is drawn as a narrowing of about half the proximal LAD and LCx. A teaching diagram, not an image of any patient and not to scale.

Equipment manifest

Item (from the packet)	Stock
6F guide	4 on hand
support wire	4 on hand
NC balloon 3.0 mm	2 on hand
DES 3.5x24 mm	3 on hand
standard PCI tray	4 on hand

Prep check (devices against findings)

Scope	Stage the devices named in the packet
Stock	all named devices in stock

On the shelf, by class (from the STOCK line)	
Guide catheters	6F guide 4, 7F guide 2
Diagnostic catheters	5F diagnostic catheters 8
Wires	support wire 4
Balloons	NC balloon 3.0 mm 2, NC balloon 3.5 mm 2
Stents (DES)	DES 3.5x24 mm 3, DES 3.5x28 mm 2, DES 3.0x18 mm 0 (no resupply scheduled)
Intravascular imaging	IVUS catheter 1
Support devices	Impella CP 0 (no resupply scheduled)

Questions for the chair (the plan asks, it does not choose a device):

- None: every check passed.

Flags from the agents

Imaging
- TIMI below 3 · L1 mid-RCA 95% TIMI 1

Labs
- Plt 82 vs ref 150-400

Meds
- history "heparin infusion stopped overnight" · med list "heparin infusion running (last aPTT 91 s at 05:15)"
- heparin infusion running · PCI to mid-RCA, radial access

Equipment ✅ nothing flagged

Relay: Imaging → Equipment, Labs → Meds.

Summary and approvals

Ruling recorded	none yet
Flags	Imaging 1 · Labs 1 · Meds 2 · Equipment 0
Rules that fired	No template rule fired; read the agents' flags below. The rules are proposed, and no rule firing is not clearance.

For the chair to decide / check (the agents only flag):

- Thresholds in thresholds.json are proposed: the chair verifies them before this plan is used.
- Template logic (likelihood weights and bands, prep rules, Imaging triggers, Heart Team factors, stage assignment, Labs' eGFR cutoff) is unreviewed.

Approvals

No approval decisions recorded yet.

For the chair's use: print and mark.

- ☐ Approve as drafted
- ☐ Chair changes the plan (record the change)
- ☐ Equipment issue noted

Status

This draft is not approved until the chair presses Allow once on the Switch card.

AWAITING CHAIR

Sources: packet (day2.md) · briefs from Imaging, Labs, Meds, Equipment · thresholds.json · evidence table docs/EVIDENCE.md (E1 to E16, mostly secondary summaries, chair verifies). Generated 2026-11-04 09:00 by plan.py (template, no model).
Provenance: template 7b83bc09dd · thresholds bea3b78f4a · plan.py fa5860885c · packet id n/a. "ref:" on a flag names a published criterion; it is not an instruction, and the criteria are unverified until the chair has checked them against the sources (docs/EVIDENCE.md).