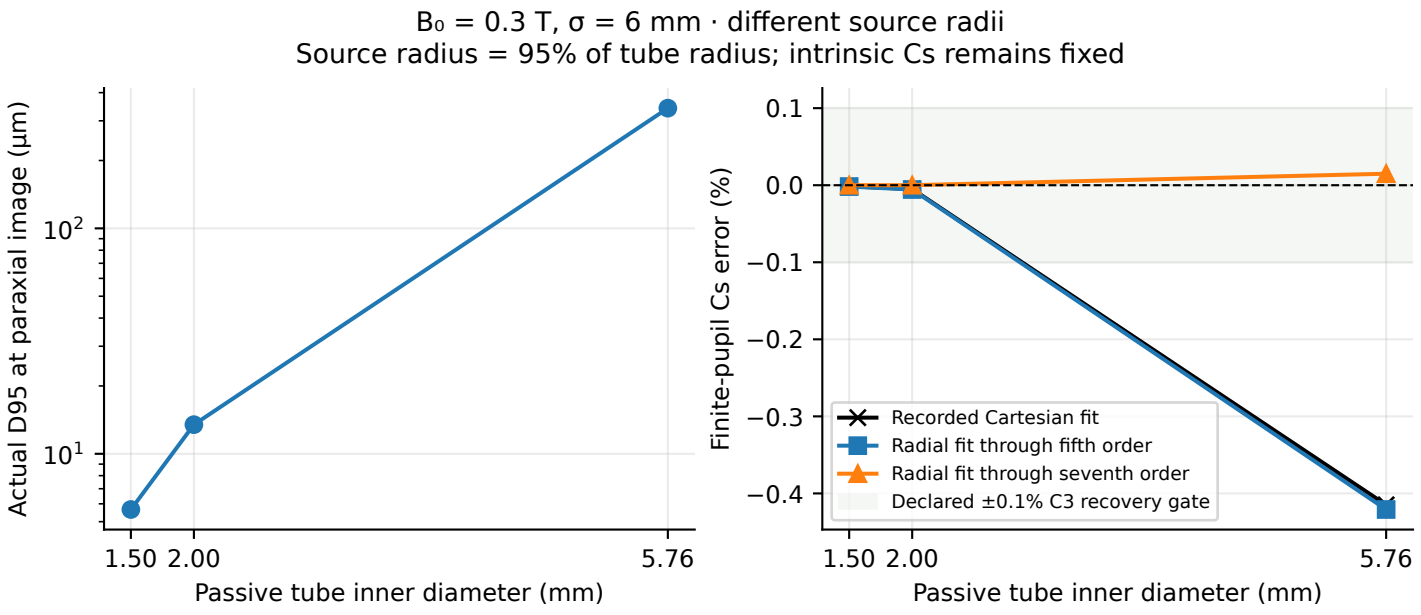
B₀ = 0.3 T, σ = 6 mm · different source radii
Source radius = 95% of tube radius; intrinsic Cs remains fixed
Actual D95 at paraxial image (μm)
10^2
10^1
1.50
2.00
5.76
Passive tube inner diameter (mm)
Finite-pupil Cs error (%)
0.1
0.0
−0.1
−0.2
−0.3
−0.4
Recorded Cartesian fit
Radial fit through fifth order
Radial fit through seventh order
Declared ±0.1% C3 recovery gate
1.50
2.00
5.76
Passive tube inner diameter (mm)