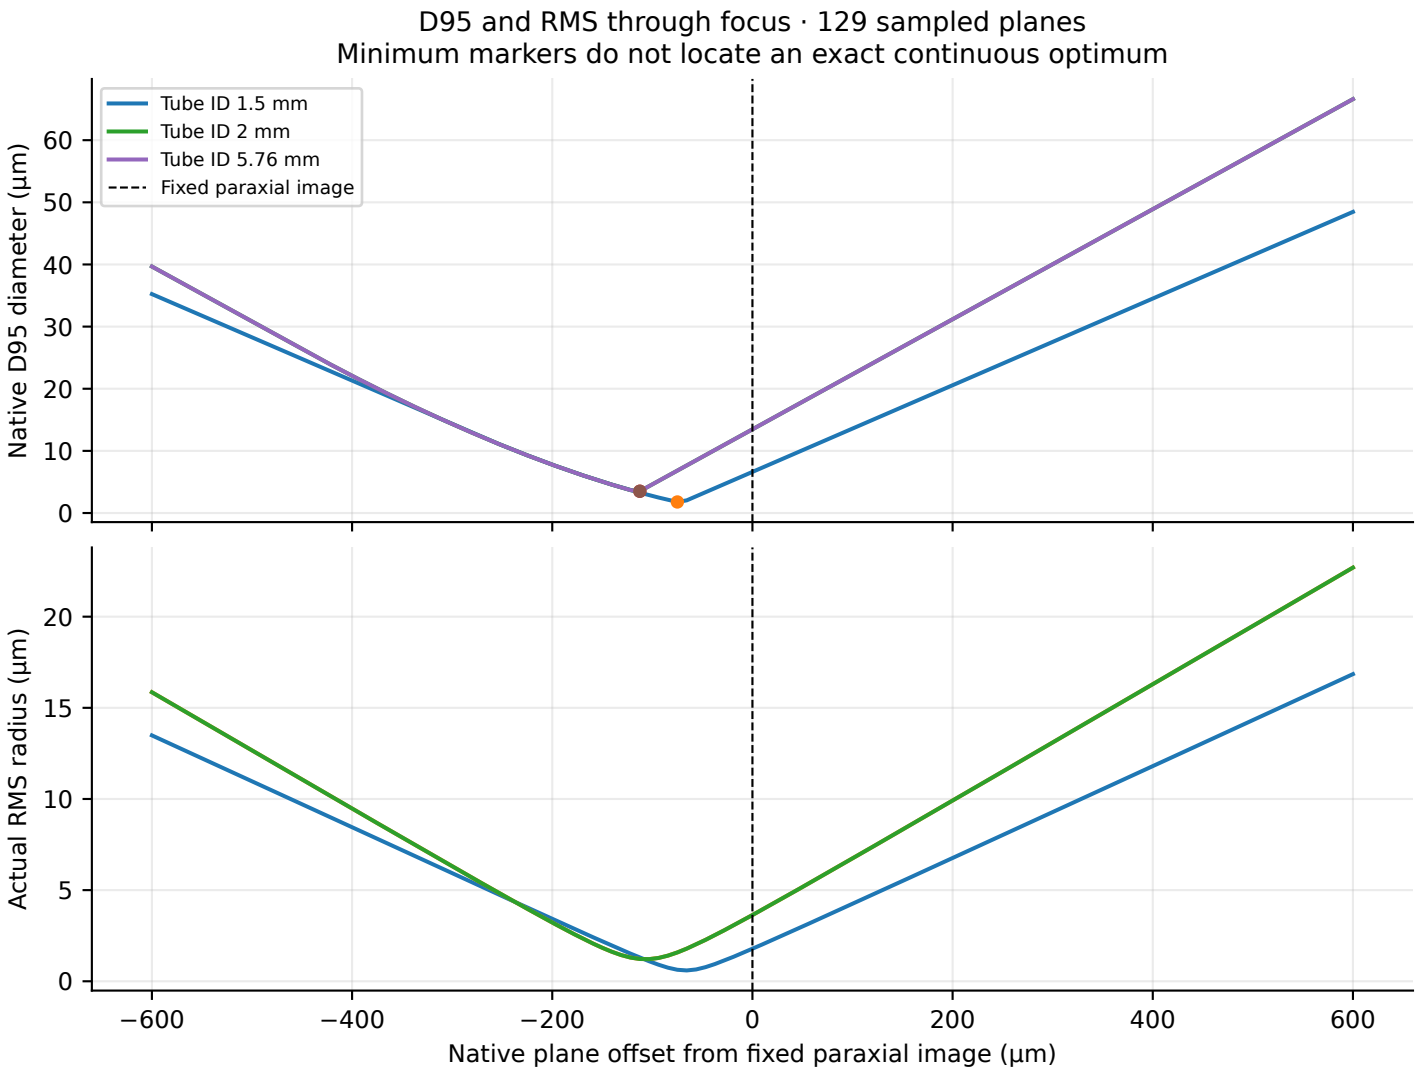
D95 and RMS through focus · 129 sampled planes
Minimum markers do not locate an exact continuous optimum
Tube ID 1.5 mm
Tube ID 2 mm
Tube ID 5.76 mm
Fixed paraxial image
Native D95 diameter (µm)
Actual RMS radius (µm)
Native plane offset from fixed paraxial image (µm)
0
10
20
30
40
50
60
5
15
−600
−400
−200
200
400
600