

Acousto-Optical Tunable Filter Atmospheric Imager for Determination of Aerosol Extinction

Brenden J Elash, Adam E Bourassa, Douglas A Degenstein, Paul(?)

March 26, 2015

1 Introduction

Purpose behind ALI - history of limb measurements - aerosol measurement and why we need them

2 Instrument Design

2.1 Acousto-Optical Tunable Filter

Start with background of AOTF theory (momentum matching etc) then Cover the rational for picking the wavelength range that was used for the AOTF as well the the significance of the testing results.

2.2 Optical Design and Performances

Outline optical layout and rational for picking it with regard to aerosol concentrations optical characteristics. Final results and expected resolutions and wavelength

3 Stratospheric Balloon Flight

3.1 Flight Day Conditions and Flight Path

As the title says

3.2 Measurements

How measurements are made. Processing from level 0 -> level 1

3.3 Retrievals

The method on how the retrievals are transferred from level 1 data to aerosol profiles (level 2). (MART method with OMPS algorithm for particle size)

3.4 results

What the final measurements showed and how they compare to SOLAMON and OSIRIS

4 Conclusions and Future Prospects

Self explanatory.

Figure for Measurement and retrieval section not completed yet.

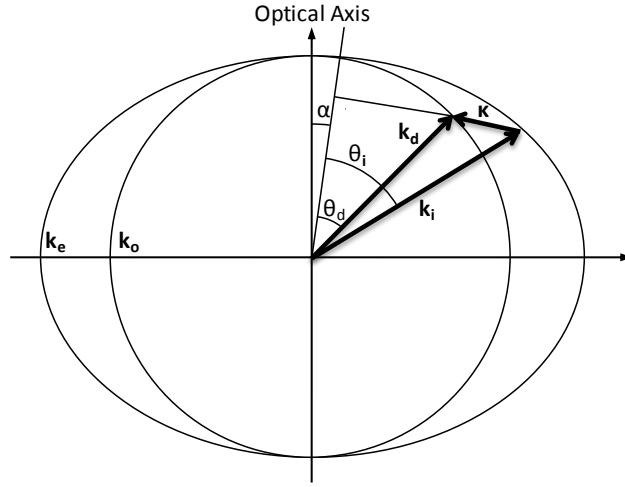


Figure 1: The wave vectors generated by the AOTF experiment set up in ???. From the above figure k_e and k_o are the wave vectors of the extraordinary and ordinary axis of the AOTF crystal and can be represented as $2\pi n_e/\lambda$ and $2\pi n_o/\lambda$ respectively. The cut angel, α , is the cut angle form the optional axis to the piezoelectric transducer.

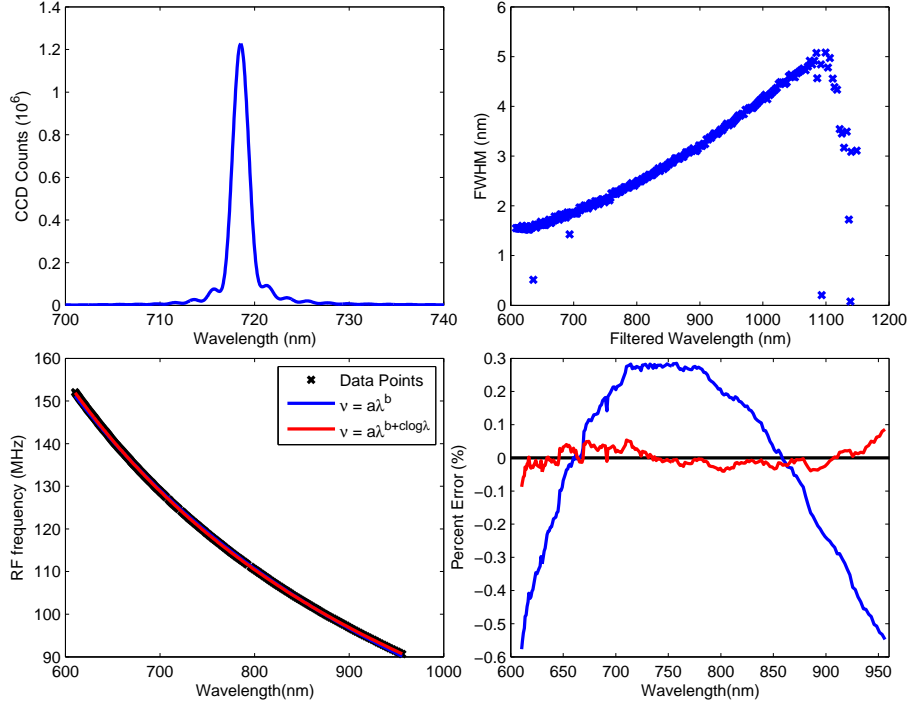


Figure 2: Top Left: A standard image taken from the AOTF calibration experiment when the tuning frequency of the AOTF was at 124.96 MHz. Top Right: The FWHM for each of the determined wavelengths for the AOTF. It should be noted that the FWHM at 600 nm is 1.5 and as the wavelengths get longer the FWHM increases to 4.9 at 1080 nm. Bottom Left: The calibration curves for the AOTF RF versus the diffracted wavelength which contains the data points recorded and two best fit curves. Bottom Right: The percent error with respect to the measured frequency for the two best fit curves in the previous panel. It can be noted the modified power function approximates the AOTF wavelength dependance to within 0.1%.

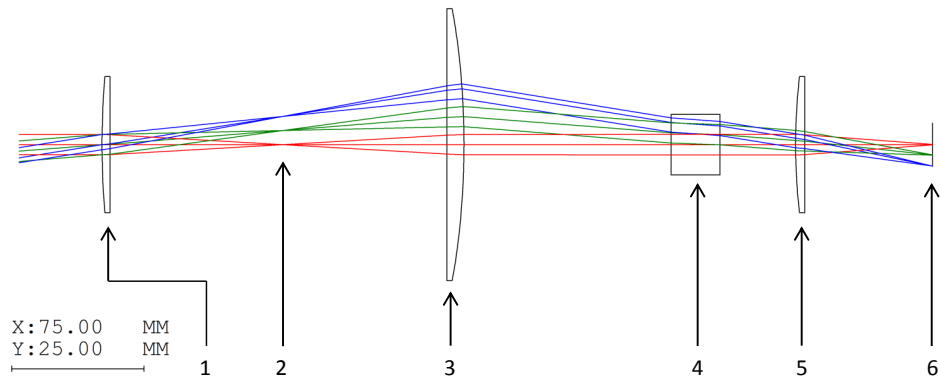


Figure 3: Ray Tracing diagram of the telescopic lens system simulated by Code V. The elements in the system are the following: (1) 100 mm focal length plano-convex lens. (2) Location where shutter will be located to limit stray light (3) 100 mm focal length plano-convex lens. (4) Brimrose AOTF characterized in ???. (5) 75.6 mm focal length plano-convex lens. (6) Imaging plane. It should be noted that the x and y scales are not the same in this image. Also, in the lab a polarizer is added in front and behind the AOTF as well as prisms behind the AOTF.