


N4 — Hallucination guard ablation

Detection quality (n=168 cases)



Recall on visual-only corruptions (n=25)

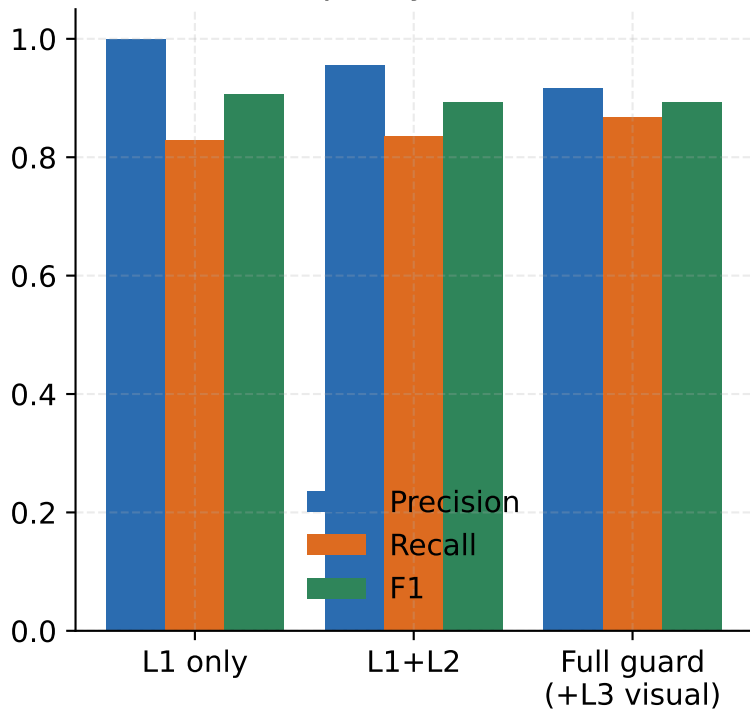