

Clinician Efficiency & Device Health



8,425

2 Hour SLA Breaches


19.8%

Overall SLA Compliance


54.2%

Critical SLA Compliance


Clinician Alert Volume with SLA Compliance

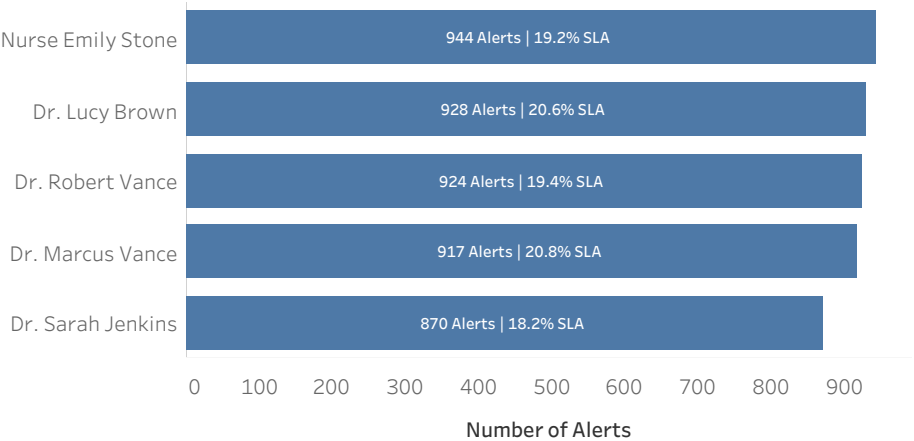

Average Response Time by Alert Severity (Hours)

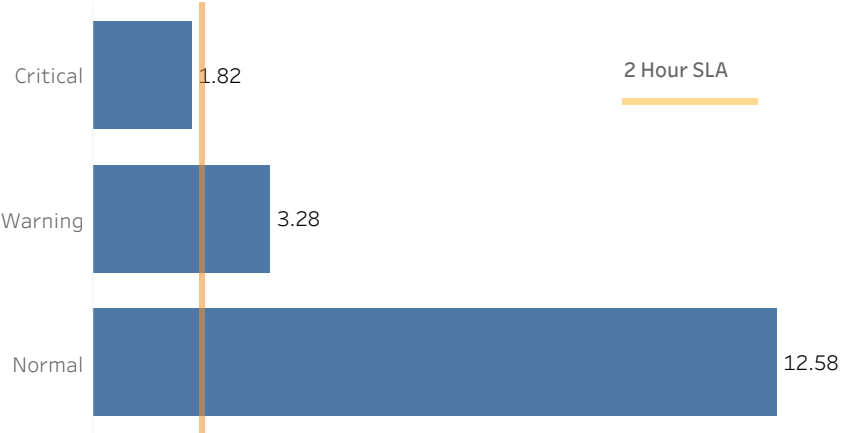

Warning Alerts per Device

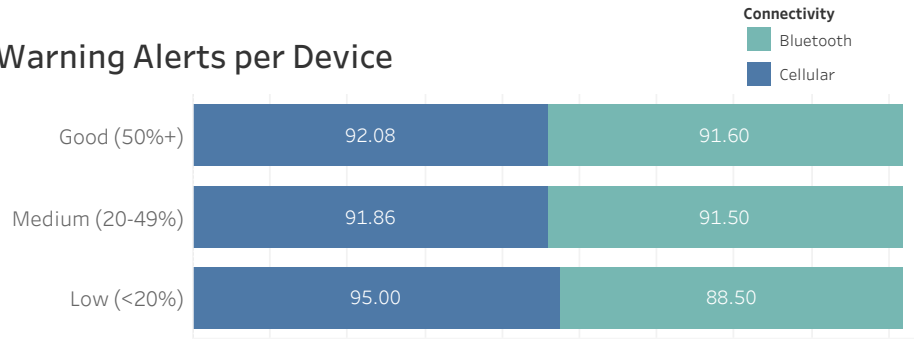

Average Response Time by Hub (Hours)

