

VoltCycle: Cyclic Voltammetry Data Visualization and Analysis

Chowdhury Ashraf², Theresa Gozzo⁴, Keertana Krishnan^{1,3}, Jaime Rodriguez², Sabiha Rustam^{1,2}

¹University of Washington DIRECT Program, ²Department of Chemical Engineering,

³Department of Materials Science & Engineering, ⁴Department of Chemistry
University of Washington, Seattle, Washington, 98195



An interactive data visualization and analytics tool for determining electrochemical reversibility from automated batch cyclic voltammetry


MOTIVATION

Introduction:

Cyclic Voltammetry (CV) is an electrochemical technique utilized to measure the current that develops in a cell under excess voltage. This method enables the classification of materials to determine if they are optimal for use in batteries. Currently, with the mass production of data, CV analysis is a time consuming procedure, where each raw file has to be analyzed individually. The purpose of this project is to develop a tool for high throughput analysis, that is able to draw relevant information from multiple data files with relatively minimized user input.

Objectives:


1. Data Mining and Cleaning
 - Read raw data files from Gamry
 - Parse required data for analysis
2. Data Visualization
 - Create an interface for visualization
 - based on user inputs
3. Classification
 - Collect pertinent information
 - Classify reversibility of the material
4. Machine Learning

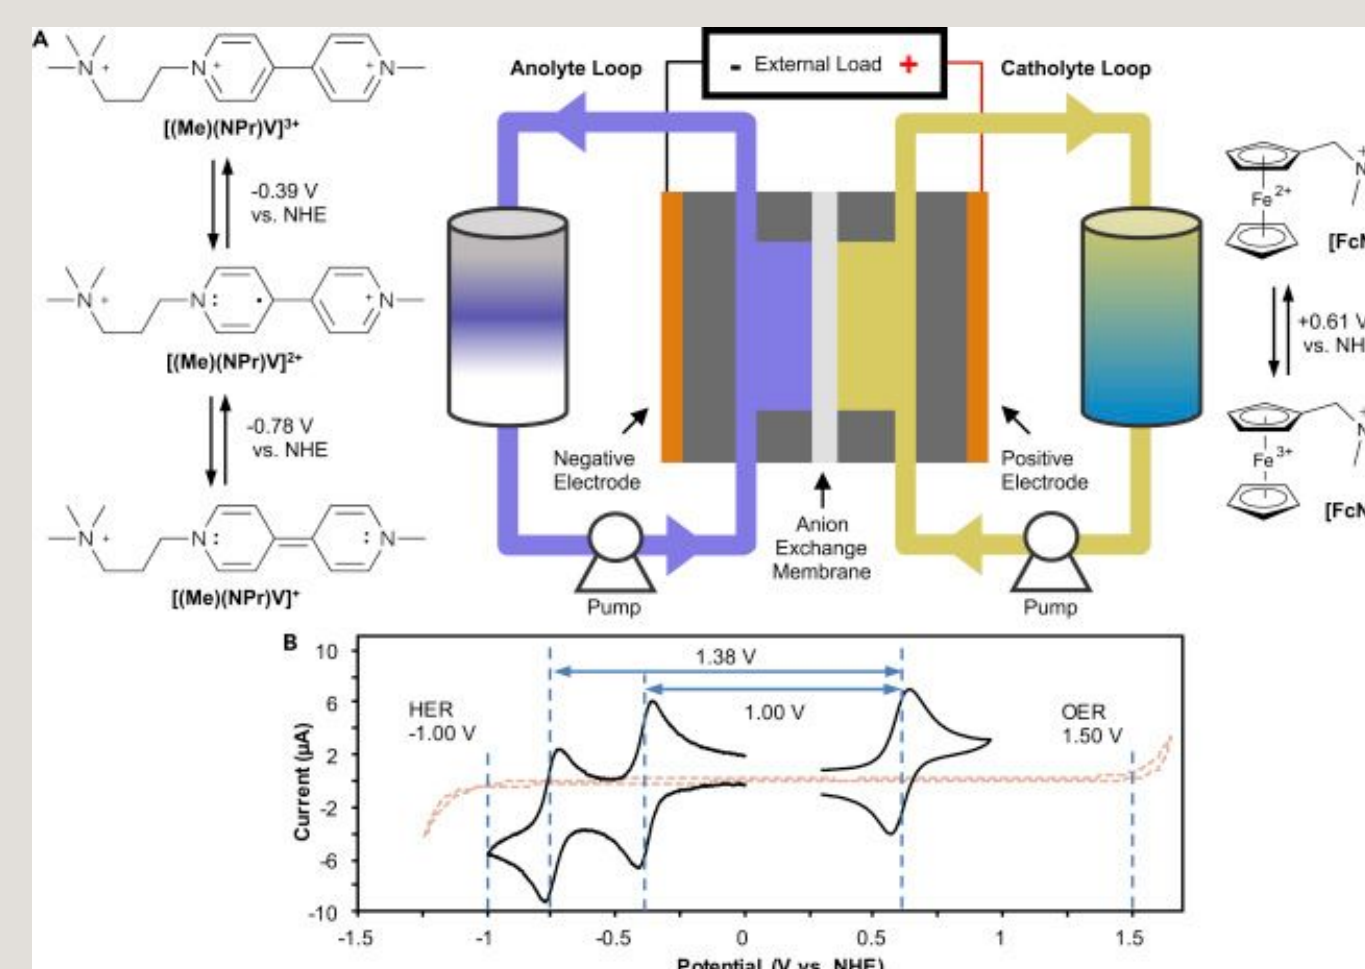

BACKGROUND


Fundamentals:

Voltammetry is an experimental method in which an analytic solution is exposed to two electrodes. When the voltage is manipulated on one of the electrodes, current flow is observed and the voltage required for electron transfer is determined. In cyclic voltammetry, the potential is swept in one direction and then reversed till the starting value is reached. This range delivers the potential window. Such experiments give thermodynamic and kinetic information on electron transfer for different analytes.

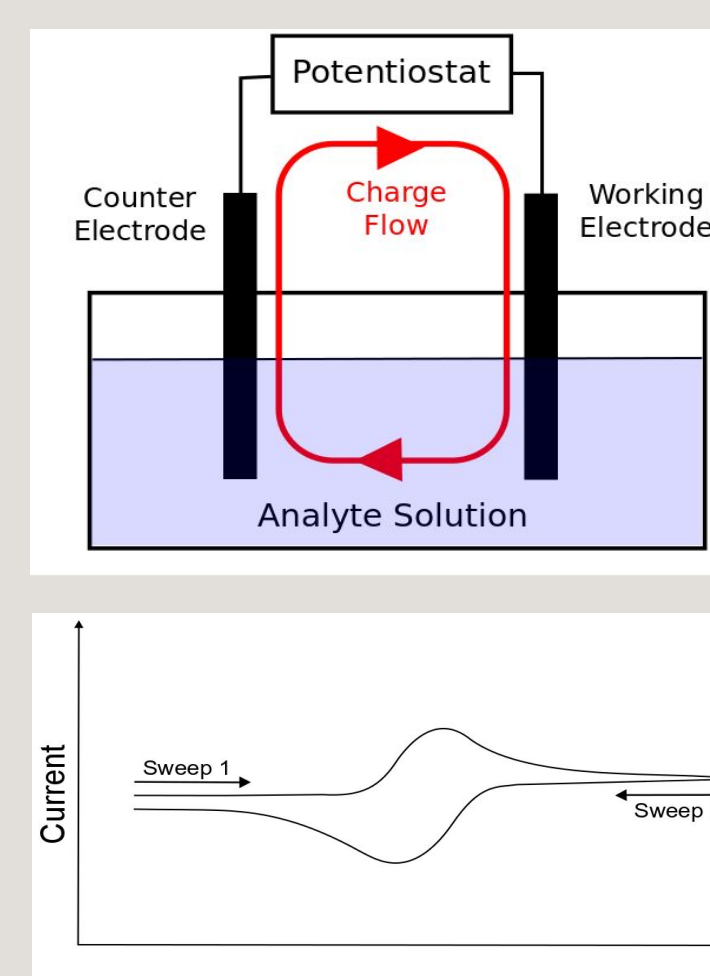

Notable values to determine reversibility:


- Peak potentials (E_{pa} , E_{pc})
- Peak-to-peak separation (ΔE_p)
- Peak Currents (Adjusted baselines, I_{pa} , I_{pc})
- Peak Current Ratio (I_{pa}/I_{pc})

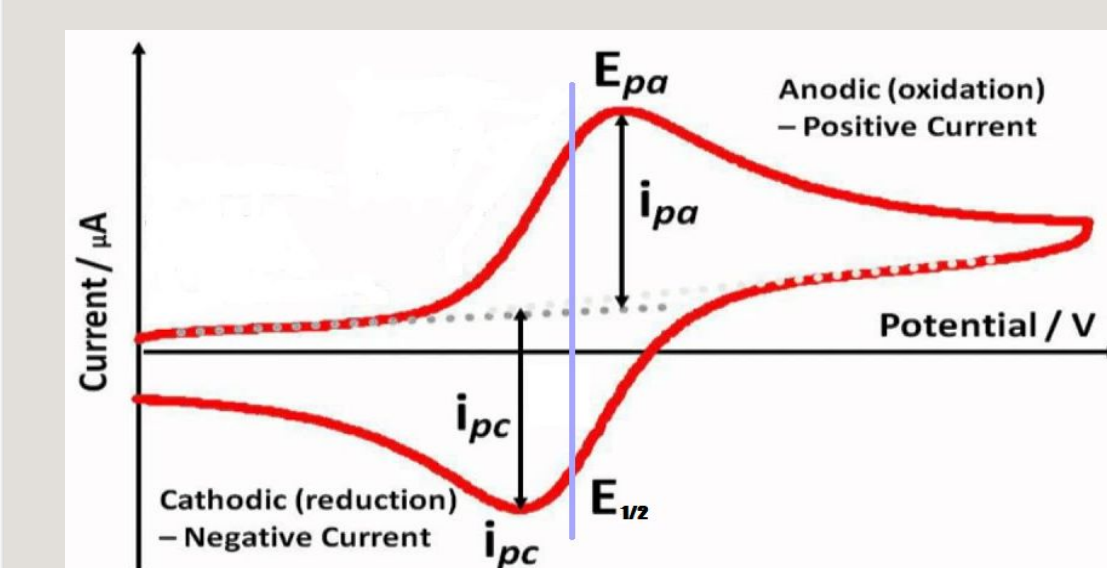

Important factors to consider:

- For completely reversible electron transfer, the peak potentials will not change with different scan rates
- Ideal peak separation at 25°C is 59mV for one electron wave CV (reversible)
- Peak:current ratio should be approximately 1
- Both analytes and catholytes are necessary for a functioning battery
 - Positive standard reduction potential ($E_{1/2}$) - catholyte (vice versa)

WORKFLOW

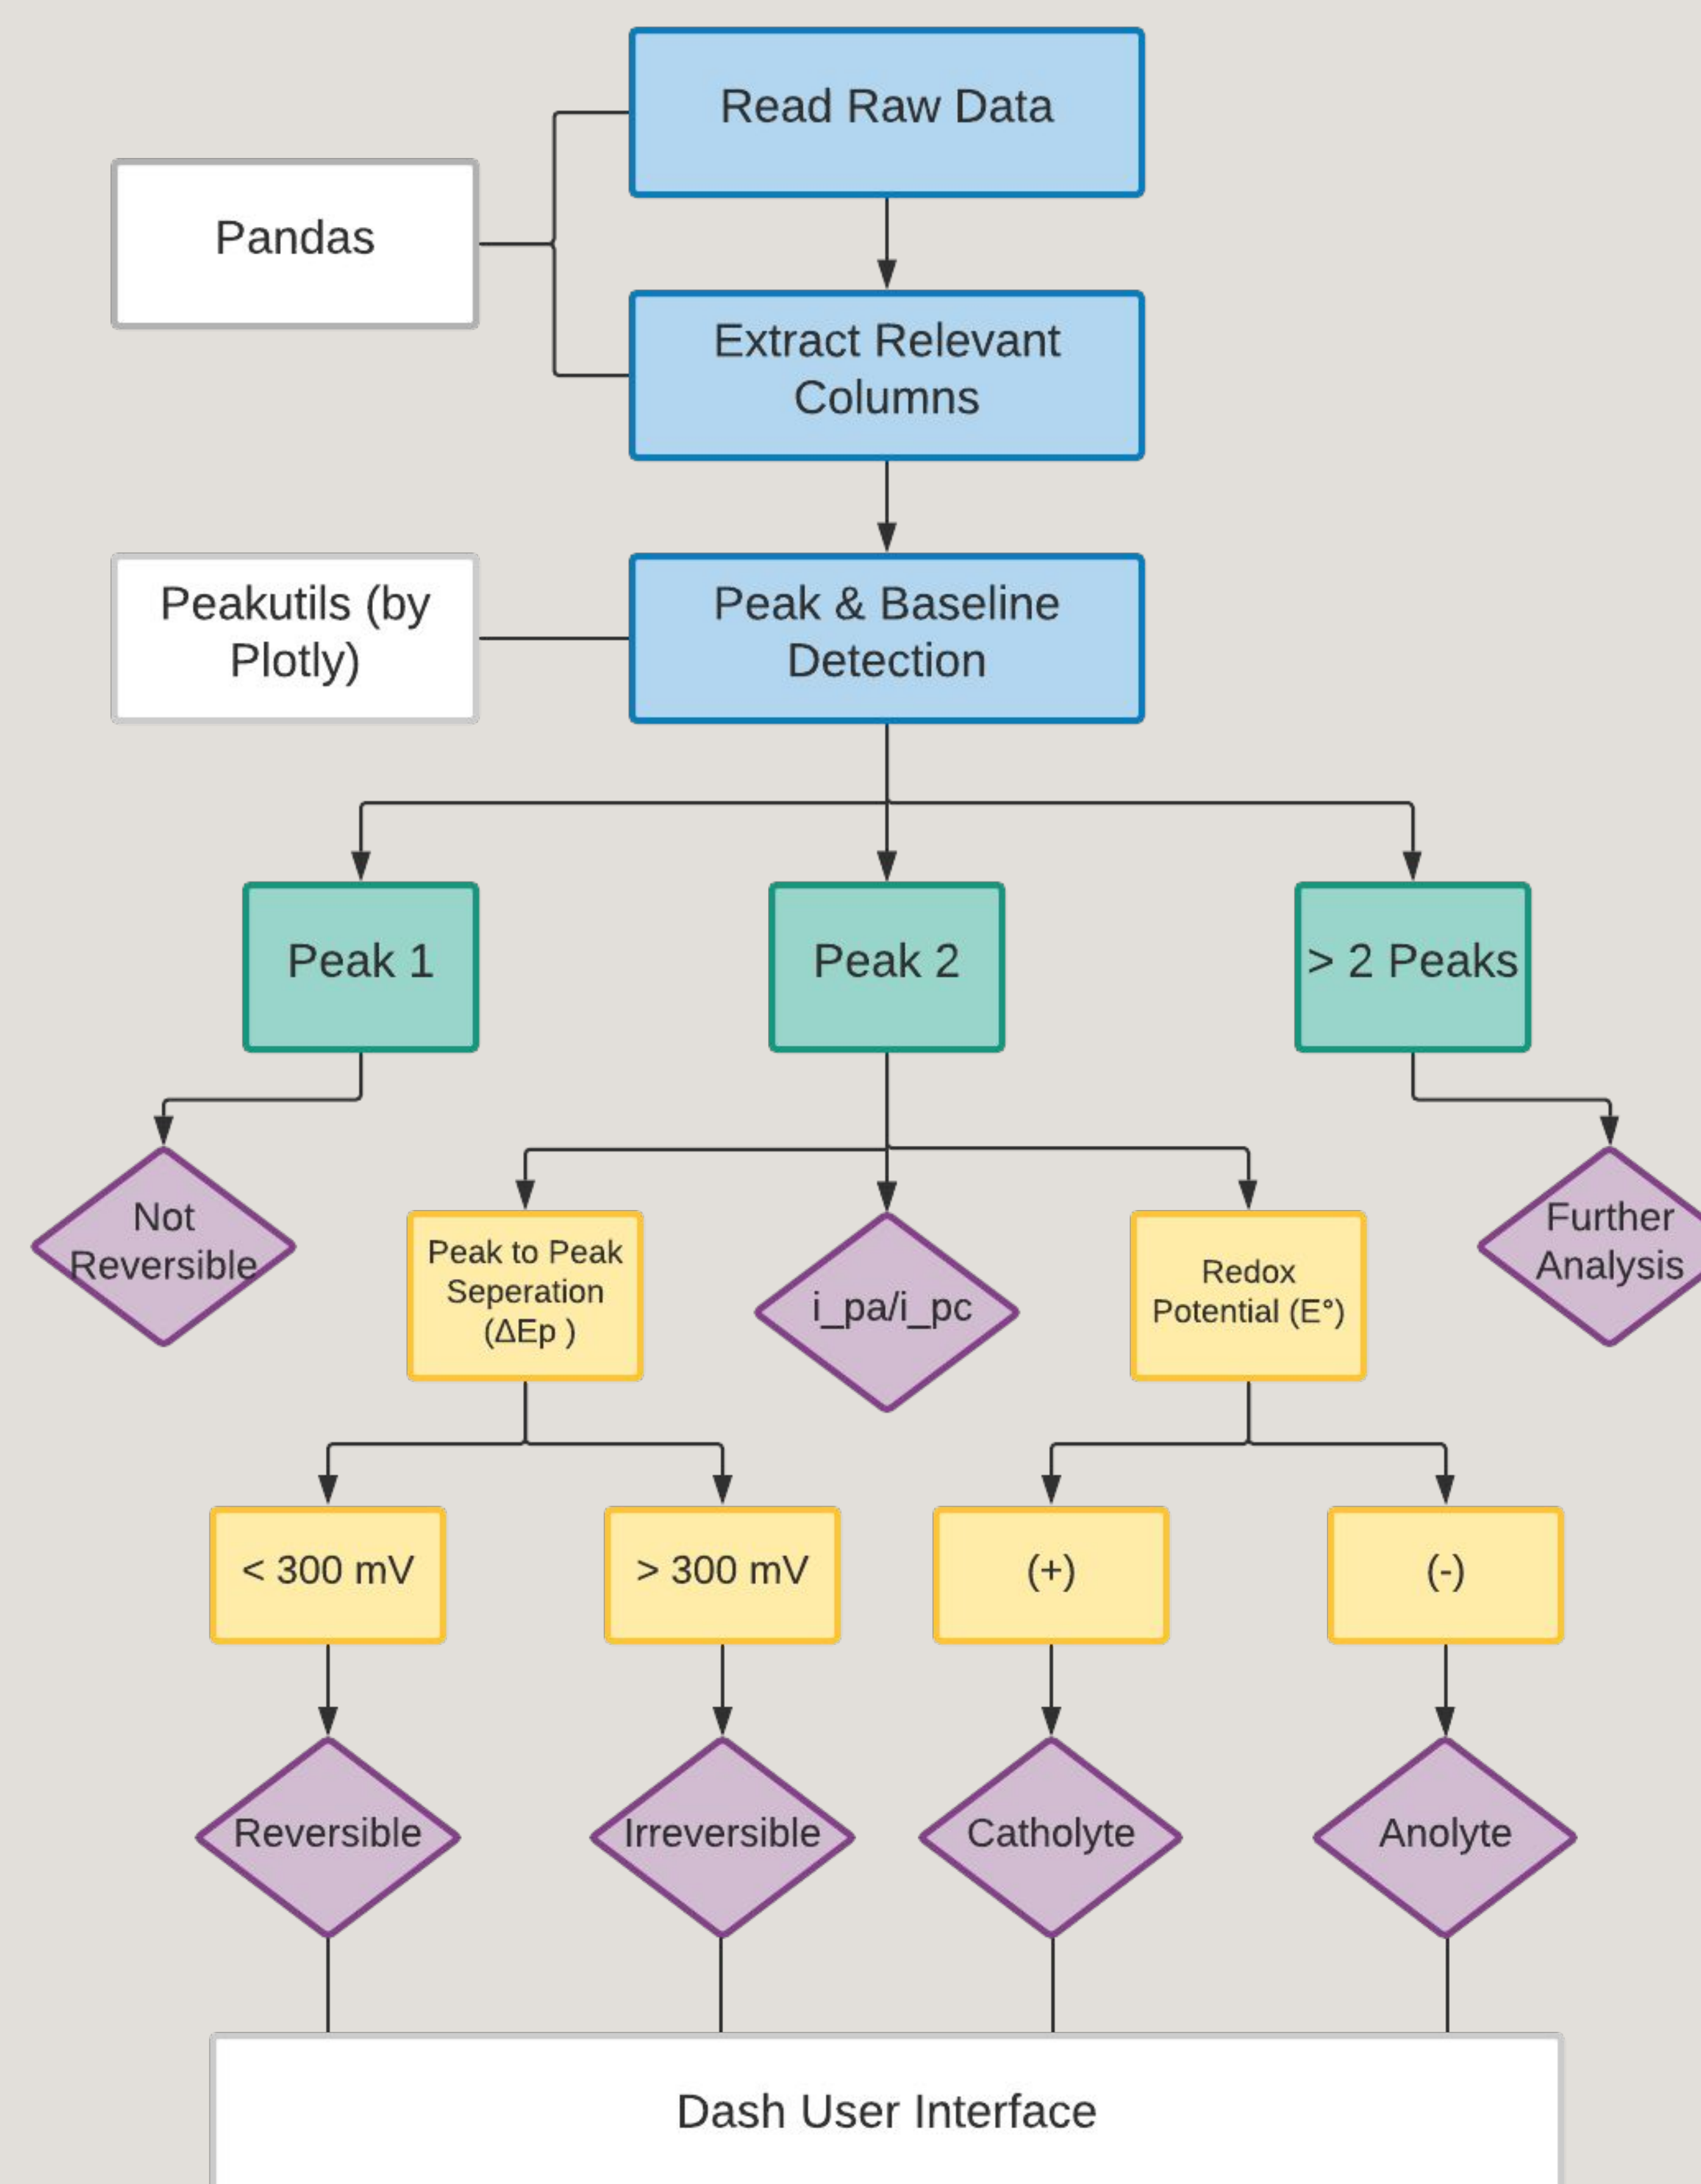


User Interface:

- Dash (by Plotly)
- Visualize and analyze multiple datasets simultaneously with ease

Limitations:

- Negative peaks proved to be a challenge
 - Used a function to split the negative values and take their absolute value
- Detecting 1 or greater than 2 peaks - further user-based analysis required
- Classifying multiple experimental cycles from the same file - current focus

RESULTS

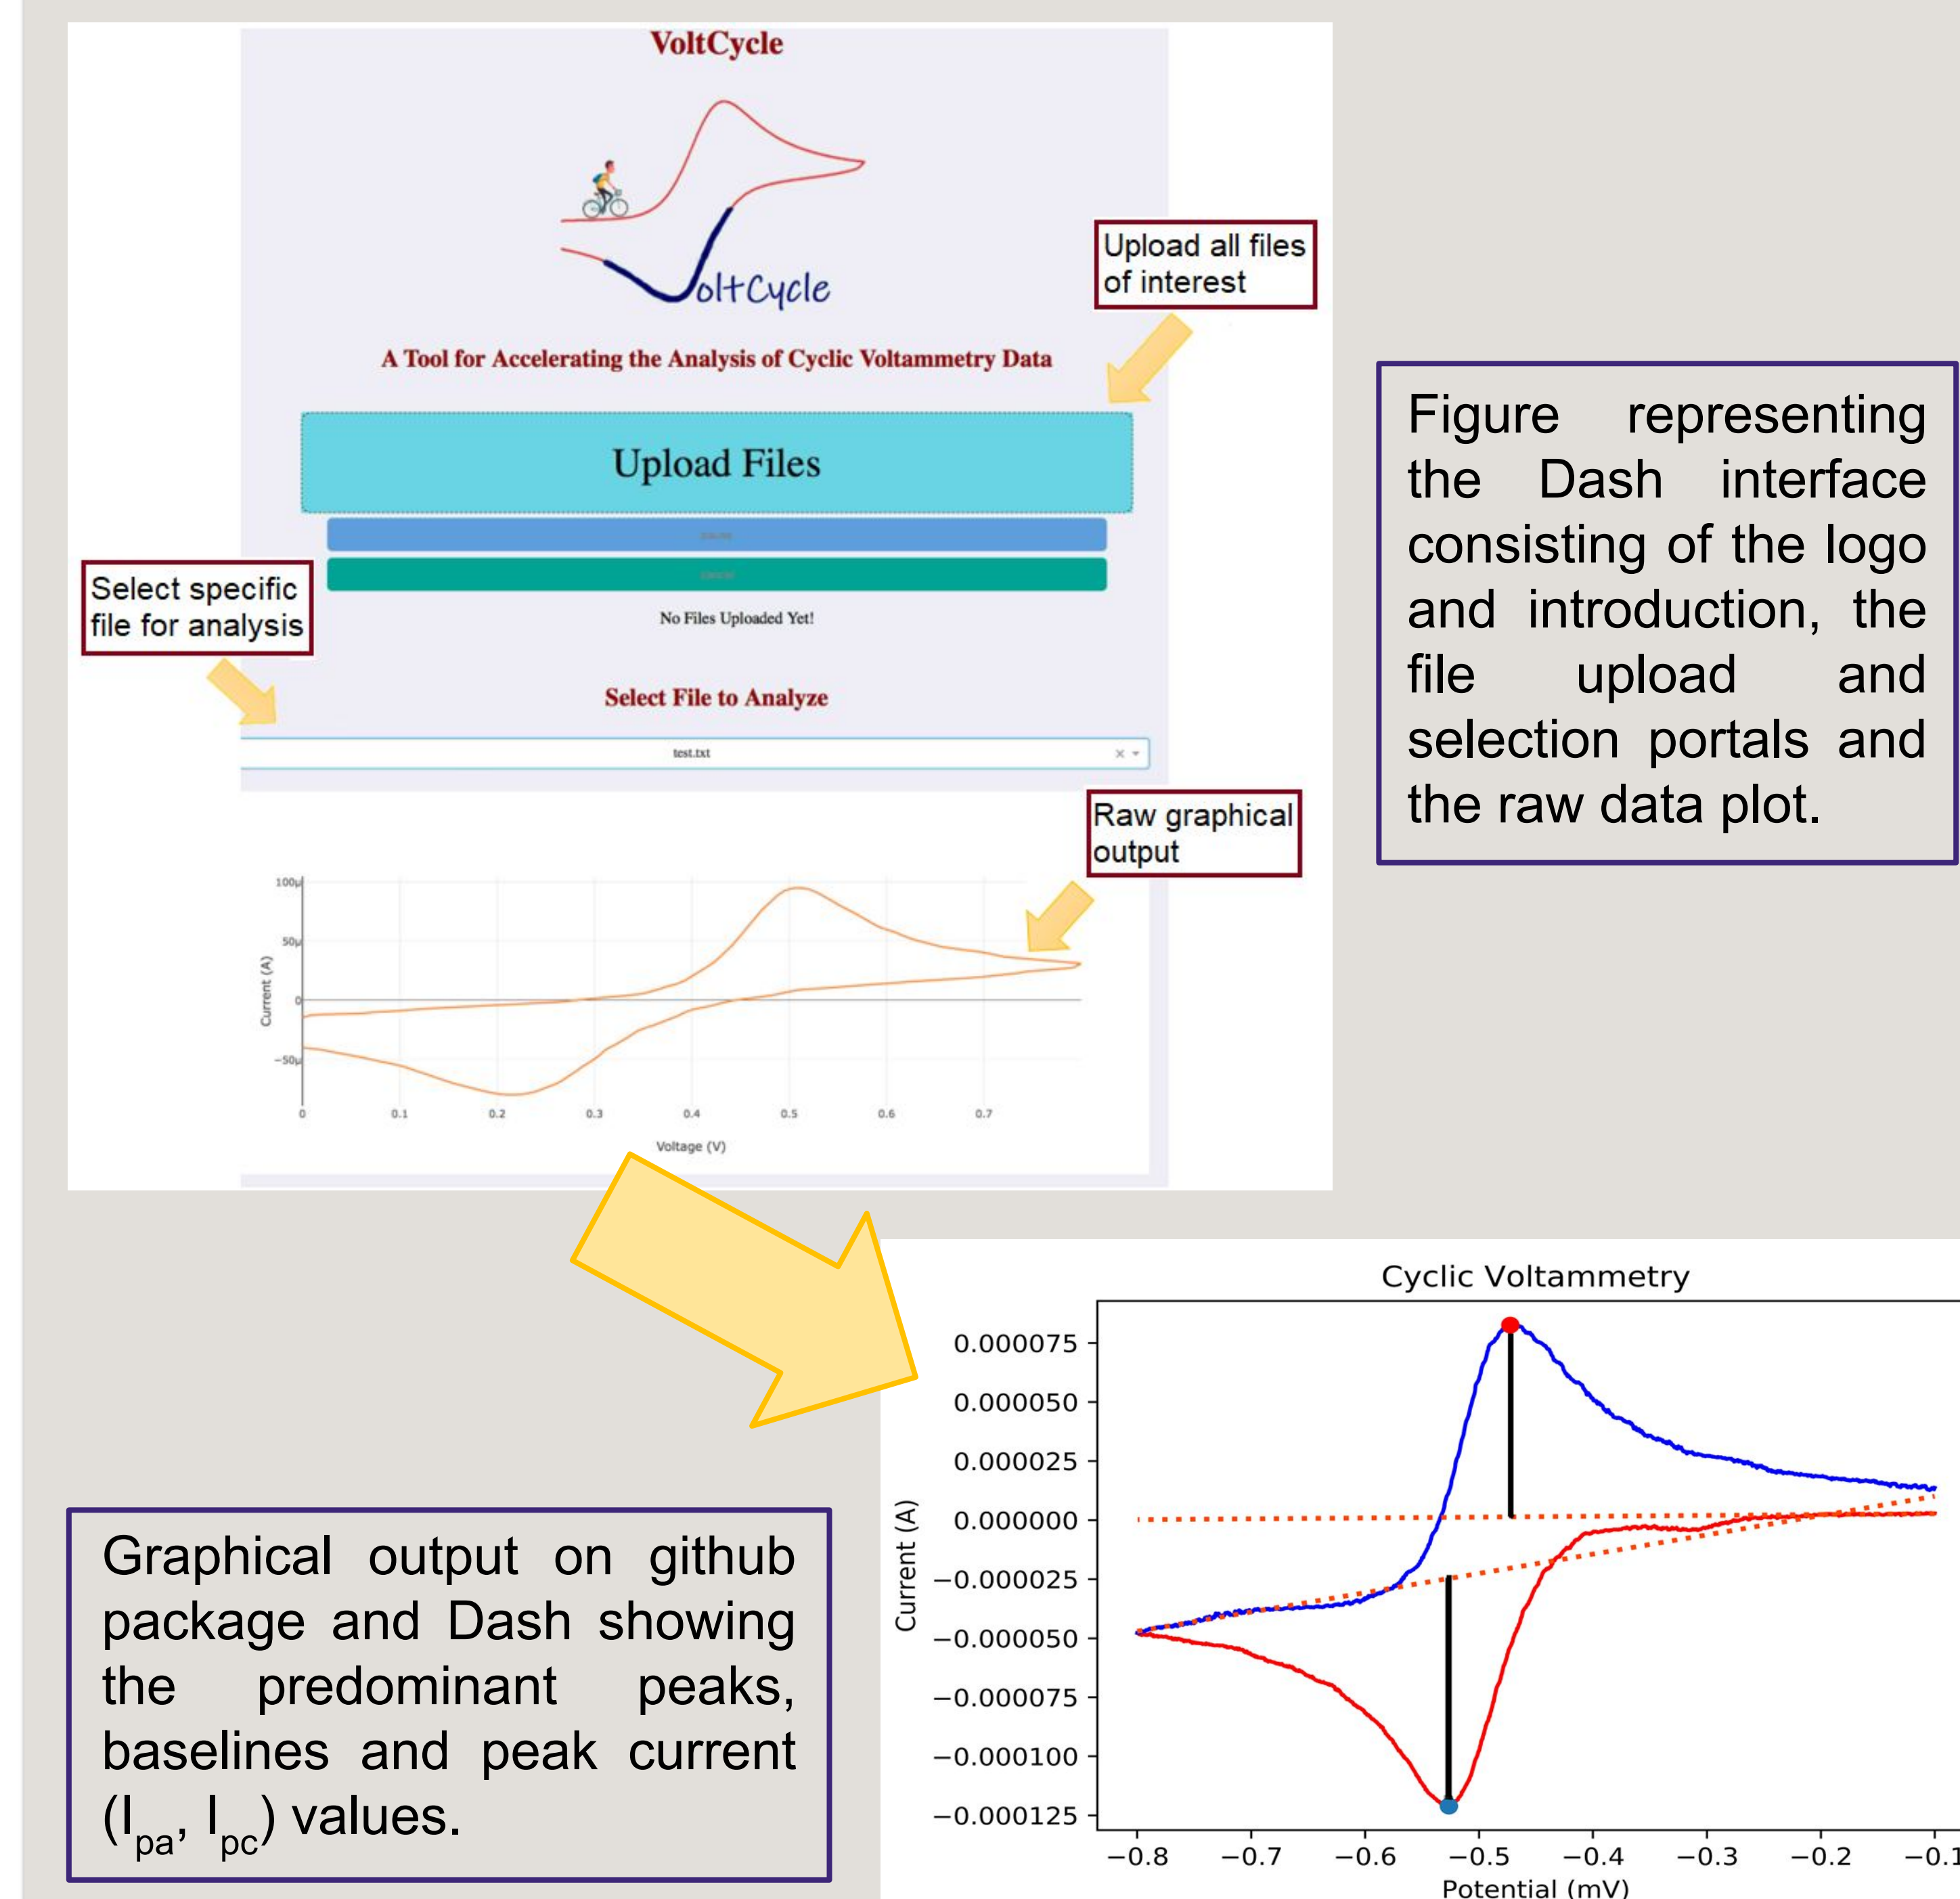

CONCLUSION & FUTURE WORKS

Conclusion:

The final package includes a Dash interface based on a single wrapper function that outputs a graphical image with the relevant parameters calculated and labeled. It also results in a dictionary consisting of important values and the final classification.

Future Direction:

- Process more complex CV raw files
 - Perform analyses for files with more than two peaks
 - Output materials classification comparison table for all input files
- Machine learning
 - Once enough data has been classified, develop design features for materials that are good candidates for this application



Acknowledgements

The authors thank Dave Beck, Chad Curtis, Kelly Thornton, Jim Pfaendtner, and DIRECT TAs for their guidance, and Lilo Pozzo for providing datasets. All packages used and generated are open source, and documentation can be found on github at <https://github.com/sabiharustam/voltcycle>

References

- [1] <https://sop4cv.com/index.html>
- [2] <http://urrjaa.blogspot.com/2013/08/cyclic-voltammetry-urrjaa-p0110-2013.html>