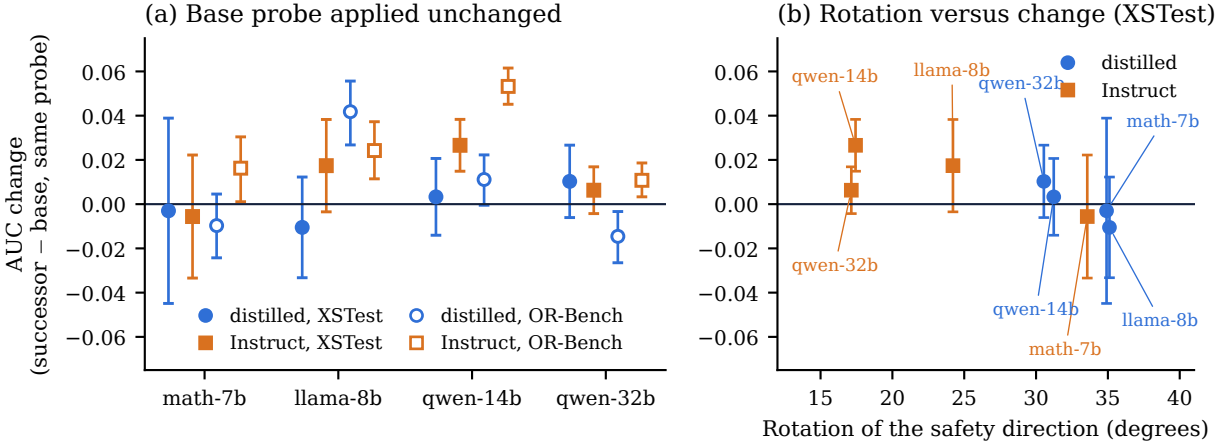
(a) Base probe applied unchanged
AUC change
(successor − base, same probe)
0.06
0.04
0.02
0.00
−0.02
−0.04
−0.06
distilled, XSTest
Instruct, XSTest
distilled, OR-Bench
Instruct, OR-Bench
math-7b
llama-8b
qwen-14b
qwen-32b
(b) Rotation versus change (XSTest)
distilled
Instruct
qwen-14b
llama-8b
qwen-32b
math-7b
15
20
25
30
35
40
Rotation of the safety direction (degrees)