



OD

Phakic eye

Target Refraction

0.0

n 1.3375			
AL 21.80mm	ACD 2.79mm		
Flat SimK (K1) 43.55D	R1 7.75mm	99°	
Steep SimK (K2) 43.92D	R2 7.68mm	9°	
Astig 0.37D		9°	
SimK 43.74D	R 7.72mm		
CCT 568µm	Mean TCPIOL 42.81D		
LT  4.44mm	WTW, N-T 11.03mm		

ABBOTT SENSOR AR40		AMO TECNIS 1 ZCB00	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
25.50	0.76	26.50	0.78
26.00	0.41	27.00	0.44
26.50	0.06	27.50	0.10
27.00	-0.30	28.00	-0.25
27.50	-0.66	28.50	-0.60
IOL@Target Refraction 26.58 D		IOL@Target Refraction 27.64 D	
IOL Constant 1.62		IOL Constant 2.02	

AMO TECNIS ZA 9003		ABBOTT sinfonyc toric	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
26.00	0.80	26.50	0.67
26.50	0.46	27.00	0.33
27.00	0.11	27.50	-0.02
27.50	-0.24	28.00	-0.36
28.00	-0.60	28.50	-0.72
IOL@Target Refraction 27.16 D		IOL@Target Refraction 27.48 D	
IOL Constant 1.84		IOL Constant 1.96	

ALCON MA60AC		ZEISS SPHERIS 204	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
26.50	0.56	25.00	0.74
27.00	0.22	25.50	0.38
27.50	-0.13	26.00	0.02
28.00	-0.48	26.50	-0.34
28.50	-0.84	27.00	-0.71
IOL@Target Refraction 27.32 D		IOL@Target Refraction 26.03 D	
IOL Constant 1.90		IOL Constant 1.40	

OS

Phakic eye

Target Refraction

0.0

n 1.3375			
AL 21.86mm	ACD 2.82mm		
Flat SimK (K1) 43.38D	R1 7.78mm	85°	
Steep SimK (K2) 45.09D	R2 7.48mm	175°	
Astig 1.71D		175°	
SimK 44.24D	R 7.63mm		
CCT 571µm	Mean TCPIOL 43.12D		
LT 4.72mm	WTW, N-T 10.76mm		

ABBOTT SENSOR AR40		AMO TECNIS 1 ZCB00	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
25.00	0.56	26.00	0.56
25.50	0.21	26.50	0.22
26.00	-0.15	27.00	-0.12
26.50	-0.50	27.50	-0.46
27.00	-0.86	28.00	-0.81
IOL@Target Refraction 25.79 D		IOL@Target Refraction 26.83 D	
IOL Constant 1.62		IOL Constant 2.02	

AMO TECNIS ZA 9003		ABBOTT sinfonyc toric	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
25.50	0.59	25.50	0.79
26.00	0.25	26.00	0.46
26.50	-0.10	26.50	0.12
27.00	-0.45	27.00	-0.23
27.50	-0.81	27.50	-0.58
IOL@Target Refraction 26.36 D		IOL@Target Refraction 26.67 D	
IOL Constant 1.84		IOL Constant 1.96	

ALCON MA60AC		ZEISS SPHERIS 204	
Holladay I		Holladay I	
IOL [D]	Ref. [D]	IOL [D]	Ref. [D]
25.50	0.69	24.50	0.54
26.00	0.35	25.00	0.18
26.50	0.01	25.50	-0.18
27.00	-0.34	26.00	-0.54
27.50	-0.69	26.50	-0.91
IOL@Target Refraction 26.51 D		IOL@Target Refraction 25.25 D	
IOL Constant 1.90		IOL Constant 1.40	




OD


Phakic eye

Anterior Axial Curvature [D]



n 1.3375

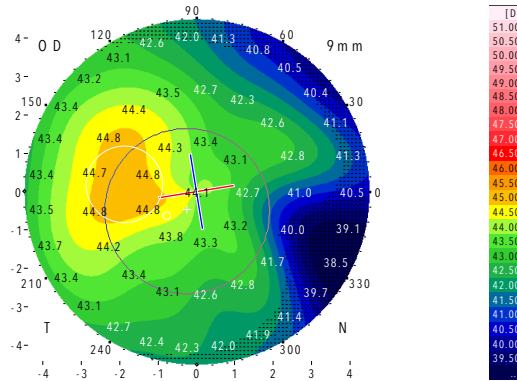

Total Corneal Power IOL (Ray Traced) [D]

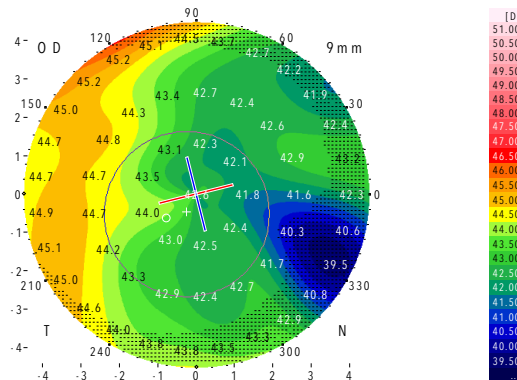

OD

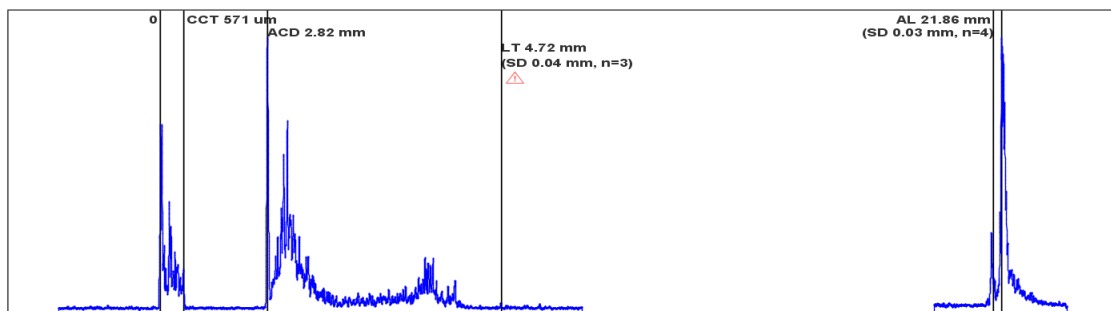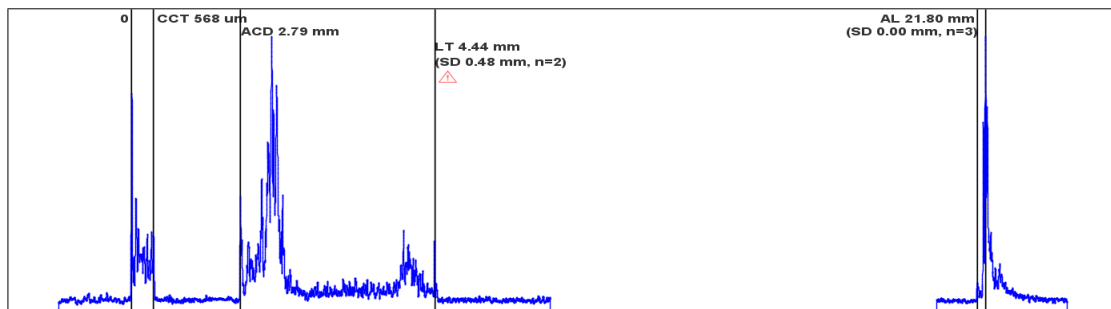

OS