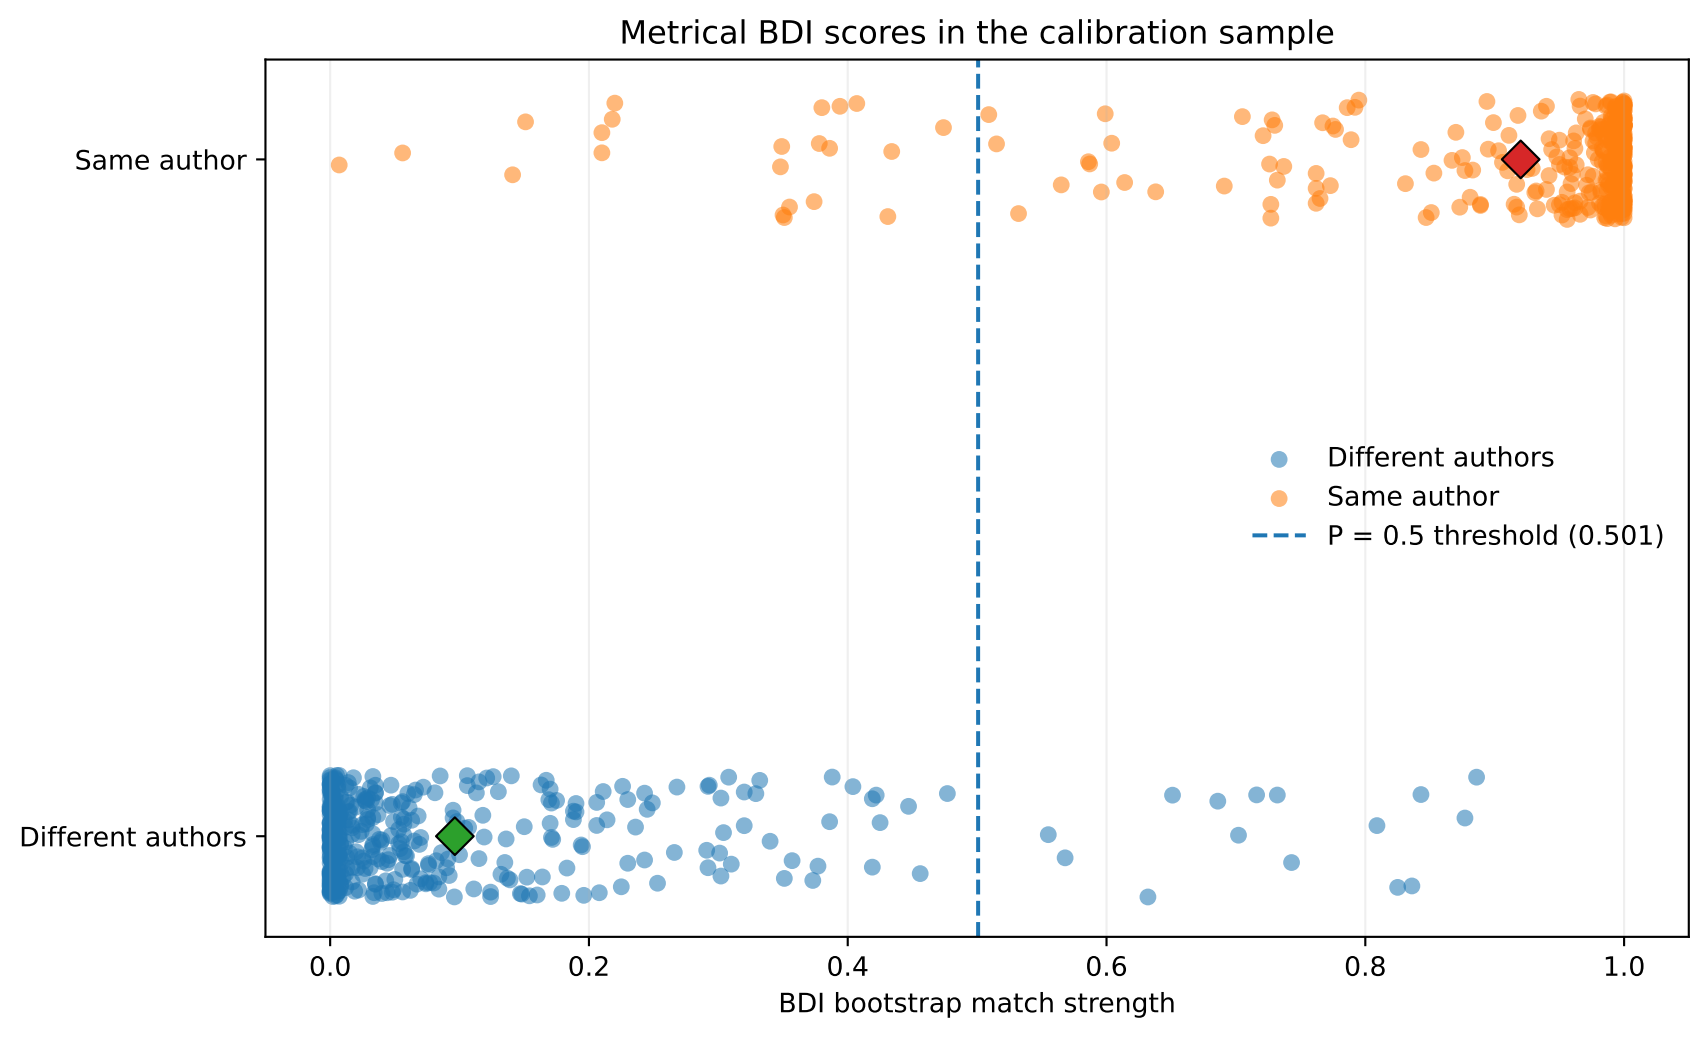
Metrical BDI scores in the calibration sample
Same author
Different authors
Different authors
Same author
P = 0.5 threshold (0.501)
0.0
0.2
0.4
0.6
0.8
1.0
BDI bootstrap match strength