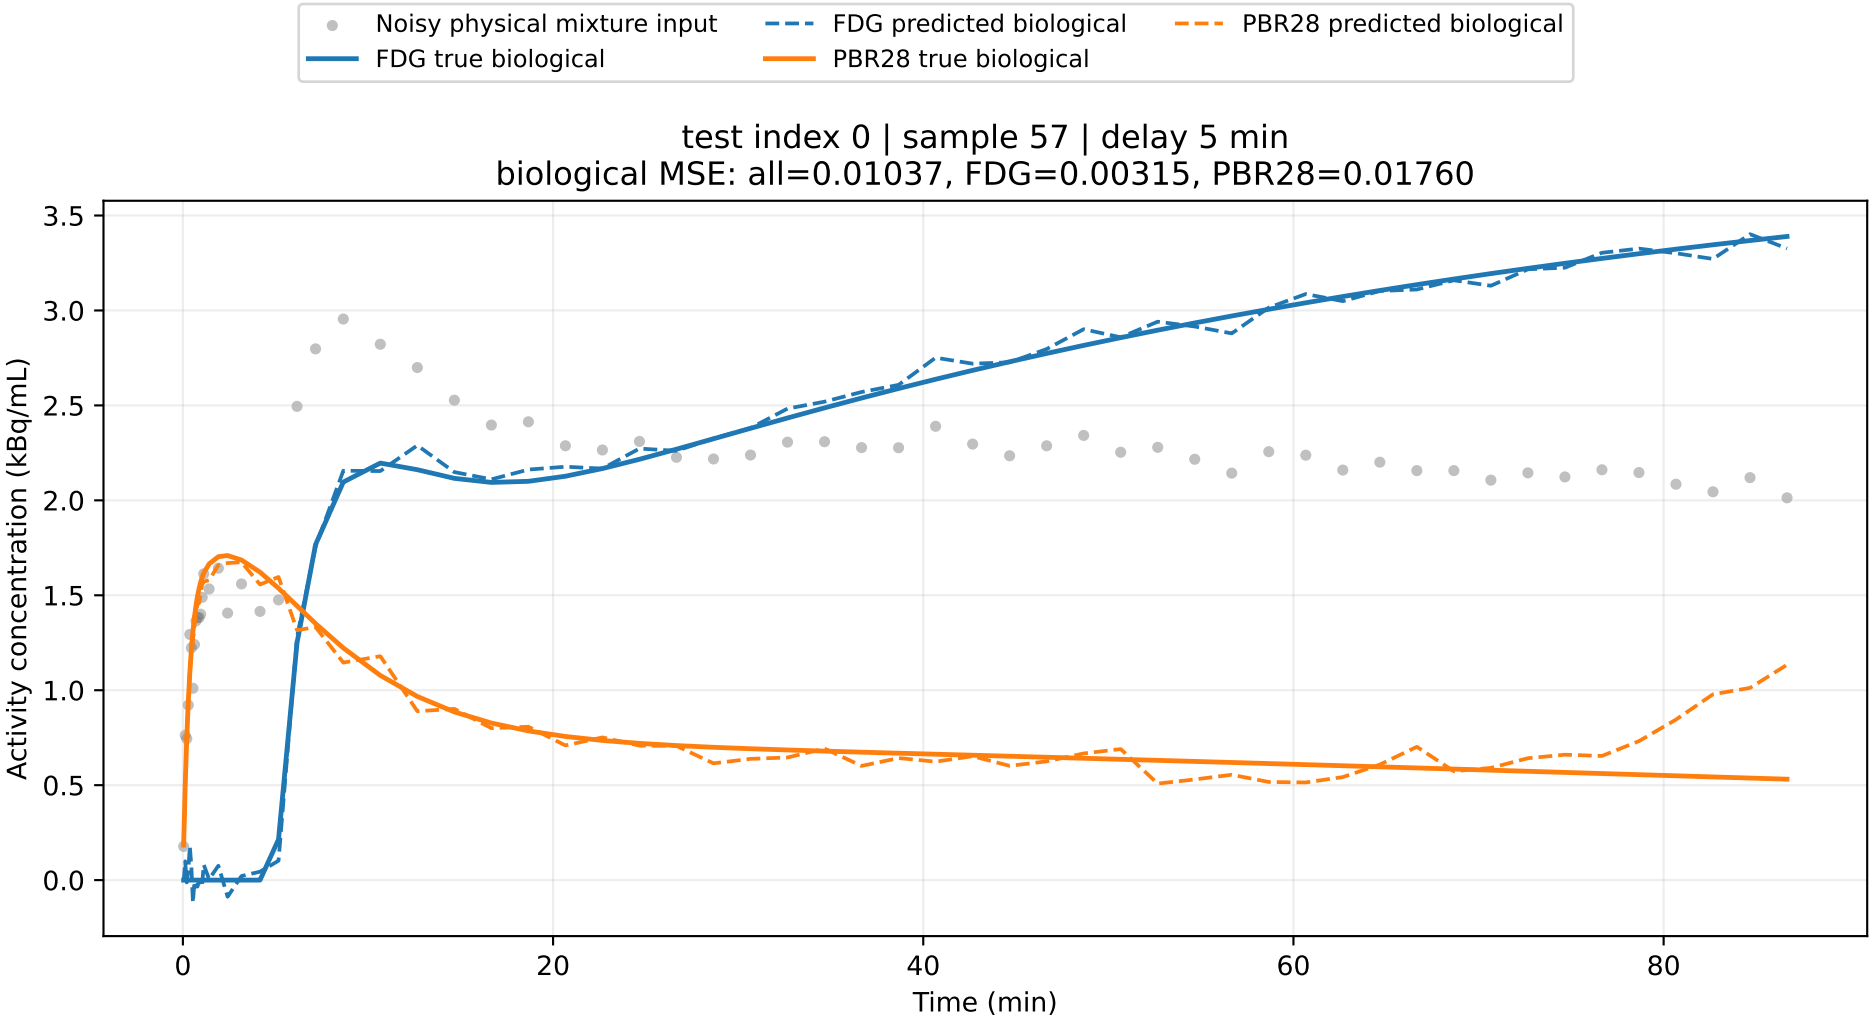
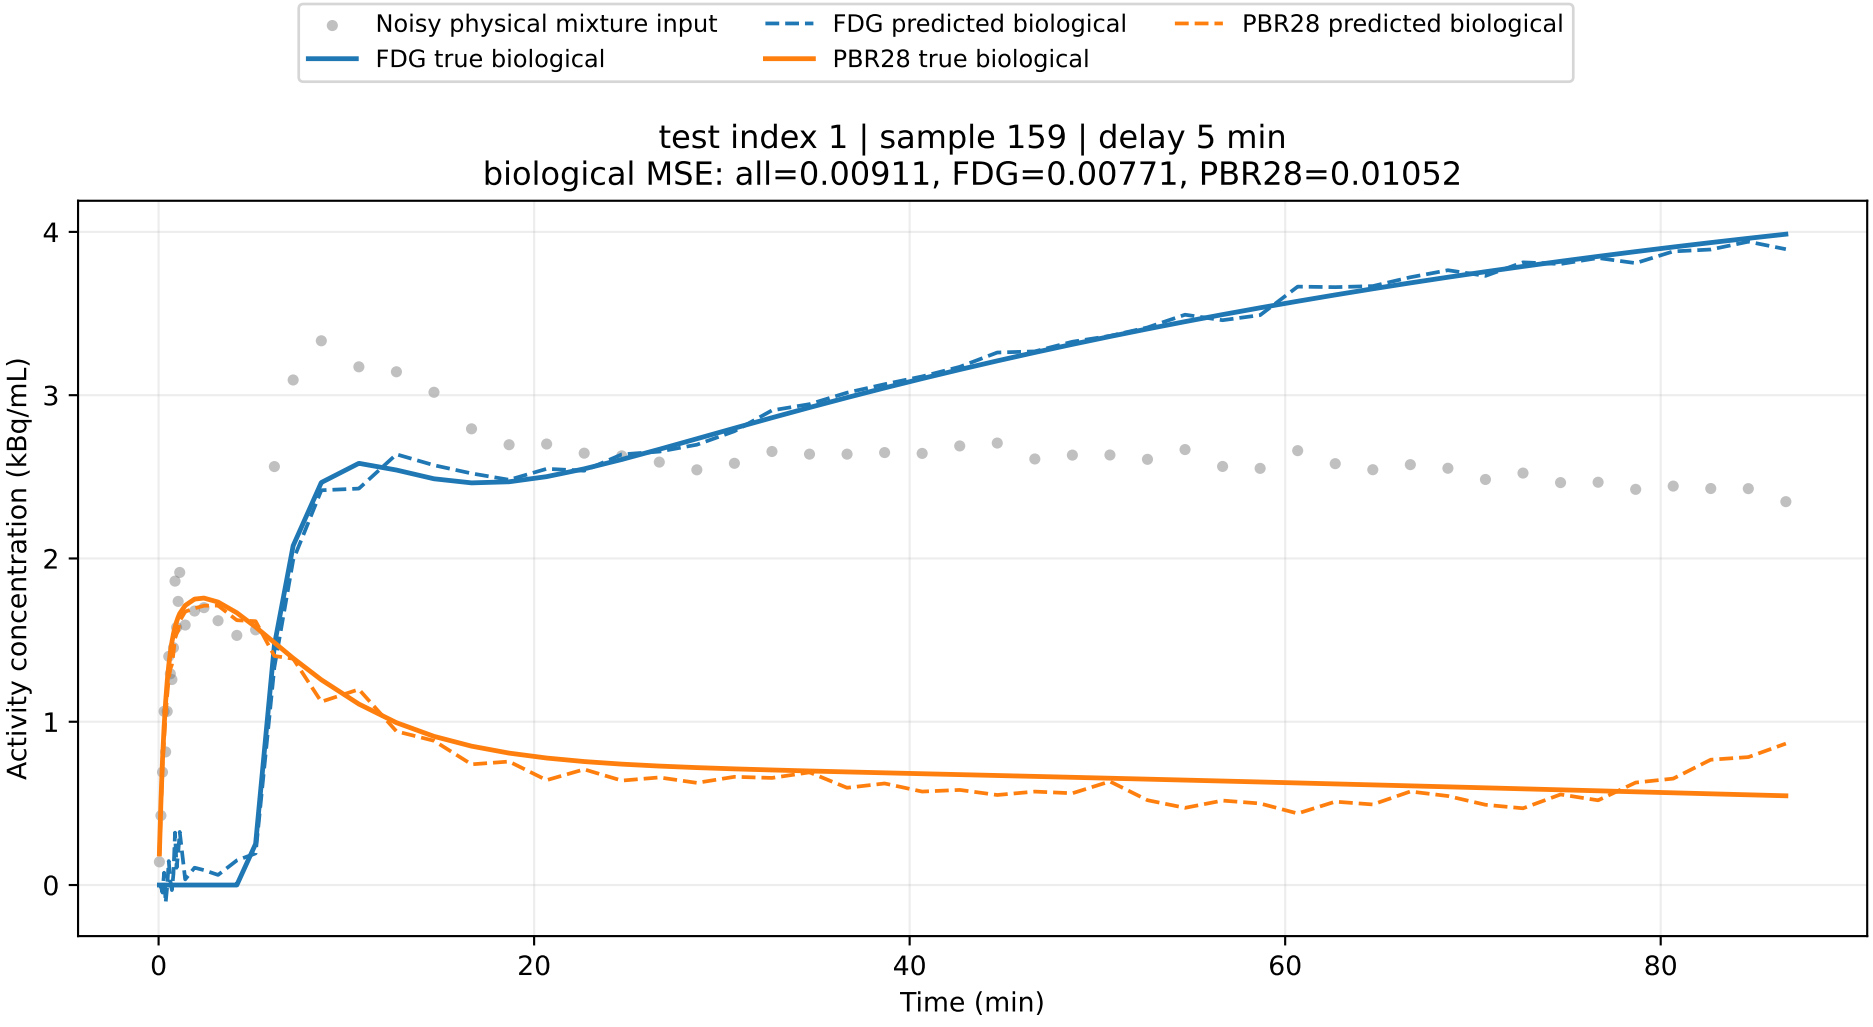
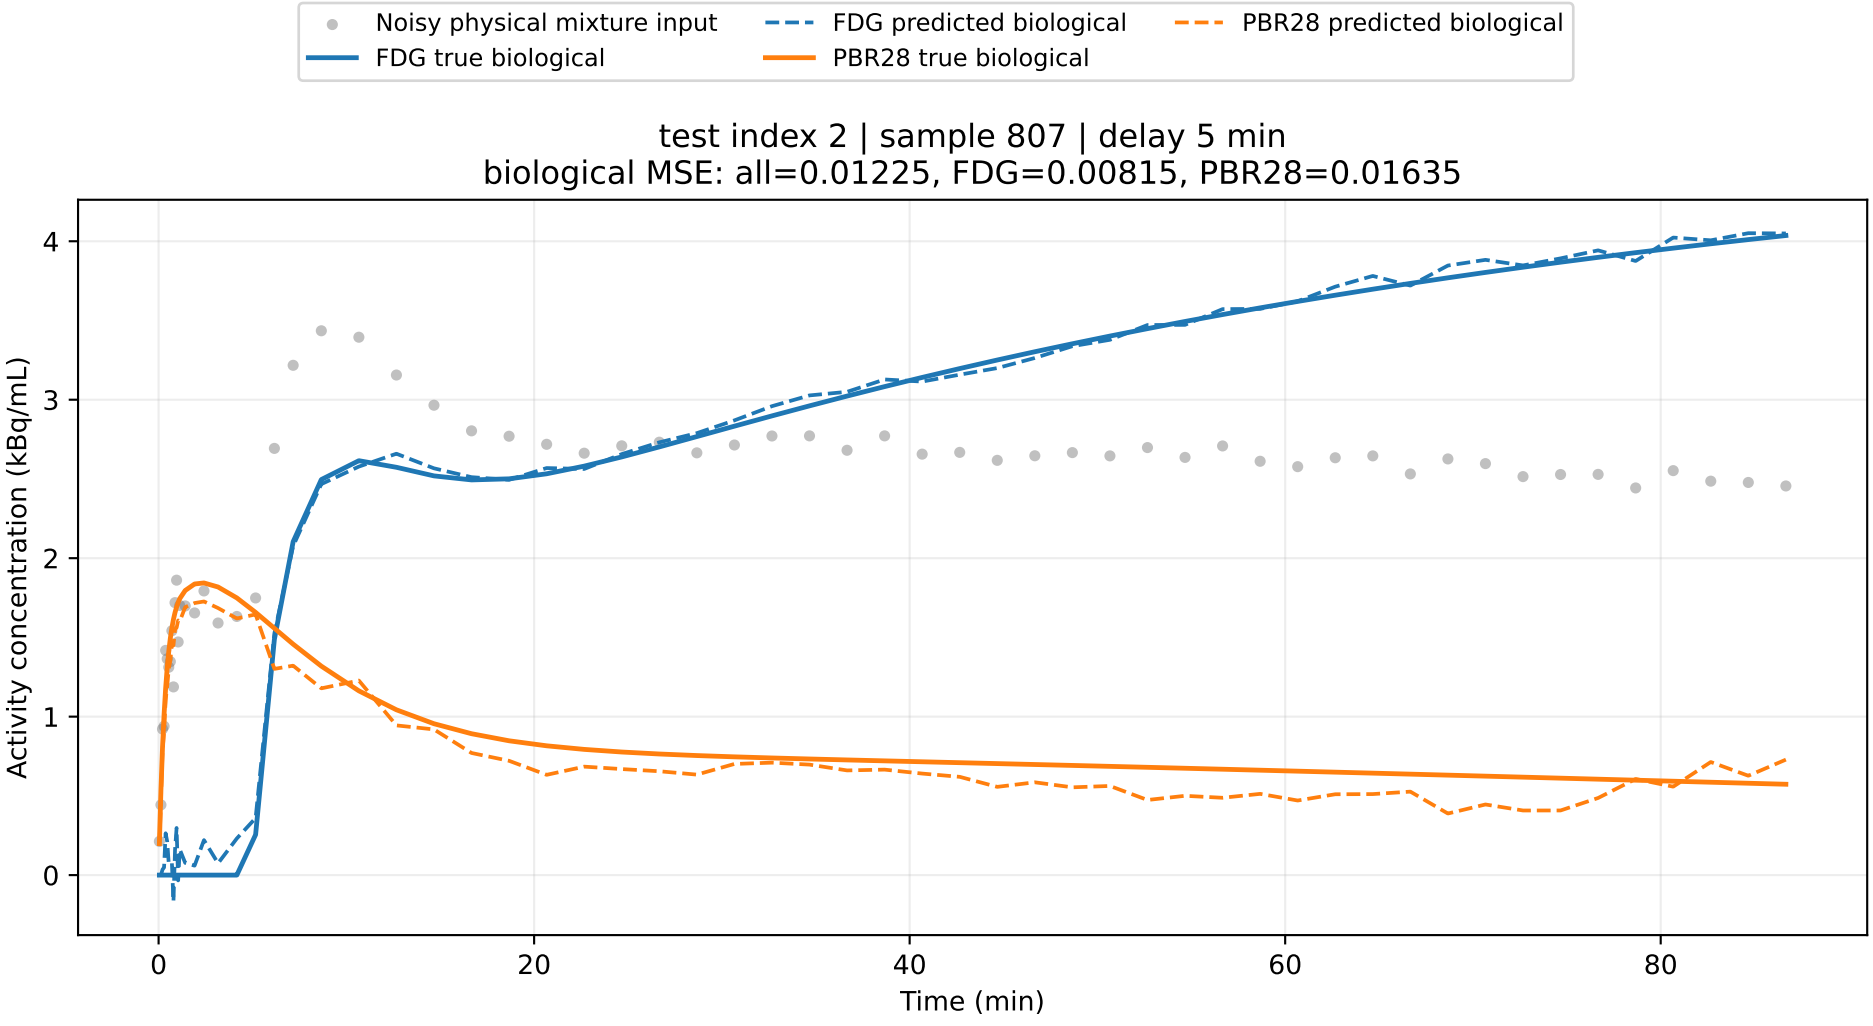
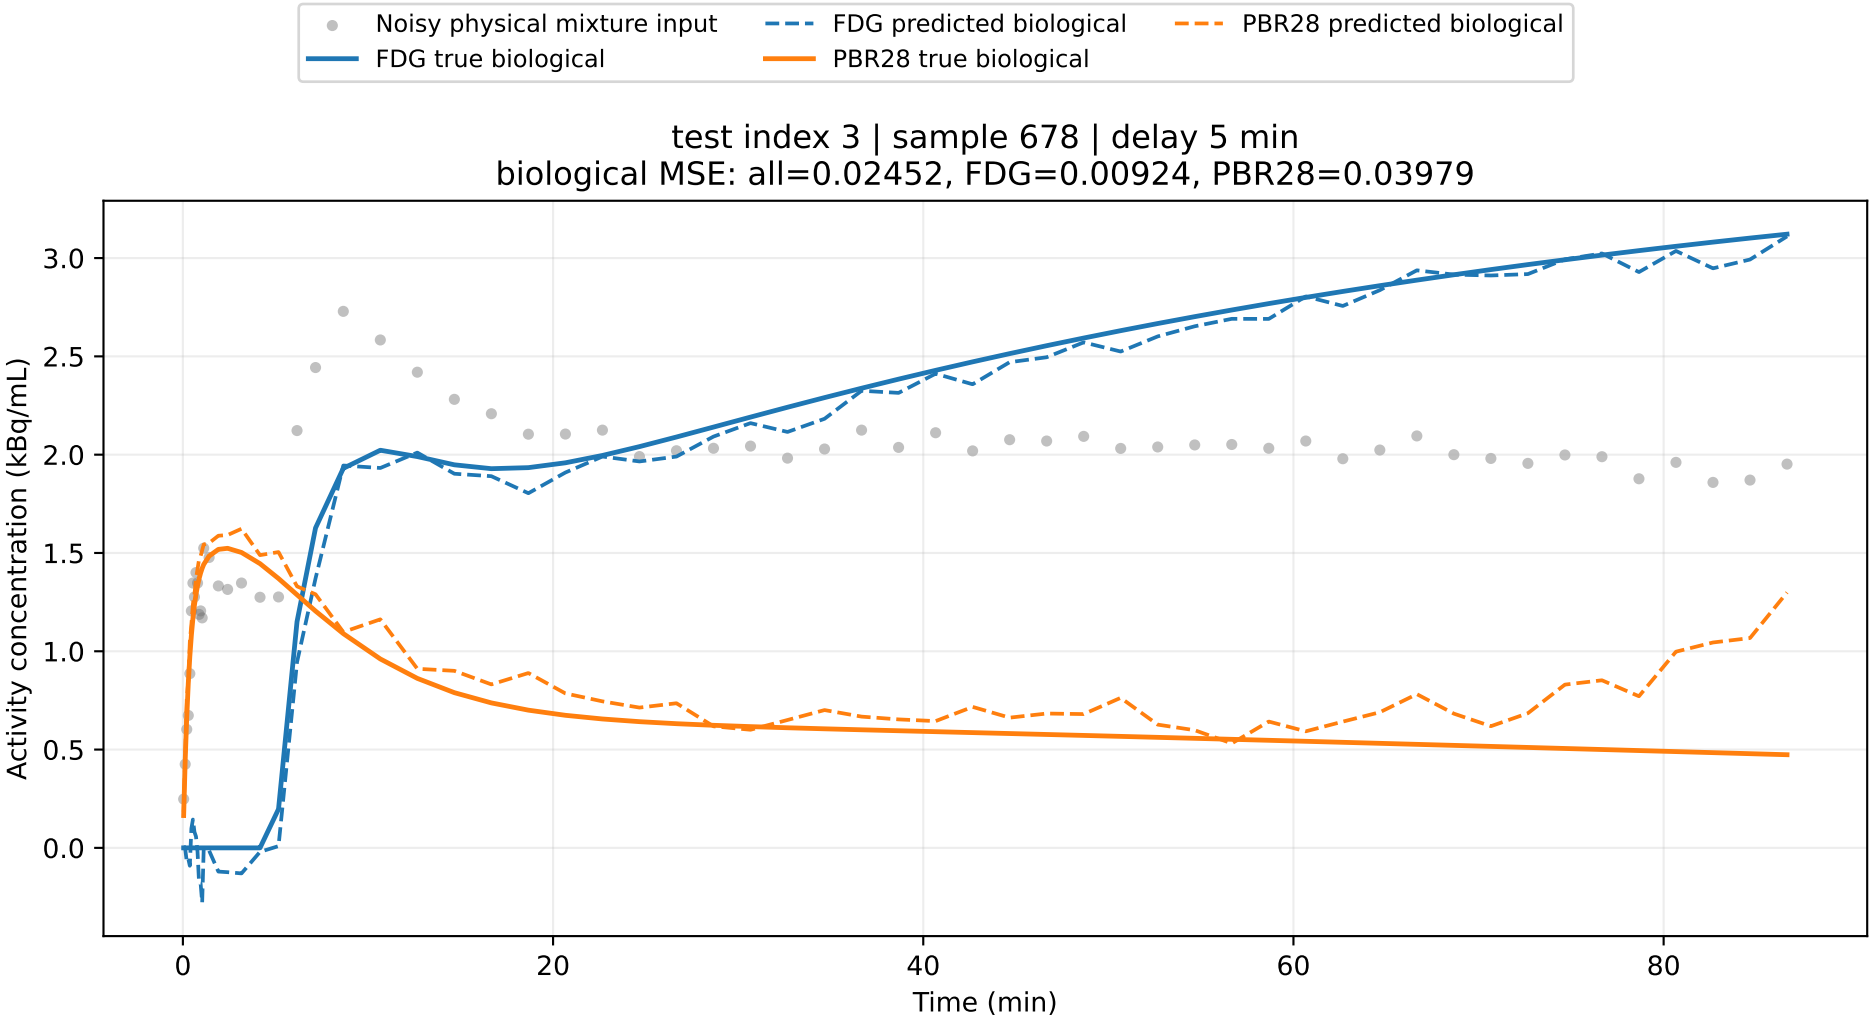
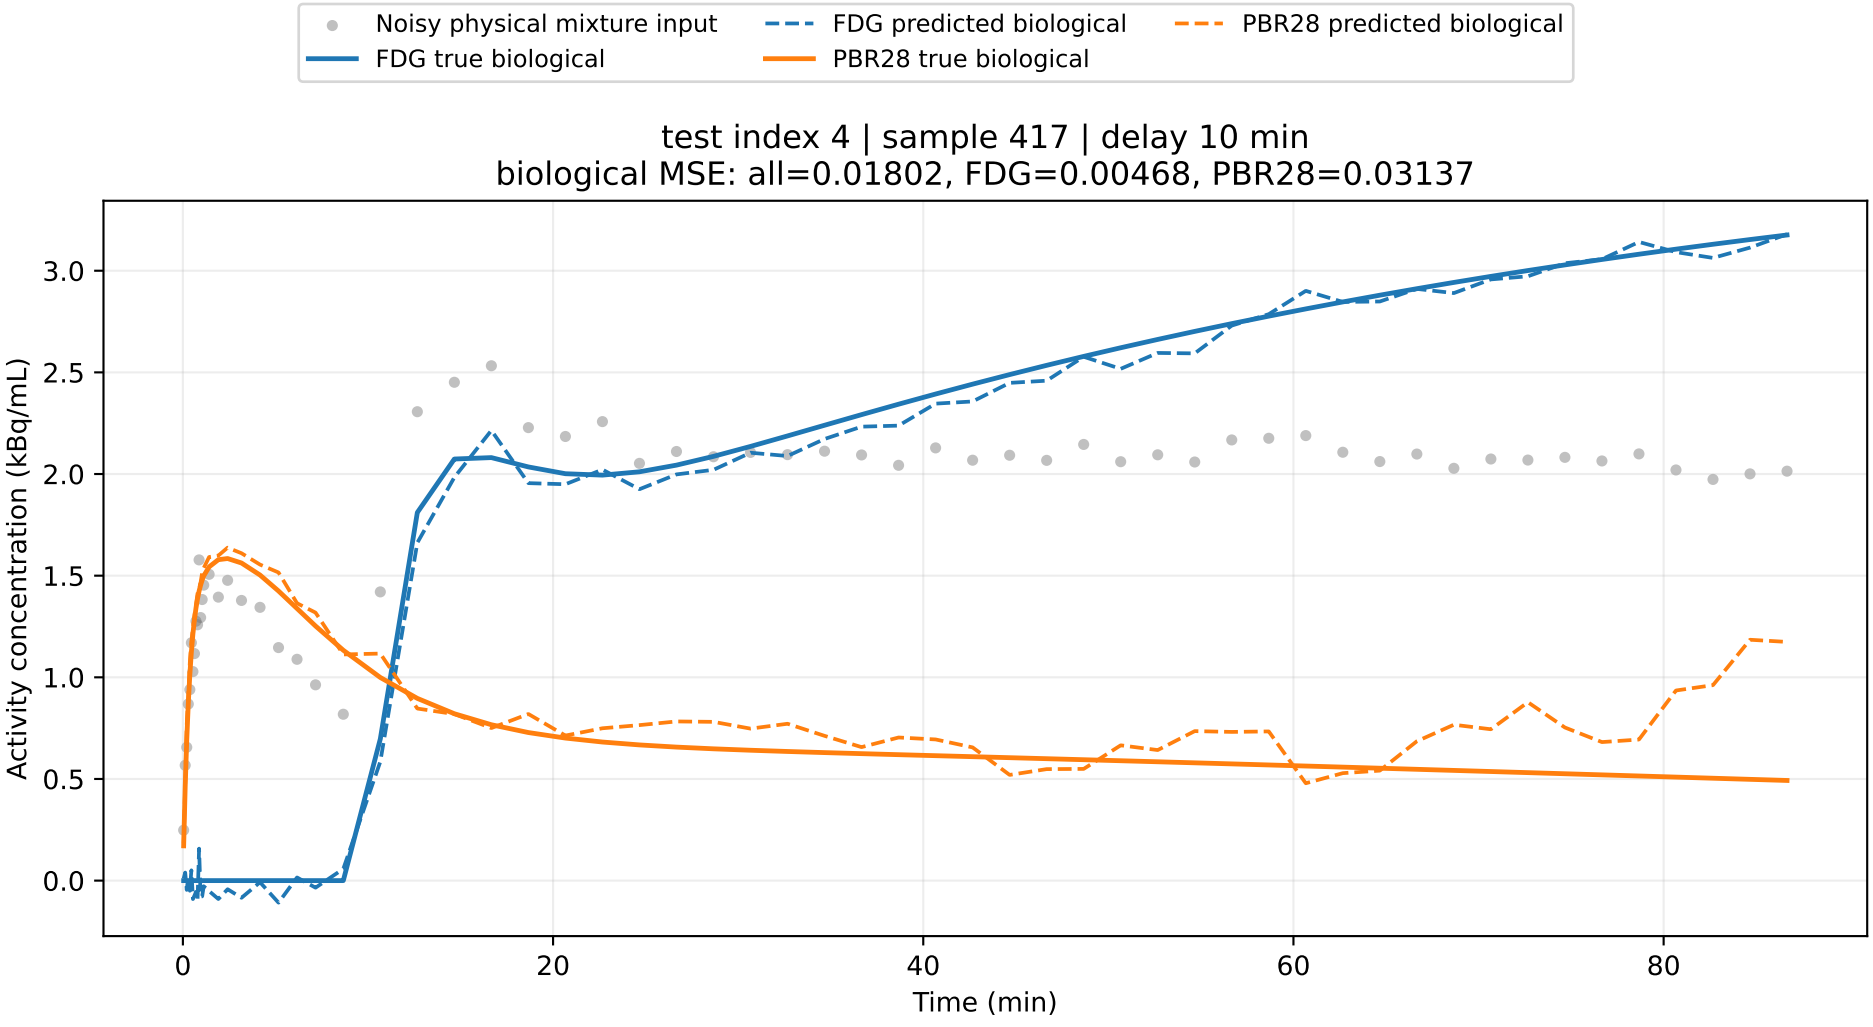
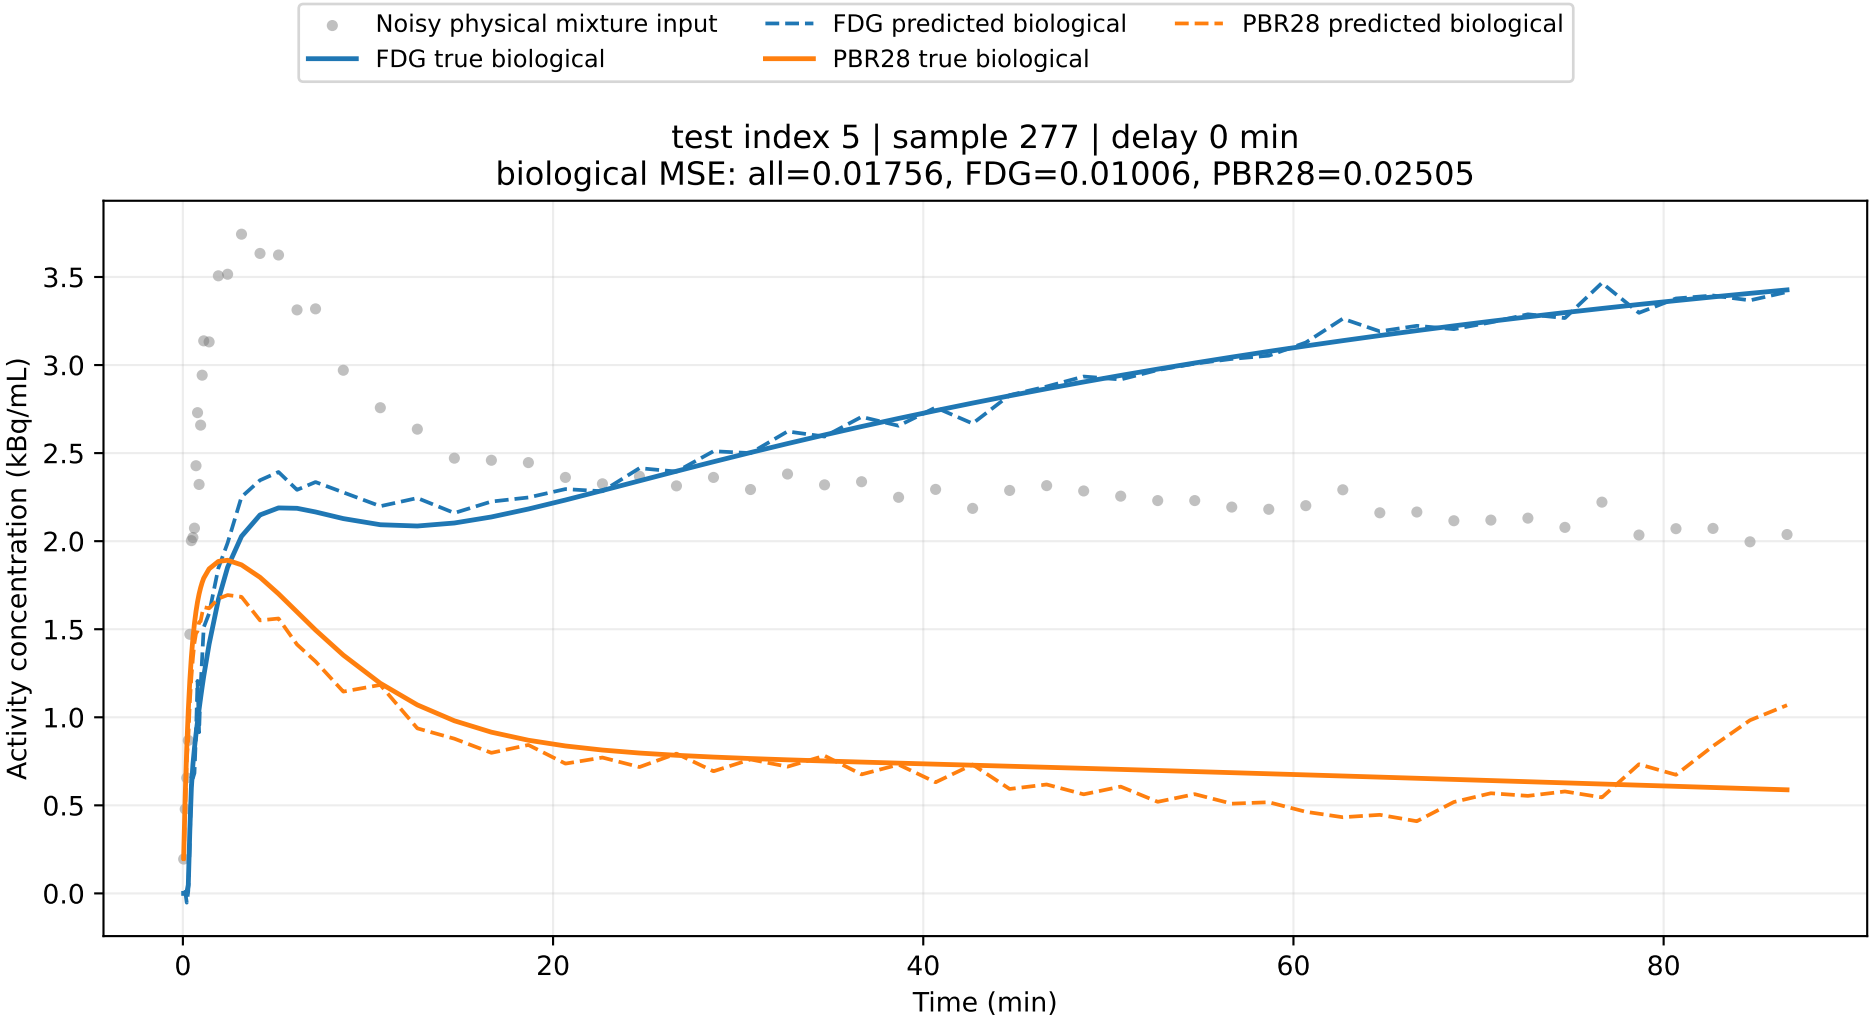

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 0 | sample 57 | delay 5 min
biological MSE: all=0.01037, FDG=0.00315, PBR28=0.01760
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

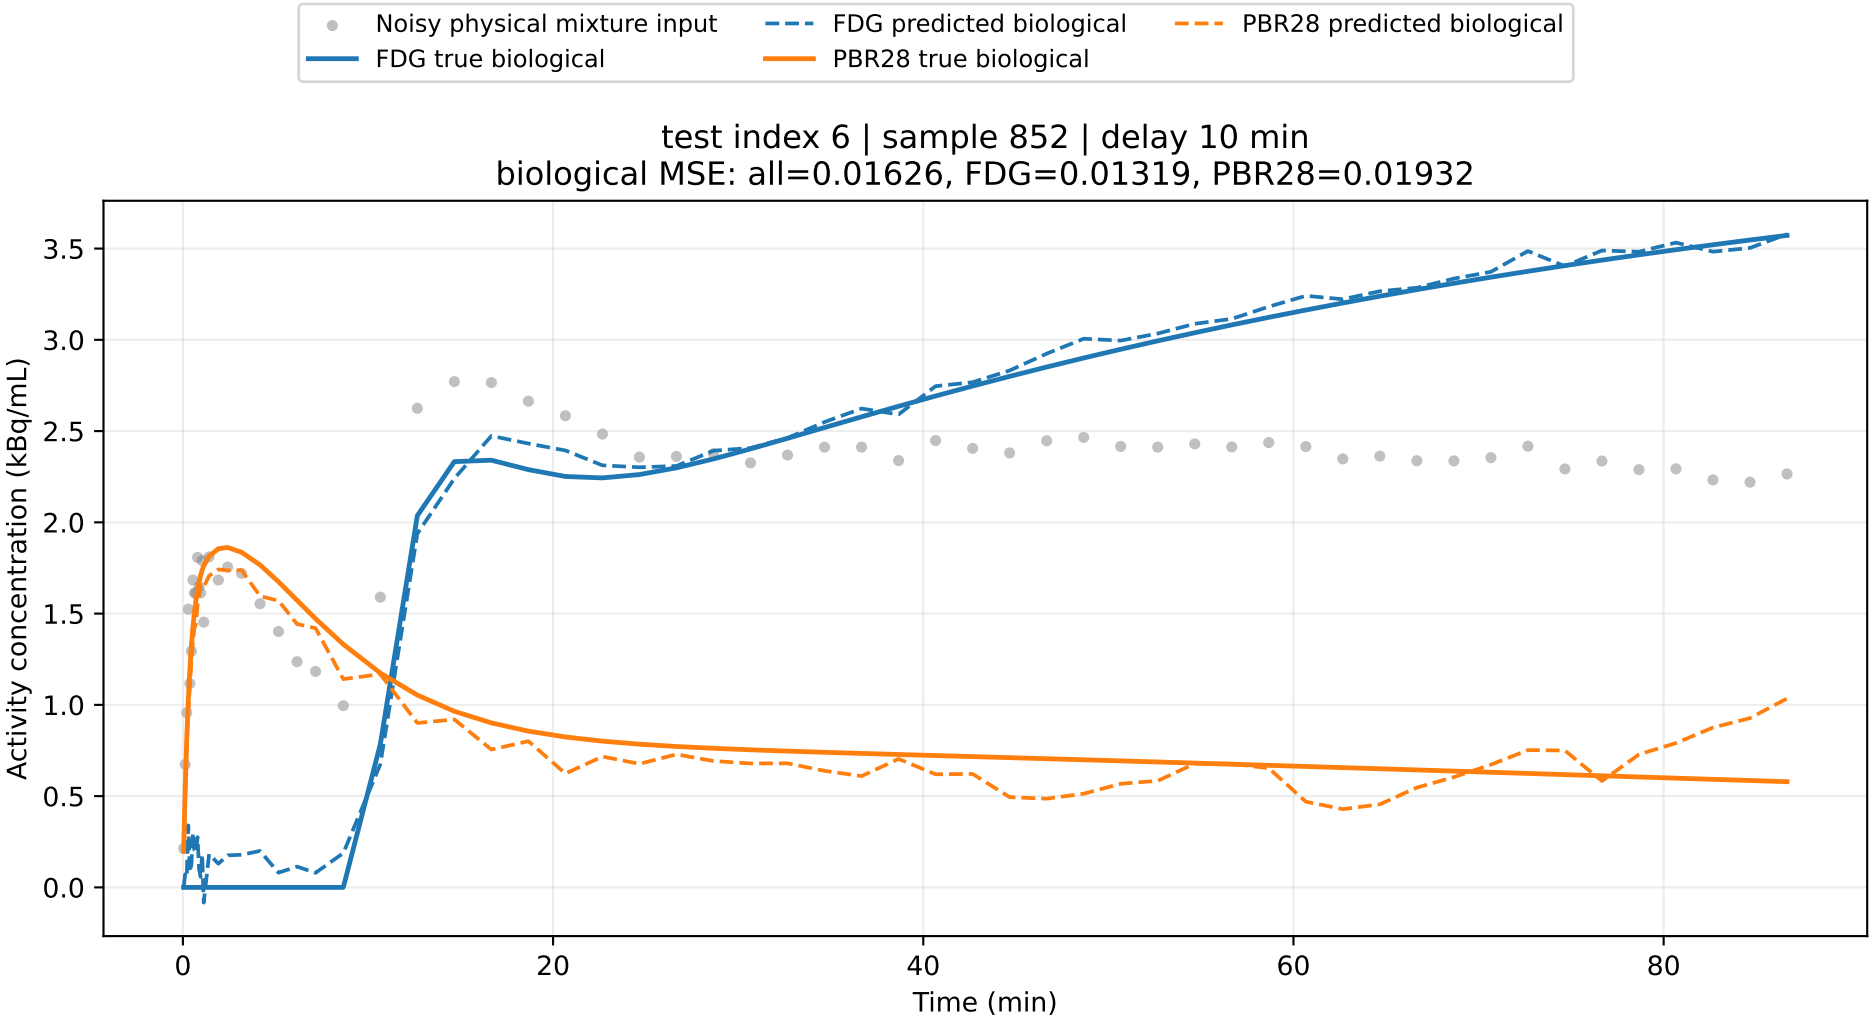

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 1 | sample 159 | delay 5 min
biological MSE: all=0.00911, FDG=0.00771, PBR28=0.01052
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

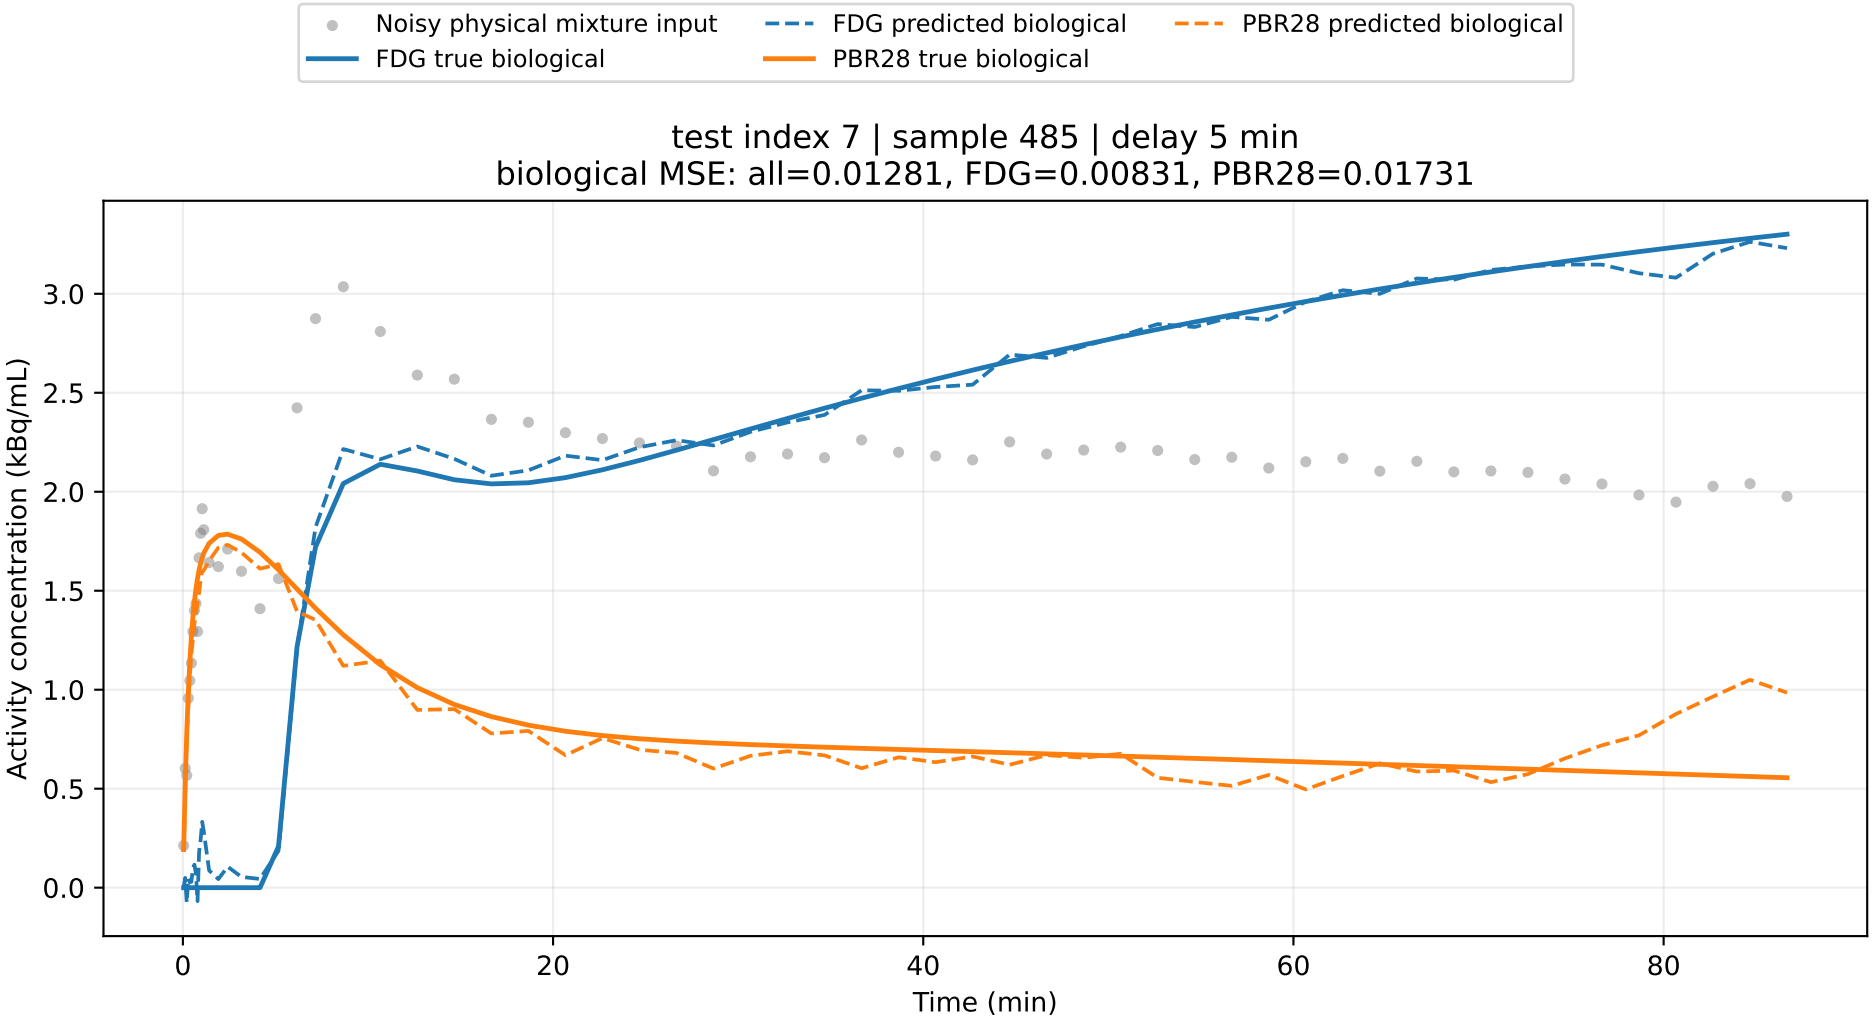

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 2 | sample 807 | delay 5 min
biological MSE: all=0.01225, FDG=0.00815, PBR28=0.01635
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

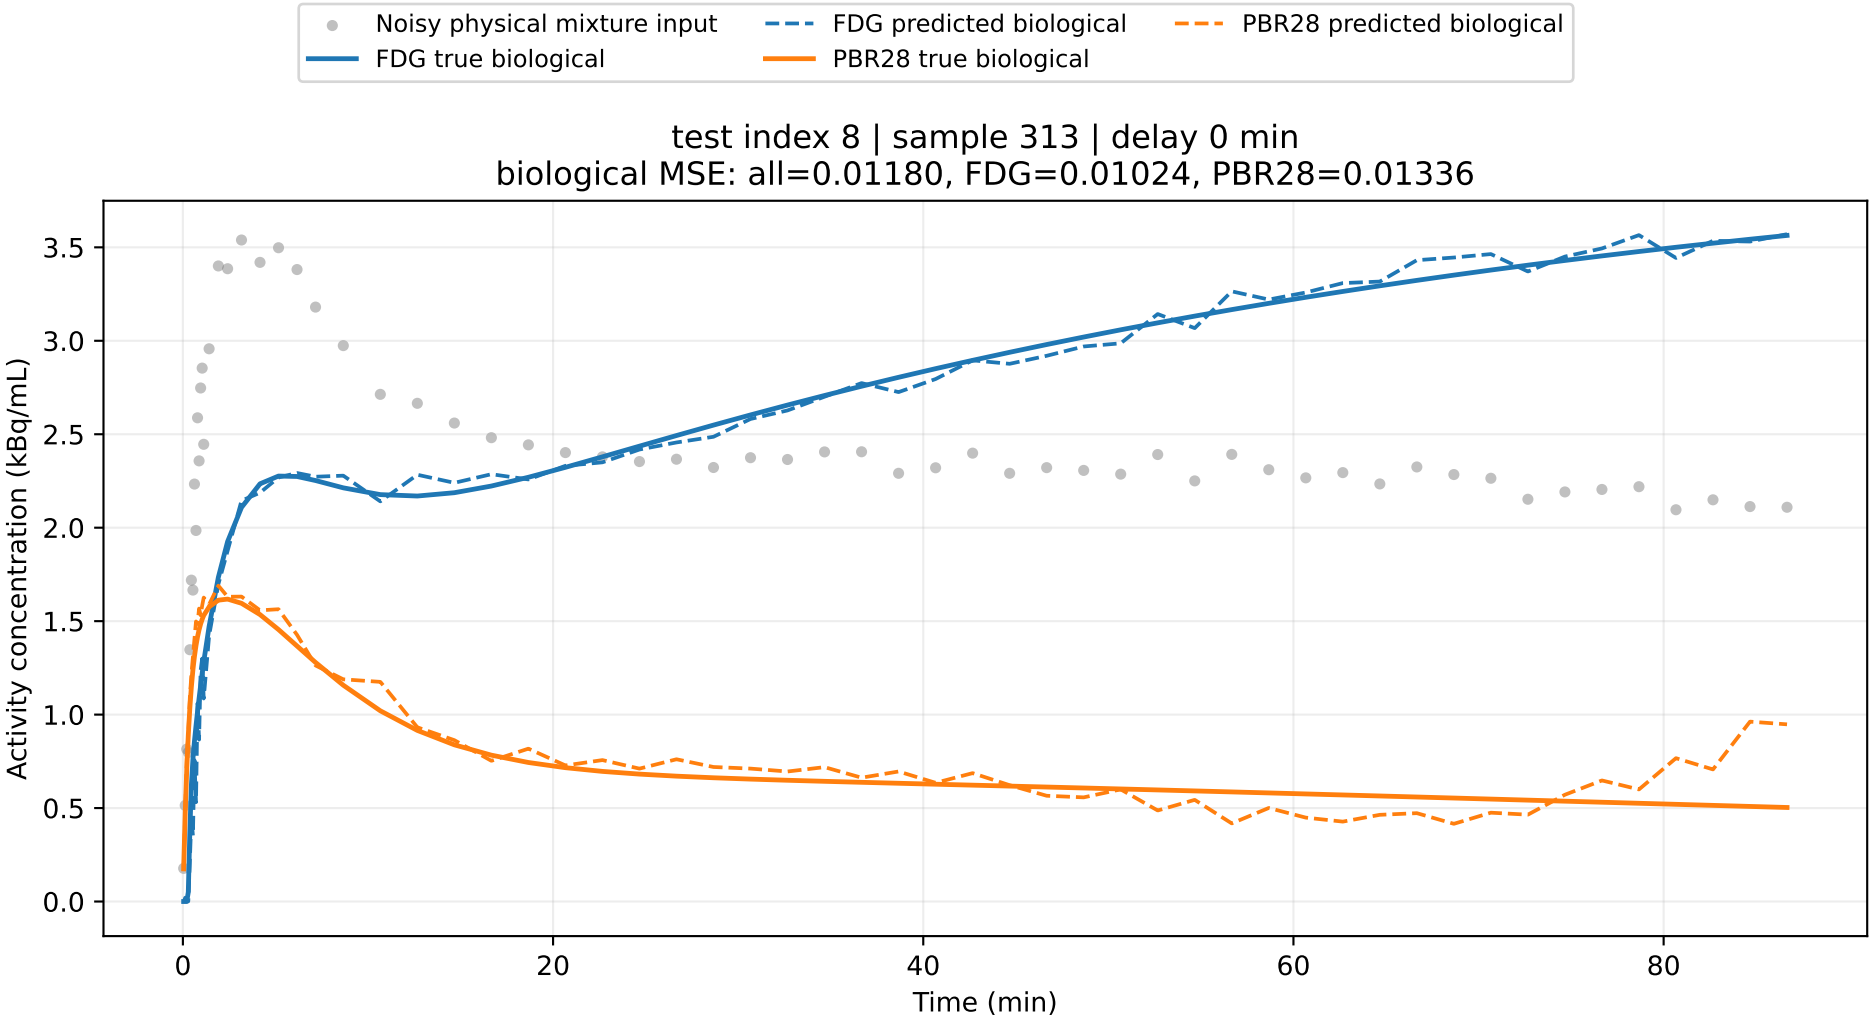

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 3 | sample 678 | delay 5 min
biological MSE: all=0.02452, FDG=0.00924, PBR28=0.03979
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

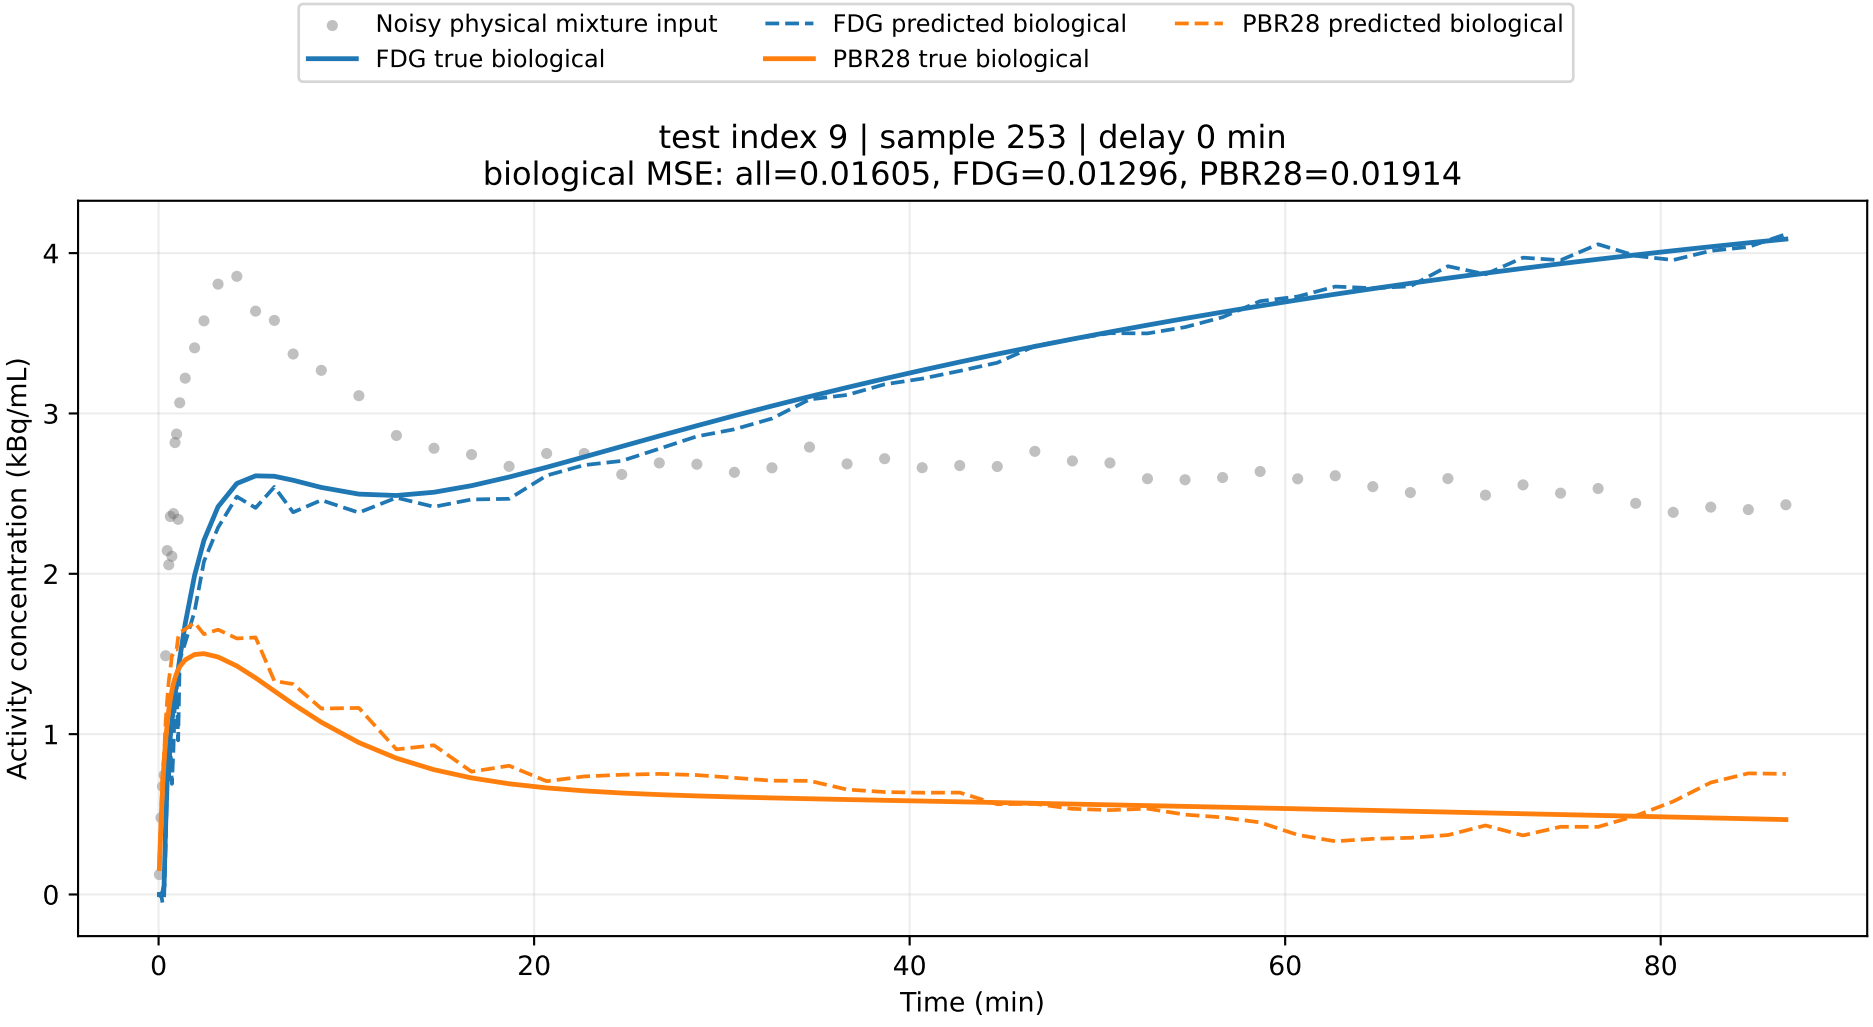

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 4 | sample 417 | delay 10 min
biological MSE: all=0.01802, FDG=0.00468, PBR28=0.03137
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

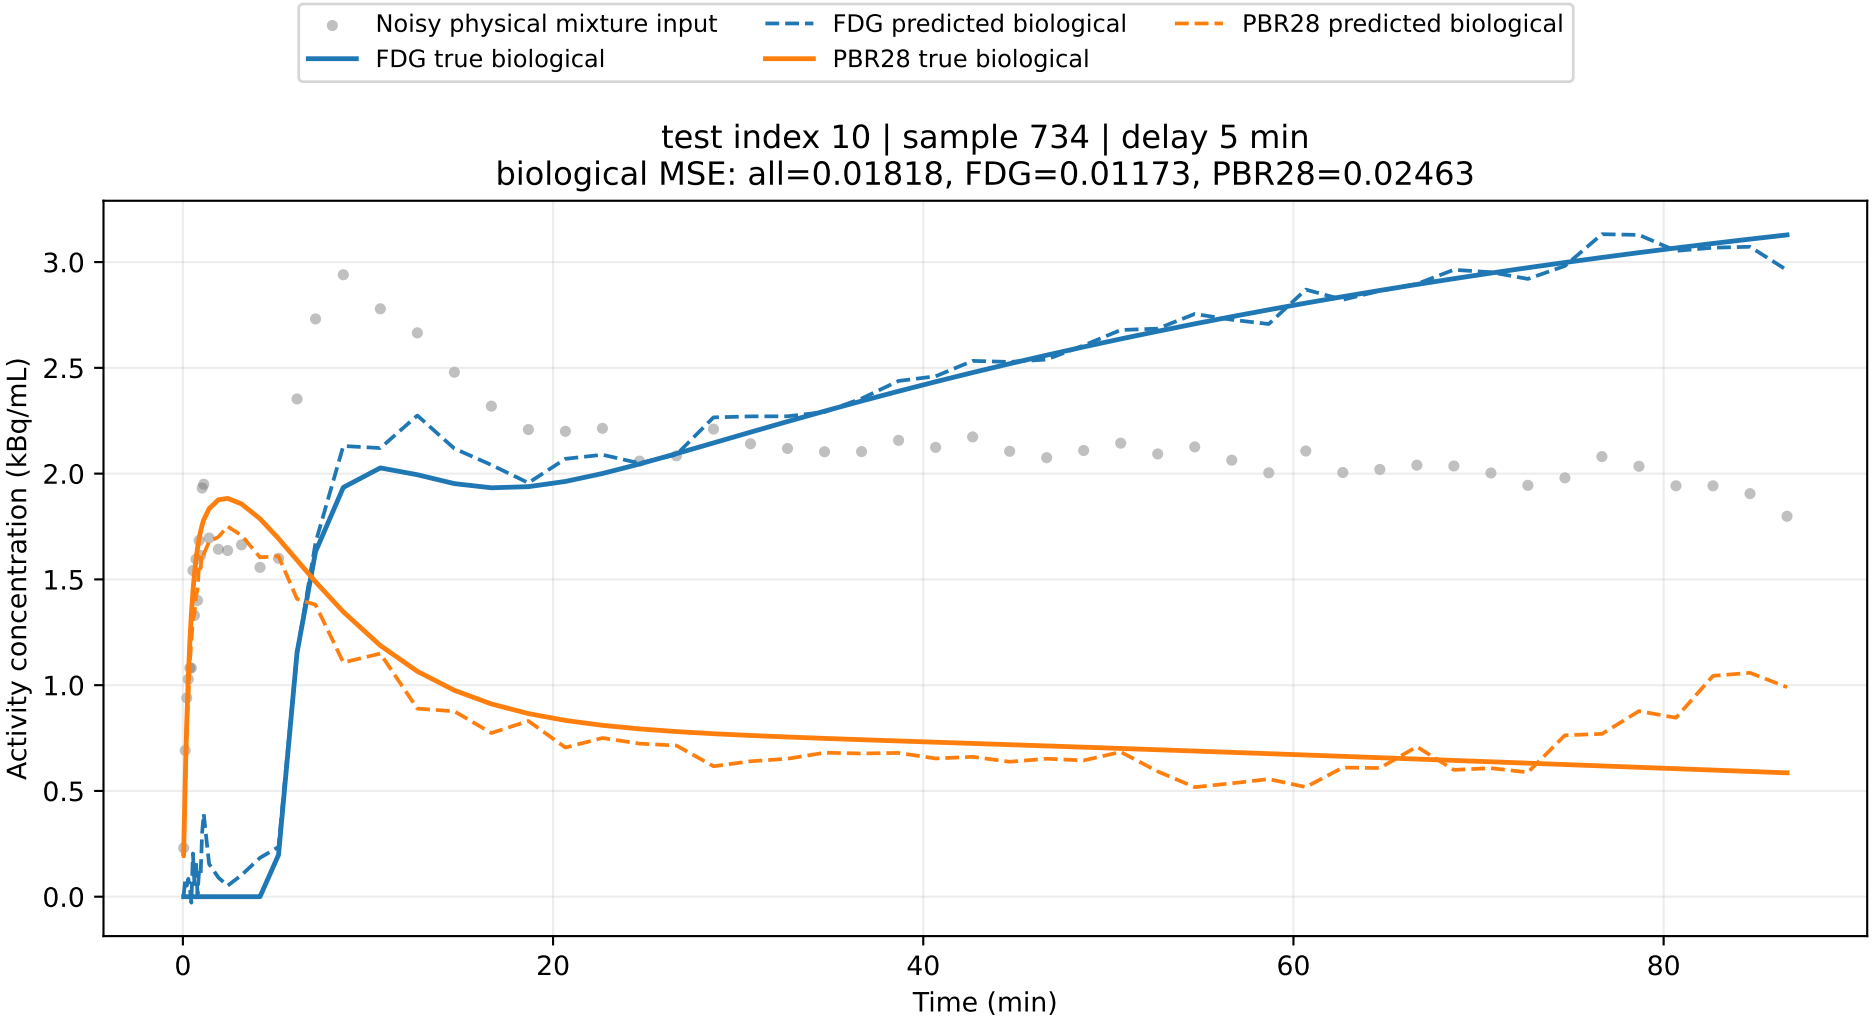

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 5 | sample 277 | delay 0 min
biological MSE: all=0.01756, FDG=0.01006, PBR28=0.02505
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

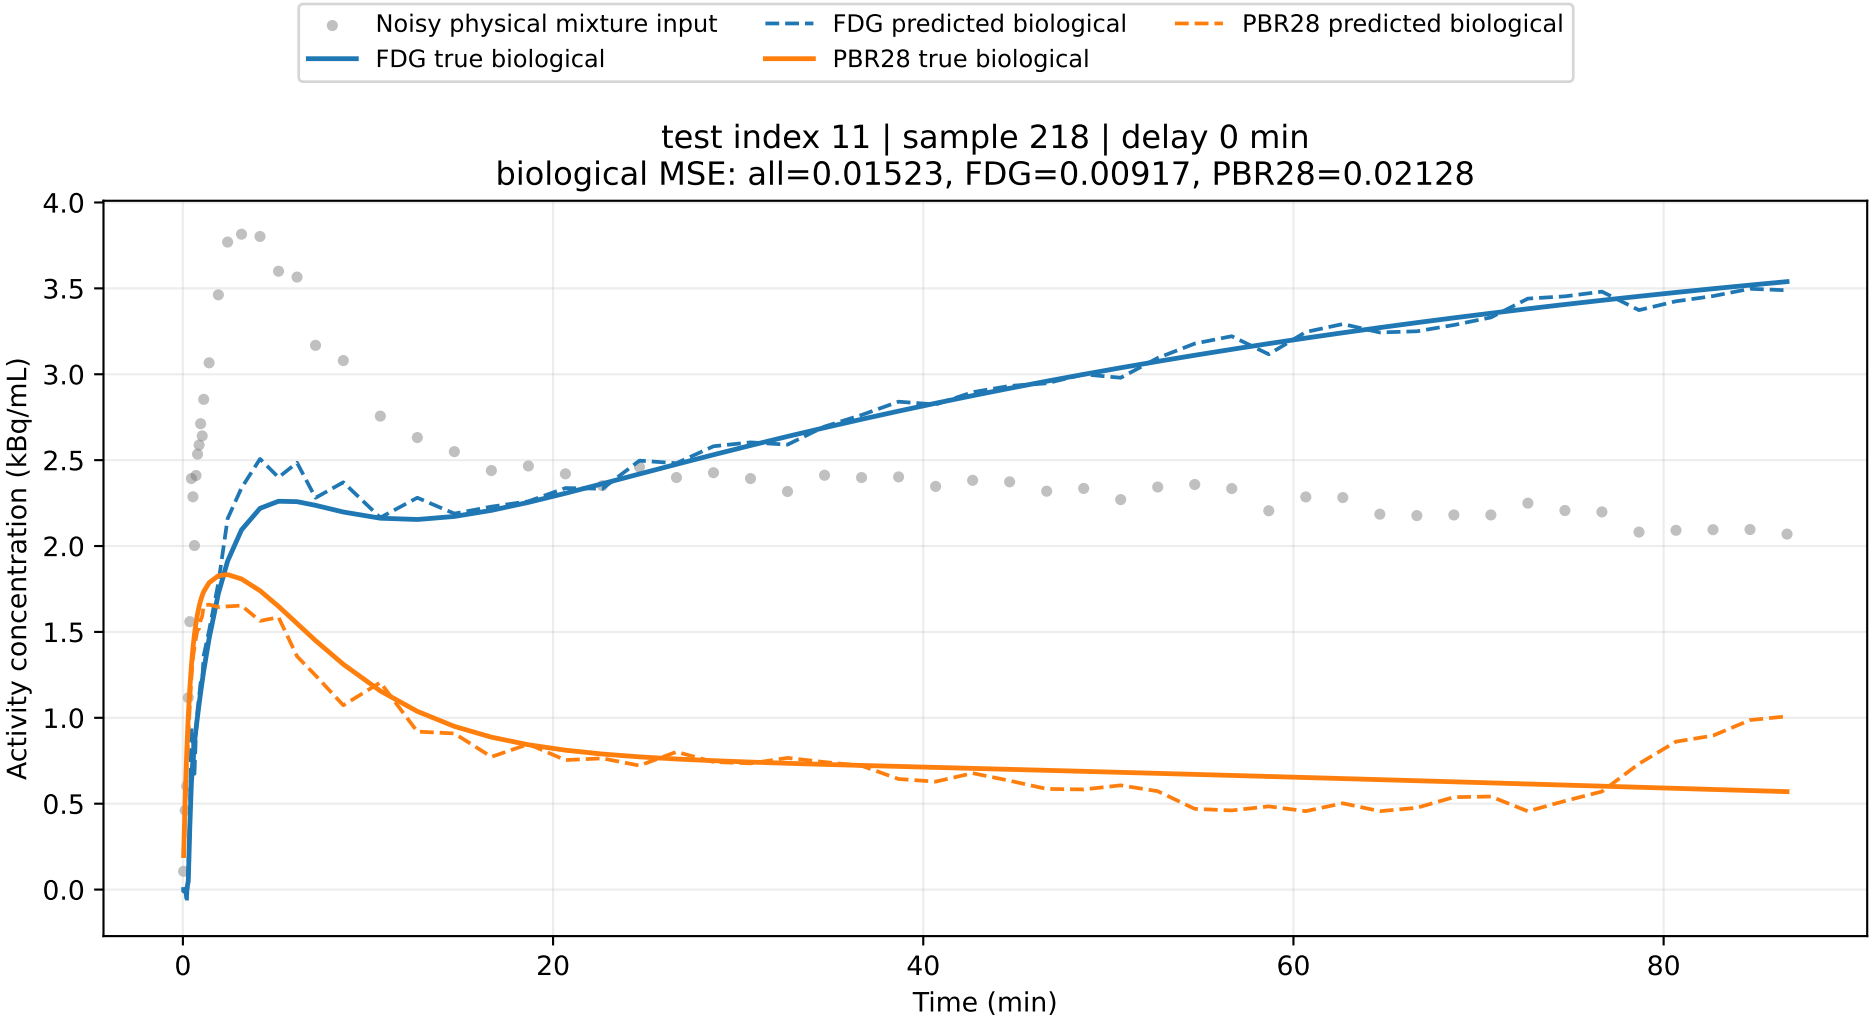

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 6 | sample 852 | delay 10 min
biological MSE: all=0.01626, FDG=0.01319, PBR28=0.01932
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

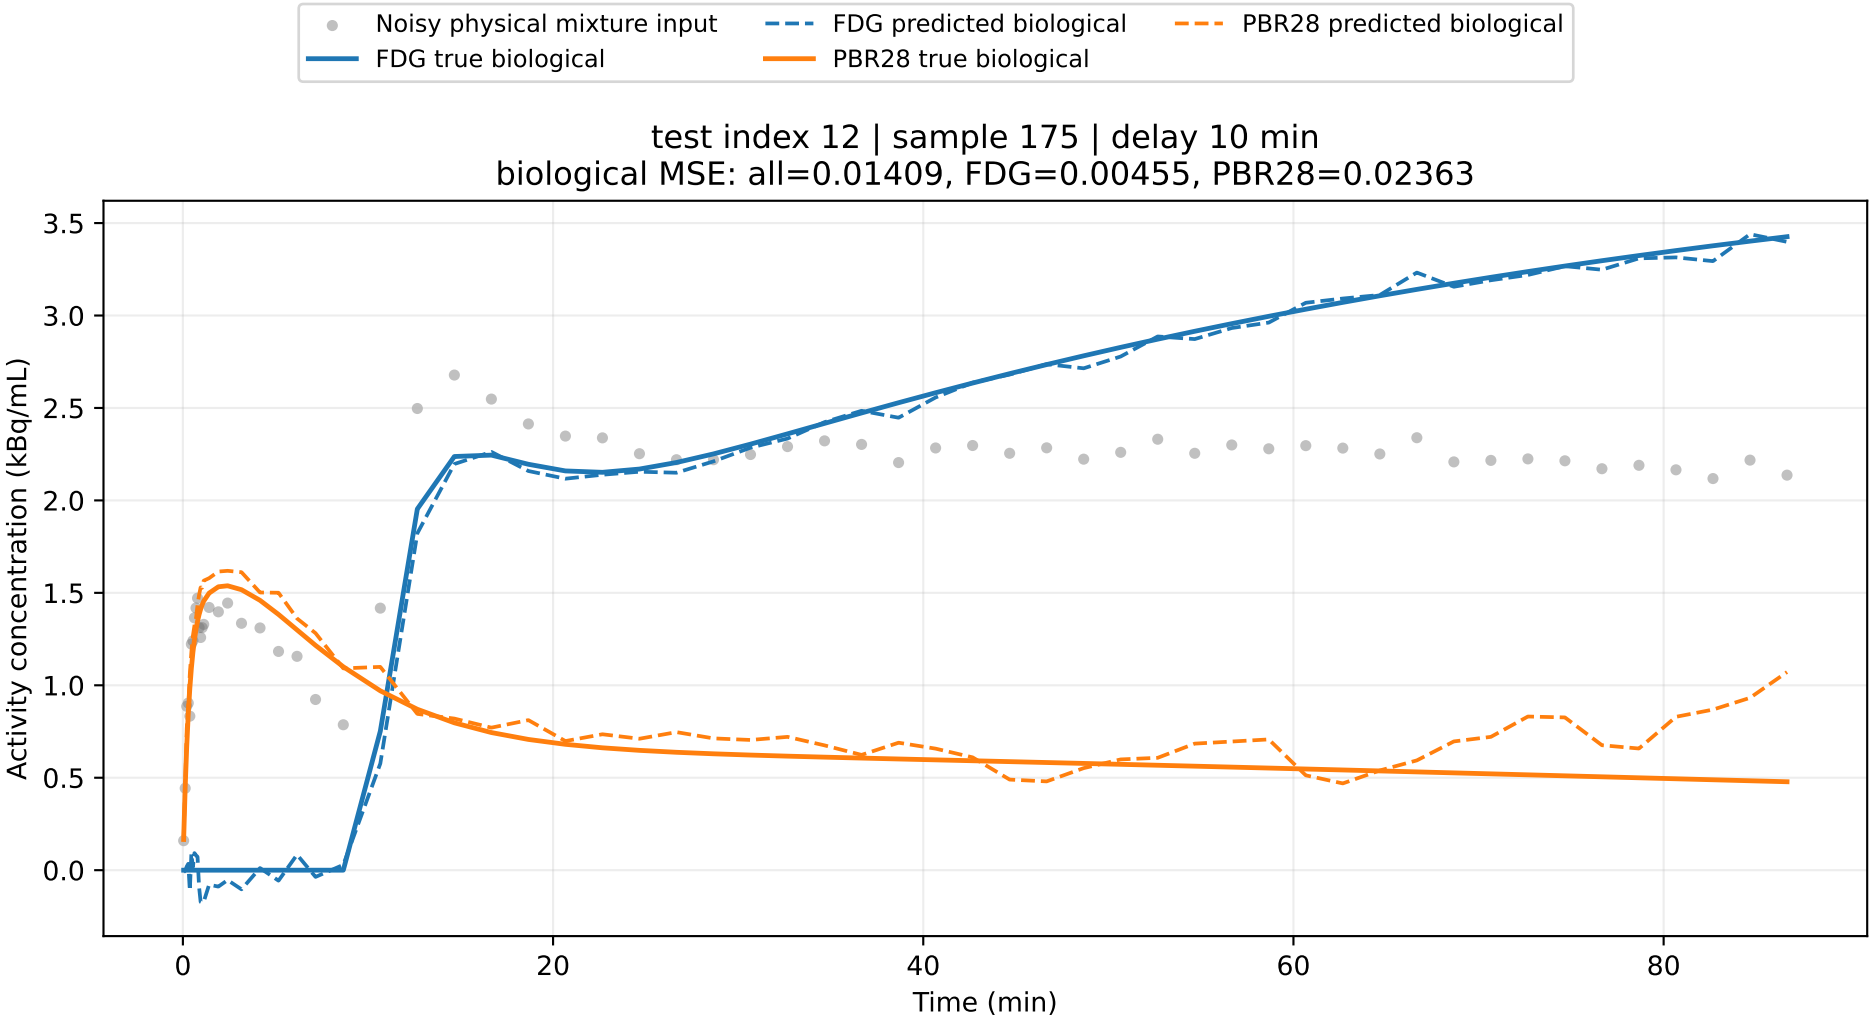

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 7 | sample 485 | delay 5 min
biological MSE: all=0.01281, FDG=0.00831, PBR28=0.01731
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

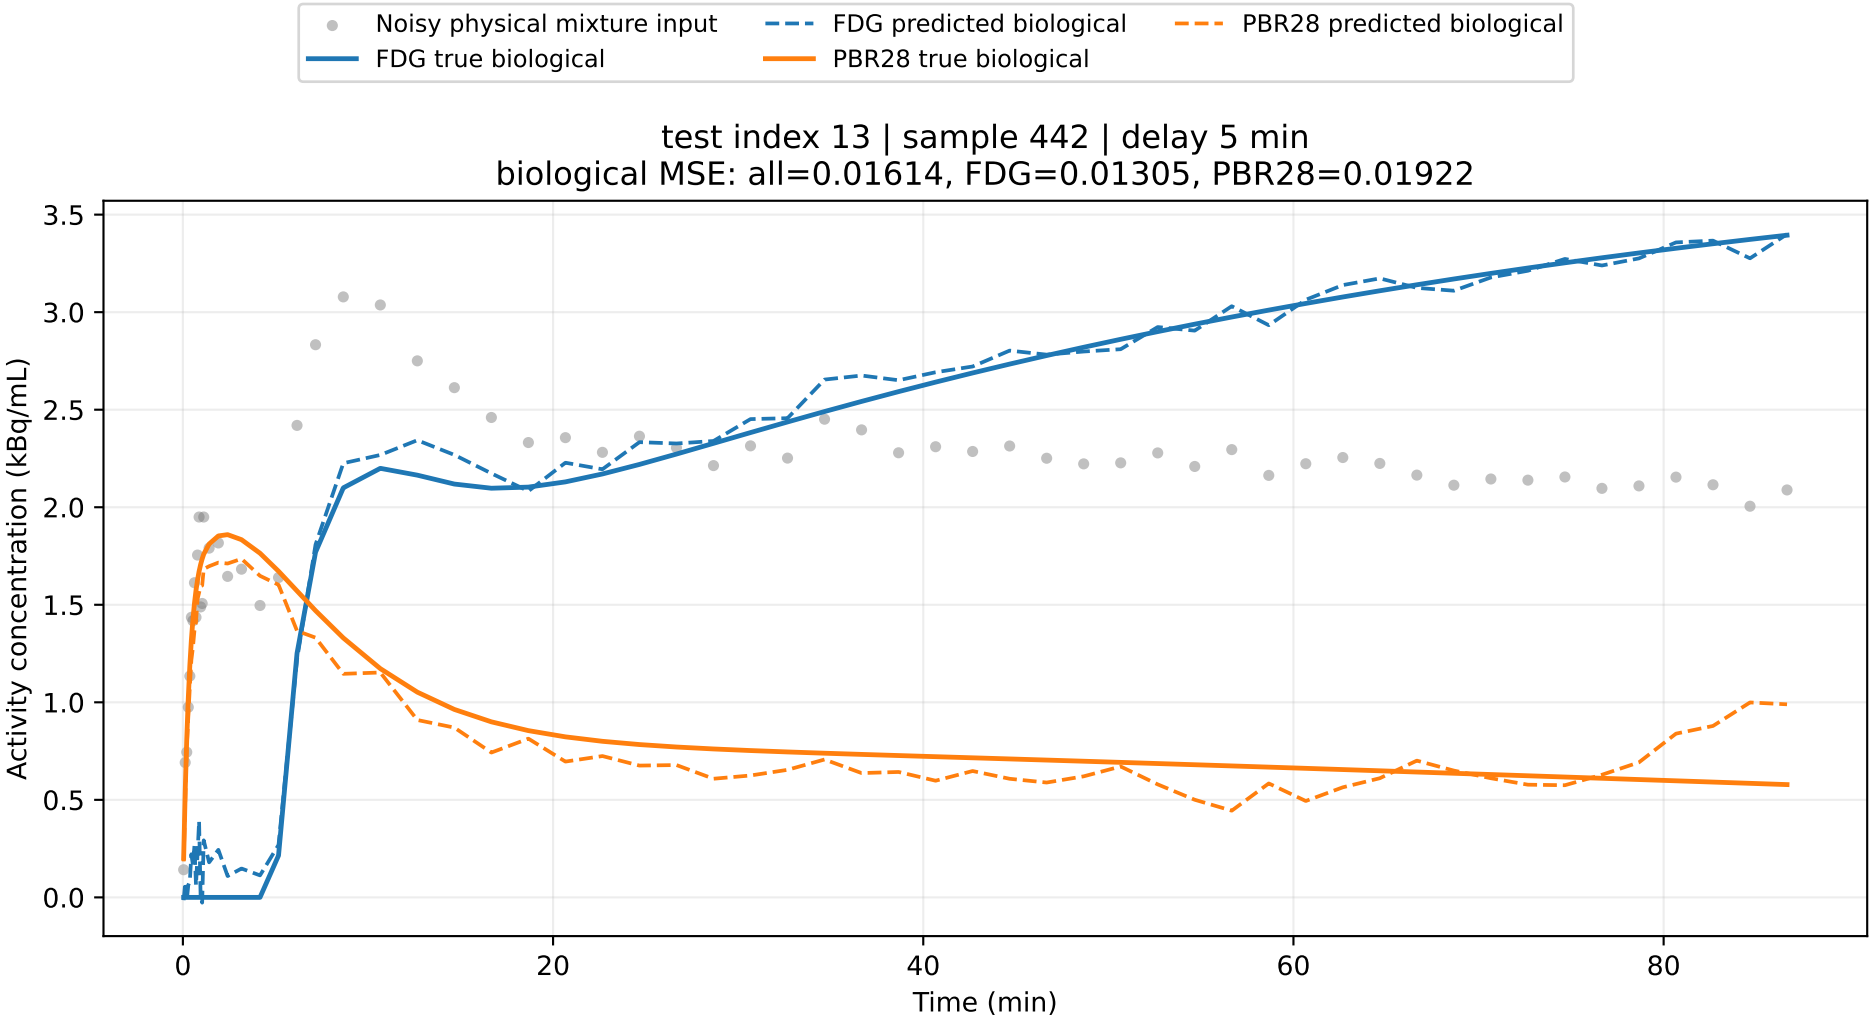

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 8 | sample 313 | delay 0 min
biological MSE: all=0.01180, FDG=0.01024, PBR28=0.01336
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

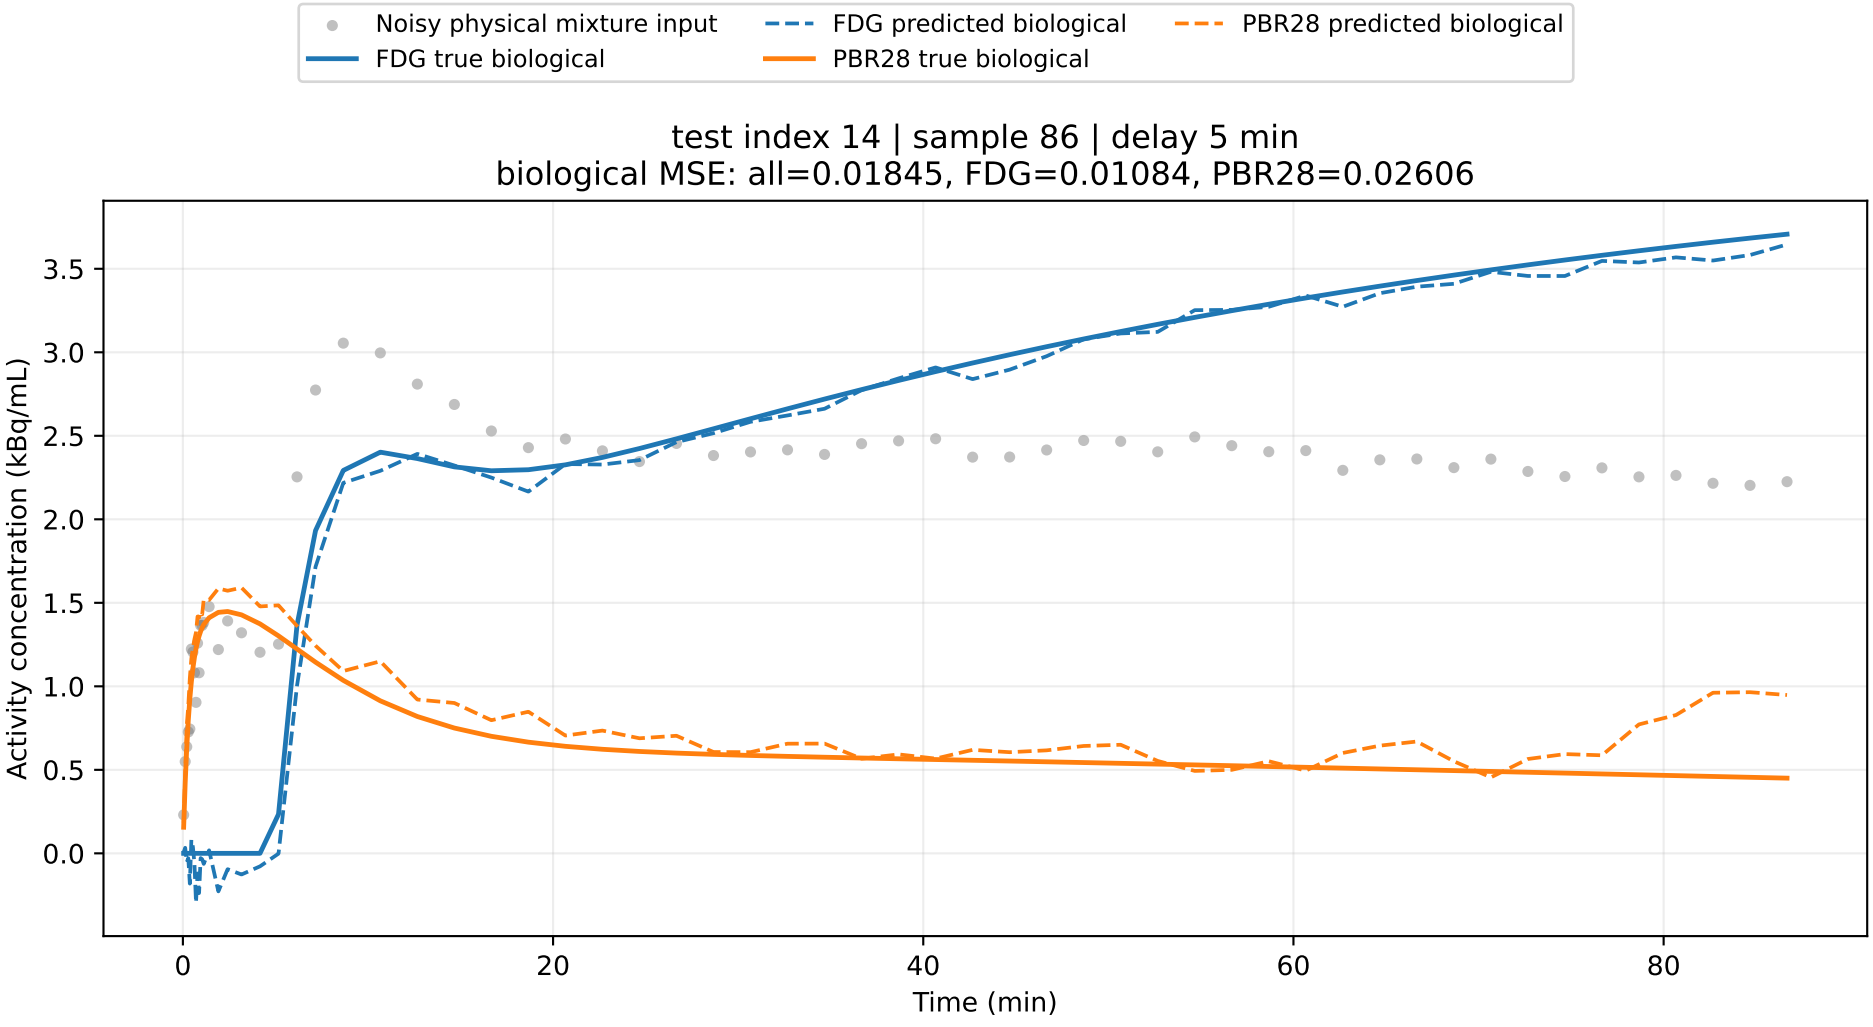

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 9 | sample 253 | delay 0 min
biological MSE: all=0.01605, FDG=0.01296, PBR28=0.01914
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

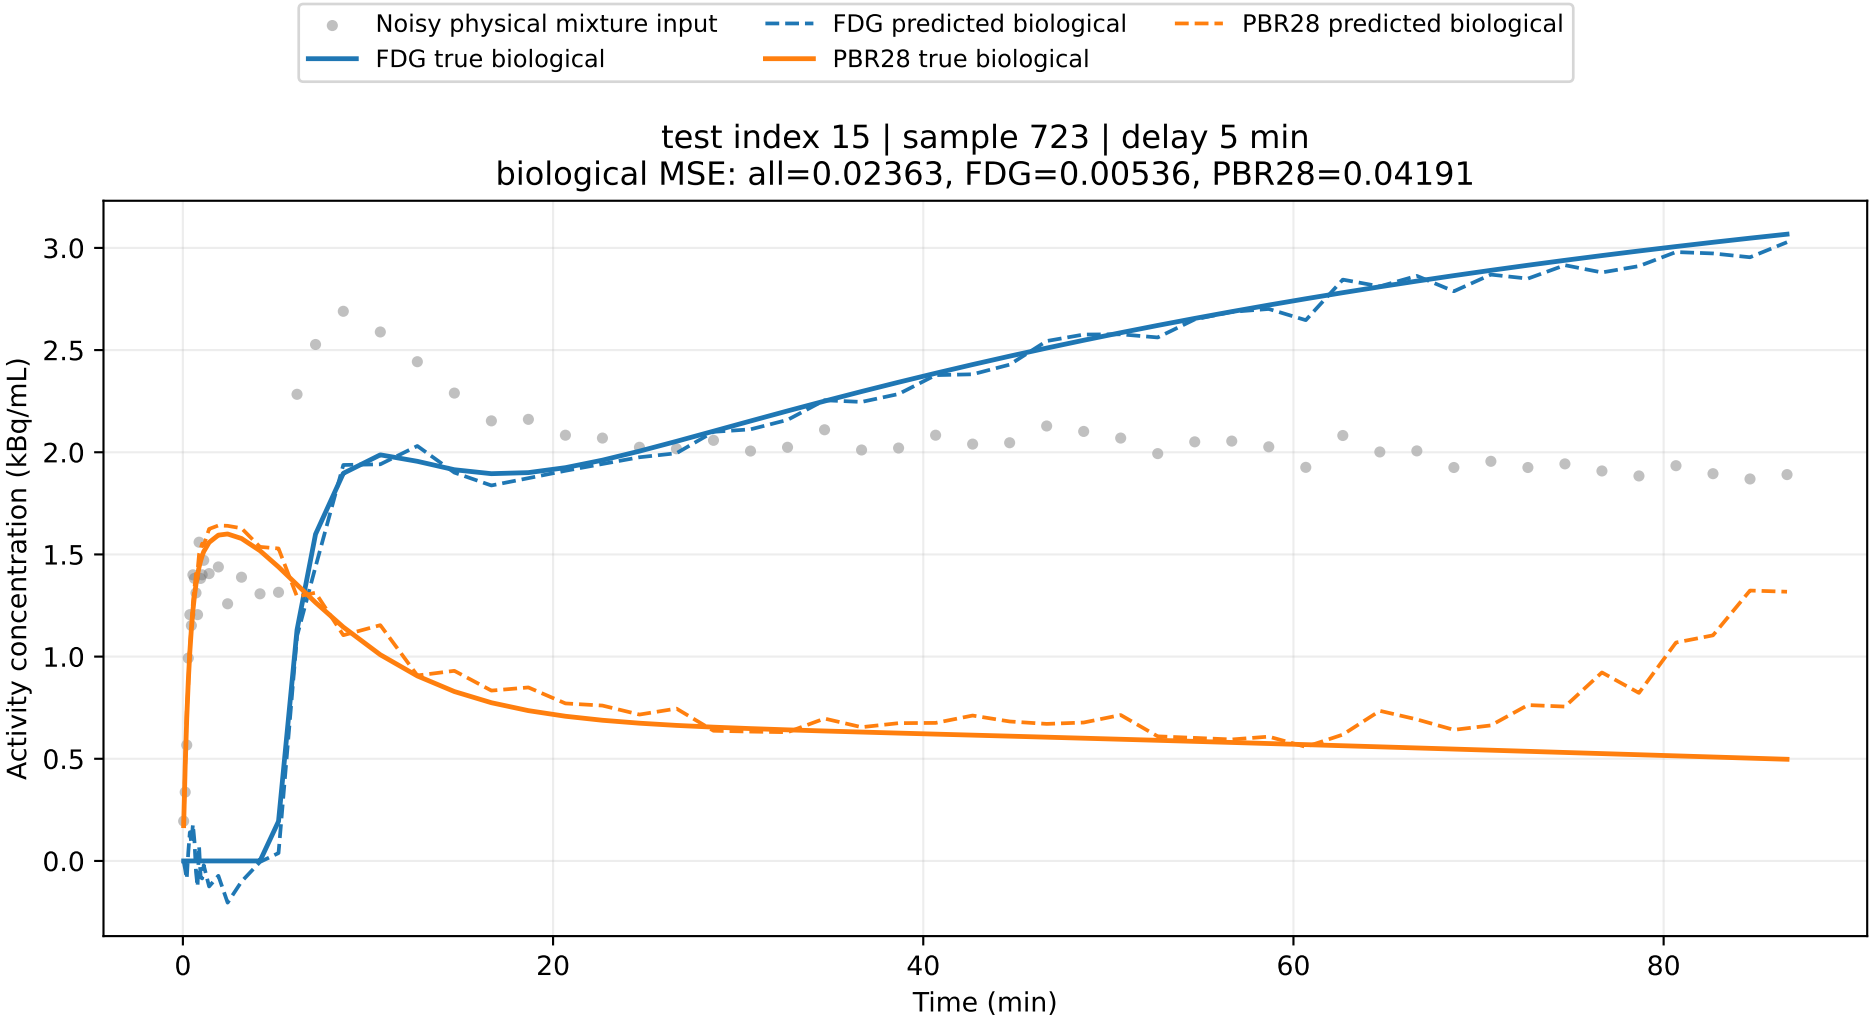

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 10 | sample 734 | delay 5 min
biological MSE: all=0.01818, FDG=0.01173, PBR28=0.02463
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

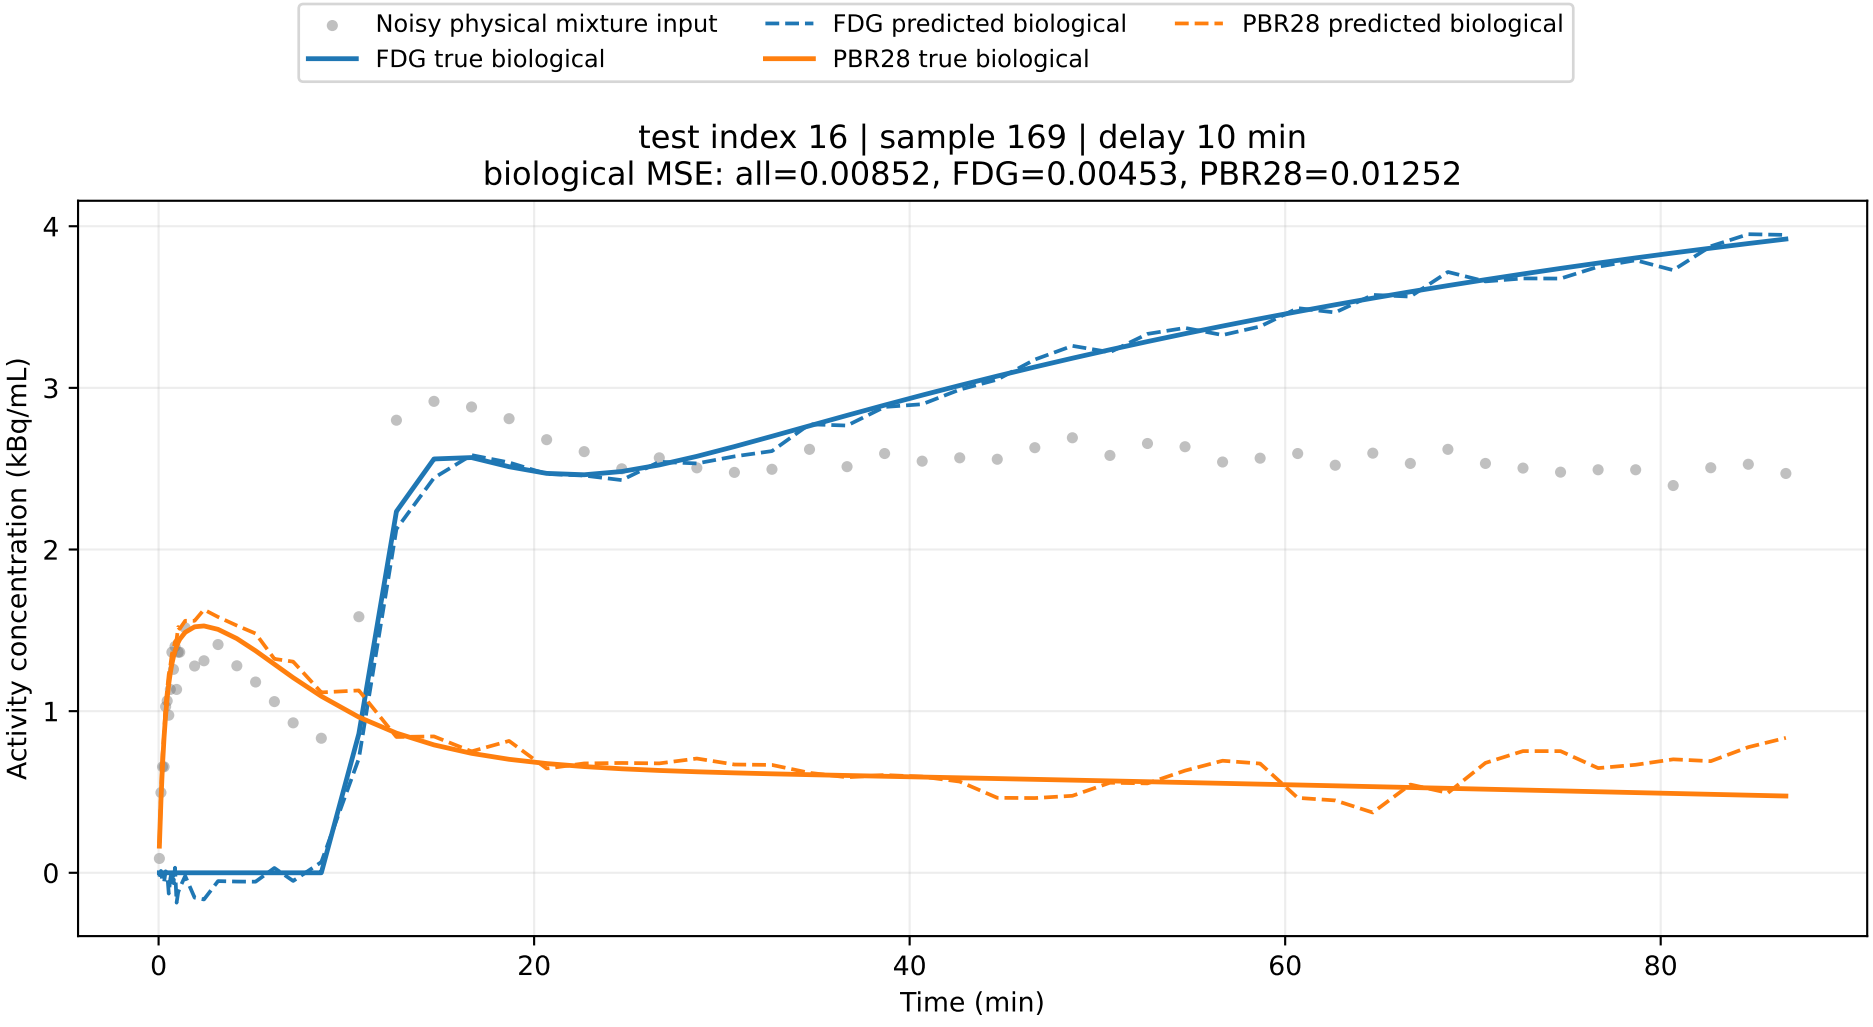

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 11 | sample 218 | delay 0 min
biological MSE: all=0.01523, FDG=0.00917, PBR28=0.02128
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

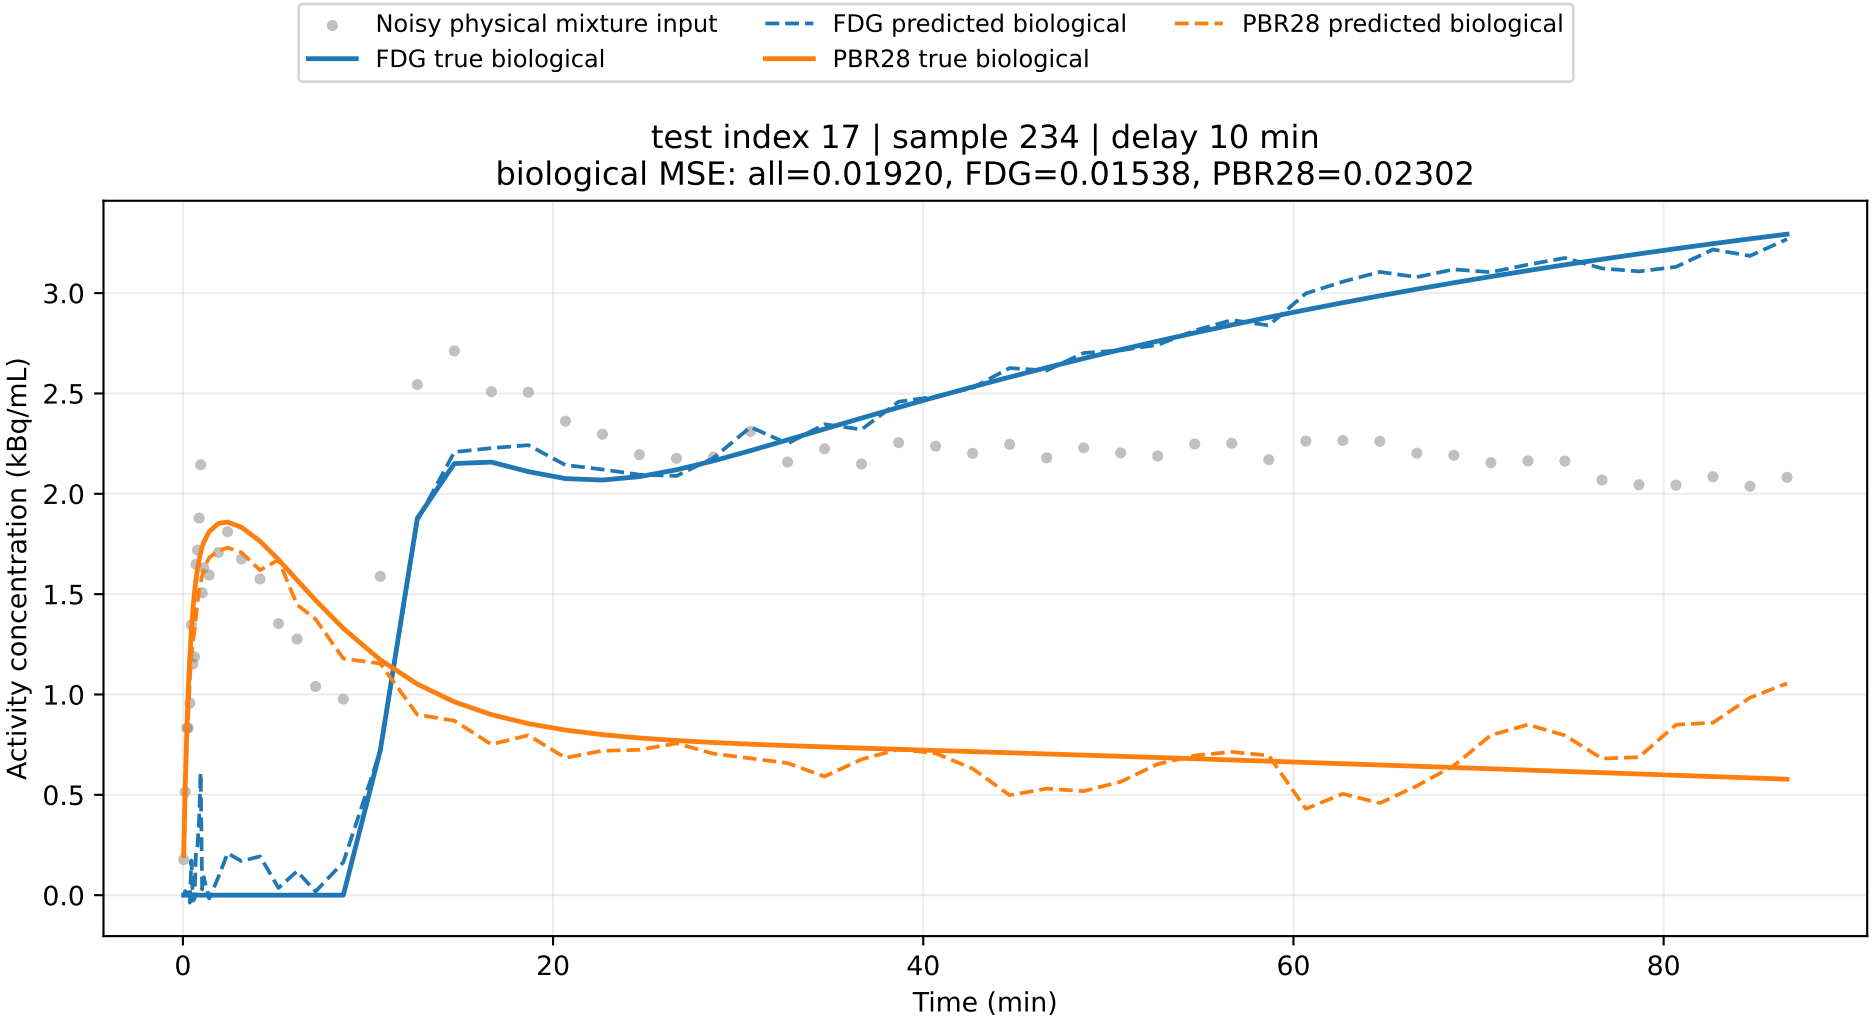

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 12 | sample 175 | delay 10 min
biological MSE: all=0.01409, FDG=0.00455, PBR28=0.02363
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

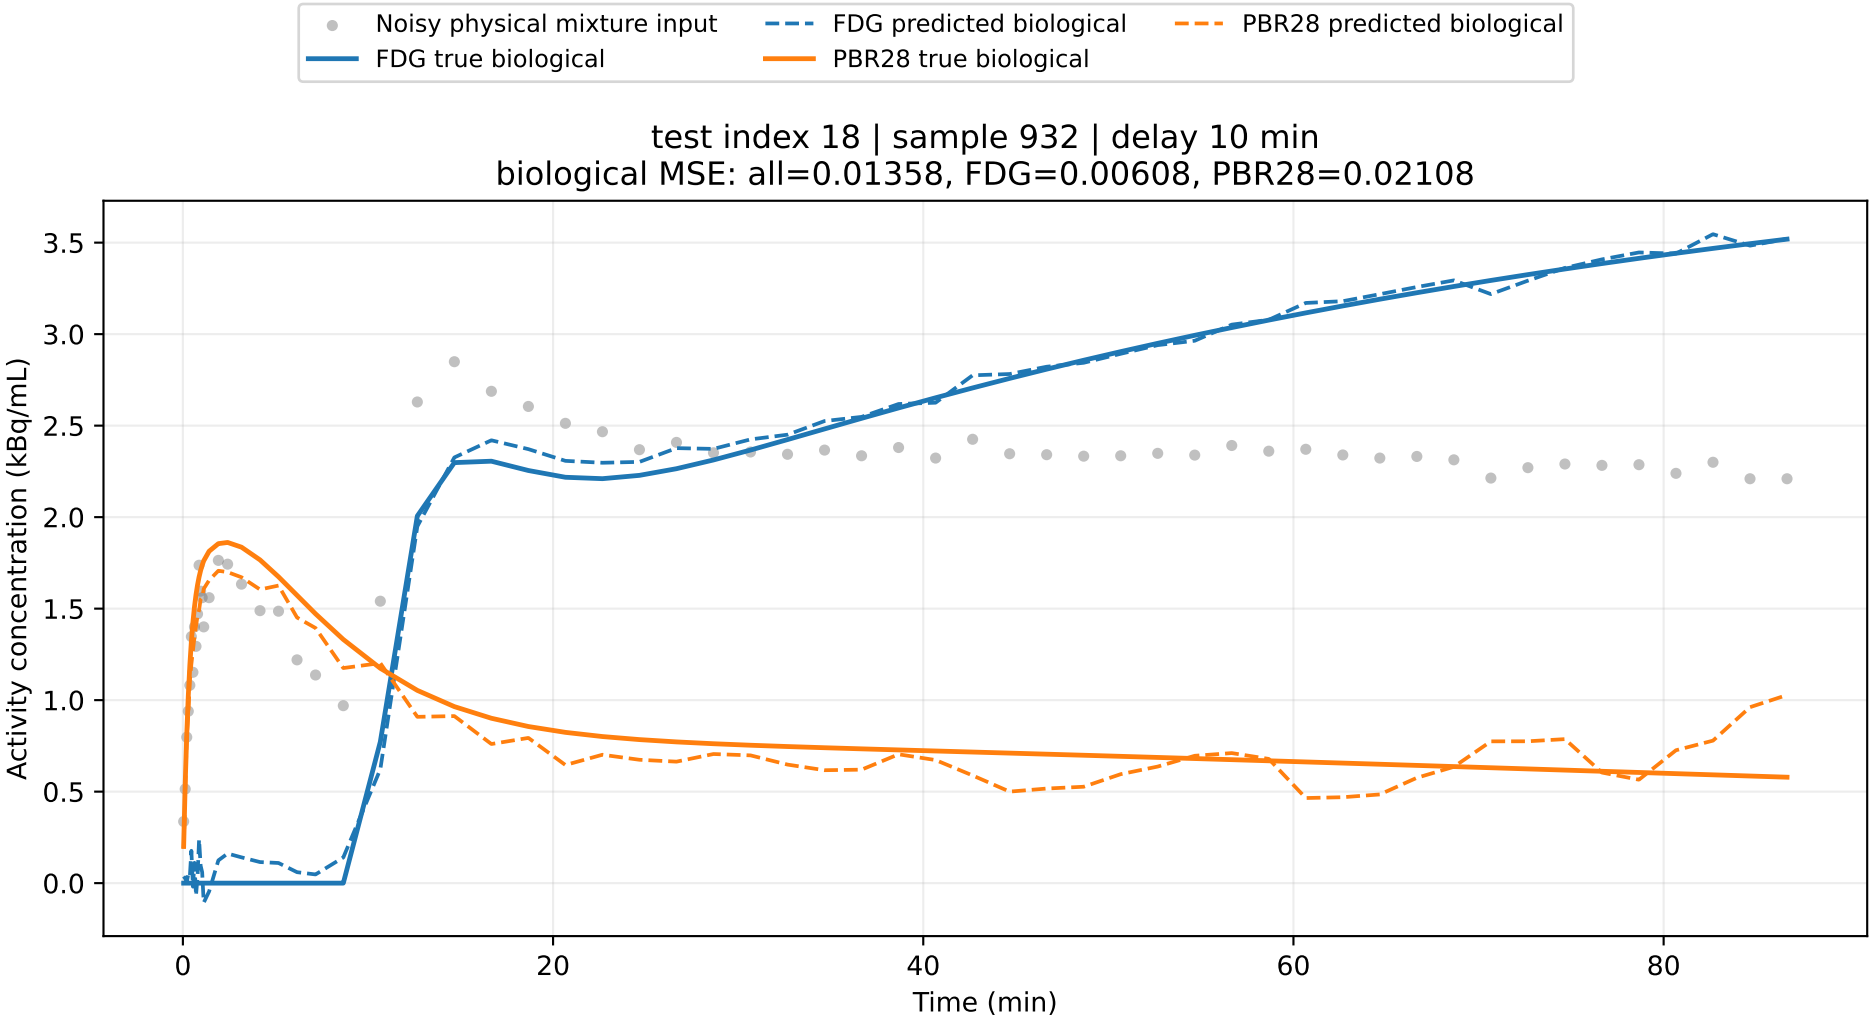

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 13 | sample 442 | delay 5 min
biological MSE: all=0.01614, FDG=0.01305, PBR28=0.01922
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

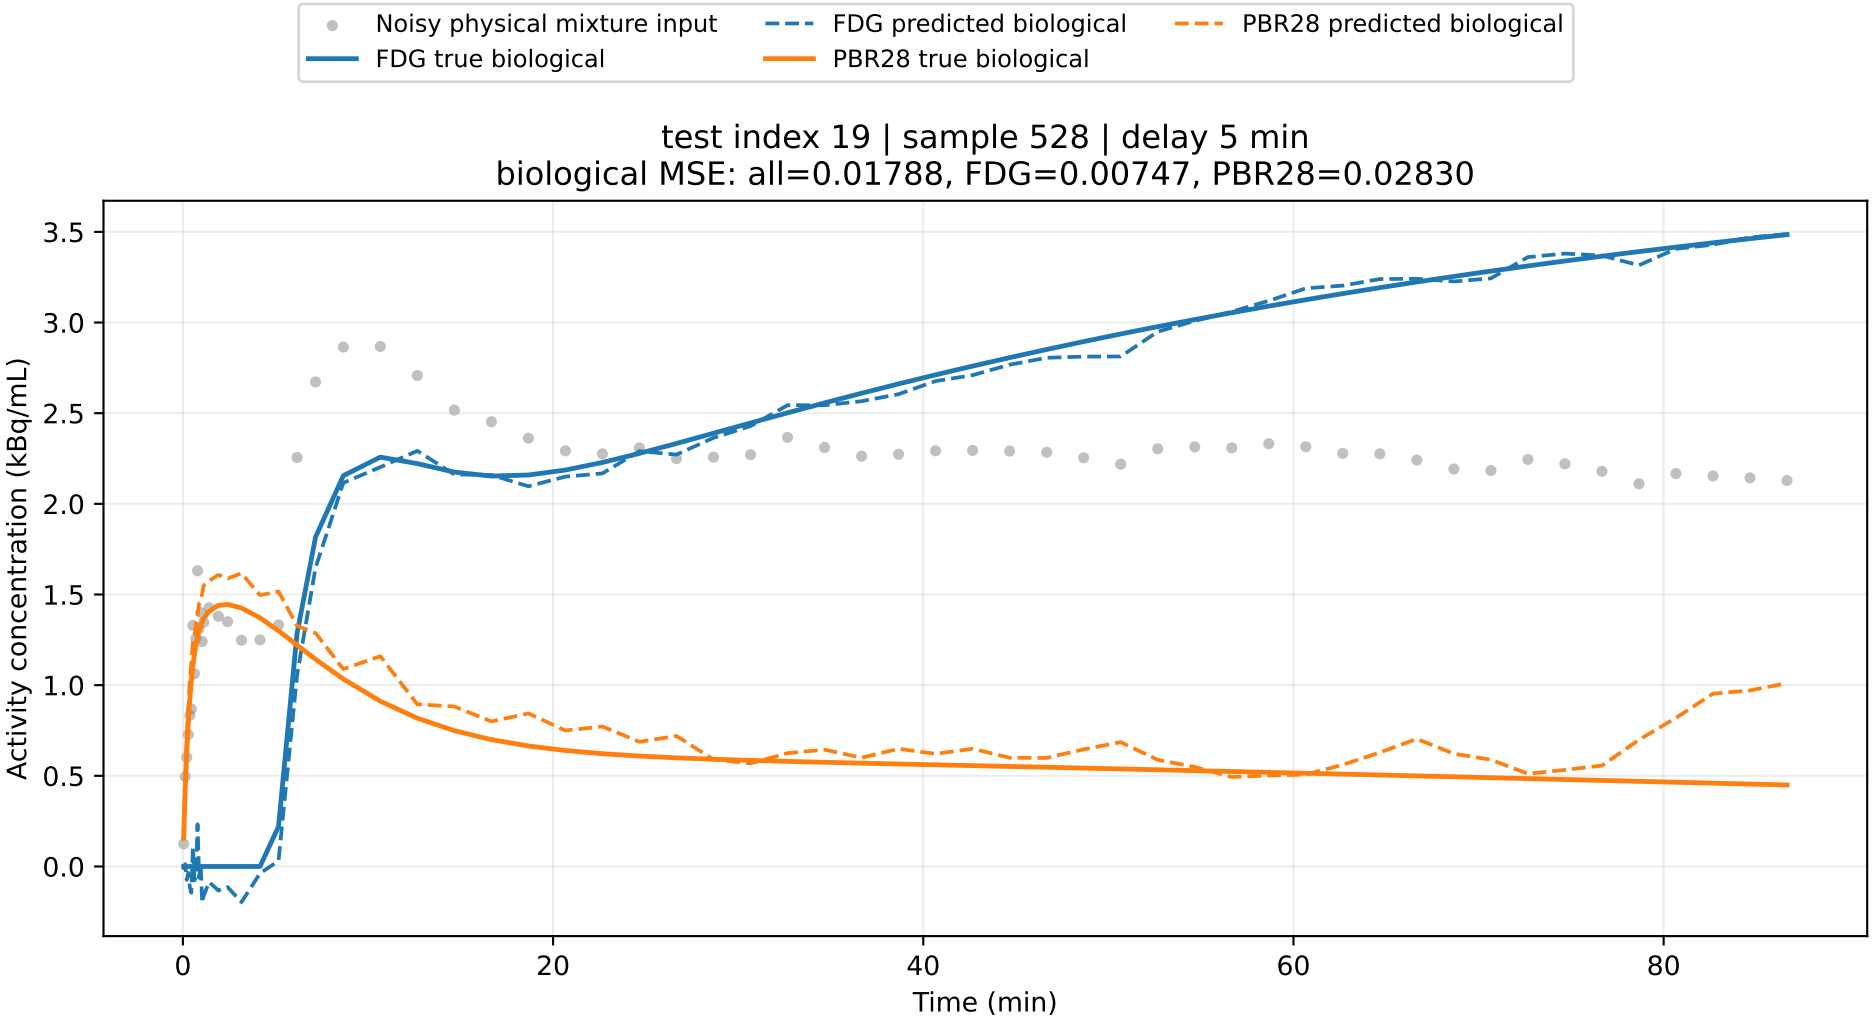

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 14 | sample 86 | delay 5 min
biological MSE: all=0.01845, FDG=0.01084, PBR28=0.02606
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

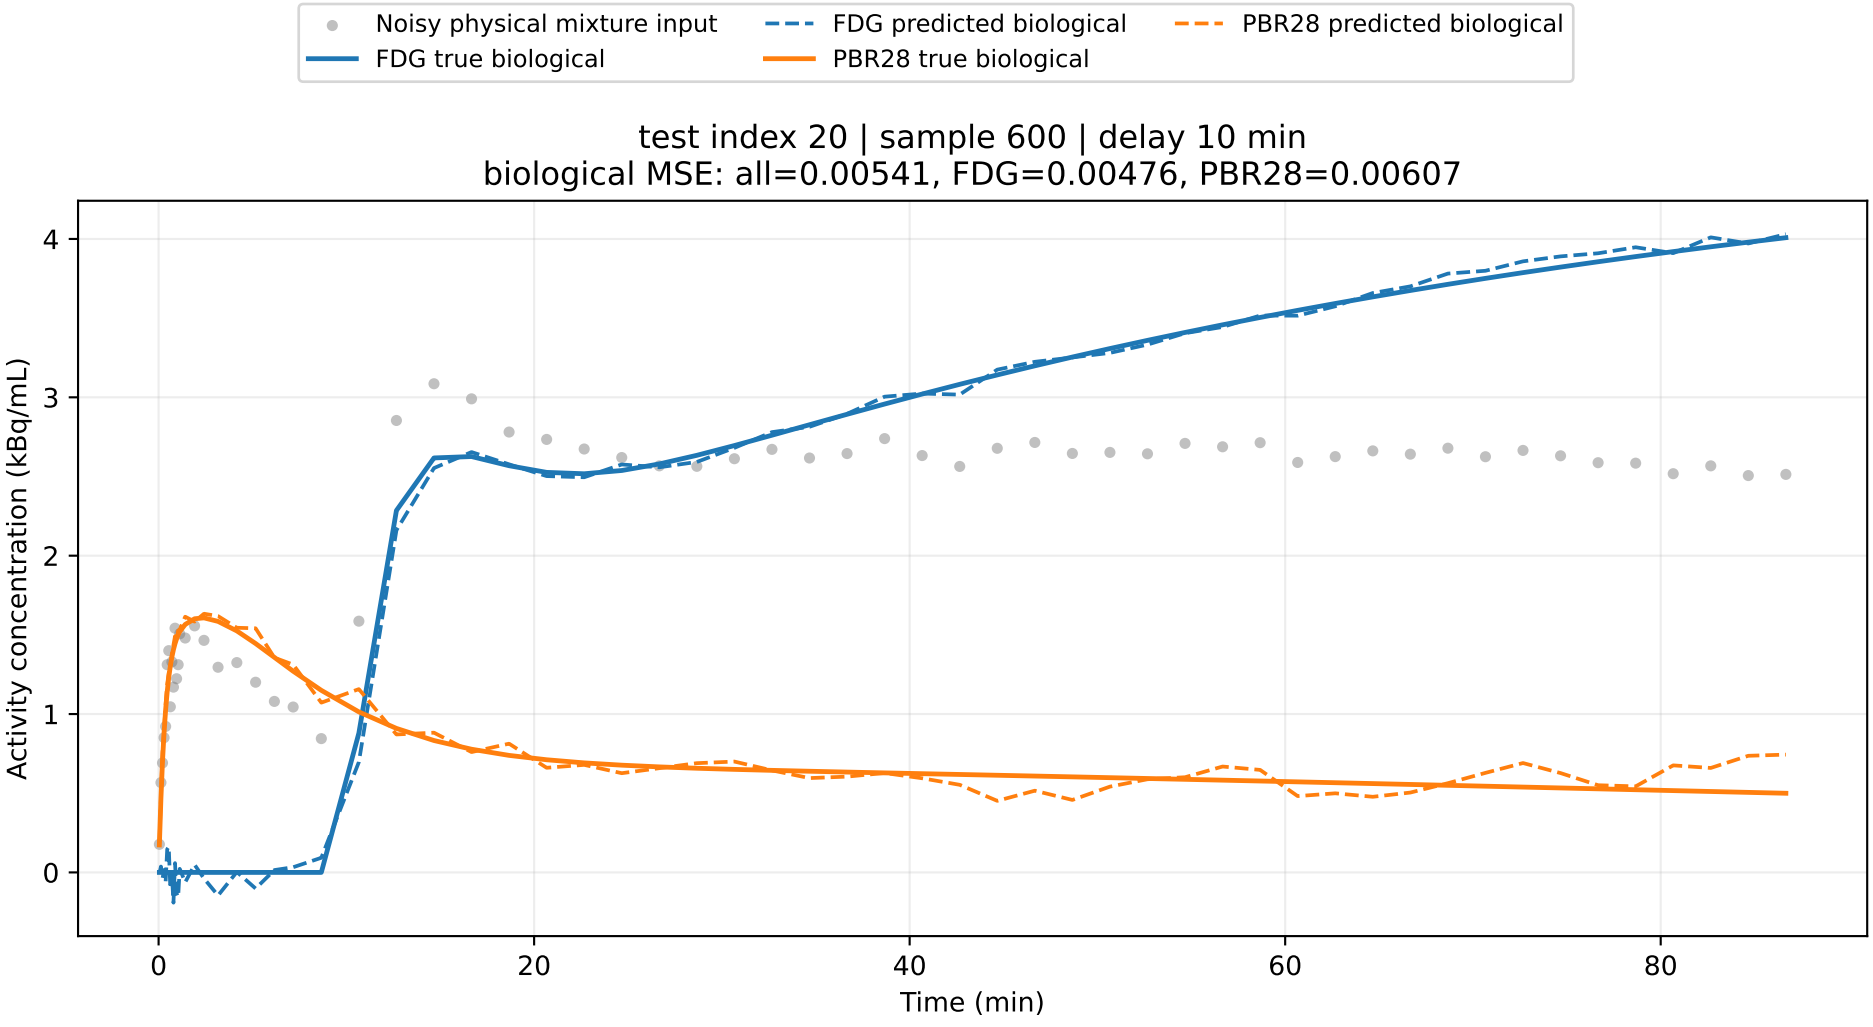

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 15 | sample 723 | delay 5 min
biological MSE: all=0.02363, FDG=0.00536, PBR28=0.04191
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

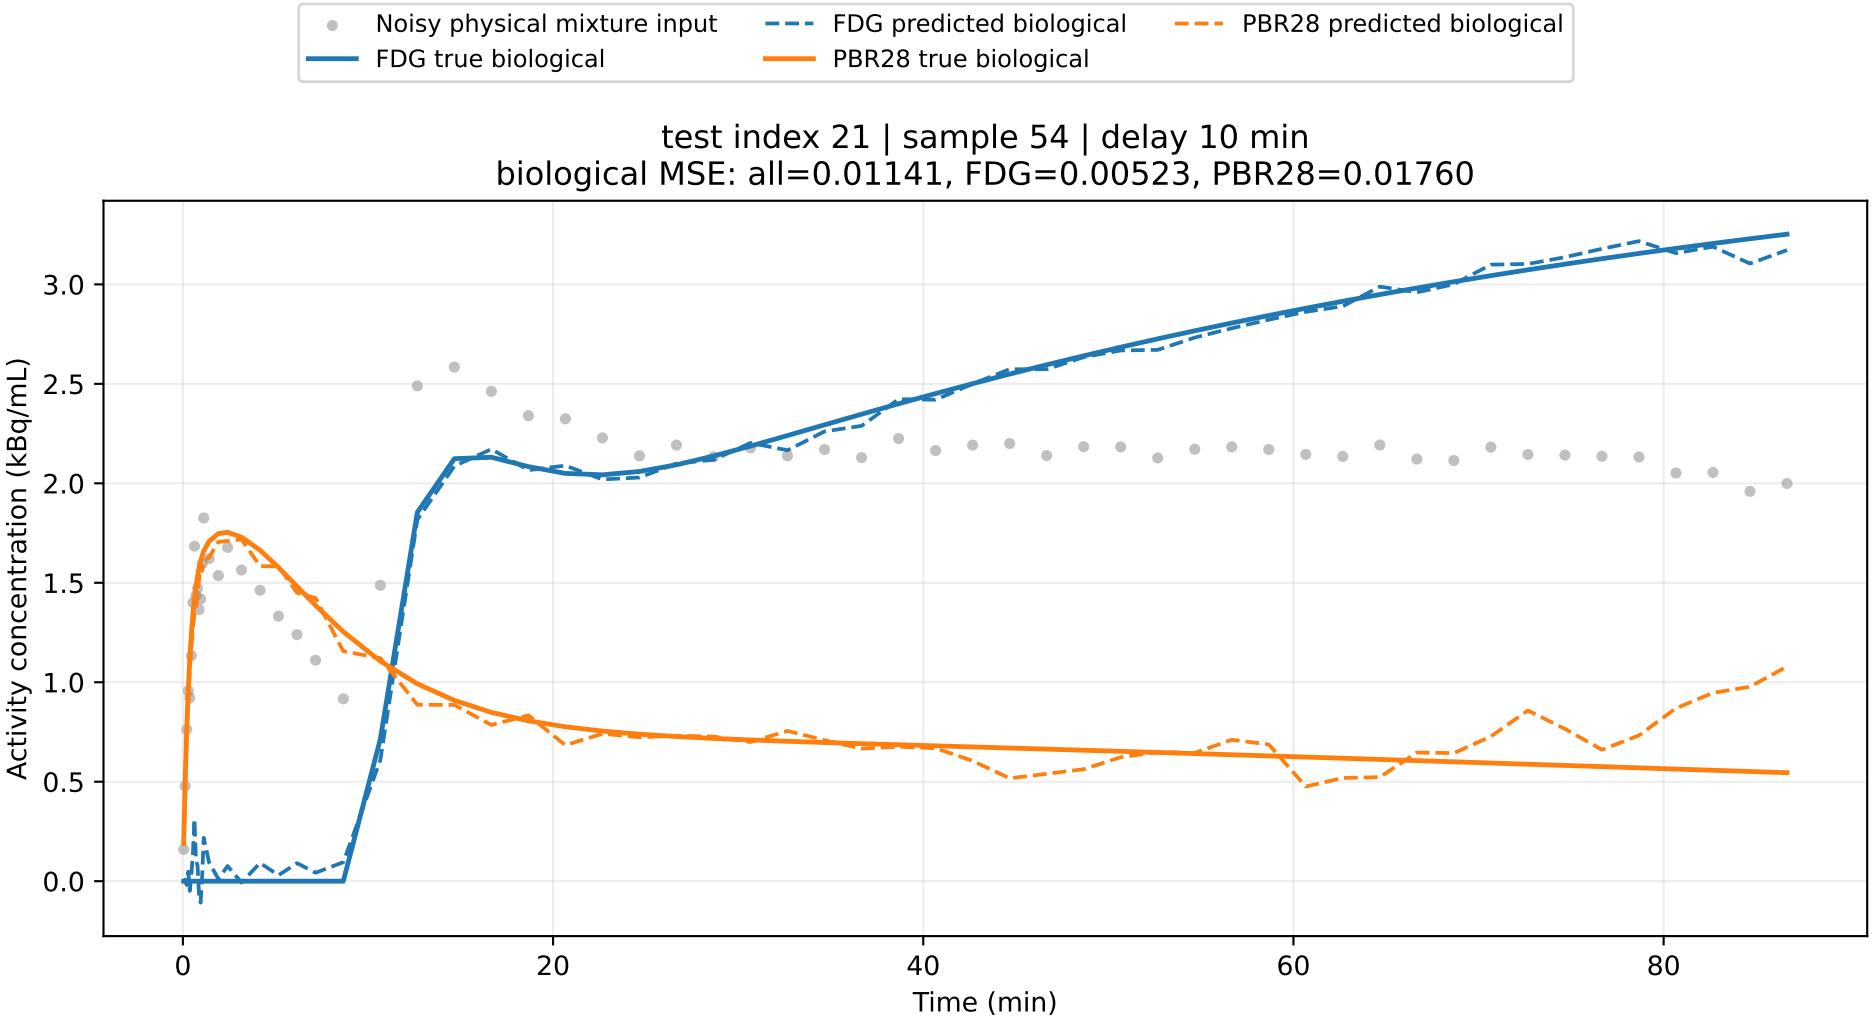

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 16 | sample 169 | delay 10 min
biological MSE: all=0.00852, FDG=0.00453, PBR28=0.01252
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

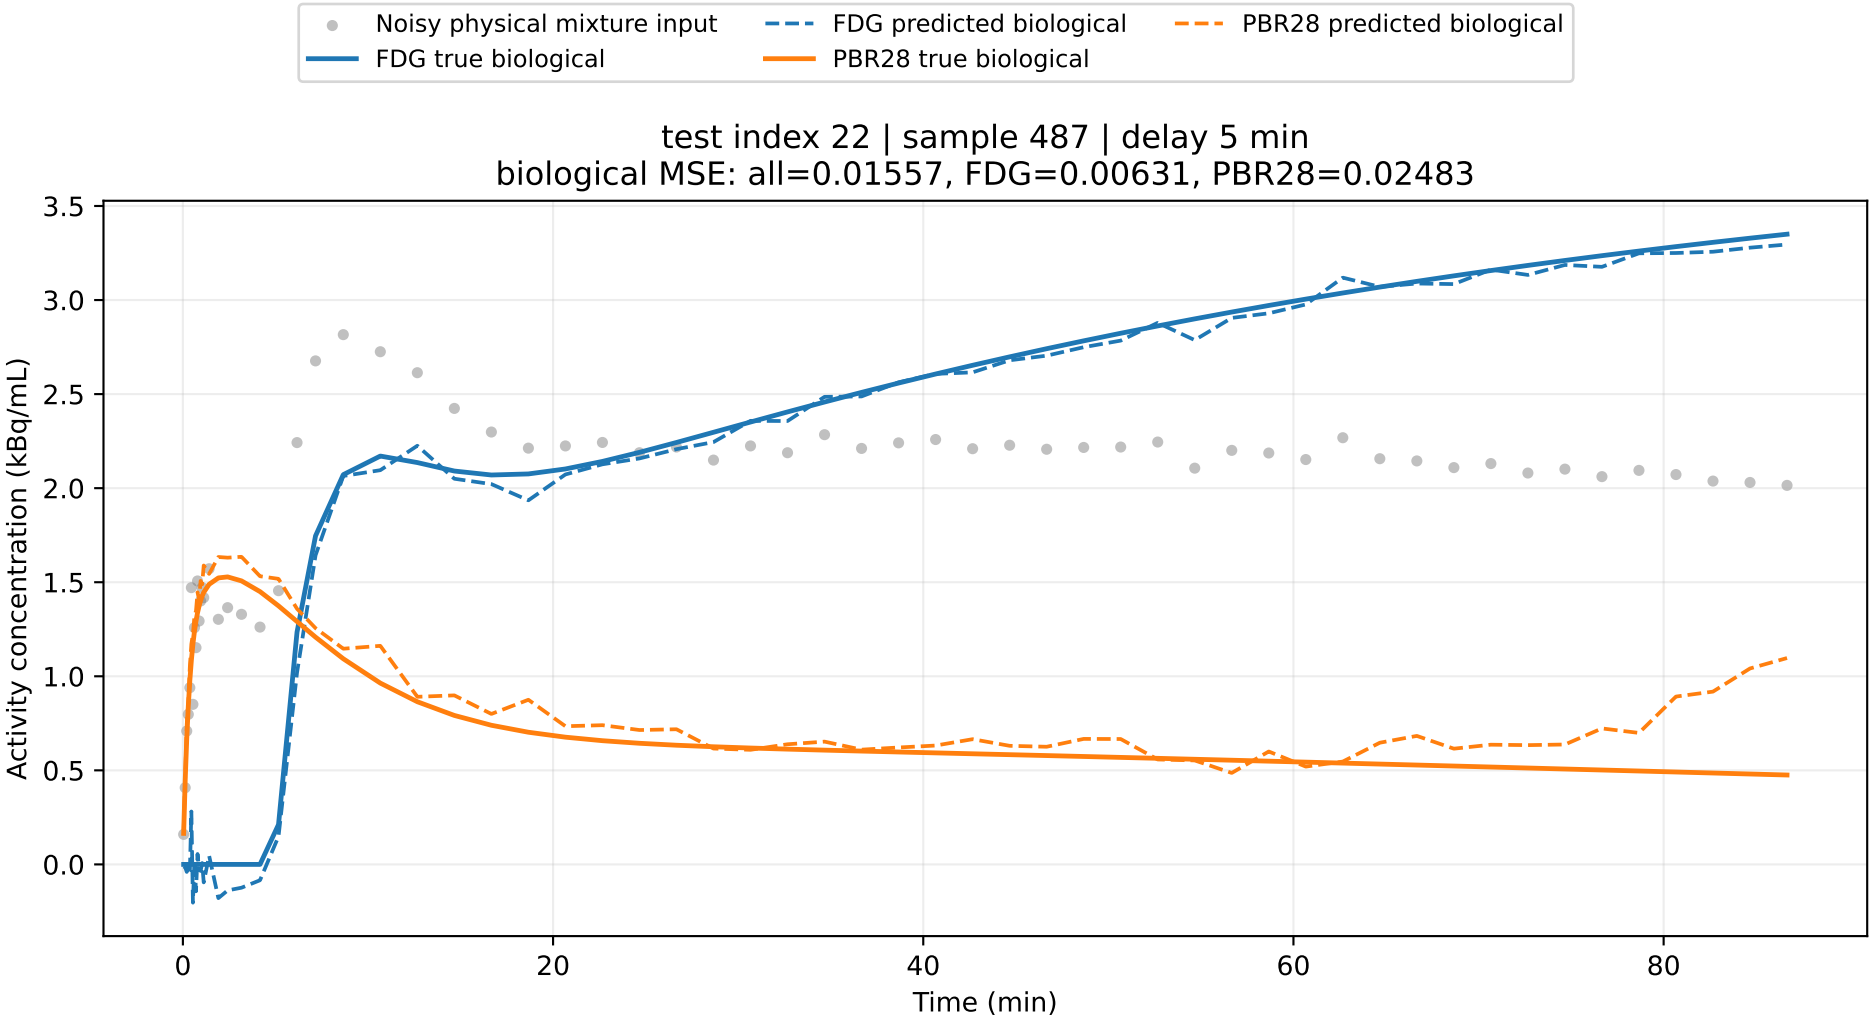

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 17 | sample 234 | delay 10 min
biological MSE: all=0.01920, FDG=0.01538, PBR28=0.02302
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

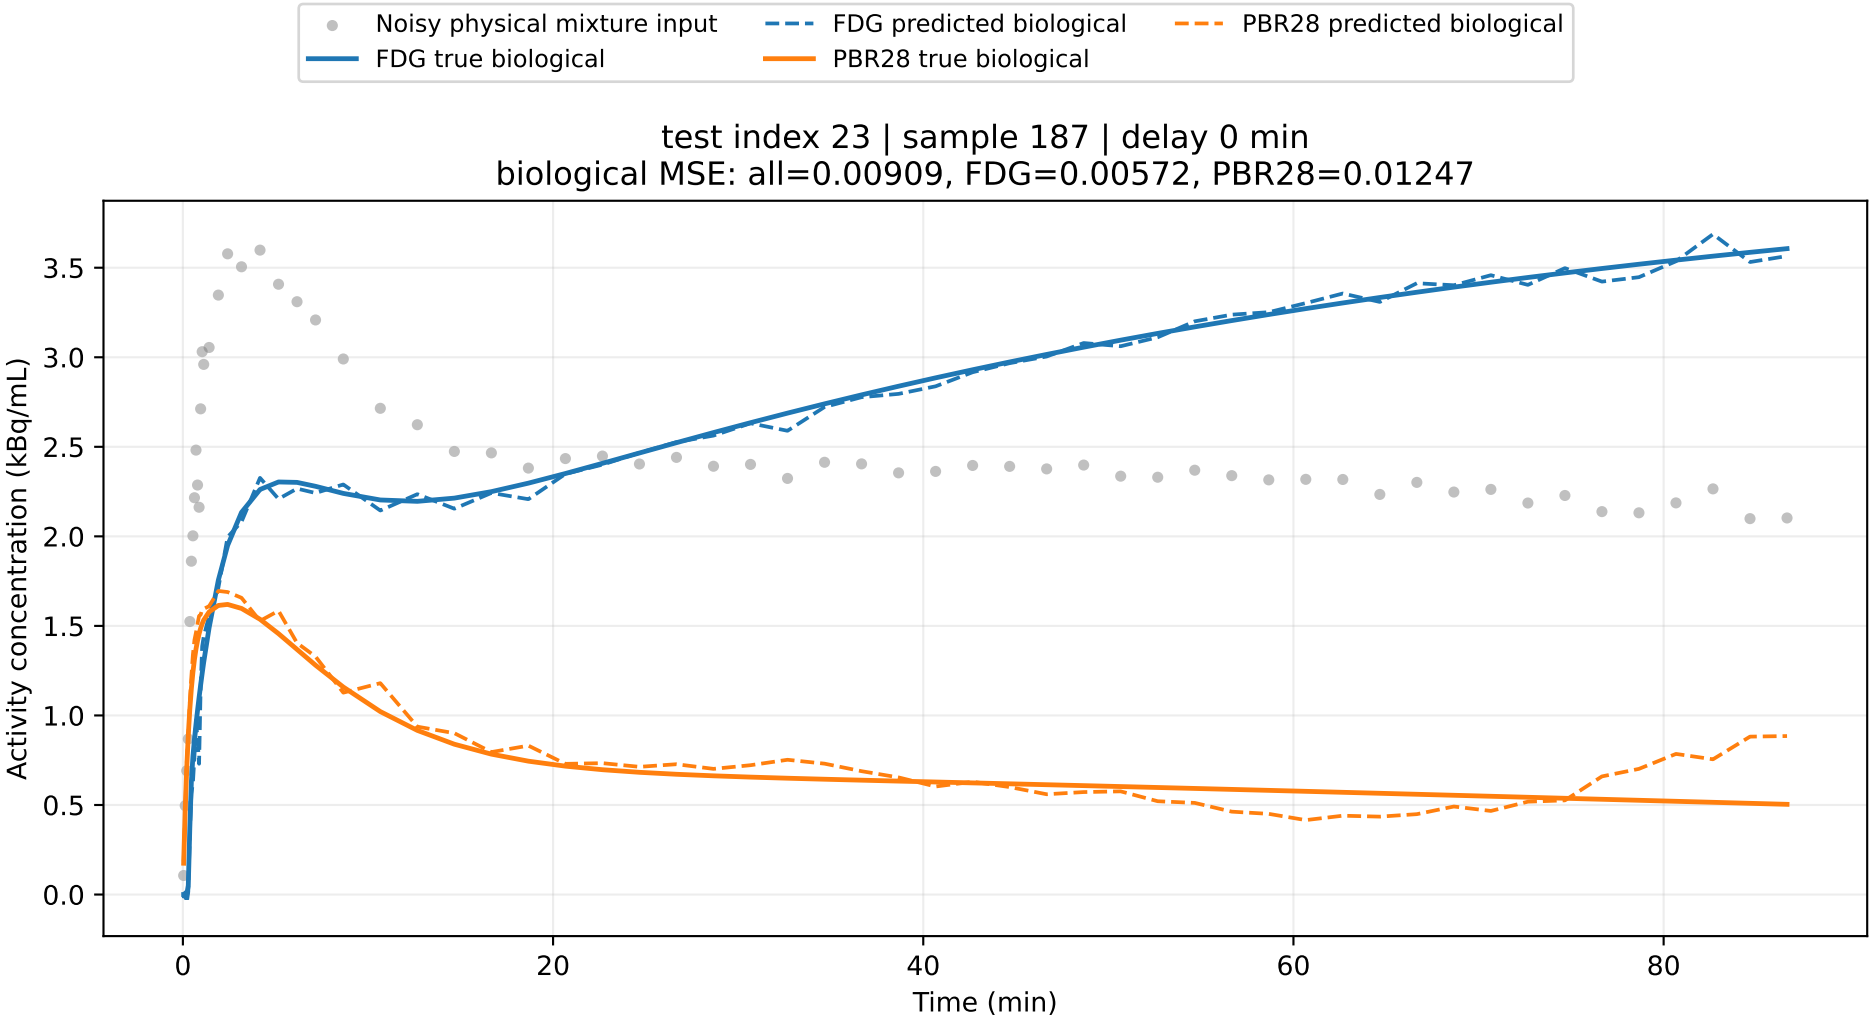

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 18 | sample 932 | delay 10 min
biological MSE: all=0.01358, FDG=0.00608, PBR28=0.02108
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

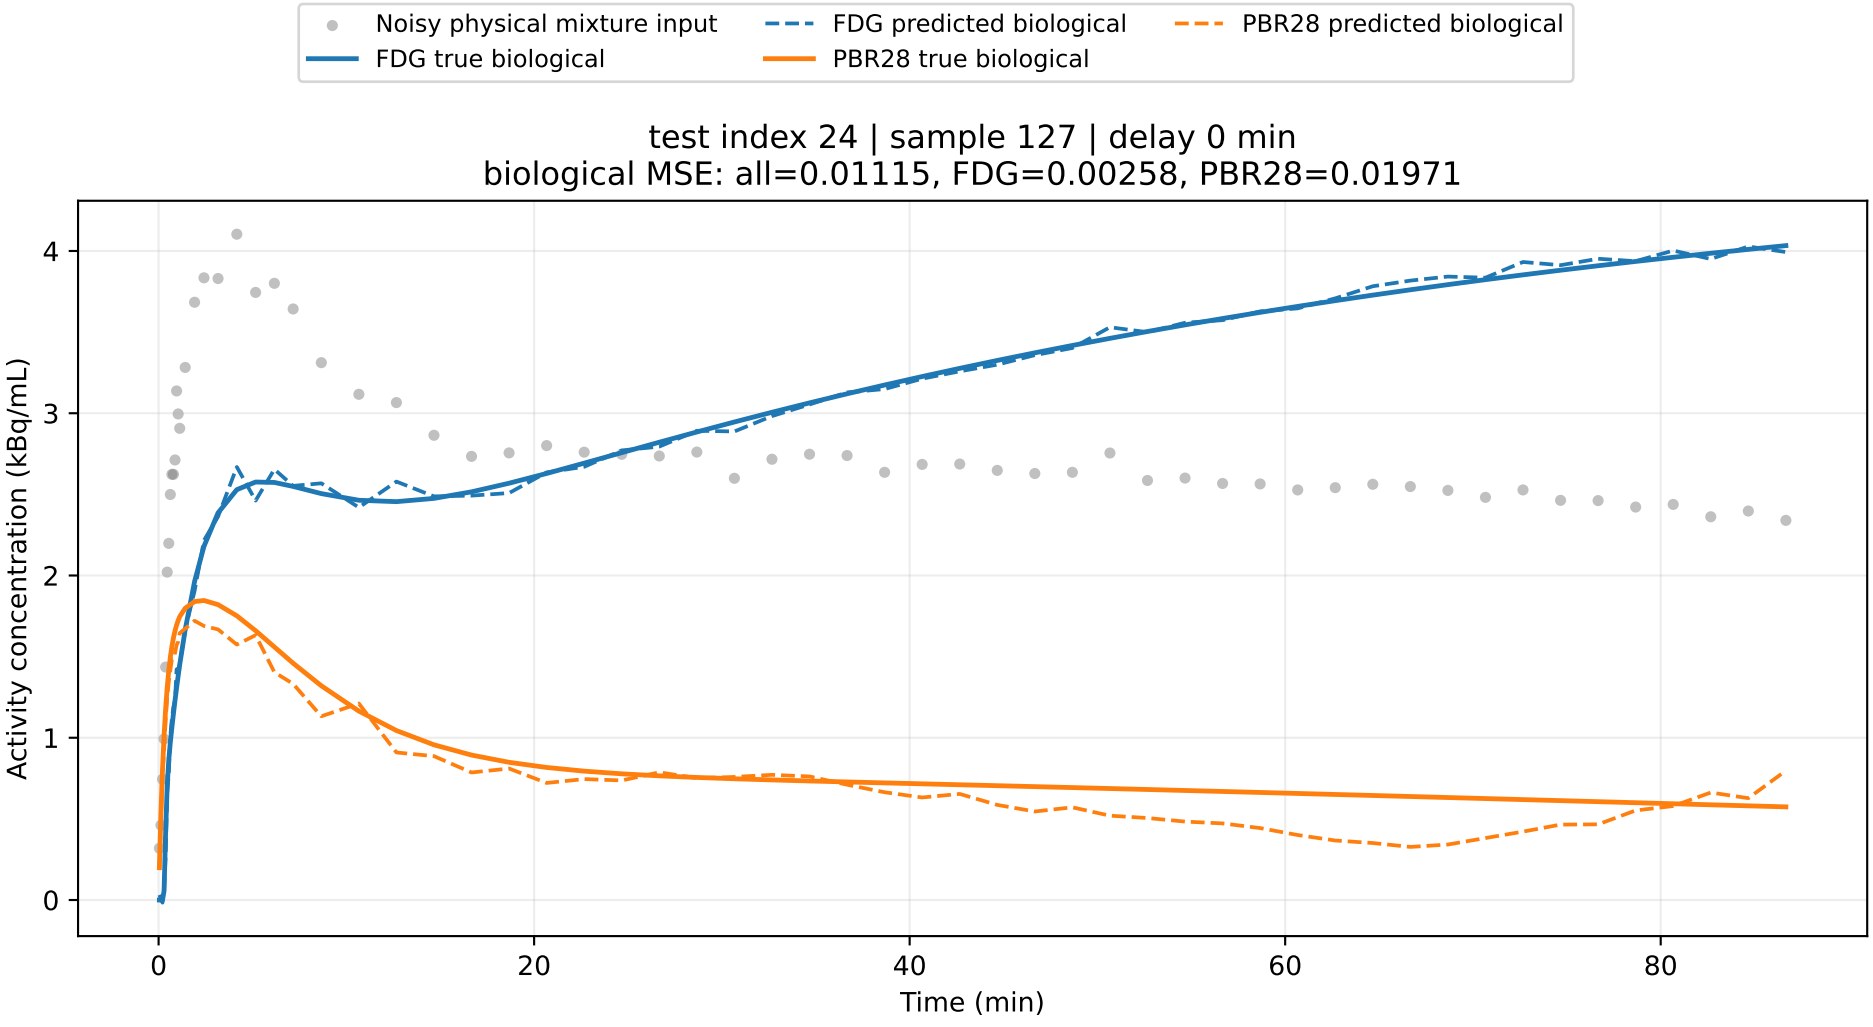

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 19 | sample 528 | delay 5 min
biological MSE: all=0.01788, FDG=0.00747, PBR28=0.02830
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

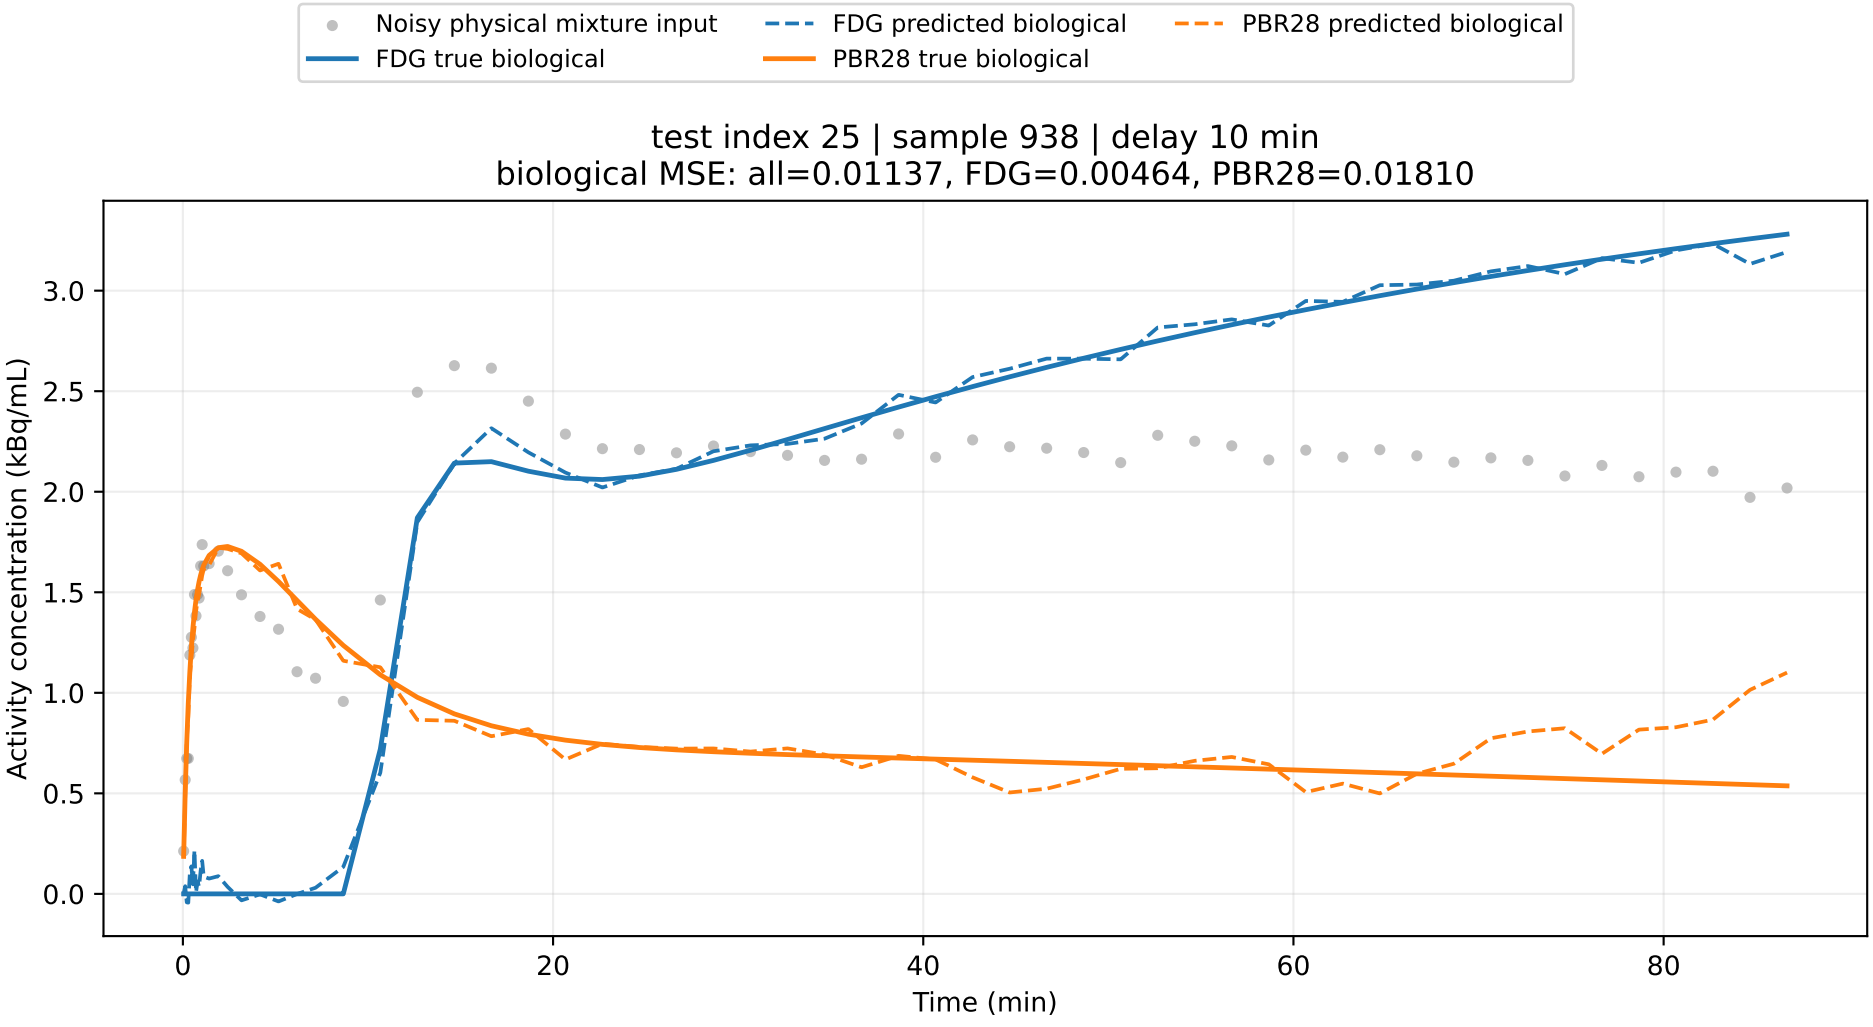

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 20 | sample 600 | delay 10 min
biological MSE: all=0.00541, FDG=0.00476, PBR28=0.00607
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

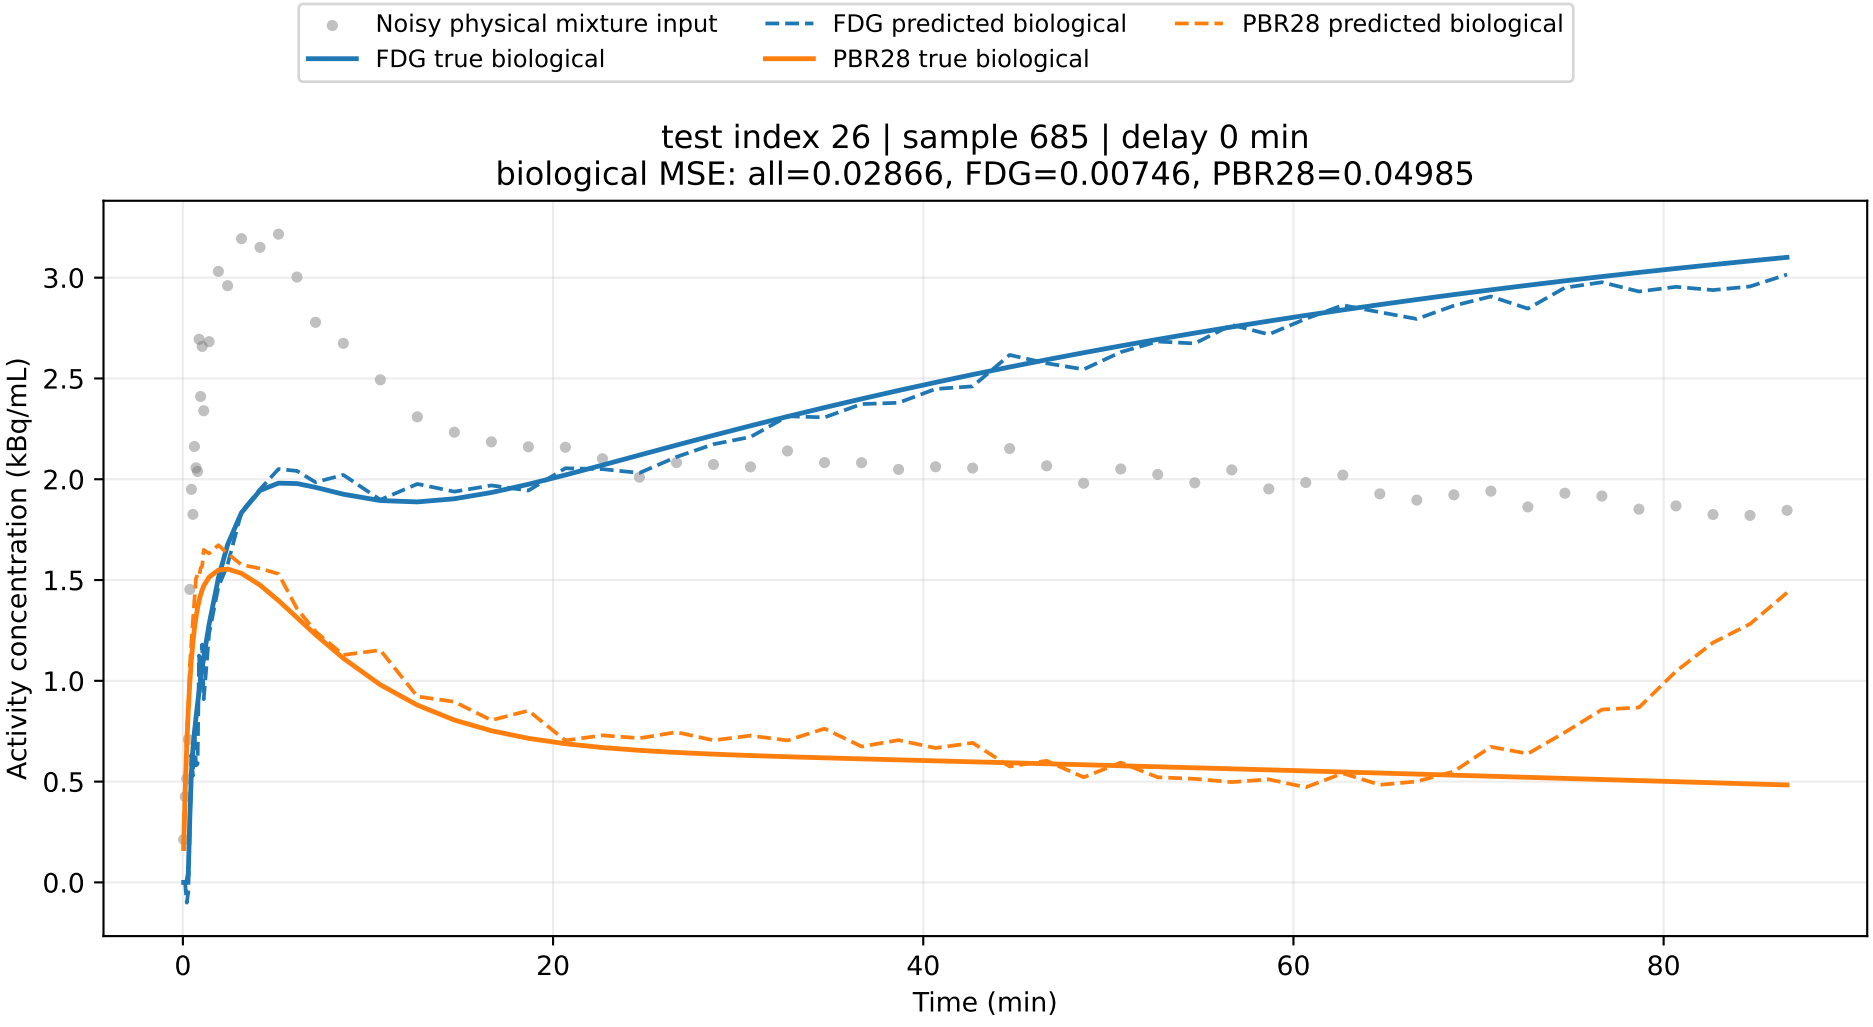

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 21 | sample 54 | delay 10 min
biological MSE: all=0.01141, FDG=0.00523, PBR28=0.01760
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

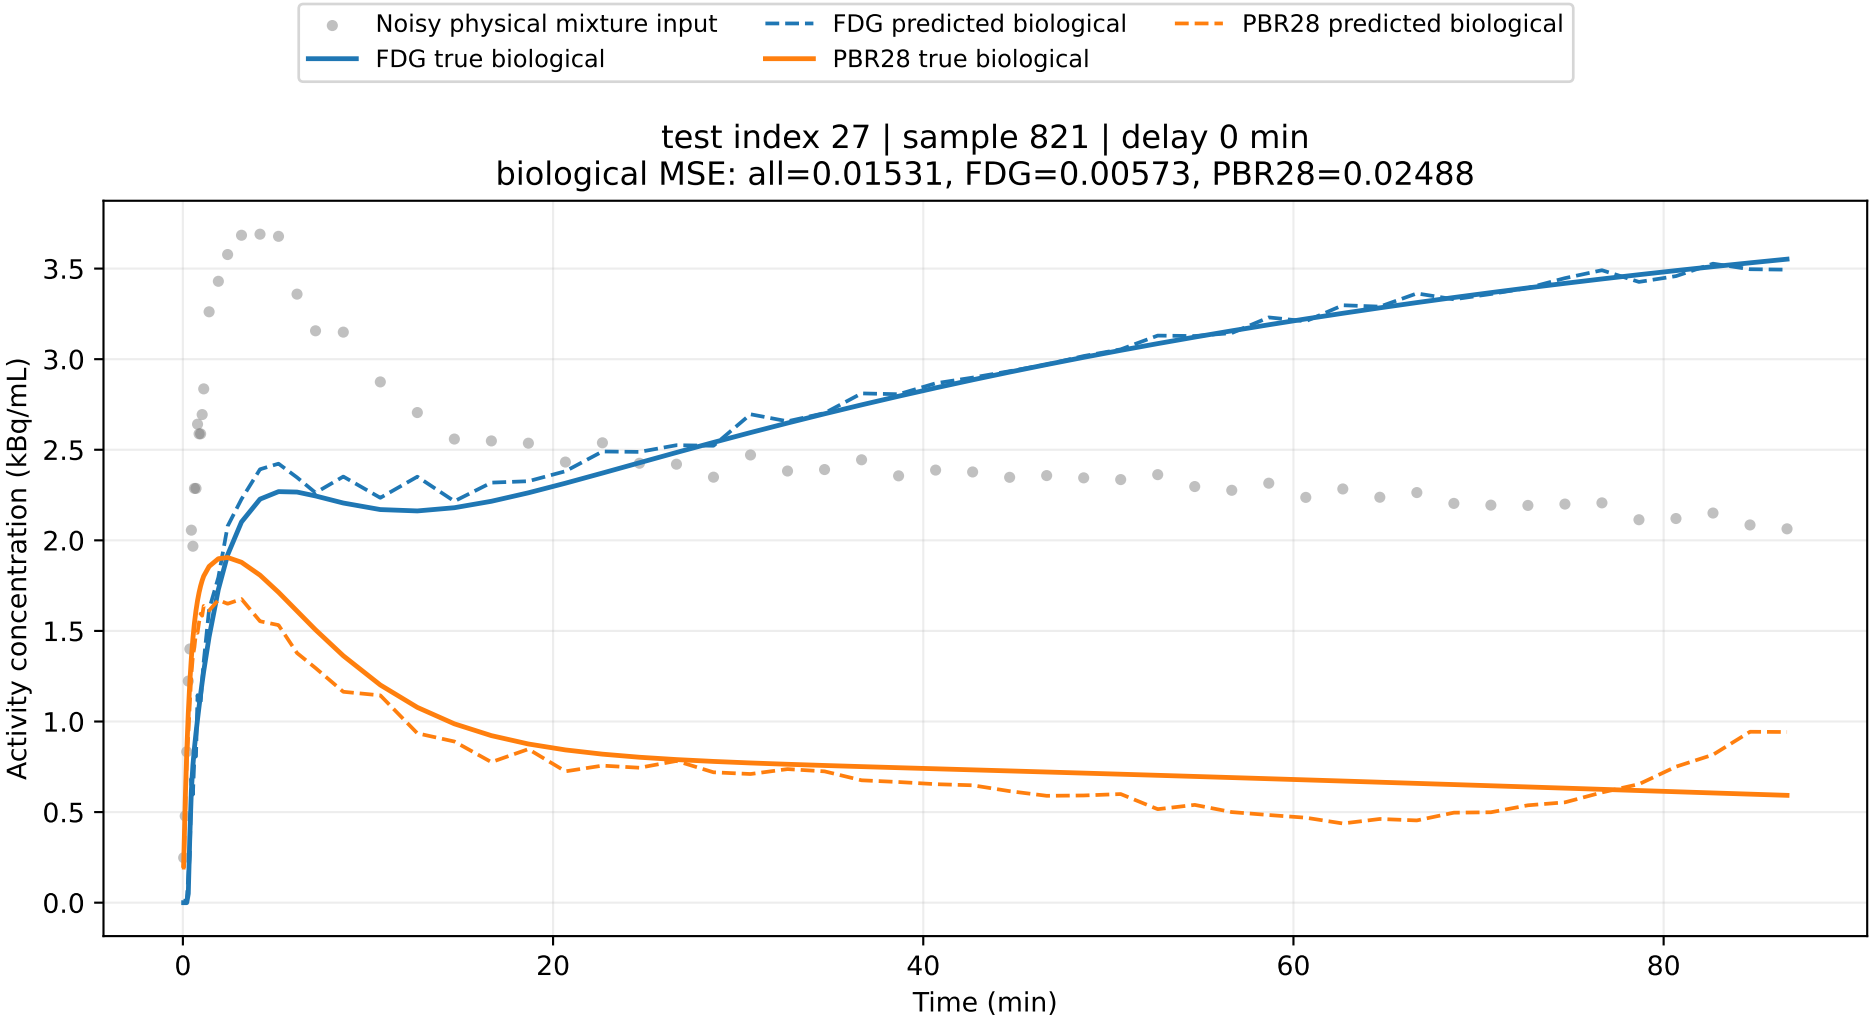

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 22 | sample 487 | delay 5 min
biological MSE: all=0.01557, FDG=0.00631, PBR28=0.02483
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

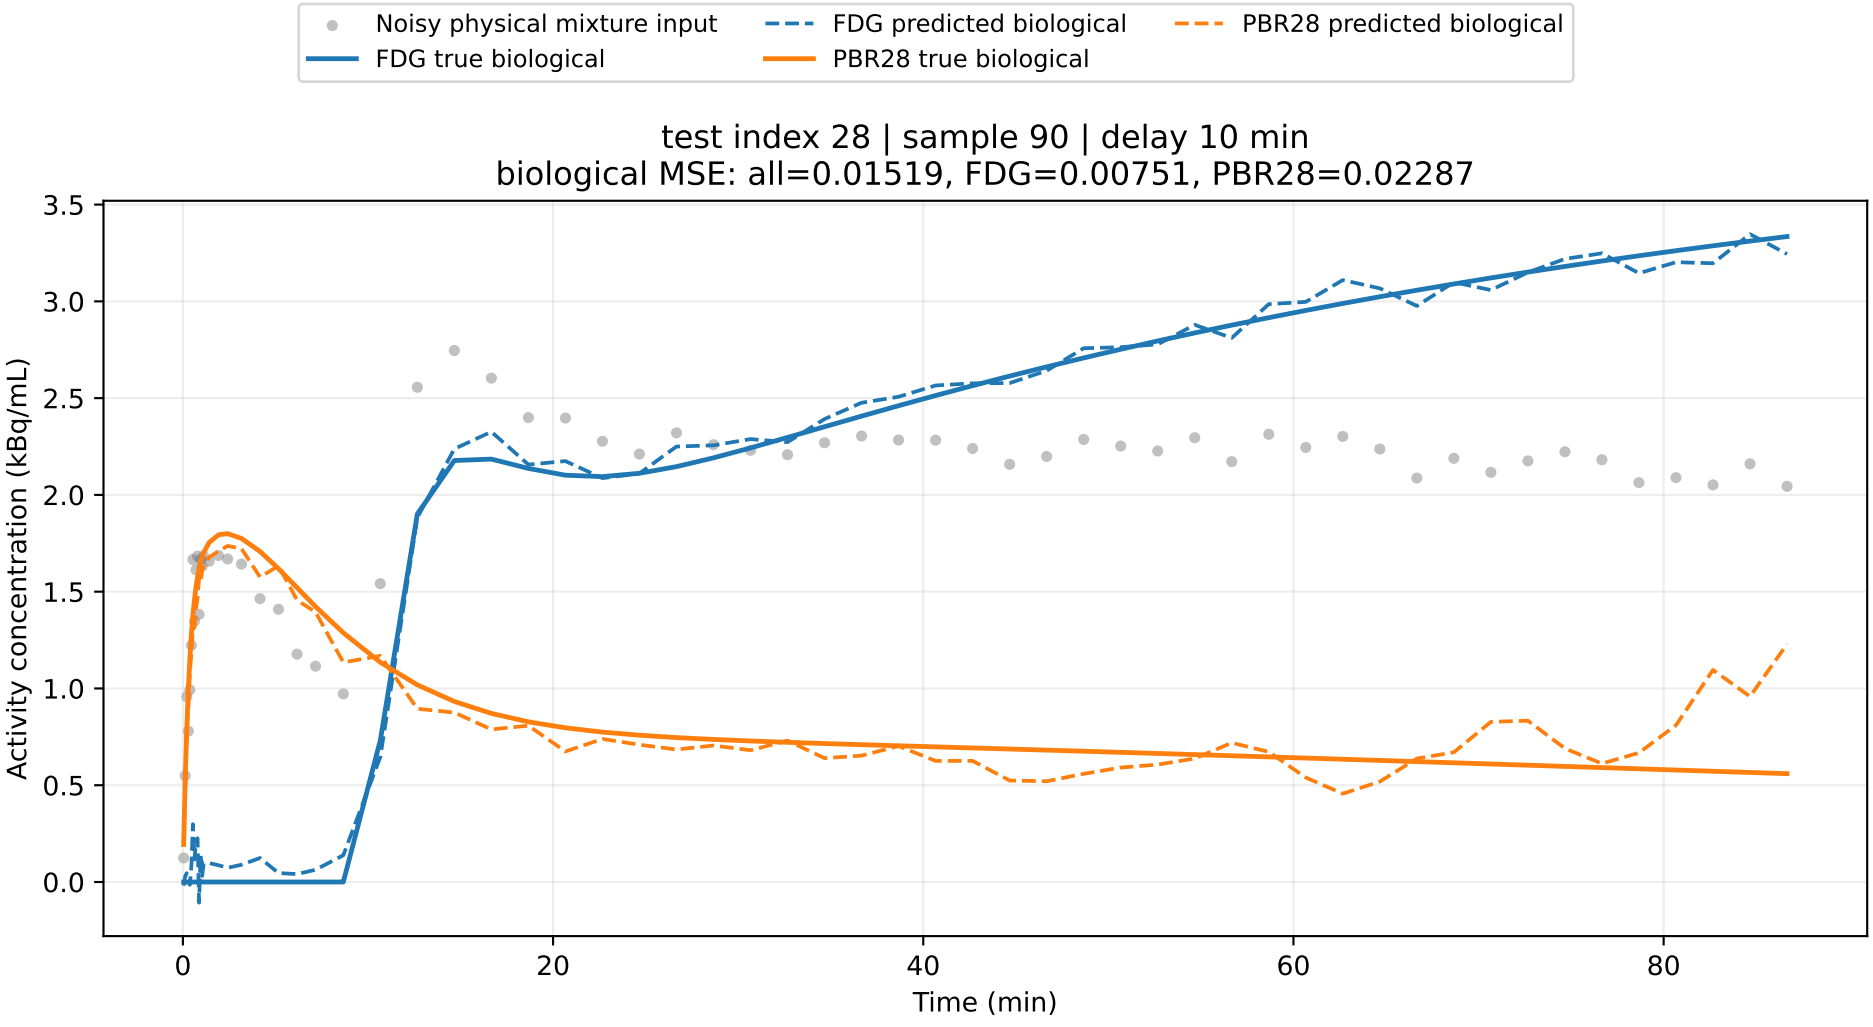

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 23 | sample 187 | delay 0 min
biological MSE: all=0.00909, FDG=0.00572, PBR28=0.01247
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

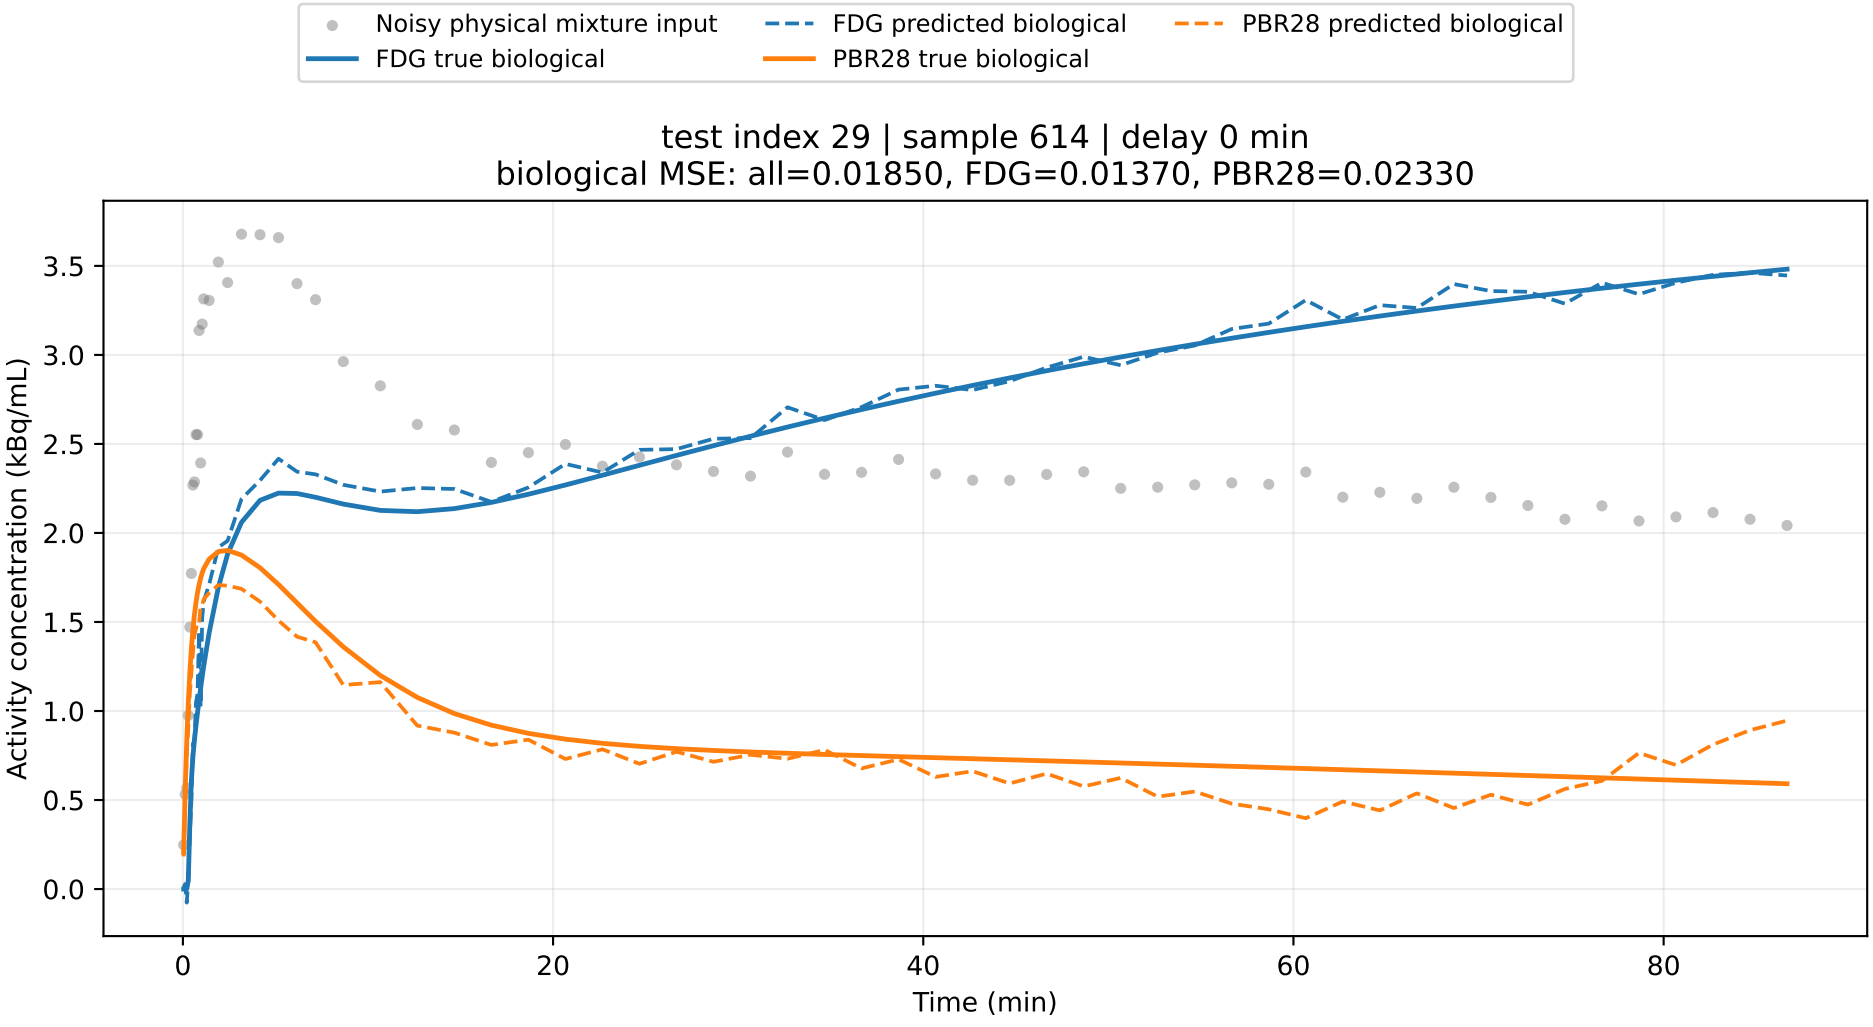

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 24 | sample 127 | delay 0 min
biological MSE: all=0.01115, FDG=0.00258, PBR28=0.01971
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

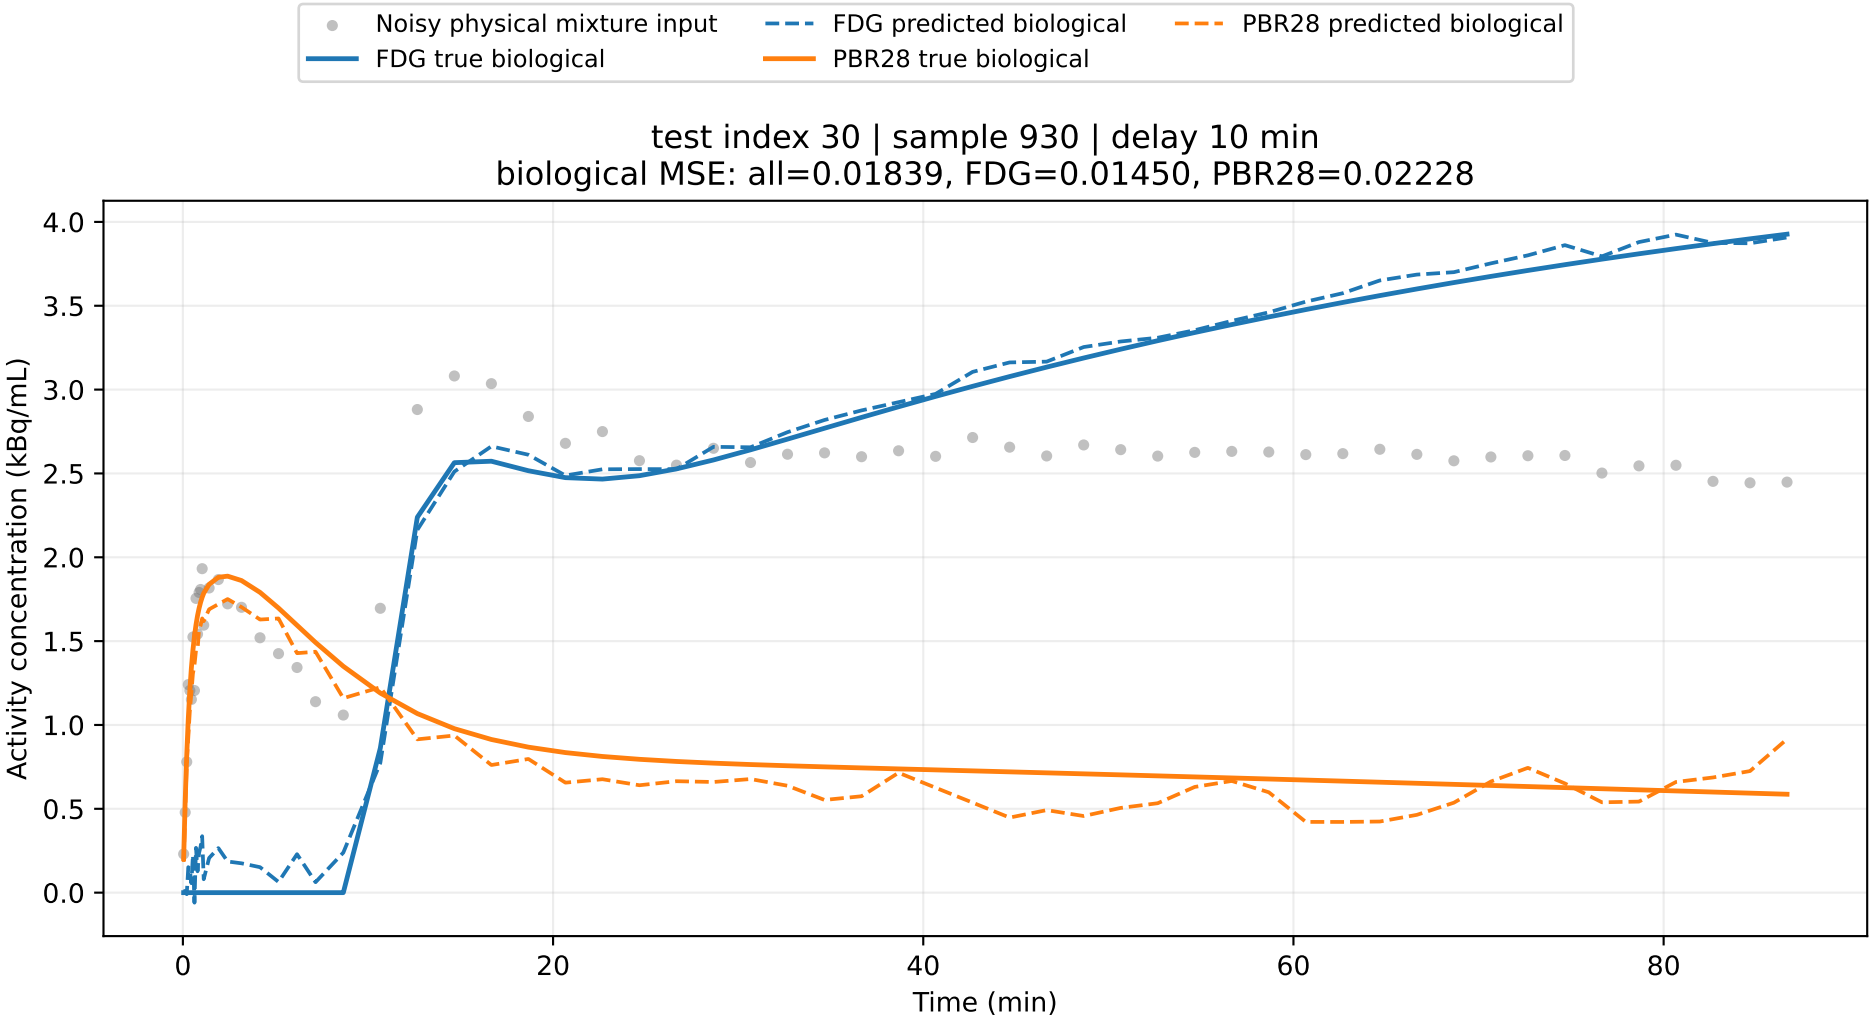

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 25 | sample 938 | delay 10 min
biological MSE: all=0.01137, FDG=0.00464, PBR28=0.01810
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

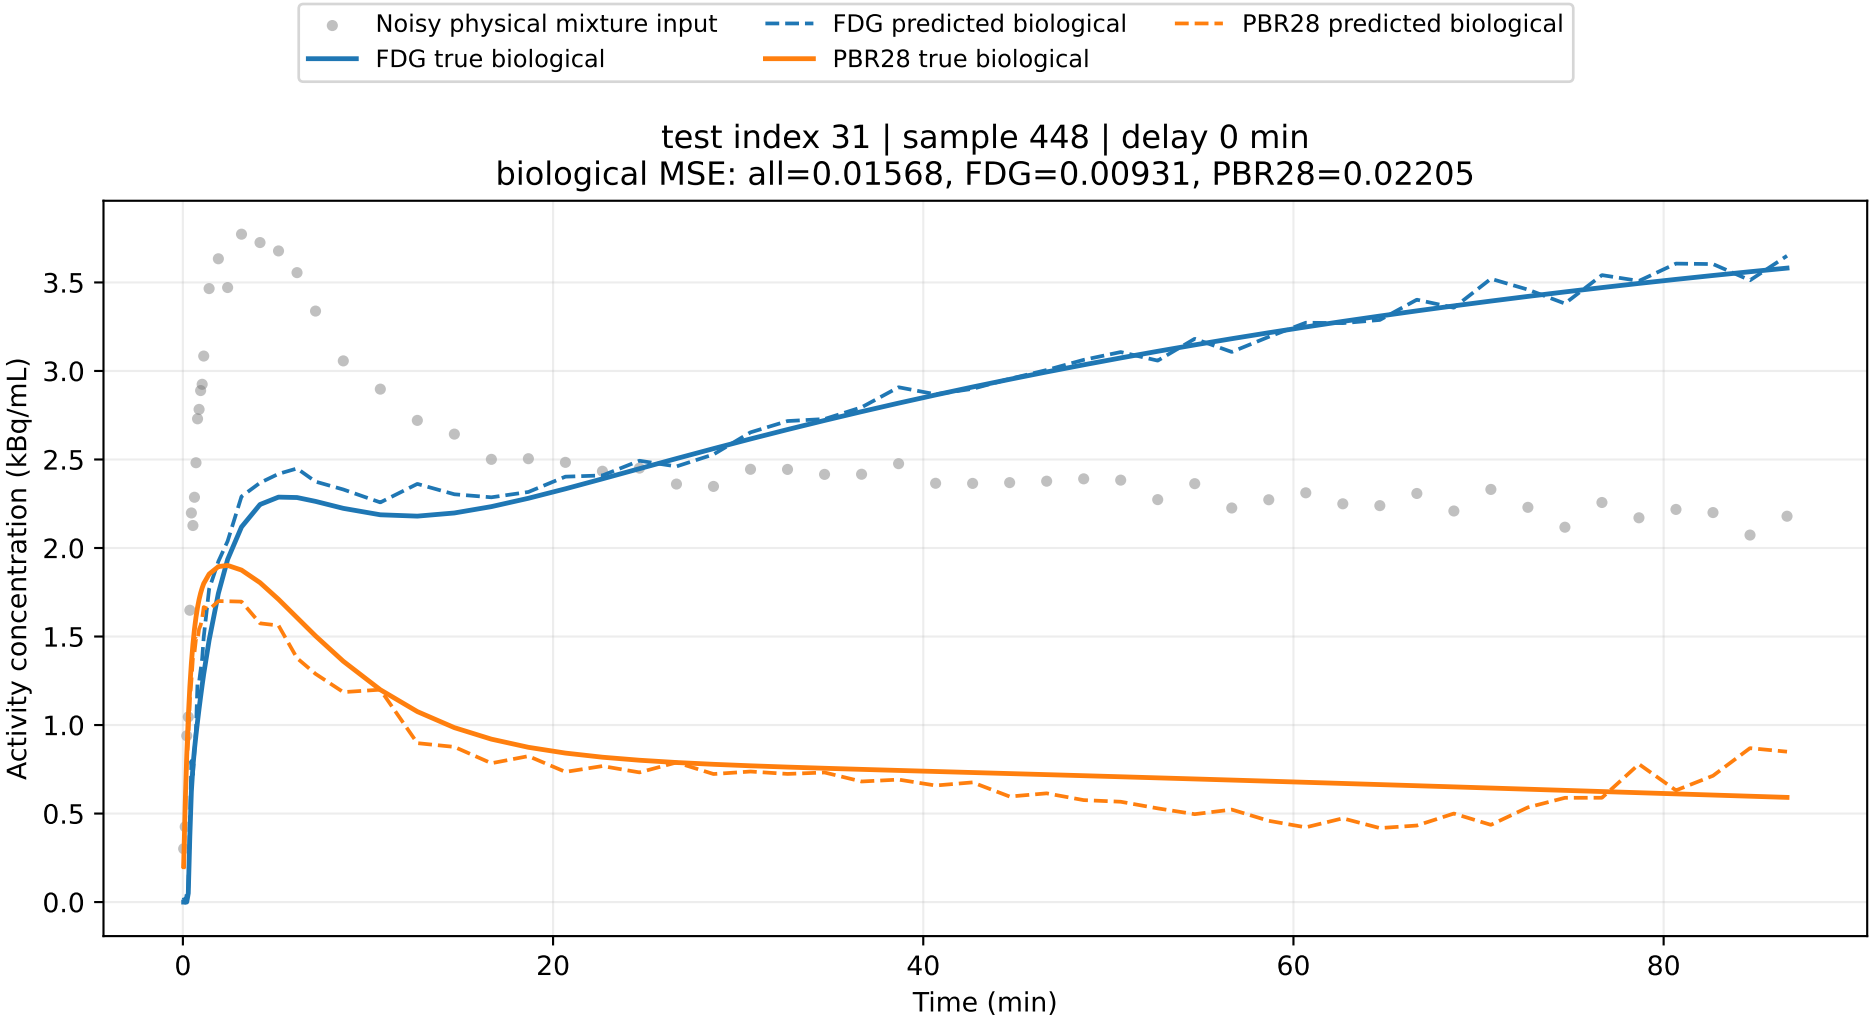

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 26 | sample 685 | delay 0 min
biological MSE: all=0.02866, FDG=0.00746, PBR28=0.04985
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

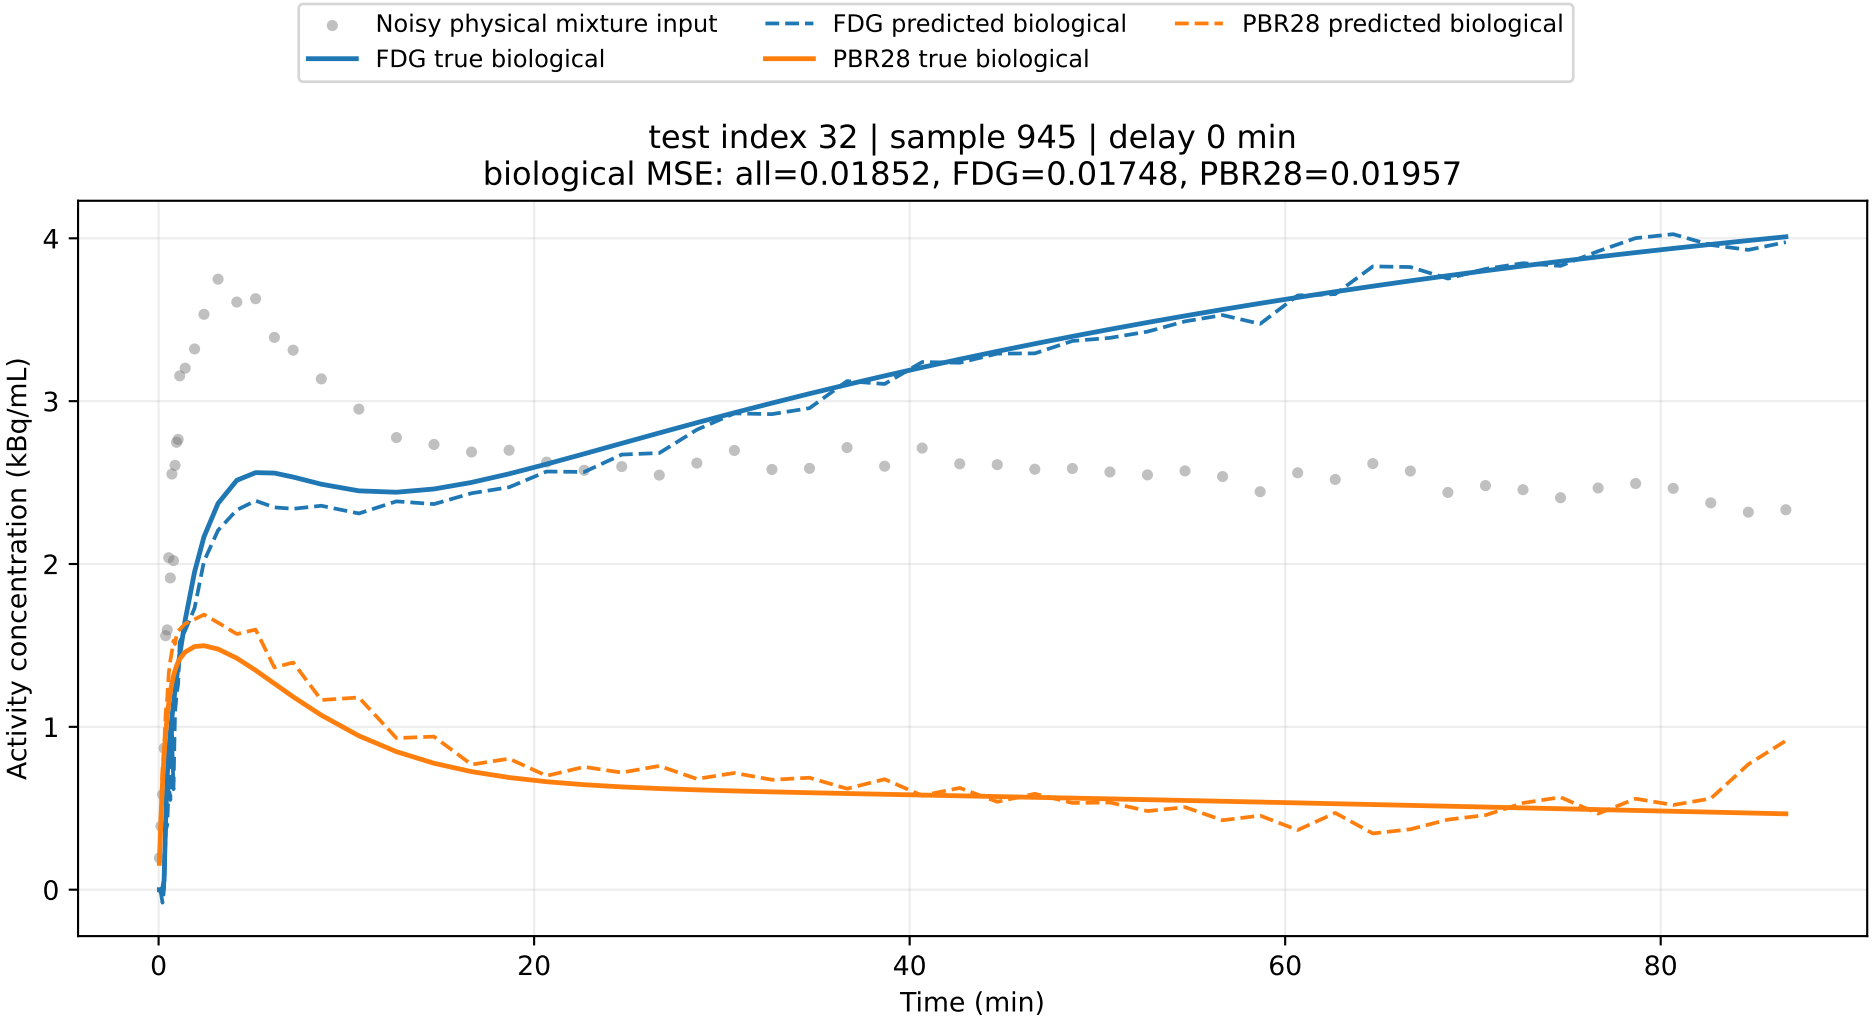

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 27 | sample 821 | delay 0 min
biological MSE: all=0.01531, FDG=0.00573, PBR28=0.02488
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

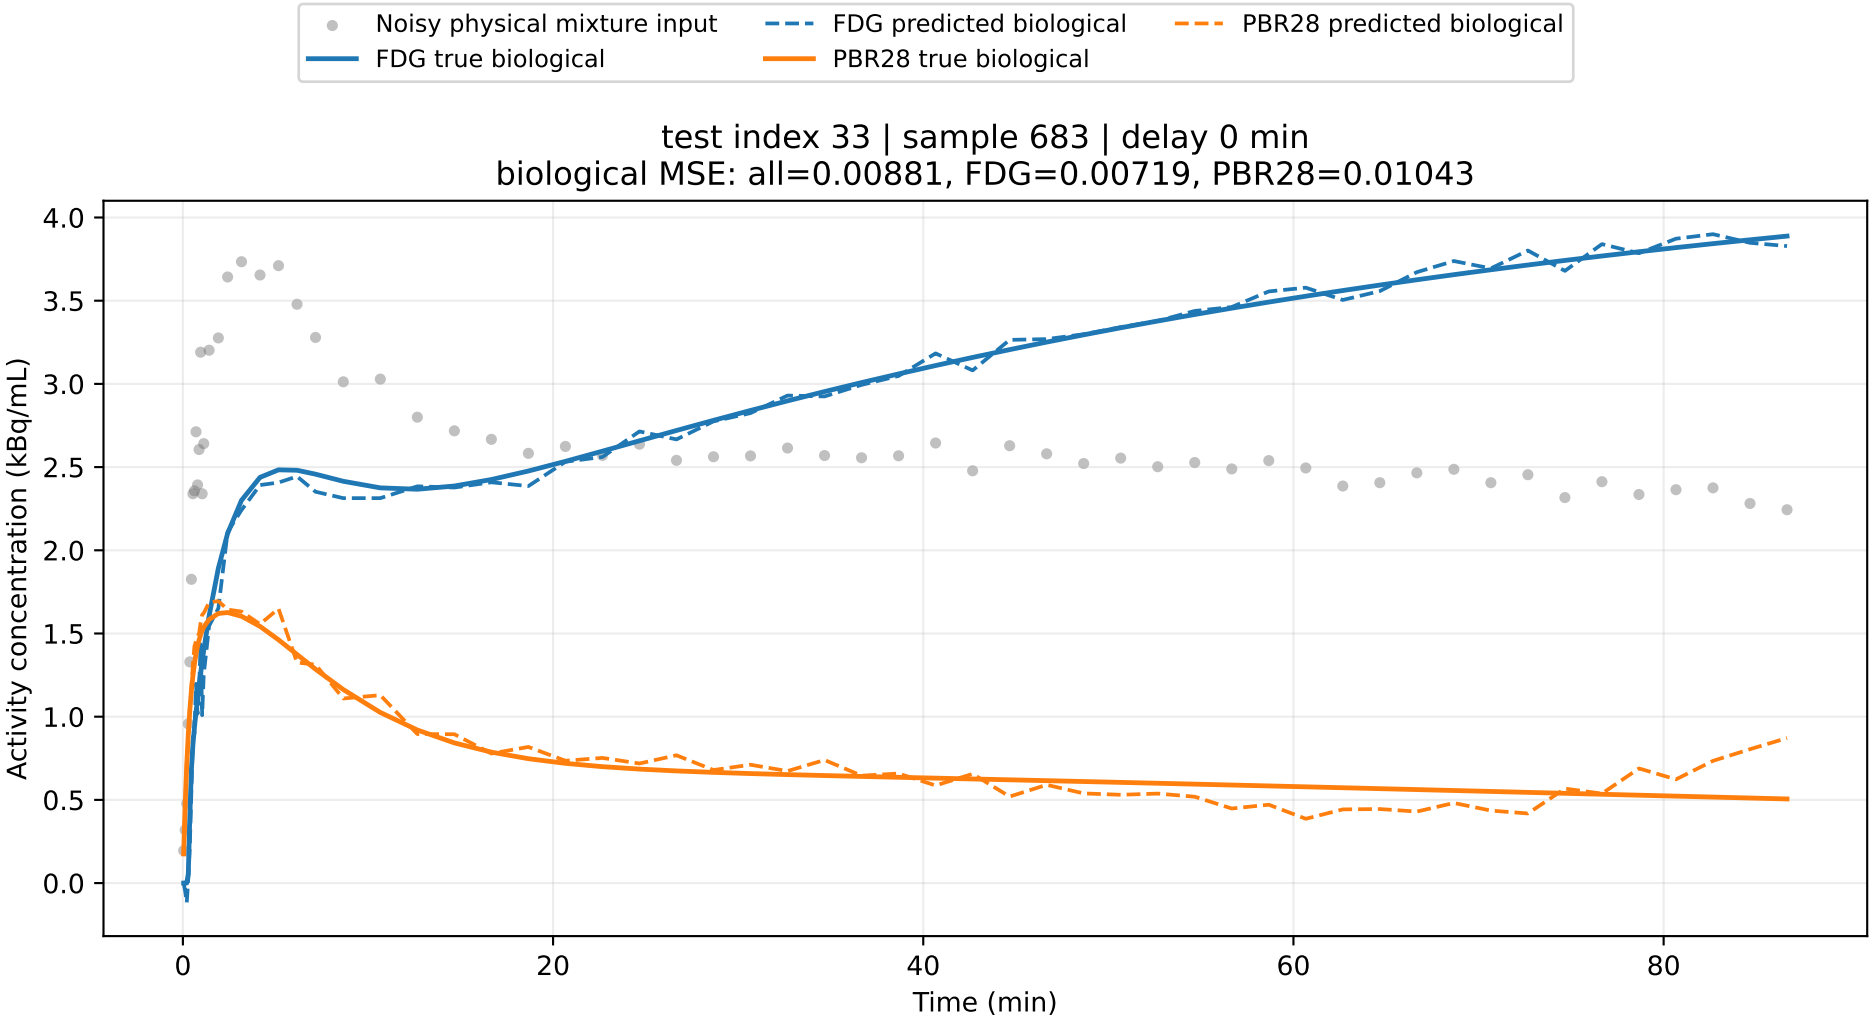

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 28 | sample 90 | delay 10 min
biological MSE: all=0.01519, FDG=0.00751, PBR28=0.02287
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

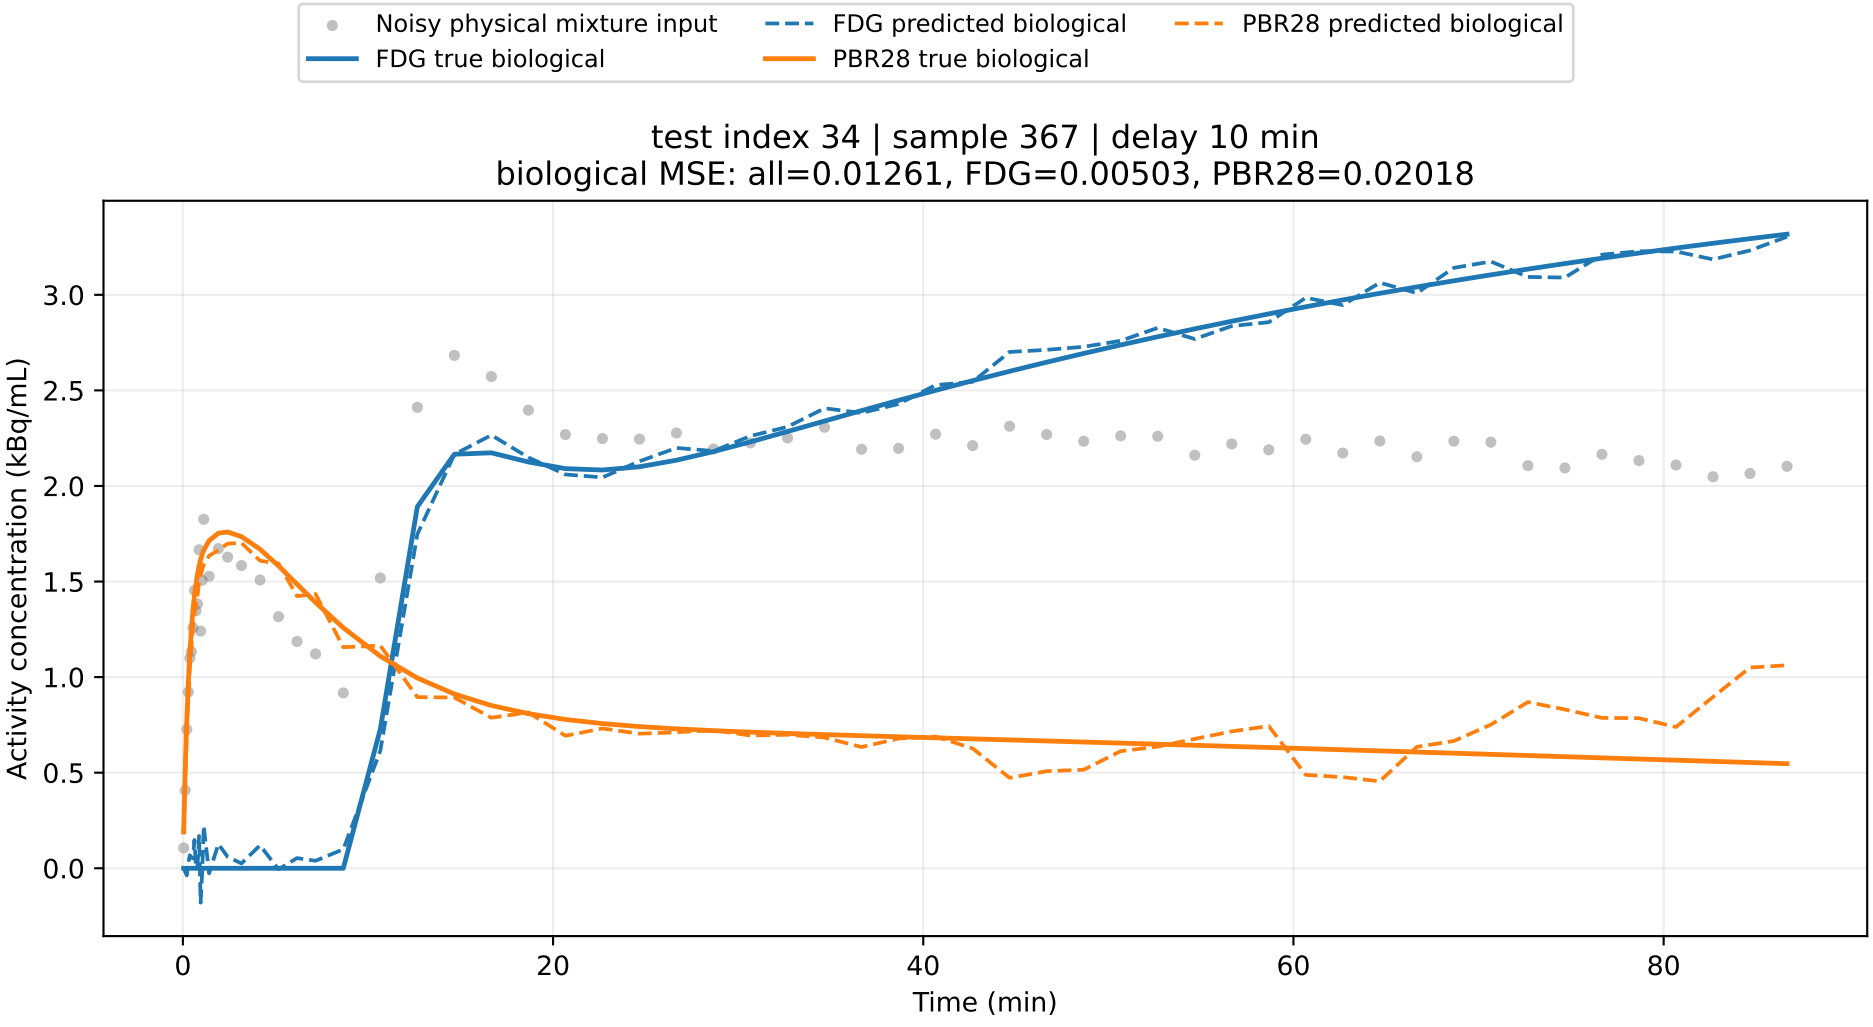

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 29 | sample 614 | delay 0 min
biological MSE: all=0.01850, FDG=0.01370, PBR28=0.02330
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

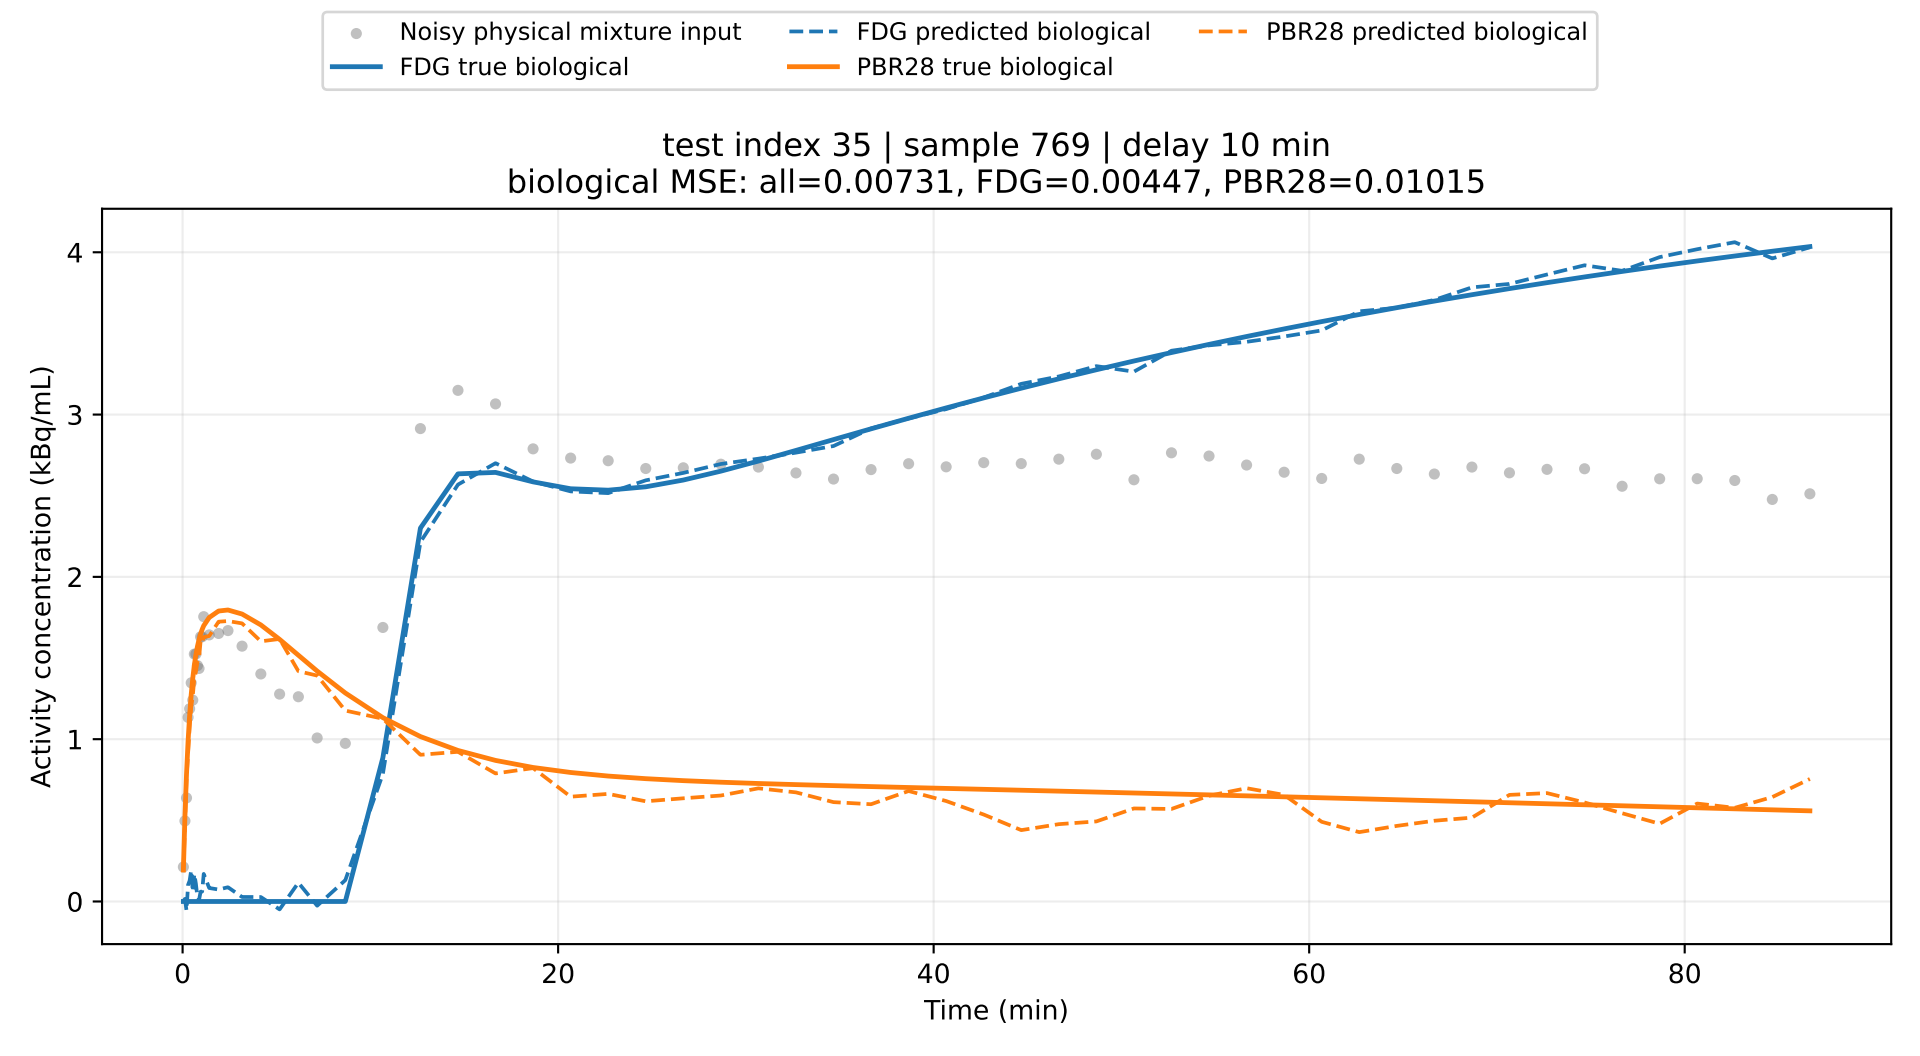

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 30 | sample 930 | delay 10 min
biological MSE: all=0.01839, FDG=0.01450, PBR28=0.02228
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

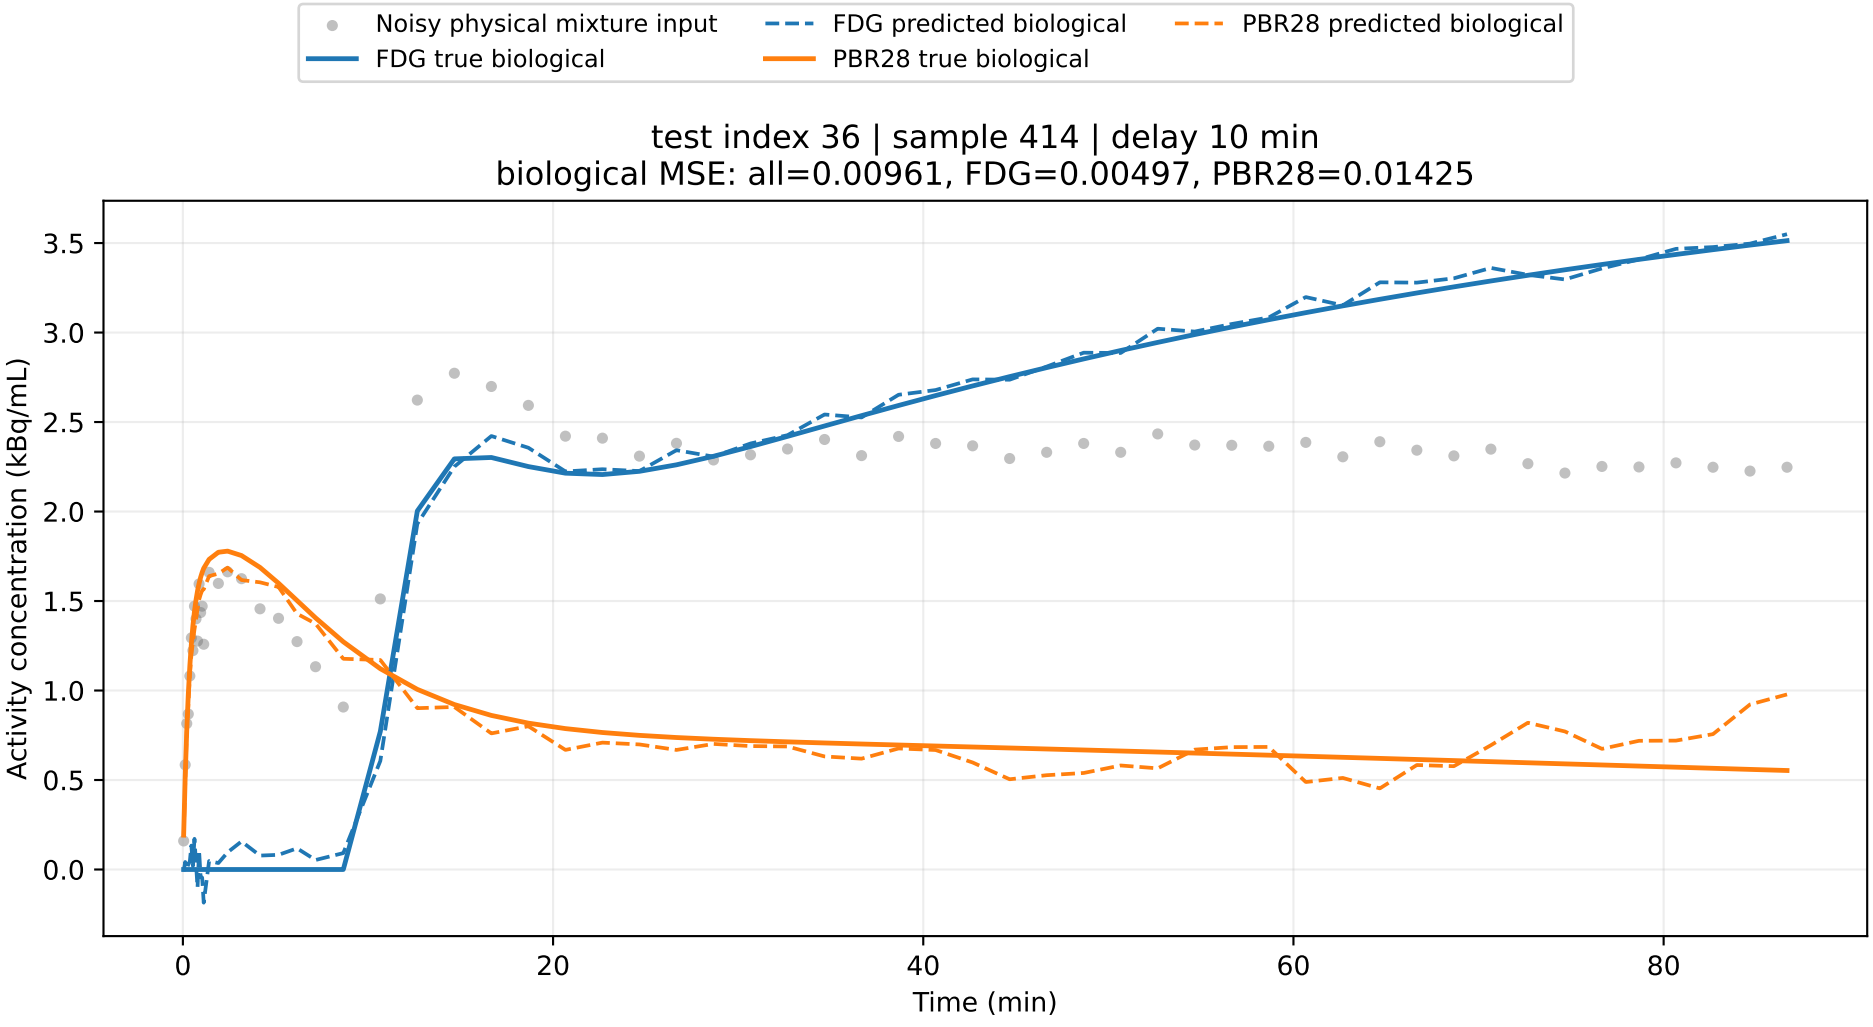

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 31 | sample 448 | delay 0 min
biological MSE: all=0.01568, FDG=0.00931, PBR28=0.02205
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

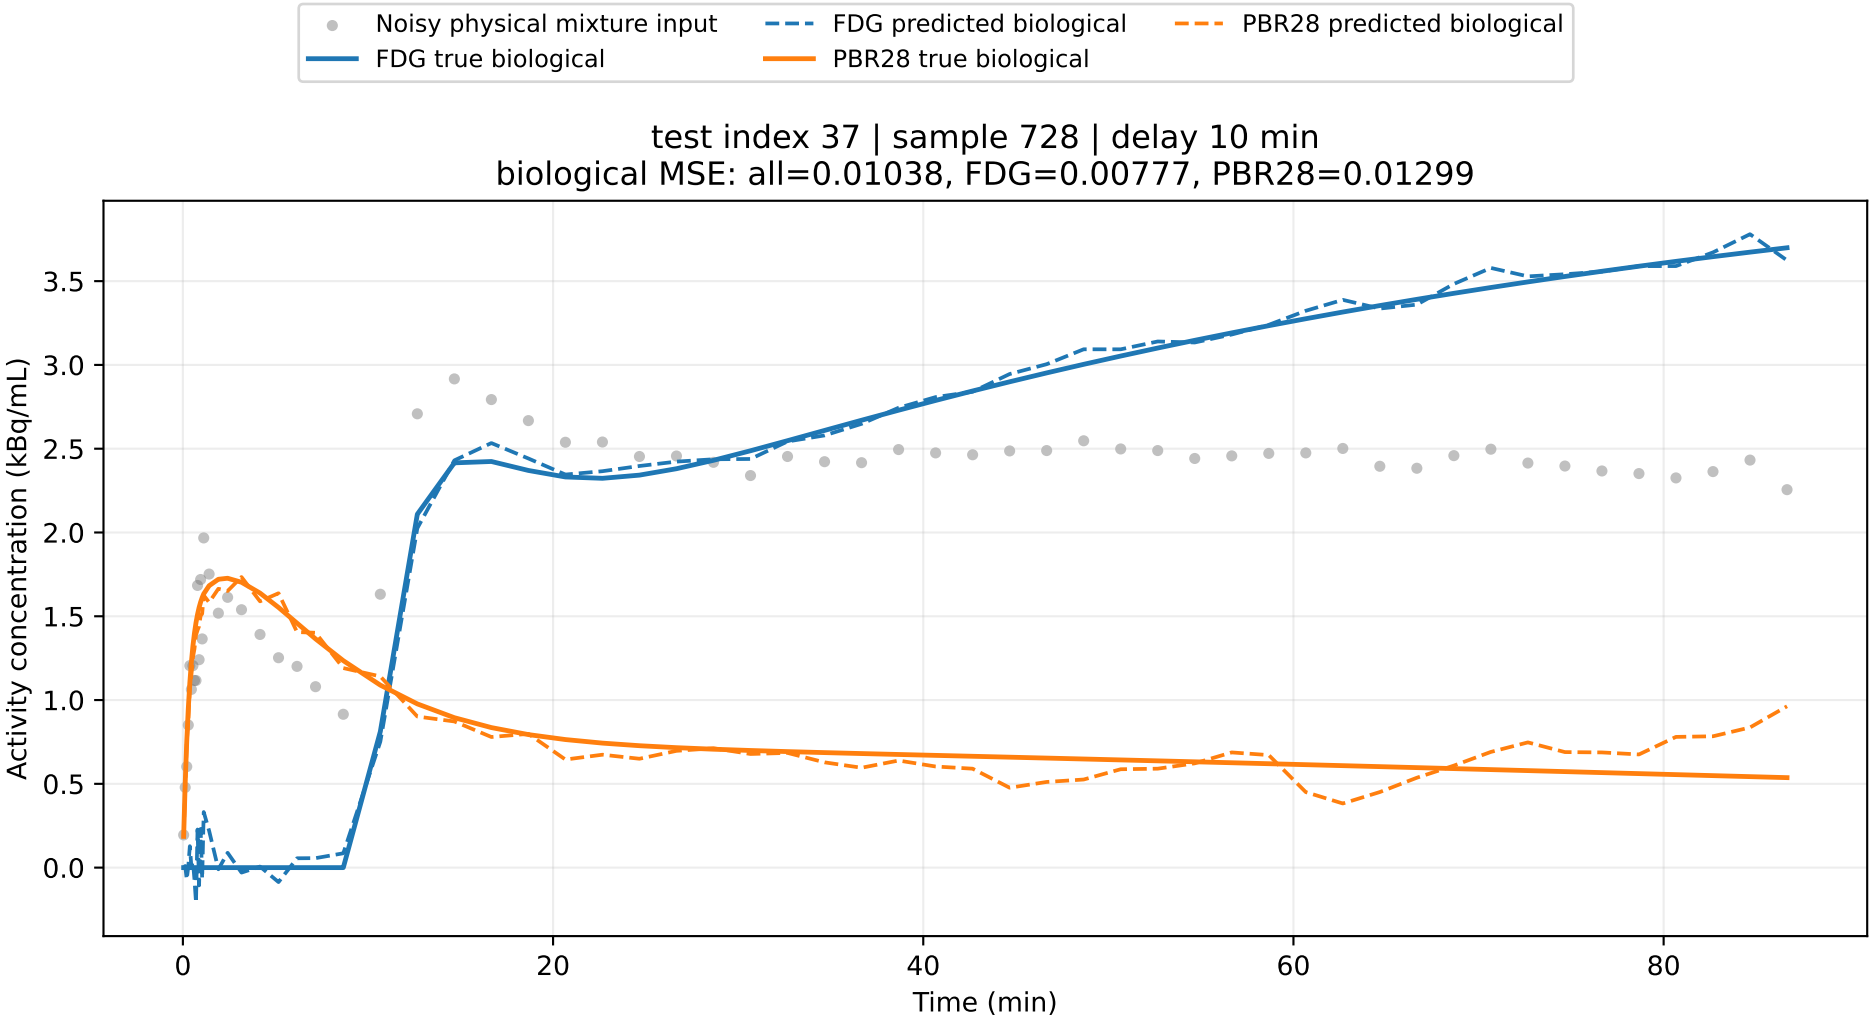

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 32 | sample 945 | delay 0 min
biological MSE: all=0.01852, FDG=0.01748, PBR28=0.01957
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

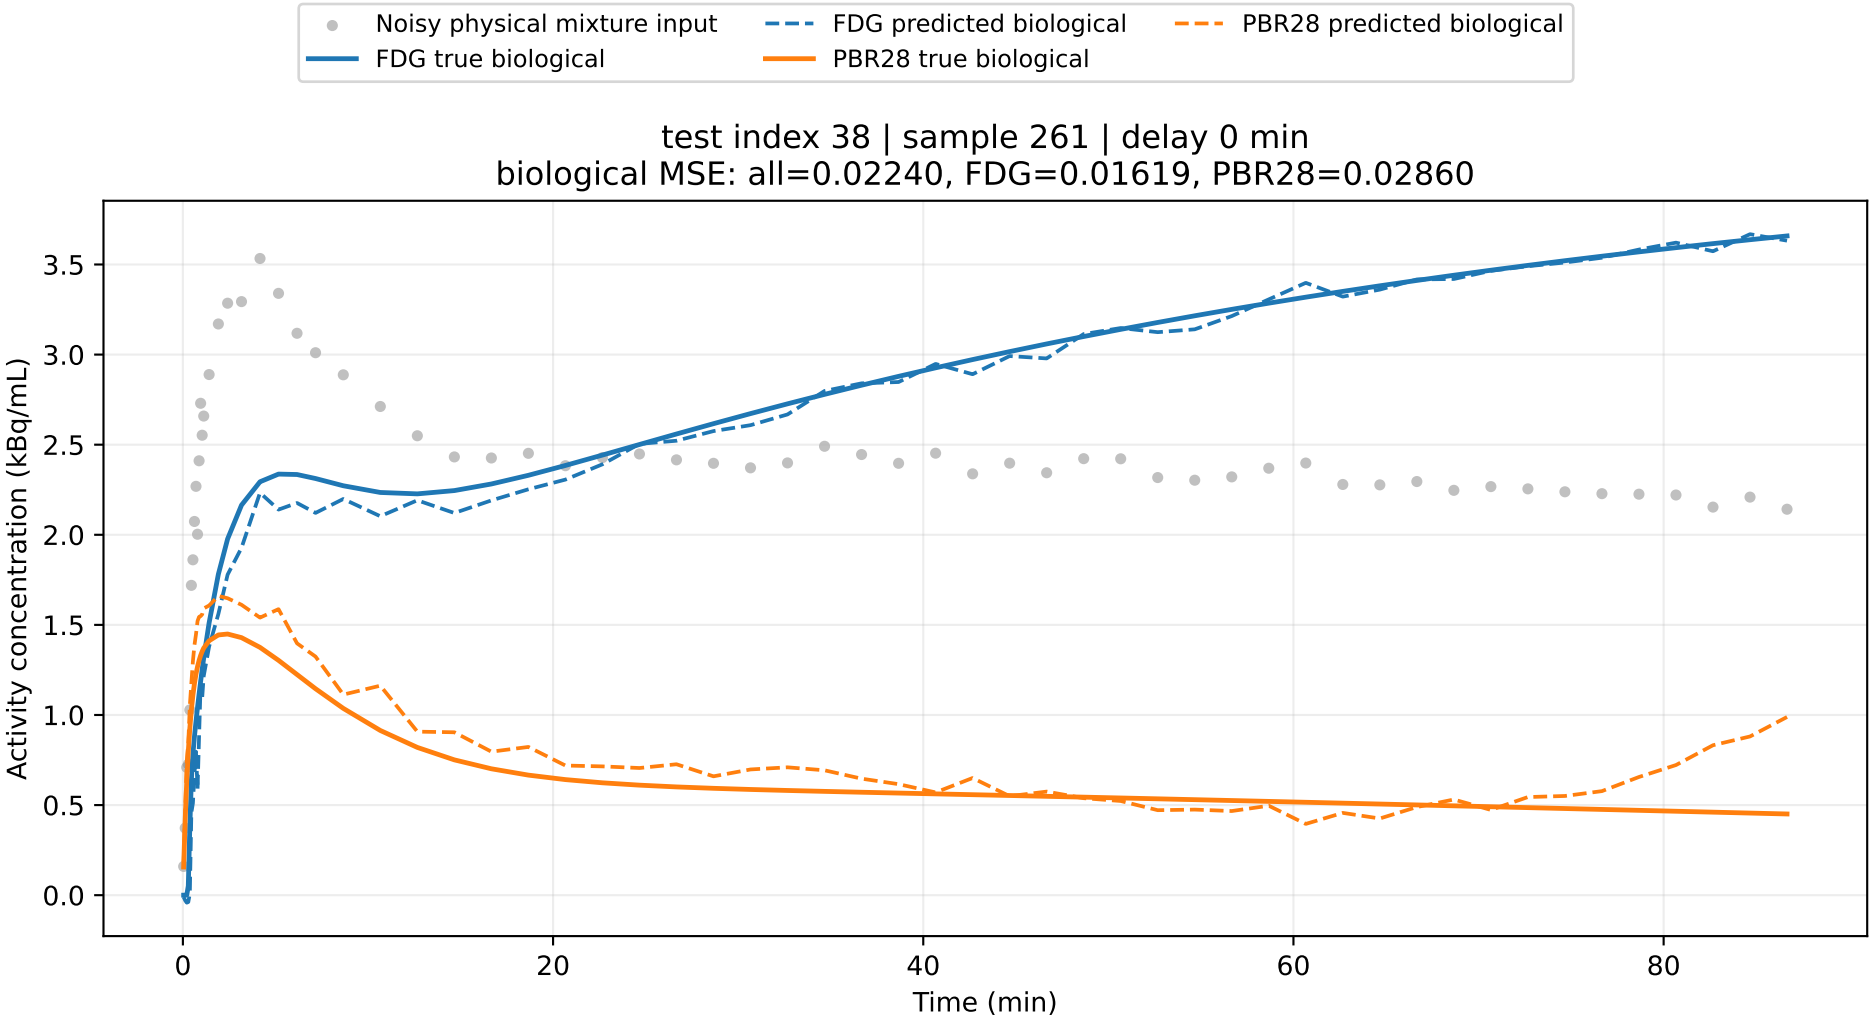

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 33 | sample 683 | delay 0 min
biological MSE: all=0.00881, FDG=0.00719, PBR28=0.01043
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

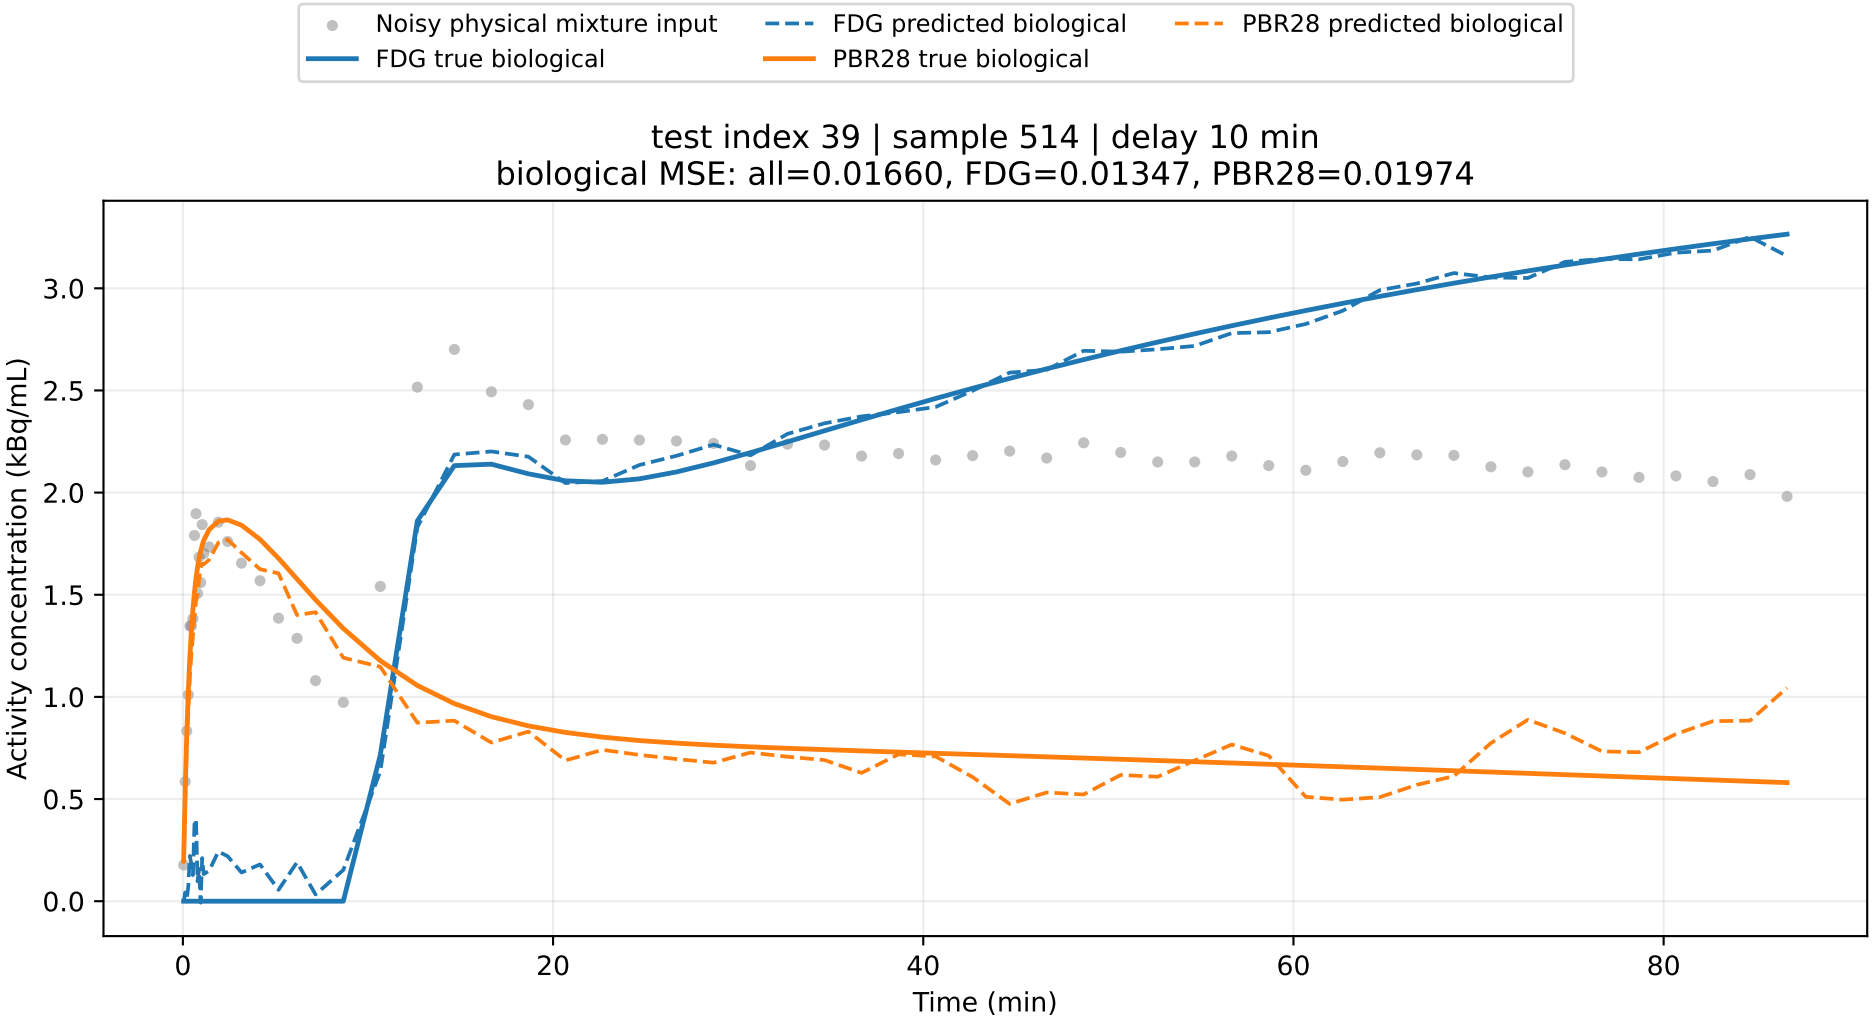

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 34 | sample 367 | delay 10 min
biological MSE: all=0.01261, FDG=0.00503, PBR28=0.02018
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

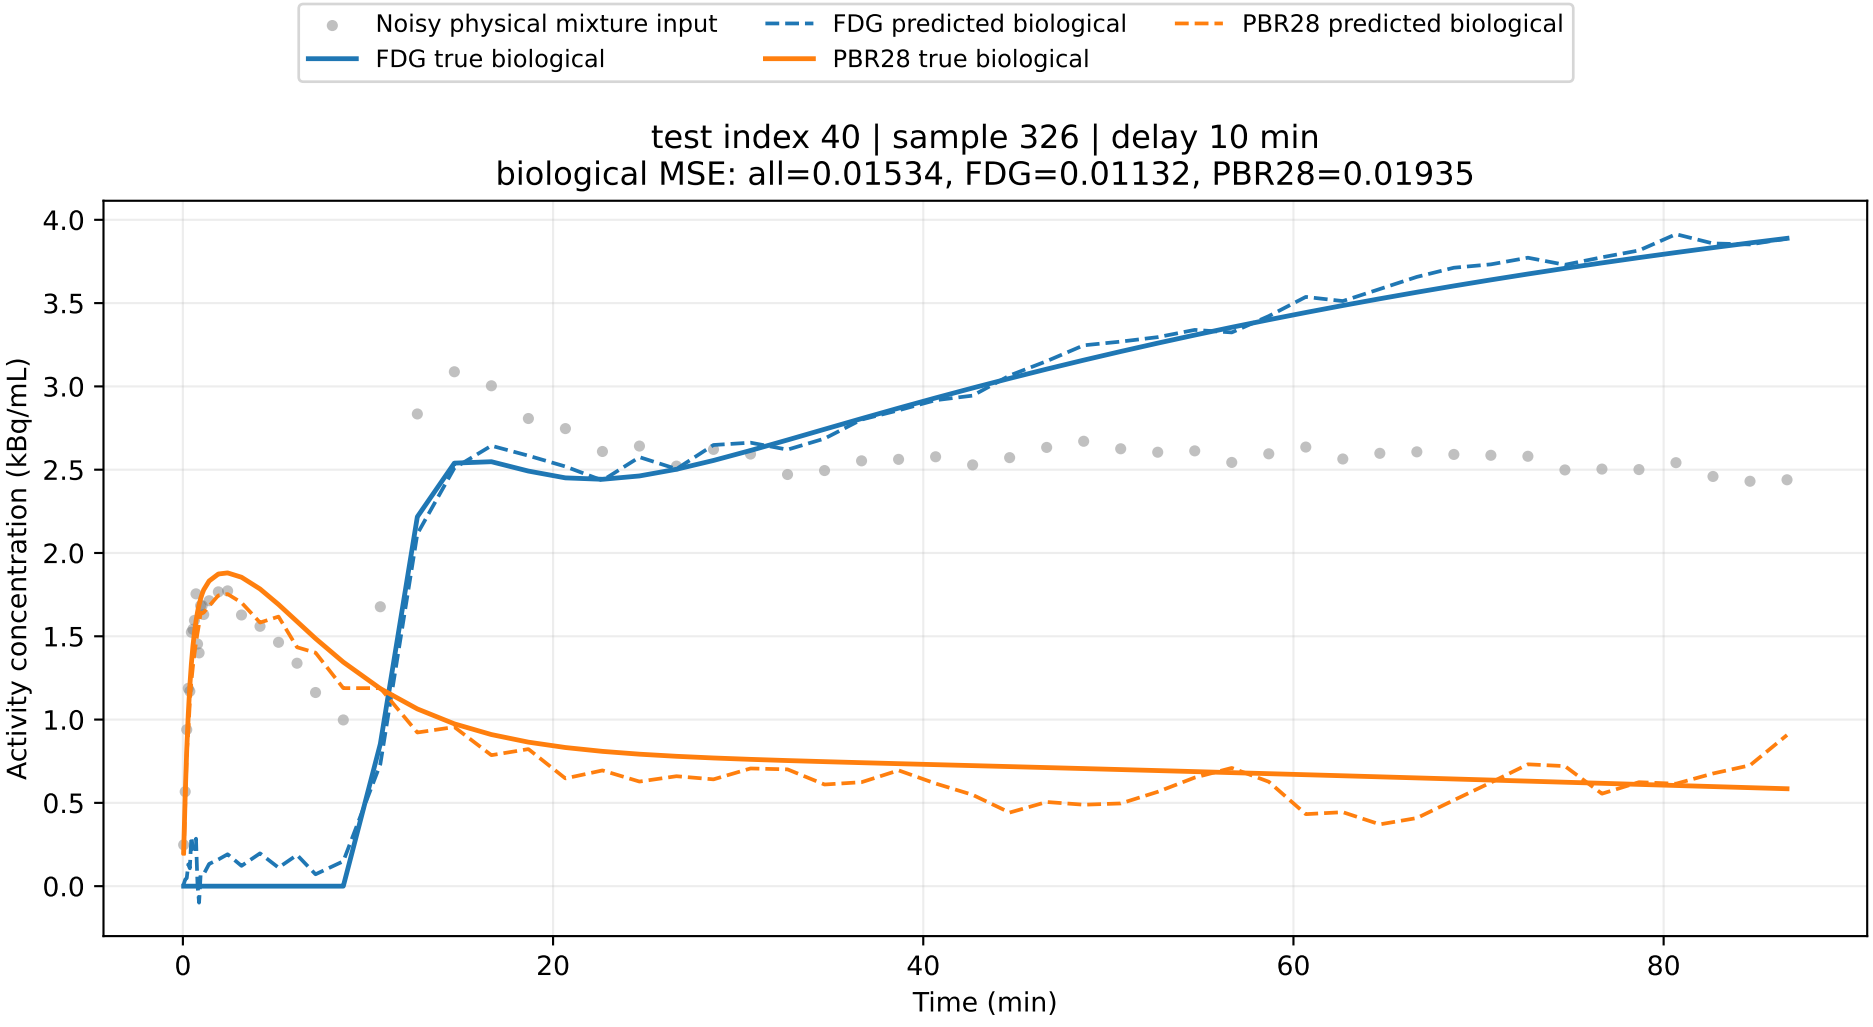

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 35 | sample 769 | delay 10 min
biological MSE: all=0.00731, FDG=0.00447, PBR28=0.01015
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

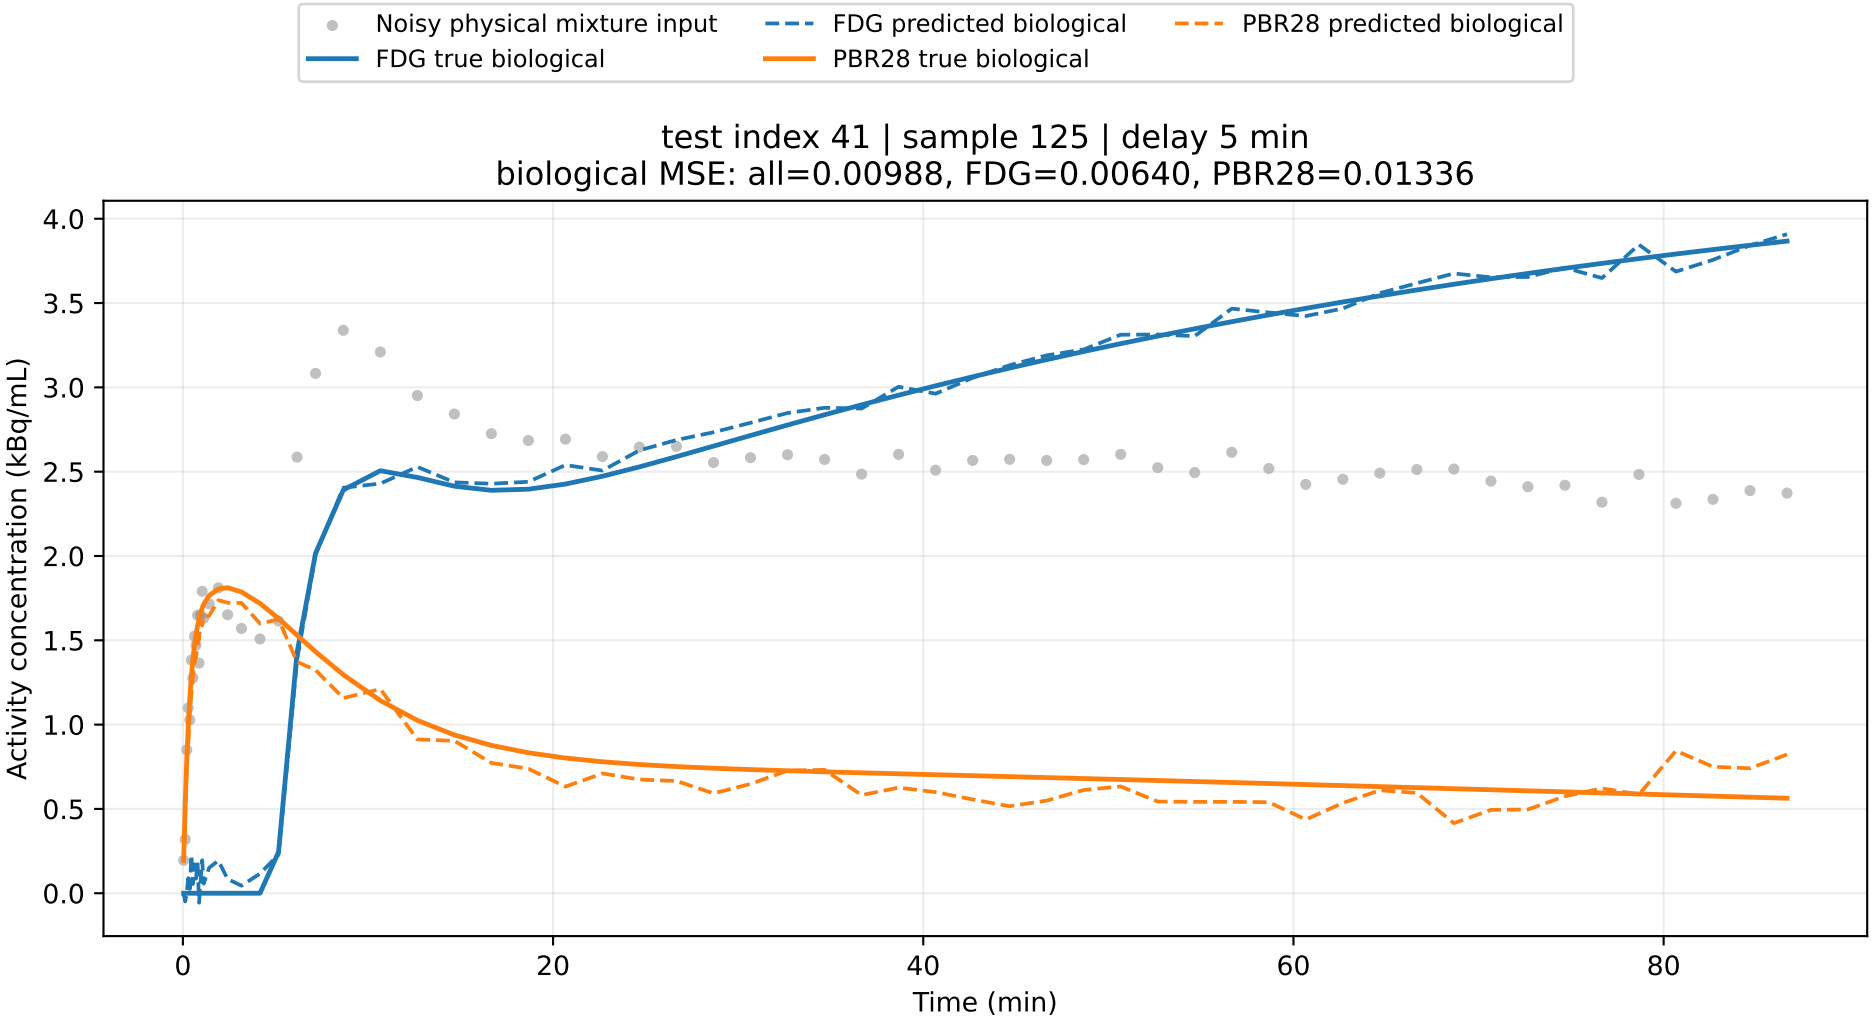

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 36 | sample 414 | delay 10 min
biological MSE: all=0.00961, FDG=0.00497, PBR28=0.01425
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

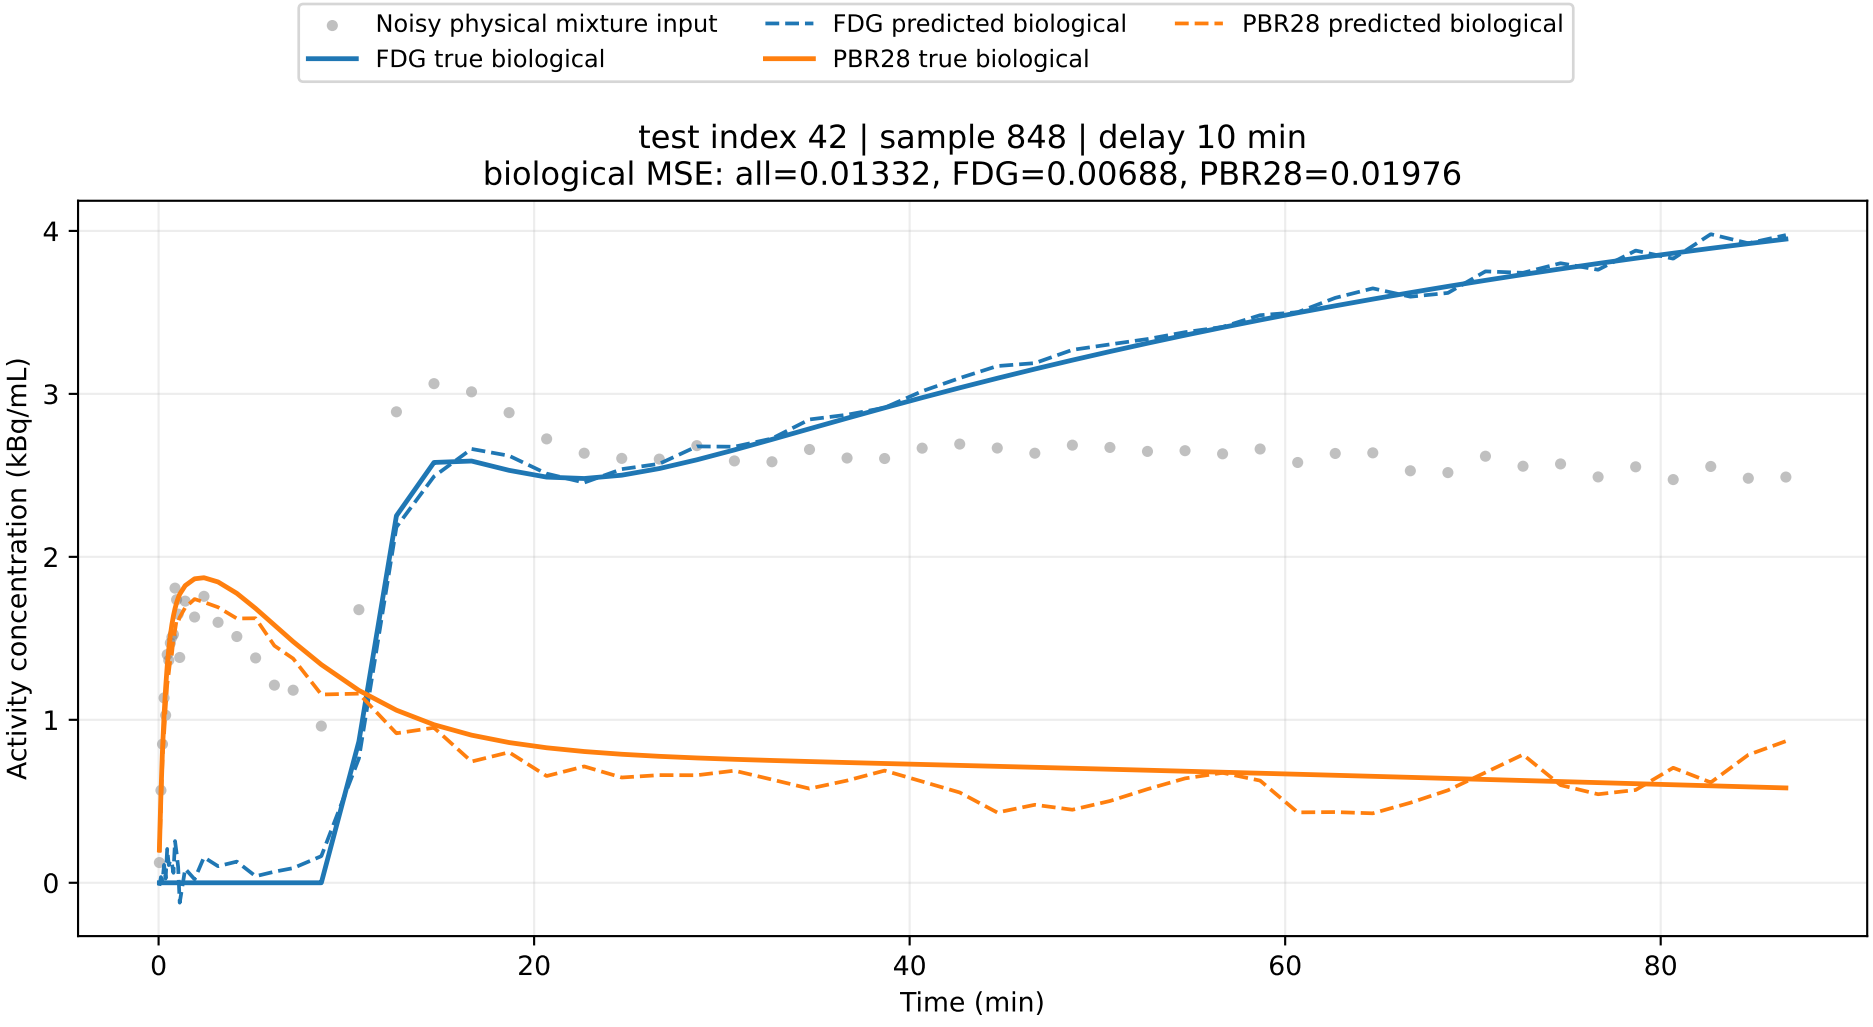

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 37 | sample 728 | delay 10 min
biological MSE: all=0.01038, FDG=0.00777, PBR28=0.01299
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

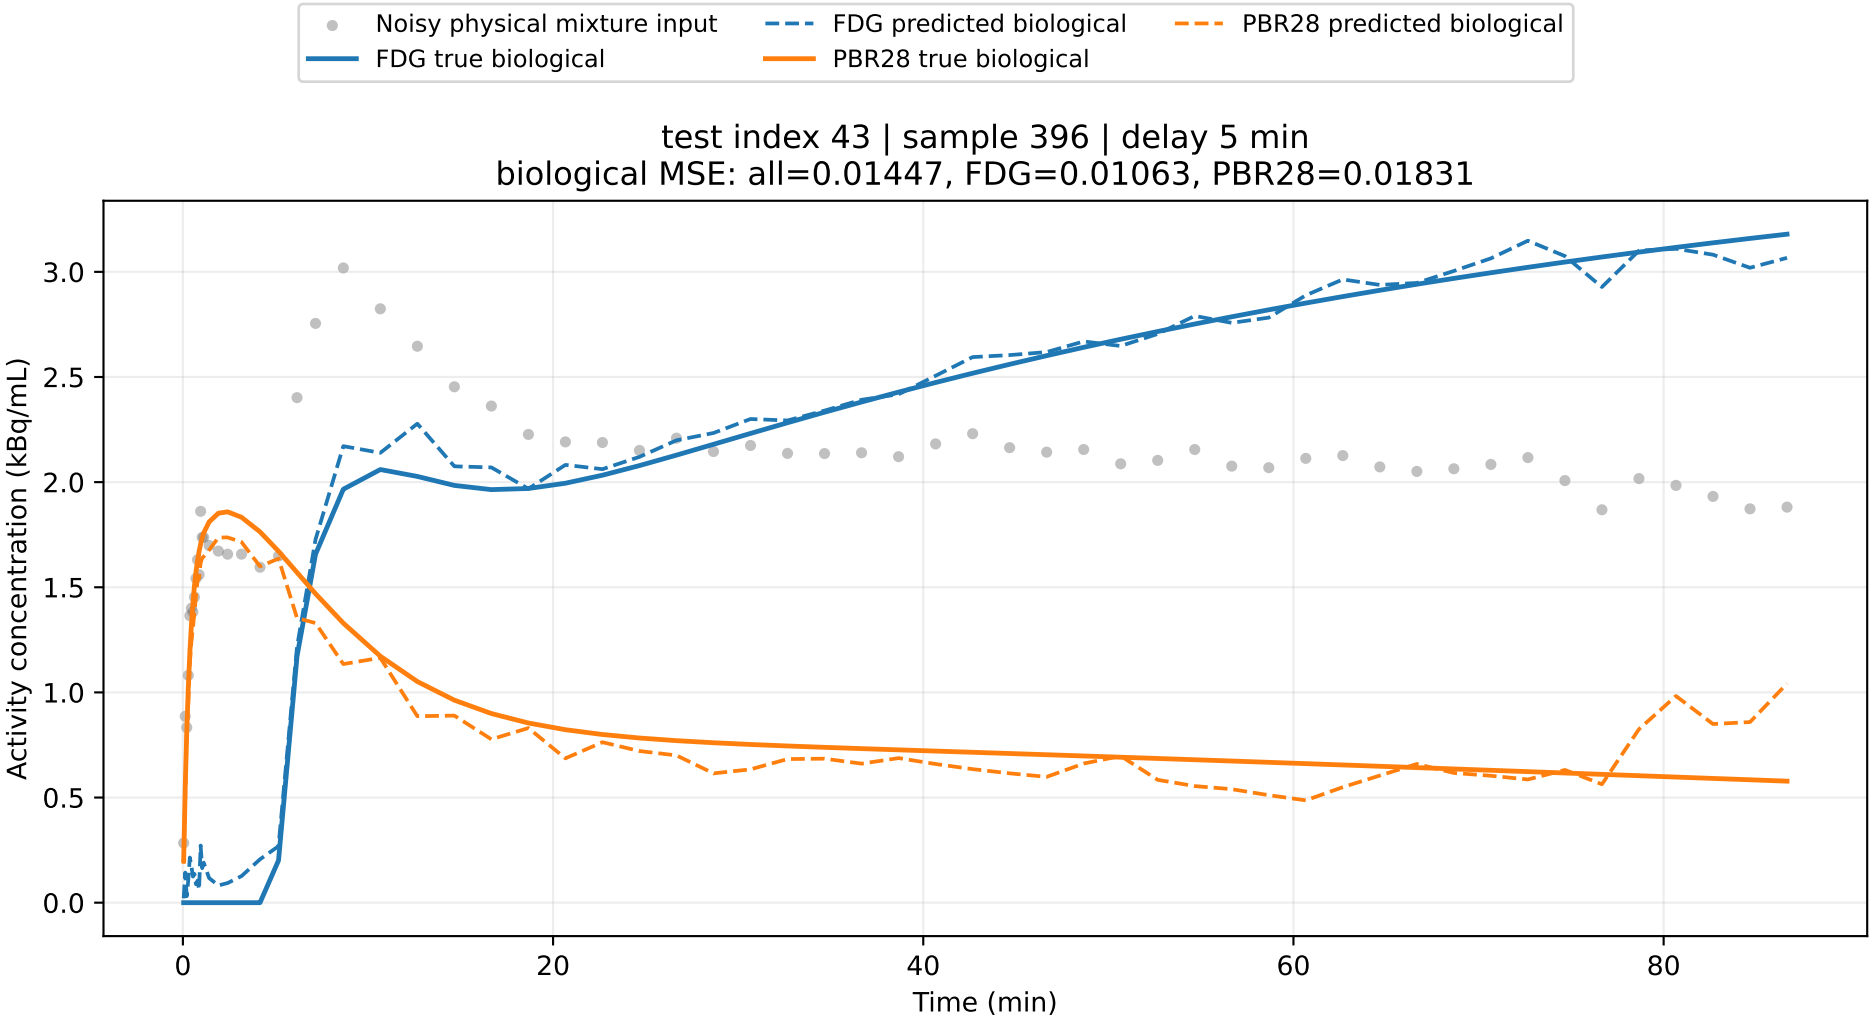

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 38 | sample 261 | delay 0 min
biological MSE: all=0.02240, FDG=0.01619, PBR28=0.02860
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

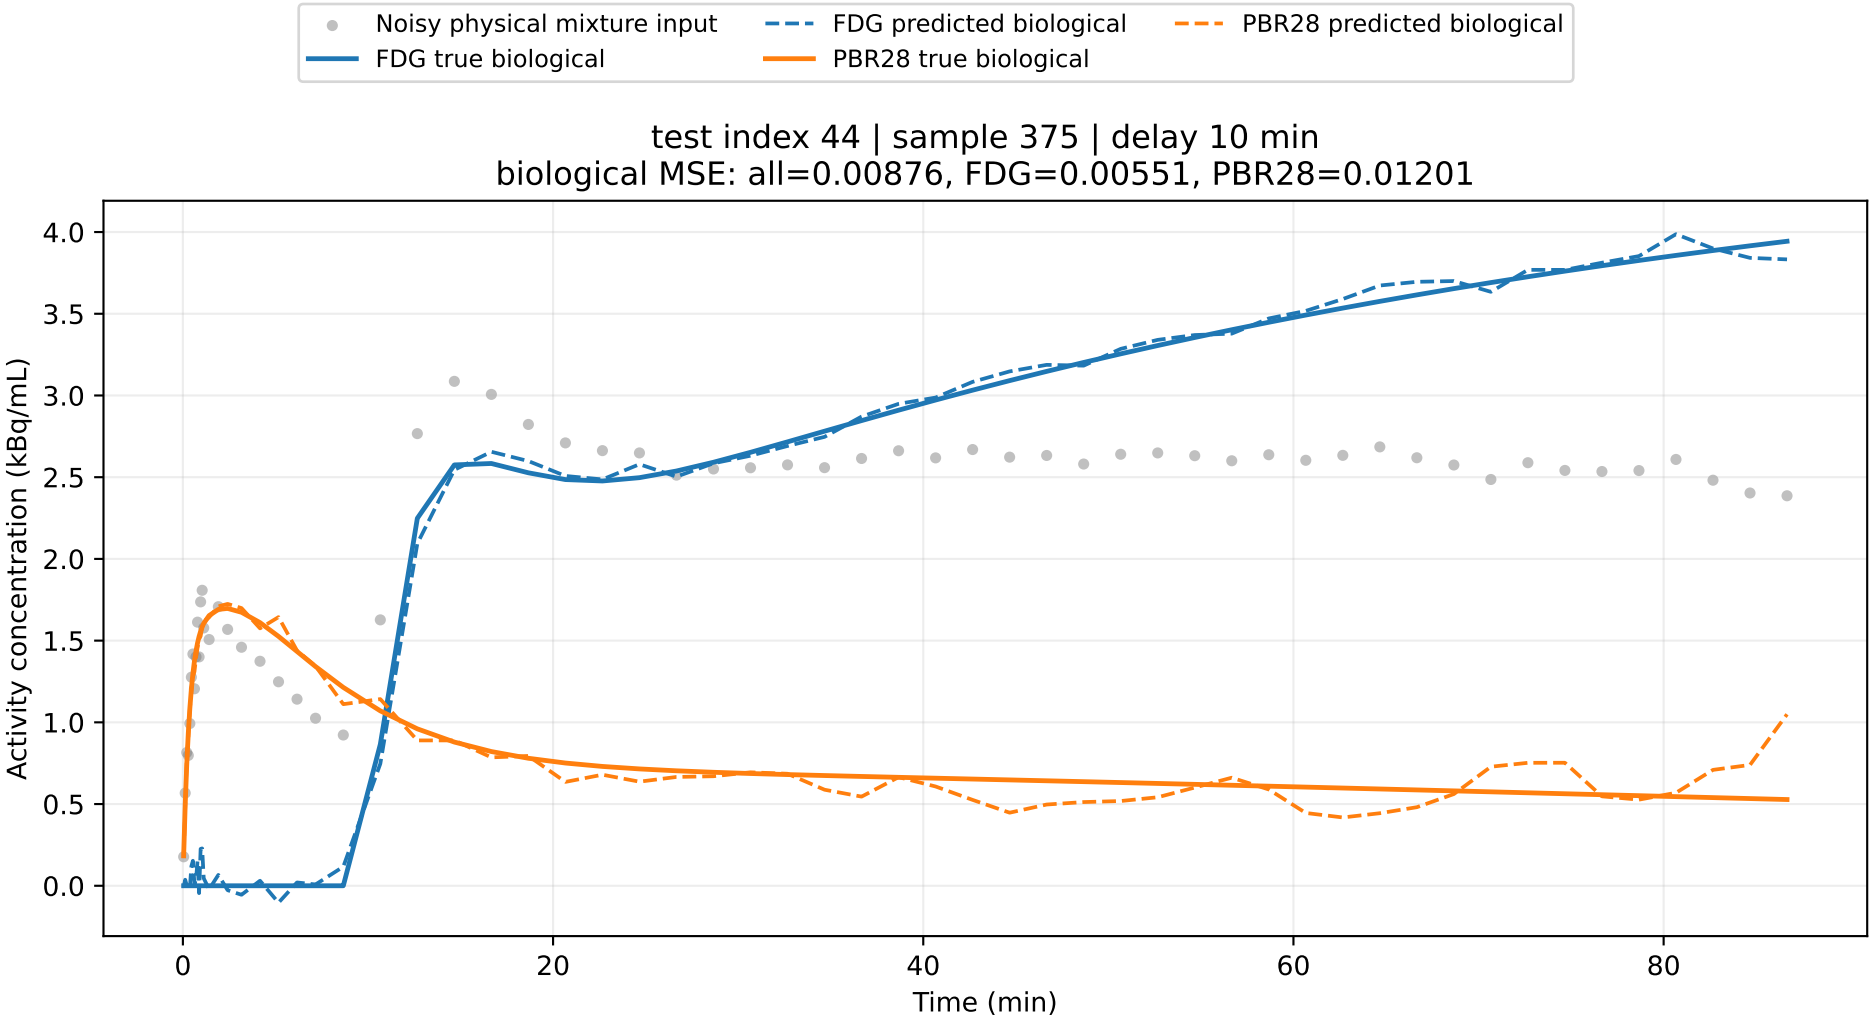

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 39 | sample 514 | delay 10 min
biological MSE: all=0.01660, FDG=0.01347, PBR28=0.01974
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

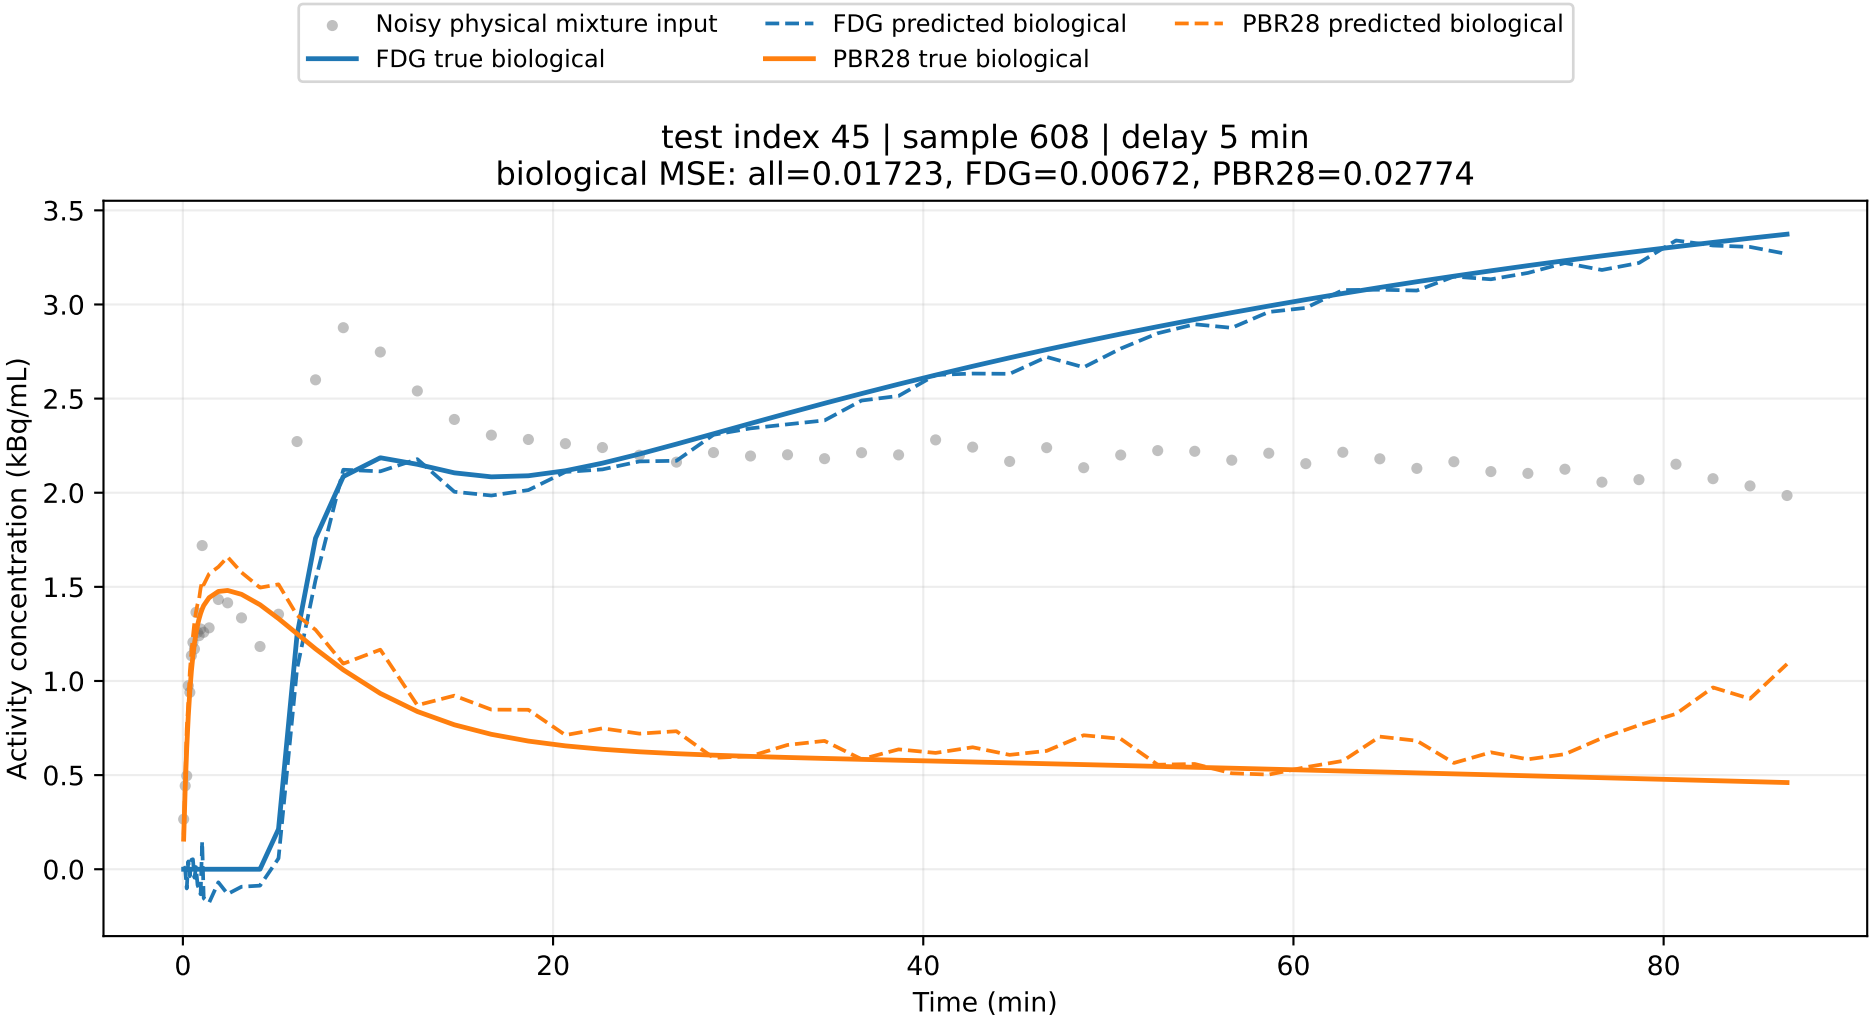

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 40 | sample 326 | delay 10 min
biological MSE: all=0.01534, FDG=0.01132, PBR28=0.01935
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

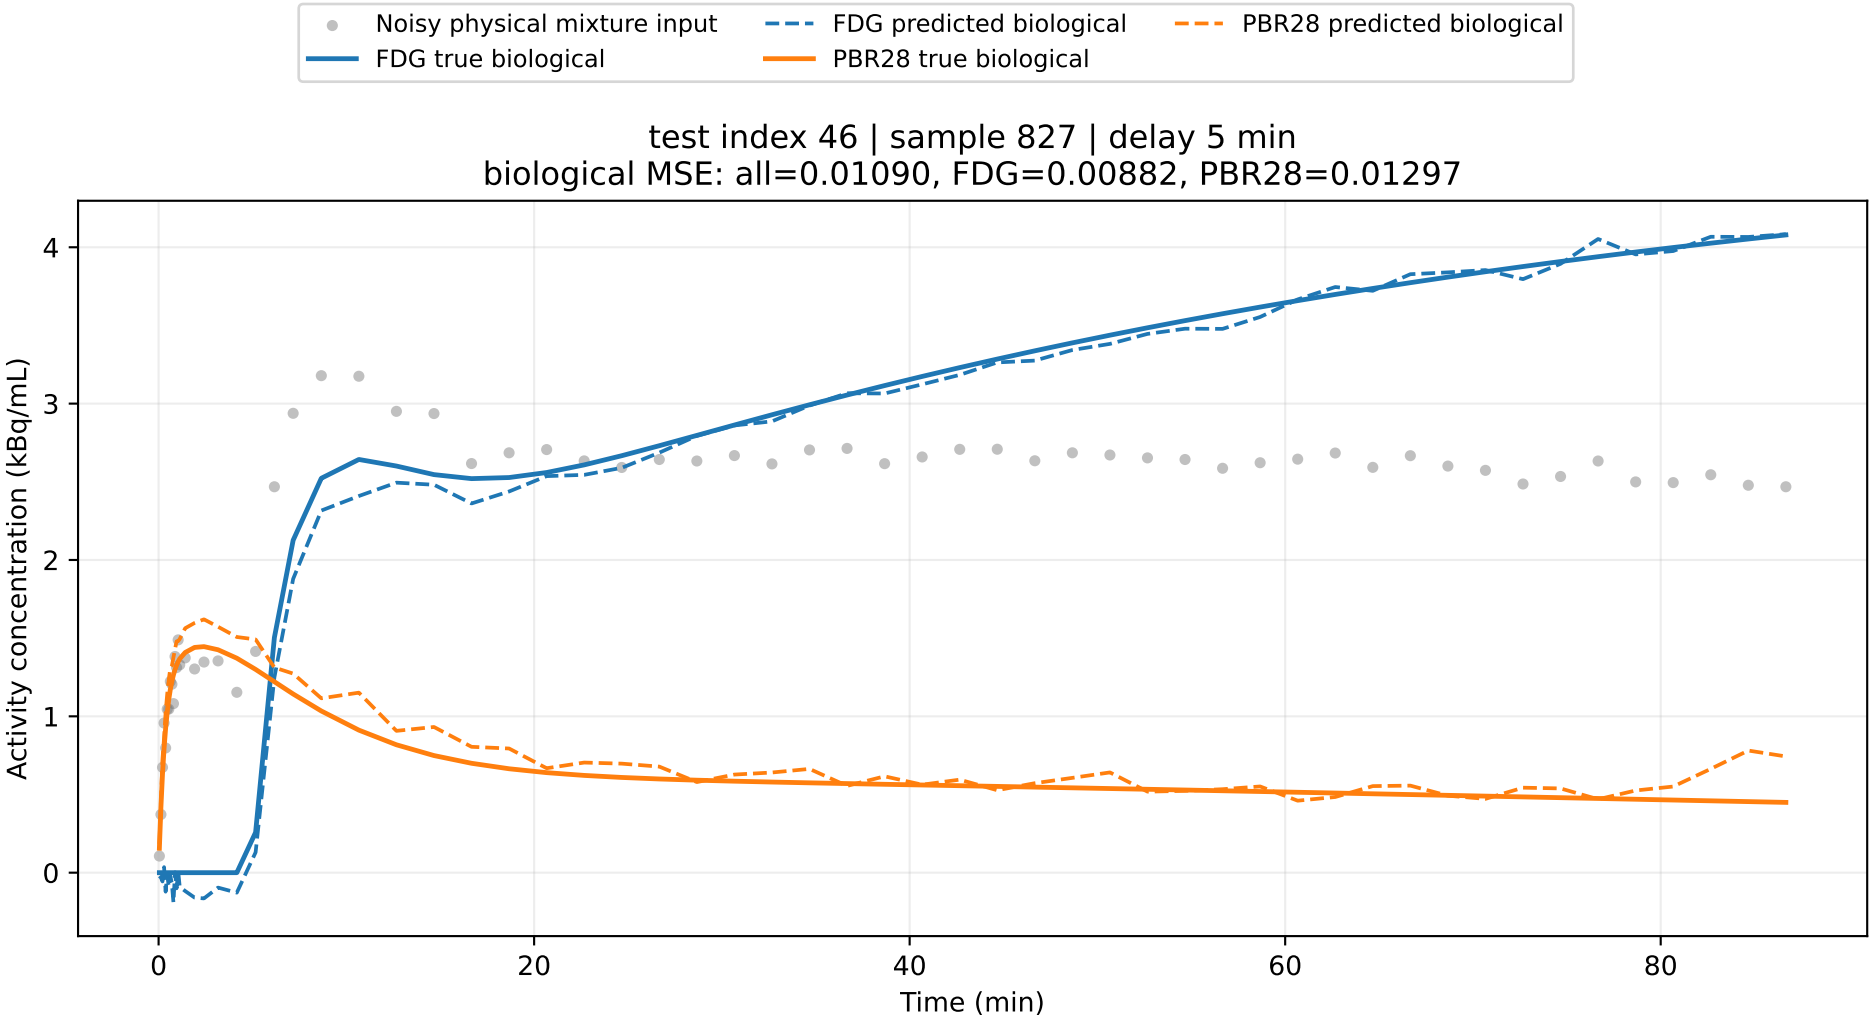

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 41 | sample 125 | delay 5 min
biological MSE: all=0.00988, FDG=0.00640, PBR28=0.01336
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

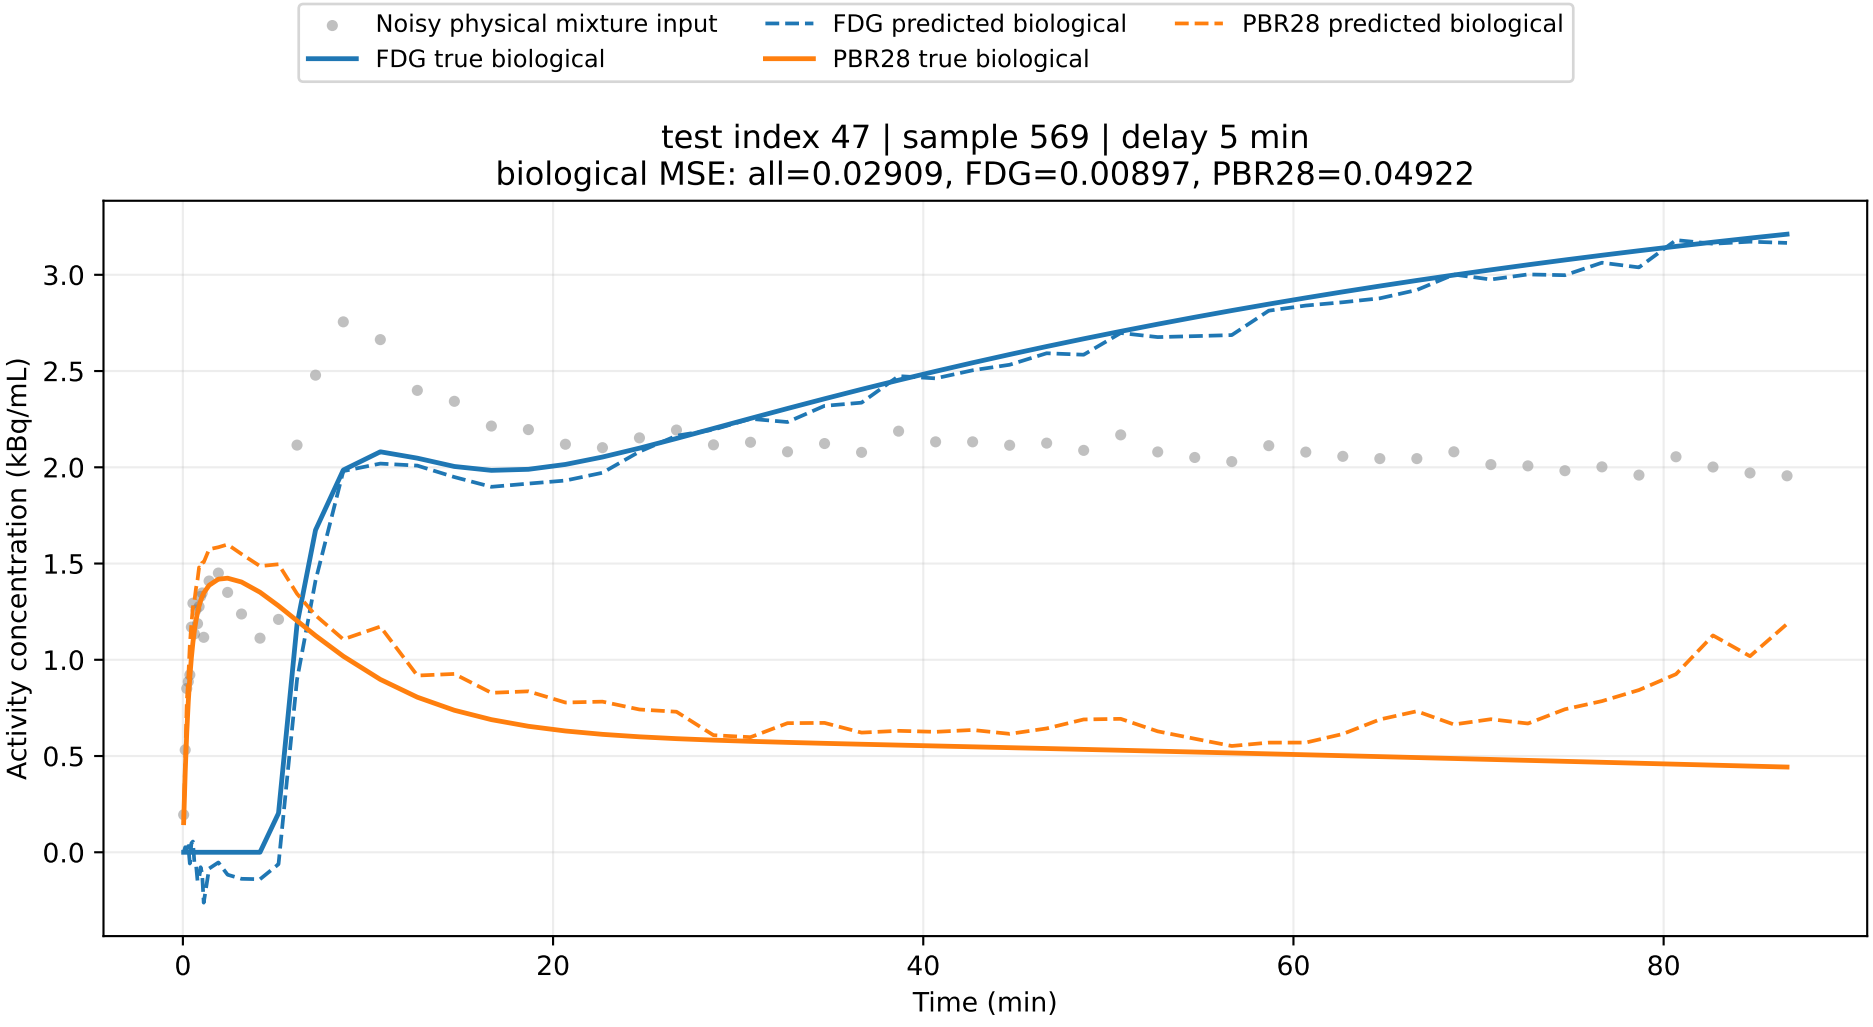

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 42 | sample 848 | delay 10 min
biological MSE: all=0.01332, FDG=0.00688, PBR28=0.01976
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

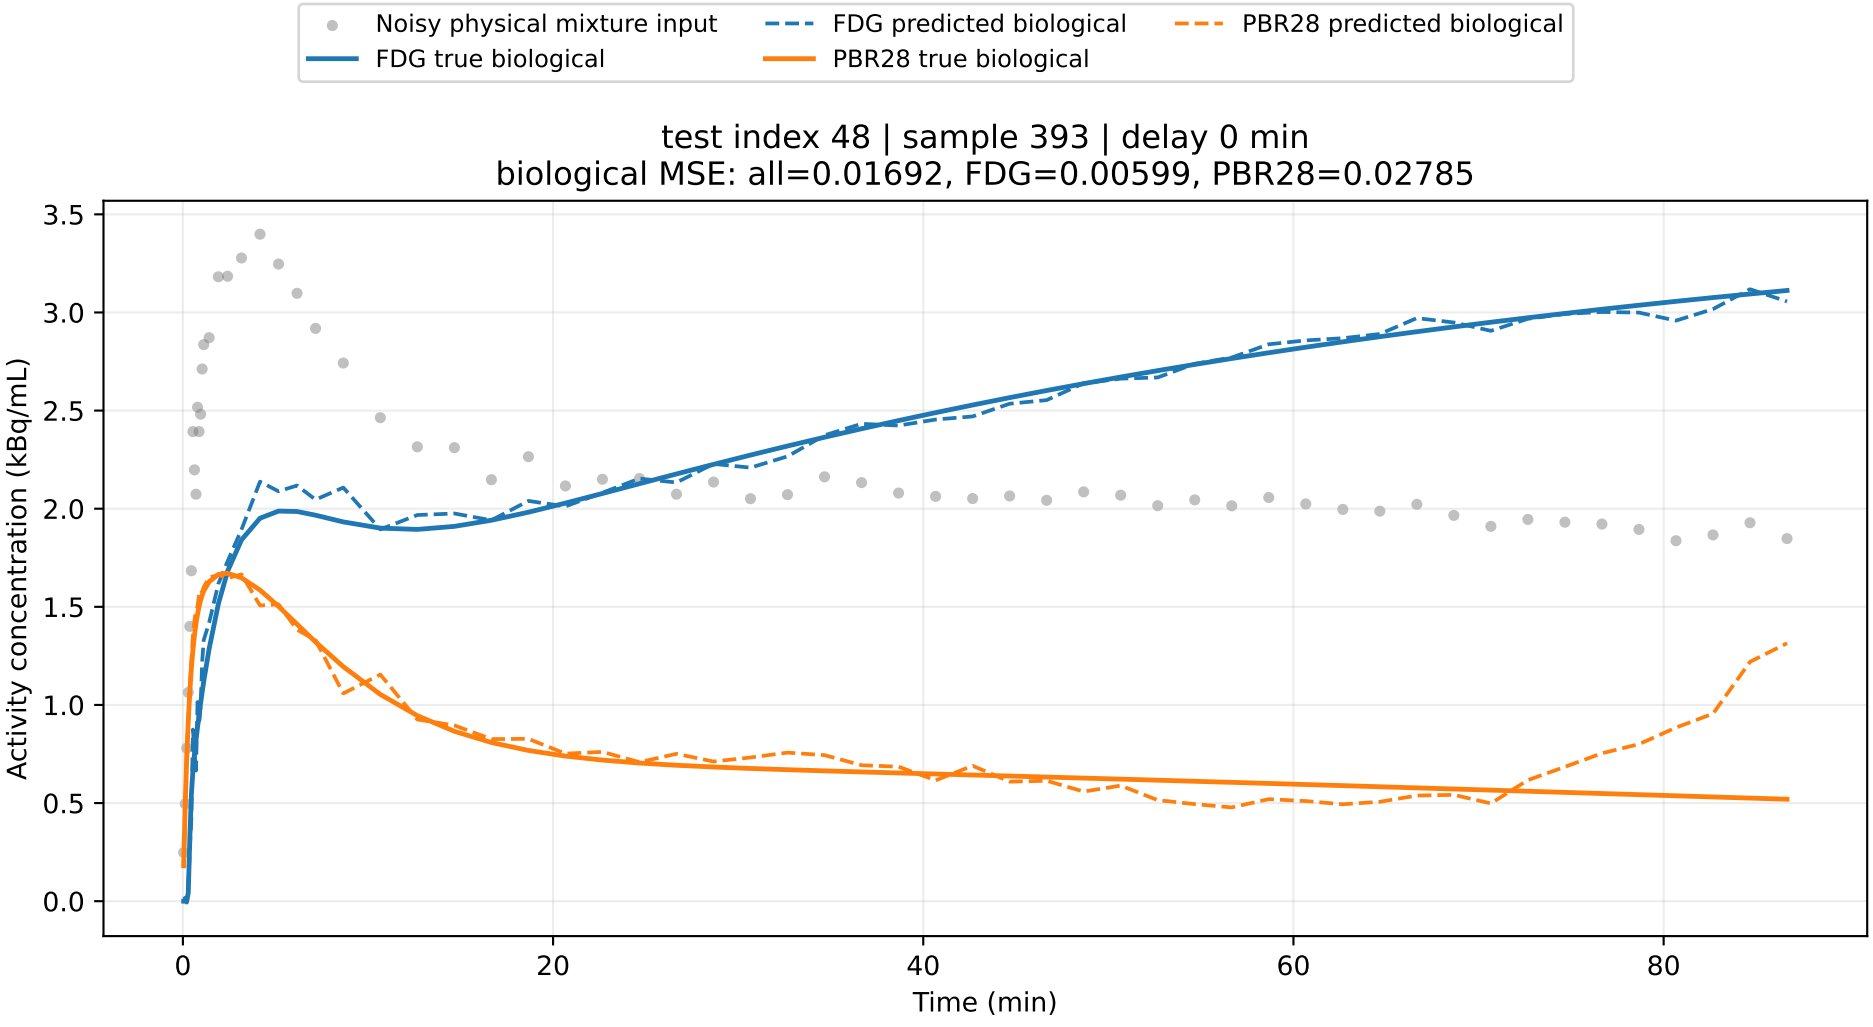

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 43 | sample 396 | delay 5 min
biological MSE: all=0.01447, FDG=0.01063, PBR28=0.01831
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

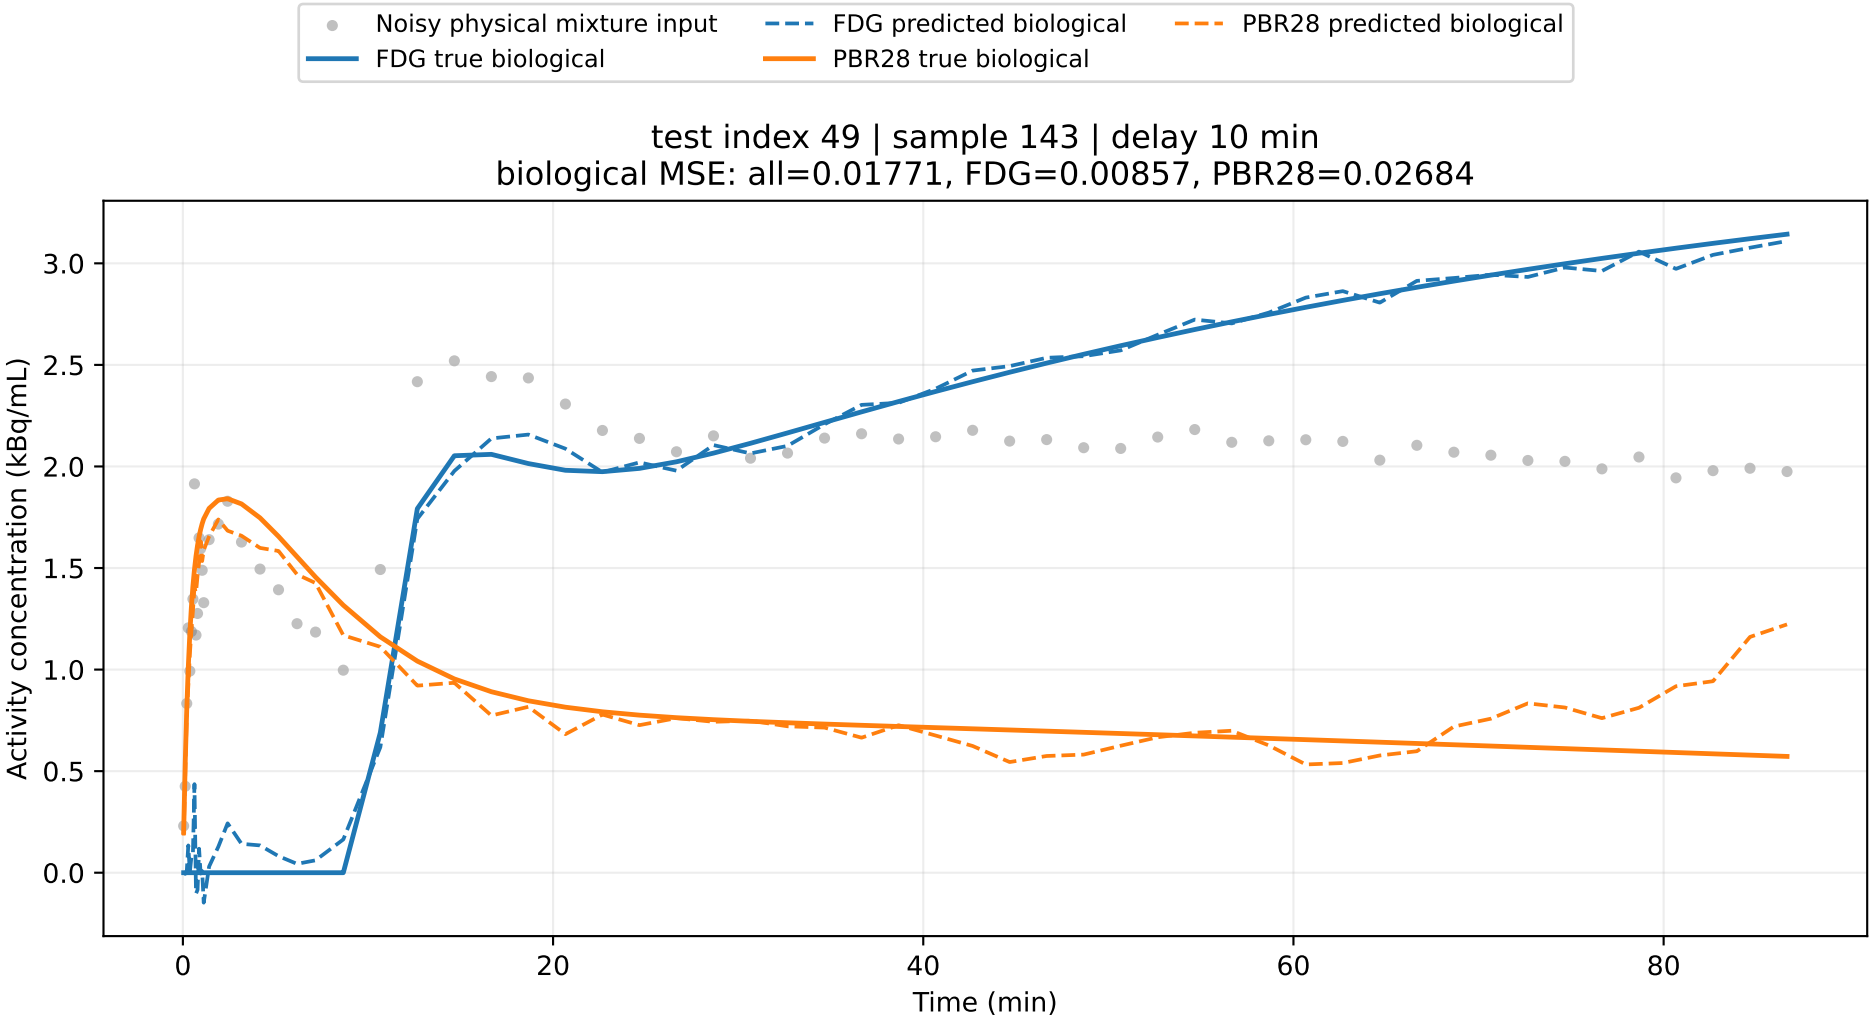

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 44 | sample 375 | delay 10 min
biological MSE: all=0.00876, FDG=0.00551, PBR28=0.01201
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

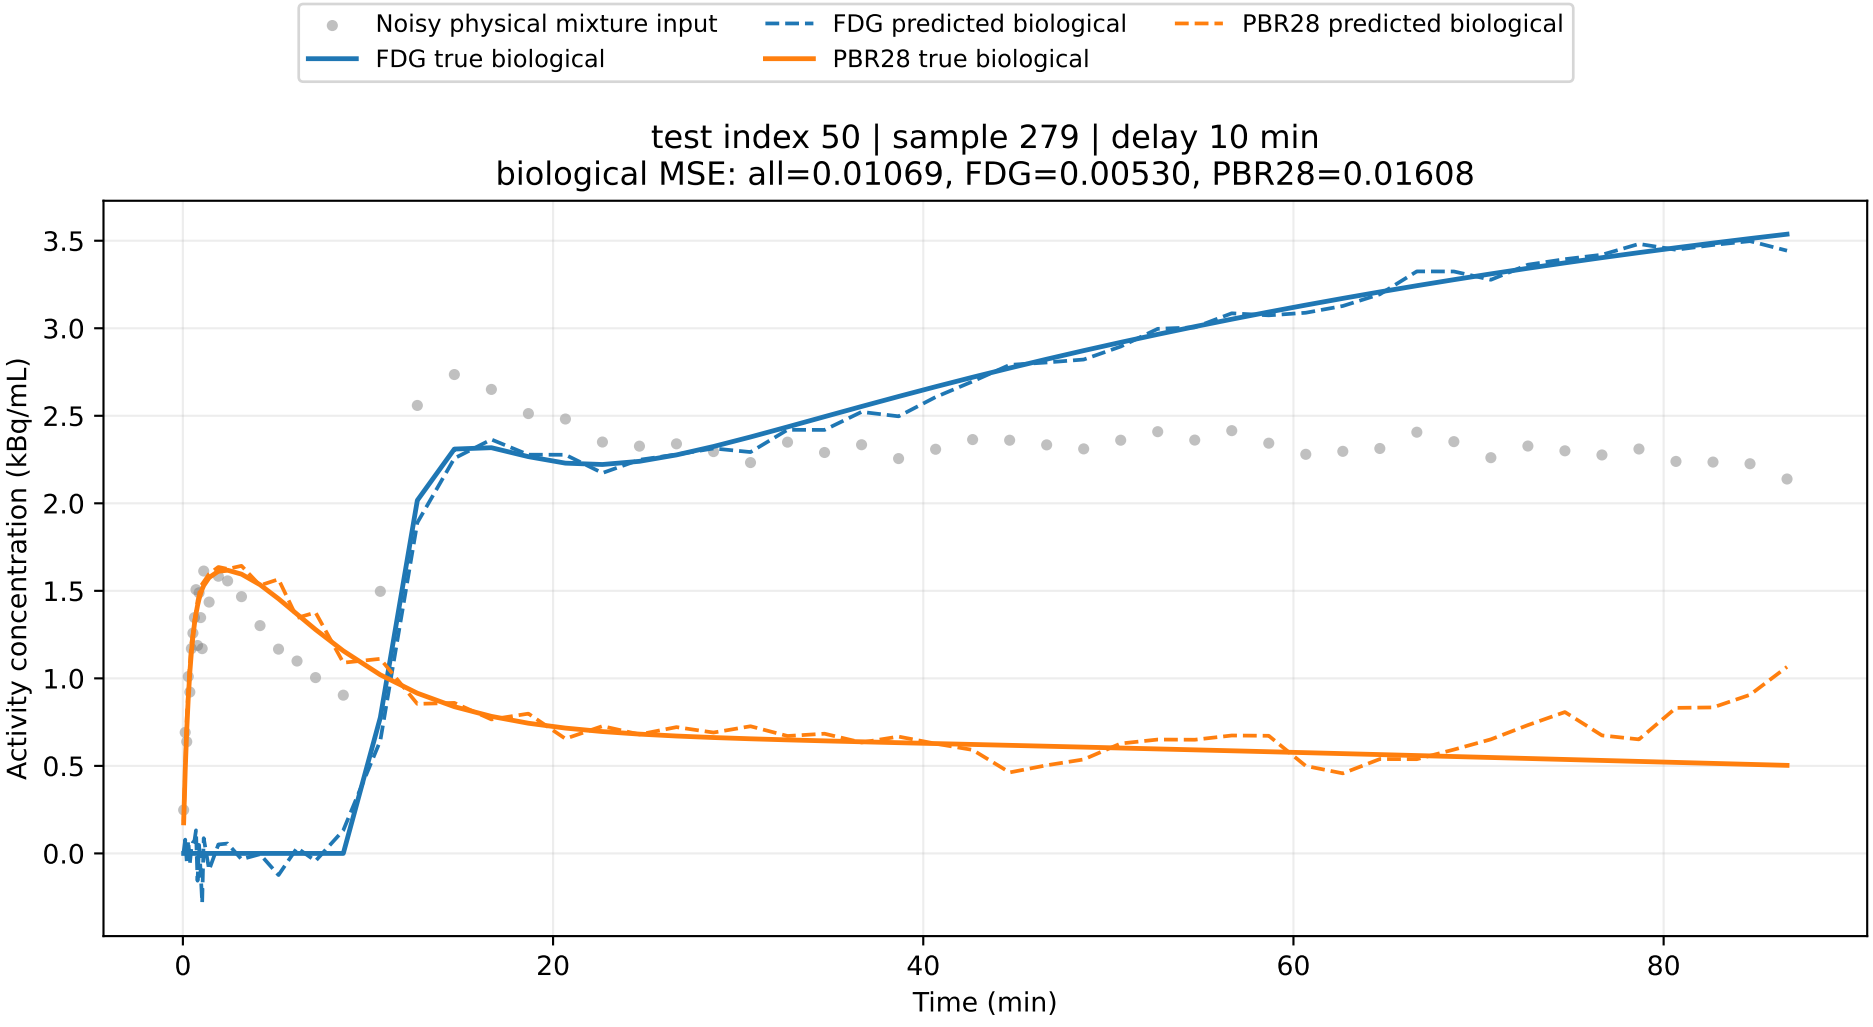

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 45 | sample 608 | delay 5 min
biological MSE: all=0.01723, FDG=0.00672, PBR28=0.02774
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

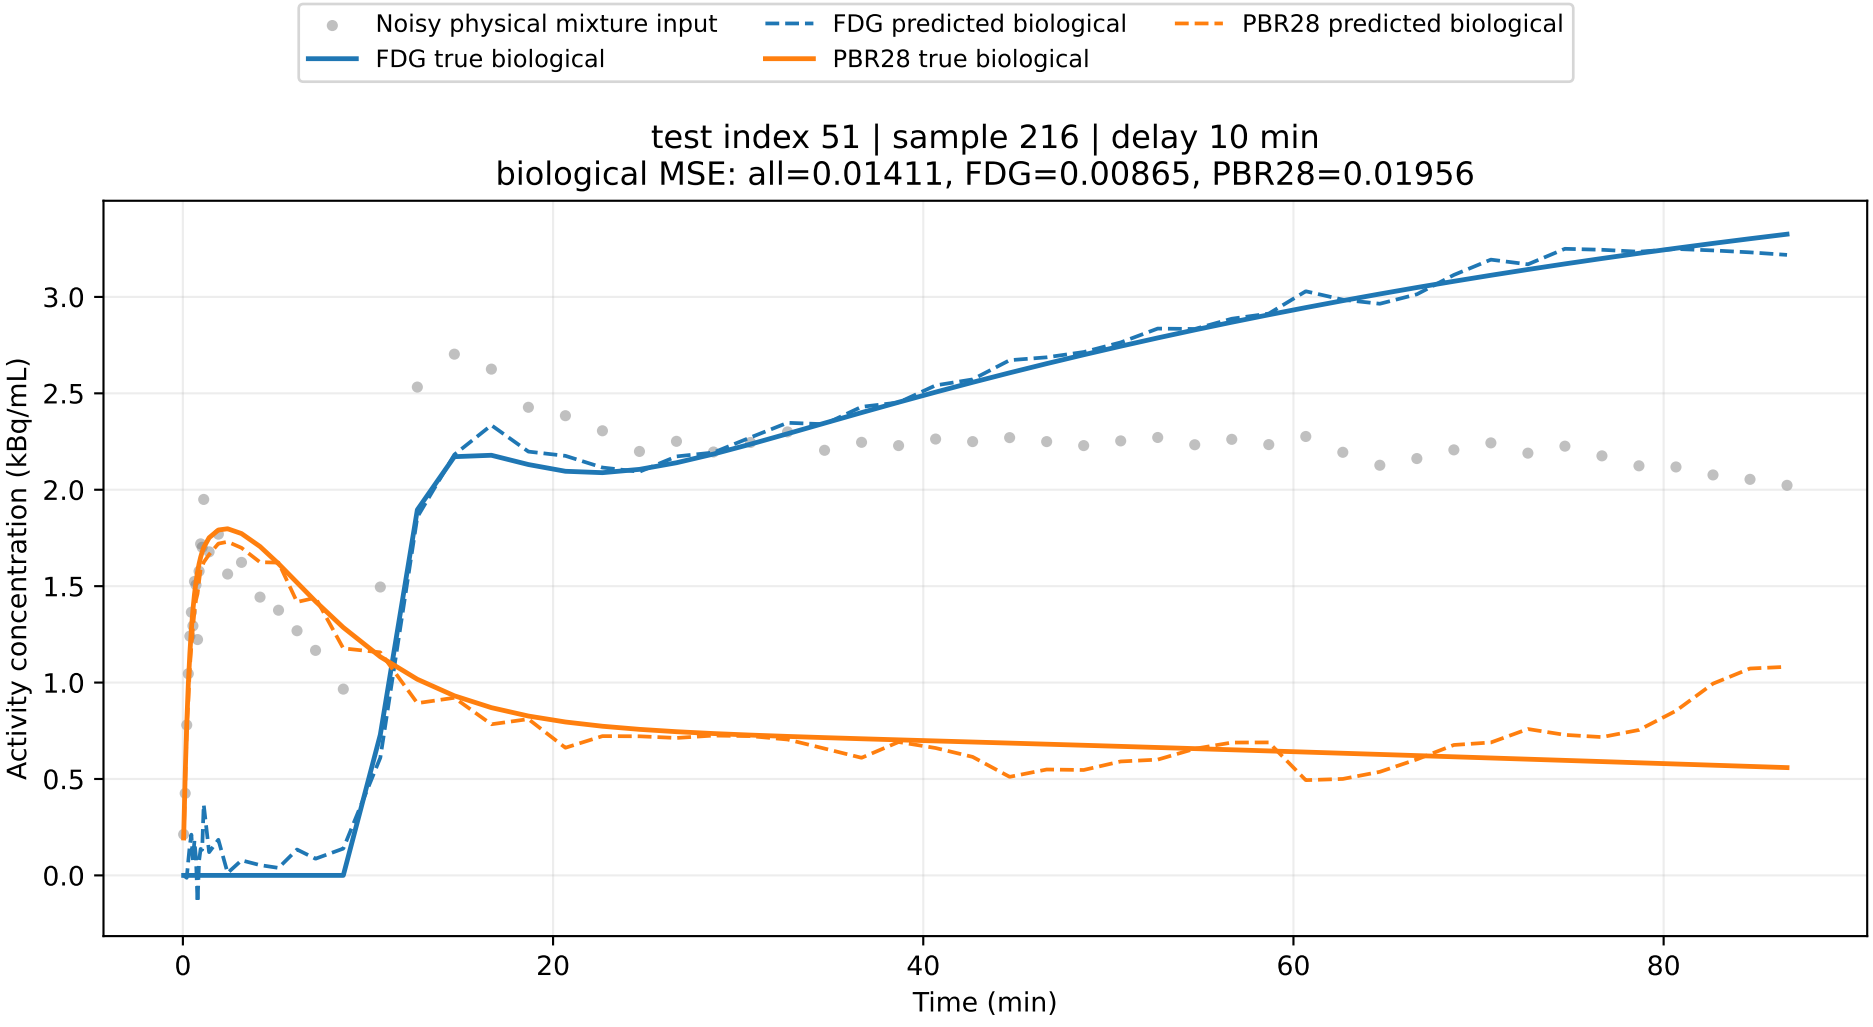

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 46 | sample 827 | delay 5 min
biological MSE: all=0.01090, FDG=0.00882, PBR28=0.01297
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

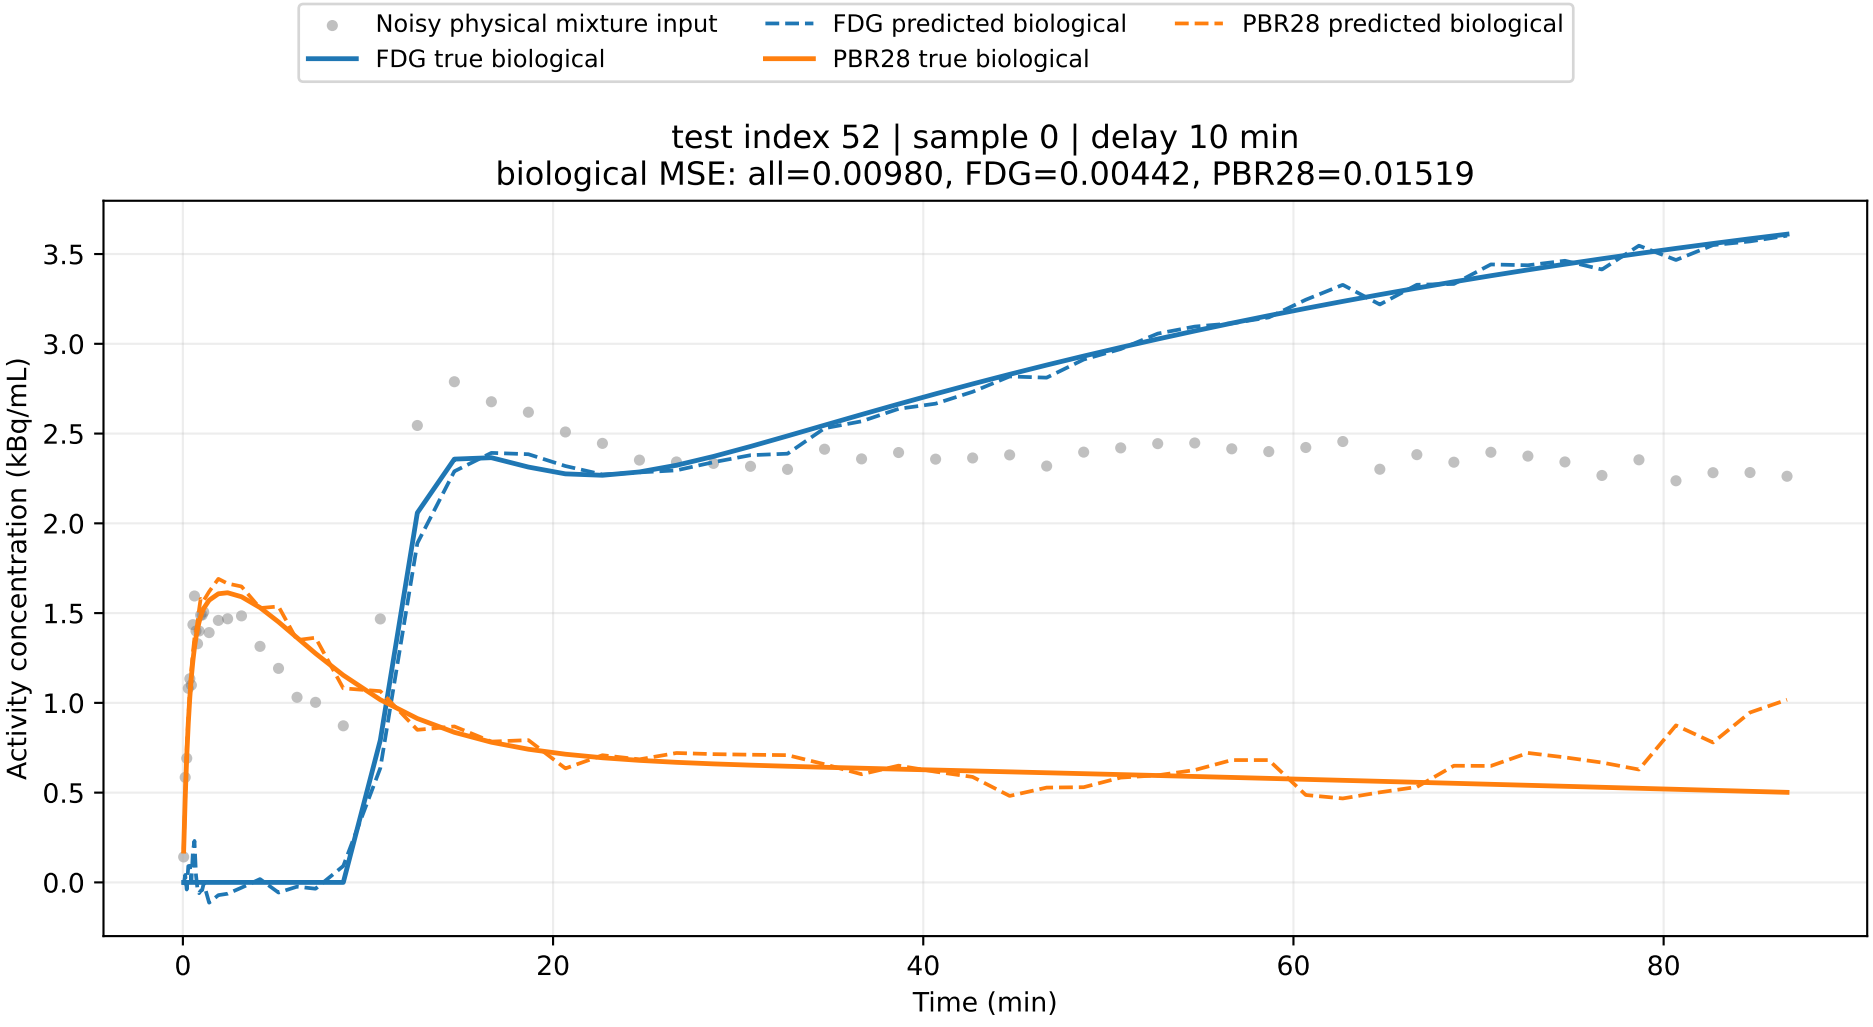

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 47 | sample 569 | delay 5 min
biological MSE: all=0.02909, FDG=0.00897, PBR28=0.04922
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

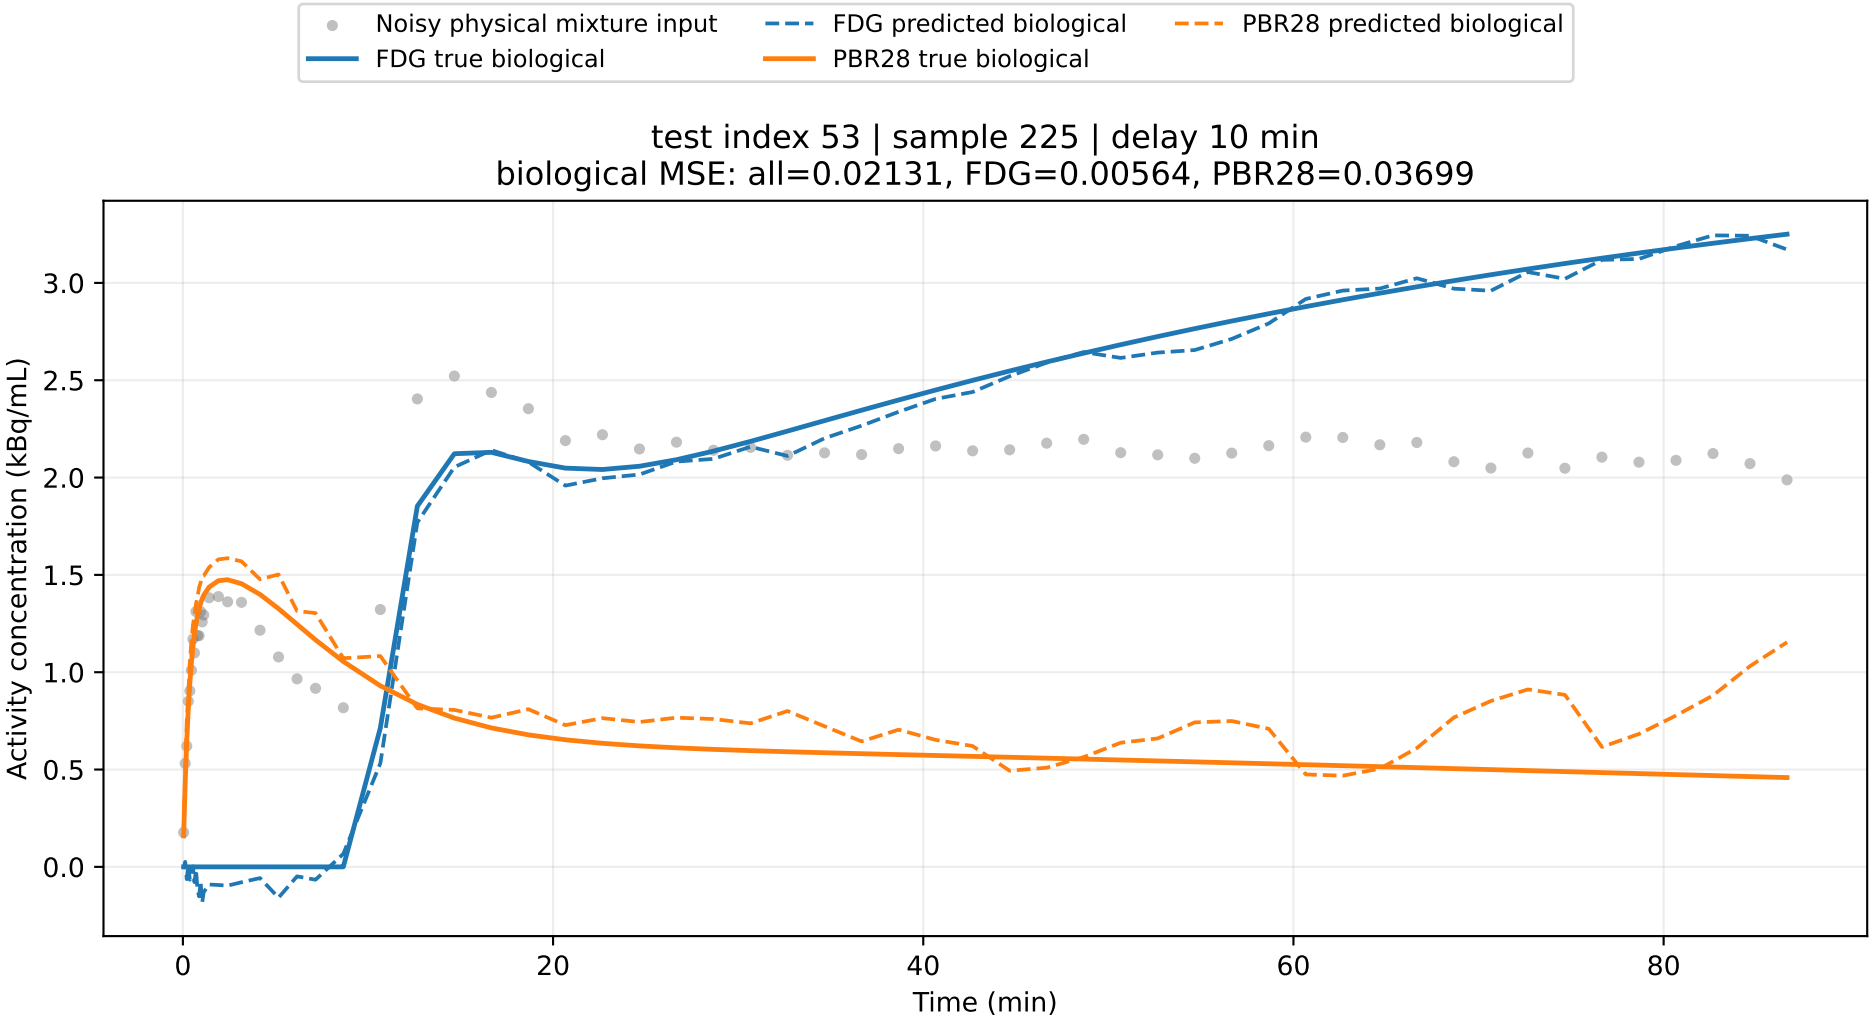

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 48 | sample 393 | delay 0 min
biological MSE: all=0.01692, FDG=0.00599, PBR28=0.02785
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

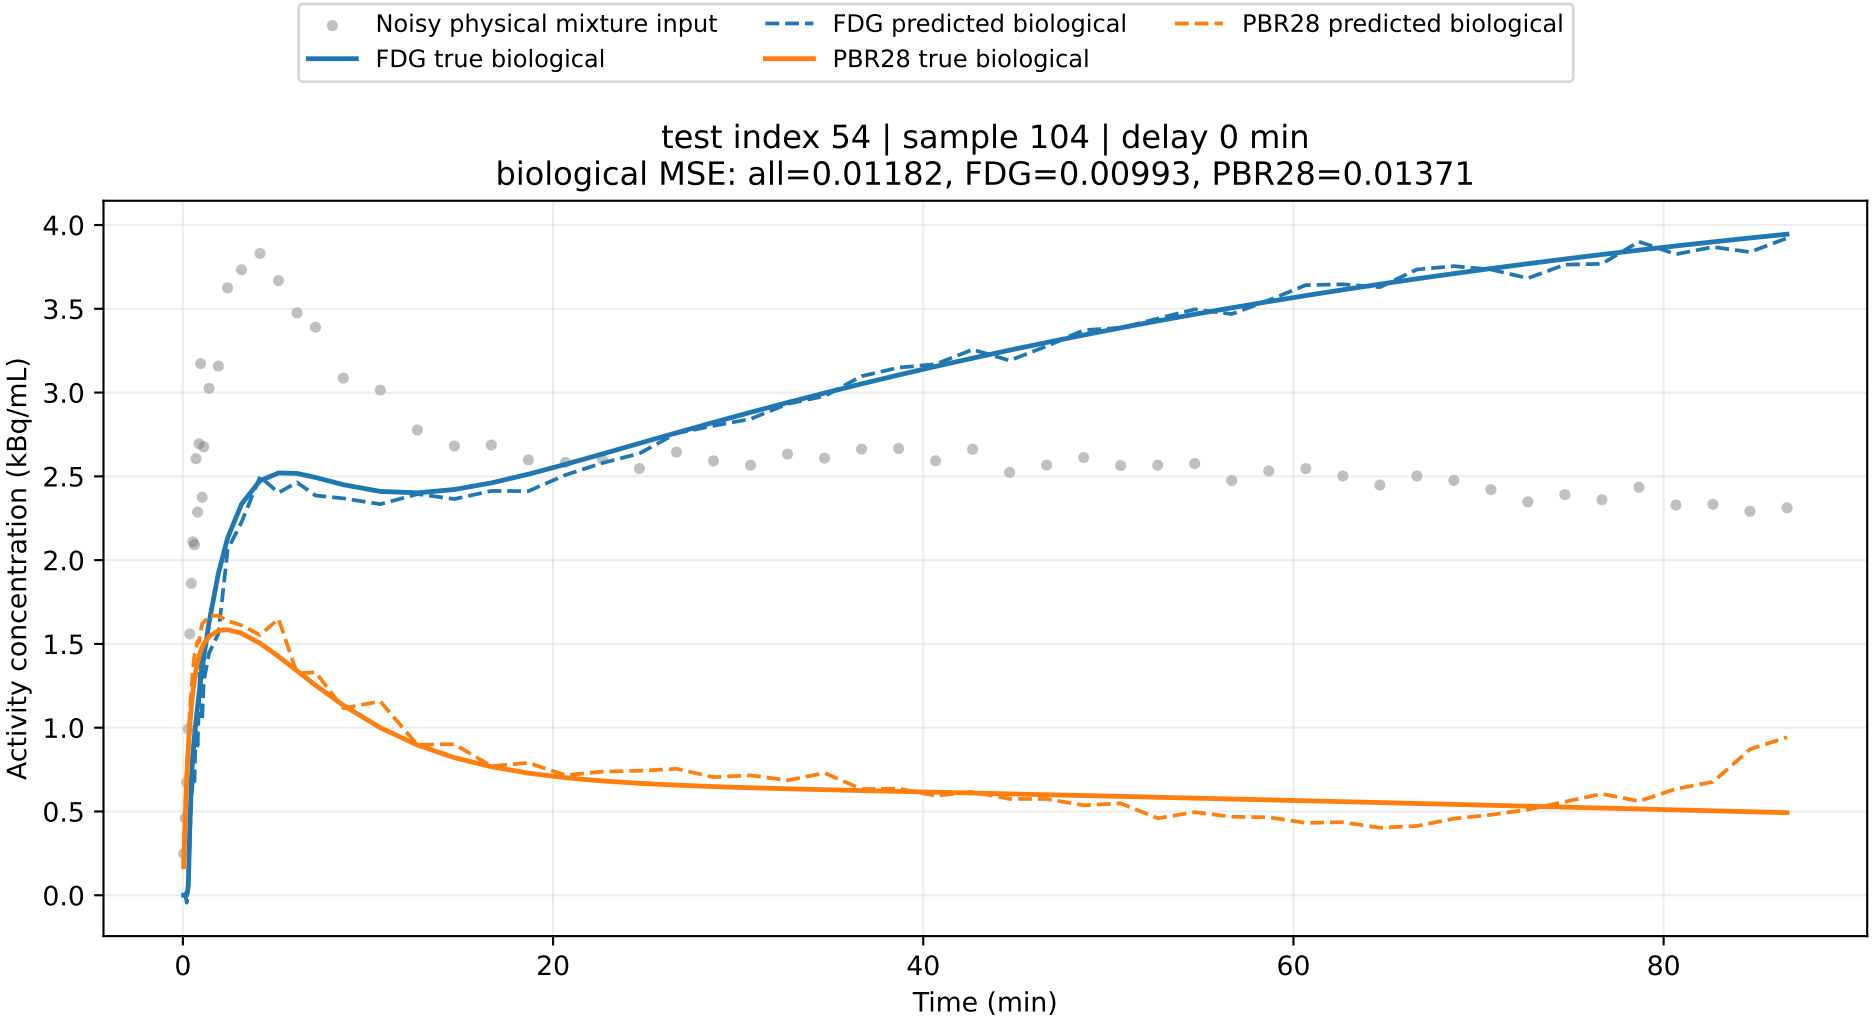

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 49 | sample 143 | delay 10 min
biological MSE: all=0.01771, FDG=0.00857, PBR28=0.02684
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

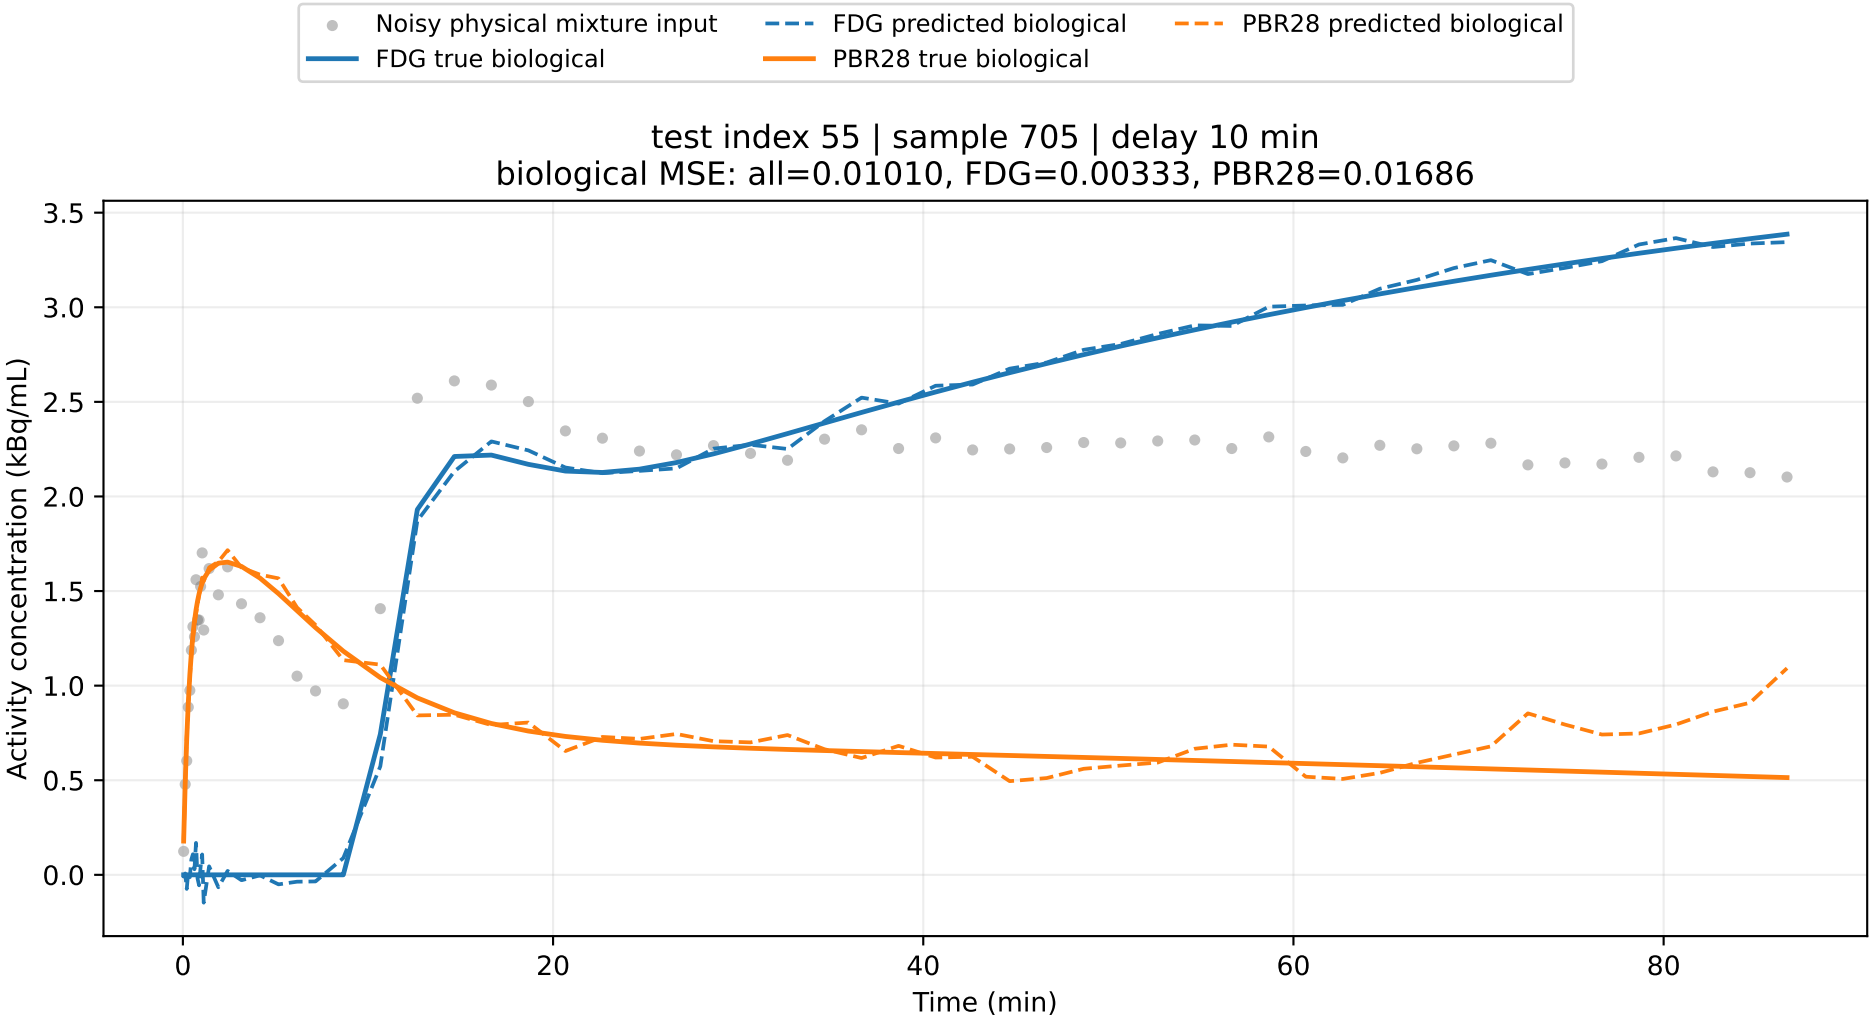

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 50 | sample 279 | delay 10 min
biological MSE: all=0.01069, FDG=0.00530, PBR28=0.01608
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

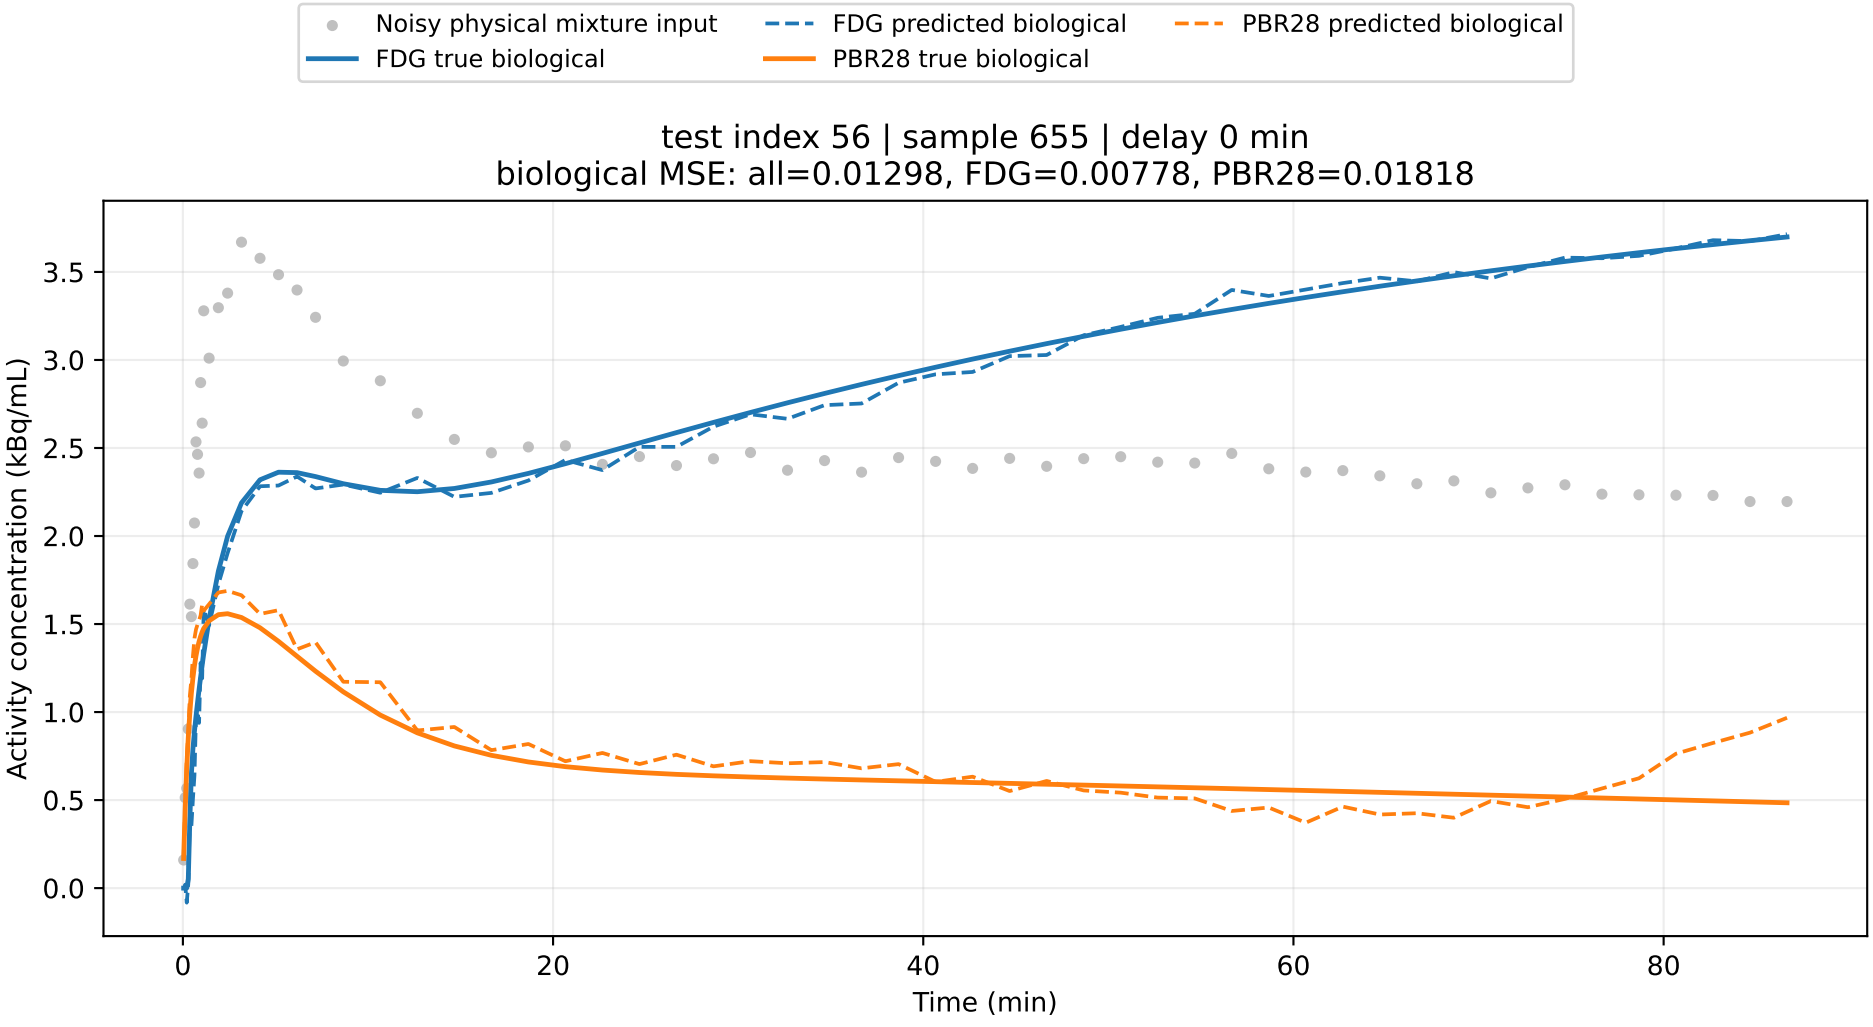

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 51 | sample 216 | delay 10 min
biological MSE: all=0.01411, FDG=0.00865, PBR28=0.01956
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

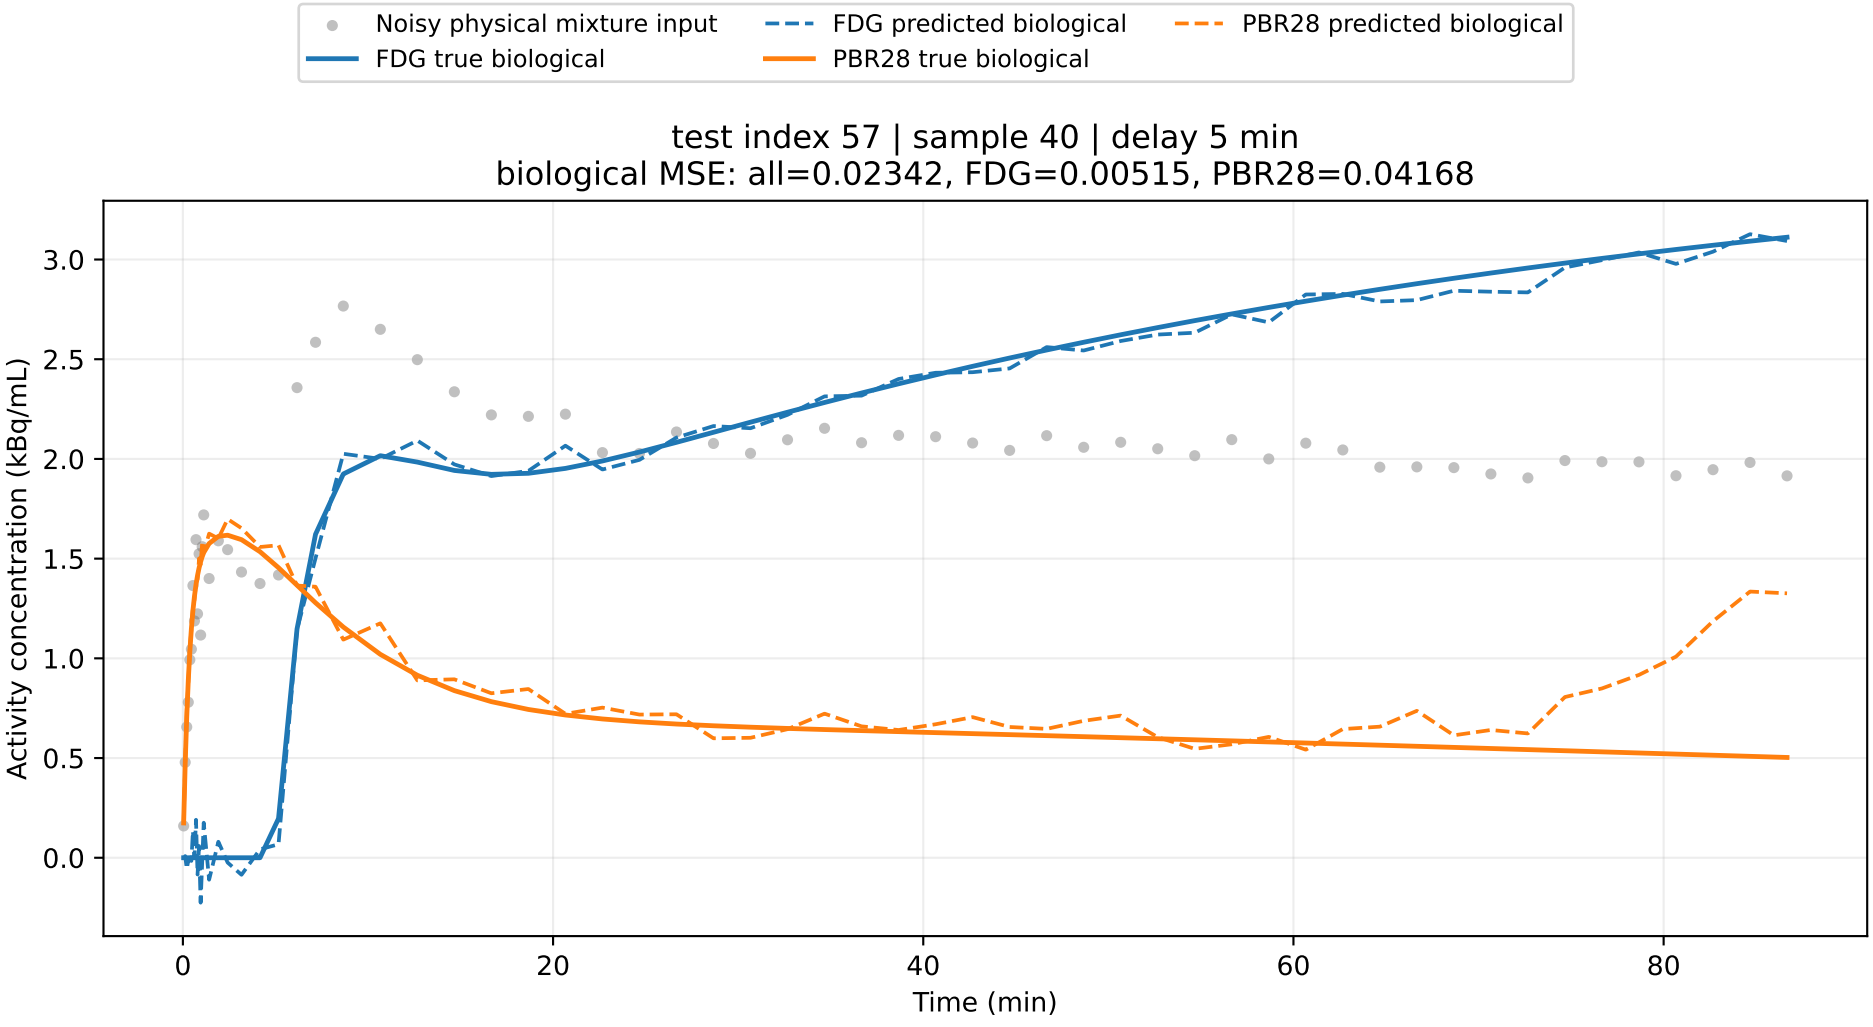

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 52 | sample 0 | delay 10 min
biological MSE: all=0.00980, FDG=0.00442, PBR28=0.01519
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

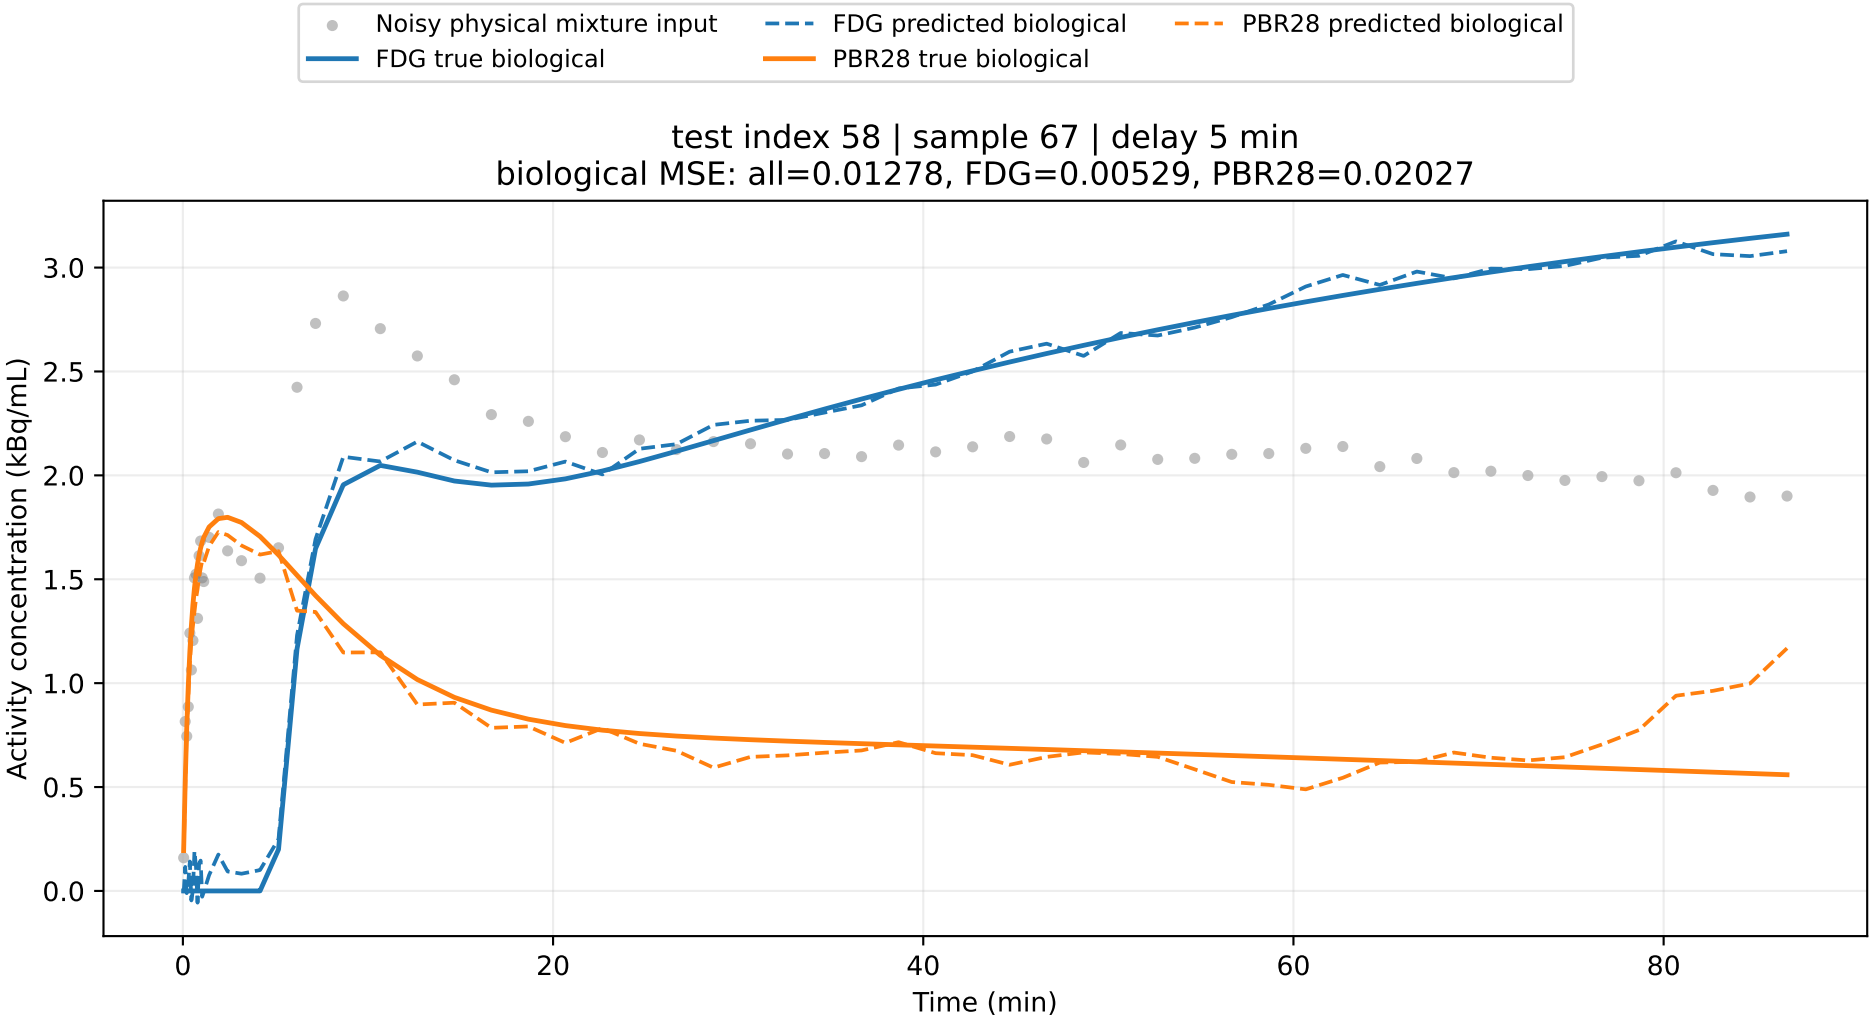

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 53 | sample 225 | delay 10 min
biological MSE: all=0.02131, FDG=0.00564, PBR28=0.03699
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

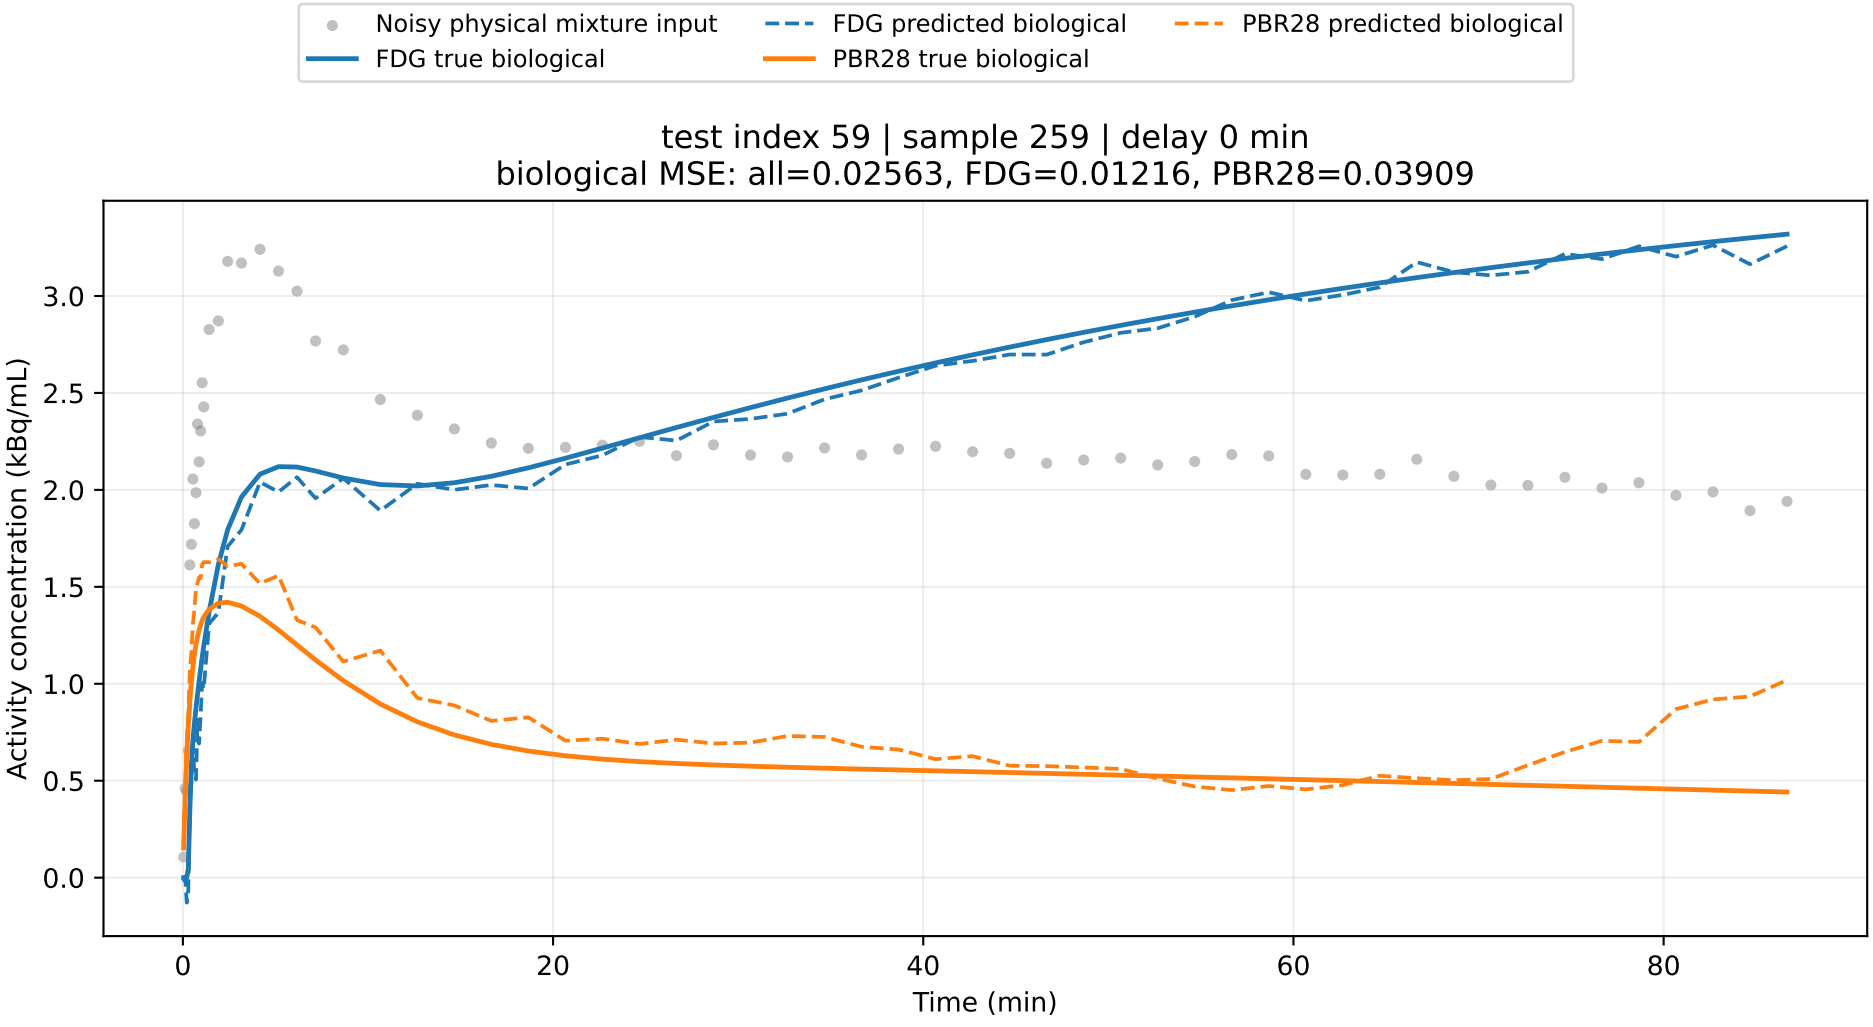

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 54 | sample 104 | delay 0 min
biological MSE: all=0.01182, FDG=0.00993, PBR28=0.01371
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

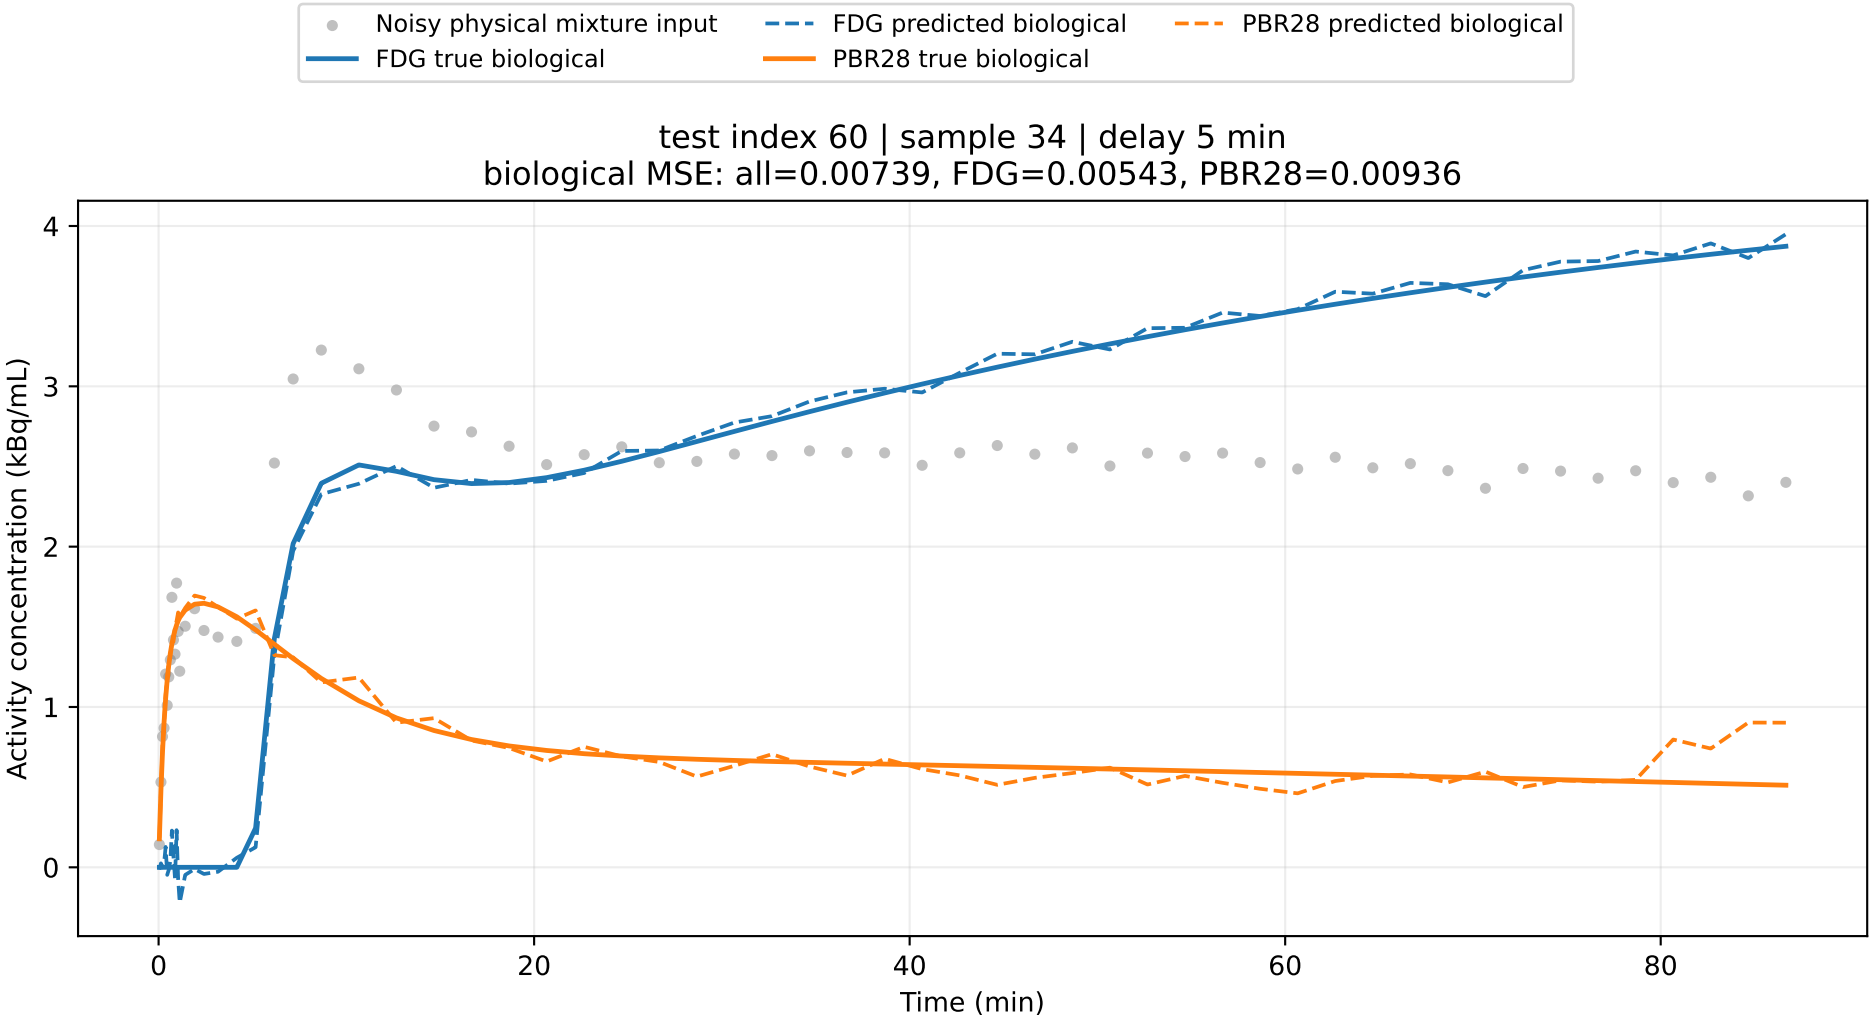

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 55 | sample 705 | delay 10 min
biological MSE: all=0.01010, FDG=0.00333, PBR28=0.01686
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

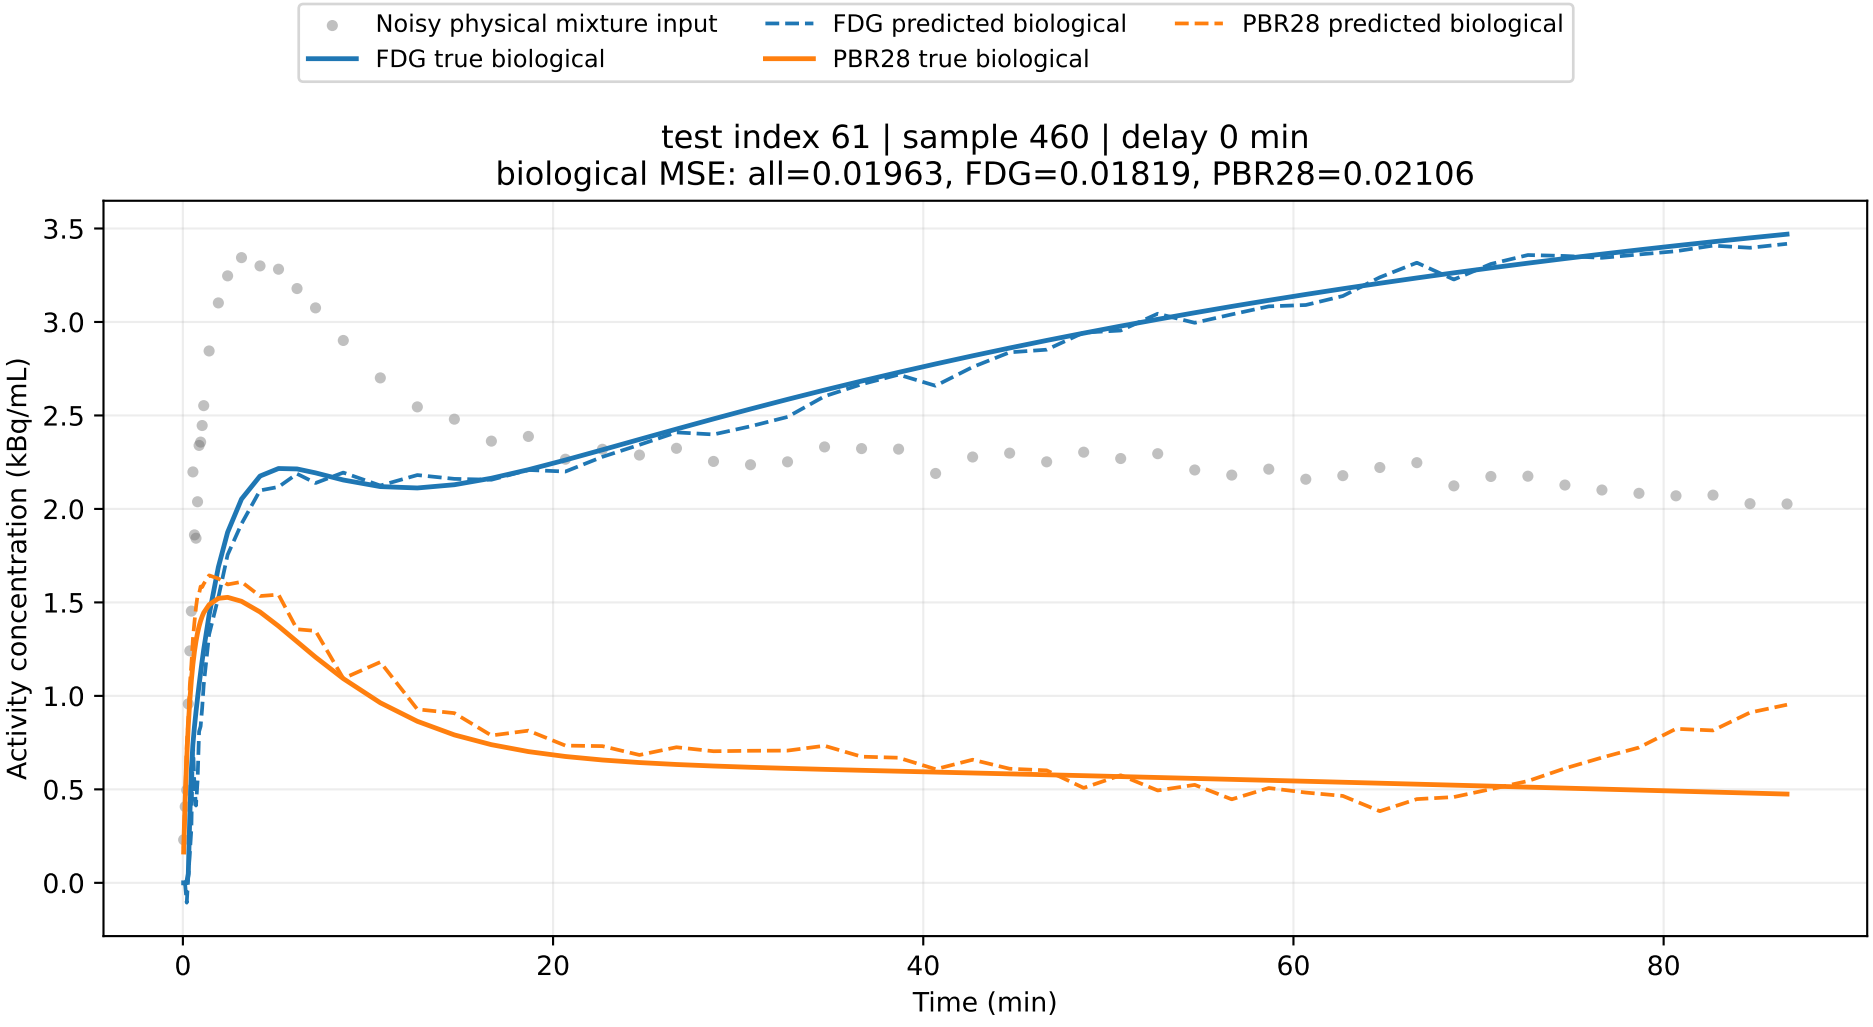

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 56 | sample 655 | delay 0 min
biological MSE: all=0.01298, FDG=0.00778, PBR28=0.01818
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

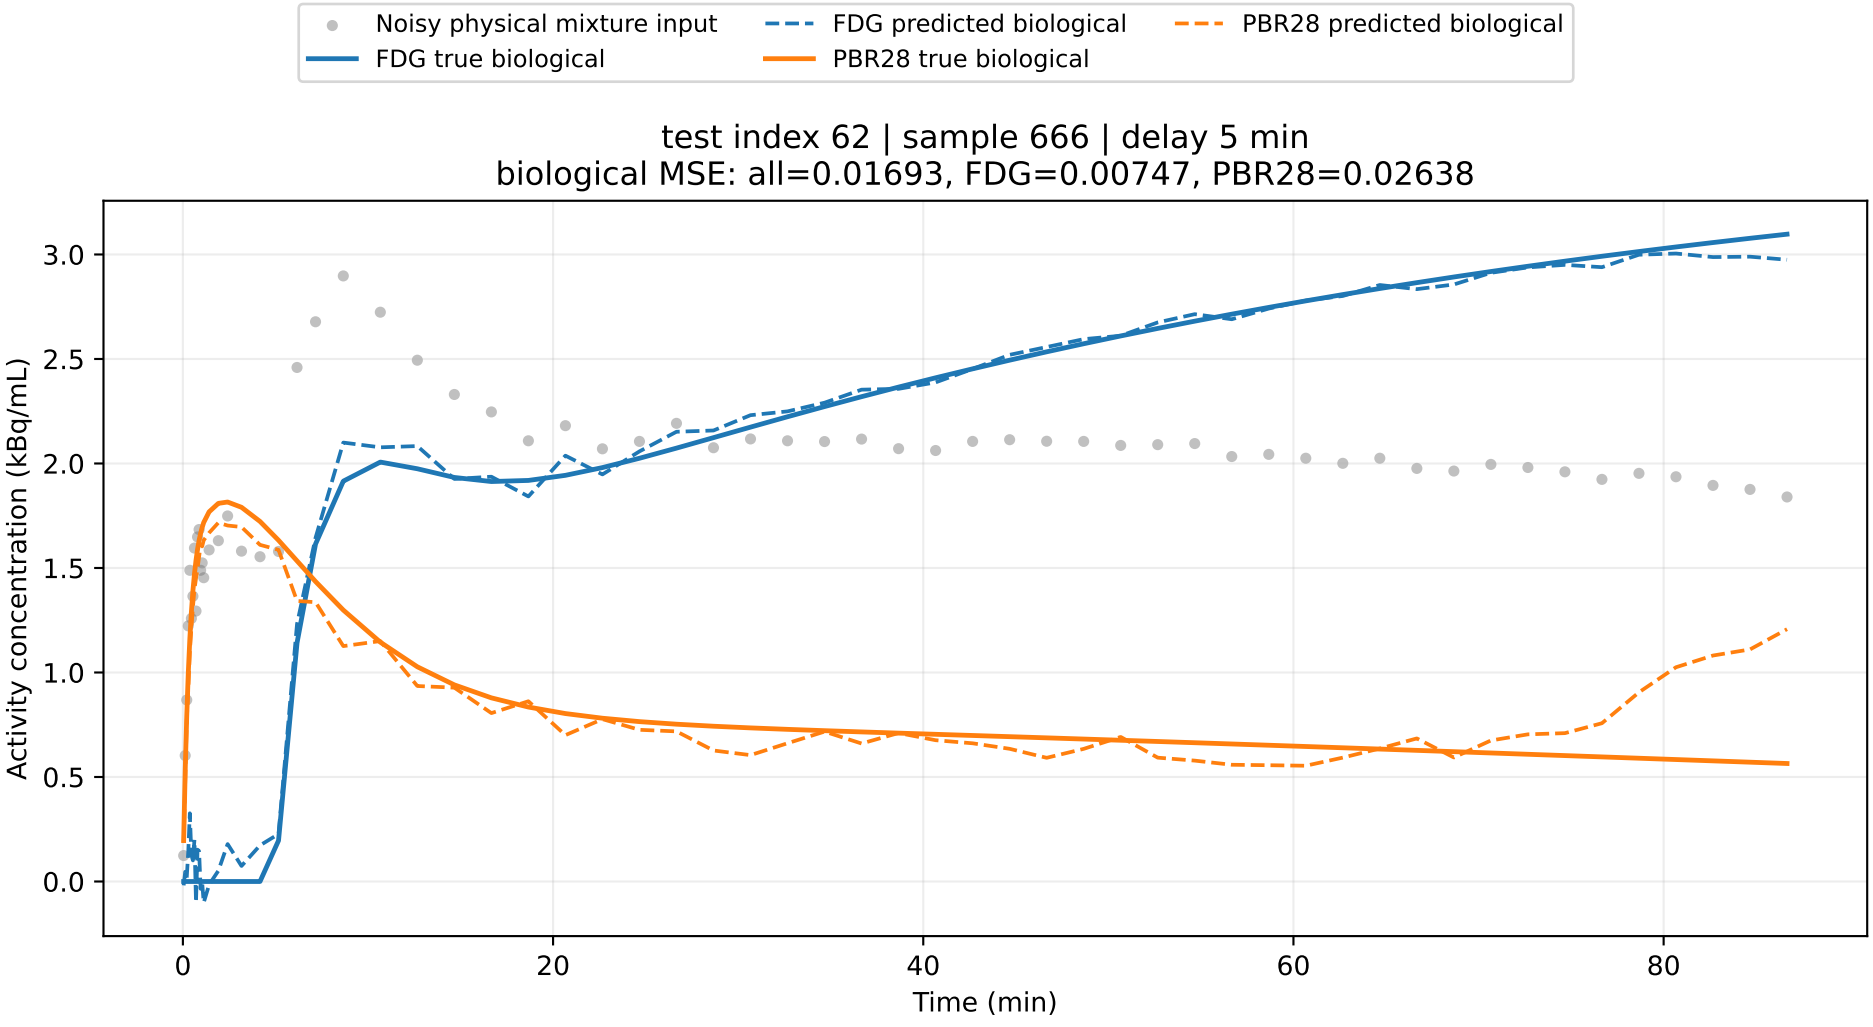

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 57 | sample 40 | delay 5 min
biological MSE: all=0.02342, FDG=0.00515, PBR28=0.04168
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

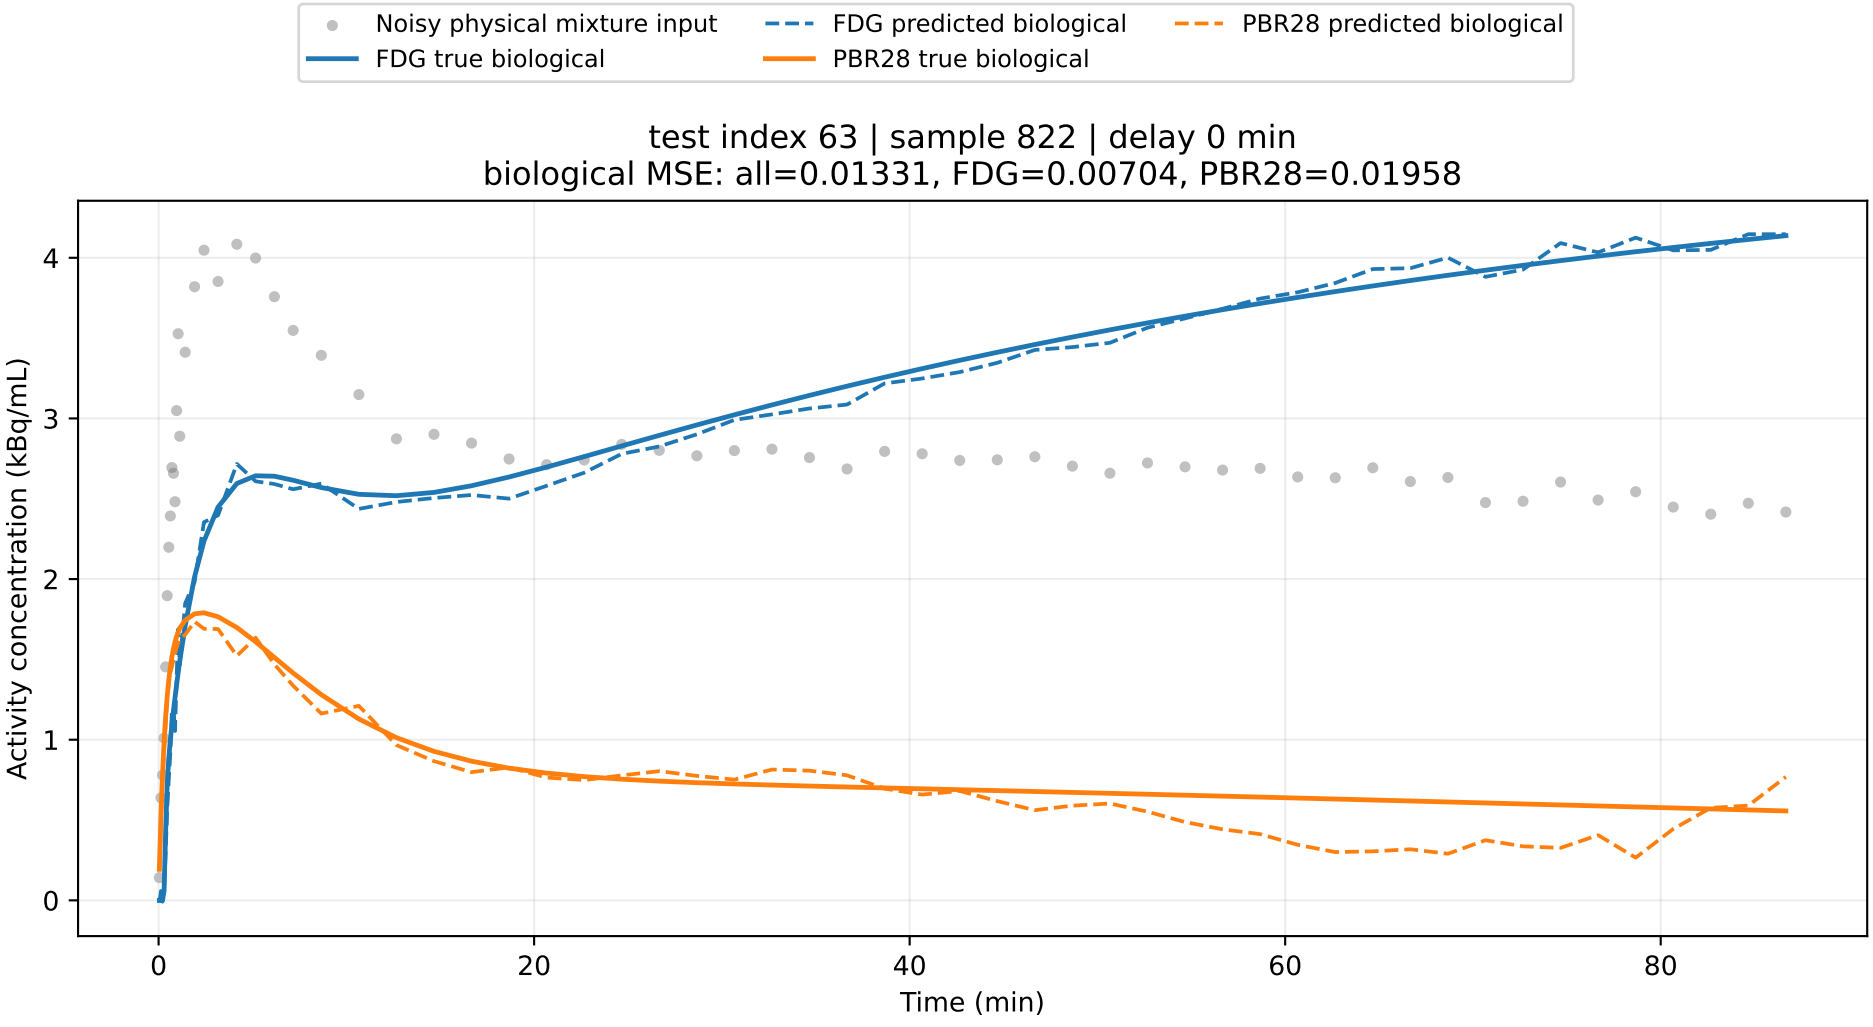

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 58 | sample 67 | delay 5 min
biological MSE: all=0.01278, FDG=0.00529, PBR28=0.02027
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

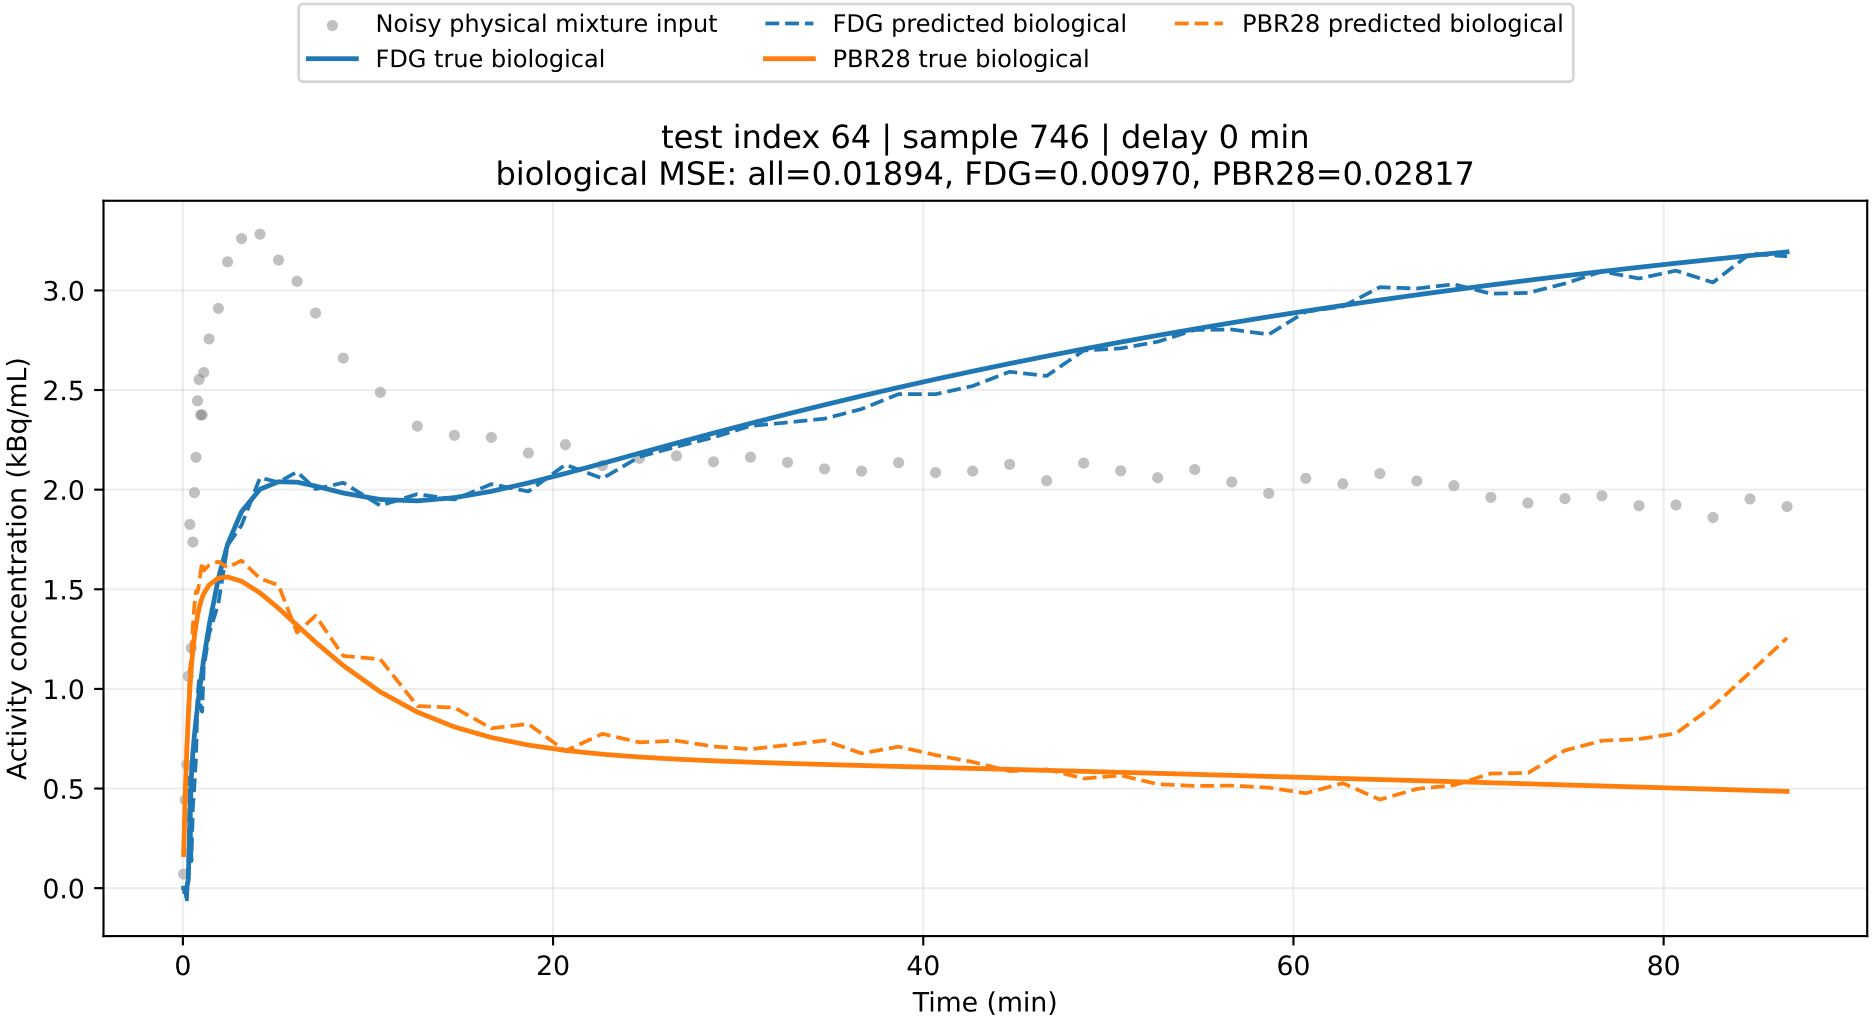

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 59 | sample 259 | delay 0 min
biological MSE: all=0.02563, FDG=0.01216, PBR28=0.03909
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

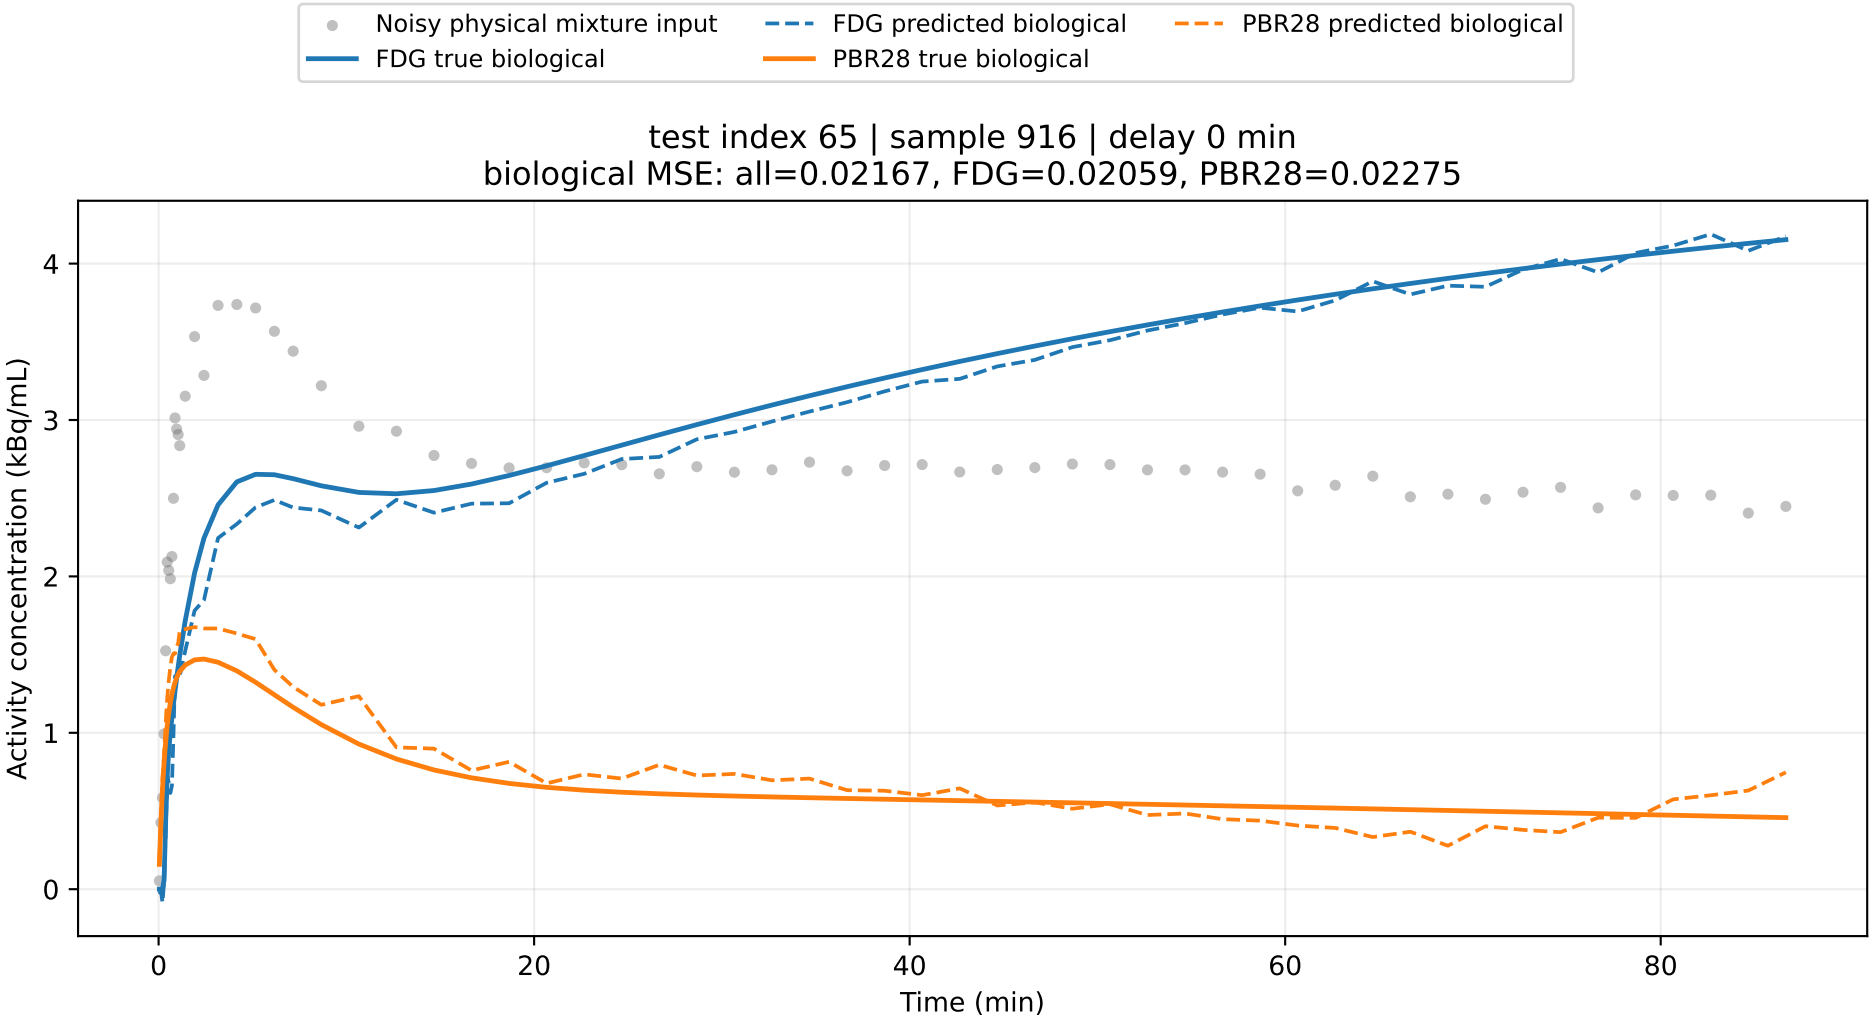

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 60 | sample 34 | delay 5 min
biological MSE: all=0.00739, FDG=0.00543, PBR28=0.00936
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

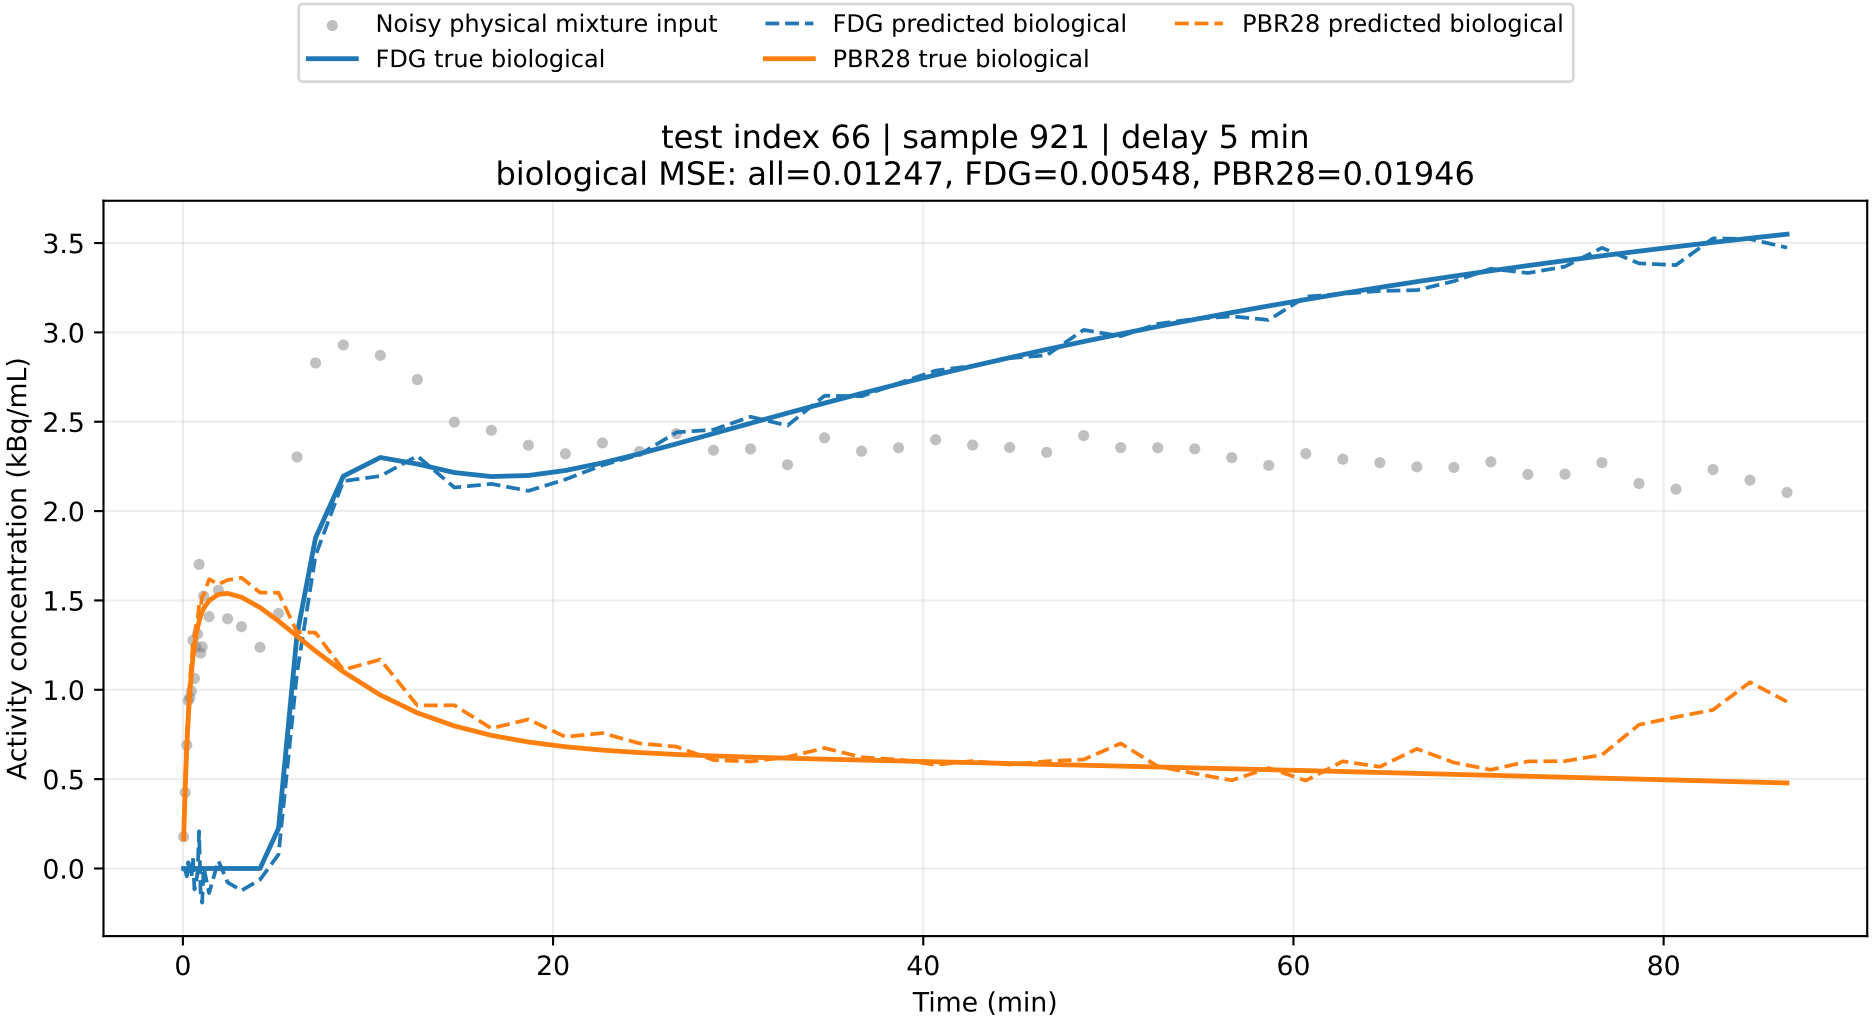

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 61 | sample 460 | delay 0 min
biological MSE: all=0.01963, FDG=0.01819, PBR28=0.02106
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

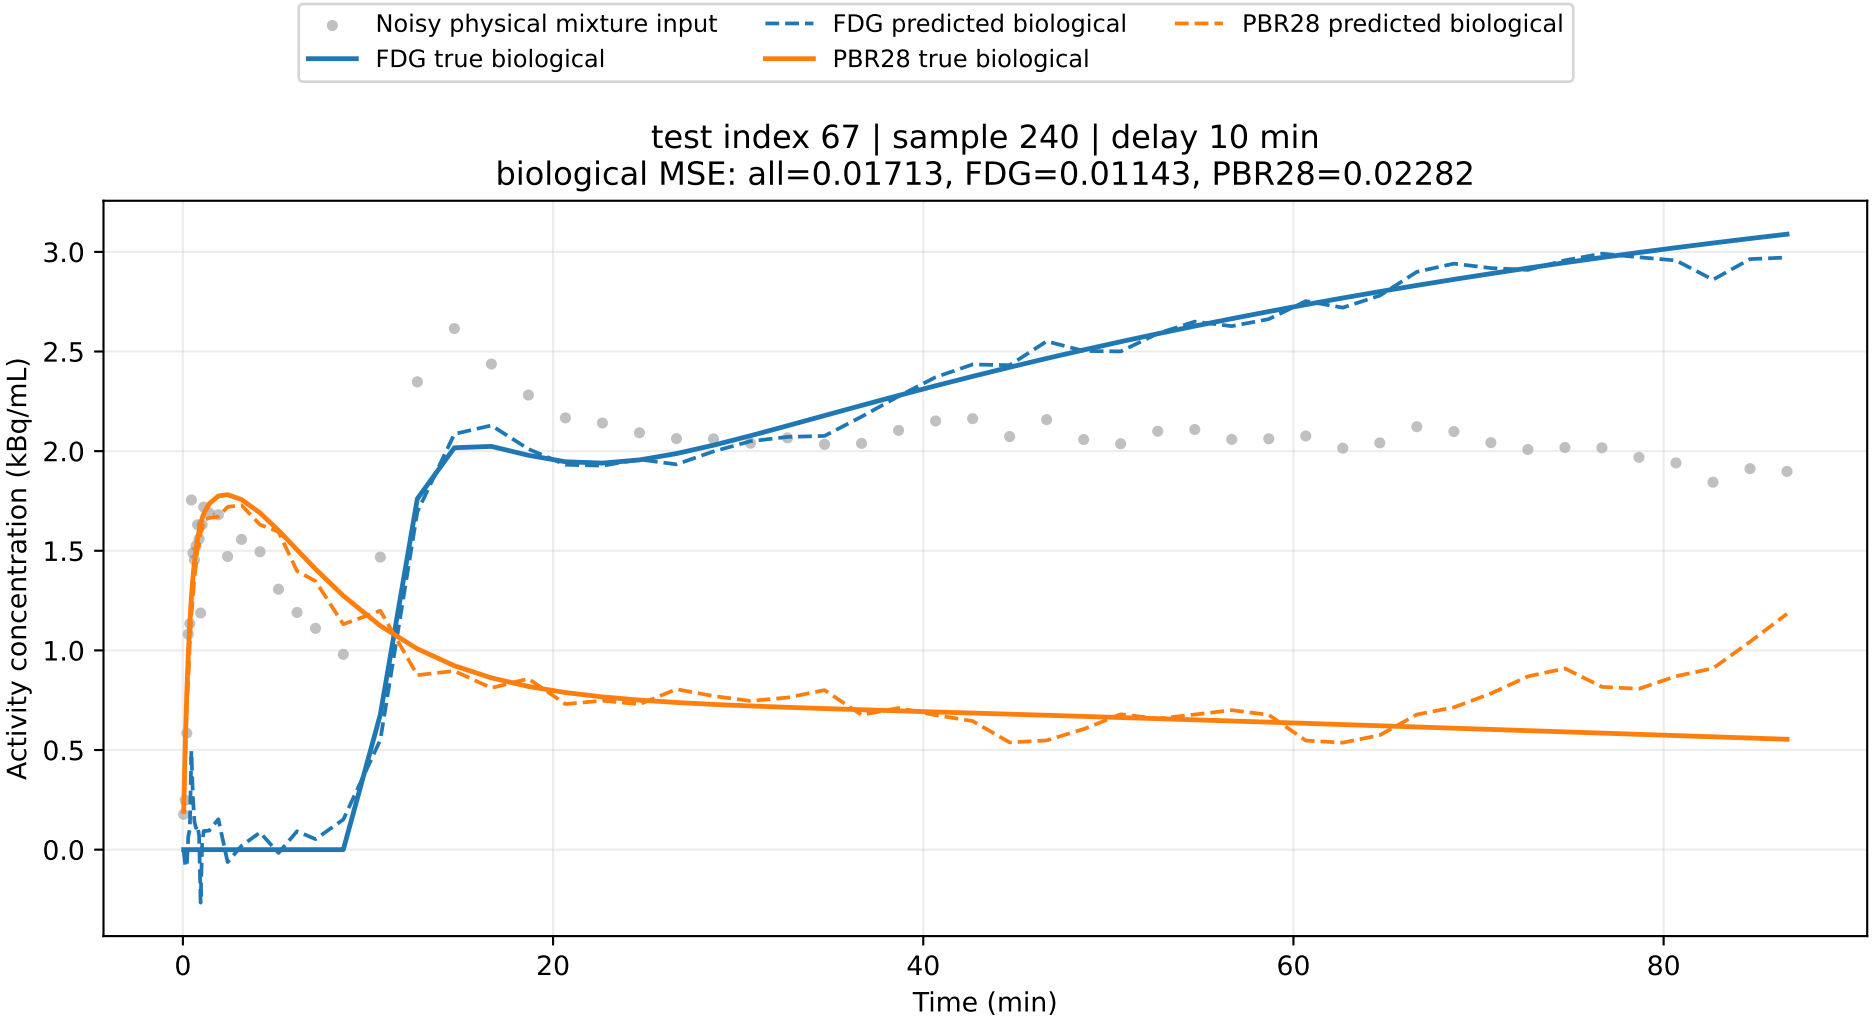

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 62 | sample 666 | delay 5 min
biological MSE: all=0.01693, FDG=0.00747, PBR28=0.02638
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

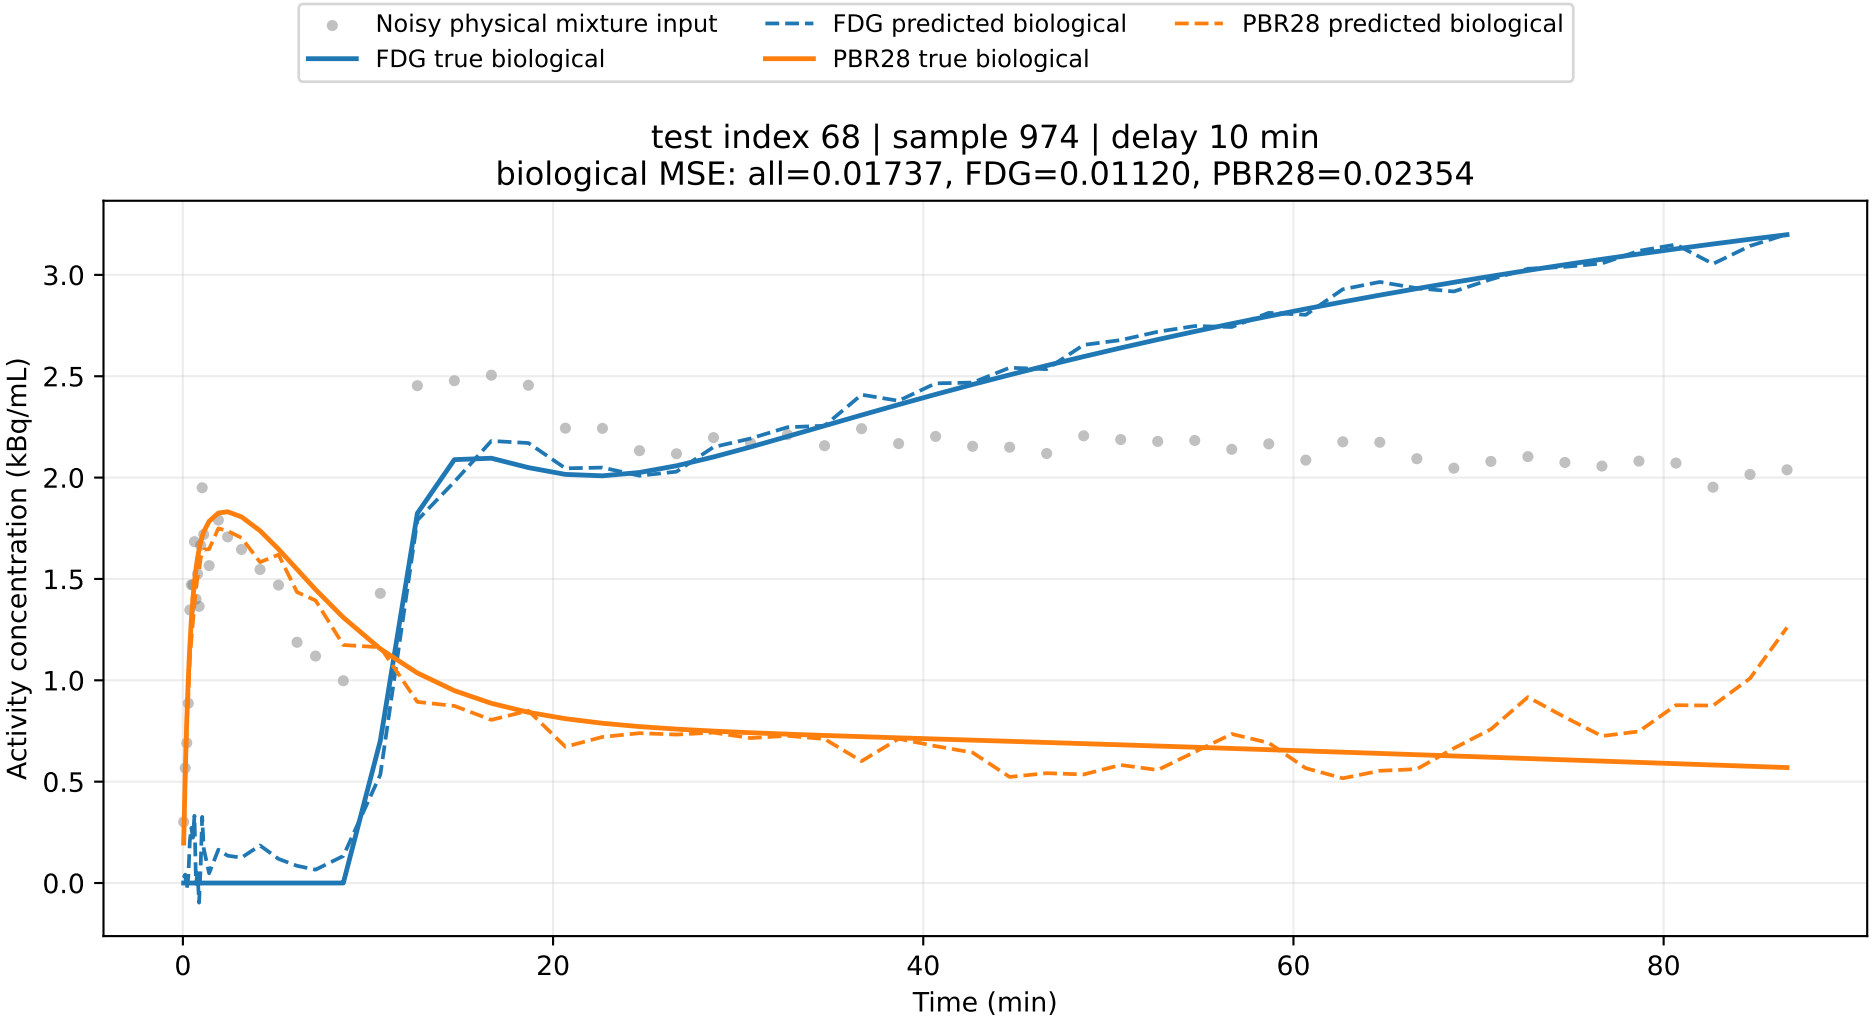

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 63 | sample 822 | delay 0 min
biological MSE: all=0.01331, FDG=0.00704, PBR28=0.01958
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

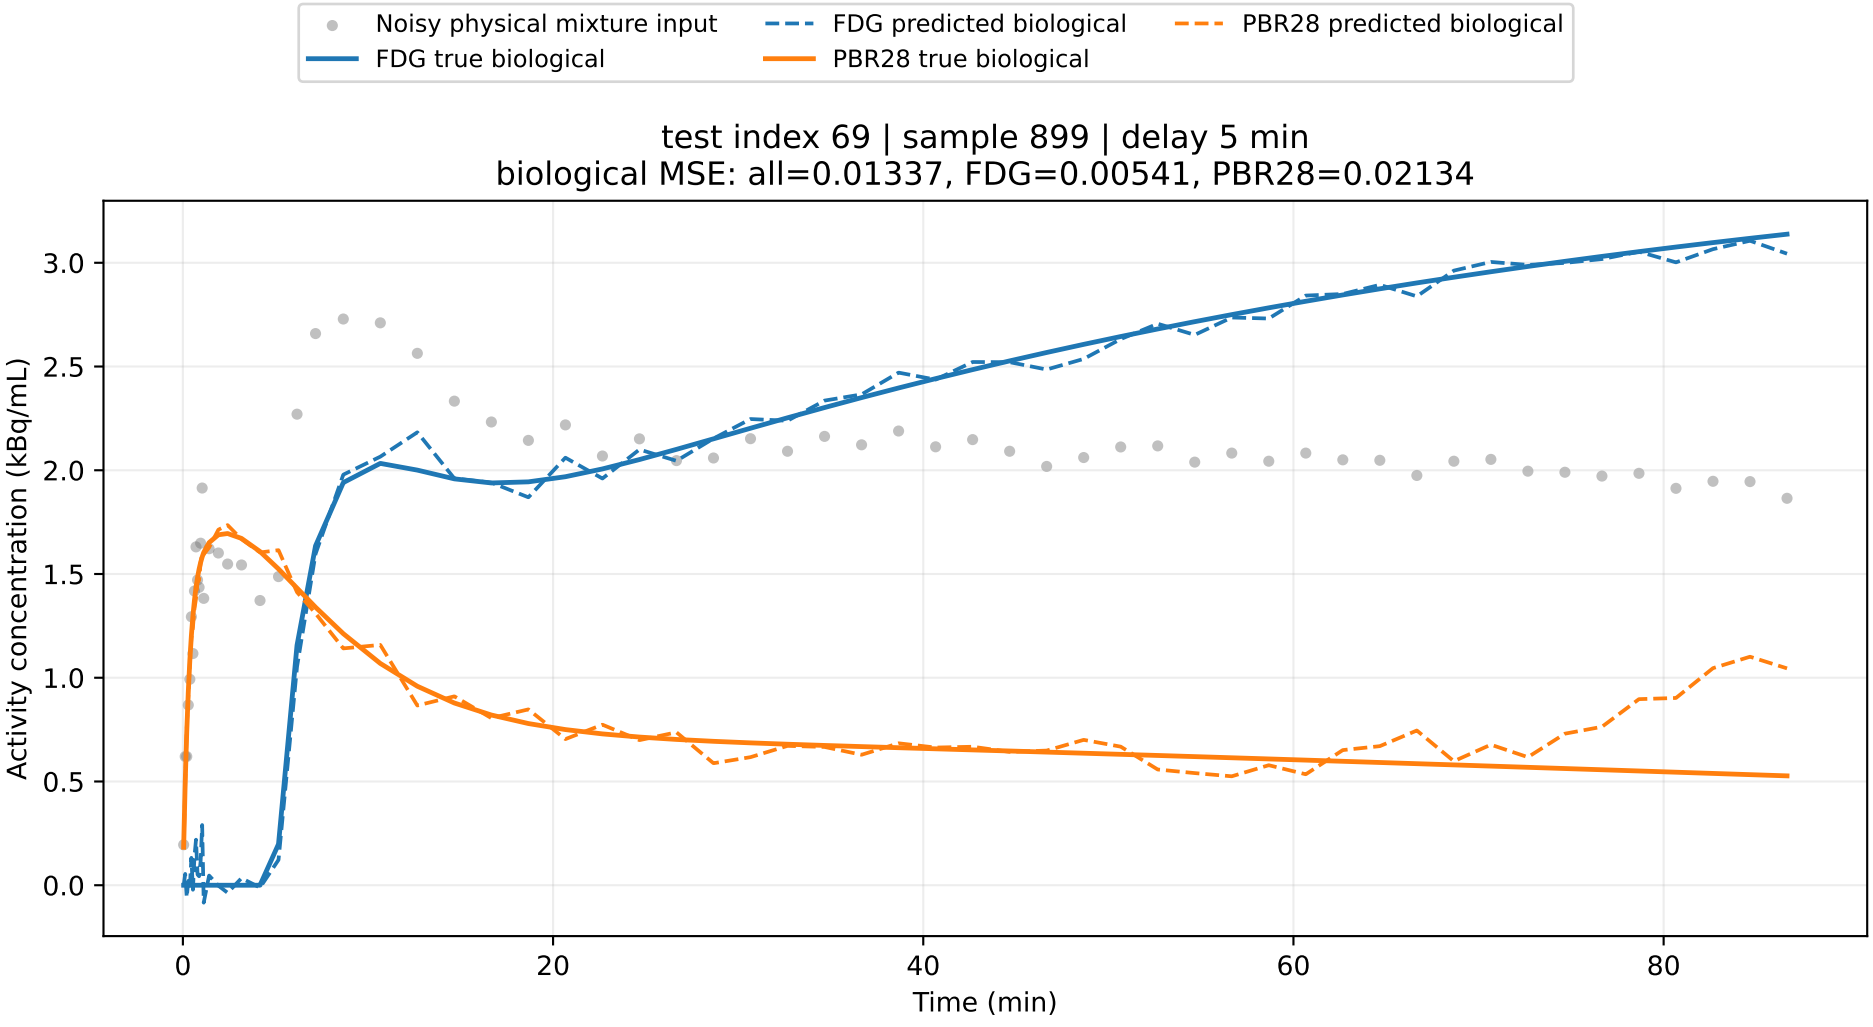

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 64 | sample 746 | delay 0 min
biological MSE: all=0.01894, FDG=0.00970, PBR28=0.02817
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

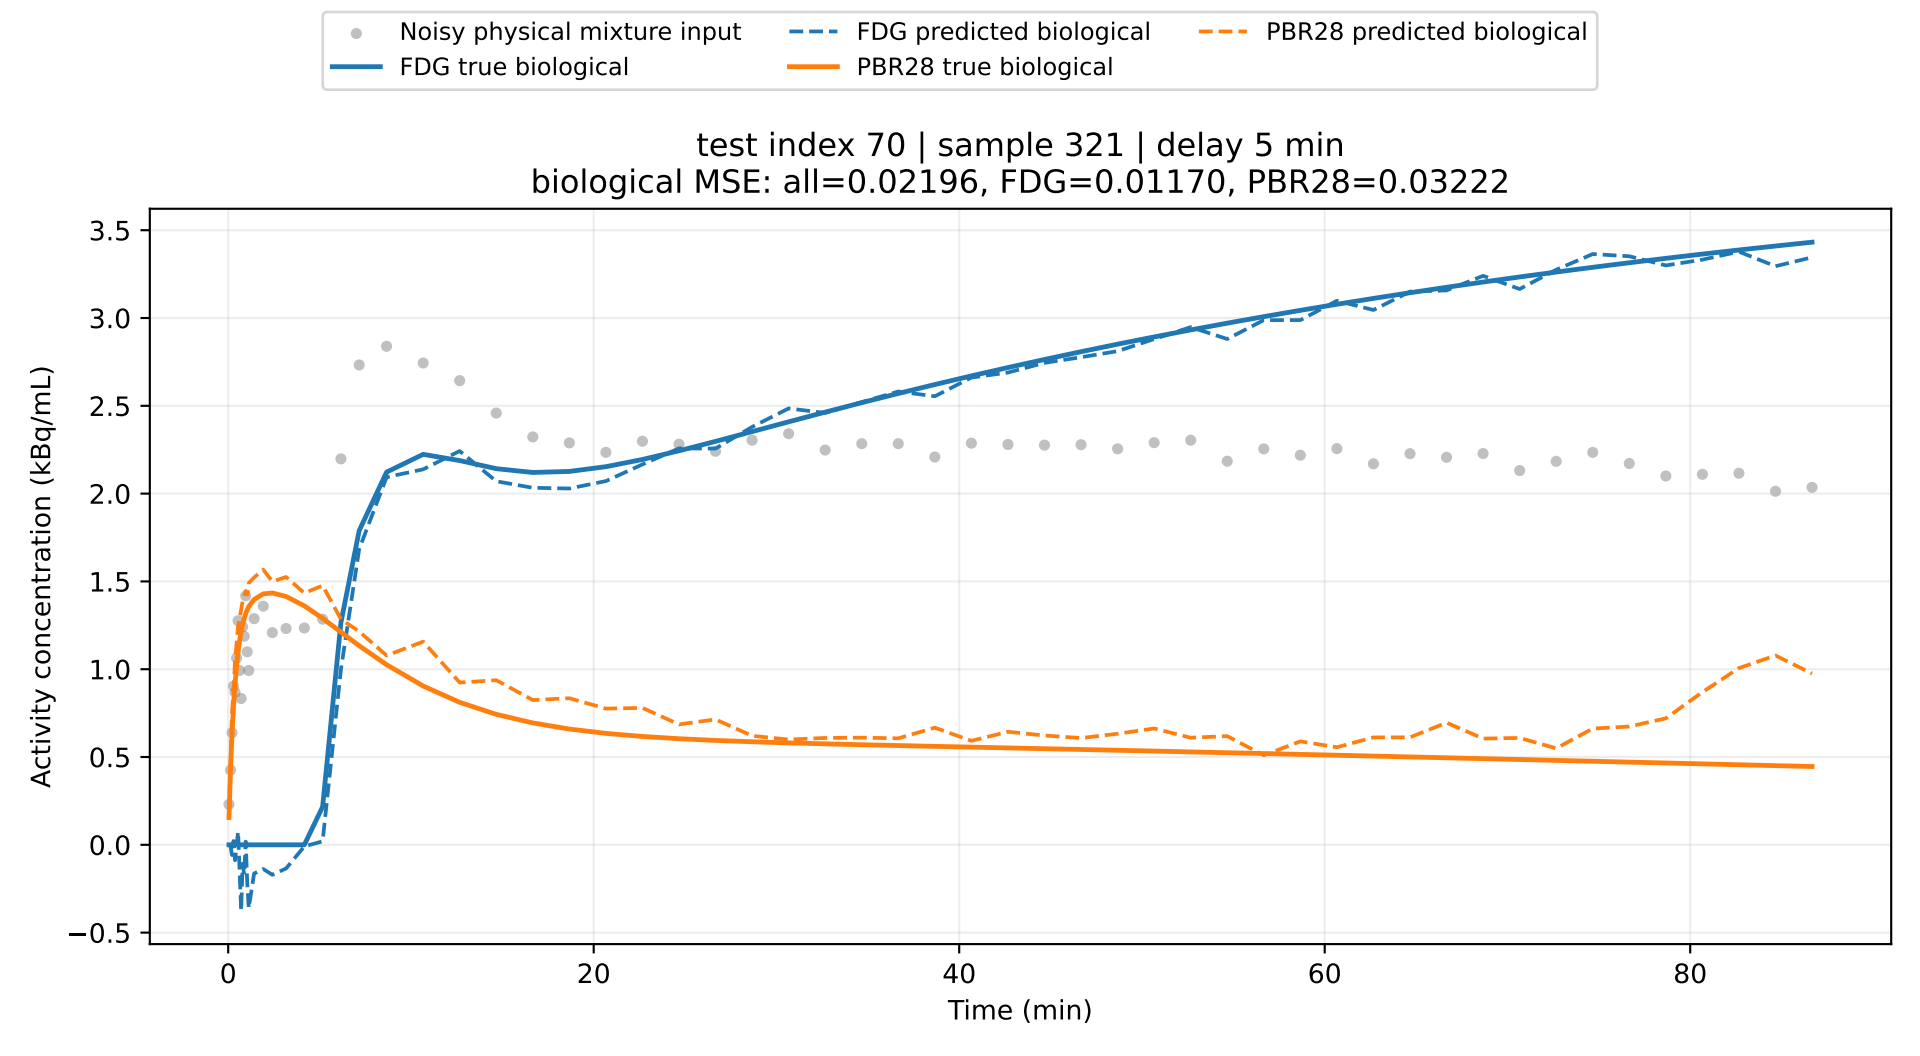

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 65 | sample 916 | delay 0 min
biological MSE: all=0.02167, FDG=0.02059, PBR28=0.02275
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

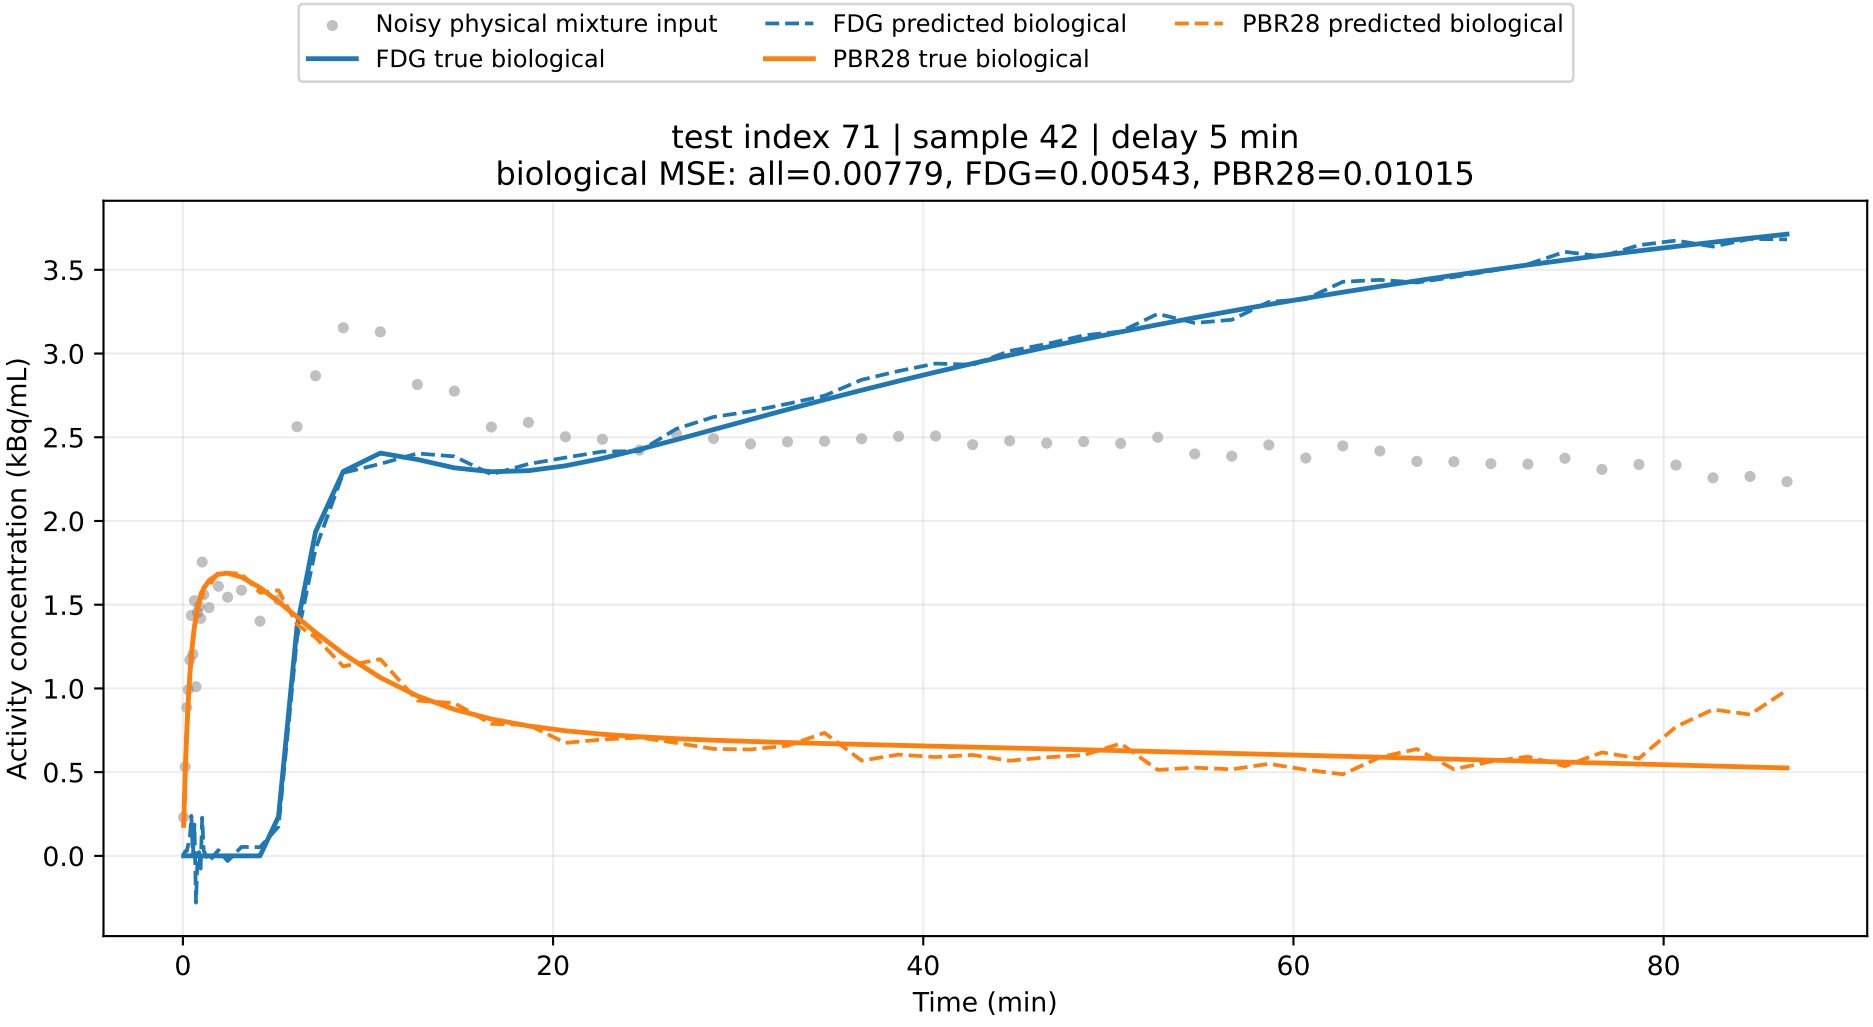

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 66 | sample 921 | delay 5 min
biological MSE: all=0.01247, FDG=0.00548, PBR28=0.01946
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

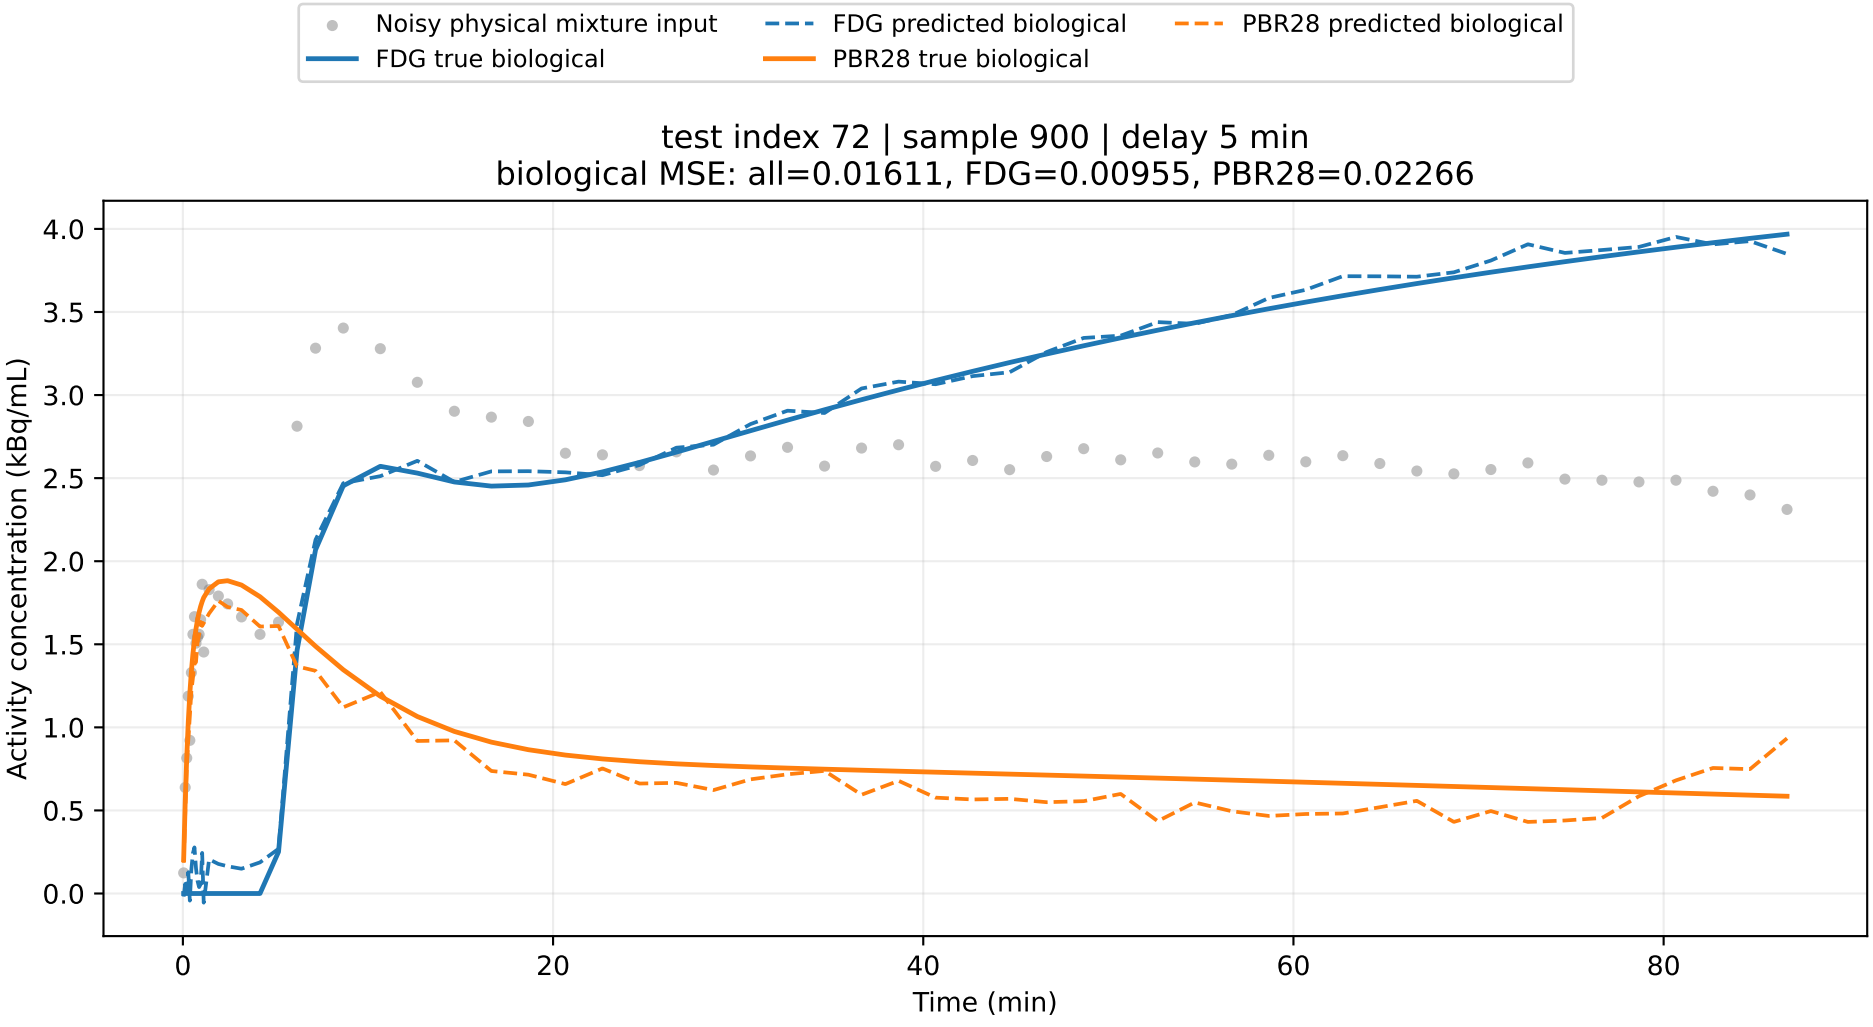

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 67 | sample 240 | delay 10 min
biological MSE: all=0.01713, FDG=0.01143, PBR28=0.02282
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

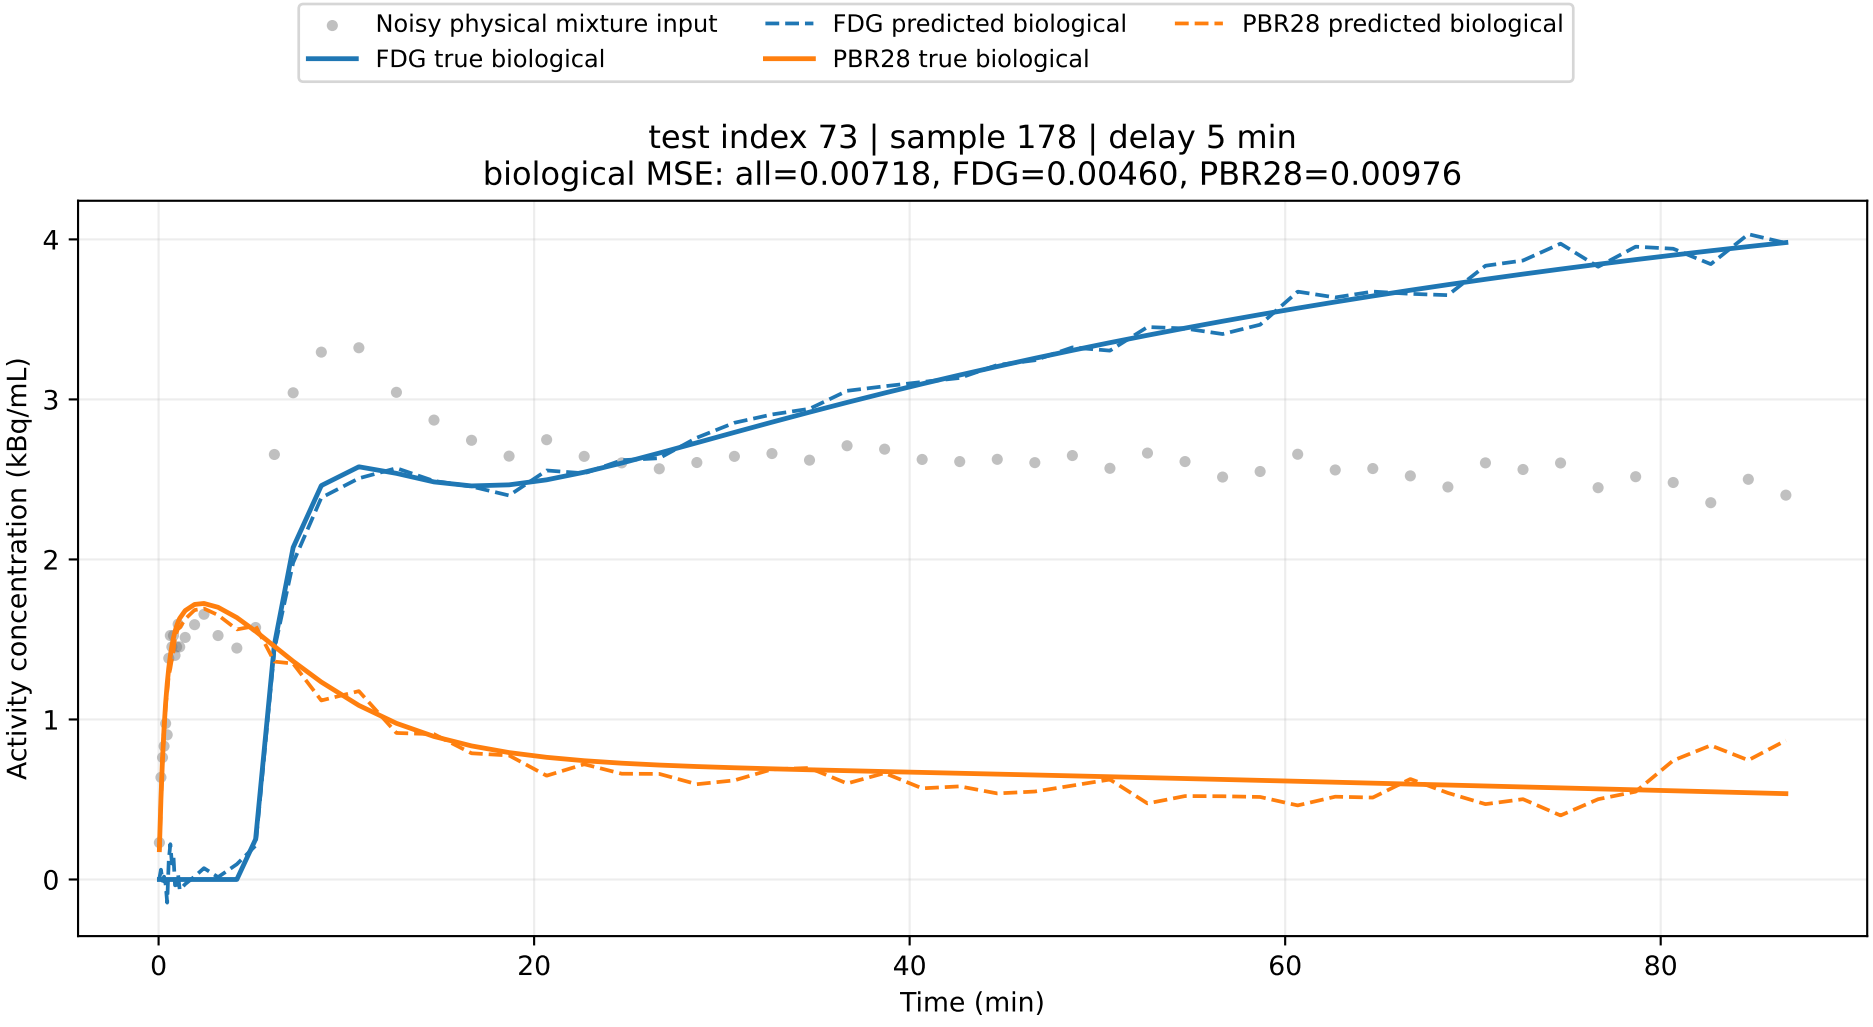

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 68 | sample 974 | delay 10 min
biological MSE: all=0.01737, FDG=0.01120, PBR28=0.02354
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

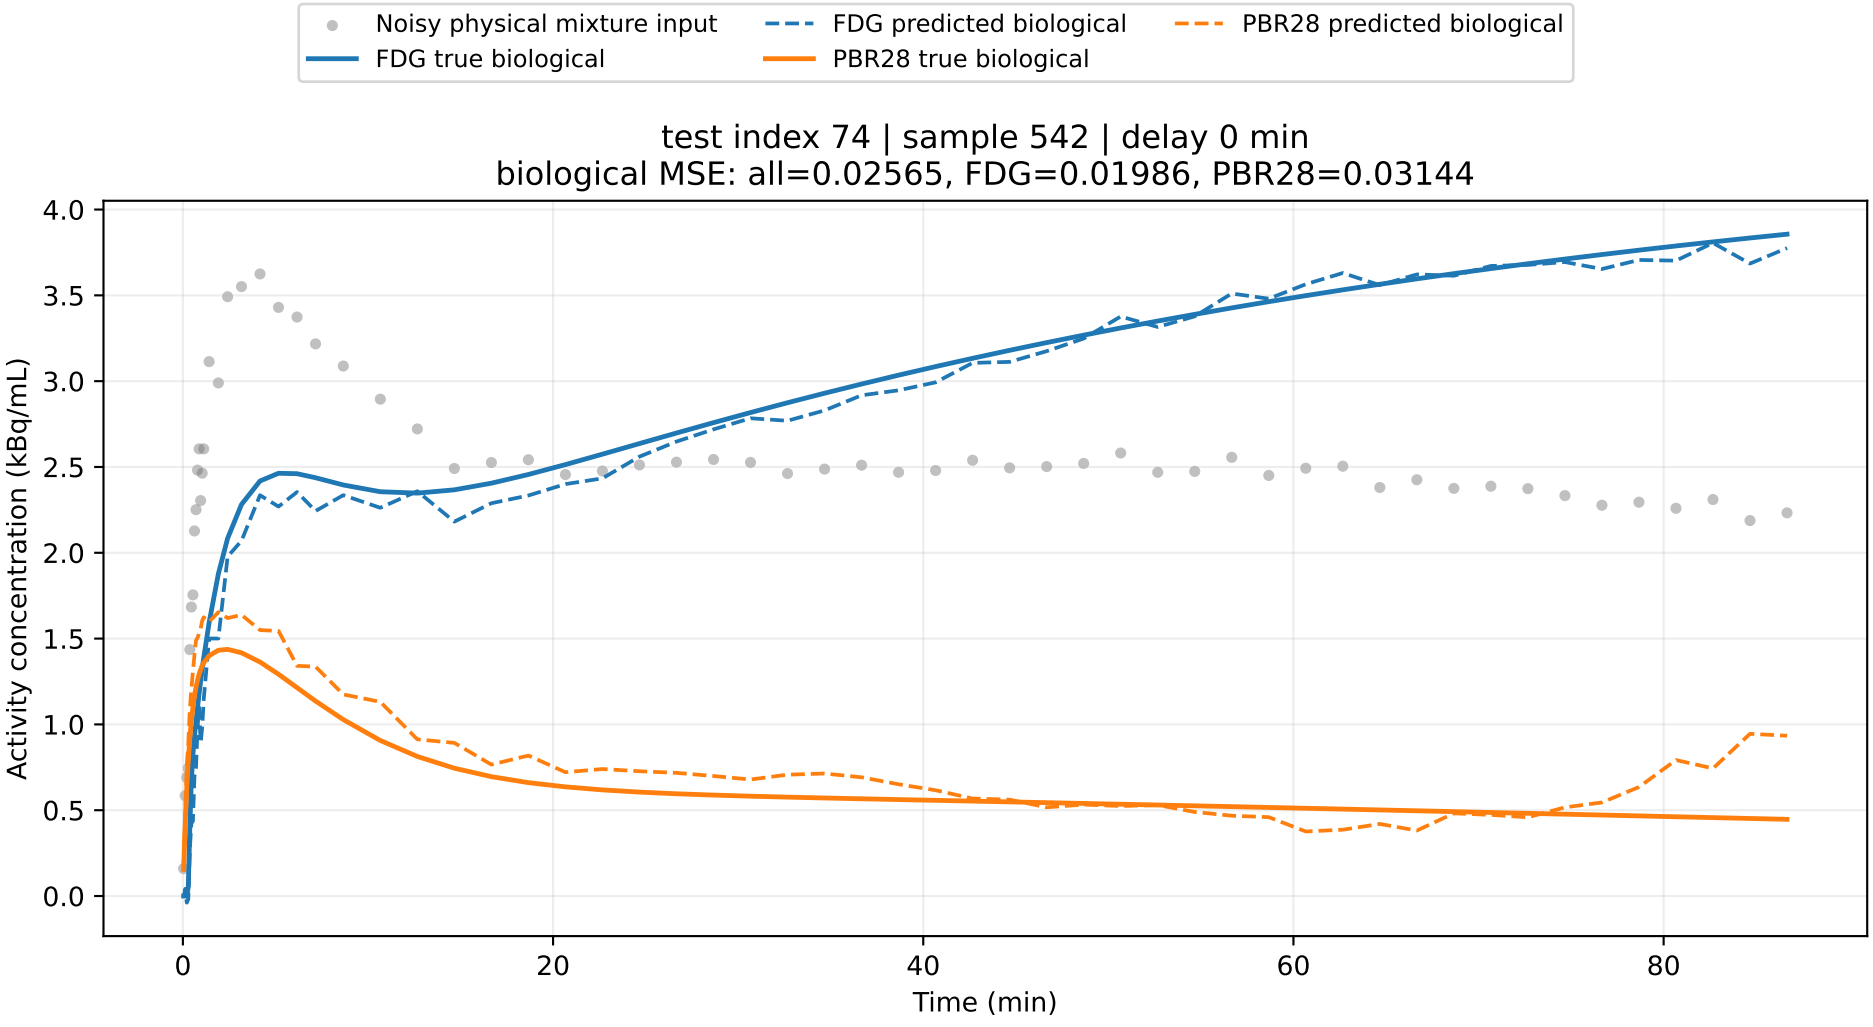

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 69 | sample 899 | delay 5 min
biological MSE: all=0.01337, FDG=0.00541, PBR28=0.02134
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

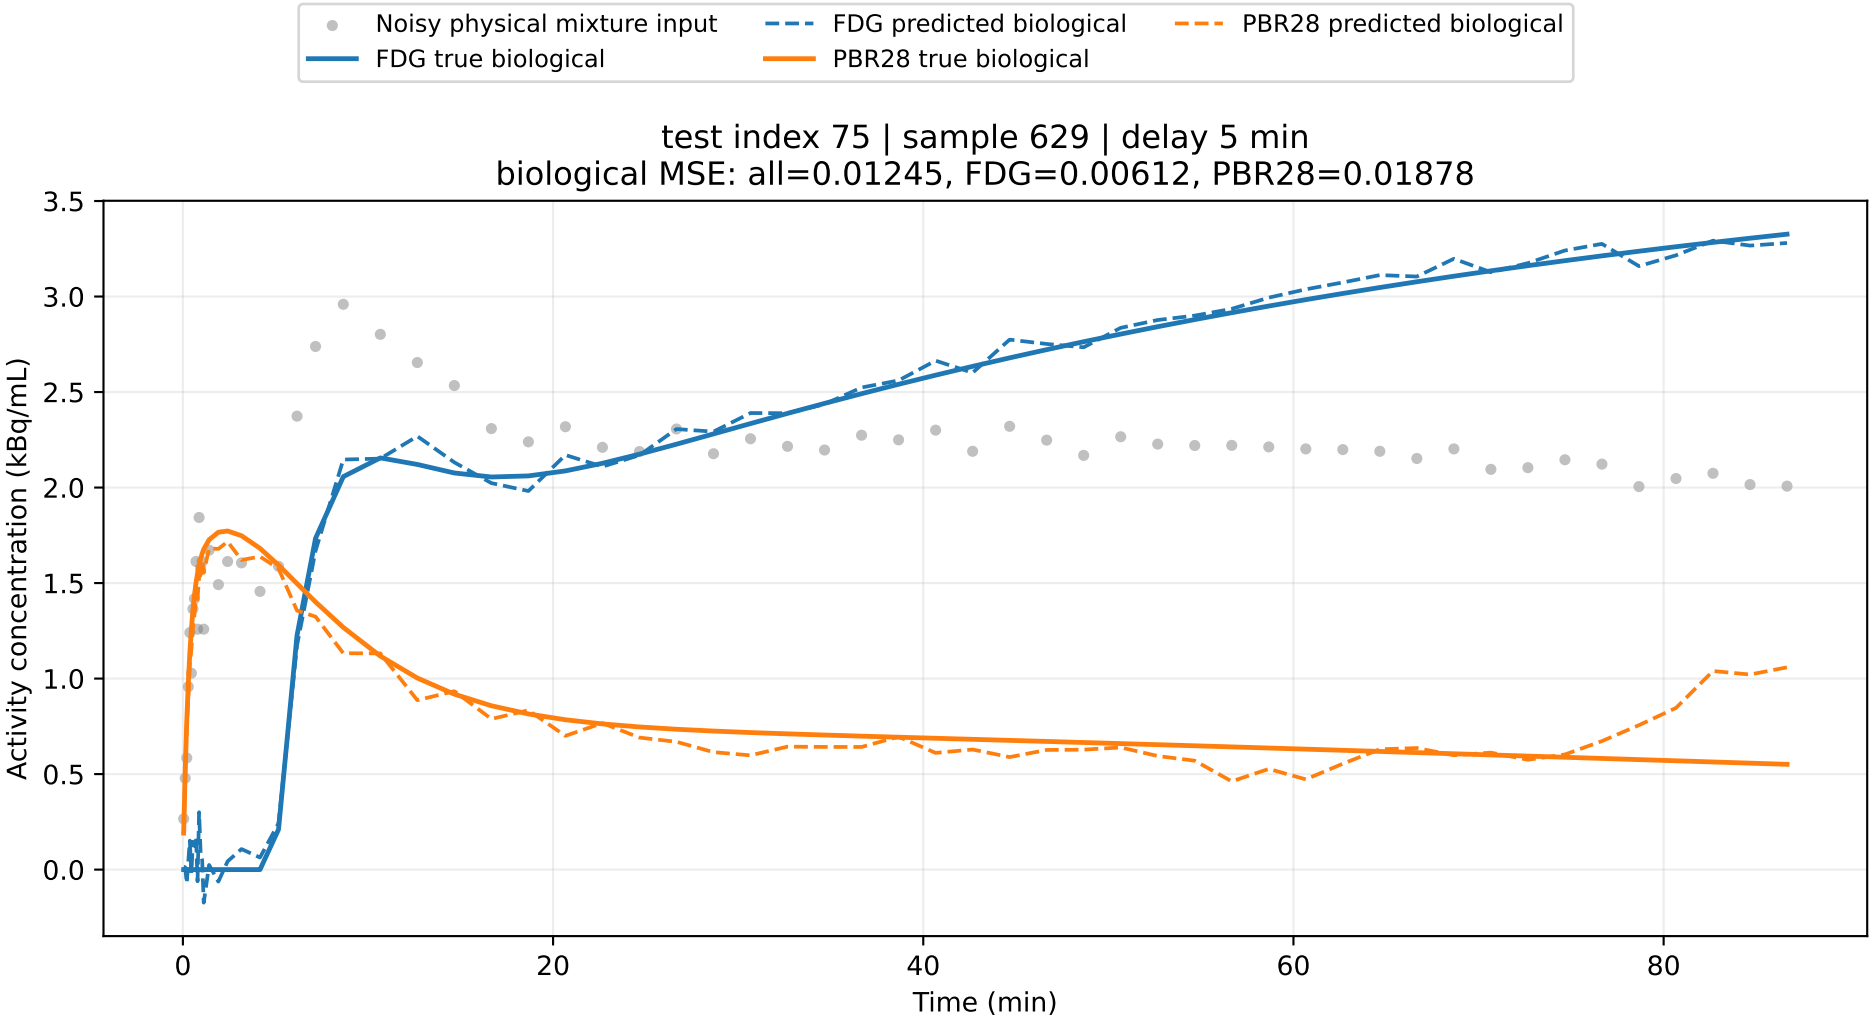

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 70 | sample 321 | delay 5 min
biological MSE: all=0.02196, FDG=0.01170, PBR28=0.03222
Activity concentration (kBq/mL)
Time (min)
3.5
3.0
2.5
2.0
1.5
1.0
0.5
0.0
−0.5
0
20
40
60
80

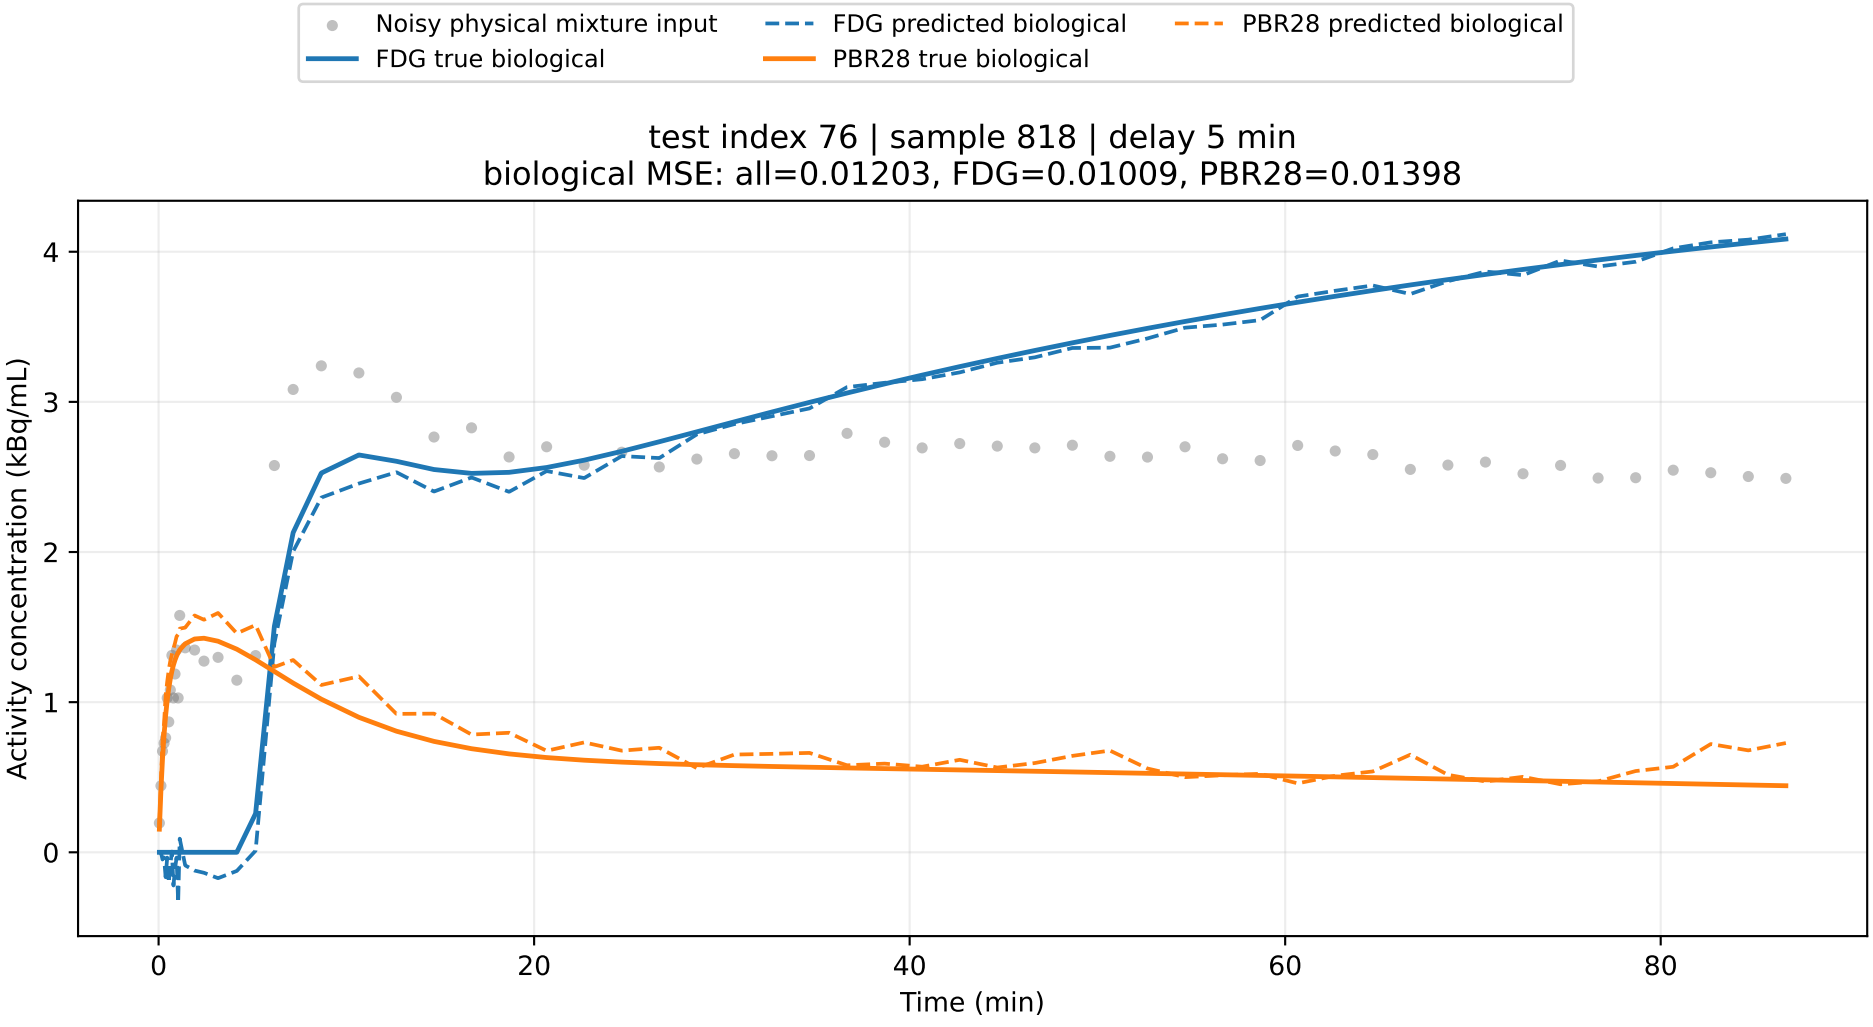

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 71 | sample 42 | delay 5 min
biological MSE: all=0.00779, FDG=0.00543, PBR28=0.01015
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

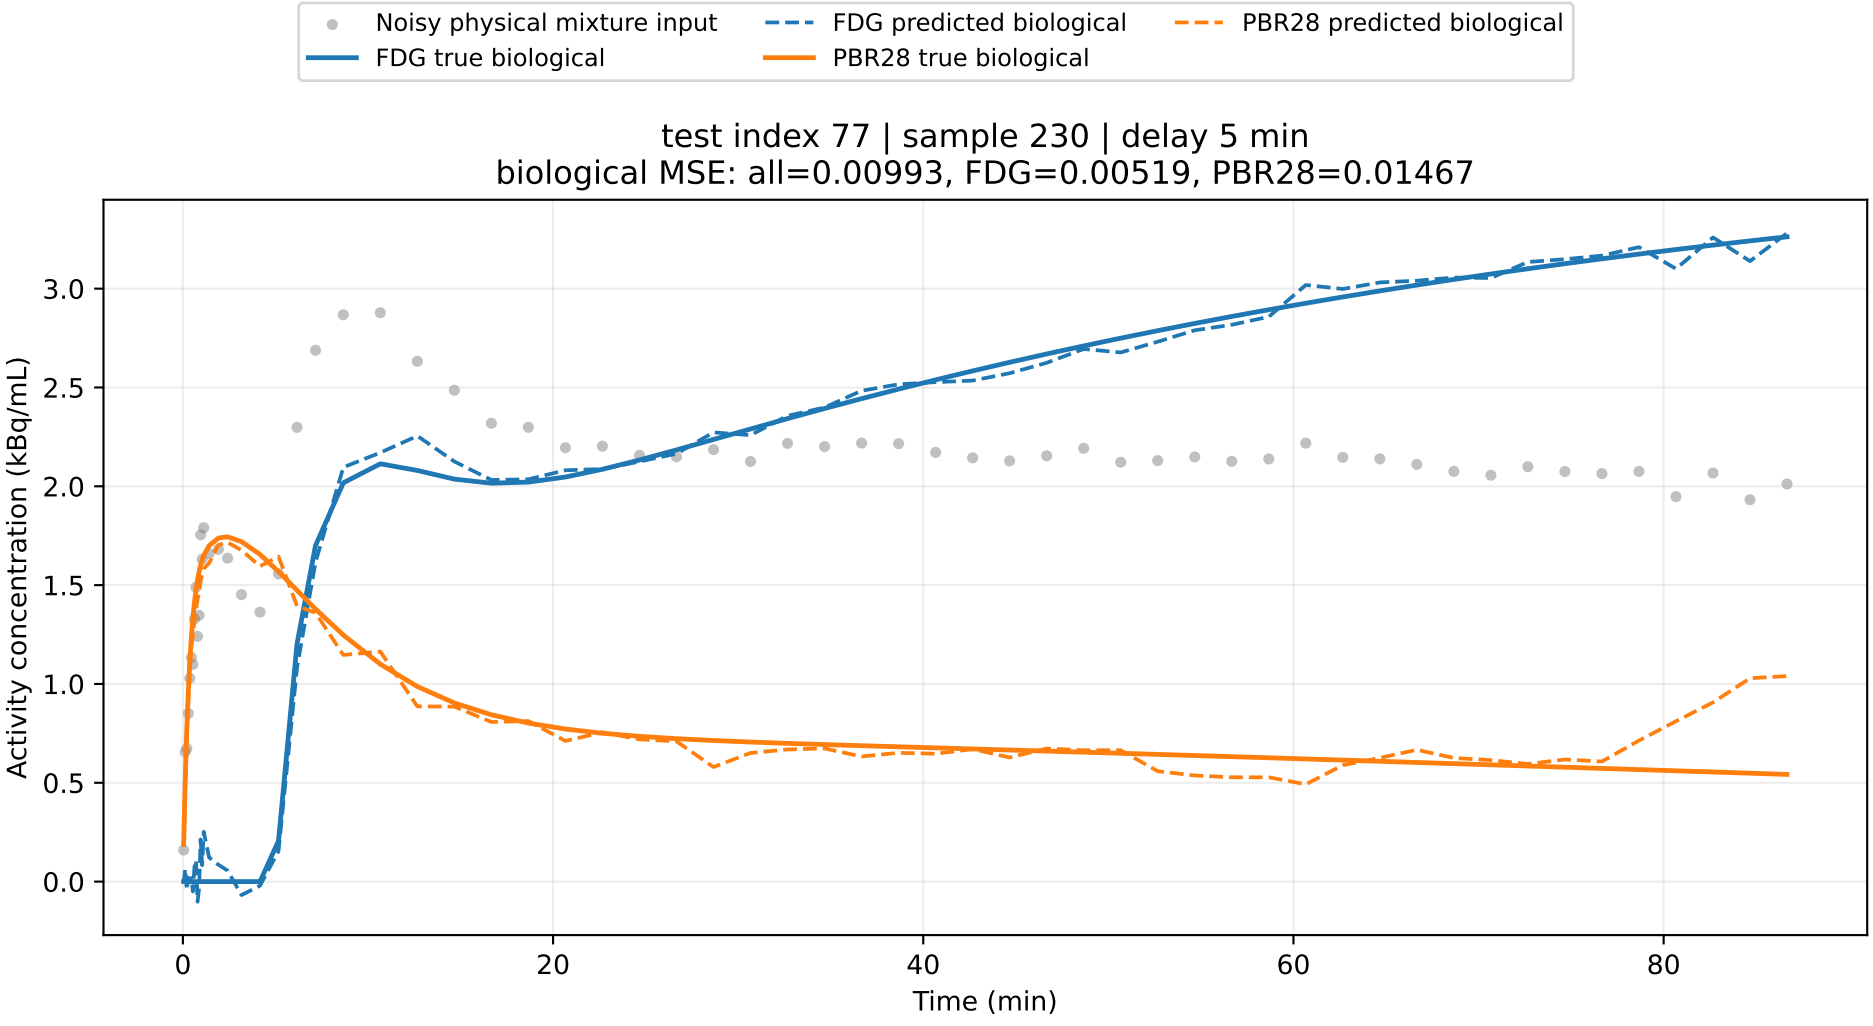

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 72 | sample 900 | delay 5 min
biological MSE: all=0.01611, FDG=0.00955, PBR28=0.02266
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

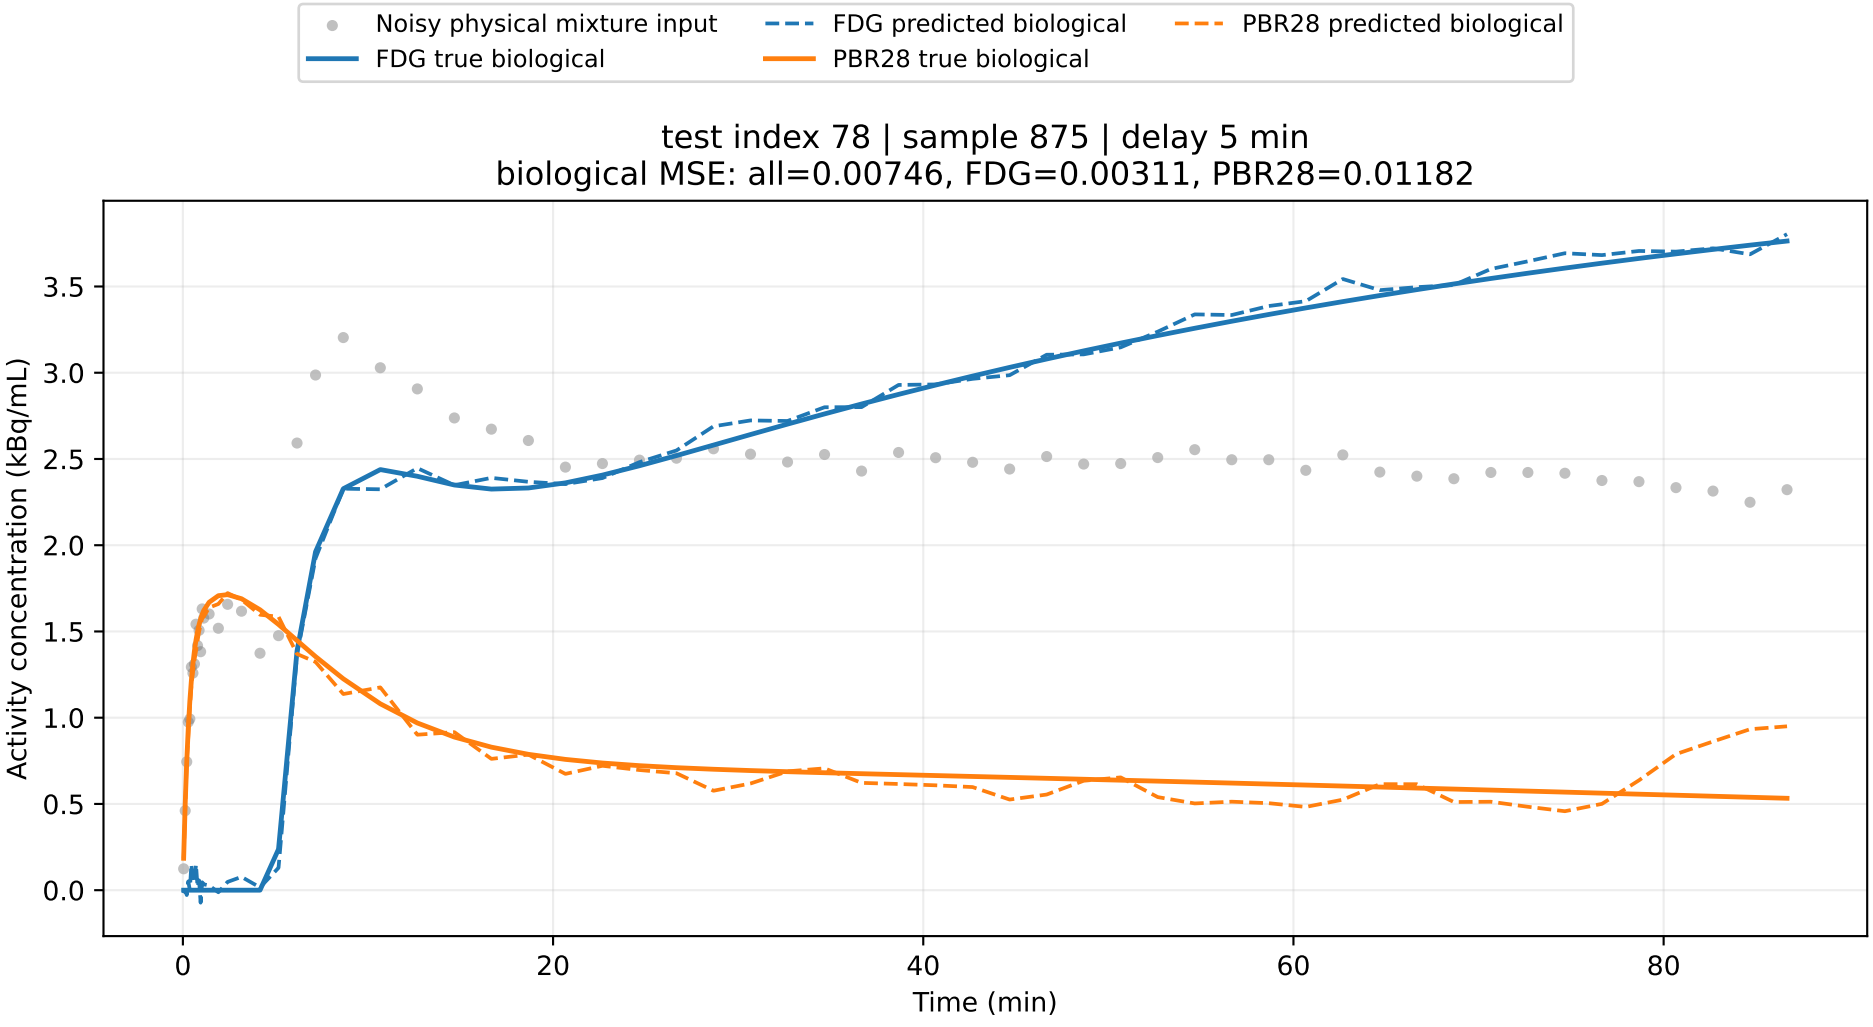

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 73 | sample 178 | delay 5 min
biological MSE: all=0.00718, FDG=0.00460, PBR28=0.00976
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

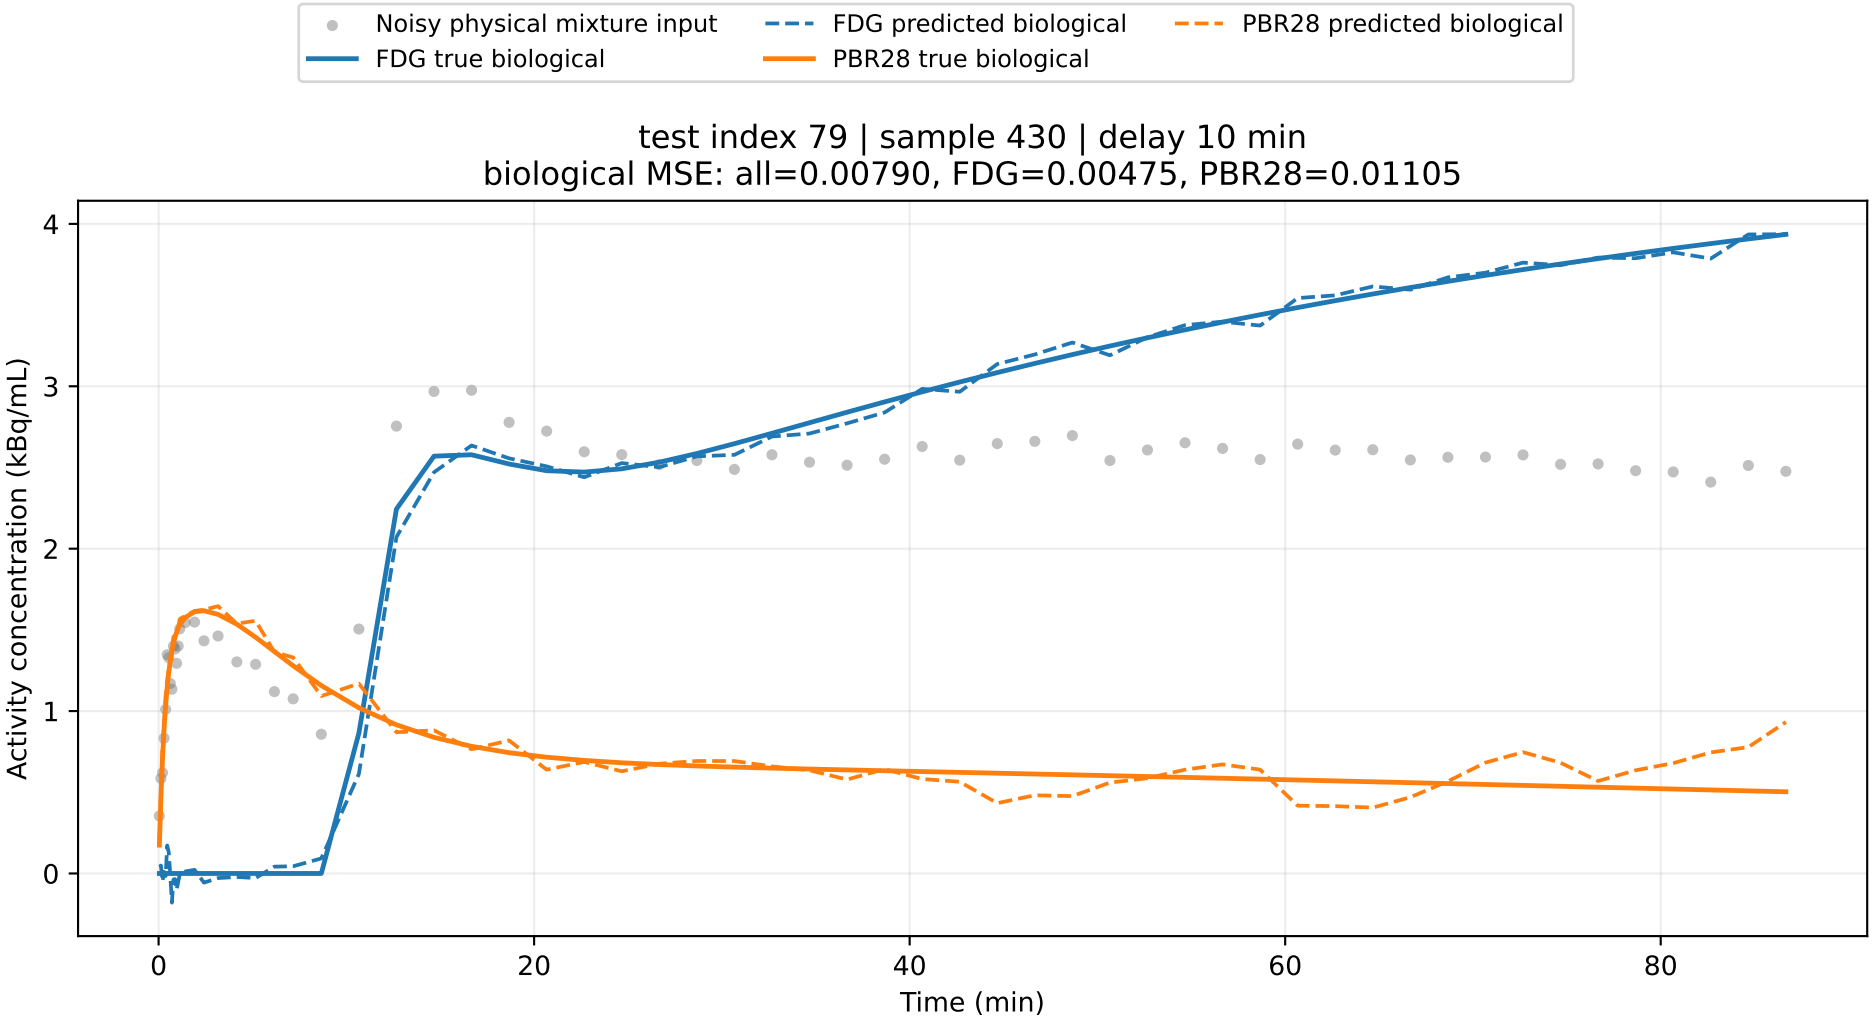

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 74 | sample 542 | delay 0 min
biological MSE: all=0.02565, FDG=0.01986, PBR28=0.03144
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

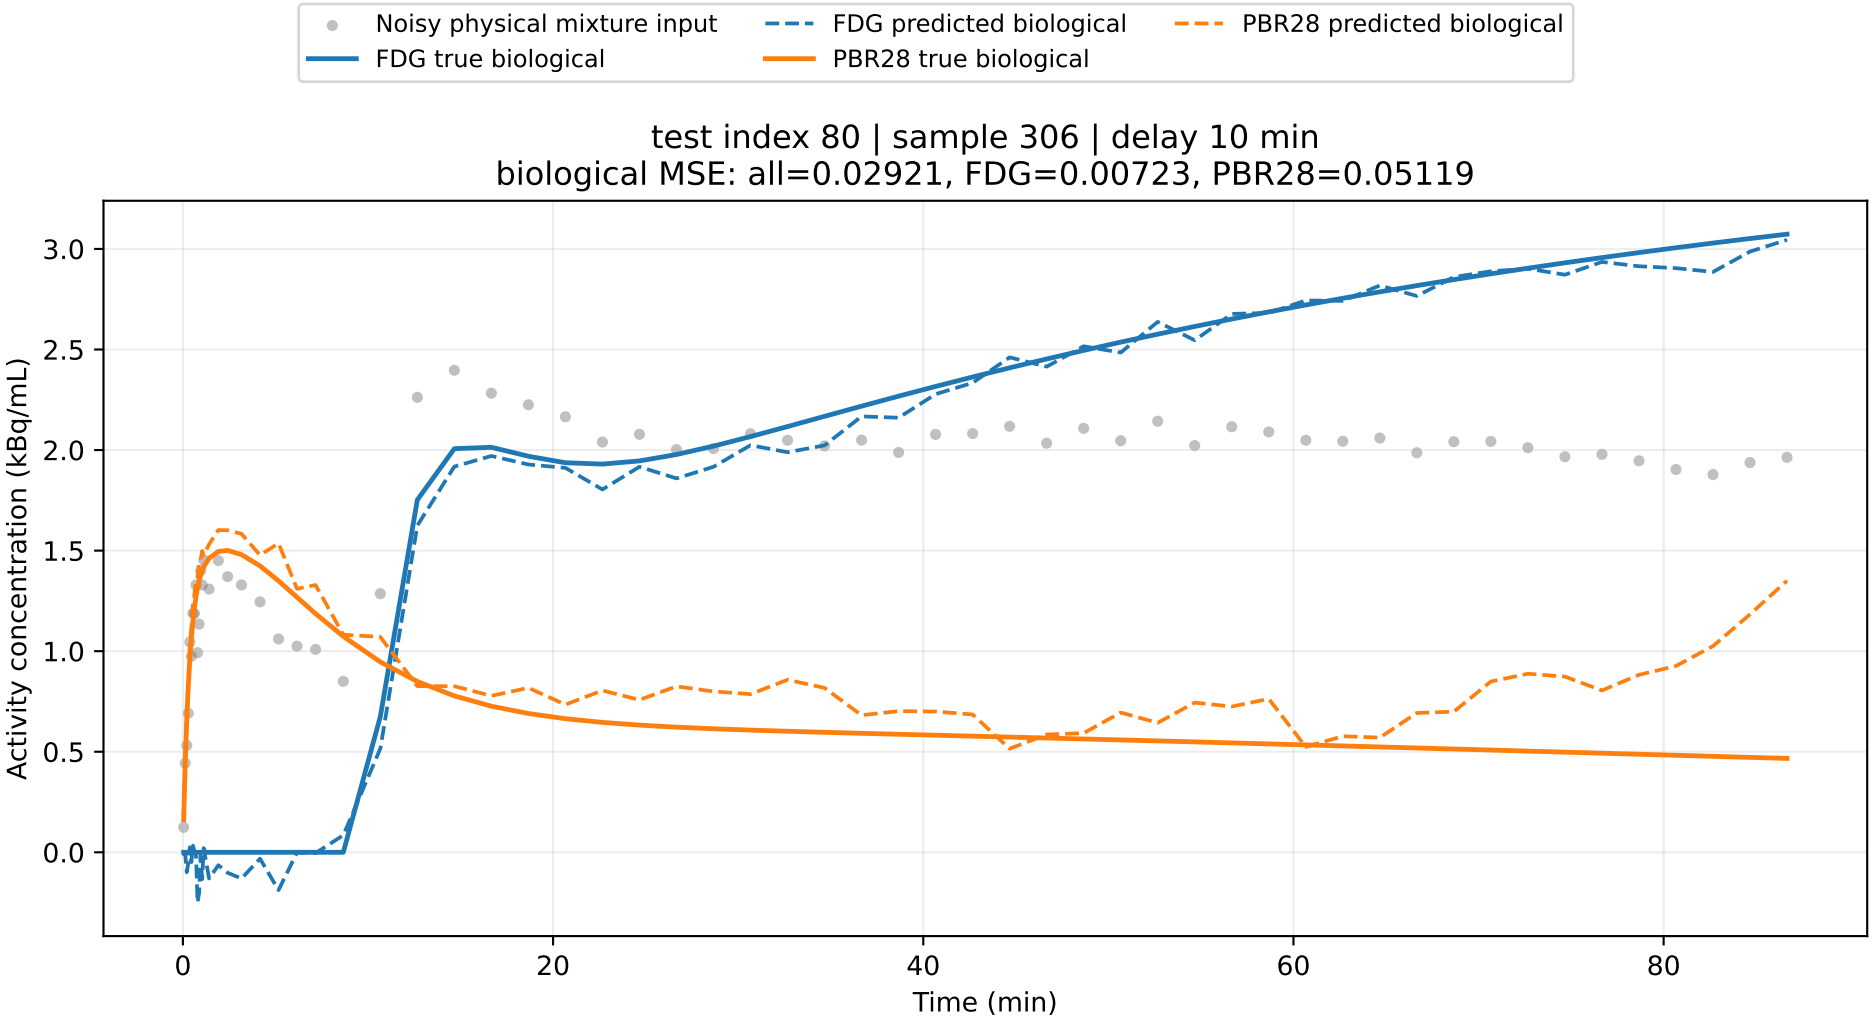

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 75 | sample 629 | delay 5 min
biological MSE: all=0.01245, FDG=0.00612, PBR28=0.01878
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

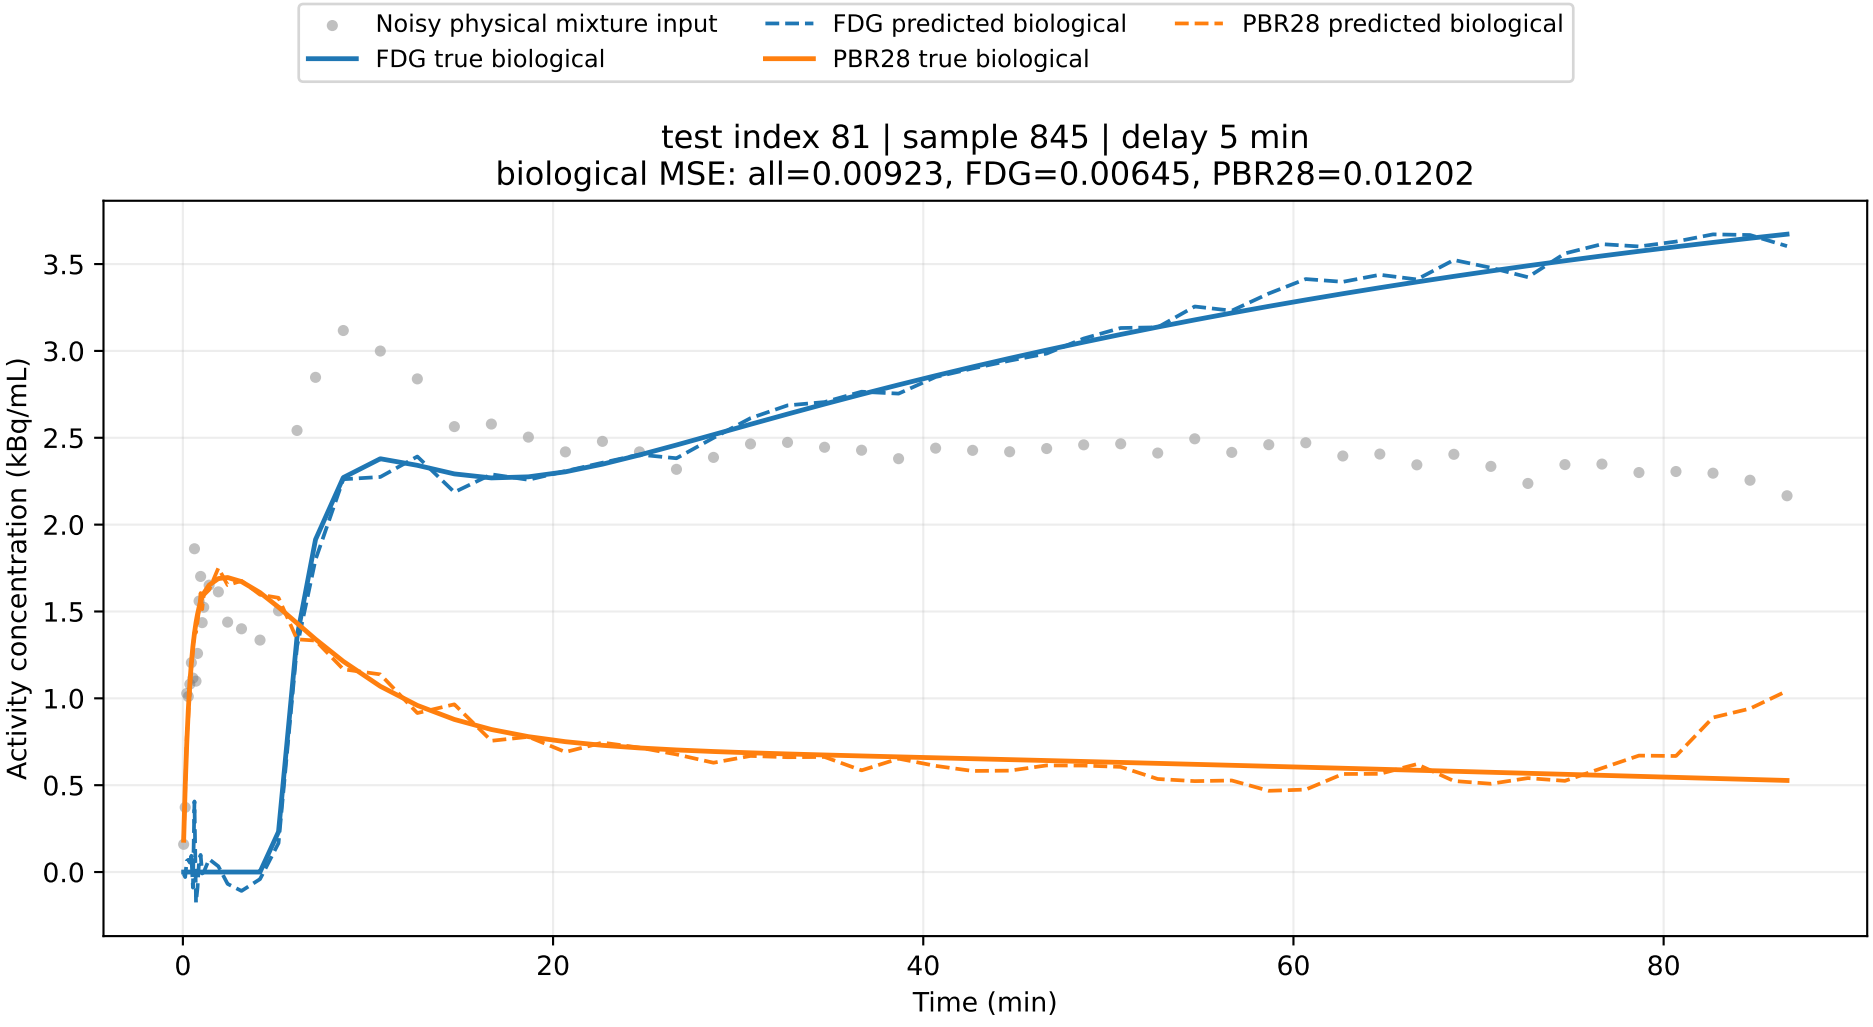

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 76 | sample 818 | delay 5 min
biological MSE: all=0.01203, FDG=0.01009, PBR28=0.01398
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

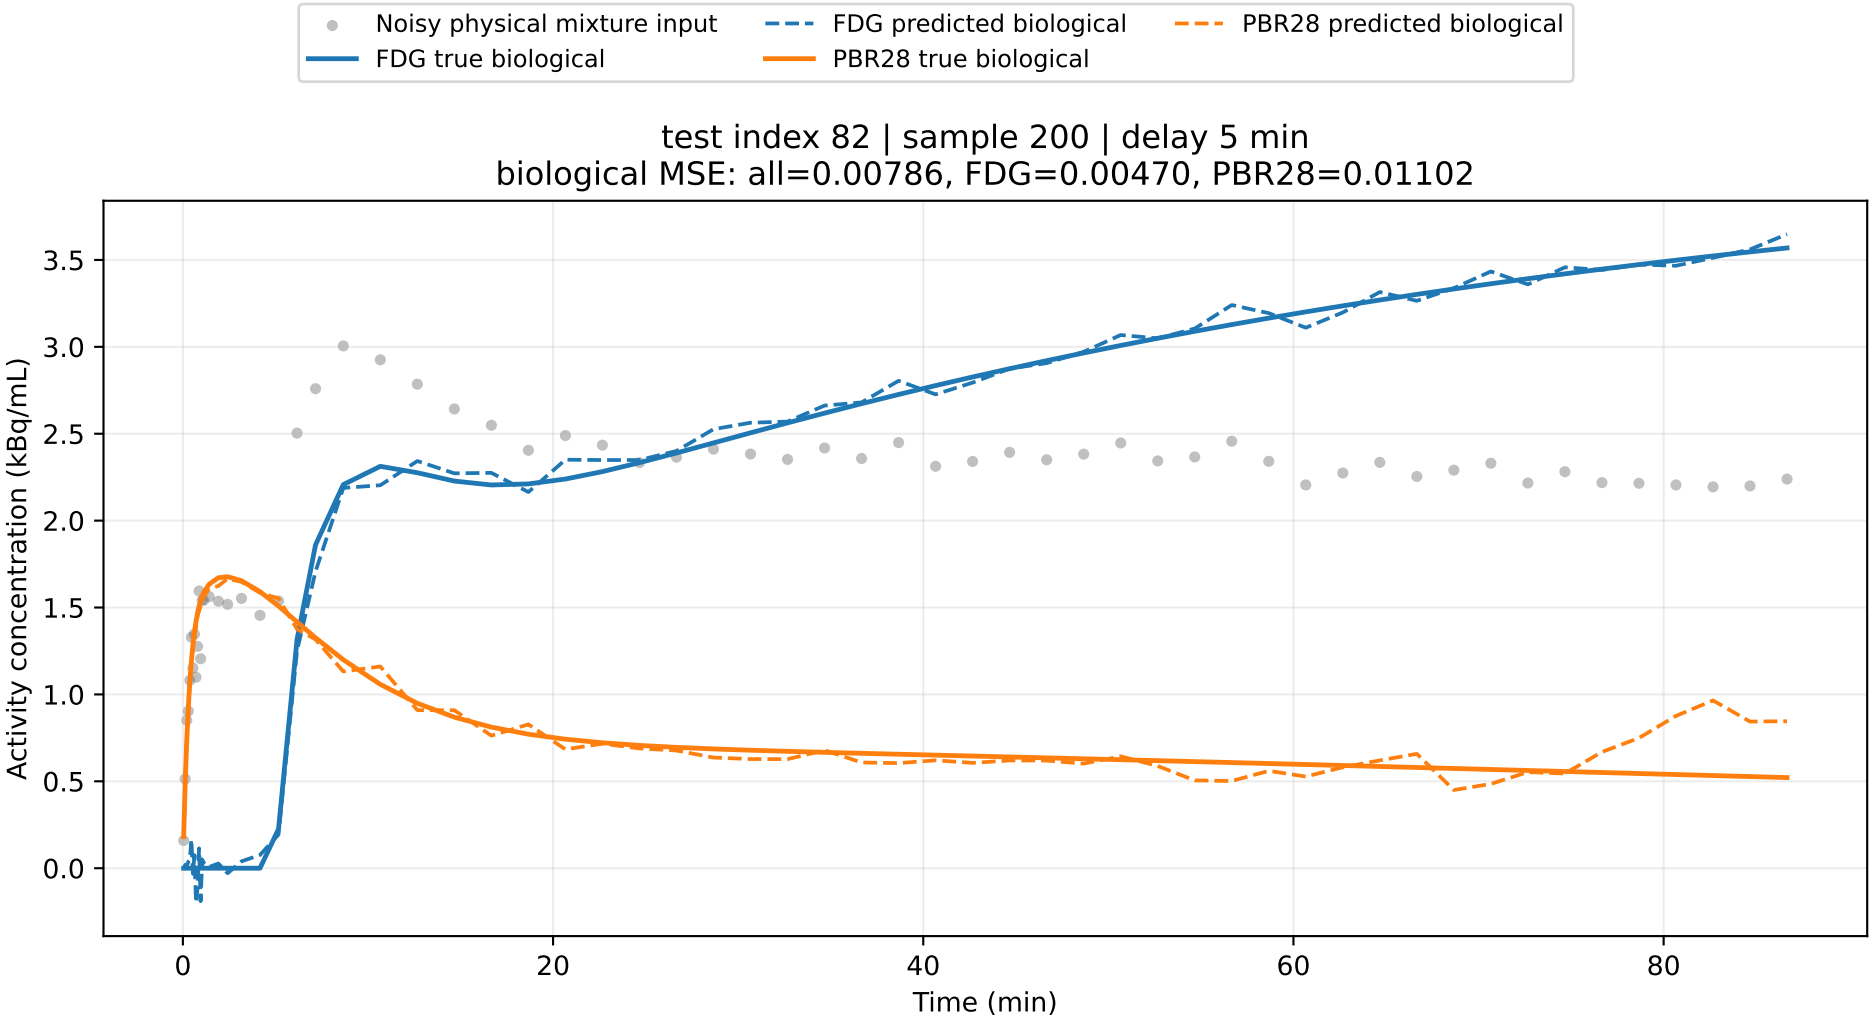

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 77 | sample 230 | delay 5 min
biological MSE: all=0.00993, FDG=0.00519, PBR28=0.01467
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

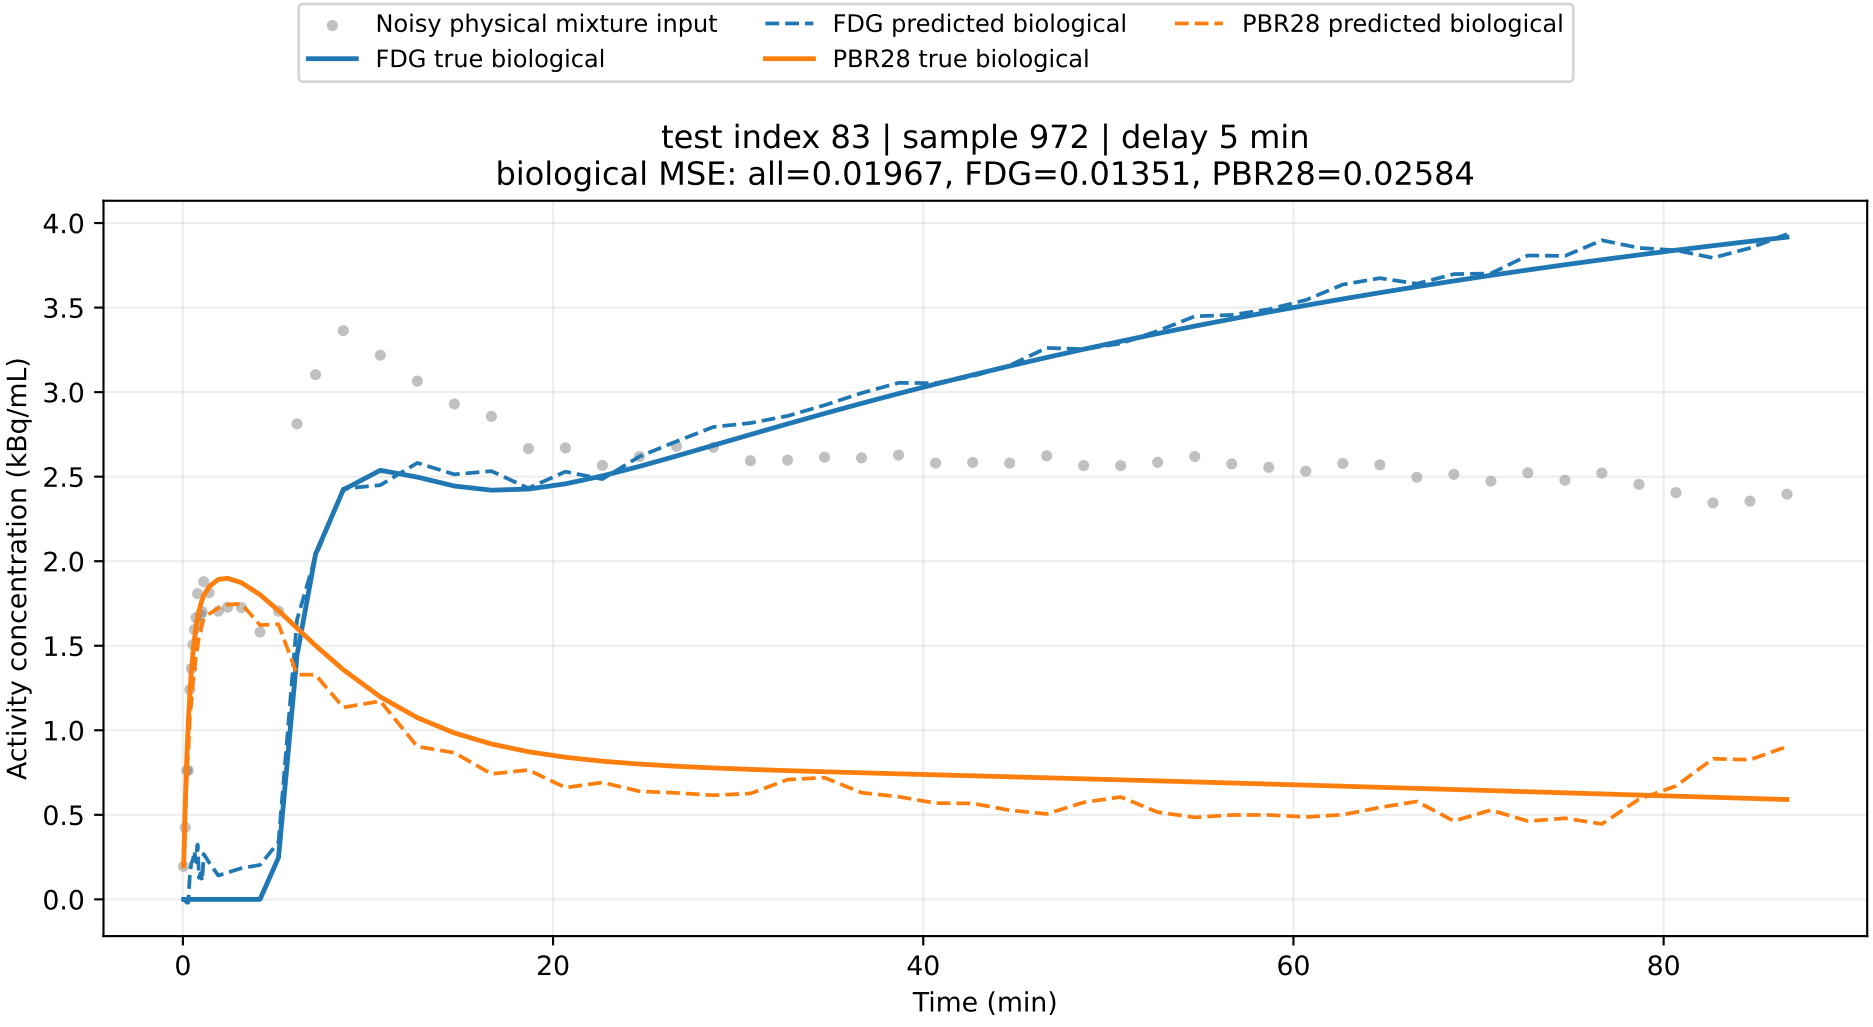

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 78 | sample 875 | delay 5 min
biological MSE: all=0.00746, FDG=0.00311, PBR28=0.01182
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

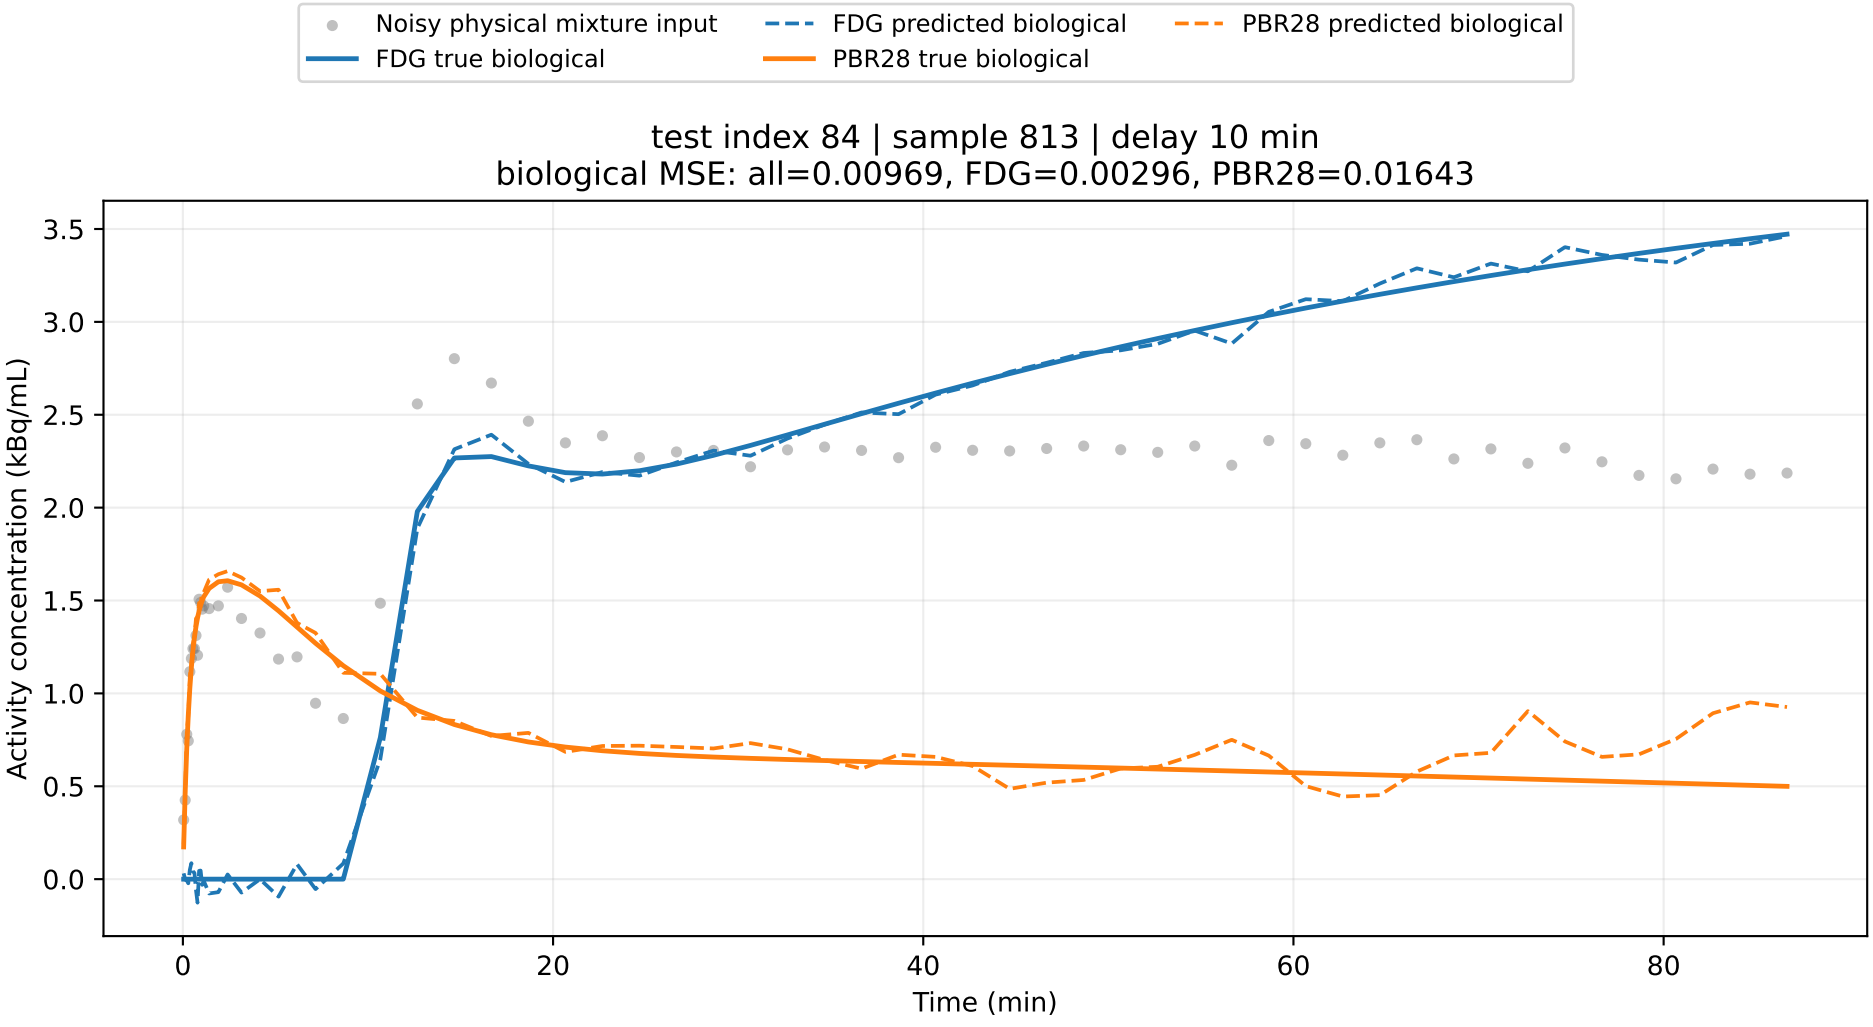

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 79 | sample 430 | delay 10 min
biological MSE: all=0.00790, FDG=0.00475, PBR28=0.01105
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

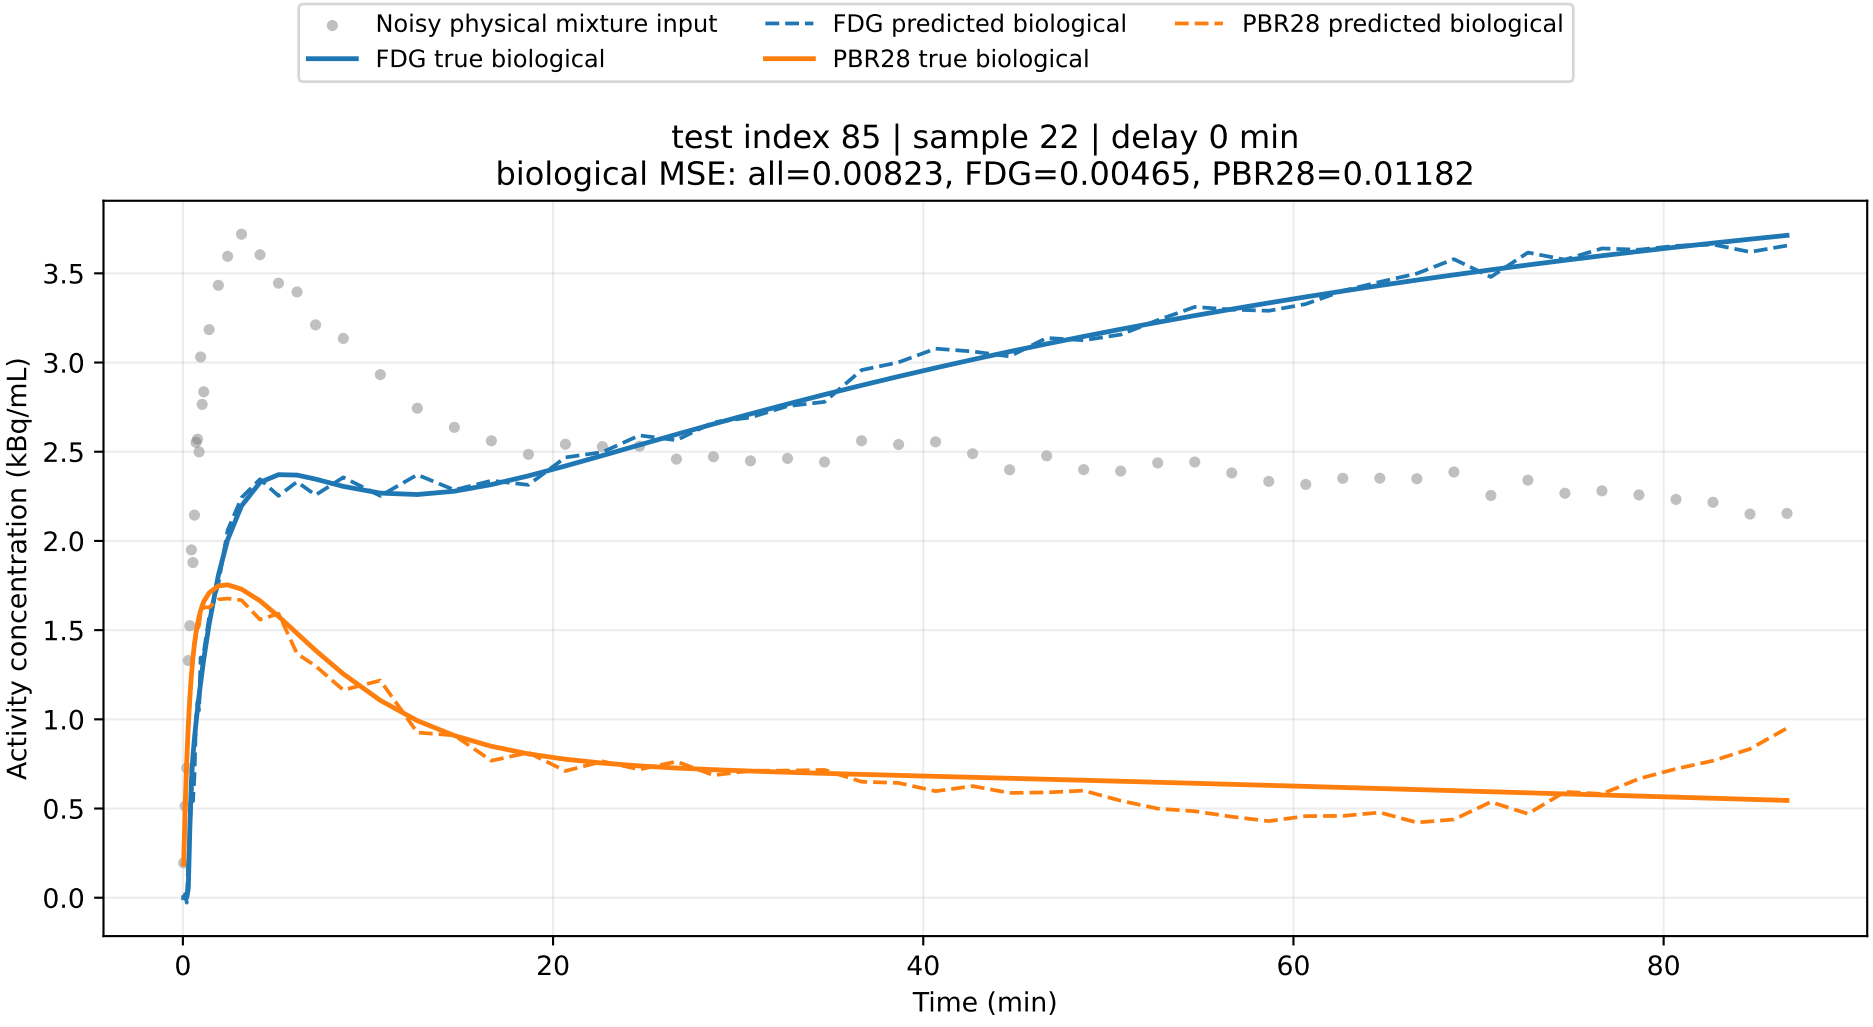

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 80 | sample 306 | delay 10 min
biological MSE: all=0.02921, FDG=0.00723, PBR28=0.05119
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

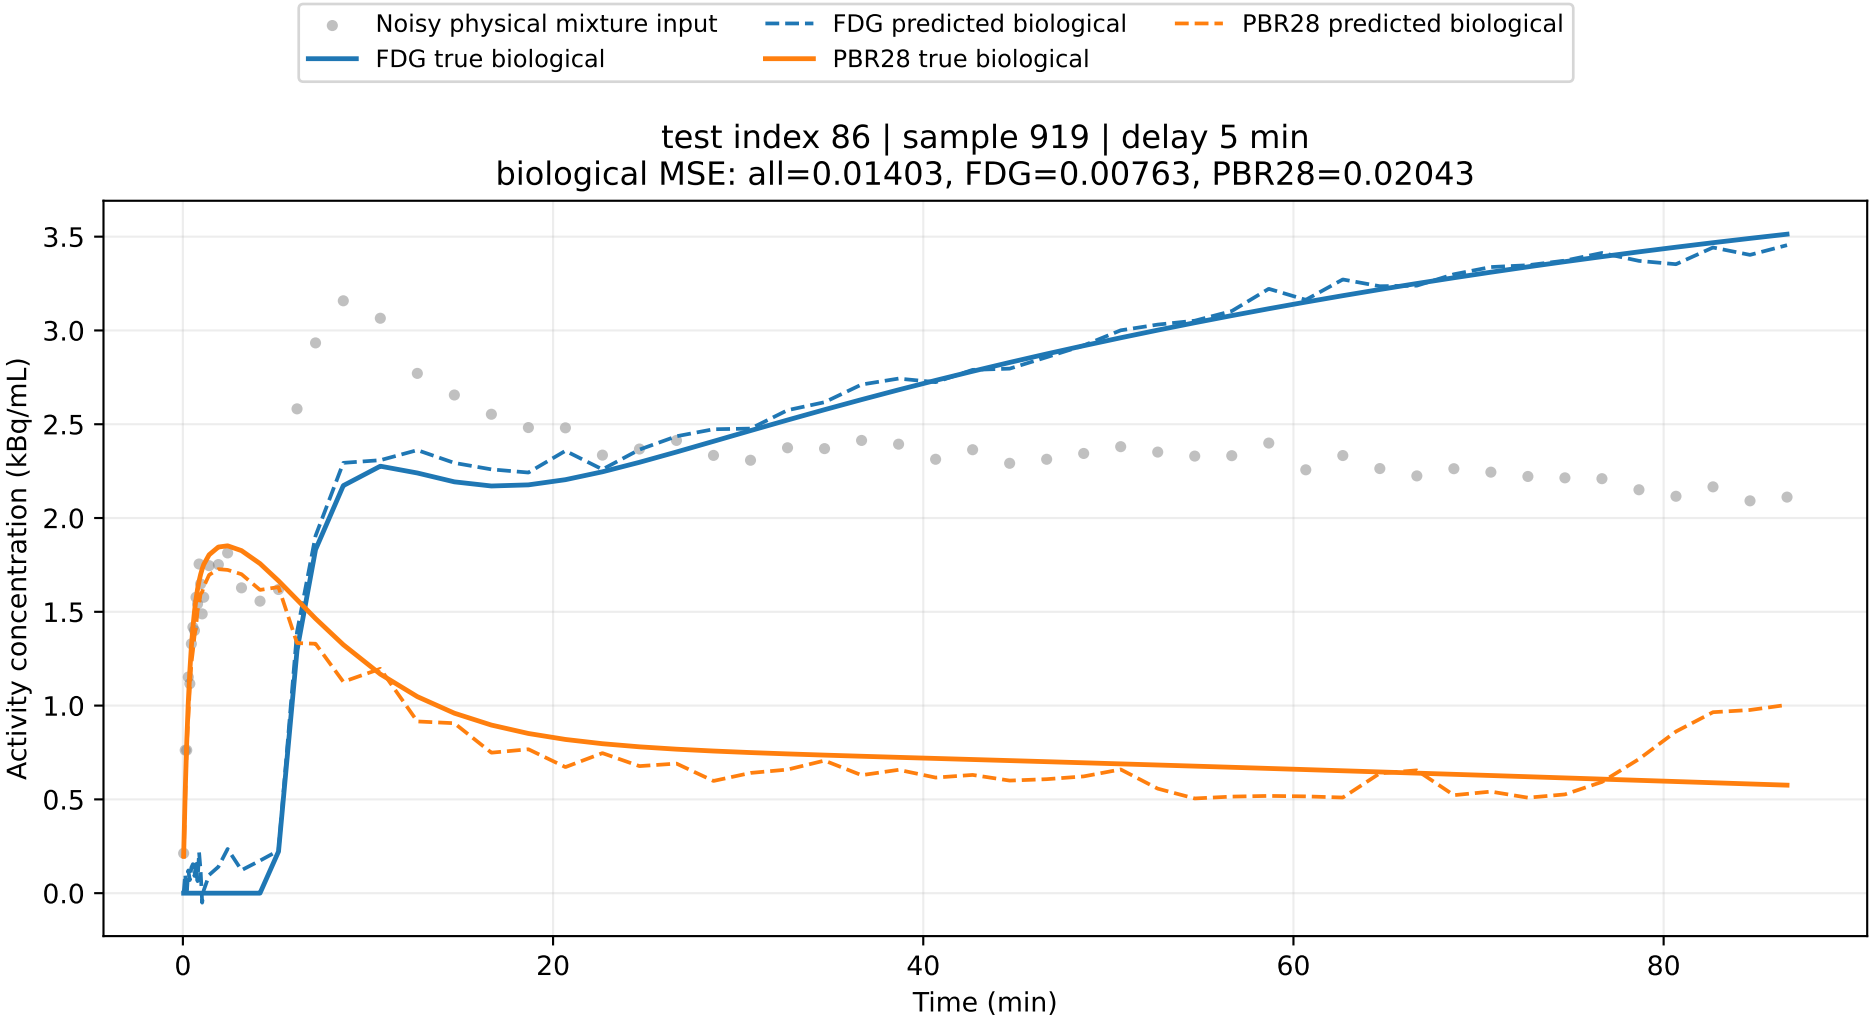

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 81 | sample 845 | delay 5 min
biological MSE: all=0.00923, FDG=0.00645, PBR28=0.01202
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

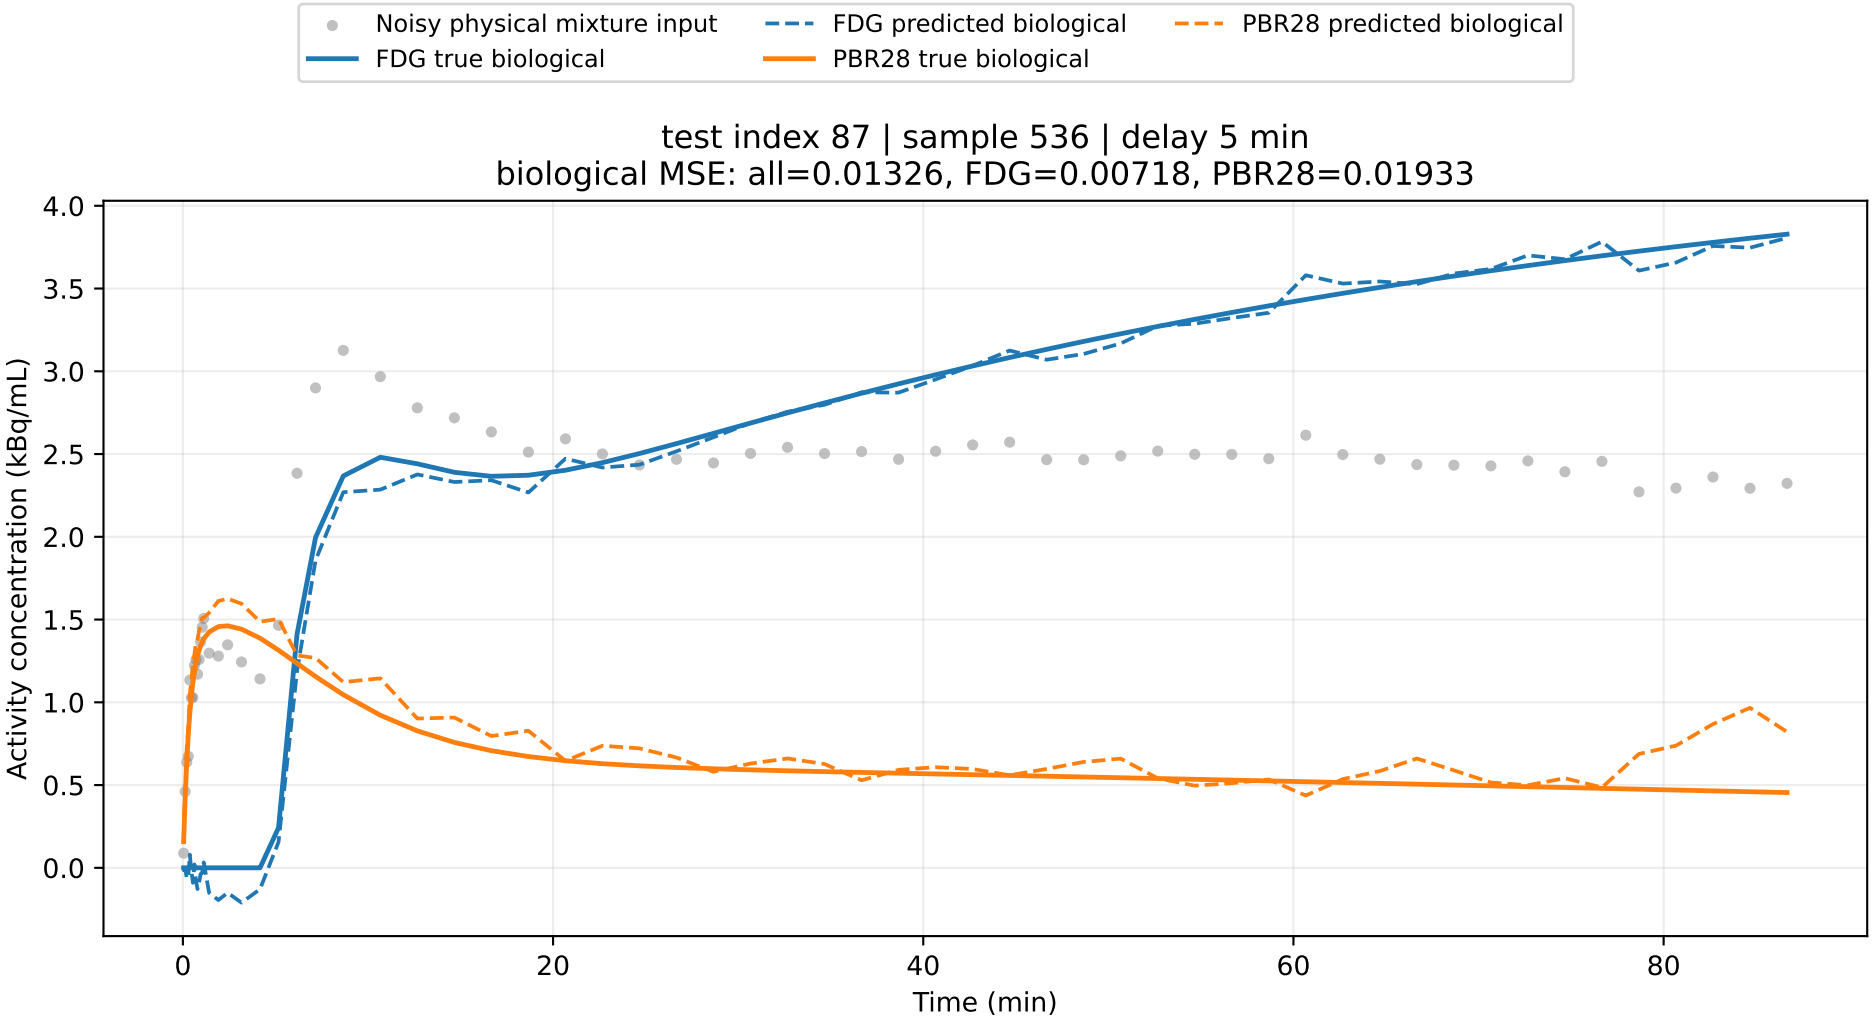

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 82 | sample 200 | delay 5 min
biological MSE: all=0.00786, FDG=0.00470, PBR28=0.01102
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

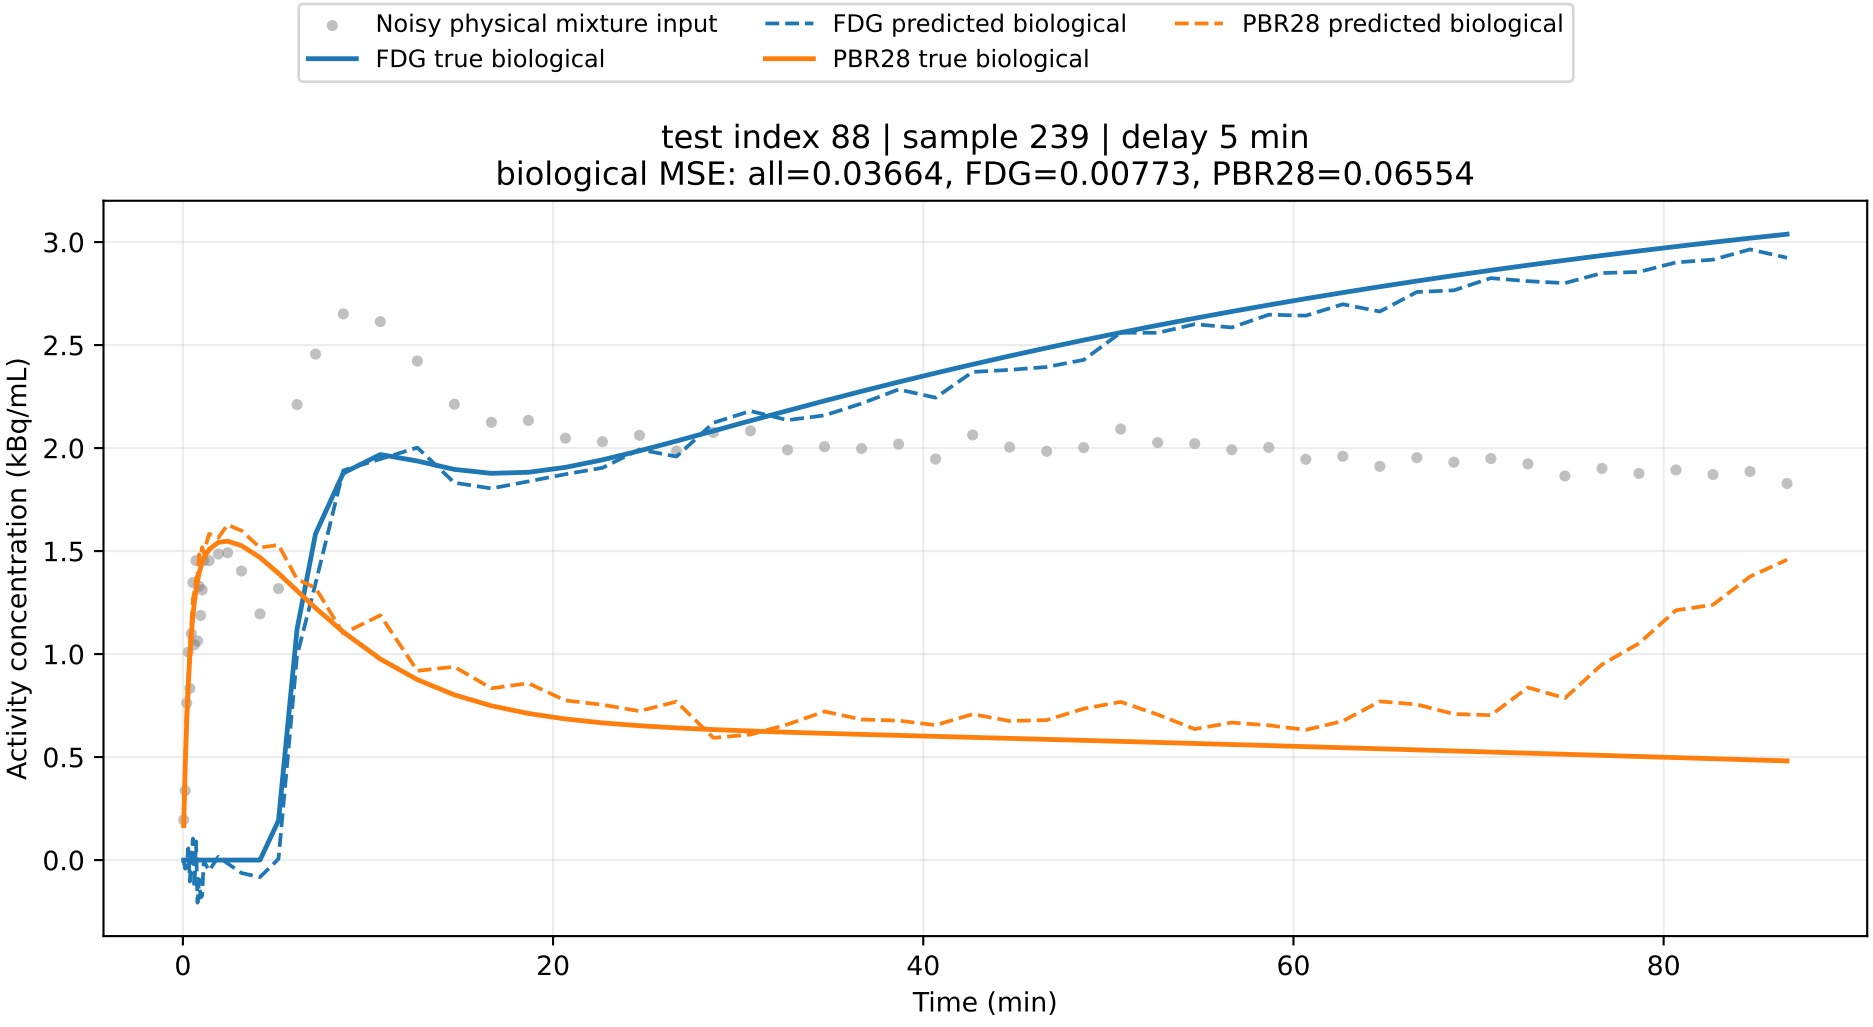

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 83 | sample 972 | delay 5 min
biological MSE: all=0.01967, FDG=0.01351, PBR28=0.02584
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

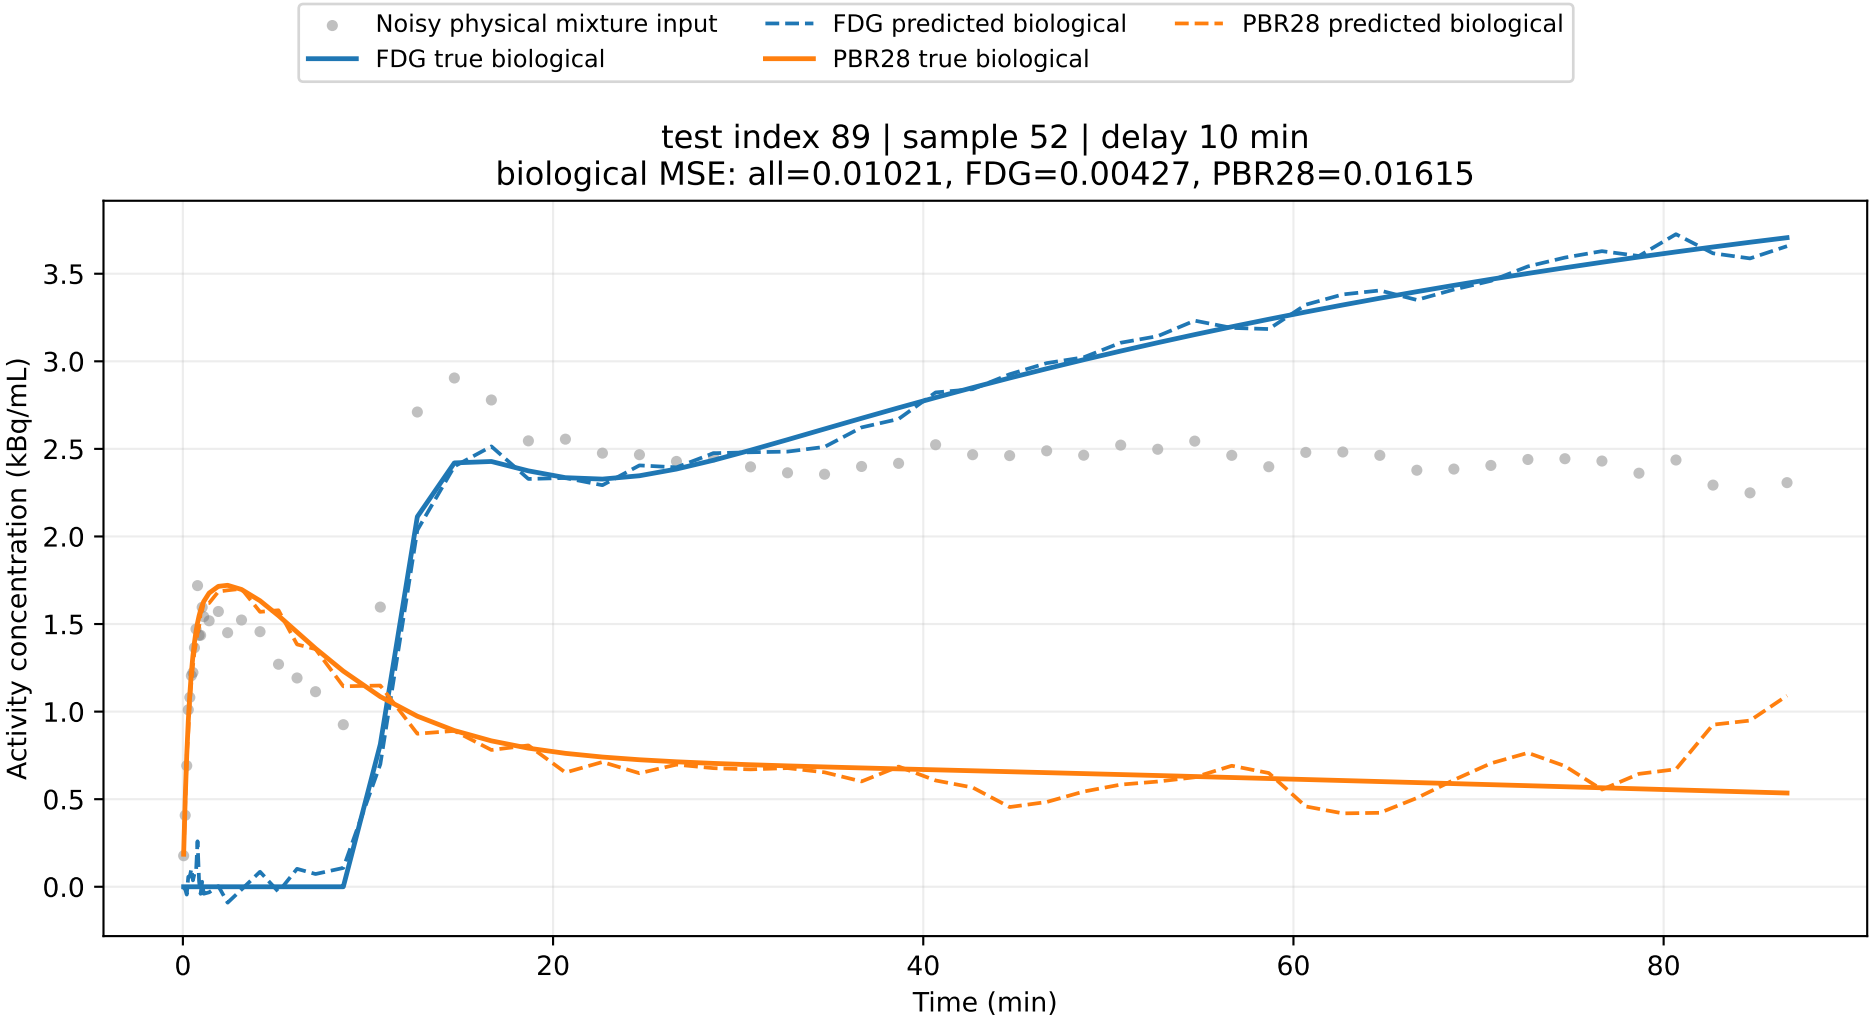

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 84 | sample 813 | delay 10 min
biological MSE: all=0.00969, FDG=0.00296, PBR28=0.01643
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

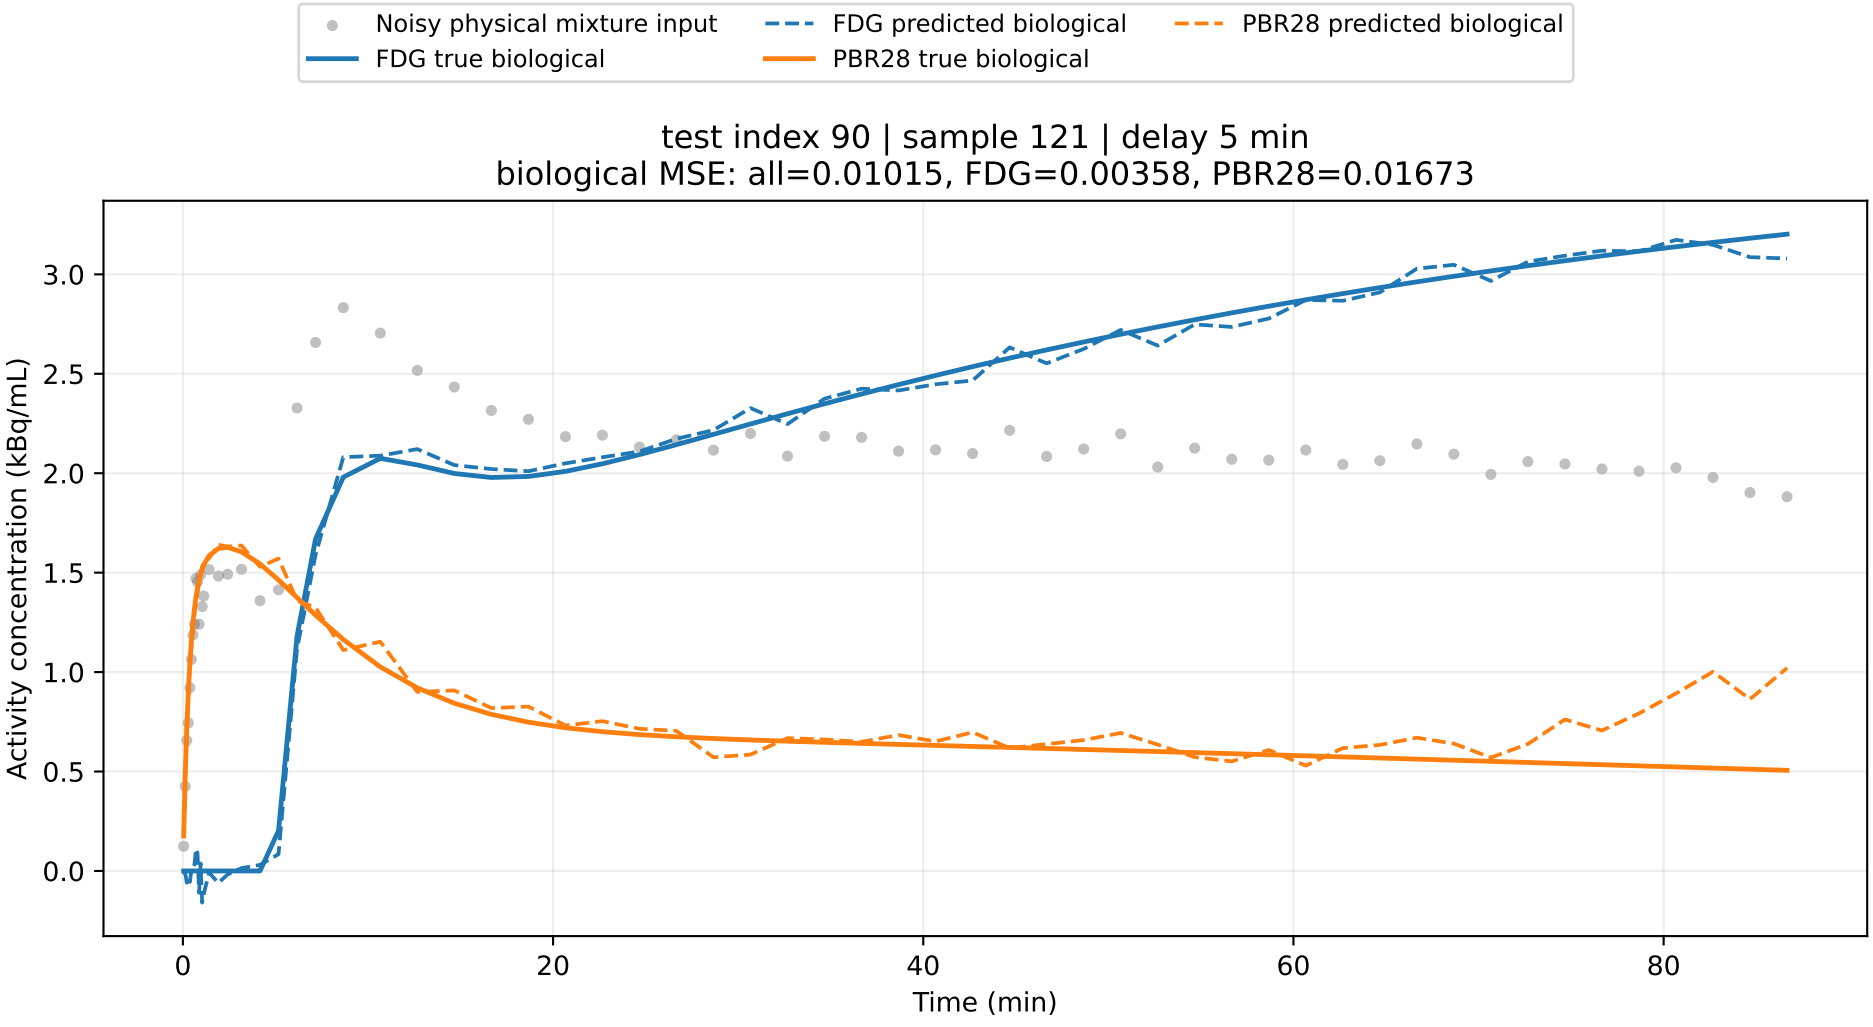

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 85 | sample 22 | delay 0 min
biological MSE: all=0.00823, FDG=0.00465, PBR28=0.01182
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

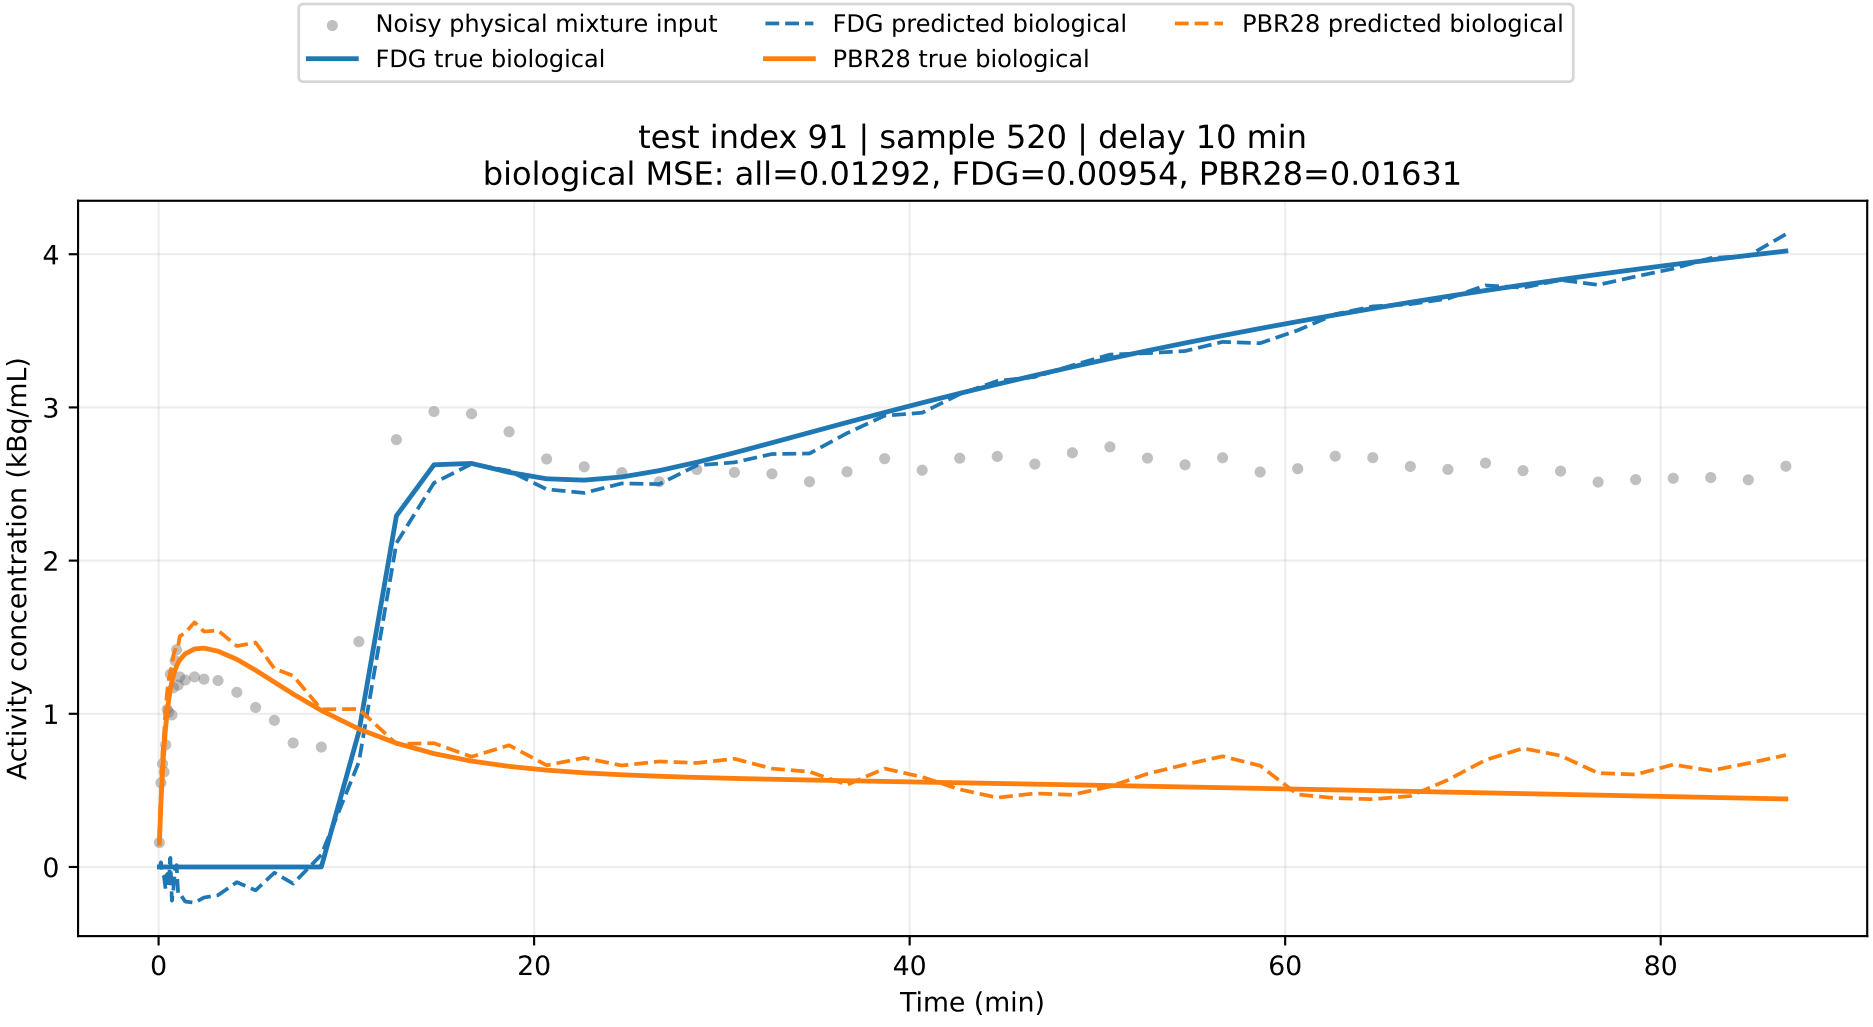

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 86 | sample 919 | delay 5 min
biological MSE: all=0.01403, FDG=0.00763, PBR28=0.02043
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

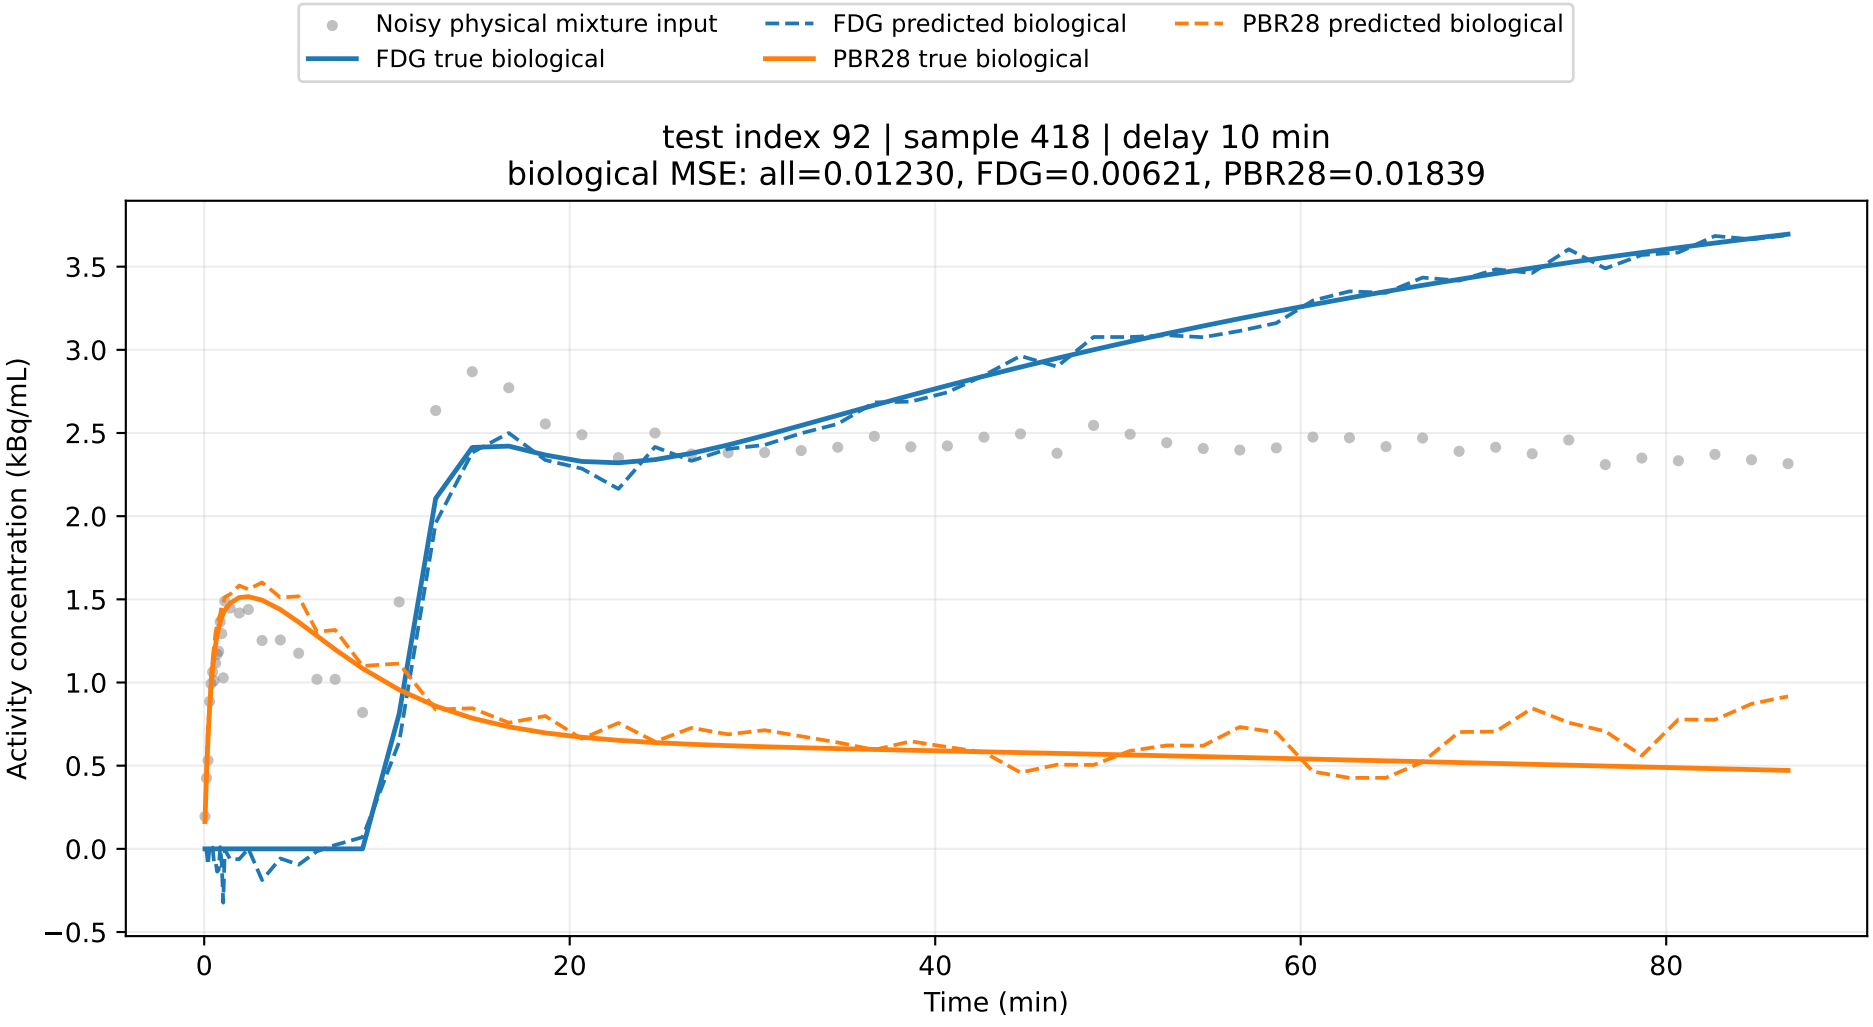

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 87 | sample 536 | delay 5 min
biological MSE: all=0.01326, FDG=0.00718, PBR28=0.01933
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
4.0
0
20
40
60
80

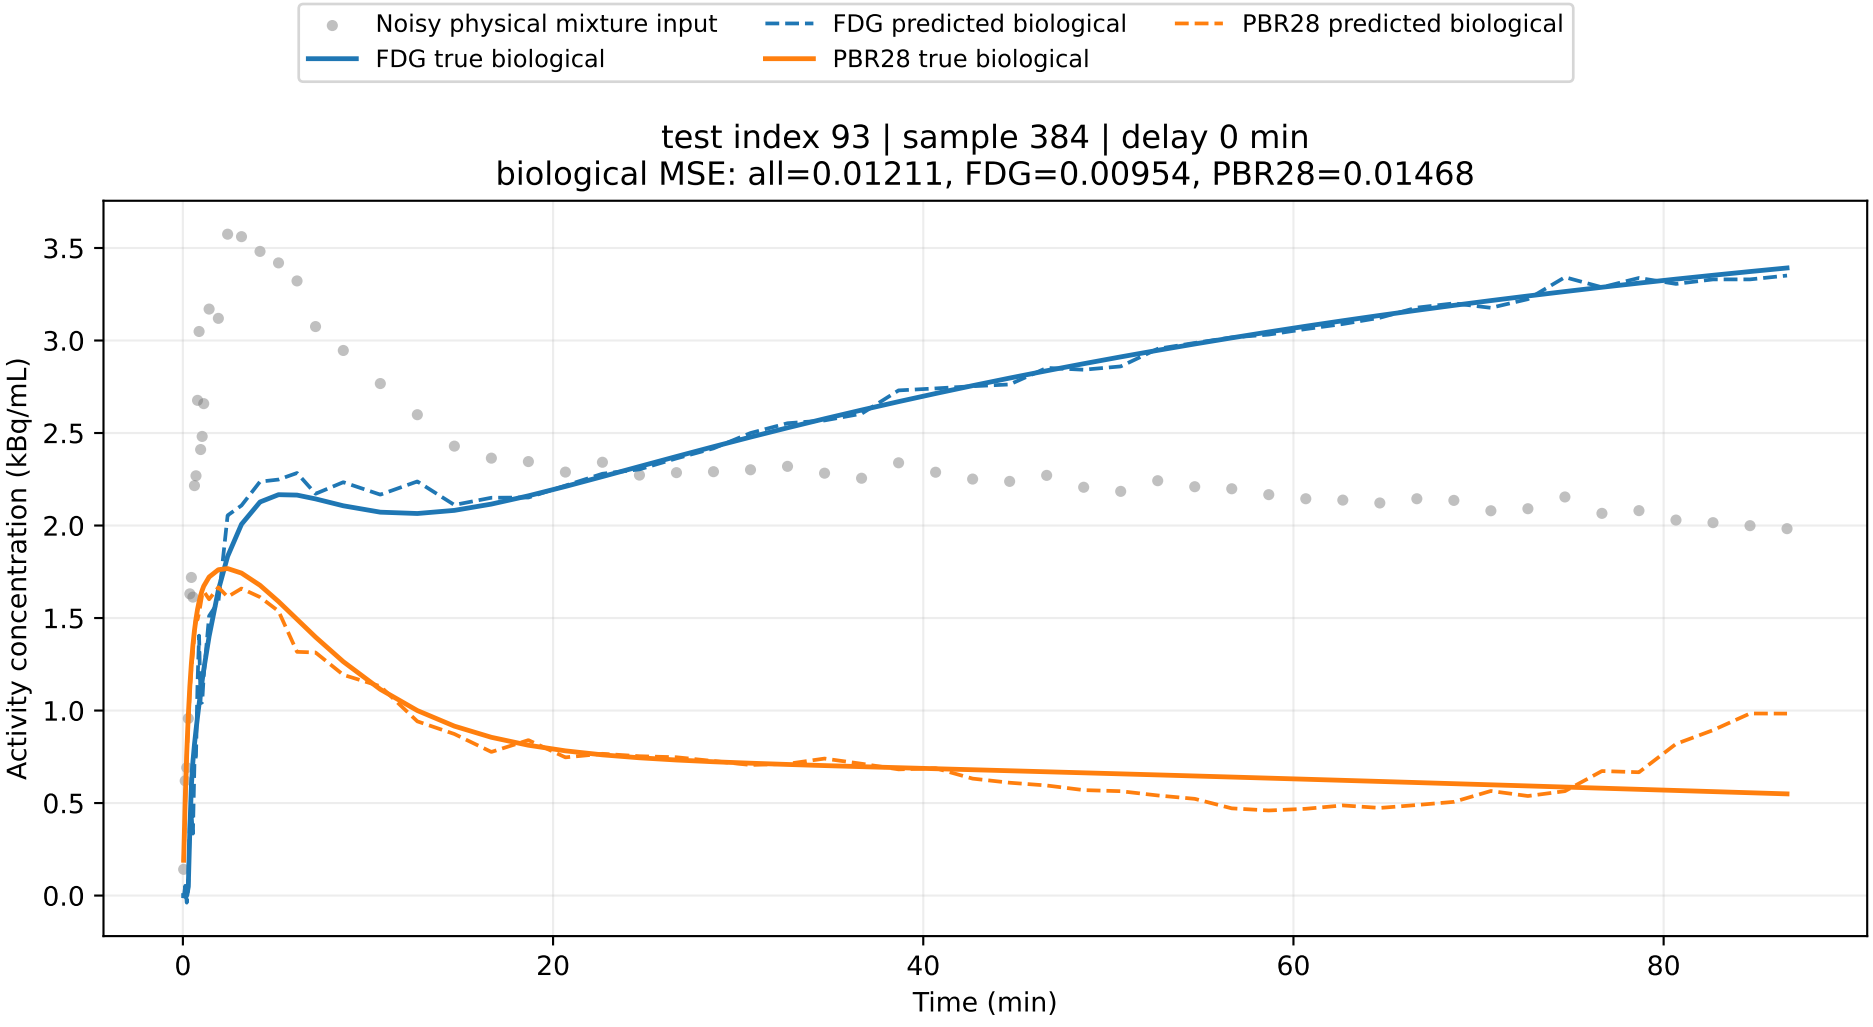

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 88 | sample 239 | delay 5 min
biological MSE: all=0.03664, FDG=0.00773, PBR28=0.06554
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

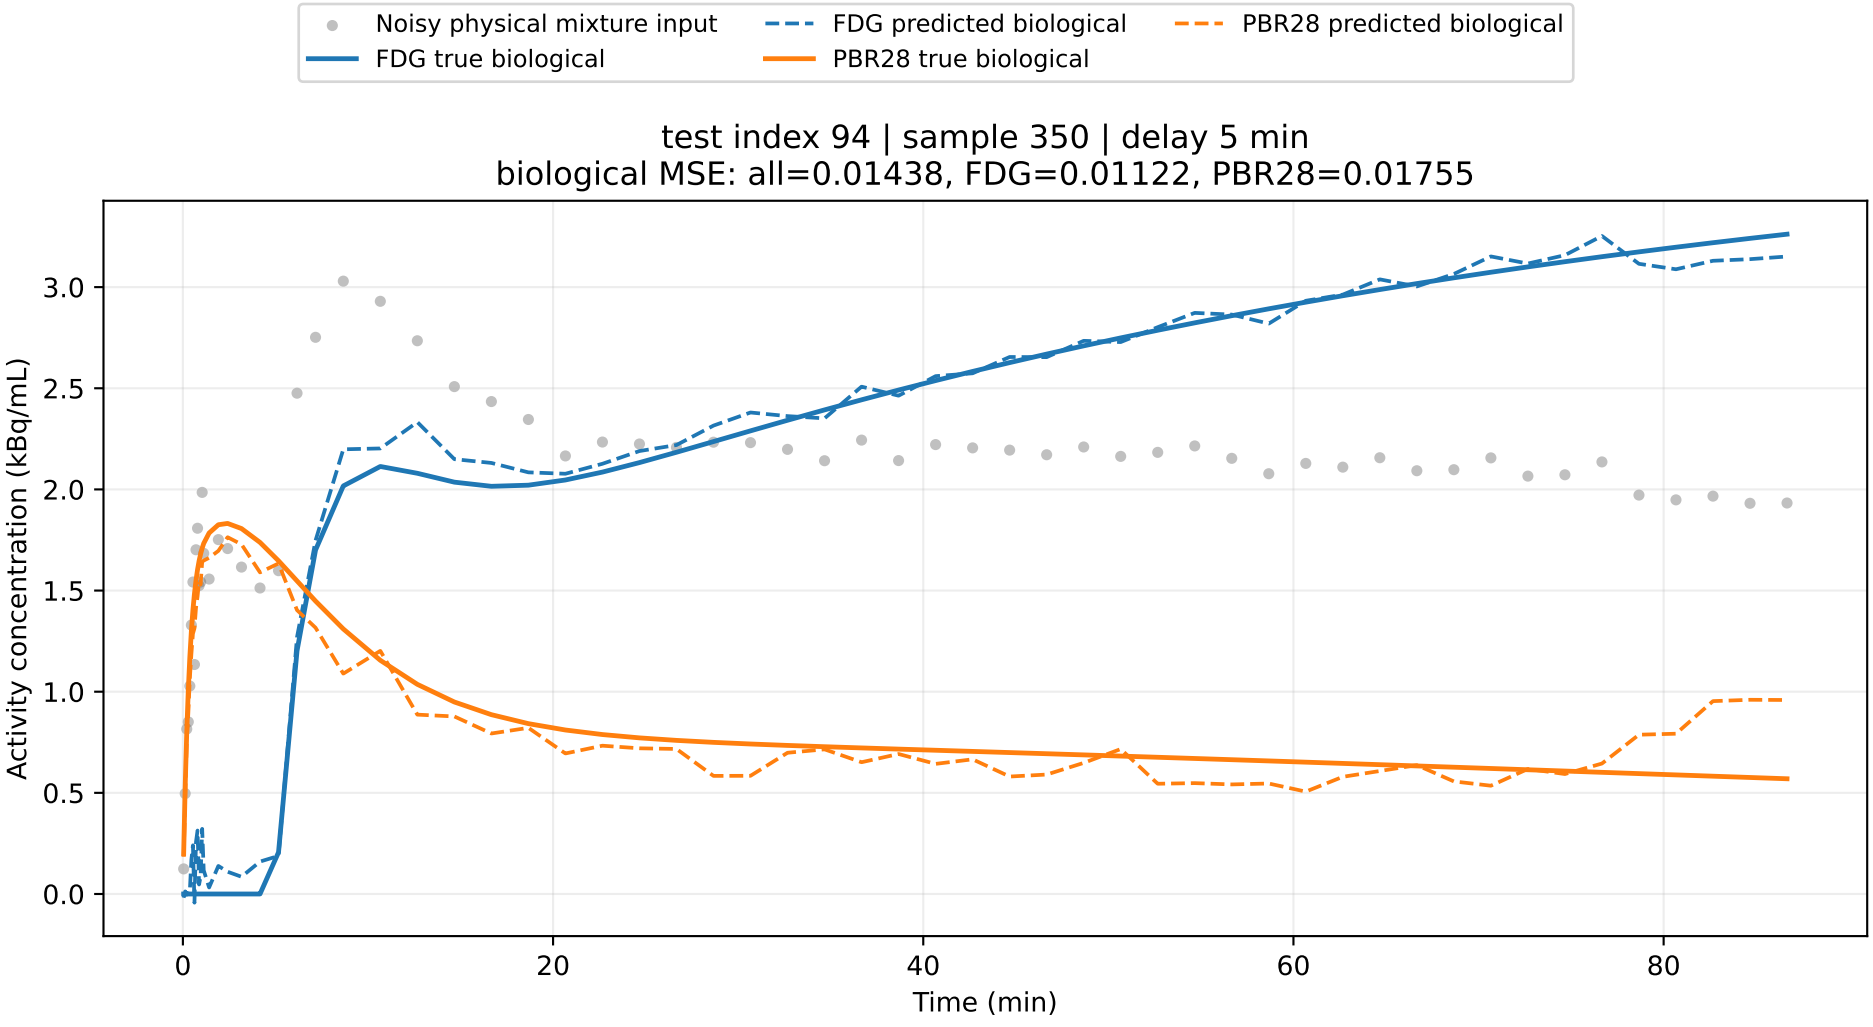

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 89 | sample 52 | delay 10 min
biological MSE: all=0.01021, FDG=0.00427, PBR28=0.01615
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

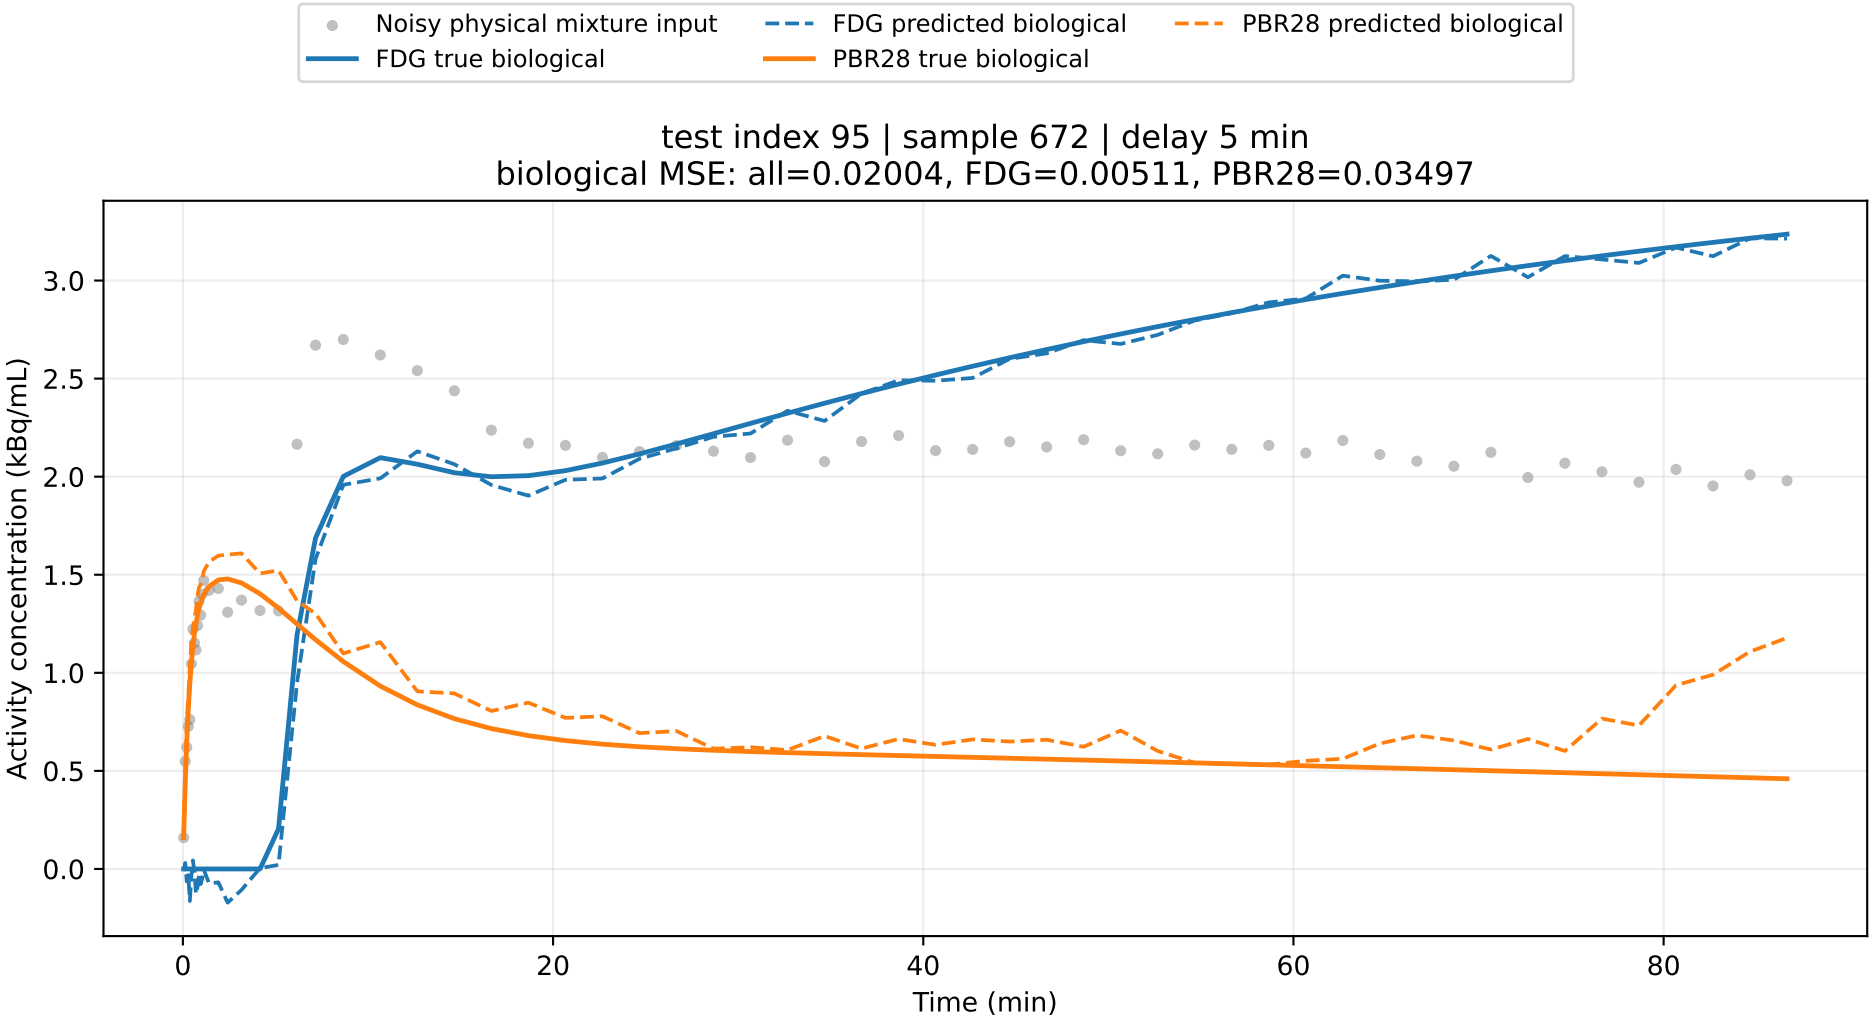

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 90 | sample 121 | delay 5 min
biological MSE: all=0.01015, FDG=0.00358, PBR28=0.01673
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80

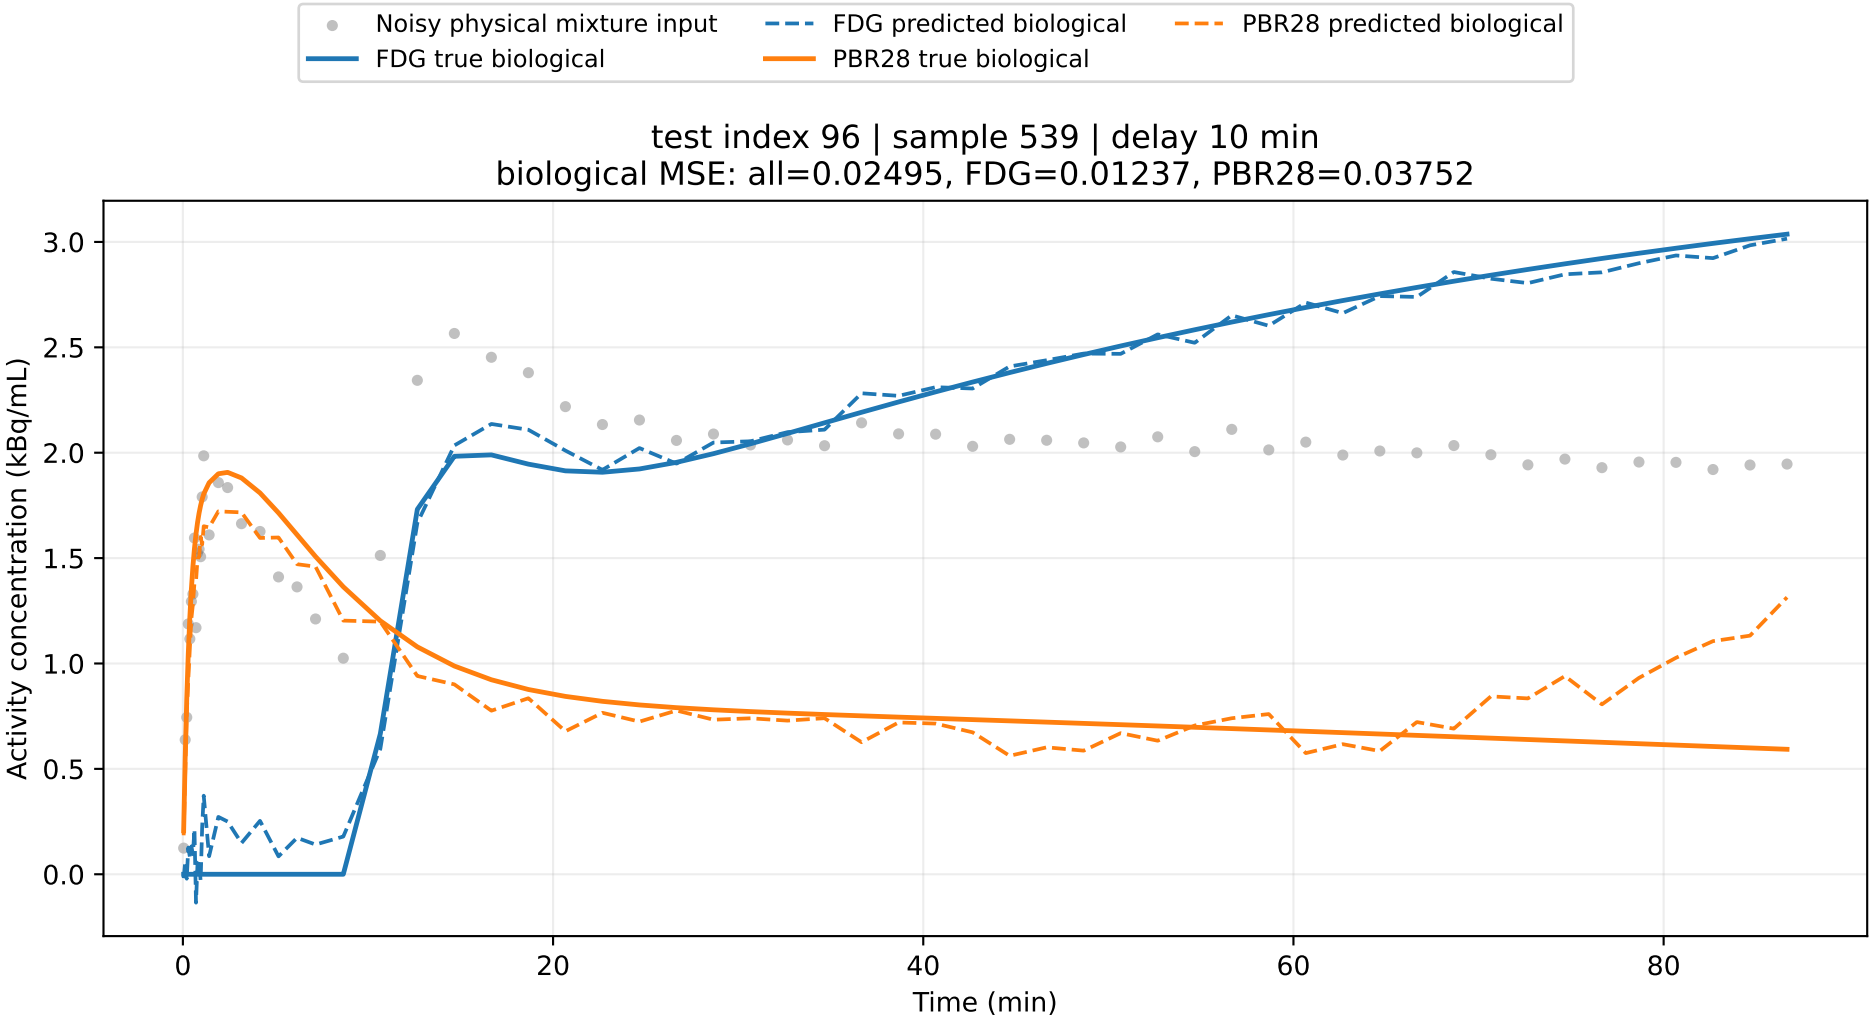

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 91 | sample 520 | delay 10 min
biological MSE: all=0.01292, FDG=0.00954, PBR28=0.01631
Activity concentration (kBq/mL)
Time (min)
0
1
2
3
4
0
20
40
60
80

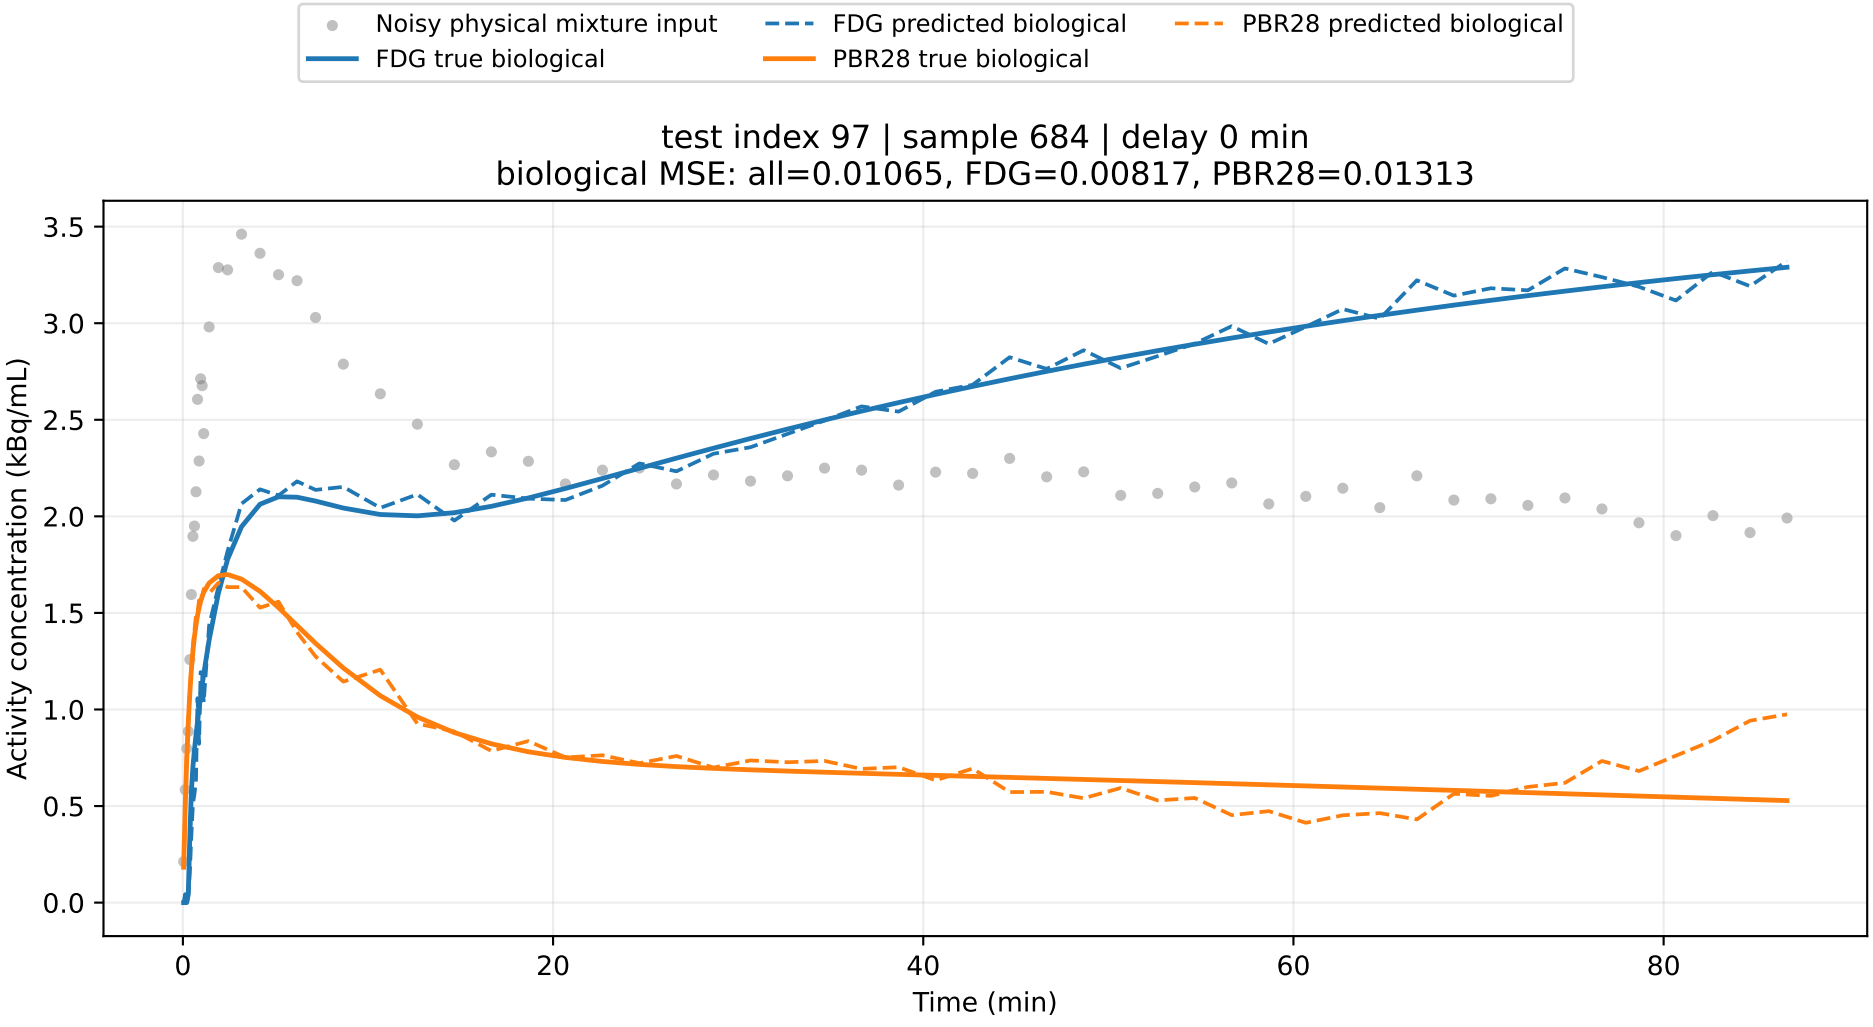

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 92 | sample 418 | delay 10 min
biological MSE: all=0.01230, FDG=0.00621, PBR28=0.01839
Activity concentration (kBq/mL)
Time (min)
3.5
3.0
2.5
2.0
1.5
1.0
0.5
0.0
−0.5
0
20
40
60
80

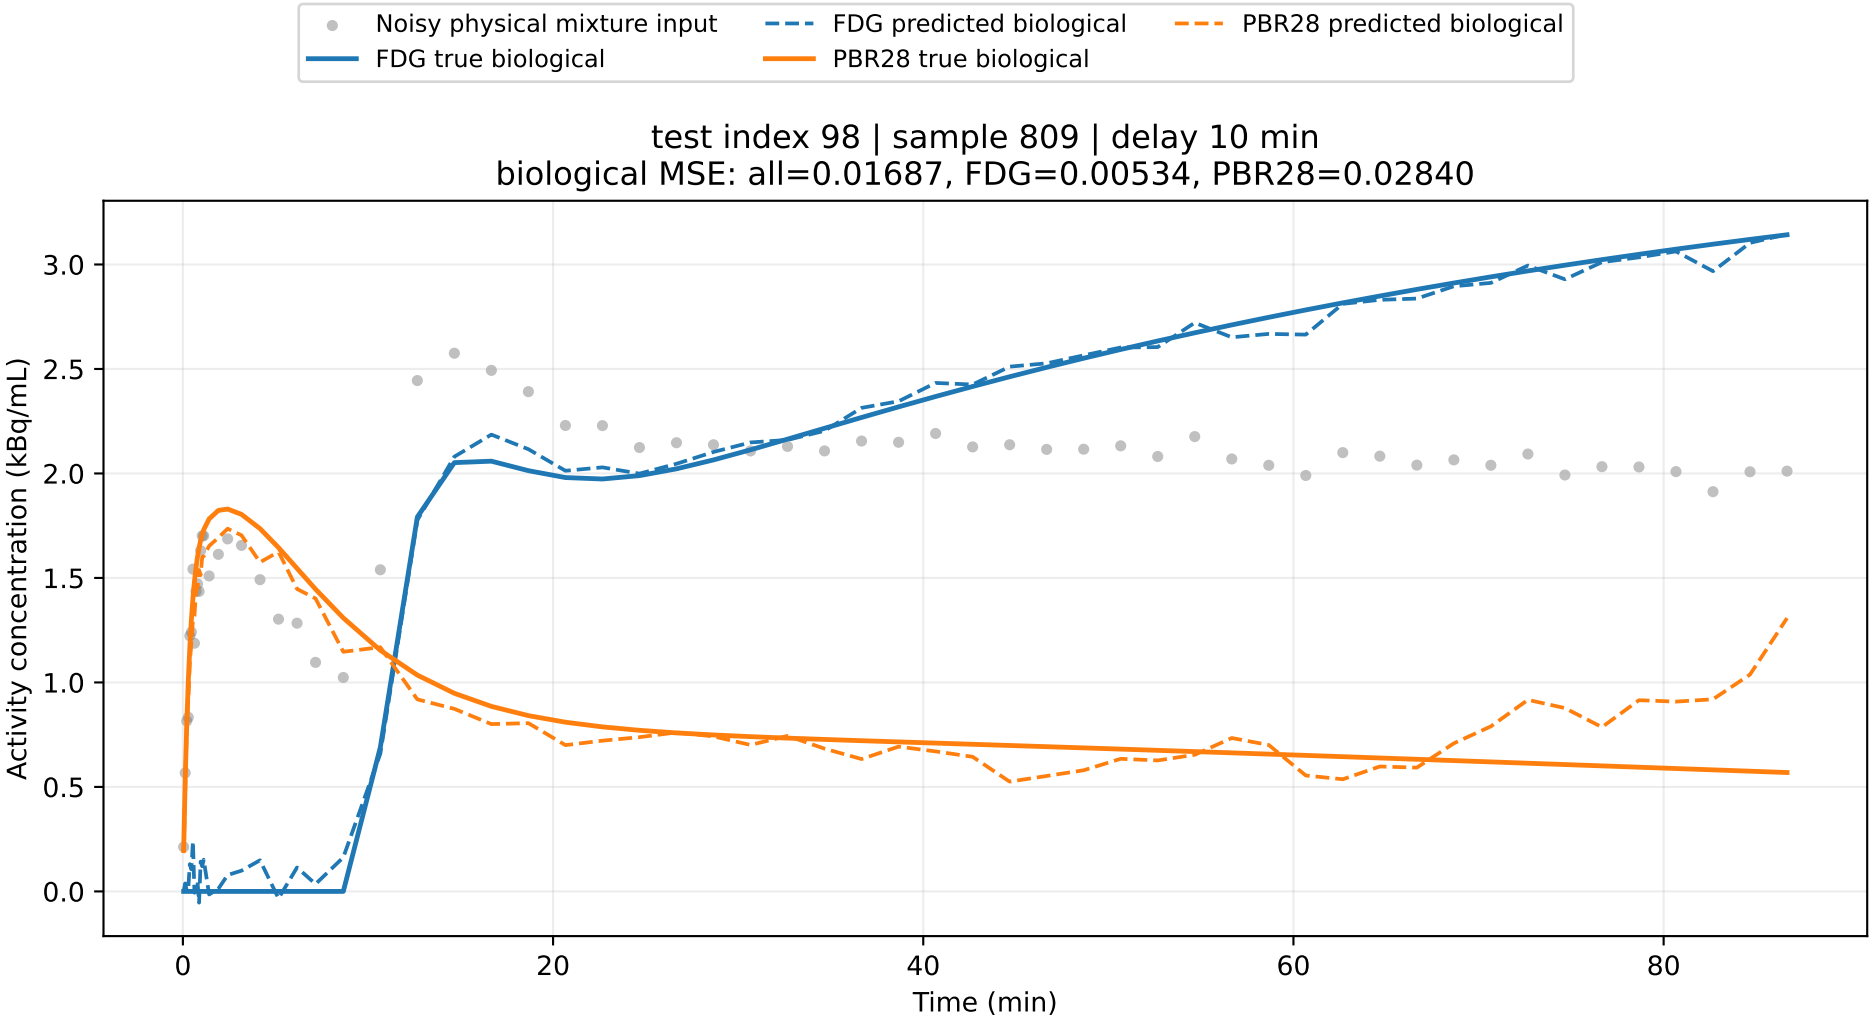

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 93 | sample 384 | delay 0 min
biological MSE: all=0.01211, FDG=0.00954, PBR28=0.01468
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80

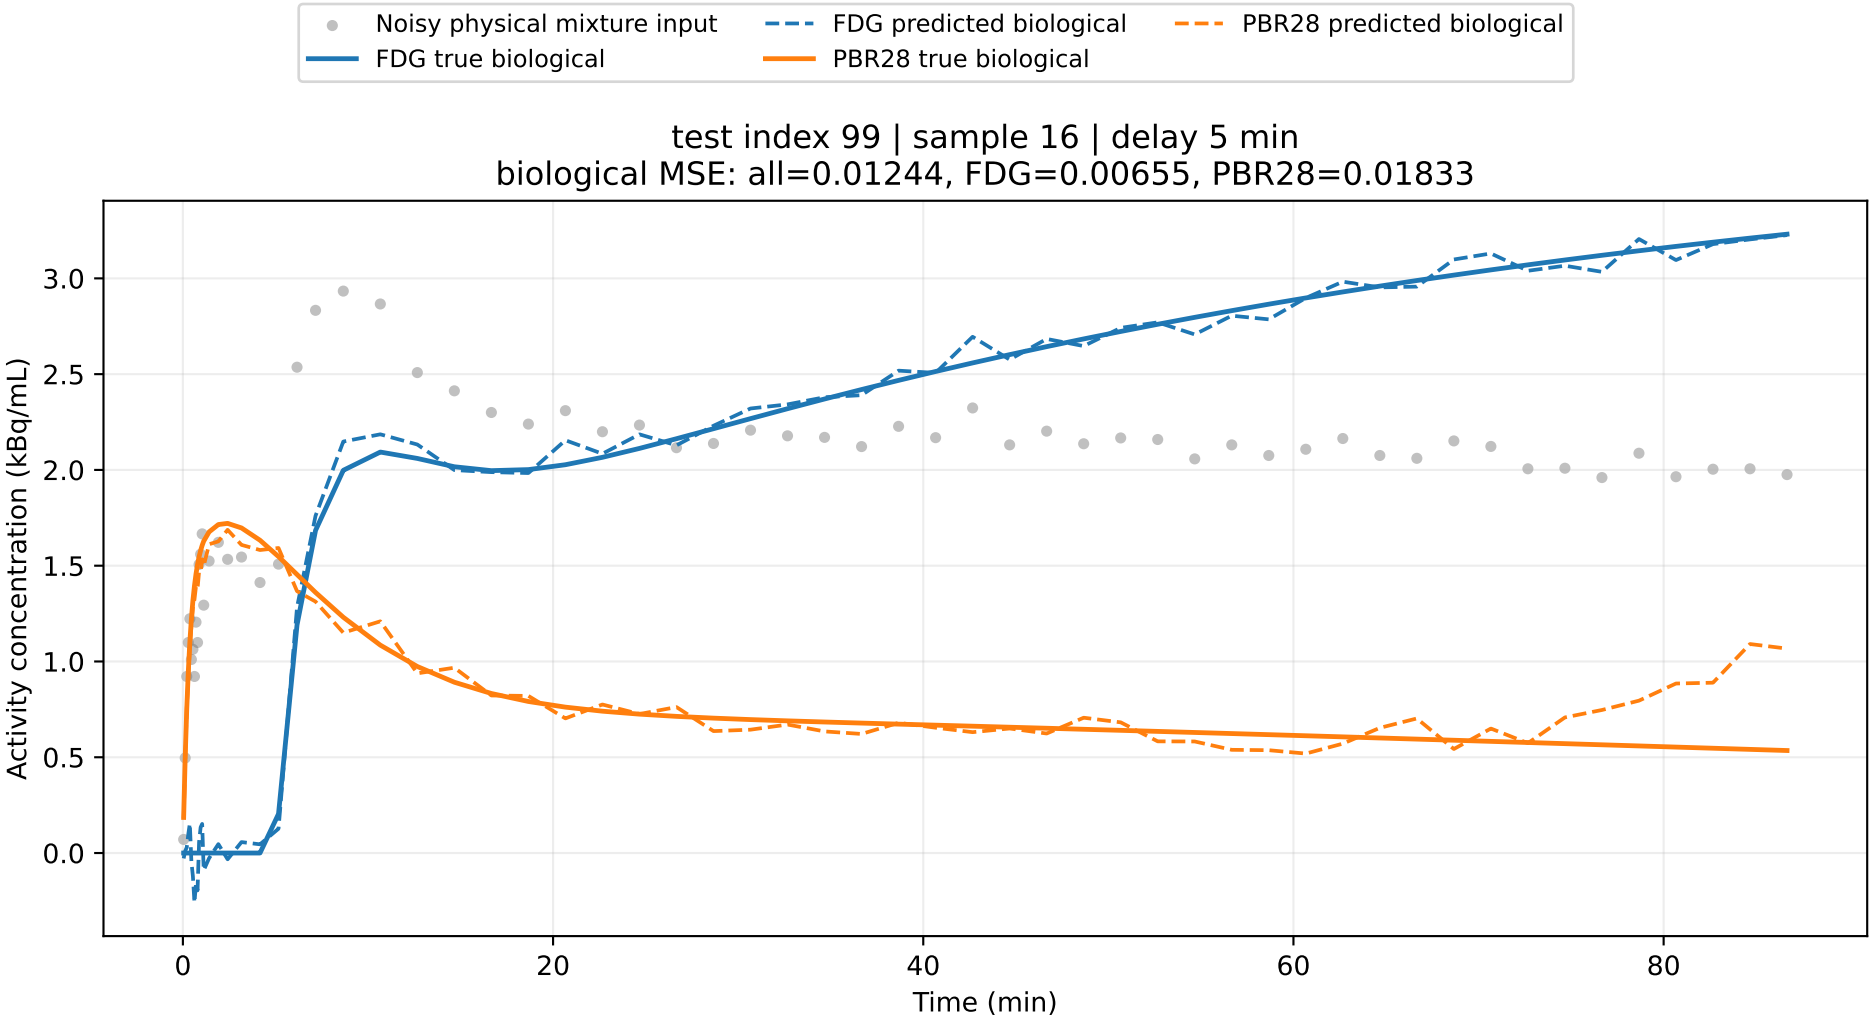

Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 94 | sample 350 | delay 5 min
biological MSE: all=0.01438, FDG=0.01122, PBR28=0.01755
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80


Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 95 | sample 672 | delay 5 min
biological MSE: all=0.02004, FDG=0.00511, PBR28=0.03497
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80


Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 96 | sample 539 | delay 10 min
biological MSE: all=0.02495, FDG=0.01237, PBR28=0.03752
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80


Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 97 | sample 684 | delay 0 min
biological MSE: all=0.01065, FDG=0.00817, PBR28=0.01313
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
3.5
0
20
40
60
80


Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 98 | sample 809 | delay 10 min
biological MSE: all=0.01687, FDG=0.00534, PBR28=0.02840
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80


Noisy physical mixture input
FDG true biological
FDG predicted biological
PBR28 true biological
PBR28 predicted biological
test index 99 | sample 16 | delay 5 min
biological MSE: all=0.01244, FDG=0.00655, PBR28=0.01833
Activity concentration (kBq/mL)
Time (min)
0.0
0.5
1.0
1.5
2.0
2.5
3.0
0
20
40
60
80