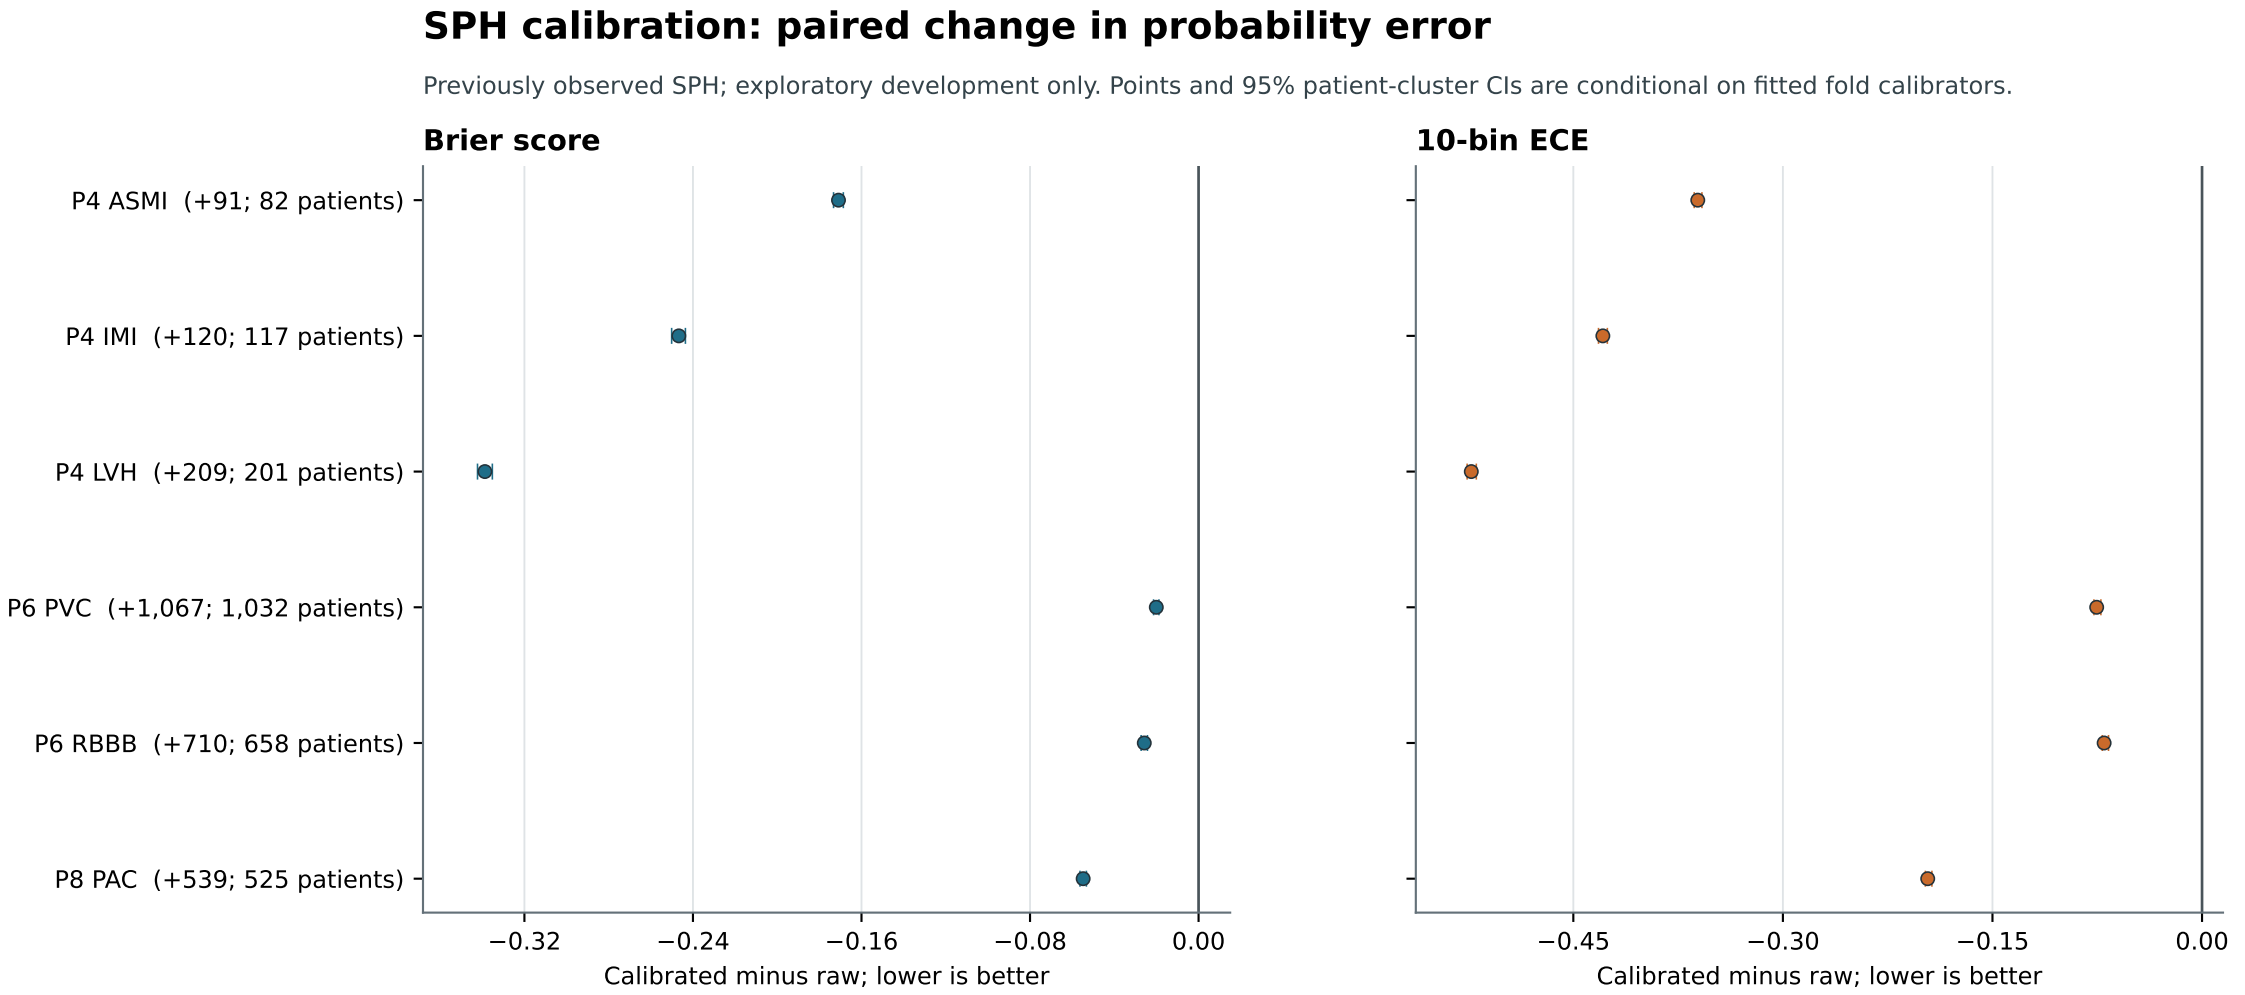
SPH calibration: paired change in probability error
Previously observed SPH; exploratory development only. Points and 95% patient-cluster CIs are conditional on fitted fold calibrators.
Brier score
10-bin ECE
P4 ASMI (+91; 82 patients)
P4 IMI (+120; 117 patients)
P4 LVH (+209; 201 patients)
P6 PVC (+1,067; 1,032 patients)
P6 RBBB (+710; 658 patients)
P8 PAC (+539; 525 patients)
−0.32
−0.24
−0.16
−0.08
0.00
−0.45
−0.30
−0.15
0.00
Calibrated minus raw; lower is better
Calibrated minus raw; lower is better
Negative values indicate lower error than raw V4.5 scores. CIs do not refit calibrators; this is not independent or clinical validation.