

Previously discussed cells after local-background recalibration
These six examples were excluded from threshold fitting and the reserved review sample

Label 63 · old C1 G2M / C2 G2M

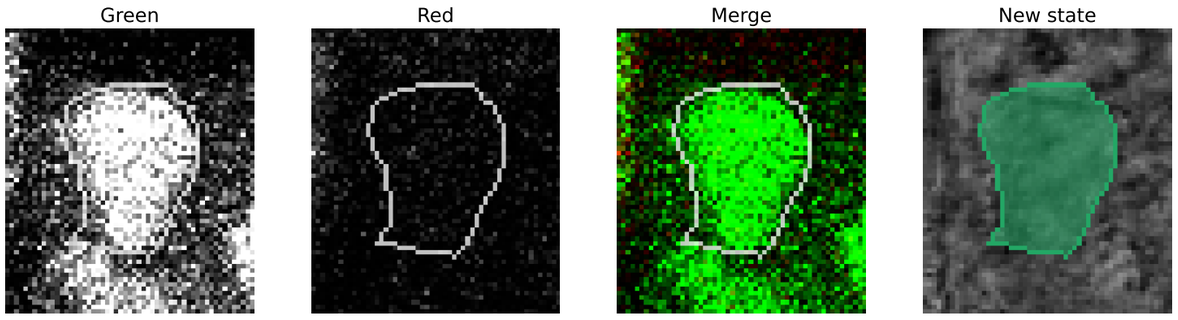


New: Green only · green excess 0.07099 · red excess 0.00205

Label 410 · old C1 G2M / C2 G2M

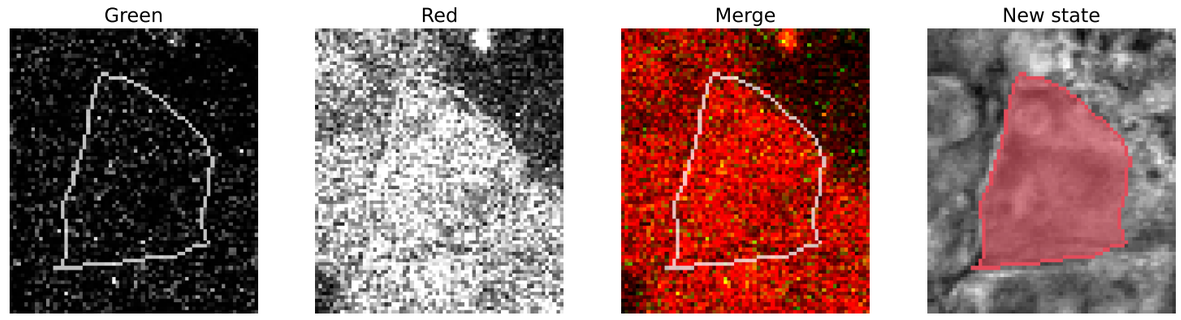


New: Red only · green excess 0.00540 · red excess 0.03004

Label 42 · old C1 G2M / C2 G1

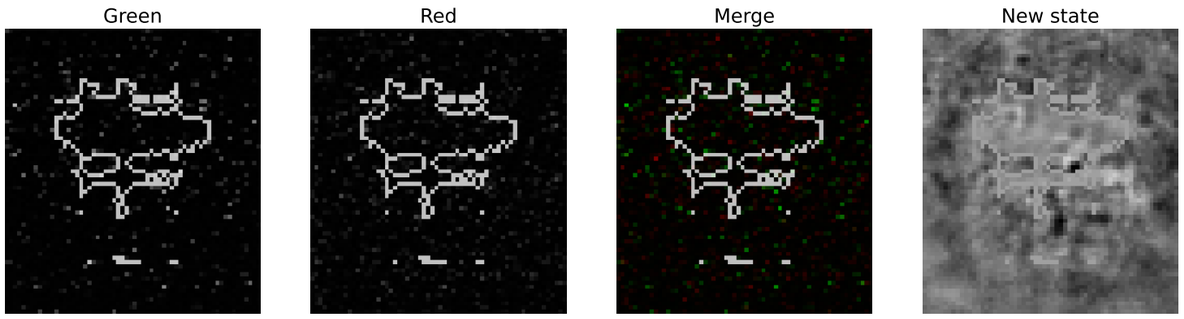


New: Unresolved · green excess 0.00212 · red excess 0.00158

Label 220 · old C1 G1 / C2 uncertain

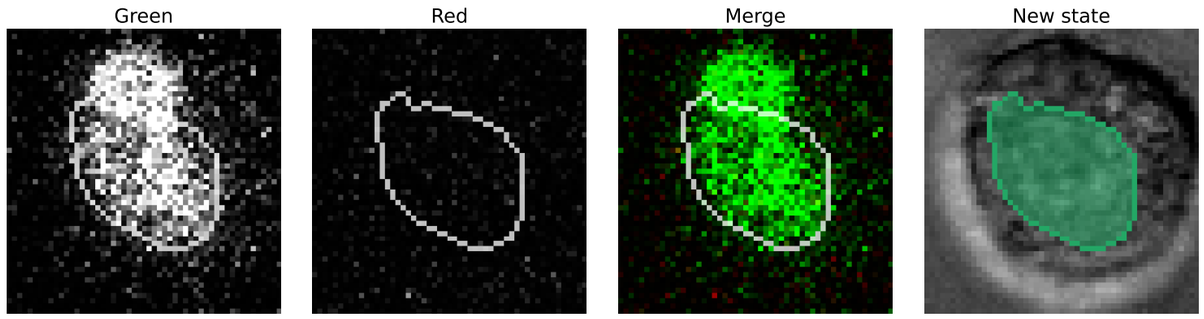


New: Green only · green excess 0.08049 · red excess 0.00128

Label 127 · old C1 G2M / C2 G1

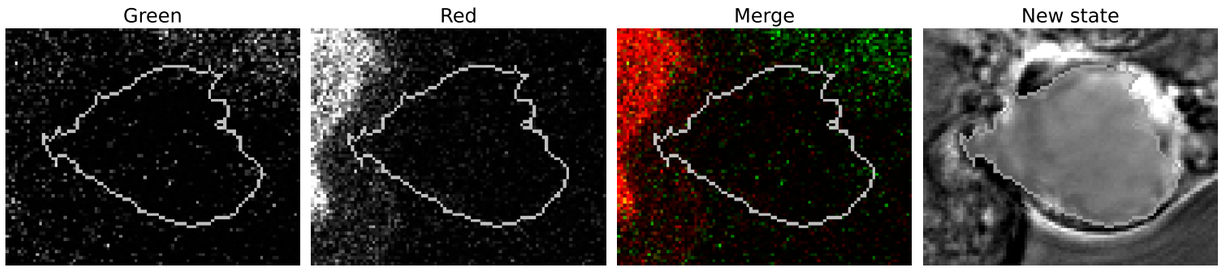

New: Unresolved · green excess 0.00149 · red excess 0.00187

Label 16 · old C1 G1 / C2 G1

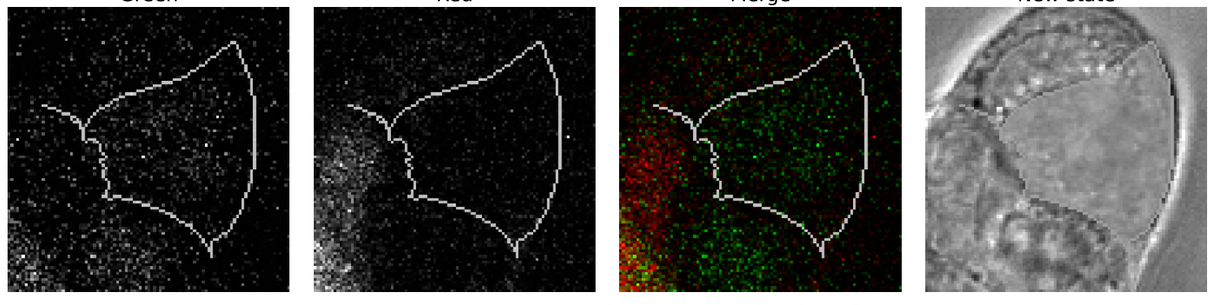

New: Unresolved · green excess 0.00364 · red excess 0.00123

Images: z=35 with fixed stretches. Scores/calls: 3D. White outlines show the selected component; dim channels can remain below their local reference.