Why panel A and the classification maps disagree
241016 / FoF 5 · dominant components visible at z=35

180 units intersect z=35
180/180 above the green gate
123/180 above the red gate

29/180 C1 calls change using slice means

Gate brightness on panel A's display:
  Green: 1.0% of full brightness
  Red: 2.9% of full brightness

Numbers 1–6 link to the example sheet.
Axes use the original normalized intensities.
These counts do not measure phase accuracy.

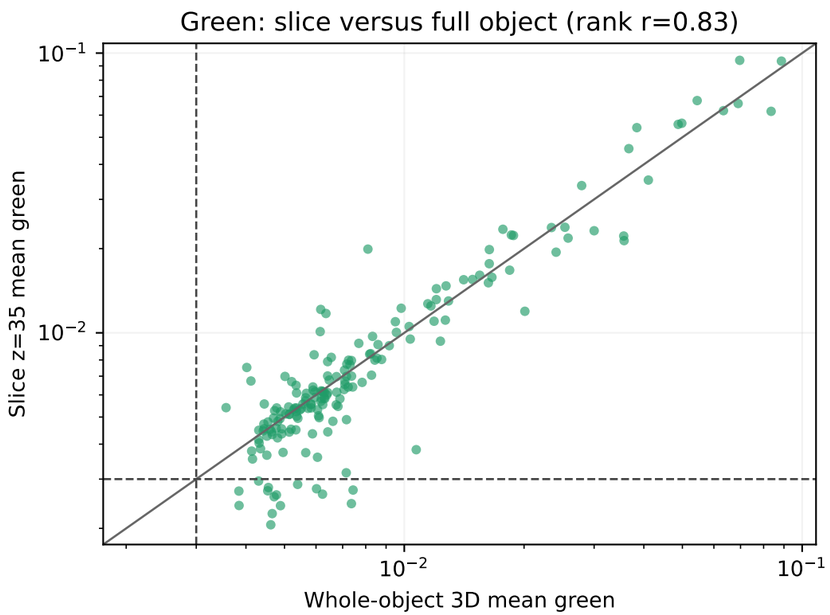

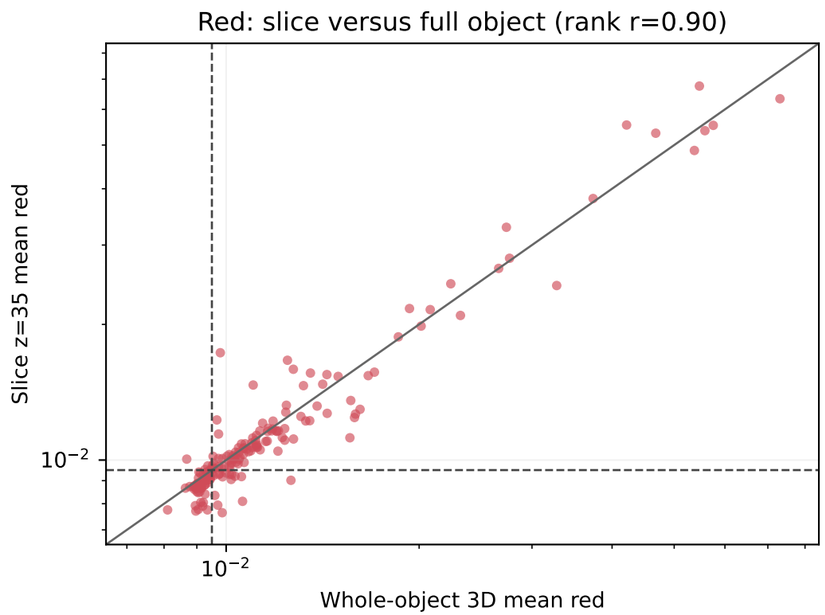

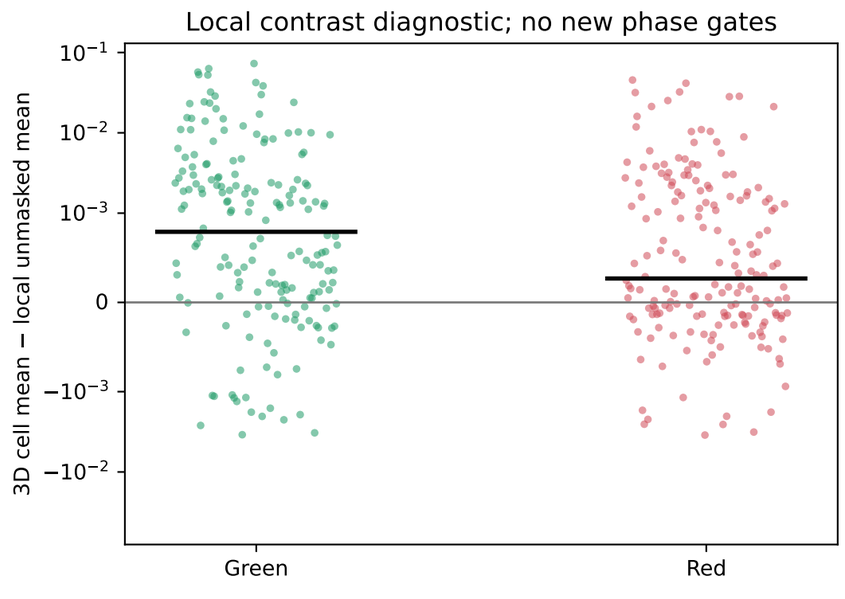

Raw image means reproduce the table values. Threshold calibration and biological phase accuracy are separate questions.