


Fig. 1 — Calibration integrity (Chromatogram & DAD)


1A

Chromatogram Total

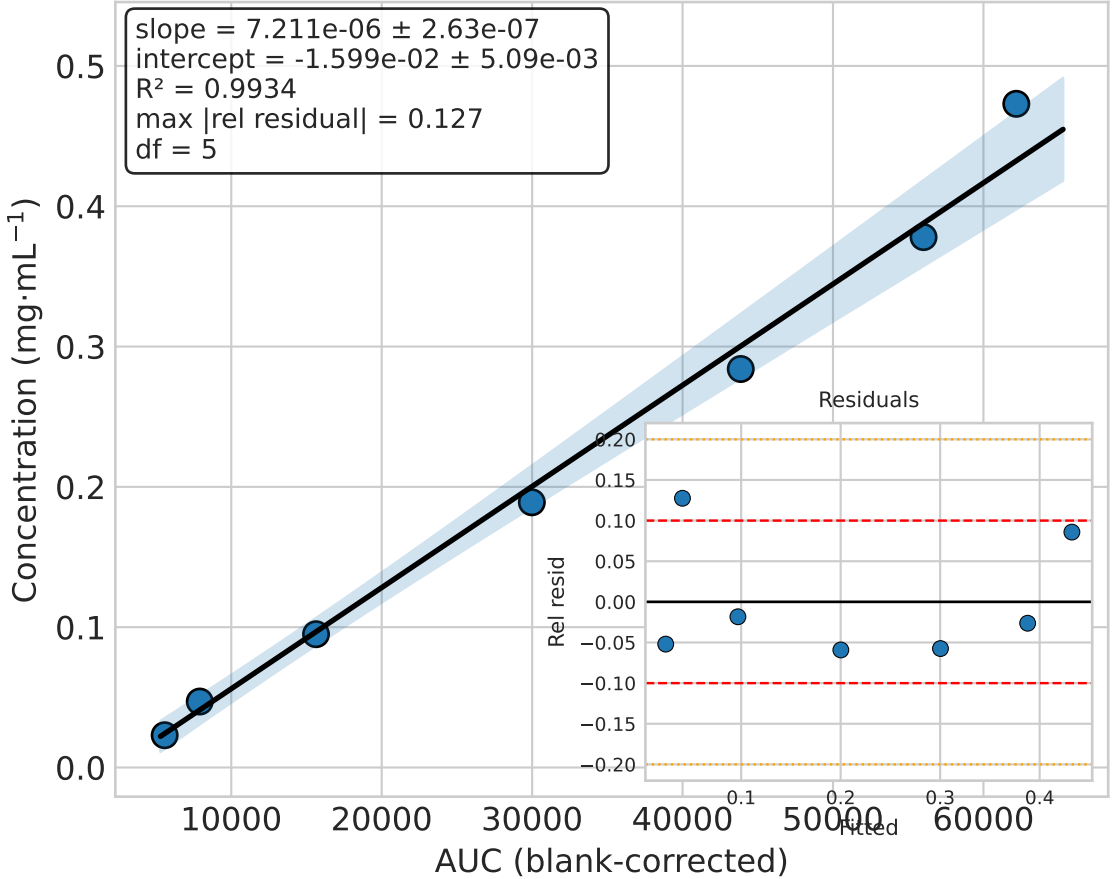


1B

Chromatogram Oxidized

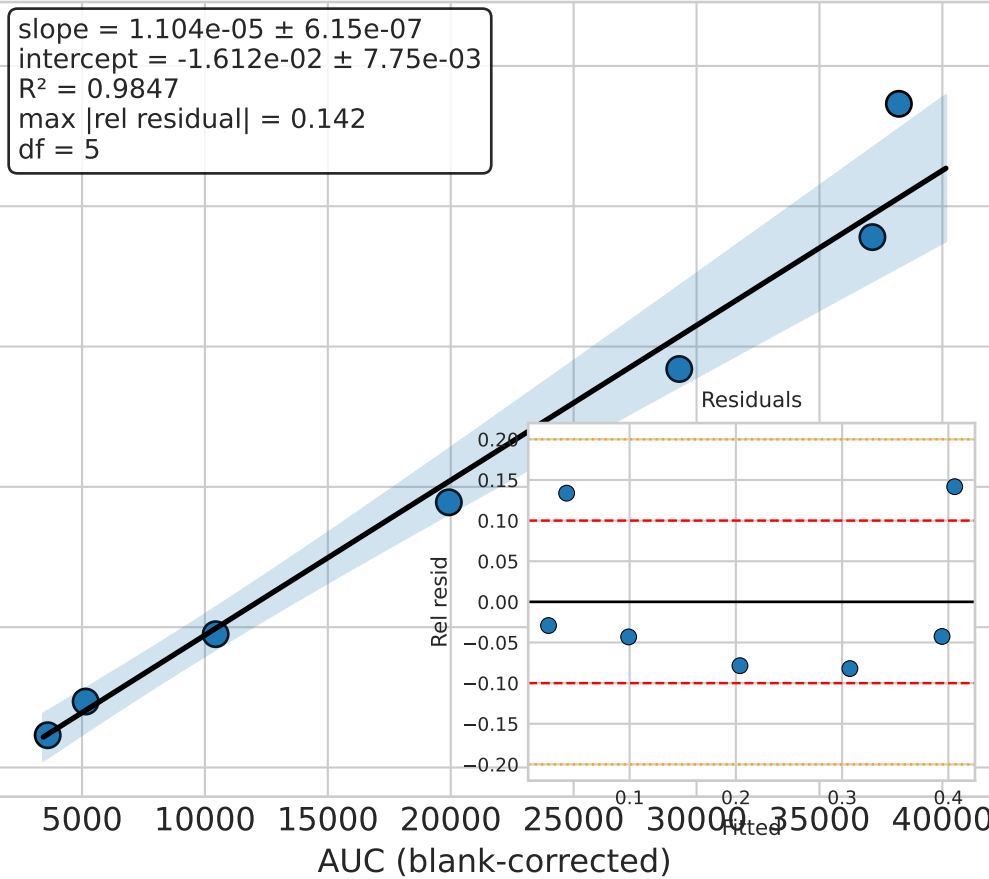


1C

Chromatogram Reduced

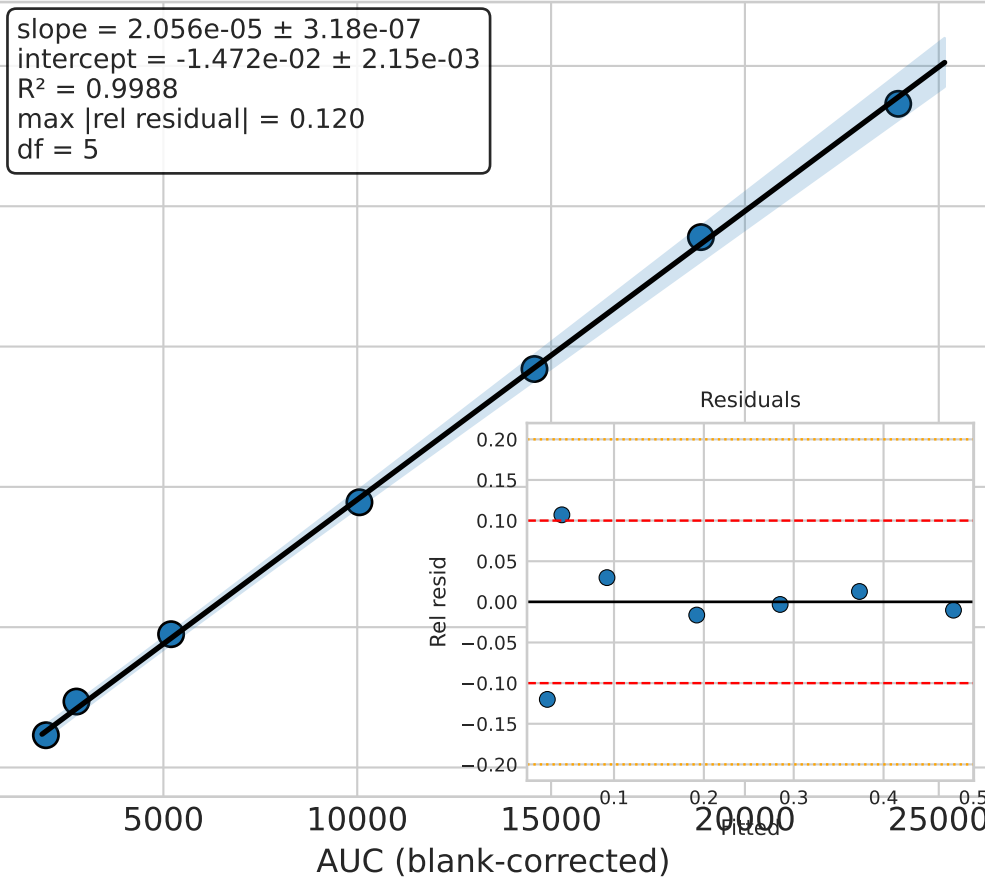


1D

DAD Total

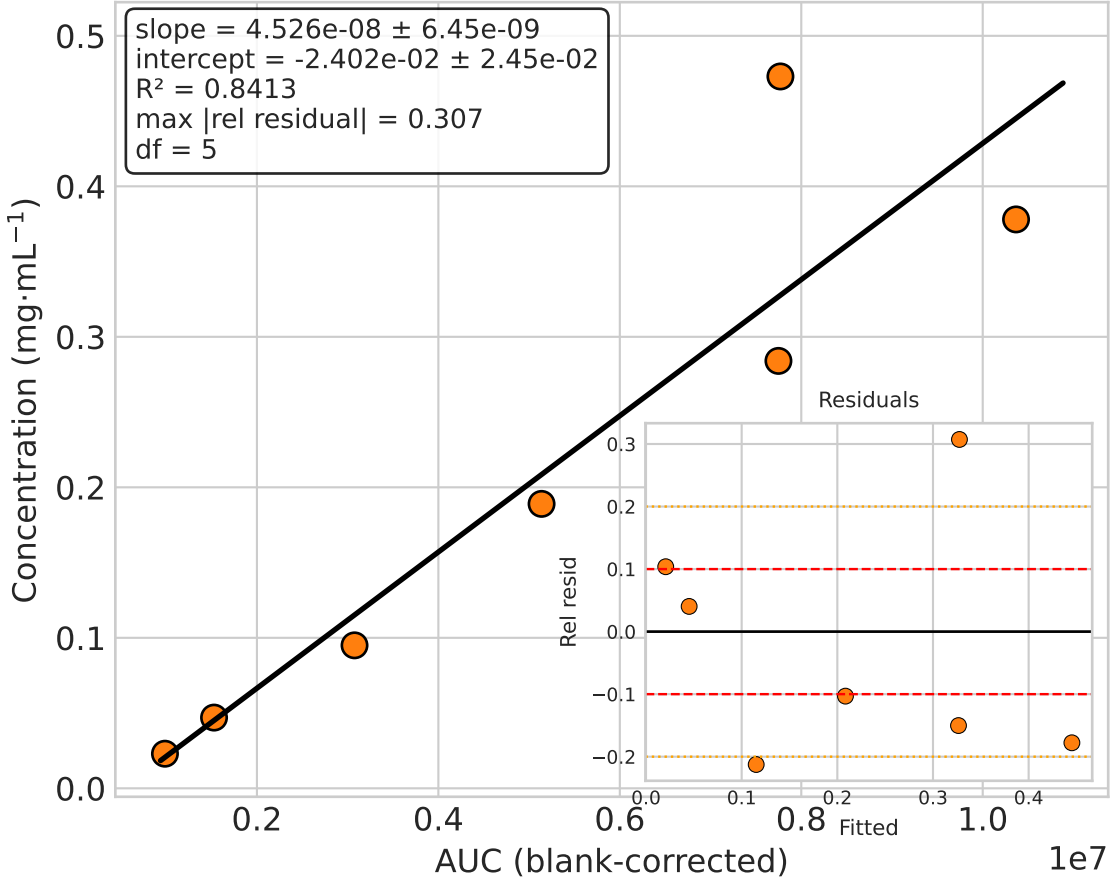

1E

DAD Oxidized

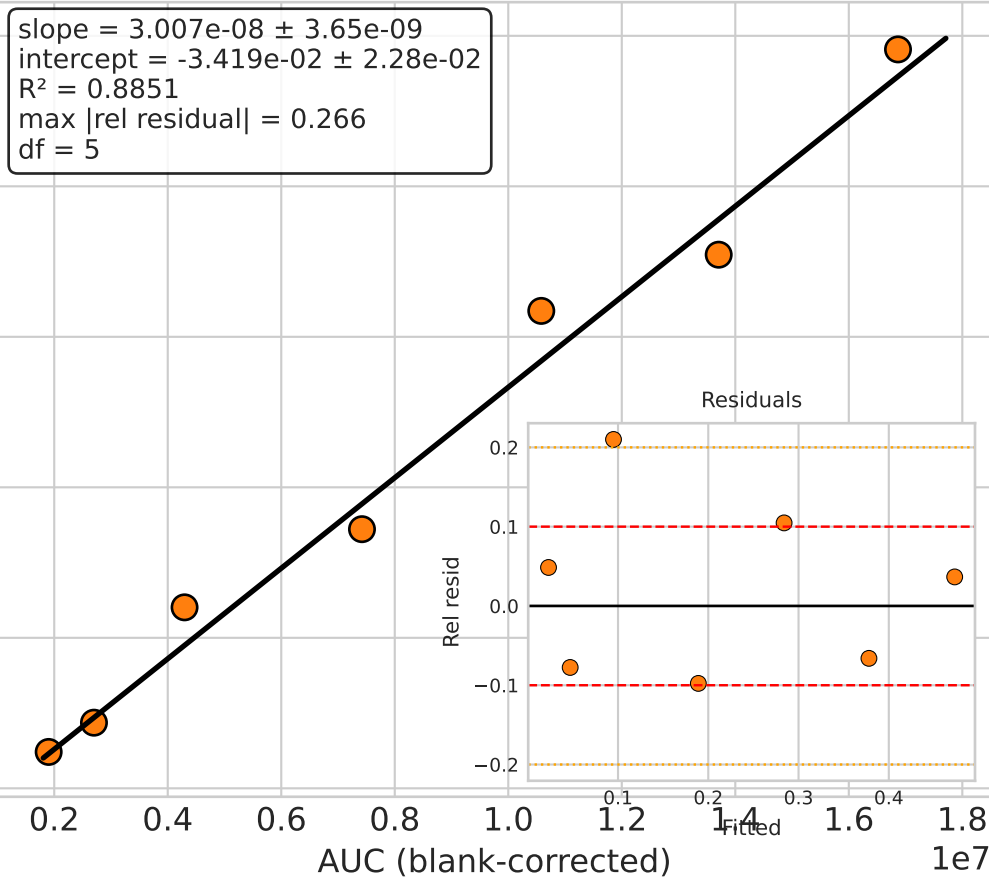

1F

DAD Reduced

