


## SME15822 — Althea Smyrna-1046 MRI


Althea · Philips MRI · Smyrna, TN (Nashville) · Jun 28 — Jul 22 monitor data (20,000 readings) · analyzed 2026-07-22

|                                                                                          |                                                                            |                                                                            |                                                                   |                                                                 |
|------------------------------------------------------------------------------------------|----------------------------------------------------------------------------|----------------------------------------------------------------------------|-------------------------------------------------------------------|-----------------------------------------------------------------|
| <b>COMPRESSOR</b><br><b>ON</b><br>recovered Jul 21 02:45Z · 14 cycles from Jul 19 22:45Z | <b>PRESSURE NOW</b><br><b>262 mbar</b><br>~2.6× the 100 mbar line · easing | <b>EVENT PEAK</b><br><b>272 mbar</b><br>Jul 21 00:48Z · 172 over threshold | <b>TEMP ALARM</b><br><b>FIRED</b><br>Jul 20 13:48 → Jul 21 04:48Z | <b>HELIUM</b><br><b>79.3%</b><br>+2.8 pts · no loss · no quench |
|------------------------------------------------------------------------------------------|----------------------------------------------------------------------------|----------------------------------------------------------------------------|-------------------------------------------------------------------|-----------------------------------------------------------------|

**HE PRESSURE — JUN 28 → JUL 22** (daily range, mbar · orange shade = the event window)

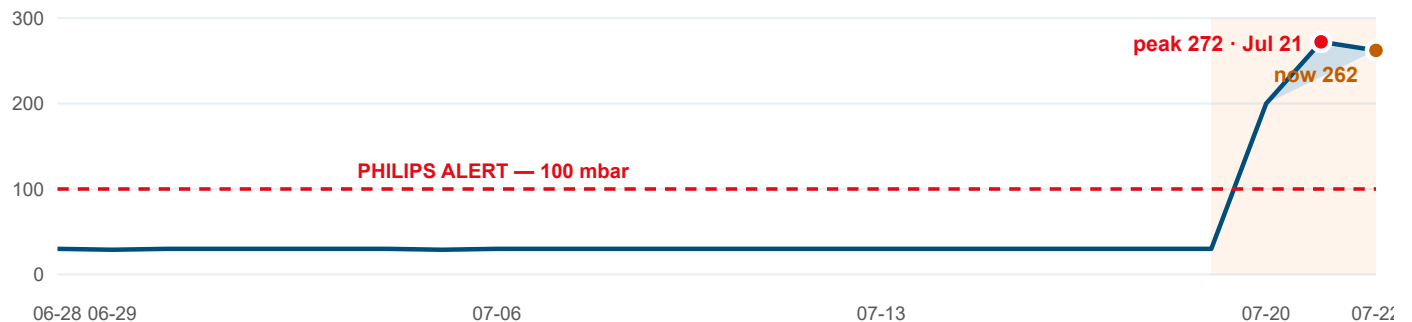

**HELIUM LEVEL — JUN 28 → JUL 22** (daily reading, %)

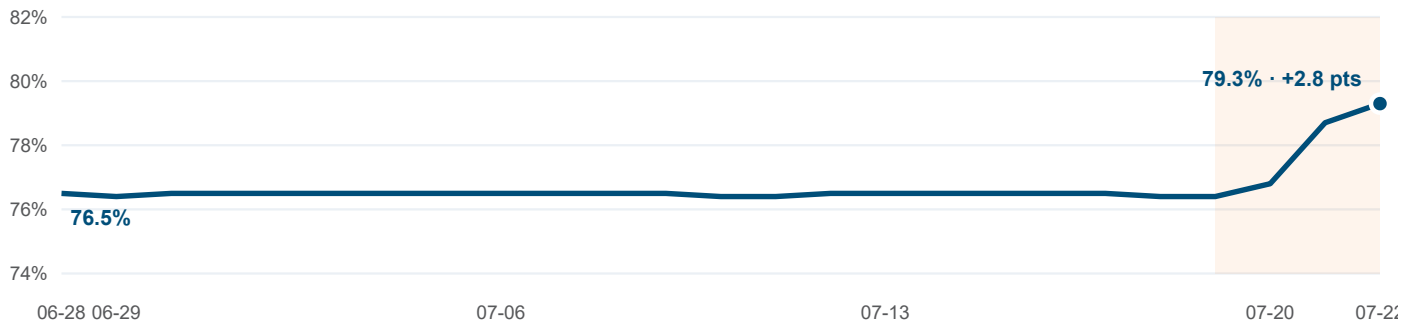

**Timeline:** Jun 28 — Jul 19: He pressure held a flat 28–30 mbar, helium 76.4–76.5%, compressor running continuously. **Jul 19 22:45Z: the compressor made its first stop (1→0)** and then cycled on/off 14 times through Jul 21 02:45Z (49 readings at 0). **Jul 20 13:48Z: He pressure first read above baseline at 200 mbar** (100 over the Philips line); helium ticked up to 76.8% and a temperature alarm fired (27 readings =1 through Jul 21 04:48Z — not continuous, it re-fired three times). Avg He Pressure peaked 274 mbar Jul 20 21:18Z; **He Pressure (STT) peaked 272 mbar Jul 21 00:48Z** (172 over threshold). The compressor recovered to running Jul 21 02:45Z and has held since. Helium rose steadily to **79.3% by Jul 22** (+2.8 points, never below 76.4%). He pressure eased to 262 mbar (Jul 22 08:48Z) — still 162 over the line. No pressure alarm, no quench, no error state anywhere in the file.

### CURRENT — JUL 22 (last readings)

Compressor ON (13:45Z). He pressure 262 mbar STT / 260 mbar avg — ~160 over the 100 mbar Philips line. Helium 79.3%.

### RATES

Pressure +233 mbar over ~3 days (29→262); peak +243 mbar (272), now easing. Helium +2.8 points over ~2 days — no loss, reads high while boiling.

### DATA NOTES

He Level blank in most rows (52 valid of 20,000). Pressure non-monotonic (200→272→231→262). Temp Alarm re-fired, not continuous. Tech Room Temp is °C (~19–21); Room Temp is °F (~74). No prior updates on the Monday item.