

SME01121 — Piedmont Columbus Regional - Midtown MRI

Piedmont HealthCare · Siemens MRI · Columbus, GA · Jul 7 – Aug 6 monitor data (1,468 captures) · analyzed 2

COMPRESSOR
ON
running continuously through the window


COLDHEAD
43.600 K
steady at base temperature

PRESSURE NOW
15.30 PSI
within the 14.4–16.4 PSI band


EVENT PEAK
15.31 PSI
Jul 7 00:45Z · 1.09 PSI under threshold

HELIUM
74.6%
+0.00 pts · no loss · no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI)

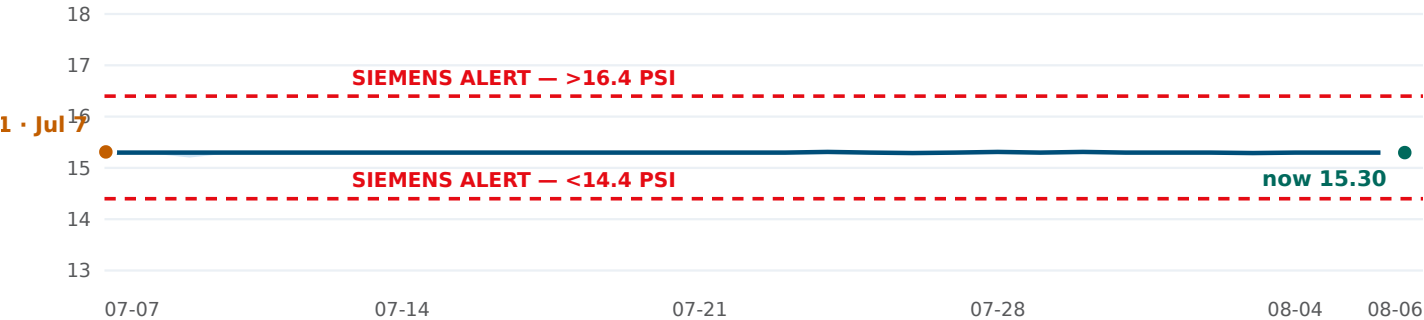

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

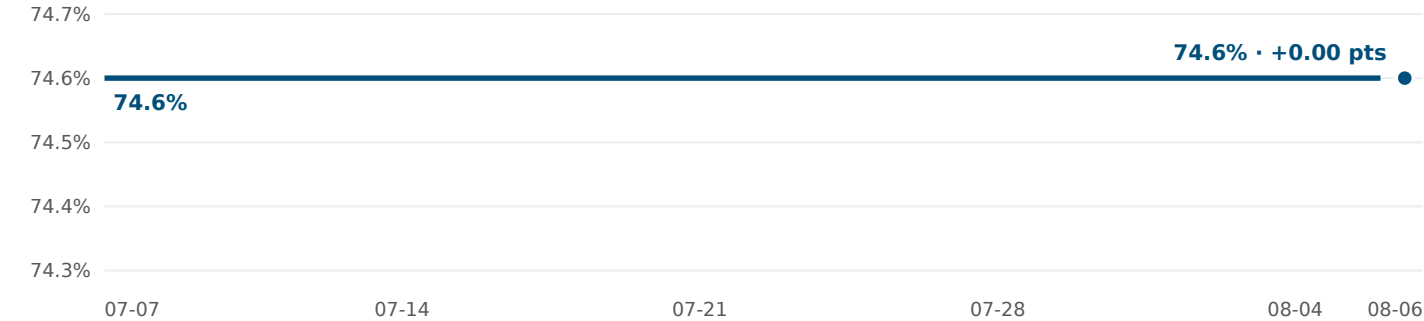

Timeline (UTC): Baseline Jul 7 – Aug 6: coldhead at base temperature. No compressor events, alarms, or threshold breaches detected across 1,468 captures. Helium rose to **74.6%** (+0.00 vs baseline). No quench. Pressure now reads 15.30 PSI (Aug 6 13:45Z) — within the 14.4–16.4 PSI band.

CURRENT — AUG 6 (last readings)
Compressor ON. He pressure 15.30 PSI (13:45Z). Helium 74.6%.

RATES
Pressure +0.00 PSI vs baseline (15.30 → 15.30); peak 15.31. Helium +0.00 points.

DATA NOTES
1,468 captures · 1,459 valid pressure · 1,459 valid helium readings. Charts show the daily min–max range with the daily last value. EDU (1,468 captures): room 66.0–72.3 °F · probes 75.8–78.1 / 75.8–81.2 °F · humidity 46–59%.