

SME01141 — Piedmont Rockdale Hospital MRI

Piedmont HealthCare · GE MRI · Conyers, GA · Jul 7 – Aug 6 monitor data (1,469 captures) · analyzed 2026-08-06

COMPRESSOR

RESTARTED

recovered Jul 13 22:15Z
 · off ~0.0 h

COLDHEAD

4.076 K

from 12.7 K

PRESSURE NOW

1.020 PSI

within the 0.5–5.2
 PSI band · easing

EVENT PEAK

1.092 PSI


Jul 13 21:45Z ·
 4.108 PSI under
 threshold

HELIUM


74.90%

–0.17 pts · no loss ·
 no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI · orange shade = the event window)

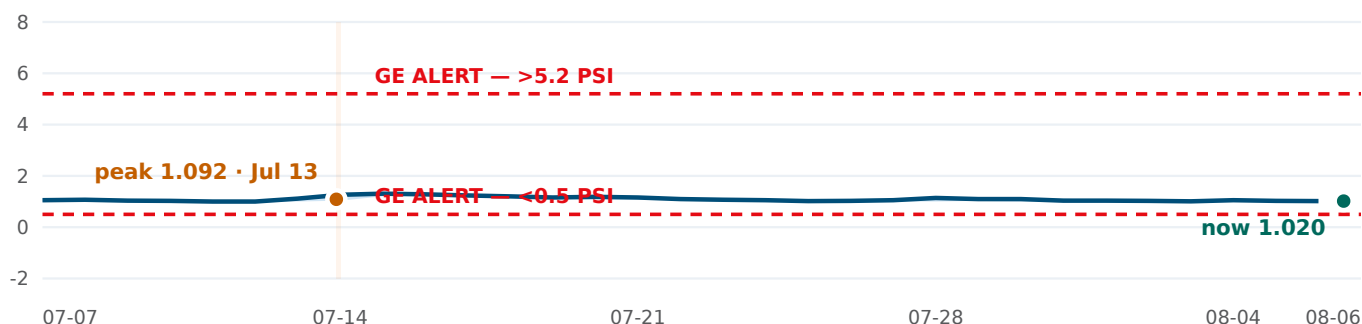

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

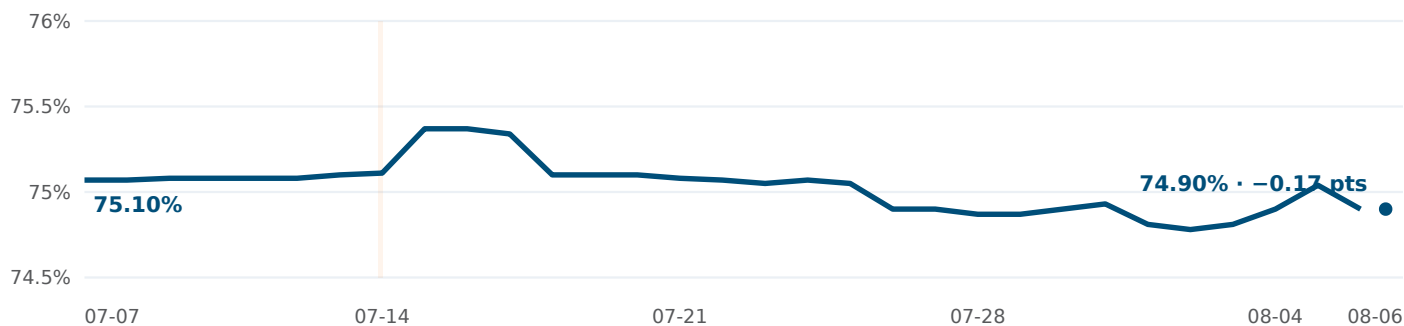

Timeline (UTC): Baseline Jul 7 – Jul 13: pressure held 0.998–1.101 PSI, helium 75.01–75.11%, coldhead at base temperature. **Jul 13 21:45Z: the compressor stopped** and stayed off ~0.0 h (1 readings off). He pressure rose from 1.079 to a **peak of 1.092 PSI at Jul 13 21:45Z** — never reached the 5.2 PSI threshold, 4.108 PSI below the line. **The compressor recovered Jul 13 22:15Z** and has held since. Helium fell to **74.90%** (–0.17 vs baseline). No quench. Pressure now reads 1.020 PSI (Aug 6 14:15Z) — within the 0.5–5.2 PSI band.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 1.020 PSI (14:15Z). Helium 74.90%.

RATES

Pressure –0.059 PSI vs baseline (1.079 → 1.020); peak 1.092. Helium –0.17 points.

DATA NOTES

1,469 captures · 1,469 valid pressure · 1,469 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,469 captures): room 79.7–84.6 °F · probes 57.4–68.3 / 62.9–84.2 °F · humidity 27–51%. Host clock ~745 min off vs capture time — times shown use capture time.