

SME02582 — Mississippi Baptist Medical Center MRI

Intelas · GE MRI · Jackson, MS · Jul 7 – Aug 6 monitor data (1,469 captures) · analyzed 2026-08-06

COMPRESSOR

ON

recovered Aug 6
14:15Z · 41 cycles
from Jul 7 17:15Z

COLDHEAD

9.523 K

from 133.7 K

PRESSURE NOW

1.939 PSI

within the 0.5–5.2
PSI band · easing

EVENT PEAK

3.782 PSI


Jul 25 13:15Z · 1.418
PSI under threshold

HELIUM


84.99%

+0.00 pts · no loss ·
no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI · orange shade = the event window)

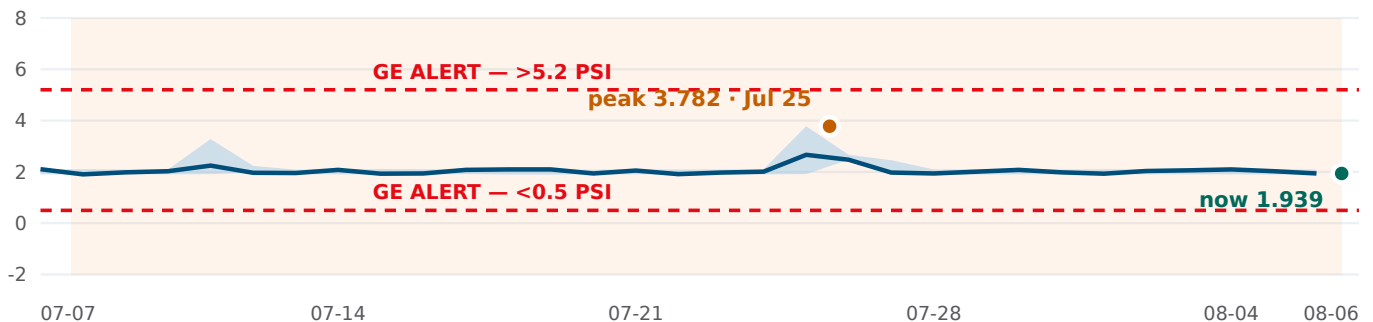

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

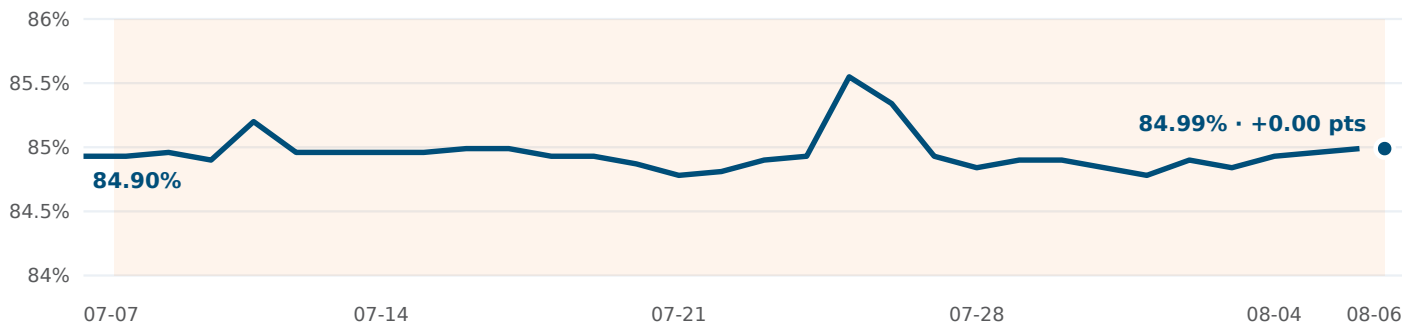

Timeline (UTC): Baseline Jul 7 - Jul 7: pressure held 1.903–2.093 PSI, helium 84.87–84.99%, coldhead at base temperature. **Jul 7 17:15Z: the compressor stopped** and then cycled on/off 41 times through Aug 6 14:15Z (75 readings off). He pressure rose from 2.034 to a **peak of 3.782 PSI at Jul 25 13:15Z** — never reached the 5.2 PSI threshold, 1.418 PSI below the line (+0.004 PSI/h avg on the ramp). **The compressor recovered Aug 6 14:15Z** and has held since. Helium rose to **84.99%** (+0.00 vs baseline). No quench. Pressure now reads 1.939 PSI (Aug 6 14:15Z) — within the 0.5–5.2 PSI band.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 1.939 PSI (14:15Z). Helium 84.99%.

RATES

Pressure –0.095 PSI vs baseline (2.034 → 1.939); peak 3.782. Ramp averaged +0.004 PSI/h. Helium +0.00 points.

DATA NOTES

1,469 captures · 1,469 valid pressure · 1,469 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,469 captures): room 32.0–97.2 °F · probes 67.9–93.8 / 64.1–87.7 °F · humidity 0–57%. Host clock ~160 min off vs capture time — times shown use capture time.