

SME19034 — Beebe Healthcare Imaging Rehoboth MRI

Renovo Solutions, LLC · Philips MRI · Rehoboth Beach, DE · Jul 7 – Aug 6 monitor data (272 captures) · analyze

COMPRESSOR

ON

recovered Jul 20
15:48Z · 2 cycles
from Jul 19 14:48Z

PRESSURE NOW

33 mbar

41% of the 80 mbar
line · easing

EVENT PEAK

144 mbar

Jul 21 07:48Z · 64
mbar over threshold

TEMP ALARM

TRIGGERED


4 readings · Jul 19
14:48Z → Jul 19 15:48Z

HELIUM


67.3%

+0.00 pts · no loss ·
no quench

HE PRESSURE — JUL 7 → AUG 6 (every capture, mbar · orange shade = the event window)

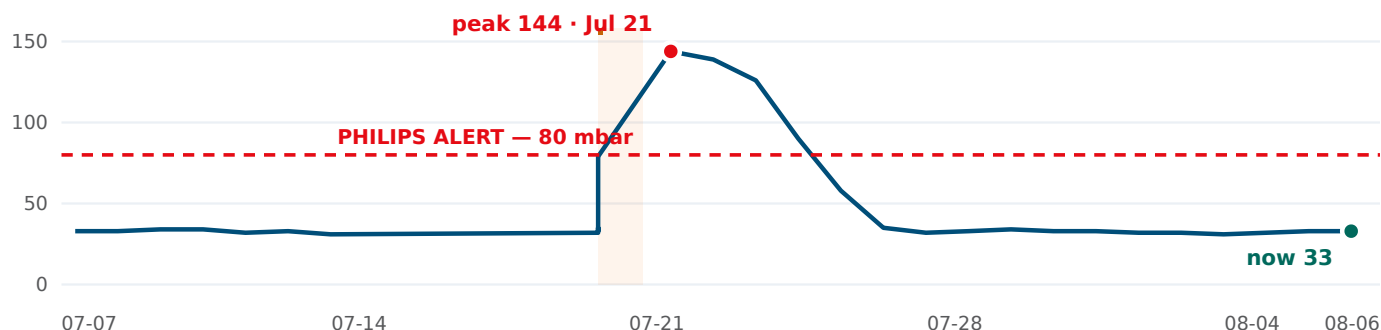

HELIUM LEVEL — JUL 7 → AUG 6 (every capture, %)

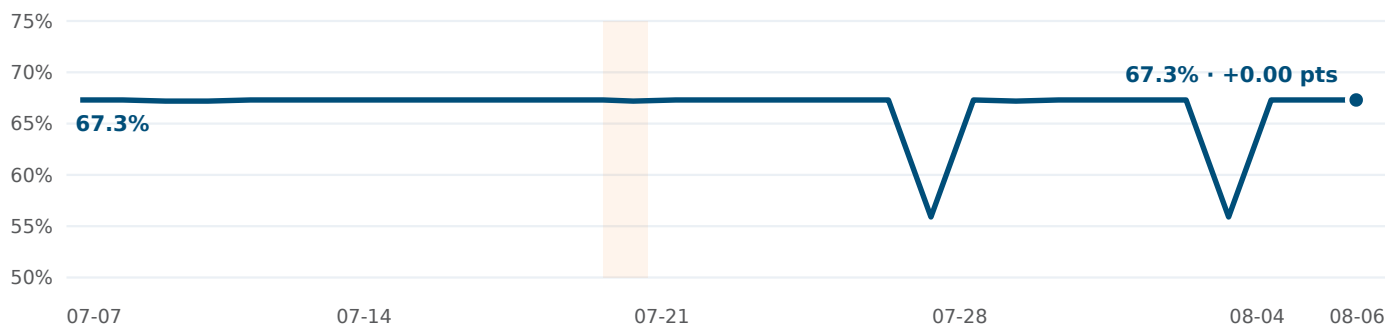

Timeline (UTC): Baseline Jul 7 - Jul 19: he pressure held 31-34 mbar, helium 67.2-67.3%. **Jul 19 14:48Z: the compressor stopped** and then cycled on/off 2 times through Jul 20 15:48Z (4 readings off). A compressor temperature alarm was triggered Jul 19 14:48Z → Jul 19 15:48Z (4 readings — not continuous, it re-triggered 1 time; amber strip on the pressure chart). Room temperature held 79.0-80.8 °F over the alarm window. He pressure rose from 31 to a **peak of 144 mbar at Jul 21 07:48Z** — 64 mbar over the 80 mbar line (+3 mbar/h avg on the ramp). **The compressor recovered Jul 20 15:48Z** and has held since. Helium rose to **67.3%** (+0.00 vs baseline). No quench. He pressure now reads 33 mbar (Aug 6 07:48Z) — 41% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 33 mbar (07:48Z). Helium 67.3%.

RATES

He pressure +2 mbar vs baseline (31 → 33); peak 144. Ramp averaged +3 mbar/h. Helium +0.00 points.

DATA NOTES

272 captures · 30 valid pressure · 31 valid helium readings. Charts plot every archived capture. EDU (629 captures): room 72.0-83.3 °F · probes -196.6-76.4 / -196.6-129.4 °F · humidity 26-47%. Host clock ~31 min off vs capture time — times shown use capture time.